



UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

APPLICATION NUMBER	PATENT NUMBER	GROUP ART UNIT	FILE WRAPPER LOCATION
11/322,568		2612	

Correspondence Address / Fee Address Change

The following fields have been set to Customer Number 23608 on 08/02/2006

- Correspondence Address
- Maintenance Fee Address

The address of record for Customer Number 23608 is:

MEDTRONIC MINIMED INC.
18000 DEVONSHIRE STREET
NORTHRIDGE, CA 91325-1219

DEXCOM
EXHIBIT 1021



UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

APPLICATION NUMBER	FILING OR 371 (c) DATE	FIRST NAMED APPLICANT	ATTORNEY DOCKET NUMBER
11/322,568	12/30/2005	John J. Mastrototaro	PD00291 CIP

MEDTRONIC MINIMED, INC.
18000 Devonshire Street
Northridge, CA 91325-1219



CONFIRMATION NO. 4822
FORMALITIES
LETTER

Date Mailed: 02/24/2006

NOTICE TO FILE MISSING PARTS OF NONPROVISIONAL APPLICATION

FILED UNDER 37 CFR 1.53(b)

Filing Date Granted

Items Required To Avoid Abandonment:

An application number and filing date have been accorded to this application. The item(s) indicated below, however, are missing. Applicant is given **TWO MONTHS** from the date of this Notice within which to file all required items and pay any fees required below to avoid abandonment. Extensions of time may be obtained by filing a petition accompanied by the extension fee under the provisions of 37 CFR 1.136(a).

- The oath or declaration is unsigned.

The application is informal since it does not comply with the regulations for the reason(s) indicated below.

The required item(s) identified below must be timely submitted to avoid abandonment:

- Replacement drawings in compliance with 37 CFR 1.84 and 37 CFR 1.121(d) are required. The drawings submitted are not acceptable because:
 - The drawings have a line quality that is too light to be reproduced (weight of all lines and letters must be heavy enough to permit adequate reproduction) or text that is illegible (reference characters, sheet numbers, and view numbers must be plain and legible) see 37 CFR 1.84(l) and (p)(1)); See Figure(s) 24.
 - The drawings submitted to the Office are not electronically reproducible. Drawing sheets must be submitted on paper, which is flexible, strong, white, smooth, non-shiny, and durable (see 37 CFR 1.84(e)). See Figure(s) 15-18.

Applicant is cautioned that correction of the above items may cause the specification and drawings page count to exceed 100 pages. If the specification and drawings exceed 100 pages, applicant will need to submit the required application size fee.

The applicant needs to satisfy supplemental fees problems indicated below.

The required item(s) identified below must be timely submitted to avoid abandonment:

05/16/2006 CCHAU1 00000065 500621 11322568
01 FC:1051 130.00 DA

- To avoid abandonment, a surcharge (for late submission of filing fee, search fee, examination fee or oath or declaration) as set forth in 37 CFR 1.16(f) of \$130 for a non-small entity, must be submitted with the missing items identified in this letter.

SUMMARY OF FEES DUE:

Total additional fee(s) required for this application is **\$130** for a Large Entity

- **\$130** Surcharge.

Replies should be mailed to: Mail Stop Missing Parts
 Commissioner for Patents
 P.O. Box 1450
 Alexandria VA 22313-1450

*A copy of this notice **MUST** be returned with the reply.*

A handwritten signature, possibly reading 'LS', is written over a horizontal line.

Office of Initial Patent Examination (571) 272-4000, or 1-800-PTO-9199, or 1-800-972-6382
PART 2 - COPY TO BE RETURNED WITH RESPONSE



PATENT
PD00291 CIP

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

Continuation-in-Part Application of:)
John J. Mastrototaro et al.) Examiner: unknown
Serial No.: 11/322,568)
Filed: December 30, 2005) Group Art Unit: 2635
For: TELEMETERED CHARACTERISTIC)
MONITOR SYSTEM AND METHOD)
OF USING THE SAME)

RESPONSE TO NOTICE TO FILE MISSING PARTS OF
NONPROVISIONAL APPLICATION

Mail Stop Missing Parts
Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

Dear Sir:

In response to the February 24, 2006 Notice to File Missing Parts of Nonprovisional Application for the above-identified application, enclosed are:

- (1) Copy of Notice to be returned with response;
- (2) 12 sheets of Formal Drawings, which is a missing part and Transmittal of Formal Drawings;
- (3) A fully-executed Declaration, which is a missing part and Transmittal of Missing Declaration;
- (4) Petition for 1 month Extension of Time;
- (5) A fully-executed Assignment with Recordation Form Cover Sheet;
- (6) Power of Attorney by Assignee and Exclusion of Inventor Under Rule 3.71; and
- (7) Return postcard.

The Commissioner is hereby authorized to charge the \$130 Surcharge, and any other fees associated with this communication, to Deposit Account No. 50-0621. A duplicate copy of this sheet is enclosed.

Respectfully submitted,

MEDTRONIC MINIMED, INC.

Date: May 10, 2006

By: Ajit S. Narang
Ajit S. Narang
Registration No. 55,480

MEDTRONIC MINIMED, INC.
18000 Devonshire Street
Northridge, California 91325-1219
Telephone (818) 576-5003

I hereby certify that this correspondence is being deposited with the United States Postal Service with sufficient postage as First class mail in an envelope addressed to: Mail Stop Missing Parts, Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450

on: May 10, 2006
Date of Deposit

Signature: Ajit S. Narang
Ajit S. Narang, Reg. No. 55,480

**COPY**PATENT
PD00291 CIPCUSTOMER NUMBER 23608IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

In re Continuation-in-Part application of:)
John J. Mastrototaro et al.)
Serial No.: 11/322,568)
Filed: December 30, 2005)
For: TELEMETERED CHARACTERISTIC)
MONITOR SYSTEM AND METHOD)
OF USING THE SAME)

Examiner: Unknown

Group Art Unit: 2635

TRANSMITTAL OF FORMAL DRAWINGS

Mail Stop Missing Parts
Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

I hereby certify that this
correspondence is being deposited
with the United States Postal Service
with sufficient postage as first class
mail in an envelope addressed to:
Mail Stop Missing Parts, Commissioner
for Patents, P.O. Box 1450, Alexandria,
VA 22313-1450 on

May 10, 2006

Date of Deposit

Ajit S. Narang, Reg. No. 55,480

Name

Ajit S. Narang 5/10/06

Signature

Date

Dear Sir:

In response to the Notice to File Missing Parts of Nonprovisional Application dated February 24, 2006, enclosed are 12 sheets of formal drawings (Figs.1-25) submitted in compliance with 37 CFR 1.84 and 37 CFR 1.121(d) for the above-captioned application. Please substitute the enclosed formal drawings for the informal drawings previously filed.

The Commissioner is hereby authorized to charge any deficiency payment or credit any overpayment to Deposit Account No. 50-0621. A copy of this transmittal is enclosed.

Respectfully submitted,

Ajit S. Narang

Ajit S. Narang, Reg. No. 55,480
MEDTRONIC MINIMED, INC.
18000 Devonshire Street
Northridge, CA 91325-1219
Telephone: (818) 576-5003
Fax: (818) 576-6202

Date: May 10, 2006



PATENT
PD00291 CIP

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

In re Continuation-in-Part Application of:)
John J. Mastrototaro et al.)
Serial No.: 11/322,568)
Filed: December 30, 2005)
For: TELEMETERED CHARACTERISTIC)
MONITOR SYSTEM AND METHOD OF)
USING THE SAME)

**Transmittal of Missing
Declaration**


Mail Stop Missing Parts
Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

Dear Sir:

Enclosed herewith is the Declaration for the above-identified application in response to the "Notice to File Missing Parts of Nonprovisional Application" dated February 24, 2006.

The Commissioner is hereby authorized to charge the late oath or declaration surcharge fee of \$130 and any other fees associated with this communication to Deposit Account No. 50-0621. A duplicate copy of this sheet is enclosed.

Respectfully submitted,


Ajit S. Narang, Reg. No. 55,480
MEDTRONIC MINIMED, INC.
18000 Devonshire Street
Northridge, CA 91325-1219
(818) 576-5003

Dated: May 10, 2006

I hereby certify that this correspondence is being deposited with the United States Postal Service as First class mail in an envelope with sufficient postage addressed to Mail Stop Missing Parts, Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.

on: May 10, 2006
Date of Deposit

Signature: 
Ajit S. Narang, Reg. No. 55,480



PATENT
PD00291 CIP

CUSTOMER NUMBER 23608

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

Inte Continuation-in-Part application of:)
John J. Mastrototaro et al.)
Serial No.: 11/322,568)
Filed: December 30, 2005)
For: TELEMETERED CHARACTERISTIC)
MONITOR SYSTEM AND METHOD)
OF USING THE SAME)

Examiner: Unknown

Group Art Unit: 2635

TRANSMITTAL OF FORMAL DRAWINGS

Mail Stop Missing Parts
Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

I hereby certify that this
correspondence is being deposited
with the United States Postal Service
with sufficient postage as first class
mail in an envelope addressed to:
Mail Stop Missing Parts, Commissioner
for Patents, P.O. Box 1450, Alexandria,
VA 22313-1450 on

May 10, 2006
Date of Deposit

Ajit S. Narang, Reg. No. 55,480
Name

Ajit S. Narang 5/10/06
Signature Date

Dear Sir:

In response to the Notice to File Missing Parts of Nonprovisional Application dated February 24, 2006, enclosed are 12 sheets of formal drawings (Figs.1-25) submitted in compliance with 37 CFR 1.84 and 37 CFR 1.121(d) for the above-captioned application. Please substitute the enclosed formals drawings for the informal drawings previously filed.

The Commissioner is hereby authorized to charge any deficiency payment or credit any overpayment to Deposit Account No. 50-0621. A copy of this transmittal is enclosed.

Respectfully submitted,

Ajit S. Narang

Ajit S. Narang, Reg. No. 55,480
MEDTRONIC MINIMED, INC.
18000 Devonshire Street
Northridge, CA 91325-1219
Telephone: (818) 576-5003
Fax: (818) 576-6202

Date: May 10, 2006



PATENT
PD00291 CIP

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

Continuation-in-Part Application of)
John J. Mastrototaro et al.) Examiner: unknown
Serial No. 11/322,568)
Filed: December 30, 2005) Group Art Unit: 2635
For: TELEMETERED CHARACTERISTIC)
MONITOR SYSTEM AND METHOD)
OF USING THE SAME)

PETITION FOR EXTENSION OF TIME

Mail Stop Missing Parts
Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

Sir:

In accordance with 37 C.F.R. § 1.136, applicant respectfully petitions the Commissioner for a one-month extension of time, extending from April 24, 2006 to May 24, 2006 the period for response to the Notice to File Missing Parts of Application dated February 24, 2006. The responsive papers are enclosed.

The Commissioner is hereby authorized to charge any fee insufficiency (or credit any overpayment) to Deposit Account No. 50-0621. A copy of this petition is enclosed.

Respectfully submitted,

Dated: May 10, 2006


By: Ajit S. Narang
Ajit S. Narang
Reg. No. 55,480

MEDTRONIC MINIMED, INC.
18000 Devonshire Street
Northridge, CA 91325-1219
(818) 576-5003

I hereby certify that this correspondence is being deposited with the U.S. Postal Service with sufficient postage as first class mail in an envelope addressed to: Mail Stop Missing Parts, Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.

on: May 10, 2006
Date of Deposit
Signature: Ajit S. Narang
Ajit S. Narang, Reg. No. 55,480

11322568
00000065 500621
05/16/2006 CCHRU1
02 FC:1251
120.00 DA



DECLARATION

PATENT (U.S.A.)
ATTORNEY'S DOCKET NO. PD00291 CIP

X ORIGINAL
CONTINUATION-IN-PART
DIVISIONAL

As a below named inventor, I declare that the information given herein is true, that I believe that I am the original, first and sole inventor if only one name is listed at 1 below, or a joint inventor if plural inventors are named below at 1-6, of the invention entitled:

TELEMETERED CHARACTERISTIC MONITOR SYSTEM AND METHOD OF USING THE SAME

Which is described and claimed in:

X the attached specification or
the specification in application Serial No. 11/322,568 filed 12/30/2005
as amended on _____

and for which a patent is sought, and that my residence, post office address and citizenship are as stated below next to my name.

I acknowledge my duty to disclose information, which is material to the examination of this application in accordance with Title 37, Code of Federal Regulations §1.56(a).

I hereby state that I have reviewed and understand the contents of the above-identified specification, including the claims, as amended by any amendment referred to above.

I hereby claim priority benefits under Title 35, United States Code, §119 of any application(s) for patent or inventor's certificate listed below and have also identified below any application for patent or inventor's certificate having a filing date before that of the application on which priority is claimed:

PRIOR
APPLICATION(S)

COUNTRY	APPLICATION NUMBER	DATE OF FILING Month Day Year	PRIORITY CLAIMED UNDER 35 U.S.C. 119
US	60/103,812	October 8, 1998	YES <u>X</u> NO

I hereby claim the benefit under Title 35, United States Code, §120 of any United States application(s) listed below and, insofar as the subject matter of each of the claims of this application is not disclosed in the prior United States application in the manner provided by the first paragraph of Title 35, United States Code §112, I acknowledge the duty to disclose material information as defined in Title 37, Code of Federal Regulations, §1.56(a) which occurred between the filing date of the prior application and the national or PCT international filing date of this application.

10/898,589	July 23, 2004	Pending
09/465,715	December 17, 1999	(Now Issued Patent 6,809,653 Issued 10/24/2004)
09/377,472	August 19, 1999	(Now abandoned)
(Application Serial No.)	(Filing Date)	(Status)







Send correspondence to:
MEDTRONIC MINIMED, INC.
18000 Devonshire Street
Northridge, CA 91325-1219

DIRECT TELEPHONE CALLS TO:
Richard Yoon
(818) 576-4110

1	LAST NAME MASTROTOTARO	FIRST NAME JOHN	MIDDLE NAME J.	Residence: CITY LOS ANGELES	STATE or COUNTRY CALIFORNIA
	Post Office Address 10642 LINDBROOK DRIVE, LOS ANGELES, CA 90024				CITIZENSHIP US
2	LAST NAME CHERNOFF	FIRST NAME EDWARD	MIDDLE NAME	Residence: CITY FRAZIER PARK	STATE or COUNTRY CALIFORNIA
	Post Office Address P.O. BOX 329, FRAZIER PARK, CA 93225				CITIZENSHIP US
3	LAST NAME CHOY	FIRST NAME DAVID	MIDDLE NAME Y.	Residence: CITY SAN GABRIEL	STATE or COUNTRY CALIFORNIA
	Post Office Address 801 MONTECITO DRIVE, SAN GABRIEL, CA 91776				CITIZENSHIP US

4	LAST NAME HENKE	FIRST NAME JAMES	MIDDLE NAME L.	Residence: CITY SIMI VALLEY	STATE or COUNTRY CALIFORNIA
	Post Office Address 5105 E. LOS ANGELES AVENUE, PMB 168, SIMI VALLEY, CA 93063				CITIZENSHIP US
5	LAST NAME PURVIS	FIRST NAME RICHARD	MIDDLE NAME E.	Residence: CITY PASADENA	STATE or COUNTRY CALIFORNIA
	Post Office Address 1478 N. MAR VISTA AVENUE, PASADENA, CA 91104				CITIZENSHIP US
6	LAST NAME HONG	FIRST NAME PETER	MIDDLE NAME I.	Residence: CITY SANTA CLARITA	STATE or COUNTRY CALIFORNIA
	Post Office Address 28030 KENTON LANE, SANTA CLARITA, CA 91350				CITIZENSHIP US

I further declare that all statements made herein of my own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under Section 1001 of Title 18 of the United States Code, and that such willful false statements may jeopardize the validity of the application or any patent issuing thereon.

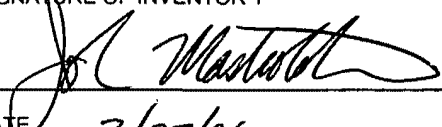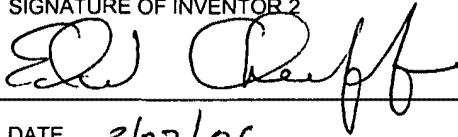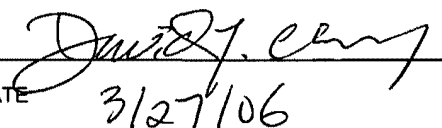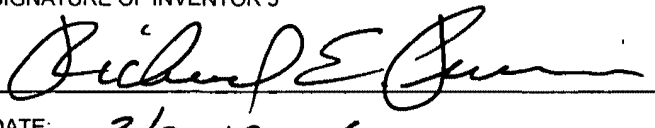SIGNATURE OF INVENTOR 1 	SIGNATURE OF INVENTOR 2 
DATE 3/27/06	DATE 3/27/06
SIGNATURE OF INVENTOR 3 	SIGNATURE OF INVENTOR 4 
DATE 3/27/06	DATE 3/27/06
SIGNATURE OF INVENTOR 5 	SIGNATURE OF INVENTOR 6 
DATE 3/27/2006	DATE 3/27/06



PATENT
PF00291 CIP

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

In re Continuation-in-Part Application of:	)	
John J. Mastrototaro et al.	)	Examiner: unknown
Serial No.: 11/322,568	)	
Filed: December 30, 2005	)	Group Art Unit: 2635
For: TELEMETERED CHARACTERISTIC	)	
MONITOR SYSTEM AND METHOD	)	
OF USING THE SAME	)	

POWER OF ATTORNEY BY ASSIGNEE
AND EXCLUSION OF INVENTOR UNDER RULE 3.71

Mail Stop Missing Parts
Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

Dear Sir:

The undersigned **Eric P. Geismar** is a representative authorized to sign on behalf of the assignee of the entire interest in the above-identified subject application, **MEDTRONIC MINIMED, INC.** and hereby appoints:

Paul H. Kovelman, Reg. No. 35,228;
Richard K. Yoon, Reg. No. 42,247;
Vivian S. Shin, Reg. No. 43,919;
Ajit S. Narang, Reg. No. 55,480;

and all of the firm of Foley & Lardner LLP:

Ted R. Rittmaster, Reg. No. 32,933;
David A. Blumenthal, Reg. No. 26,257;
Richard D. Malone, Reg. No. 51,991;
William J. Robinson, Reg. No. 29,430;
Victor deGyarfas, Reg. No. 40,583

to prosecute this application and to transact all business in the United States Patent and Trademark Office connected therewith, said appointment to be to the exclusion of the inventor and his attorney in accordance with the provisions of Rule 32 of the Patent Office Rules of Practice.

MEDTRONIC MINIMED, INC., per 37 C.F.R. §3.73(b), certifies that the evidentiary documents with respect to its ownership have been reviewed and that to the best of the undersign's knowledge and belief, title is in the assignee seeking this action.

MEDTRONIC MINIMED, INC., declares that 100% ownership is established by an assignment to be in the Regular Utility Patent Application, and that the Inventors are under an obligation to assign the application to **MEDTRONIC MINIMED, INC.**

Please direct all telephone calls to Richard Yoon at (818) 576-4110 and all correspondence relative to said application to the following address:

Medtronic MiniMed, Inc.
18000 Devonshire Street
Northridge, CA 91325

ASSIGNEE: **MEDTRONIC MINIMED, INC.**

Date: 3/30/2006

Signature:



Eric P. Geismar

Title: Vice President and Senior Counsel

Address: 18000 Devonshire Street
Northridge, CA 91325-1219



1/12

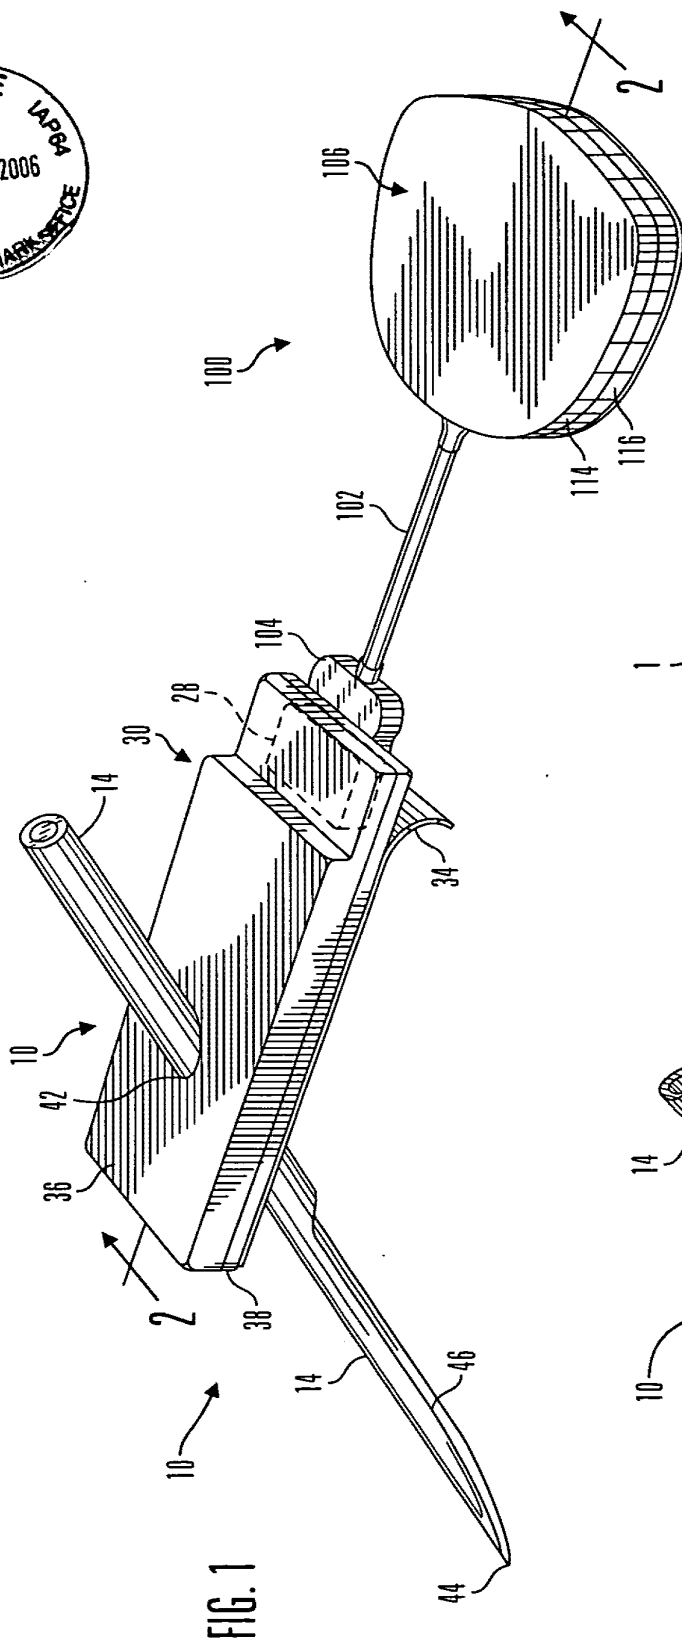


FIG. 1

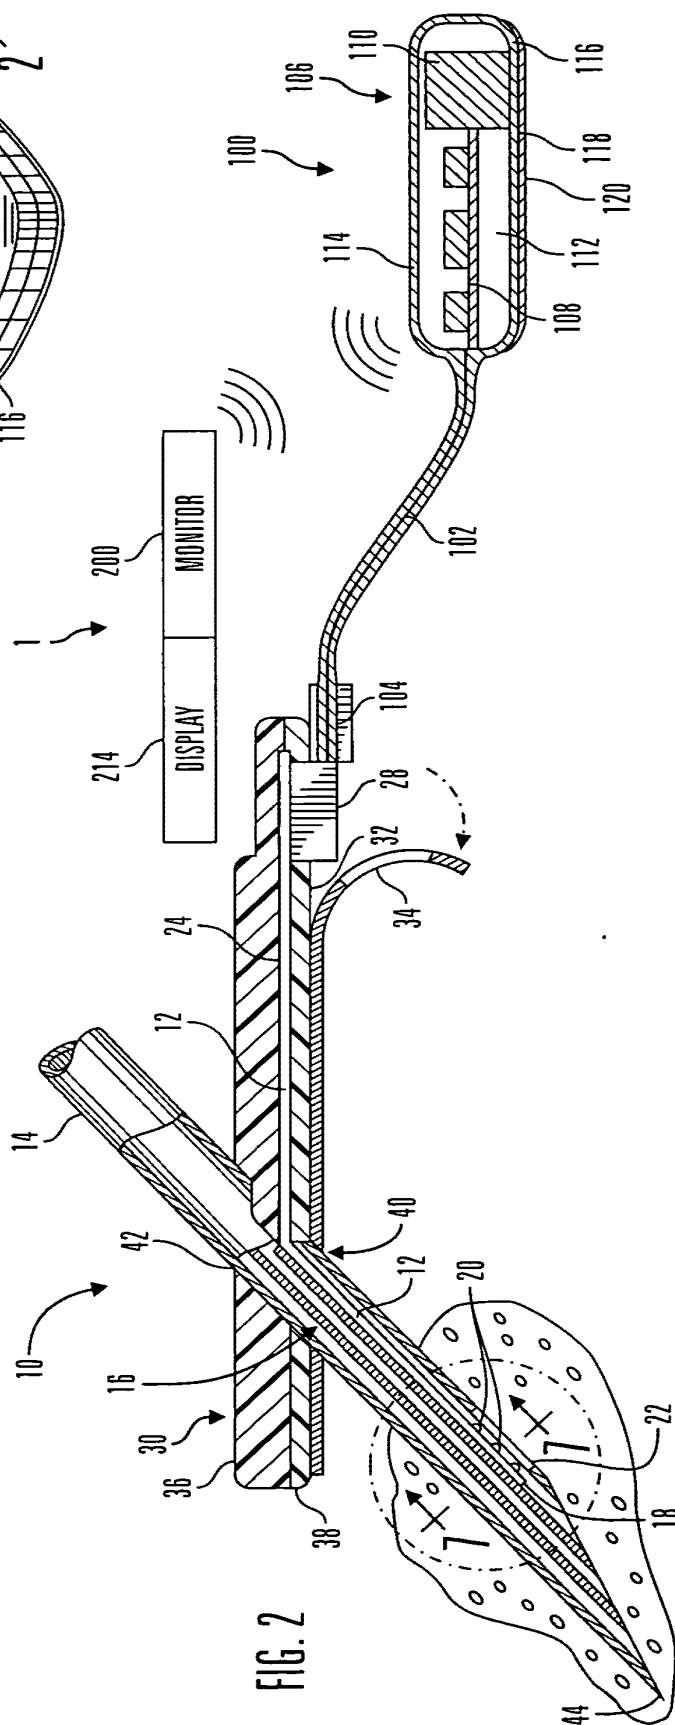


FIG. 2

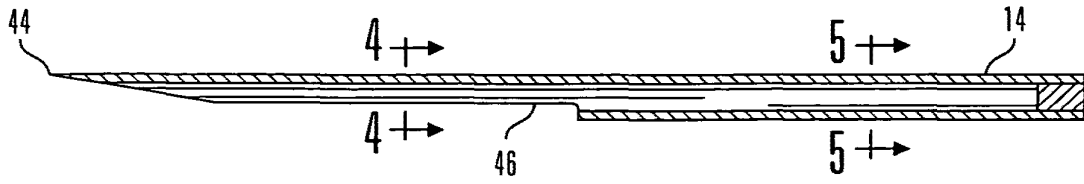


FIG. 3




FIG. 4




FIG. 5

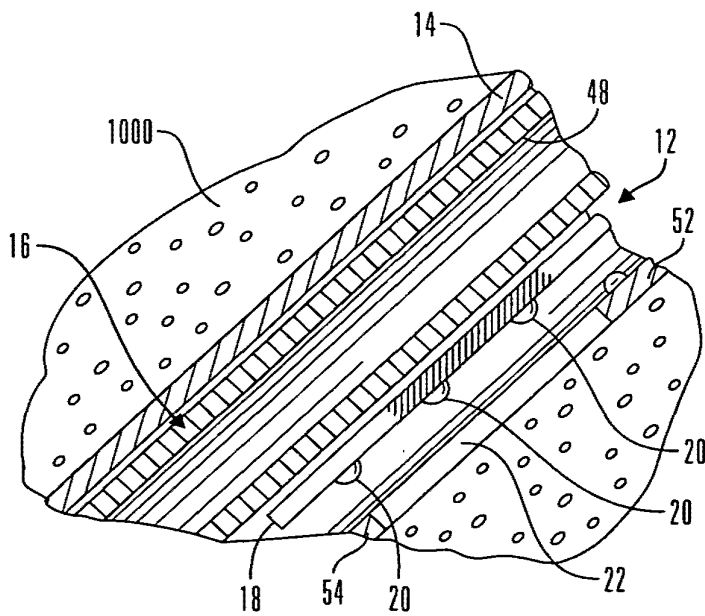


FIG. 6

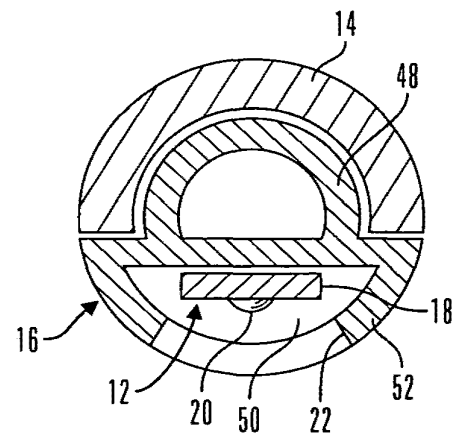


FIG. 7

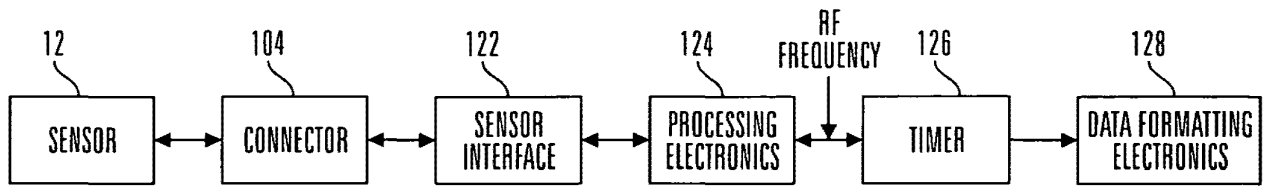
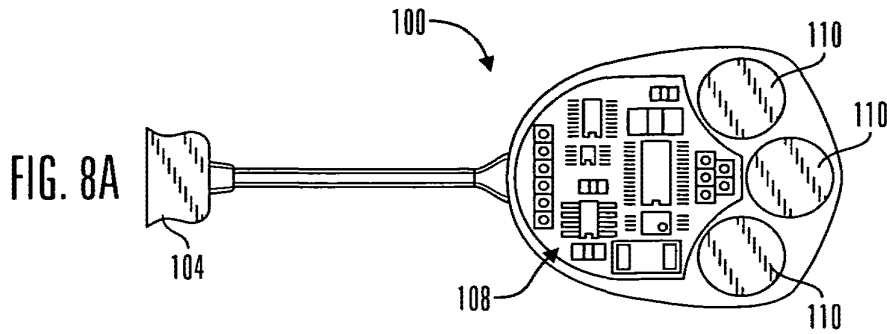


FIG. 8B

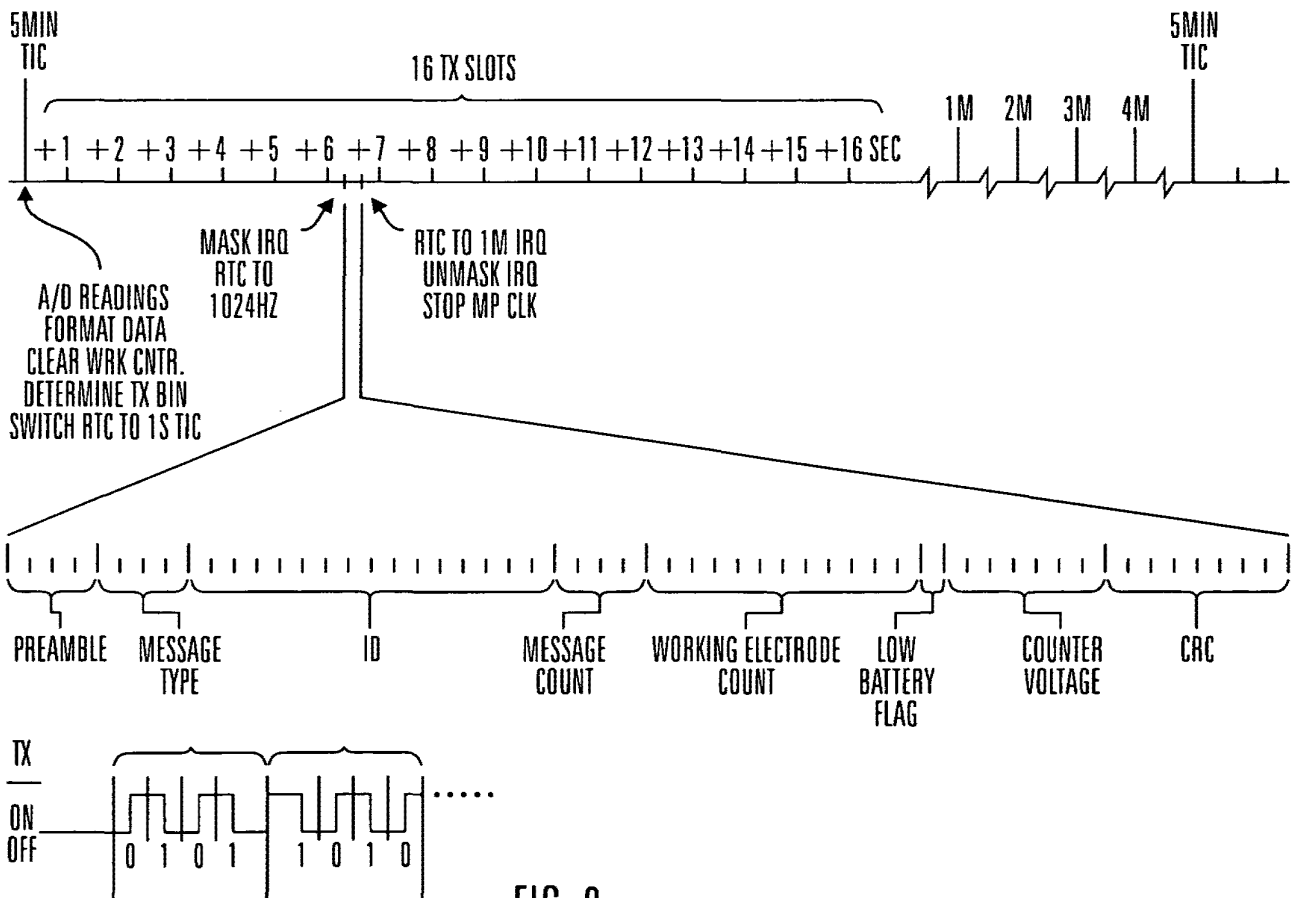


FIG. 9

FIG. 10


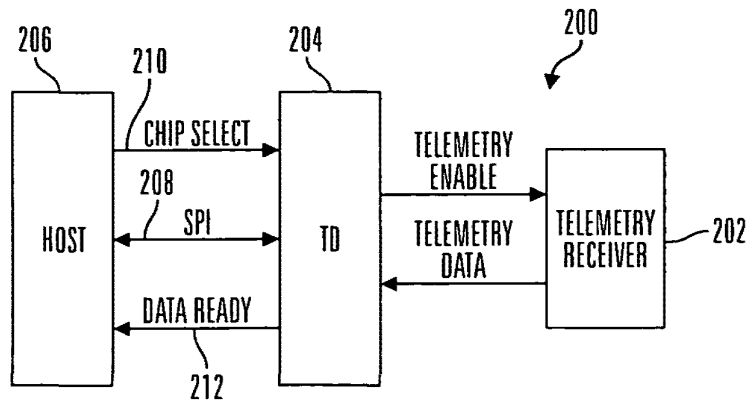


FIG. 11

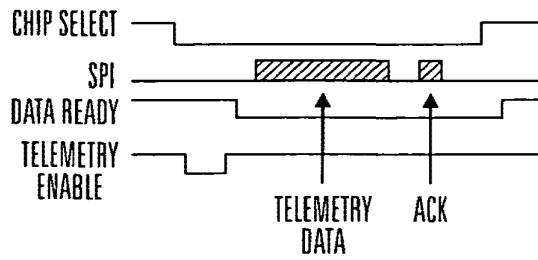

HOST INITIATES RF SESSION
TD WAKES UP
THROUGH RBO / INT
TD SIGNALS DATA READY

HOST SENDS COMMAND

TD SENDS STATUS
DATA TO HOST

TD ENABLES RF RECEIVER

TD COLLECTS RF DATA

HOST TERMINATES
RF SESSION

TD CLOSES OUT
RF SESSION AND
GOES TO SLEEP

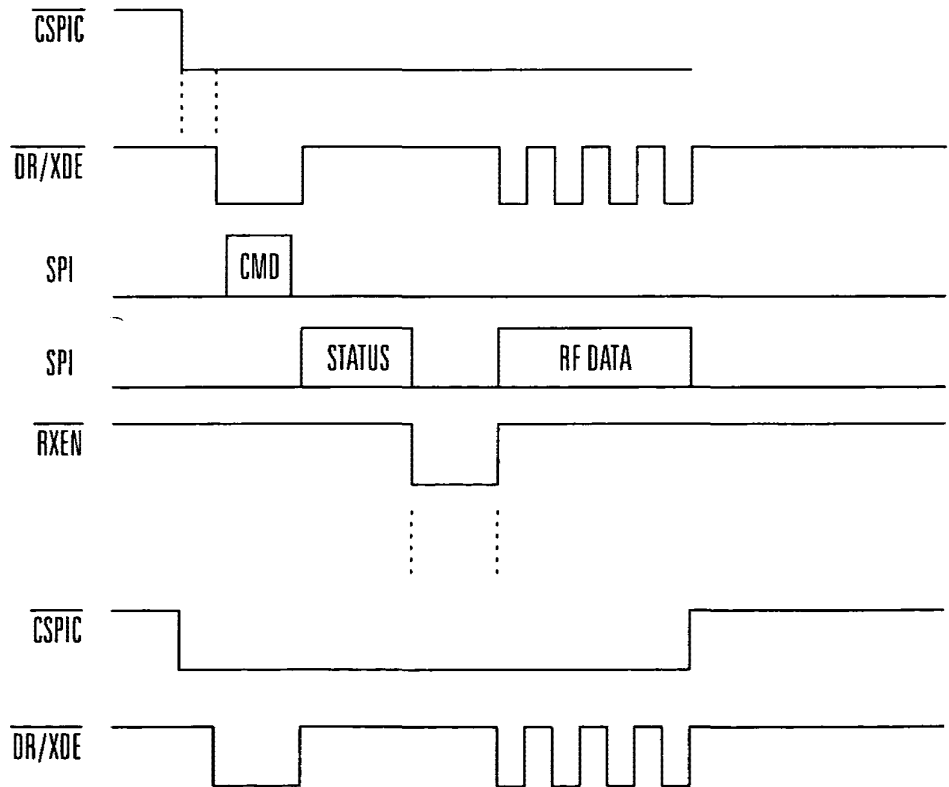


FIG. 12

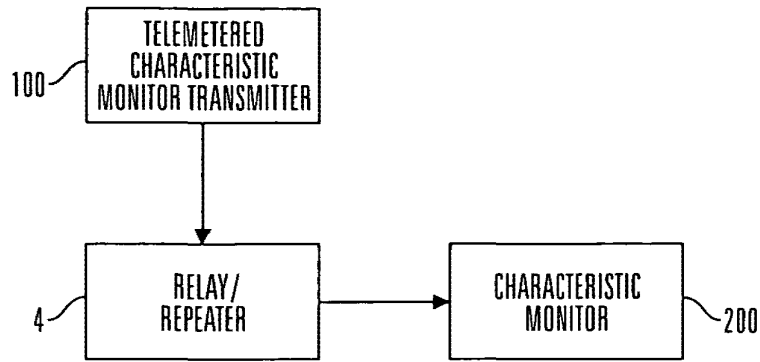


FIG. 13

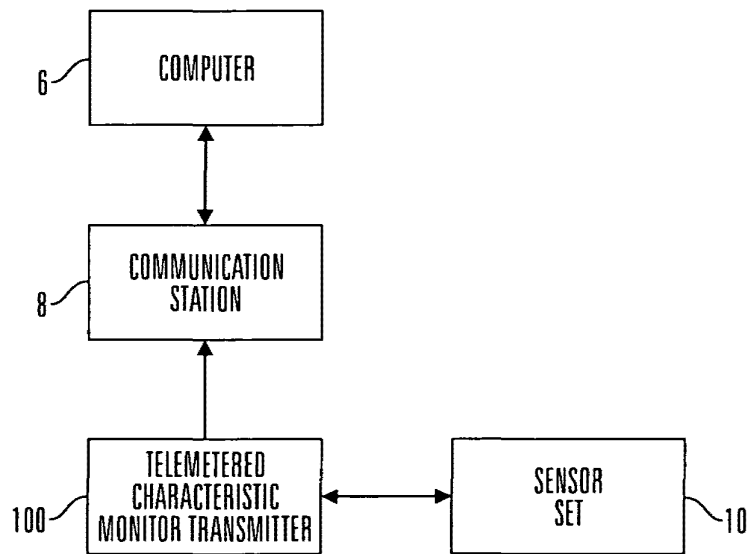


FIG. 14

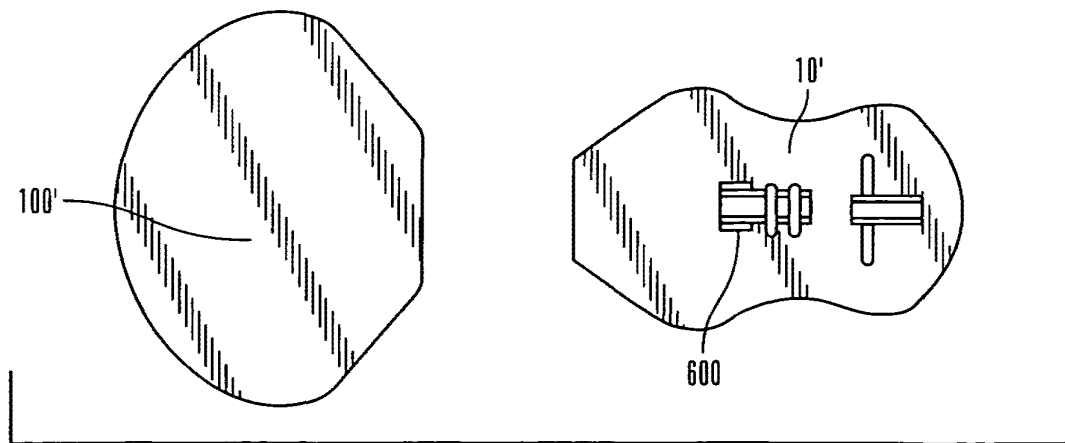
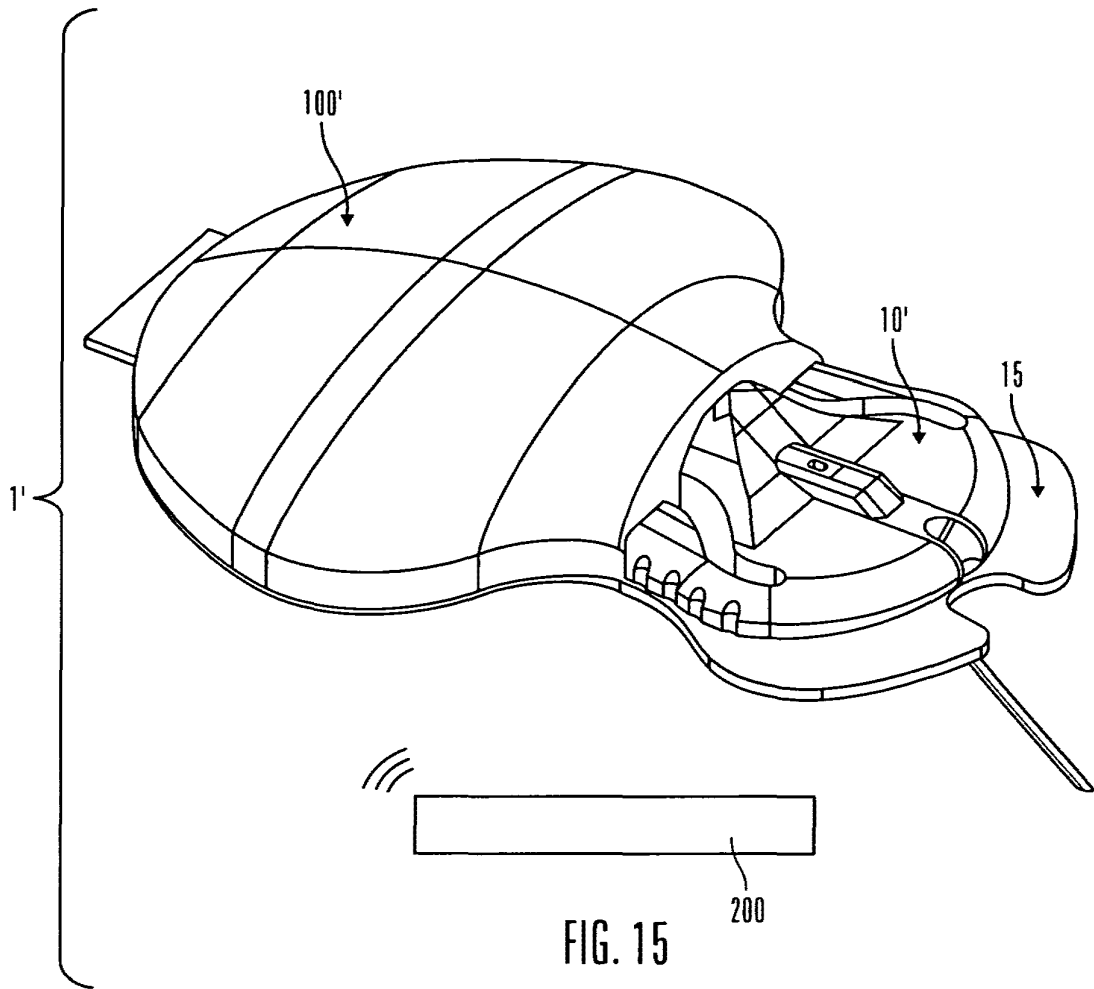


FIG. 16

7/12

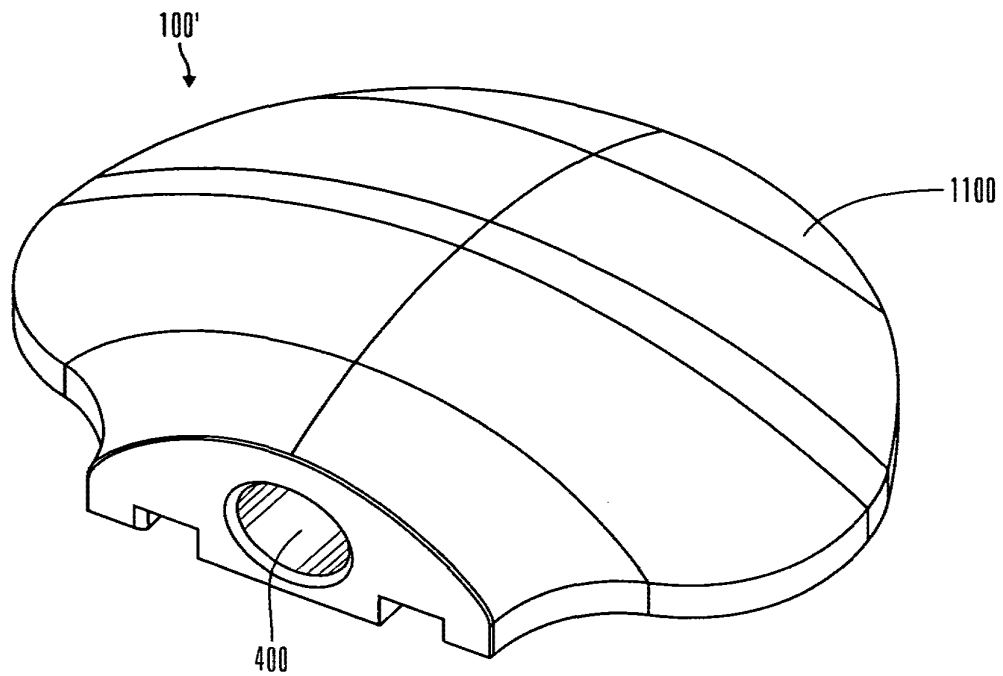


FIG. 17

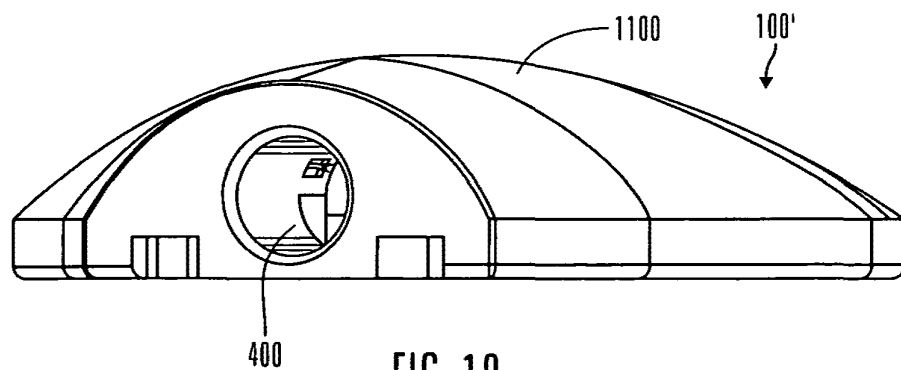


FIG. 18

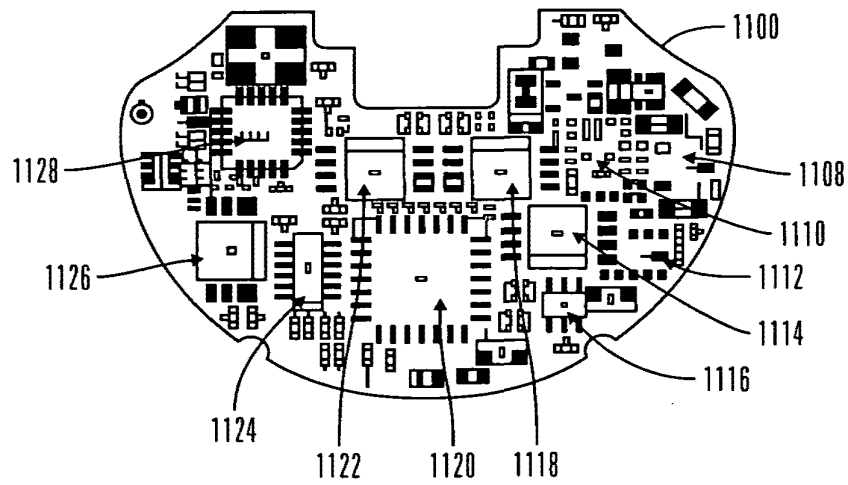


FIG. 19

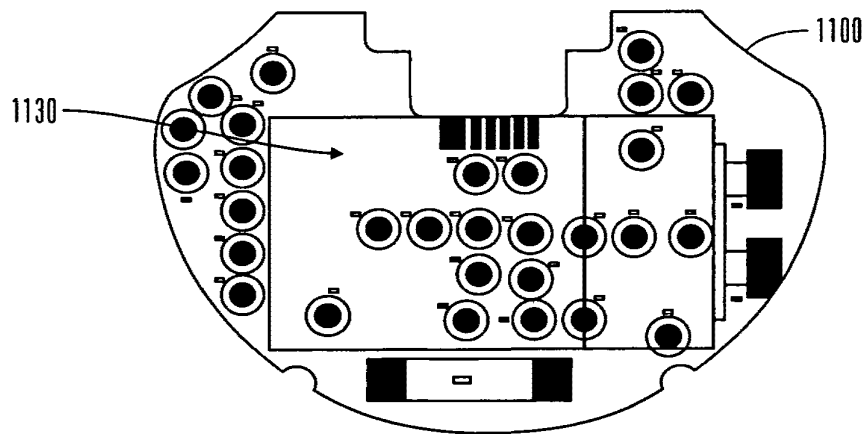


FIG. 20

9/12

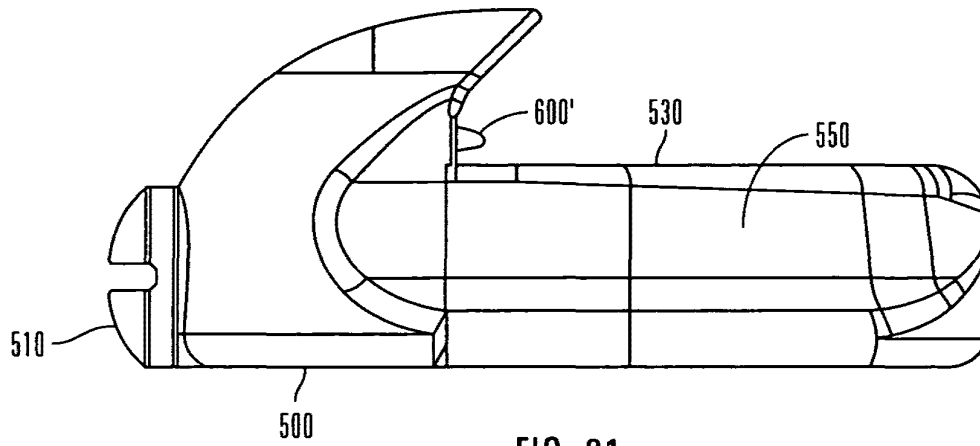


FIG. 21

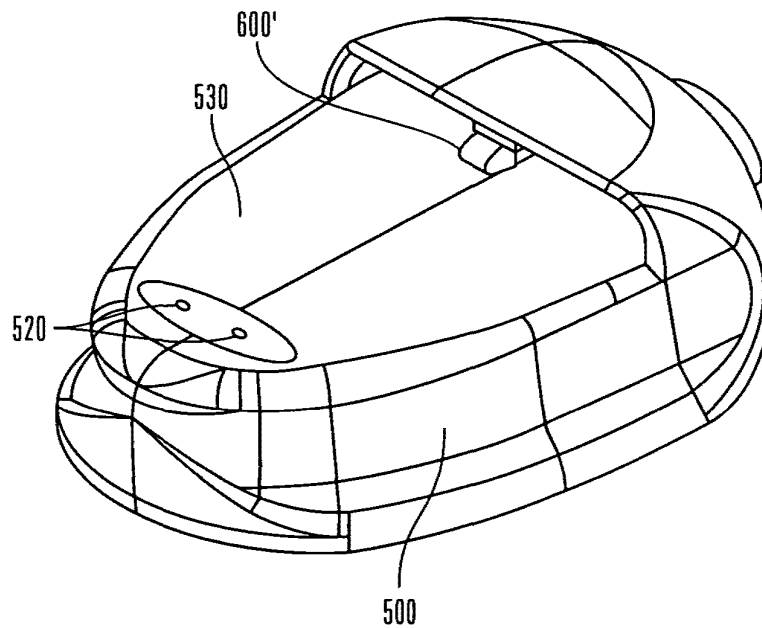


FIG. 22

+

10/12

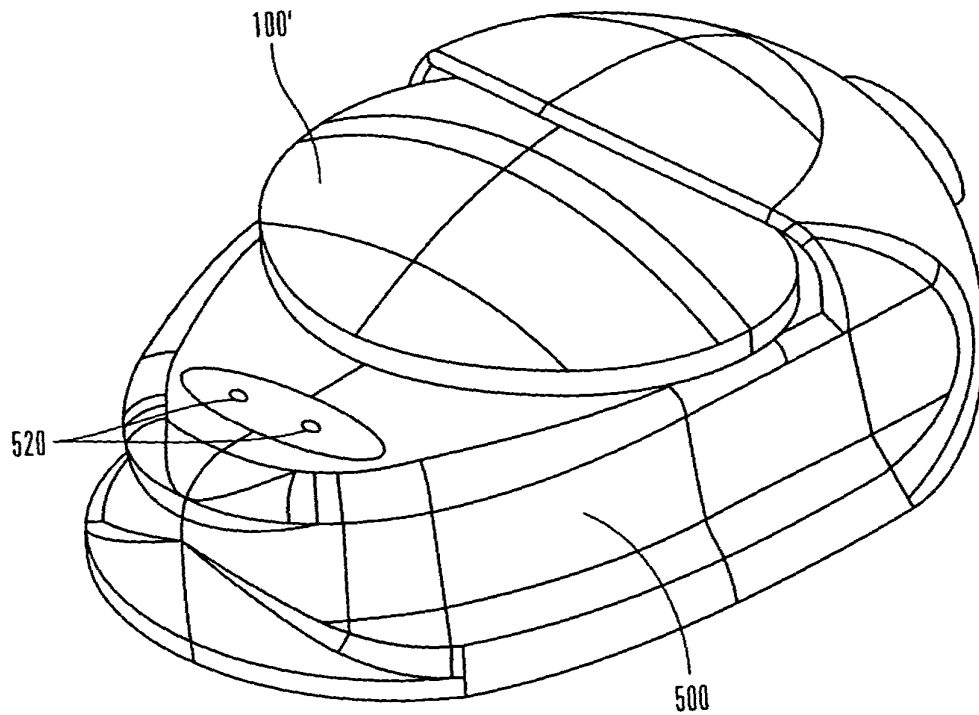


FIG. 23

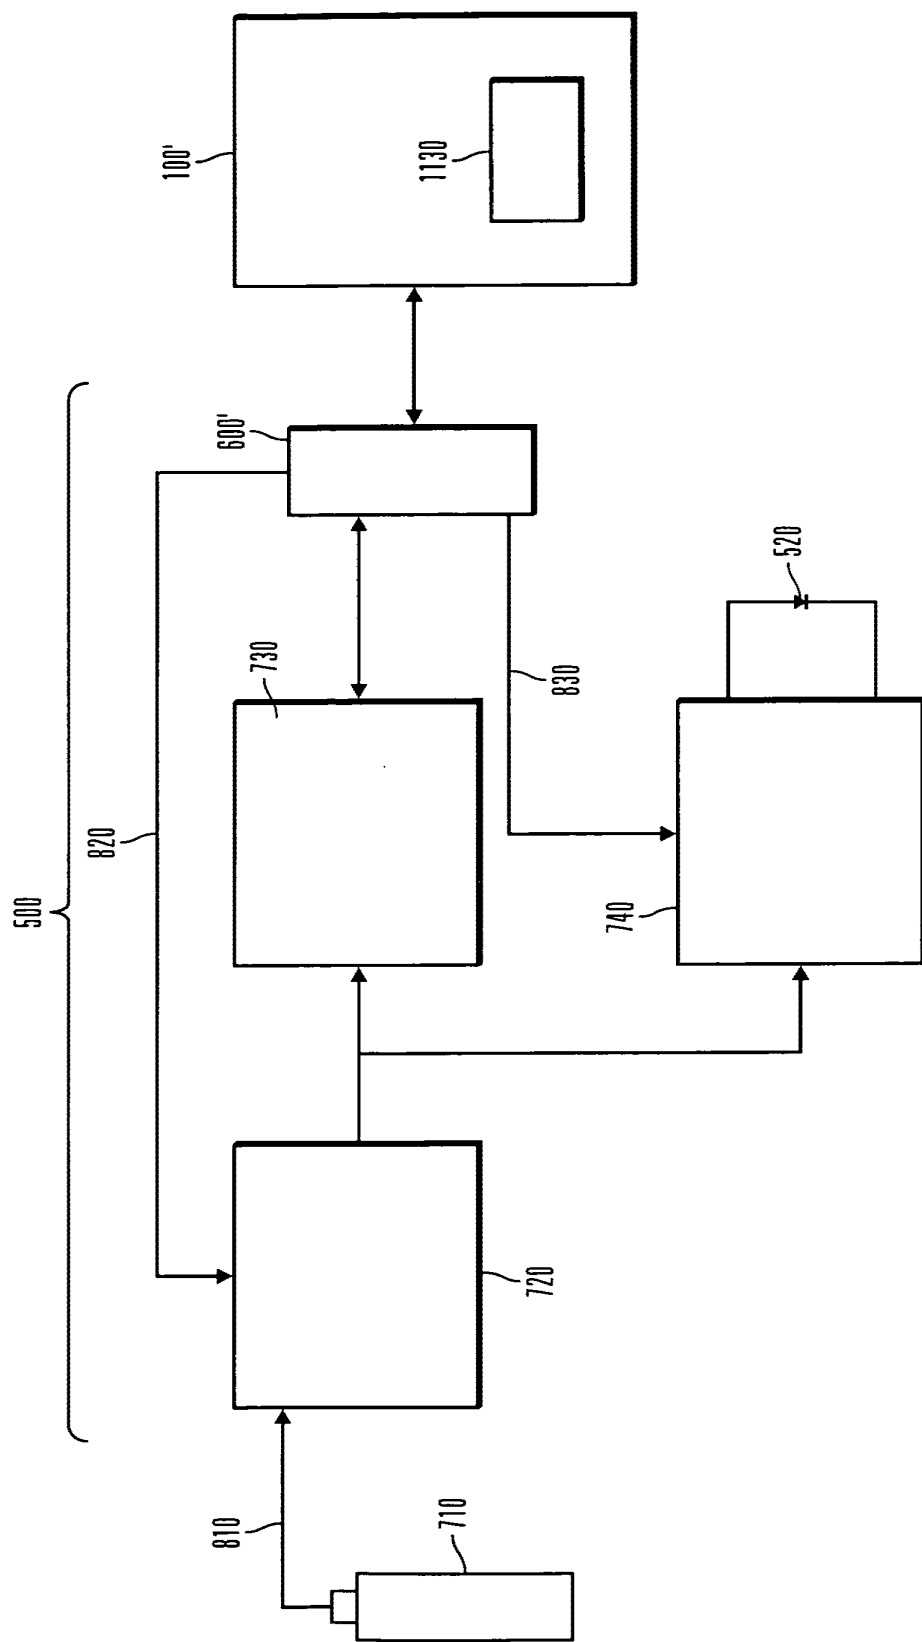


FIG. 24

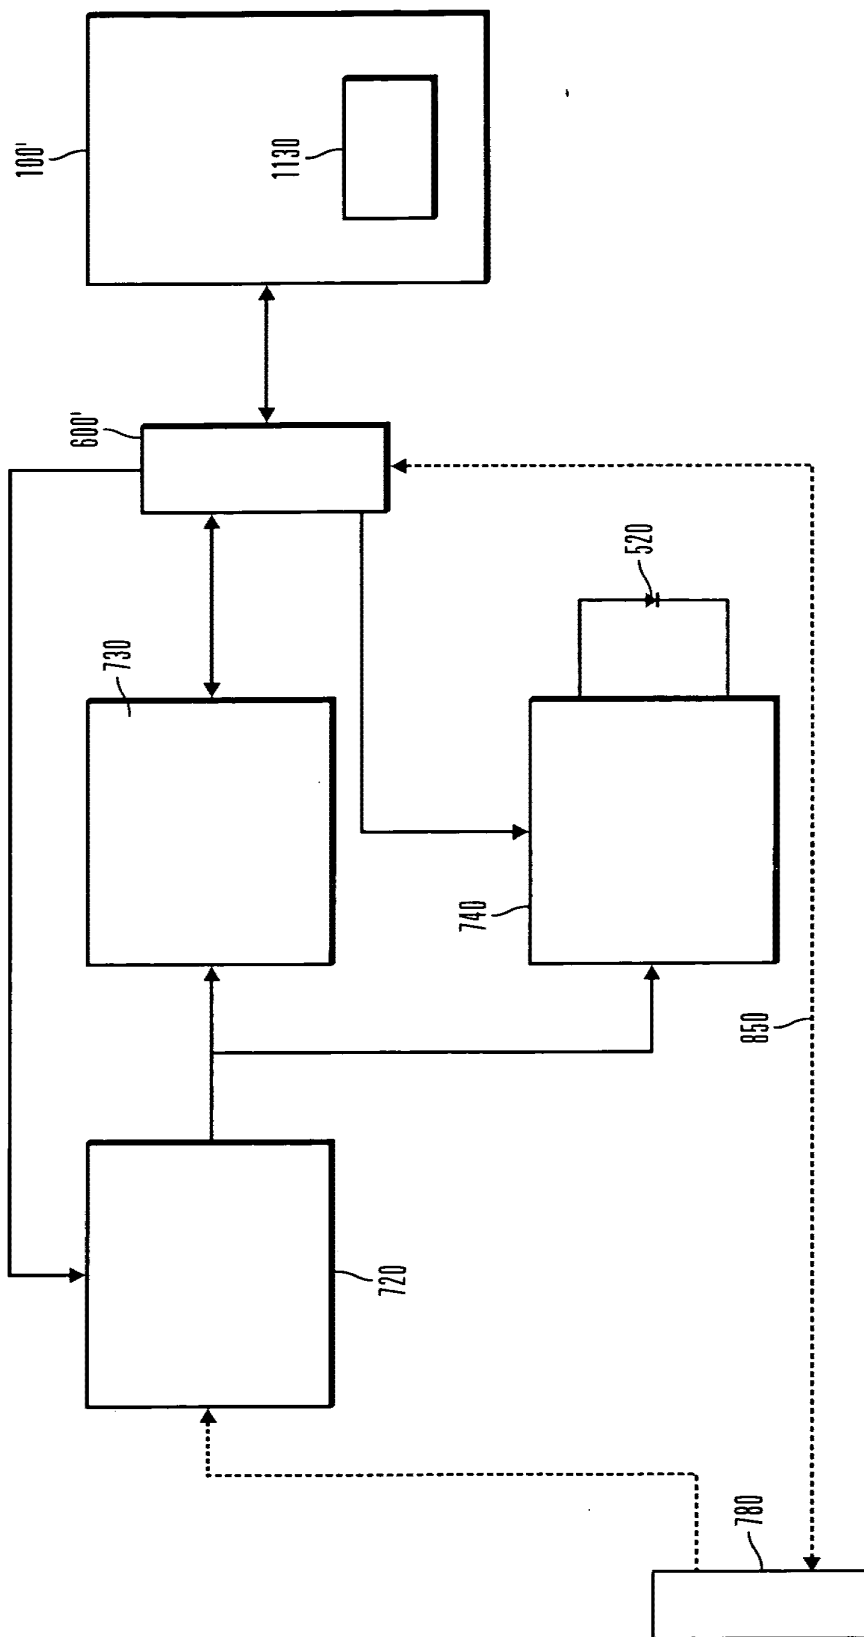


FIG. 25



IFW

PATENT
PD00291 CIP

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

In re Continuation-in-Part Application of:)
John J. Mastrototaro et al.) Group Art Unit : 2635
Serial No: 11/322,568)
Filed: December 30, 2005) Examiner: Unknown
For: TELEMETERED CHARACTERISTIC)
MONITOR SYSTEM AND METHOD)
OF USING THE SAME)

TRANSMITTAL OF INFORMATION DISCLOSURE STATEMENT

Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

Dear Sir:

1. ☒ The information disclosure statement submitted herewith is being filed within three months of the filing date of the application or date of entry into the national stage of an international application or before the mailing date of a first Office Action on the merits, whichever event occurs last. 37 C.F.R. §1.97(b).
2. ☐ The information disclosure statement transmitted herewith is being filed *after* three months of the filing date of this national application or the date of entry of the national stage as set forth in §1.491 in an international application or after the mailing date of the first Office Action on the merits, whichever event occurred last but *before* the mailing date of either:
 - (1) a final action under §1.113 or
 - (2) a notice of allowance under §1.311
 - (3) or an action that otherwise closes prosecution.

CERTIFICATION OR FEE

- A. Included with this transmittal is
- i. ☐ a certification (set forth below) in accordance with 37 C.F.R. §1.97(e). (If for any reason the certificate set forth below should be unsatisfactory, the Commissioner is provisionally authorized to charge the \$180 fee (37 C.F.R. §1.17(p)) to Deposit Account No. 50-0621. A copy of this sheet is enclosed.)

OR

- ii. ☐ the attached fee set forth in 37 C.F.R. §1.17(p) for submission of an information disclosure statement under §1.97(c). (\$180.00).
- 3. ☐ The information disclosure statement transmitted herewith is being filed *after* a final action under §1.113 or a notice of allowance under §1.311, or an action that otherwise closes prosecution, whichever occurs first, but before, or simultaneously with the payment of the issue fee.

CERTIFICATION, PETITION AND FEE

- A. In accordance with the requirements of 37 C.F.R. §1.97(d):
 - i. Set forth below is a certification as specified in 37 C.F.R. §1.97(e).
 - ii. Applicant hereby petitions for the consideration of the accompanying information disclosure statement. 37 C.F.R. §1.97(d)(ii).
 - iii. Applicant submits the petition fee set forth in §1.17(i)(1). (\$180.00).

CERTIFICATION

(Required if 2Ai or 3 above is marked)

- 4. I, the person signing below, certify
 - ☐ that each item of information contained in the information disclosure statement was first cited in the attached communication from a foreign patent office in a counterpart foreign application and was not made in any communication dated more than three months prior to the filing of the statement. 37 C.F.R. §1.97(e)(1).

OR


- ☐ that no item of information contained in the information disclosure statement was first cited in any communication from a foreign patent office in a counterpart foreign application or to the knowledge of the person signing the certification after making reasonable inquiry, was known to any individual designated in §1.56(c) more than three months prior to the filing of the statement. 37 C.F.R. §1.97(e)(2).

5. ■ If it should be determined that for any reason either an insufficient fee or an excessive has been paid, please charge any insufficiency or credit any overpayment necessary to ensure consideration of the information disclosure statement for the above-identified application to Deposit Account No. 50-0621. A copy of this petition is enclosed.

Respectfully submitted,

MEDTRONIC MINIMED, INC.


Date: March 10, 2006

By: 
Richard Yoon
Registration No. 42,247

18000 Devonshire Street
Northridge, CA 91325-1219
(818) 576-4110

I hereby certify that this correspondence is being deposited with the U.S. Postal Service with sufficient postage as first class mail in an envelope addressed to: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450, on the date indicated below.

on: March 10, 2006
Date of Deposit

Signature: 
Richard Yoon, Reg. No. 42,247

FORM PTO-1449
REV. 7.801


U.S. Department of Commerce
PATENT AND TRADEMARK OFFICE

Attorney Docket No.
PD00291 CIP

Serial No.
11/322,568

INFORMATION DISCLOSURE STATEMENT

(Use several sheets if necessary)



Applicant
John J. Mastrototaro et al.

Filing Date
December 30, 2005

Group
2635

U.S. PATENT DOCUMENTS

Examiner Initial		Document Number							Date	Name	Class	Sub-Class	Filing Date If Appropriate
	AA	4	4	9	4	9	5	0	1/22/85	R. E. Fischell	604	66	1/19/82
	AB	4	9	3	5	1	0	5	6/19/90	S. J. Churchouse	204	153.12	10/18/89
	AC	5	1	0	8	8	1	9	4/28/92	J. W. Heller et al.	428	195	2/14/90
	AD	5	3	9	1	2	5	0	2/21/95	P. S. Cheney II et al.	156	268	3/15/94
	AE	5	4	1	1	6	4	7	5/2/95	K. W. Johnson et al.	204	153.1	1/25/94
	AF	5	7	7	7	0	6	0	7/7/98	W. P. Van Antwerp	528	28	9/26/96
	AG	5	7	8	6	4	3	9	7/28/98	W. P. Van Antwerp et al.	528	77	10/24/96
	AH	5	9	6	5	3	8	0	10/12/99	A. Heller et al.	435	14	1/12/99

FOREIGN PATENT DOCUMENTS

		Document Number							Date	Country	Class	Sub-Class	Translation	
													Yes	No
	AI													
	AJ													

OTHER DOCUMENTS

AK	
AL	

Examiner

Date Considered

* EXAMINER: Initial if reference considered, whether or not citation is in conformance with MPEP 609; Draw line through citation if not in conformance and not considered. Include copy of this form with next communication to applicant.

FORM PTO-1449 IREV. 7.801 U.S. Department of Commerce PATENT AND TRADEMARK OFFICE INFORMATION DISCLOSURE STATEMENT (Use several sheets if necessary)		Attorney Docket No. PD00291 CIP	Serial No. 11/322.568
		Applicant John J. Mastrototaro et al.	
		Filing Date December 30, 2005	Group 2635

U.S. PATENT DOCUMENTS												
Examiner Initial	Document Number	Date	Name	Class	Sub-Class	Filing Date If Appropriate						
AA												

FOREIGN PATENT DOCUMENTS												
Document Number	Date	Country	Class	Sub-Class	Translation							
					Yes	No						
AB	9 5 2 8 8 7 8	11/2/95	PCT	A61B	5/05							
AC	9 8 5 6 2 9 3	12/17/98	PCT	A61B	5/04							
AD	9 9 4 5 3 7 5	9/10/99	PCT	G01N	27/327							
AE	9 9 4 5 3 8 7	9/10/99	PCT	G01N	33/487							
AF	9 9 5 6 6 1 3	11/11/99	PCT	A61B	5/00							
AG	0 0 9 8 5 9 2	1/18/84	EP	A61M	5/00							
AH	0 6 8 0 7 2 7	11/08/95	EP	A61B	5/00							

OTHER DOCUMENTS	
AI	Rebrin, Kerstin et al.. "Subcutaneous glucose predicts plasma glucose independent of insulin: implications for continuous monitoring". <u>The American Physiological Society</u> (1999), pp. E561-E571
AJ	Velho, G. et al.. "Strategies for calibrating a subcutaneous glucose sensor". <u>Biomed. Biochim. Acta</u> 48 (1989), pp. 957-964

Examiner	Date Considered
----------	-----------------

* EXAMINER: Initial if reference considered, whether or not citation is in conformance with MPEP 609; Draw line through citation if not in conformance and not considered. Include copy of this form with next communication to applicant.

FORM PTO-1449 IREV. 7.801 INFORMATION DISCLOSURE STATEMENT (Use several sheets if necessary)		U.S. Department of Commerce PATENT AND TRADEMARK OFFICE		Attorney Docket No. PD00291 CIP		Serial No. 11/322.568	
		Applicant John J. Mastrototaro et al.					
		Filing Date December 30, 2005				Group 2635	

U.S. PATENT DOCUMENTS												
Examiner Initial	Document Number	Date	Name	Class	Sub-Class	Filing Date If Appropriate						
AA												

FOREIGN PATENT DOCUMENTS												
Document Number	Date	Country	Class	Sub-Class	Translation							
					Yes	No						
AB	9 6 3 7 2 4 6	11/28/96	PCT	A61M	5/20							
AC	0 2 0 5 8 5 37	8/1/02	PCT	A61B								
AD	1 3 3 8 2 9 5	8/27/03	EP	A61M	5/172							

OTHER DOCUMENTS	
AE	International Search Report for International Application No. PCT/US96/06649 filed 10 May 1995.
AF	Reach, G. et al., "A Method for Evaluating <i>in vivo</i> the Functional Characteristics of Glucose Sensors", <u>Biosensors 2</u> (Elsevier Applied Science Publishers Ltd., England - 1986), pp. 211-220
AG	Abel, P. et al., "Experience with an implantable glucose sensor as a prerequisite of an artificial beta cell", <u>Biomed. Biochim. Acta</u> 43 (1984) 5, pp. 577-584
AH	Boguslavsky, L. et al., "Applications of redox polymers in biosensors", <u>Solid State Ionics</u> 60 (Elsevier Science Publishers B.V., North-Holland), (1993), pp. 189-197
AI	Geise, R.J. et al., "Electropolymerized 1,3-diaminobenzene for the construction of a 1,1'-dimethylferrocene mediated glucose biosensor", <u>Analytica Chimica Acta</u> , 281 (Elsevier Science Publishers B.V., Amsterdam), (1993), pp. 467-473
AJ	Gernet, S. et al., "Fabrication and Characterization of a Planar Electrochemical Cell and Its Application as a Glucose Sensor", <u>Sensors and Actuators</u> , 18 (Elsevier Sequoia, The Netherlands - 1989), pp. 59-70
AK	Gernet, S. et al., "A Planar Glucose Enzyme Electrode", <u>Sensors and Actuators</u> , 17 (Elsevier Sequoia, The Netherlands - 1989), pp. 537-540
AL	Kanapieniene, J.J. et al., "Miniature glucose biosensor with extended linearity", <u>Sensors and Actuators B</u> , 10, (Elsevier Sequoia), (1992), pp. 37-40

Examiner	Date Considered
----------	-----------------

* EXAMINER: Initial if reference considered, whether or not citation is in conformance with MPEP 609; Draw line through citation if not in conformance and not considered. Include copy of this form with next communication to applicant.

FORM PTO-1449 IREV. 7.801		U.S. Department of Commerce PATENT AND TRADEMARK OFFICE		Attorney Docket No. PD00291 CIP	Serial No. 11/322,568
INFORMATION DISCLOSURE STATEMENT (Use several sheets if necessary)				Applicant John J. Mastrototaro et al.	
				Filing Date December 30, 2005	Group 2635

U.S. PATENT DOCUMENTS									
Examiner Initial	Document Number	Date	Name	Class	Sub-Class	Filing Date If Appropriate			
AA									

FOREIGN PATENT DOCUMENTS									
Document Number	Date	Country	Class	Sub-Class	Translation				
AB					Yes No				

OTHER DOCUMENTS	
AC	Gorton, L. et al., "Amperometric glucose sensors based on immobilized glucose-oxidizing enzymes and chemically modified electrodes". <u>Analytica Chimica Acta</u> , 249 (Elsevier Science Publishers BV, Amsterdam), (1991), pp. 43-54
AD	Gorton, L. et al., "Amperometric Biosensors Based on an Apparent Direct Electron Transfer Between Electrodes and Immobilized Peroxidases". (Plenary Lecture at Department of Analytical Chemistry, University of Lund - Sweden), (August 1992), Vol. 117, pp. 1235-1241
AE	Gough, D. et al., "Two-Dimensional Enzyme Electrode Sensor for Glucose". (American Chemical Society). Reprinted from <u>Analytical Chemistry</u> (1985) 57, pp. 2351-2357
AF	Gregg, B.A. et al., "Cross-Linked Redox Gels Containing Glucose Oxidase for Amperometric Biosensor Applications". <u>Anal. Chem.</u> 62, (Department of Chemical Engineering, University of Texas, Austin), (American Chemical Society), (1990), pp. 258-263
AG	Gregg, B.A. et al., "Redox Polymer Films Containing Enzymes. 1. A Redox-Conducting Epoxy Cement: Synthesis, Characterization, and Electrocatalytic Oxidation of Hydroquinone, <u>J. Phys. Chem.</u> 95, (1991), pp. 5970-5975
AH	Heller, A., "Electrical Wiring of Redox Enzymes", <u>Accounts of Chemical Research</u> , (American Chemical Society), (May 1990) (Vol. 23, Number 5), pp. 128-134
AI	Johnson, K.W. et al., "In vivo evaluation of an electroenzymatic glucose sensor implanted in subcutaneous tissue", <u>Biosensors & Bioelectronics</u> 7, (Elsevier Science Publishers Ltd.), (1992), pp. 709-714
AJ	Jönsson, G. et al., "An Electrochemical Sensor for Hydrogen Peroxide Based on Peroxidase Adsorbed on a Spectrographic Graphite Electrode", <u>Electroanalysis</u> 1, (VCH Publishers, Inc.), (1989), pp. 465-468

Examiner	Date Considered
----------	-----------------

* EXAMINER: Initial if reference considered, whether or not citation is in conformance with MPEP 609; Draw line through citation if not in conformance and not considered. Include copy of this form with next communication to applicant.

FORM PTO-1449
REV. 7.801

U.S. Department of Commerce
PATENT AND TRADEMARK OFFICE

Attorney Docket No.
PD00291 CIP

Serial No.
11/322,568

INFORMATION DISCLOSURE STATEMENT

(Use several sheets if necessary)

Applicant
John J. Mastrototaro et al.

Filing Date
December 30, 2005

Group
2635

U.S. PATENT DOCUMENTS

Examiner Initial		Document Number	Date	Name	Class	Sub-Class	Filing Date If Appropriate
	AA						

FOREIGN PATENT DOCUMENTS

		Document Number	Date	Country	Class	Sub-Class	Translation	
							Yes	No
	AB							

OTHER DOCUMENTS

AC	Kawamori, R. et al., "Perfect Normalization of Excessive Glucagon Responses to Intravenous Arginine in Human Diabetes Mellitus with the Artificial Beta-Cell", <u>Rapid Publication from Diabetes</u> , Vol. 29, (September 1980), pp. 762-765
AD	Kimura, J. et al., "An Immobilized Enzyme Membrane Fabrication Method using an Ink Jet Nozzle", <u>Biosensors 4</u> , (Elsevier Science Publishers Ltd. - England), (1988), pp. 41-52
AE	Koudelka, M. et al., "In-vivo Behaviour of Hypodermically Implanted Microfabricated Glucose Sensors", <u>Biosensors & Bioelectronics 6</u> (Elsevier Science Publishers Ltd., England - 1991), pp. 31-36
AF	Mastrototaro, John J. et al., "An electroenzymatic glucose sensor fabricated on a flexible substrate", <u>Sensors and Actuators B. 5</u> (Elsevier Sequoia - 1991), pp. 139-144
AG	Mastrototaro, John J. et al., "An Electroenzymatic Sensor Capable of 72 Hour Continuous Monitoring of Subcutaneous Glucose", Presentation given at the 14 th International Diabetes Federation Congress in Washington, D.C., (June 23-28, 1991), 19 pages
AH	McKean, B.D., et al., "A Telemetry-Instrumentation System for Chronically Implanted Glucose and Oxygen Sensors", <u>IEEE Transactions on Biomedical Engineering</u> , (July 1988), Vol. 35, No. 7, pp. 526-532
AI	Monroe, D., "Novel implantable glucose sensors", <u>ACL</u> , (December 1989), pp. 8-16
AJ	Morff, R.J. et al., "Microfabrication of Reproducible, Economical, Electroenzymatic Glucose Sensors", <u>Annual International Conference of IEEE Engineering in Medicine and Biology Society</u> , (1990), Vol. 12, No. 2, pp. 0483-0484
AK	Nakamoto, S. et al., "A Lift-Off Method for Patterning Enzyme-Immobilized Membranes in Multi-Biosensors", <u>Sensors and Actuators</u> , 13, (Elsevier Sequoia), (1988), pp. 165-172
AL	Nishida, K. et al., "Clinical applications of the wearable artificial endocrine pancreas with the newly designed needle-type glucose sensor", (Elsevier Science B.V.), (1994), pp. 353-358

Examiner

Date Considered

* EXAMINER: Initial if reference considered, whether or not citation is in conformance with MPEP 609; Draw line through citation if not in conformance and not considered. Include copy of this form with next communication to applicant.

FORM PTO-1449 IREV. 7.801		U.S. Department of Commerce PATENT AND TRADEMARK OFFICE			Attorney Docket No. PD00291 CIP		Serial No. 11/322,568			
INFORMATION DISCLOSURE STATEMENT (Use several sheets if necessary)					Applicant John J. Mastrototaro et al.					
					Filing Date December 30, 2005		Group 2635			
U.S. PATENT DOCUMENTS										
Examiner Initial		Document Number			Date	Name	Class	Sub-Class	Filing Date If Appropriate	
	AA									
FOREIGN PATENT DOCUMENTS										
		Document Number			Date	Country	Class	Sub-Class	Translation	
									Yes	No
	AB									
OTHER DOCUMENTS										
	AC	Shichiri, M. et al., "An artificial endocrine pancreas - problems awaiting solution for long-term clinical applications of a glucose sensor", <i>Frontiers Med. Biol. Engng. (VSP)</i> , (1991), Vol. 3., No. 4, pp. 283-292								
	AD	Shichiri, M. et al., "Wearable Artificial Endocrine Pancreas with Needle-Type Glucose Sensor", <i>The Lancet</i> , (November 20, 1982), pp. 1129-1131								
	AE	Shichiri, M. et al., "Telemetry Glucose Monitoring Device with Needle-Type Glucose Sensor: A Useful Tool for Blood Glucose Monitoring in Diabetic Individuals", <i>Diabetes Care</i> , (May-June 1986), Vol. 9, No. 3, pp. 298-301								
	AF	Shichiri, M. et al., "Normalization of the Paradoxical Secretion of Glucagon in Diabetics Who Were Controlled by the Artificial Beta Cell", <i>Diabetes</i> , (April 1979), Vol., 28, pp. 272-275								
	AG	Shichiri, M. et al., "Closed-Loop Glycemic Control with a Wearable Artificial Endocrine Pancreas Variations in Daily Insulin Requirements to Glycemic Response", <i>Rapid Publication from Diabetes</i> , Vol. 33, (December 1984), pp. 1200-1202								
	AH	Shichiri, M. et al., "In Vivo Characteristics of Needle-Type Glucose Sensor - Measurements of Subcutaneous Glucose Concentrations in Human Volunteers-", <i>Hormone and Metabolic Research</i> , (Thieme Medical Publishers, Inc.), Supplement Series Vol. No. 20, (1988), pp. 17 - 20								
	AI	Shichiri, M. et al., "A Needle-Type Glucose Sensor - A Valuable Tool Not Only for a Self-Blood Glucose Monitoring But for a Wearable Artificial Pancreas-", <i>Life Support Systems</i> , Proceedings XI Annual Meeting ESAO Alpbach-Innsbruck Austria, (September 1984), Vol. 2, Supplement 1, pp. 7-9								
	AJ	Shichiri, M. et al., "The Wearable Artificial Endocrine Pancreas with a Needle-Type Glucose Sensor: Perfect Glycemic Control in Ambulatory Diabetics", <i>Acta Paediatr Jpn</i> 26, (1984), pp. 359-370								
	AK	Shichiri, M. et al., "Glycaemic Control in Pancreatectomized Dogs with a Wearable Artificial Endocrine Pancreas", <i>Diabetologica</i> 24, (1983), pp. 179-184								
	AL	Shichiri, M. et al., "Membrane design for extending the long-life of an implantable glucose sensor", <i>Diab. Nutr. Metab.</i> , Vol. 2, No. 4, (1989), pp. 309-313								
Examiner					Date Considered					
* EXAMINER: Initial if reference considered, whether or not citation is in conformance with MPEP 609; Draw line through citation if not in conformance and not considered. Include copy of this form with next communication to applicant.										

FORM PTO-1449 REV. 7.801		U.S. Department of Commerce PATENT AND TRADEMARK OFFICE		Attorney Docket No. PD00291 CIP		Serial No. 11/322,568	
INFORMATION DISCLOSURE STATEMENT (Use several sheets if necessary)				Applicant John J. Mastrototaro et al.			
				Filing Date December 30, 2005		Group 2635	
U.S. PATENT DOCUMENTS							
Examiner Initial	AA	Document Number	Date	Name	Class	Sub-Class	Filing Date If Appropriate
FOREIGN PATENT DOCUMENTS							
		Document Number	Date	Country	Class	Sub-Class	Translation
							Yes No
OTHER DOCUMENTS							
AC	Shinkai, S. et al., "Molecular Recognition of Mono- and Di-saccharides by Phenylboronic Acids in Solvent Extraction and as a Monolayer", J. Chem. Soc., Chem. Commun., (1991), pp. 1039-1041						
AD	Tamiya, E. et al., "Micro Glucose Sensors Using Electron Mediators Immobilized on a Polypyrrole-Modified Electrode", Sensors and Actuators, 18, (Elsevier Sequoia), (1989), pp. 297-307						
AE	Tsukagoshi, K. et al., "Specific Complexation with Mono- and Disaccharides that Can be Detected by Circular Dichroism", J. Org. Chem 56, (1991), pp. 4089-4091						
AF	Urban, G. et al., "Miniaturized multi-enzyme biosensors integrated with pH sensors on flexible polymer carriers for <i>in vivo</i> applications", Biosensors & Bioelectronics 7, (Elsevier Science Publishers Ltd.), (1992), pp. 733-739						
AG	Urban, G. et al., "Miniaturized thin-film biosensors using covalently immobilized glucose oxidase", Biosensors & Bioelectronics 6, (Elsevier Science Publishers Ltd.), (1991), pp. 555-562						
AH	Velho, G. et al., "In vivo calibration of a subcutaneous glucose sensor for determination of subcutaneous glucose kinetics", Diab. Nutr. Metab. 3 (1988), pp. 227-233						
AI	Yokoyama, K., "Integrated Biosensor for Glucose and Galactose", Analytica Chimica Acta, 218, (Elsevier Science Publishers B.V. - Amsterdam), (1989), pp. 137-142						
AJ	Nishida, K. et al., "Development of a ferrocene-mediated needle-type glucose sensor covered with newly designed biocompatible membrane, 2-methacryloyloxyethyl phosphorylcholine -co-n-butyl methacrylate", Medical Progress through Technology 21, (Kluwer Academic Publishers), (1995), pp. 91-103						
AK	Koudelka, M. et al., "Planar Amperometric Enzyme-Based Glucose Microelectrode", <u>Sensors and Actuators</u> , 18 (Elsevier Sequoia, The Netherlands - 1989), pp. 157-165						
Examiner				Date Considered			
* EXAMINER: Initial if reference considered, whether or not citation is in conformance with MPEP 609; Draw line through citation if not in conformance and not considered. Include copy of this form with next communication to applicant.							

FORM PTO-1449 REV. 7.801	U.S. Department of Commerce PATENT AND TRADEMARK OFFICE	Attorney Docket No. PD00291 CIP	Serial No. 11/322,568
INFORMATION DISCLOSURE STATEMENT (Use several sheets if necessary)		Applicant John J. Mastrototaro et al.	
		Filing Date December 30, 2005	Group 2635

U.S. PATENT DOCUMENTS

Examiner Initial		Document Number	Date	Name	Class	Sub-Class	Filing Date If Appropriate
	AA						

FOREIGN PATENT DOCUMENTS

		Document Number	Date	Country	Class	Sub-Class	Translation
							Yes No
	AB						

OTHER DOCUMENTS

AC	Yamasaki, Y. et al., "Direct measurement of whole blood glucose by a needle-type sensor", Clinica Chimica Acta, 93, (Elsevier Science Publishers B.V.), (1989), pp. 93-98
AD	Sternberg, R. et al., "Study and Development of Multilayer Needle-type Enzyme-based Glucose Microsensors", Biosensors 4, (Elsevier Science Publishers Ltd - England), (1988), pp. 27-40
AE	Shaw, G.W. et al., "In vitro testing of a simply constructed, highly stable glucose sensor suitable for implantation in diabetic patients", Biosensors & Bioelectronics 6, (Elsevier Publishers Ltd - England), (1991), pp. 401-406
AF	Poitout, V. et al., "A glucose monitoring system for on line estimation in man of blood glucose concentration using a miniaturized glucose sensor implanted in the subcutaneous tissue and a wearable control unit", Diabetologia 36, (1993), pp. 658-663
AG	Hashiguchi, Y. et al., "Development of a Miniaturized Glucose Monitoring System by Combining a Needle-Type Glucose Sensor with Microdialysis Sampling Method Long-term subcutaneous tissue glucose monitoring in ambulatory diabetic patients", Diabetes Care, (1994), Vol. 17, No. 5, pp. 387-389
AH	Jobst, G. et al., "Thin-Film Microbiosensors for Glucose-Lactate Monitoring", Anal. Chem. 68, (American Chemical Society), (1996), Vol. 68, No. 18, pp. 3173-3179
AI	Shults, M.C. et al., "A Telemetry-Instrumentation System for Monitoring Multiple Subcutaneously Implanted Glucose Sensors", IEEE Transactions on Biomedical Engineering, (Oct. 1994), Vol. 41, No. 10, pp. 937-942
AJ	Wang, J. et al., "Needle-Type Dual Microsensor for the Simultaneous Monitoring of Glucose and Insulin", Analytical Chemistry, (February 15, 2001), Vol. 73, No. 4, pp. 844-847
AK	Moussy, F. et al., "Performance of Subcutaneously Implanted Needle-Type Glucose Sensors Employing a Novel Trilayer Coating", Anal. Chem. 65, (American Chemical Society), (1993), pp. 2072-2077
AL	Bindra, D.S. et al., "Design and in Vitro studies of a Needle-Type Glucose Sensor for Subcutaneous Monitoring", Anal. Chem. 63, (American Chemical Society), (1991), pp. 1692-1696

Examiner	Date Considered
----------	-----------------

* EXAMINER: Initial if reference considered, whether or not citation is in conformance with MPEP 609; Draw line through citation if not in conformance and not considered. Include copy of this form with next communication to applicant.



UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
 United States Patent and Trademark Office
 Address: COMMISSIONER FOR PATENTS
 P.O. Box 1450
 Alexandria, Virginia 22313-1450
 www.uspto.gov

APPLICATION NUMBER	FILING OR 371 (c) DATE	FIRST NAMED APPLICANT	ATTORNEY DOCKET NUMBER
11/322,568	12/30/2005	John J. Mastrototaro	PD00291 CIP

MEDTRONIC MINIMED, INC.
 18000 Devonshire Street
 Northridge, CA 91325-1219

CONFIRMATION NO. 4822
FORMALITIES
LETTER

Date Mailed: 02/24/2006

NOTICE TO FILE MISSING PARTS OF NONPROVISIONAL APPLICATION

FILED UNDER 37 CFR 1.53(b)

Filing Date Granted

Items Required To Avoid Abandonment:

An application number and filing date have been accorded to this application. The item(s) indicated below, however, are missing. Applicant is given **TWO MONTHS** from the date of this Notice within which to file all required items and pay any fees required below to avoid abandonment. Extensions of time may be obtained by filing a petition accompanied by the extension fee under the provisions of 37 CFR 1.136(a).

- The oath or declaration is unsigned.

The application is informal since it does not comply with the regulations for the reason(s) indicated below.

The required item(s) identified below must be timely submitted to avoid abandonment:

- Replacement drawings in compliance with 37 CFR 1.84 and 37 CFR 1.121(d) are required. The drawings submitted are not acceptable because:
 - The drawings have a line quality that is too light to be reproduced (weight of all lines and letters must be heavy enough to permit adequate reproduction) or text that is illegible (reference characters, sheet numbers, and view numbers must be plain and legible) see 37 CFR 1.84(l) and (p)(1)); See Figure(s) 24.
 - The drawings submitted to the Office are not electronically reproducible. Drawing sheets must be submitted on paper, which is flexible, strong, white, smooth, non-shiny, and durable (see 37 CFR 1.84(e)). See Figure(s) 15-18.

Applicant is cautioned that correction of the above items may cause the specification and drawings page count to exceed 100 pages. If the specification and drawings exceed 100 pages, applicant will need to submit the required application size fee.

The applicant needs to satisfy supplemental fees problems indicated below.

The required item(s) identified below must be timely submitted to avoid abandonment:

- To avoid abandonment, a surcharge (for late submission of filing fee, search fee, examination fee or oath or declaration) as set forth in 37 CFR 1.16(f) of \$130 for a non-small entity, must be submitted with the missing items identified in this letter.


SUMMARY OF FEES DUE:

Total additional fee(s) required for this application is **\$130** for a Large Entity

- **\$130** Surcharge.

Replies should be mailed to: Mail Stop Missing Parts
 Commissioner for Patents
 P.O. Box 1450
 Alexandria VA 22313-1450

*A copy of this notice **MUST** be returned with the reply.*



Office of Initial Patent Examination (571) 272-4000, or 1-800-PTO-9199, or 1-800-972-6382
PART 3 - OFFICE COPY

CUSTOMER NUMBER: 23608

Attorney's Docket No.: PD00291 CIP
Date: December 30, 2005
Express Mail Label No. EV 119698309 US

Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

Dear Sir:

Transmitted herewith for filing is the Continuation-in-Part patent application of:
Inventor(s): **JOHN J. MASTROTOTARO; EDWARD CHERNOFF; DAVID Y. CHOY;**
JAMES L. HENKE; RICHARD E. PURVIS; and PETER I. HONG

For: **TELEMETERED CHARACTERISTIC MONITOR SYSTEM AND METHOD OF
USING THE SAME**

Enclosed are:

- ☒ 38 page(s) CIP patent application including cover sheet, 18 claims, and 1 page abstract
- ☒ 12 sheets of informal drawings (Figs. 1 - 25)
- ☒ unexecuted Declaration
- ☐ Assignment with Recordation Form Cover Sheet
- ☐ Power of Attorney by Assignee
- ☒ return postcard

CALCULATION OF FEES						
ITEM		NO. OF CLAIMS FILED MINUS BASE*	NO. OF CLAIMS OVER BASE	X SM/LG ENTITY FEE	\$ AMOUNT	\$ FEE
A	TOTAL CLAIMS FEE	18 - 20* =	0	X \$25 or X \$50	\$0	
B	INDEPENDENT CLAIMS FEE**	1 - 3* =	0	X \$100 or X 200	\$0	
C	SUBTOTAL - ADDITIONAL CLAIMS FEE (ADD FINAL COLUMN IN LINES A + B)					0
D	MULTIPLE-DEPENDENT CLAIMS FEE SMALL ENTITY FEE = \$180 MULTIPLE-DEPENDENT CLAIMS FEE LARGE ENTITY FEE = \$360					0
E	BASIC FEE*SMALL ENTITY FEE = \$150 BASIC FEE*LARGE ENTITY FEE = \$300					300
F	SEARCH FEE = \$500					500
G	EXAMINATION FEE = \$200					200
H	TOTAL FILING FEE (ADD TOTALS FOR LINES C, D, E, F AND G)					
	**LIST INDEPENDENT CLAIMS: 1					

☒ Please charge my Deposit Account No.
50-0621 the amount of

\$1,000

**A copy of this letter is
enclosed.**

☐ A check in the amount of

\$

to cover the filing fee is
enclosed.

___ A check in the amount of

\$

to cover Assignment
Recordation fee is enclosed.

X The Commissioner is hereby authorized to charge payment of the following fees associated with this communication or credit any overpayment to Deposit Account No. 50-0621

X Any additional filing fees required under 37 CFR 1.16.

X Any patent application processing fees under 37 CFR 1.17.

X The Commissioner is hereby authorized to charge payment of the following fees during the pendency of this application or credit any overpayment to Deposit Account No. 50-0621


X Any patent application processing fees under 37 CFR 1.17.

— The issue fee set in 37 CFR 1.18 at or before mailing of the Notice of Allowance, pursuant to 37 CFR 1.311(b).

X Any filing fees under 37 CFR 1.16 for presentation of extra claims.

Respectfully submitted,

Date: 12/30/2005



Richard Yoon
Reg. No. 42,247

MEDTRONIC MINIMED, INC.
18000 Devonshire Street
Northridge, CA 91325-1219
Telephone: (818) 576-4110
Facsimile: (818) 576-6202

Express Mail No. EV 119698309 US

PATENT
PD00291 CIP

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

In re Continuation-in-Part Application of:	)	
John J. Mastrototaro et al.	)	Group Art Unit: unknown
Serial No.: unknown	)	
Filed: December 30, 2005	)	Examiner: unknown
For: TELEMETERED CHARACTERISTIC	)	
MONITOR SYSTEM AND METHOD	)	
OF USING THE SAME	)	

CERTIFICATE OF U.S. EXPRESS MAIL

Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

Sir:

Express Mail Mailing Label No. EV 119698309 US
Date of Deposit: December 30, 2005


I hereby certify that a 38 page(s) Continuation-in-Part patent application including cover sheet, 32 pages of specification, 18 claims, 1 page abstract, and 12 pages of informal drawings (Figs. 1 - 25), transmittal letter, unexecuted Declaration, and return postcard are being deposited using the "Express Mail Post Office to Addressee" service of the United States Postal Service under 37 C.F.R. § 1.10 on the above date and addressed to Mail Stop Patent Application, Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.

December 30, 2005

Date of deposit

Jonathan Bailey

Name of person mailing papers



Signature

MEDTRONIC MINIMED, INC.
18000 Devonshire Street
Northridge, CA 91325-1219
Tel.: (818) 576-4110
Fax: (818) 576-6202

**APPLICATION FOR
UNITED STATES PATENT
IN THE NAME OF**

**JOHN J. MASTROTOTARO, EDWARD CHERNOFF, DAVID CHOY,
JAMES HENKE, RICHARD PURVIS, AND PETER HONG**

ASSIGNED TO

MEDTRONIC MINIMED, INC.

FOR

**TELEMETERED CHARACTERISTIC MONITOR SYSTEM
AND METHOD OF USING THE SAME**

DOCKET NO. PD00291 CIP

**Richard Yoon, Reg. No.: 42,247
Medtronic MiniMed, Inc.
18000 Devonshire Street
Northridge, California 91326
(818) 576-4110
(818) 576-6202 facsimile**

Express Mail No. EV 119 698 309 US

TITLE

Telemetered Characteristic Monitor System And Method Of Using The Same

RELATED APPLICATIONS

5 This application is a continuation-in-part of U.S. Patent Application Serial No.
10/898,589, filed on July 23, 2004, which is a continuation of U.S. Patent Application Serial No.
10/465,715, filed on December 17, 1999 and issued as U.S. Patent No. 6,809,653 on October 26,
2005, which is a continuation of U.S. Patent Application Serial No. 09/377,472, filed on August
19, 1999 and later abandoned, which claimed priority from U.S. Provisional Application Serial
10 No. 60/103,812, filed on October 8, 1998, each of which are herein incorporated by reference.

FIELD OF THE INVENTION

 This invention relates to telemetered subcutaneous sensor devices and, in particular
embodiments, to devices and methods for wireless communication between an implantable
15 subcutaneous sensor set at a selected insertion site within the body of a user and a remotely
located characteristic monitor.

BACKGROUND OF THE INVENTION

 Over the years, a variety of implantable electrochemical sensors have been developed for
20 detecting and/or quantifying specific agents or compositions in a patient's blood. For instance,
glucose sensors have been developed for use in obtaining an indication of blood glucose levels in
a diabetic patient. Such readings are useful in monitoring and/or adjusting a treatment regimen
which typically includes the regular administration of insulin to the patient. Thus, blood glucose
readings improve medical therapies with semi-automated medication infusion pumps of the
25 external type, as generally described in U.S. Patent Nos. 4,562,751; 4,678,408; and 4,685,903; or
automated implantable medication infusion pumps, as generally described in U.S. Patent No.

4,573,994, which are herein incorporated by reference.

Generally, small and flexible electrochemical sensors can be used to obtain periodic readings over an extended period of time. In one form, flexible subcutaneous sensors are constructed in accordance with thin film mask techniques in which an elongated sensor includes
5 thin film conductive elements encased between flexible insulative layers of polyimide sheets or similar material. Such thin film sensors typically include a plurality of exposed electrodes at one end for subcutaneous placement with a user's interstitial fluid, blood, or the like, and a corresponding exposed plurality of conductive contacts at another end for convenient external electrical connection with a suitable monitoring device through a wire or cable. Typical thin film
10 sensors are described in commonly assigned U.S. Patent Nos. 5,390,671; 5,391,250; 5,482,473; and 5,586,553 which are incorporated by reference herein. See also U.S. Patent No. 5,299,571.

Drawbacks to the use of implantable sensors arise from the use of a wired connection between the implantable sensor set and the monitor. The use of the wire or cable is an additional inconvenience to users that already utilize an external infusion pump that includes an infusion
15 insertion set and tube to infuse the medication. Also, the preferred site for some sensing device may be inconvenient for connection by wire to a characteristic monitor. For implantable pumps, the wire or cable negates the very benefit of having an internal device without external wires or cables. For Type 2 diabetics, who do not necessarily need or use an infusion pump, the use of a cable is seen as an inconvenience that may inhibit use of the device. In addition, the use of a
20 wire or cable limits a user's ability to position the monitor, since it can be placed no further away than the ultimate length of the wire or cable. Thus, the user must normally wear the monitor, which can be problematic. For example, removal of the monitor for sleeping can be difficult, since a user would tend to become "tangled" in the wire or cable, between the sensor and the monitor, during the normal tossing and turning that occurs during sleep. Furthermore, the more
25 connections the user must deal with (e.g., infusion pump and catheter and/or monitor with wire to sensor), the more complicated it is to use the devices, and the less likely the user will maintain

compliance with the medical regimen due to perceived and actual difficulties with all of the wires and cables.

SUMMARY OF THE DISCLOSURE

5 It is an object of an embodiment of the present invention to provide an improved telemetered implantable sensor set (such as a subcutaneous or percutaneous sensor) and monitor connection device, which obviates for practical purposes, the above mentioned limitations.

 According to an embodiment of the invention, a telemetered characteristic monitor system includes a remotely located data receiving device, a sensor for producing signal indicative
10 of a characteristic of a user, and a transmitter device. In preferred embodiments, the transmitter device includes a housing, a sensor connector, a processor, and a transmitter. A potentiostat within the transmitter device may be coupled to the sensor connector and applies power to the sensor. The sensor connector receives the produced signals from the sensor. The processor is coupled to the sensor connector and processes the signals from the sensor for delivery to the
15 remotely located data receiving device. The transmitter is coupled to the processor for wirelessly transmitting the processed signals to the remotely located data receiving device. In preferred embodiments, the data receiving device is a characteristic monitor. However, in other embodiments, the data receiving device is a data receiver that provides data to another device, an RF programmer, a medication delivery device (such as an infusion pump), or the like.

20 In particular embodiments, the transmitter of the transmitter device transmits the processed signals by radio frequencies. In other embodiments, the sensor may be implanted in and/or through subcutaneous, dermal, sub-dermal, intra-peritoneal or peritoneal tissue, and the sensor connector of the transmitter device includes a cable that is connected to the sensor. Also, the implantable sensor can be configured for a wired connection to a characteristic monitor, and
25 the sensor connector of the transmitter device is formed to connect to the configured implantable sensor. Still further embodiments of the transmitter device include a receiver to receive data and

instructions from the characteristic monitor, or the like.

Embodiments of the transmitter device (when used with a subcutaneous or percutaneous sensor) may include a bio-compatible adhesive to secure the housing to a skin surface of the user.

Preferably, the housing of the transmitter device is less than about 3.0 inches in diameter by 0.5
5 inches thick. In addition, the housing is resistant to fluids when immersed in a fluid, operable in a temperature range of 0°C to 50°C, and has an operable life of at least 3 months. If the sensor is fully implanted, the transmitter that is connected to the sensor may be secured by sutures, sewing rings, or the like.

Other features and advantages of the invention will become apparent from the following
10 detailed description, taken in conjunction with the accompanying drawings which illustrate, by way of example, various features of embodiments of the invention.

BRIEF DESCRIPTION OF THE DRAWINGS

A detailed description of embodiments of the invention will be made with reference to the
15 accompanying drawings, wherein like numerals designate corresponding parts in the several figures.

Fig. 1 is a perspective view illustrating a subcutaneous sensor insertion set and telemetered characteristic monitor transmitter device embodying the novel features of the invention;

20 Fig. 2 is an enlarged longitudinal vertical section taken generally on the line 2-2 of Fig. 1;

Fig. 3 is an enlarged longitudinal sectional of a slotted insertion needle used in the insertion set of Figs. 1 and 2;

Fig. 4 is an enlarged transverse section taken generally on the line 4-4 of Fig. 3;

Fig. 5 is an enlarged transverse section taken generally on the line 5-5 of Fig. 3;

25 Fig. 6 is an enlarged fragmented sectional view corresponding generally with the encircled region 6 of Fig. 2; and

Fig. 7 is an enlarged transverse section taken generally on the line 7-7 of Fig. 2.

Fig. 8(a) is a top plan and partial cut-away view of the telemetered characteristic monitor transmitter device in accordance with the embodiment shown in Fig. 1.

Fig. 8(b) is a simplified block diagram of the printed circuit board of the telemetered
5 characteristic monitor transmitter device in accordance with the embodiments shown in Fig. 1.

Fig. 9 is a timing diagram illustrating an embodiment of a message and timing format used by the telemetered characteristic monitor transmitter device shown in Fig. 1.

Fig. 10 is a simplified block diagram of a characteristic monitor used in accordance with an embodiment of the present invention.

10 Fig. 11 is a timing diagram for the characteristic monitor shown in Fig. 10.

Fig. 12 is another timing diagram for the characteristic monitor shown in Fig. 10.

Fig. 13 is a simplified block diagram of a telemetered characteristic monitor transmitter and sensor set system in accordance with another embodiment of the present invention.

Fig. 14 is a simplified block diagram of a telemetered characteristic monitor transmitter
15 and characteristic monitor system in accordance with still another embodiment of the present invention.

Fig. 15 is a perspective view illustrating another preferred embodiment of the subcutaneous sensor insertion set and telemetered characteristic monitor transmitter device when mated together in relation to the characteristic monitor system.

20 Fig. 16 is a top view of the subcutaneous sensor insertion set and telemetered characteristic monitor transmitter device when separated.

Figs. 17 and 18 are two perspective views of the characteristic monitor transmitter in accordance with the embodiment shown in Fig. 16.

Figs. 19 and 20 are top and bottom plan and partial cut-away views of the telemetered
25 characteristic monitor transmitter device in accordance with the embodiment shown in Fig. 16.

Fig. 21 is a side view of the charger associated with telemetered characteristic monitor

transmitter device.

Fig. 22 is a perspective view of the charger associated with telemetered characteristic monitor transmitter device.

Fig. 23 is a perspective view of the charger mated with telemetered characteristic monitor transmitter device.

Figs. 24 and 25 are simplified block diagrams of the charger system used to charge the telemetered characteristic monitor transmitter device.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

As shown in the drawings for purposes of illustration, the invention is embodied in a telemetered characteristic monitor transmitter coupled to a sensor set, that may be implanted in and/or through subcutaneous, dermal, sub-dermal, inter-peritoneal or peritoneal tissue, that transmits data from the sensor set to the characteristic monitor for determining body characteristics. In preferred embodiments of the present invention, the sensor set and monitor are for determining glucose levels in the blood and/or body fluids of the user without the use of, or necessity of, a wire or cable connection between the transmitter and the monitor. However, it will be recognized that further embodiments of the invention may be used to determine the levels of other agents, characteristics or compositions, such as hormones, cholesterol, medication concentrations, pH, oxygen saturation, viral loads (e.g., HIV), or the like. In other embodiments, the sensor set may also include the capability to be programmed or calibrated using data received by the telemetered characteristic monitor transmitter device, or may be calibrated at the monitor device (or receiver). The telemetered characteristic monitor system is primarily adapted for use in subcutaneous human tissue. However, still further embodiments may be placed in other types of tissue, such as muscle, lymph, organ tissue, veins, arteries or the like, and used in animal tissue. Embodiments may provide sensor readings on an intermittent or continuous basis.

The telemetered characteristic monitor system 1, in accordance with a preferred

embodiment of the present invention include a percutaneous sensor set 10, a telemetered characteristic monitor transmitter device 100 and a characteristic monitor 200. The percutaneous sensor set 10 utilizes an electrode-type sensor, as described in more detail below. However, in alternative embodiments, the system may use other types of sensors, such as chemical based, optical based or the like. In further alternative embodiments, the sensors may be of a type that is used on the external surface of the skin or placed below the skin layer of the user. Preferred embodiments of a surface mounted sensor would utilize interstitial fluid harvested from underneath the skin. The telemetered characteristic monitor transmitter 100 generally includes the capability to transmit data. However, in alternative embodiments, the telemetered characteristic monitor transmitter 100 may include a receiver, or the like, to facilitate two-way communication between the sensor set 10 and the characteristic monitor 200. The characteristic monitor 200 utilizes the transmitted data to determine the characteristic reading. However, in alternative embodiments, the characteristic monitor 200 may be replaced with a data receiver, storage and/or transmitting device for later processing of the transmitted data or programming of the telemetered characteristic monitor transmitter 100.

In addition, a relay or repeater 4 may be used with a telemetered characteristic monitor transmitter 100 and a characteristic monitor 200 to increase the distance that the telemetered characteristic monitor transmitter 100 can be used with the characteristic monitor 200, as shown in Fig. 13. For example, the relay 4 could be used to provide information to parents of children using the telemetered characteristic monitor transmitter 100 and the sensor set 10 from a distance. The information could be used when children are in another room during sleep or doing activities in a location remote from the parents. In further embodiments, the relay 4 can include the capability to sound an alarm. In addition, the relay 4 may be capable of providing telemetered characteristic monitor transmitter 100 data from the sensor set 10, as well as other data, to a remotely located individual via a modem connected to the relay 4 for display on a monitor, pager or the like. The data may also be downloaded through a Communication-Station

8 to a remotely located computer 6 such as a PC, lap top, or the like, over communication lines, by modem or wireless connection, as shown in Fig. 14. Also, some embodiments may omit the Communication Station 8 and uses a direct modem or wireless connection to the computer 6. In further embodiments, the telemetered characteristic monitor transmitter 100 transmits to an RF
5 programmer, which acts as a relay, or shuttle, for data transmission between the sensor set 10 and a PC, laptop, Communication-station, a data processor, or the like. In further alternatives, the telemetered characteristic monitor transmitter 100 may transmit an alarm to a remotely located device, such as a communication-station, modem or the like to summon help. In addition, further embodiments may include the capability for simultaneous monitoring of multiple sensors and/or
10 include a sensor for multiple measurements.

Still further embodiments of the telemetered characteristic monitor transmitter 100 may have and use an input port for direct (e.g., wired) connection to a programming or data readout device and/or be used for calibration of the sensor set 10. Preferably, any port would be water proof (or water resistant) or include a water proof, or water resistant, removable cover.

15 The purpose of the telemetered characteristic monitor system 1 (see Fig. 2) is to provide for better treatment and control in an outpatient or a home use environment. For example, the monitor system 1 can provide indications of glucose levels, a hypoglycemia/hyperglycemia alert and outpatient diagnostics. It is also useful as an evaluation tool under a physician's supervision.

The monitor system 1 also removes inconvenience by separating the monitor electronics
20 into two separate devices; a telemetered characteristic monitor transmitter 100, which attaches to the implantable sensor set 10; and a characteristic monitor 200 (or other receiver), which is carried like a pager. This provides several advantages over wire connected devices. For instance, the user can more easily conceal the presence of the monitor system 1, since a wire will not be visible (or cumbersome), within clothing. Such remote communication also provides
25 greater convenience and flexibility in the placement of the sensor. It also makes it is easier to protect the characteristic monitor 200, which can be removed from the user's body during

showers, exercise, sleep or the like. In addition, the use of multiple components (e.g., transmitter 100 and characteristic monitor 200) facilitates upgrades or replacements, since one module or the other can be modified or replaced without requiring complete replacement of the monitor system 1. Further, the use of multiple components can improve the economics of manufacturing, since
5 some components may require replacement on a more frequent basis, sizing requirements may be different for each module, there may be different assembly environment requirements, and modifications can be made without affecting the other components.

The telemetered characteristic monitor transmitter 100 takes characteristic information, such as glucose data or the like, from the percutaneous sensor set 10 and transmits it via wireless
10 telemetry to the characteristic monitor 200, which displays and logs the received glucose readings. Logged data can be downloaded from the characteristic monitor 200 to a personal computer, laptop, or the like, for detailed data analysis. In further embodiments, the telemetered characteristic monitor system 1 may be used in a hospital environment or the like. Still further
15 embodiments of the present invention may include one or more buttons (on the telemetered characteristic monitor transmitter 100 or characteristic monitor 200) to record data and events for later analysis, correlation, or the like. In addition, the telemetered characteristic monitor transmitter 100 may include a transmit on/off button for compliance with safety standards and regulations to temporarily suspend transmissions. Further buttons can include a sensor on/off
20 button to conserve power and to assist in initializing the sensor set 10. The telemetered characteristic monitor transmitter 100 and characteristic monitor 200 may also be combined with other medical devices to combine other patient data through a common data network and telemetry system.

Further embodiments of the percutaneous sensor set 10 would monitor the temperature of the sensor set 10, which can then be used to improve the calibration of the sensor. For instance,
25 for a glucose sensor, the enzyme reaction activity may have a known temperature coefficient. The relationship between temperature and enzyme activity can be used to adjust the sensor values

to more accurately reflect the actual characteristic levels. In addition to temperature measurements, the oxygen saturation level can be determined by measuring signals from the various electrodes of the sensor set 10. Once obtained, the oxygen saturation level may be used in calibration of the sensor set 10 due to changes in the oxygen saturation levels, and its effects
5 on the chemical reactions in the sensor set 10. For instance, as the oxygen level goes lower the sensor sensitivity may be lowered. The oxygen level can be utilized in calibration of the sensor set 10 by adjusting for the changing oxygen saturation. In alternative embodiments, temperature measurements may be used in conjunction with other readings to determine the required sensor calibration.

10 As shown in Figs. 1-7, a percutaneous sensor set 10 is provided for subcutaneous placement of an active portion of a flexible sensor 12 (see Fig. 2), or the like, at a selected site in the body of a user. The subcutaneous or percutaneous portion of the sensor set 10 includes a hollow, slotted insertion needle 14, and a cannula 16. The needle 14 is used to facilitate quick and easy subcutaneous placement of the cannula 16 at the subcutaneous insertion site. Inside the
15 cannula 16 is a sensing portion 18 of the sensor 12 to expose one or more sensor electrodes 20 to the user's bodily fluids through a window 22 formed in the cannula 16. After insertion, the insertion needle 14 is withdrawn to leave the cannula 16 with the sensing portion 18 and the sensor electrodes 20 in place at the selected insertion site.

In preferred embodiments, the percutaneous sensor set 10 facilitates accurate placement
20 of a flexible thin film electrochemical sensor 12 of the type used for monitoring specific blood parameters representative of a user's condition. Preferably, the sensor 12 monitors glucose levels in the body, and may be used in conjunction with automated or semi-automated medication infusion pumps of the external or implantable type as described in U.S. Pat. Nos. 4,562,751; 4,678,408; 4,685,903 or 4,573,994, to control delivery of insulin to a diabetic patient.

25 Preferred embodiments of the flexible electrochemical sensor 12 are constructed in accordance with thin film mask techniques to include elongated thin film conductors embedded

or encased between layers of a selected insulative material such as polyimide film or sheet, and membranes. The sensor electrodes 20 at a tip end of the sensing portion 18 are exposed through one of the insulative layers for direct contact with patient blood or other body fluids, when the sensing portion 18 (or active portion) of the sensor 12 is subcutaneously placed at an insertion
5 site. The sensing portion 18 is joined to a connection portion 24 (see Fig. 2) that terminates in conductive contact pads, or the like, which are also exposed through one of the insulative layers. In alternative embodiments, other types of implantable sensors, such as chemical based, optical based, or the like, may be used.

As is known in the art, and illustrated schematically in Fig. 2, the connection portion 24
10 and the contact pads are generally adapted for a direct wired electrical connection to a suitable monitor 200 for monitoring a user's condition in response to signals derived from the sensor electrodes 20. Further description of flexible thin film sensors of this general type are be found in U.S. Patent. No. 5,391,250, entitled METHOD OF FABRICATING THIN FILM SENSORS, which is herein incorporated by reference. The connection portion 24 may be conveniently
15 connected electrically to the monitor 200 or a telemetered characteristic monitor transmitter 100 by a connector block 28 (or the like) as shown and described in U.S. Pat. No. 5,482,473, entitled FLEX CIRCUIT CONNECTOR, which is also herein incorporated by reference. Thus, in accordance with embodiments of the present invention, subcutaneous sensor sets 10 are configured or formed to work with either a wired or a wireless characteristic monitor system.

20 The proximal part of the sensor 12 is mounted in a mounting base 30 adapted for placement onto the skin of a user. As shown, the mounting base 30 is a pad having an underside surface coated with a suitable pressure sensitive adhesive layer 32, with a peel-off paper strip 34 normally provided to cover and protect the adhesive layer 32, until the sensor set 10 is ready for use. As shown in Figs. 1 and 2, the mounting base 30 includes upper and lower layers 36 and 38,
25 with the connection portion 24 of the flexible sensor 12 being sandwiched between the layers 36 and 38. The connection portion 24 has a forward section joined to the active sensing portion 18

of the sensor 12, which is folded angularly to extend downwardly through a bore 40 formed in the lower base layer 38. In preferred embodiments, the adhesive layer 32 includes an anti-bacterial agent to reduce the chance of infection; however, alternative embodiments may omit the agent. In the illustrated embodiment, the mounting base is generally rectangular, but alternative
5 embodiments may be other shapes, such as circular, oval, hour-glass, butterfly, irregular, or the like.

The insertion needle 14 is adapted for slide-fit reception through a needle port 42 formed in the upper base layer 36 and further through the lower bore 40 in the lower base layer 38. As shown, the insertion needle 14 has a sharpened tip 44 and an open slot 46 which extends
10 longitudinally from the tip 44 at the underside of the needle 14 to a position at least within the bore 40 in the lower base layer 36. Above the mounting base 30, the insertion needle 14 may have a full round cross-sectional shape, and may be closed off at a rear end of the needle 14. Further description of the needle 14 and the sensor set 10 are found in U.S. Patent No. 5,586,553, entitled "TRANSCUTANEOUS SENSOR INSERTION SET" and co-pending U.S. Patent
15 Application Serial No. 08/871,831, entitled 'DISPOSABLE SENSOR INSERTION ASSEMBLY,' which are herein incorporated by reference.

The cannula 16 is best shown in Figs. 6 and 7, and includes a first portion 48 having partly-circular cross-section to fit within the insertion needle 14 that extends downwardly from the mounting base 30. In alternative embodiments, the first portion 48 may be formed with a
20 solid core; rather than a hollow core. In preferred embodiments, the cannula 16 is constructed from a suitable medical grade plastic or elastomer, such as polytetrafluoroethylene, silicone, or the like. The cannula 16 also defines an open lumen 50 in a second portion 52 for receiving, protecting and guideably supporting the sensing portion 18 of the sensor 12. The cannula 16 has one end fitted into the bore 40 formed in the lower layer 38 of the mounting base 30, and the
25 cannula 16 is secured to the mounting base 30 by a suitable adhesive, ultrasonic welding, snap fit or other selected attachment method. From the mounting base 30, the cannula 16 extends

angularly downwardly with the first portion 48 nested within the insertion needle 14, and terminates before the needle tip 44. At least one window 22 is formed in the lumen 50 near the implanted end 54, in general alignment with the sensor electrodes 20, to permit direct electrode exposure to the user's bodily fluid when the sensor 12 is subcutaneously placed. Alternatively, a
5 membrane can cover this area with a porosity that controls rapid diffusion of glucose through the membrane.

As shown in Figs. 1, 2 and 8(a), the telemetered characteristic monitor transmitter 100 is coupled to a sensor set 10 by a cable 102 through a connector 104 that is electrically coupled to the connector block 28 of the connector portion 24 of the sensor set 10. In alternative
10 embodiments, the cable 102 may be omitted, and the telemetered characteristic monitor transmitter 100 may include an appropriate connector (not shown) for direct connection to the connector portion 24 of the sensor set 10 or the sensor set 10 may be modified to have the connector portion 24 positioned at a different location, such as for example, on the top of the sensor set 10 to facilitate placement of the telemetered characteristic monitor transmitter over the
15 subcutaneous sensor set 10. This would minimize the amount of skin surface covered or contacted by medical devices, and tend to minimize movement of the sensor set 10 relative to the telemetered characteristic monitor transmitter 100. Specifically, according to another preferred embodiment of the present invention, characteristic monitor transmitter 100 and the sensor set 10 have been modified to allow a side-by side direct connection between the characteristic monitor
20 transmitter 100' and the sensor set 10' such that the characteristic monitor transmitter 100' detachable from the sensor set 10', as seen in Fig. 15. As shown in Figs. 16-18, according to the preferred embodiments of the present invention, the characteristic monitor transmitter 100' is coupled to a sensor set 10' using a male/female connection scheme for direct connection to the the sensor set 10'. In preferred embodiments, the characteristic monitor transmitter 100' shall
25 have a female connector interface 400 built into the housing 1100 of the characteristic monitor transmitter 100'. Detents at the female connector interface 400 are used to mate and lock with

locking prongs located on the male sensor connector 600 of the sensor set 10'. Alternatively, other detachable connector systems may be used including the modification of the connection scheme to place a female connector on the sensor 10' and the male connector on characteristic monitor transmitter 100'. This provides several advantages over other embodiments of the present invention. First of all, the use of multiple components in the monitor system 1' (e.g., 5 sensor set 10', transmitter 100' and characteristic monitor 200) facilitates upgrades or replacements, since one module or the other can be modified or replaced without requiring complete replacement of the monitor system 1'. In other embodiments, the transmitter 100 was discarded along with the sensor set 10 after the 3 to 5 day use period since they were directly 10 connected. Another key improvement of the characteristic transmitter 100' of the present invention compared to other embodiments is the relative size of the transmitter 100'. The size of the transmitter 100' has been reduced to fit directly onto the sensor set 10' and be supported by the sensor set 10' itself. Unlike the other embodiments of the present invention that required the transmitter 100 to be attached separately to the body of a user by a separate adhesive tape 15 118, the transmitter 100' can remain fixed in its location by being attached to the sensor set 10'. In other words, a single adhesive tape 34 used to attach the sensor set to the patient can also support the transmitter 100'. In further alternative embodiments, the cable 102 and the connector 104 may be formed as add-on adapters to fit different types of connectors on different types or kinds of sensor sets. The use of adapters would facilitate adaptation of the telemetered 20 characteristic monitor transmitter 100 to work with a wide variety of sensor systems. In further embodiments, the telemetered characteristic monitor transmitter 100 may omit the cable 102 and connector 104 and is instead optically couple with an implanted sensor, in the subcutaneous, dermal, sub-dermal, inter-peritoneal or peritoneal tissue, to interrogate the implanted sensor using visible, and/or IR frequencies, either transmitting to and receiving a signal from the 25 implanted sensor or receiving a signal from the implanted sensor.

The telemetered characteristic monitor transmitter 100 (also known as Potentiostat

Transmitter Device) includes a housing 106 that supports a printed circuit board 108, batteries 110, antenna 112, and the cable 102 with the connector 104. In preferred embodiments, the housing 106 is formed from an upper case 114 and a lower case 116 that are sealed with an ultrasonic weld to form a waterproof (or resistant) seal to permit cleaning by immersion (or swabbing) with water, cleaners, alcohol or the like. In preferred embodiments, the upper and lower case 114 and 116 are formed from a medical grade plastic. However, in alternative embodiments, the upper case 114 and lower case 116 may be connected together by other methods, such as snap fits, sealing rings, RTV (silicone sealant) and bonded together, or the like, or formed from other materials, such as metal, composites, ceramics, or the like. In other embodiments, the separate case can be eliminated and the assembly is simply potted in epoxy or other moldable materials that is compatible with the electronics and reasonably moisture resistant. In preferred embodiments, the housing 106 is disk or oval shaped. However, in alternative embodiments, other shapes, such as hour glass, rectangular or the like, may be used. Preferred embodiments of the housing 106 are sized in the range of 2.0 square inches by 0.35 inches thick to minimize weight, discomfort and the noticeability of the telemetered characteristic monitor transmitter 100 on the body of the user. However, larger or smaller sizes, such as 1.0 square inches and 0.25 inches thick or less, and 3.0 square inches and 0.5 inches thick or more, may be used. As seen in Figs. 15-18, alternative preferred embodiments of the housing 1100 are sized in the range of 29 mm x 36 mm by 15 mm thick to minimize weight, discomfort and the noticeability of the telemetered characteristic monitor transmitter 100' on the body of the user. Also, the housing may simply be formed from potted epoxy, or other material, especially if the battery life relative to the device cost is long enough, or if the device is rechargeable.

As shown, the lower case 116 may have an underside surface coated with a suitable pressure sensitive adhesive layer 118, with a peel-off paper strip 120 normally provided to cover and protect the adhesive layer 118, until the sensor set telemetered characteristic monitor transmitter 100 is ready for use. In preferred embodiments, the adhesive layer 118 includes an

anti-bacterial agent to reduce the chance of infection; however, alternative embodiments may omit the agent. In further alternative embodiments, the adhesive layer 118 may be omitted and the telemetered characteristic monitor transmitter 100 is secured to the body by other methods, such as an adhesive overdressing, straps, belts, clips or the like. In addition, as seen in Fig. 15, the telemetered characteristic monitor transmitter 100' can be supported by the sensor set 10' itself.

In preferred embodiments, the cable 102 and connector 104 are similar to (but not necessarily identical to) shortened versions of a cable and connector that are used to provide a standard wired connection between the sensor set 10 and the characteristic monitor 200. This allows the telemetered characteristic monitor transmitter 100 to be used with existing sensor sets 10, and avoids the necessity to re-certify the connector portion 24 of the sensor set 10 for use with a wireless connection. The cable 102 should also include a flexible strain relief portion (not shown) to minimize strain on the sensor set 10 and prevent movement of the inserted sensor 12, which can lead to discomfort or dislodging of the sensor set 10. The flexible strain relief portion is intended to minimize sensor artifacts generated by user movements that might cause the sensing area of the sensor set 10 to move relative to the body tissues in contact with the sensing area of the sensor set 10.

The printed circuit board 108 of the telemetered characteristic monitor transmitter 100 includes a sensor interface 122, processing electronics 124, timers 126, and data formatting electronics 128, as shown in Fig. 8(b). In preferred embodiments, the sensor interface 122, processing electronics 124, timers 126, and data formatting electronics 128 are formed as separate semiconductor chips; however, alternative embodiments may combine the various semiconductor chips into a single customized semiconductor chip. The sensor interface 122 connects with the cable 102 that is connected with the sensor set 10. In preferred embodiments, the sensor interface is permanently connected to the cable 102. However, in alternative embodiments, the sensor interface 122 may be configured in the form of a jack to accept different

types of cables that provide adaptability of the telemetered characteristic monitor transmitter 100 to work with different types of sensors and/or sensors placed in different locations of the user's body. In additional preferred embodiments of the present invention, the connector 104 is eliminated and the sensor interface 122 is directly linked with the sensor 12 when the telemetered characteristic monitor 100' and the sensor set 10' are connected. An alternative preferred embodiment of the electronic circuitry of such a system is shown in Figs. 19-20. Figs. 19 and 20 show top and bottom schematic diagrams of the characteristic monitor transmitter 100' according to the preferred embodiments. The characteristic monitor transmitter 100' includes a housing 1100 that supports a printed circuit board that contains a voltage regulator 1108, comparators 1110 and 1116, power switch 1112, analog switch 1114, Op Amps 1118, Microprocessor 1120, Digital to Analog Converter 1122, Real Time Clock 1126, EEPROM 1126, RF Transceiver 1128, and a battery 1130. In preferred embodiments, the electronics of the characteristic monitor transmitter 100 and 100', are capable of operating in a temperature range of 0° C and 50° C. However, larger or smaller temperature ranges may be used.

Preferably, the battery assembly will use a weld tab design to connect power to the system. For example, it can use three series silver oxide 357 battery cells 110, or the like. However, it is understood that different battery chemistries may be used, such as lithium based chemistries, alkaline batteries, nickel metalhydride, or the like, and different numbers of batteries can be used. In further embodiments, the sensor interface 122 will include circuitry and/or a mechanism for detecting connection to the sensor set 10. This would provide the capability to save power and to more quickly and efficiently start initialization of the sensor set 10. In preferred embodiments, the batteries 110 have a life in the range of 3 months to 2 years, and provide a low battery warning alarm. Alternative embodiments may provide longer or shorter battery lifetimes, or include a power port, solar cells or an inductive coil to permit recharging of rechargeable batteries in the telemetered characteristic monitor transmitter 100.

According to the alternative preferred embodiments of the present invention, a

rechargeable battery is used with characteristic monitor transmitter 100'. The electronics of the characteristic monitor transmitter 100' as seen in Figs. 19 and 20 are arranged to work the rechargeable battery 1130 and its associated charger 500. Although the concept of a rechargeable battery in the characteristic monitor transmitter 100 has been proposed in the past, the use of a
5 rechargeable battery is contrary to conventional wisdom. Typically, rechargeable batteries are big and heavy and need heavy current to recharge the battery. However, the characteristic monitor transmitter 100 and 100' are low current circuits that would not work well with conventional rechargeable batteries. In preferred embodiments, the rechargeable battery 1130 is a lithium polymer battery that avoids the problems with conventional rechargeable batteries.
10 The lithium polymer battery has the preferred characteristics of being light, thin, having a high energy density and a shallow current discharge, and good for multiple recharges. In alternative embodiments, different battery chemistry may be used that have the same preferred characteristics of the lithium polymer battery.

The associated charger 500 is shown in Figs 21-23. According to preferred embodiments
15 of the present invention, the charger 500 is a self contained standalone external battery charger for the charging of the characteristic monitor transmitter 100'. Preferably, the charger housing 550 is made from plastic molding to provide a lightweight, water tight design. A single AAA alkaline battery is inserted in the battery compartment 510 and charges the rechargeable battery 1130 when the characteristic monitor transmitter 100' is docked or connected to the charger 500.
20 Fig. 23 shows the configuration when characteristic monitor transmitter 100' is docked in the charger 500. In accordance with the preferred embodiments, the charger 500 provides a docking surface 530 for supporting the transmitter 100' while docked with charger 500. The charger 500 has a male connector 600' to mate with the female connector 400 of the characteristic monitor transmitter 100'. A retention mechanism which is part of the connection system will securely
25 hold the characteristic monitor transmitter 100' in place to ensure that the electrical contacts maintain contact with the charger electrical contact regardless of the rotational orientation of the

charger 500. For example, when a user picks up the charger 500 with the transmitter 100' engaged, the transmitter 100' will remain engaged and continue to be charged even if the charger 500 is turned on its side or upside down. In preferred embodiments, the charger 500 is about 1.6 inches tall in the back and 0.6 inches tall in the front, with a length of 2.25 inches and a width of 1.5 inches. In alternative designs, the charger 500 may be built to larger or smaller dimensions. The charger 500 will also have an indicator 520 to provide visual indication regarding the status of the charger 500 battery as well as the status of the battery integrity and charge status of the transmitter 100'. In preferred embodiments, the indicator 520 is comprised of one or two light emitting diodes (LEDs) that make use of color and various flashing rates to properly communicate information to the user. Preferably, a green light will indicate normal operation and a red light will indicate an abnormal operation. Alternatively, the indication lights 520 can comprise additional LEDs or a larger LCD display to communicate information about the charger 500 and the transmitter 100' to the user.

The charger 500 is able to charge the characteristic monitor transmitter battery 1130 with enough charge to last for at least three days of continuous use of the characteristic monitor transmitter 100'. Fig. 24 is a block diagram describing the charger system 700. As seen in Fig. 24, the charger system 700, according to the preferred embodiments of the present invention, includes the characteristic monitor transmitter 100' and the charger 500, which contains a battery 710, a power source switch and voltage converter circuit 720, charging circuit 730, a status logic circuit 740, an indicator 520, and the connector 600'. As previously discussed, the battery 710 is preferably a AAA battery used to supply the power 810 for the recharging process. The power source switch and voltage converter 720 turns on the charger after receiving a confirmation 820 from the connector 600' that the characteristic monitor transmitter 100' has been docked into the charger 500. In preferred embodiments, the power switch and voltage converter 720 employs the auto power on/auto power off function based on the whether the transmitter 100' is attached to the charger. In alternative embodiments, the power source switch and voltage converter 720 may

be substituted with a mechanical power switch which does not have the auto power on/auto power off feature. Once the charger is turned on, the power source switch and voltage converter 720 steps up the voltage received from the battery 710 to deliver enough power to drive the charging circuit 730 as well as the status logic circuit 740. The charging circuit 730 delivers
5 charging power through the connector 600' to charge the rechargeable battery 1130 located in the transmitter 100'. The status logic circuit 740 monitors when the rechargeable battery 1130 is fully charged or detects any problems with the recharging process by receiving feedback 830. In addition, the status logic circuit 740 also can keep tabs on the life of battery 710. The status logic circuit 740 controls the indicator 520 to make use of color and various flashing rates to properly
10 communicate information to the user. For example in a two LED system, one LED will give information regarding the charger 500 ("LED 1"), and the other LED will give information regarding the rechargeable battery 1130 in the transmitter 100' ("LED 2"). A possible indication protocol would be that LED 1 will flash a green light every two seconds to indicate the charging process is being performed properly or a red light every two second to indicate a low battery
15 power in the battery 710. LED 2 will also flash a green light every two seconds to indicate that the rechargeable battery 1130 is being properly charged (i.e. in this case, both LED 1 & 2 will be flashing green at the same rate) or the LED will flash a continuous green light to indicate that the charging cycle is complete or flash red light to indicate that the rechargeable battery 1130 is not recharging and entire transmitter 100' needs to be replaced. The status logic circuit 740 can
20 employ numerous other protocols to deliver the same basic information to the user.

In alternative embodiments, as seen in Fig. 25, the charger 500 is capable of taking other power sources 780 besides a AAA battery, including but not limited to other conventional battery sources (e.g. AA battery), USB port, wall transformer, or automobile power outlet. If the other power source 780 is a USB port, the USB port may also function as a communications link 850
25 between the transmitter 100' and a computer for such purposes as data downloading or updating the transmitter 100' firmware.

In preferred embodiments, the telemetered characteristic monitor transmitter 100 provides power, through the cable 102 and cable connector 104 to the sensor set 10. The power is used to monitor and drive the sensor set 10. The power connection is also used to speed the initialization of the sensor 12, when it is first placed under the skin. The use of an initialization process can
5 reduce the time for sensor 12 stabilization from several hours to an hour or less. The preferred initialization procedure uses a two step process. First, a high voltage (preferably between 1.0-1.2 volts - although other voltages may be used) is applied to the sensor 12 for 1 to 2 minutes (although different time periods may be used) to allow the sensor 12 to stabilize. Then, a lower voltage (preferably between 0.5-0.6 volts - although other voltages may be used) is applied for
10 the remainder of the initialization process (typically 58 minutes or less). Other stabilization/initialization procedures using differing currents, currents and voltages, different numbers of steps, or the like, may be used. Other embodiments may omit the initialization/stabilization process, if not required by the sensor or if timing is not a factor.

At the completion of the stabilizing process, a reading may be transmitted from the sensor
15 set 10 and the telemetered characteristic monitor transmitter 100 to the characteristic monitor 200, and then the user will input a calibrating glucose reading into characteristic monitor 200. In alternative embodiments, a fluid containing a known value of glucose may be injected into the site around the sensor set 10, and then the reading is sent to the characteristic monitor 200 and the user inputs the known concentration value, presses a button (not shown) or otherwise
20 instructs the monitor to calibrate using the known value. During the calibration process, the telemetered characteristic monitor transmitter 100 checks to determine if the sensor set 10 is still connected. If the sensor set 10 is no longer connected, the telemetered characteristic monitor transmitter 100 will abort the stabilization process and sound an alarm (or send a signal to the characteristic monitor 200 to sound an alarm).

25 Preferably, the transmissions (or telemetry) of the telemetered characteristic monitor transmitter 100 will contain at least the following information: a unique ID code that uniquely

identifies each telemetered characteristic monitor transmitter 100, a sensor characteristic data signal representative of the measured characteristic value (e.g., glucose or the like) from the sensor 18 of the subcutaneous sensor set 10, a counter electrode voltage, a low battery flag, and error detection bits (such as CRC). Fig. 9 and Table 1 illustrate a preferred message format for the telemetry of the telemetered characteristic monitor transmitter 100. However, it will be understood that different message protocols and structures may be used.

1.	Encoding method: OOK MANCHESTER (1=1/0, 0=0/1 sequence, where 1 = transmitter (TX) on)
2.	Clock rate 1024 Hz (512Hz symbol/bit rate).
3.	Message format:
	Preamble: 4 bits (0101, want only one transition per bit)
	Message Type: 4 bits (1010 = transmitter 100, 15 others for pump/ppc protocol)
	Unique ID #: 16 bits (65536 unique numbers)
	Message count #: 4 bits (also determines TX time slot)
	Working Electrode: 12 bits (9MSBs + 3 magnitude bits = 16bit range – converted by the characteristic monitor 200 into a value representative of characteristic level, such as glucose level)
	Low battery flag: 1 bit (0=ok, 1=low)
	Counter Voltage: 7 bits (0-1.2V typ., 8bit a/d 3.2V FS)
	CRC: 8 bits
	Total 56 bits (x 1/512hz = 109 mS)
4.	Message TX interval: 300 seconds (5 min) + 1-16 seconds pseudo-random delay (TX time slot)
5.	TX duty cycle: $56\text{bits} \times 1/512\text{Hz} \times 1/300\text{S} \times 1/2 = 1.823\text{e-}4$

Table 1. Message format

Preferred embodiments utilize a time-slicing transmission protocol. Use of the time slicing protocol facilitates the use of multiple signals on the same frequency bands or to the same receiver from multiple transmitters. The time-slicing may also be used to obviate the need for a receiver in the telemetered characteristic monitor transmitter 100. For instance, the use of intermittent transmission reduces the amount of power required to operate the transmitter 100 and to extend the life of the device. It also saves power in the characteristic monitor 200 by

reducing the amount of time the characteristic monitor 200 must spend in the receive mode.

In preferred embodiments, when the telemetered characteristic monitor transmitter 100 is connected to the sensor set 10, it detects the connection and is activated. Next, if desired or necessary, the telemetered characteristic monitor transmitter 100 initializes the sensor 12 of the sensor set 10. After (or in some cases during) initialization, the telemetered characteristic monitor transmitter 100 sends out a message of between 100-150 ms length every 5 minutes. Although other timing intervals ranging from 1 second to 30 minutes may be used.

Preferably, the message is transmitted in a pseudo-randomly selected time window within the 128 seconds following the 5 minute interval. In preferred embodiments, the telemetered characteristic transmitter 100 utilizes its own unique ID as a random-seed to set up a table of transmission time windows that defines the order in which the telemetered characteristic monitor 100 will transmit a message following the 5 minute interval. The order is repeated after the table is set-up. Included in the message sent will be the message count number, which indicates where in the sequence of time windows the telemetered characteristic monitor transmitter is currently transmitting. The characteristic monitor 200 uses the unique ID code of the telemetered characteristic monitor transmitter 100 to set up a corresponding table in the characteristic monitor 200 and the received message count to synchronize the characteristic monitor 200 with the current position in the table being used by the telemetered characteristic monitor transmitter 100 to predict the next time window to be used. The use of pseudo-random time windows prevents multiple transmitters from continuously interfering with other transmitting devices that are temporarily, or inadvertently, synchronized with the telemetered characteristic monitor transmitter 100. The characteristic monitor 200 acquires the transmitted message, and determines the time window in which the characteristic monitor 200 must be in a receive mode to acquire the next message. The characteristic monitor 200 then places itself in the receive mode every 5 minutes (although other timing intervals from 1 second to 30 minutes may be used) to receive the next message and data from the telemetered characteristic monitor transmitter 100 at

the next predicted time window. Thus, the characteristic monitor 200 needs only be in the receive mode for 1 second (i.e., 1 time window); rather than 128 seconds (128 time windows). In alternative embodiments, the characteristic monitor 200 may not use the unique ID and the message count and may remain in the receive mode during the entire period (e.g., for 128 time windows) during which a transmission is possible. In addition, other embodiments may cause the characteristic monitor 200 to enter the receive mode 1 time window ahead and stay on for 1 time window longer to maximize the likelihood of receiving the next transmission. In further alternative embodiments, the telemetered characteristic monitor transmitter 100 and/or characteristic monitor 200 may utilize other methods or numbers to determine when transmission time windows are selected. Alternative message time-slicing transmission parameters, such as message length, number of time windows, frequency of transmissions, or the like, that are larger or smaller than those describe above, may also be used. Preferred embodiments transmit the data and/or information at a data rate between 1000 Hz to 4000 Hz modulated onto a high frequency carrier wave. However, alternative embodiments may use smaller or larger transmission rates, with the rate being selected based on user environment, power requirements, interference issues, redundancy criteria, or the like.

If a transmitted message is not received by the characteristic monitor 200 after a predetermined period of time, an alarm will be sounded or provided. In addition, the characteristic monitor 200 may continue to attempt to receive the next message by entering the receive mode at the next anticipated transmission time or may expand to enter the receive mode to cover all time windows until the next message is received.

In another alternative embodiment, if there is little or no likelihood of interference from other telemetered characteristic monitor transmitter 100, such as by message length, frequency selections or the like, the telemetered characteristic monitor transmitter 100 may transmit at one time window for all cases (typically the choice of window may be randomly selected at connection of a sensor set 10 or set at the factory). This permits the characteristic monitor 200 to

be in the receive mode for even shorter periods of time (i.e., approximately 200 ms to bracket the telemetered characteristic monitor transmitter 100 transmission instead of the 128 seconds (or 1 second if able to predict the next time window) needed to bracket 128 windows) to conserve power in the characteristic monitor 200. For instance, in this scenario, the characteristic monitor
5 200 will be in a non-receive mode for 299.8 seconds and in a receive mode for 200 ms. In particular embodiments the non-receive mode and receive mode periods will be determined by the message length and expected frequency of transmission. It is also noted that in a system where the receiver must cover a range of time windows, the receiver may lock on to a particular range of time windows to permit the receiver being in the receive mode for shorter periods of
10 time.

The use of these transmission protocols obviates the need for a transmitter and receiver in both the telemetered characteristic monitor transmitter 100 and characteristic monitor 200, which reduces costs, simplifies the system design, reduces power consumption and the like. However, alternative embodiments may include the capability for two-way communication, if desirable. In
15 further embodiments, the telemetered characteristic monitor transmitter 100 transmits continuously and the characteristic monitor 200 enters the receive mode when desired or required to determine a characteristic value, such as a glucose level or the like.

In preferred embodiments, the telemetered characteristic monitor transmitter 100 will have the ability to uniquely identify itself to the characteristic monitor 200. The telemetered
20 characteristic monitor transmitter 100 will have an operating range to the characteristic monitor 200 of at least 10 feet. In alternative embodiments, larger or smaller ranges may be used, with the selection being dependent on the environment in which the telemetered characteristic monitor transmitter 100 will be used, the size and needs of the user, power requirements, and the like.

In further alternative embodiments, the telemetered characteristic monitor transmitter 100
25 can be combined with a sensor set 10 as a single unit. This would be particularly well adapted where batteries and the transmitter can be made cheaply enough to facilitate changing the

transmitter 100 with each new sensor set 10.

As shown in Fig. 10, the characteristic monitor 200 includes a telemetry receiver 202, a Telemetry Decoder (TD) 204 and a host micro-controller (Host) 206 for communication with the telemetered characteristic monitor transmitter 100. The TD 204 is used to decode a received
5 telemetry signal from the transmitter device and forward the decoded signal to the Host 206. The Host 206 is a microprocessor for data reduction, data storage, user interface, or the like. The telemetry receiver 202 receives the characteristic data (e.g., glucose data) from the telemetered characteristic monitor transmitter, and passes it to the TD 204 for decoding and formatting. After complete receipt of the data by the TD 204, the data is transferred to the Host 206 for processing,
10 where calibration information, based upon user entered characteristic readings (e.g., blood glucose readings), is performed to determine the corresponding characteristic level (e.g., glucose level) from measurement in the characteristic data (e.g., glucose data). The Host 206 also provides for storage of historical characteristic data, and can download the data to a personal computer, lap-top, or the like, via a com-station, wireless connection, modem or the like. For
15 example, in preferred embodiments, the counter electrode voltage is included in the message from the telemetered characteristic monitor transmitter 100 and is used as a diagnostic signal. The raw current signal values generally range from 0 to 999, which represents sensor electrode current in the range between 0.0 to 99.9 nanoAmperes, and is converted to characteristic values, such as glucose values in the range of 40 to 400 mg/dl. However, in alternative embodiments,
20 larger or smaller ranges may be used. The values are then displayed on the characteristic monitor 200 or stored in data memory for later recall.

The characteristic monitor 200 also includes circuitry in the TD 204 to uniquely mate it to an identified telemetered characteristic monitor transmitter 100. In preferred embodiments, the identification number of the telemetered characteristic monitor transmitter 100 is entered
25 manually by the user using keys located on the characteristic monitor 200. In alternative embodiments, the characteristic monitor 200 includes a "learn ID" mode. Generally, the "learn

ID” mode is best suited for the home environment, since multiple telemetered characteristic monitor transmitters 100, typically encountered in a hospital setting, are less likely to cause confusion in the characteristic monitor 200 when it attempts to learn an ID code. In addition, the characteristic monitor 200 will include the ability to learn or be reprogrammed to work with a different (or replacement) telemetered characteristic monitor transmitter 100. The preferred operating distance is at least 10 feet. In alternative embodiments, larger or smaller ranges may be used, with the selection being dependent on the environment in which the telemetered characteristic monitor transmitter 100 will be used, the size and needs of the user, power requirements, and the like. Furthermore, if the characteristic monitor 200 does not receive a transmission from the identified telemetered characteristic monitor transmitter 100 after a certain period of time (e.g., one or more missed transmissions), an alarm will be sounded.

In preferred embodiments, the characteristic monitor 200 utilizes a two processor system, in which the Host 206 is the master processor and the TD 204 is a slave processor dedicated to telemetry processing. A first communication protocol between the Host 206 and the TD 204 is shown in Fig. 11. The first protocol uses a serial peripheral interface (SPI) 208 and two control lines 210 and 212; one control line (chip select – CSPIC) 210 is used by Host 206 to wake up the TD 204 to initiate telemetry receiving task; and the other control line (data ready – DR) 212 is used by the TD 204 to indicate to the Host 206 that the telemetry data from the telemetered characteristic monitor transmitter has been received and is ready to be transferred to the HC08 206. Upon receiving data through the SPI 208, the Host 206 sends an acknowledgment through the SPI 208 to the TD 204. In preferred embodiments, fixed length data blocks are used. However, in alternative embodiments, variable length data blocks may be used. In preferred embodiments, the Host 206 may pull the Chip Select (CSPIC) 210 high at any time to abort the telemetry data transfer from the TD 204. Alternatively, an additional line (not shown) may be used to reset the TD 204. Fig. 12 shows a second, more complex, alternative protocol that is used by the Host 206 and the TD 204.

In alternative embodiments, the TD 204 and Host 206 may be combined together in a single semiconductor chip to obviate the need for dual processors and to reduce the space needed for the electronics. In further embodiments, the functions of the TD 204 and Host 206 may be allocated differently between one or more processors.

5 As shown in Fig. 2, the characteristic monitor may include a display 214 that is used to display the results of the measurement received from the sensor 18 in the sensor set 10 via the telemetered characteristic monitor transmitter 100. The results and information displayed includes, but is not limited to, trending information of the characteristic (e.g., rate of change of glucose), graphs of historical data, average characteristic levels (e.g., glucose), or the like.

10 Alternative embodiments include the ability to scroll through the data. The display 214 may also be used with buttons (not shown) on the characteristic monitor to program or update data in the characteristic monitor 200. It is noted that the typical user can be expected to have somewhat diminished visual and tactile abilities due to complications from diabetes or other conditions. Thus, the display 214 and buttons should be configured and adapted to the needs of a user with
15 diminished visual and tactile abilities. In alternative embodiments, the value can be conveyed to the user by audio signals, such as beeps, speech or the like. Still further embodiments may use a touch screen instead of (or in some cases addition to) buttons to facilitate water proofing and to ease changes in the characteristic monitor 200 hardware to accommodate improvements or upgrades.

20 Preferably, the characteristic monitor uses batteries (not shown) to provide power to the characteristic monitor. For example, a plurality of silver oxide batteries may be used. However, it is understood that different battery chemistries may be used, such as lithium based, alkaline based, nickel metalhydride, or the like, and different numbers of batteries can be used. In preferred embodiments, the batteries have a life in the range of 1 month to 2 years, and provide a
25 low battery warning alarm. Alternative embodiments may provide longer or shorter battery lifetimes, or include a power port, solar cells or an induction coil to permit recharging of

rechargeable batteries in the characteristic monitor 200. In preferred embodiments, the batteries are not replaceable to facilitate waterproofing the housing 106.

In further embodiments of the present invention, the characteristic monitor 200 may be replaced by a different device. For example, in one embodiment, the telemetered characteristic
5 monitor transmitter 100 communicates with an RF programmer (not shown) that is also used to program and obtain data from an infusion pump or the like. The RF programmer may also be used to update and program the transmitter 100, if the transmitter 100 includes a receiver for remote programming, calibration or data receipt. The RF programmer can be used to store data obtained from the sensor 18 and then provide it to either an infusion pump, characteristic
10 monitor, computer or the like for analysis. In further embodiments, the transmitter 100 may transmit the data to a medication delivery device, such as an infusion pump or the like, as part of a closed loop system. This would allow the medication delivery device to compare sensor results with medication delivery data and either sound alarms when appropriate or suggest corrections to the medication delivery regimen. In preferred embodiments, the transmitter 100 would include a
15 transmitter to receive updates or requests for additional sensor data. An example of one type of RF programmer can be found in U.S. Patent Application Serial No. 60/096,994 filed August 18, 1998 and is entitled "INFUSION DEVICE WITH REMOTE PROGRAMMING, CARBOHYDRATE CALCULATOR AND/OR VIBRATION ALARM CAPABILITIES," or U.S. Patent Application Serial No. 09/334,858 filed June 17, 1999 and is entitled "EXTERNAL
20 INFUSION DEVICE WITH REMOTE PROGRAMMING, BOLUS ESTIMATOR AND/OR VIBRATION ALARM CAPABILITIES," both of which are herein incorporated by reference.

In further embodiments, the telemetered characteristic monitor transmitter can include a modem, or the like, to transfer data to and from a healthcare professional. Further embodiments, can receive updated programming or instructions via a modem connection.

25 In use, the sensor set 10 permits quick and easy subcutaneous placement of the active sensing portion 18 at a selected site within the body of the user. More specifically, the peel-off

strip 34 (see Fig. 1) is removed from the mounting base 30, at which time the mounting base 30 can be pressed onto and seated upon the patient's skin. During this step, the insertion needle 14 pierces the user's skin and carries the protective cannula 16 with the sensing portion 18 to the appropriate subcutaneous placement site. During insertion, the cannula 16 provides a stable
5 support and guide structure to carry the flexible sensor 12 to the desired placement site. When the sensor 12 is subcutaneously placed, with the mounting base 30 seated upon the user's skin, the insertion needle 14 can be slidably withdrawn from the user. During this withdrawal step, the insertion needle 14 slides over the first portion 48 of the protective cannula 16, leaving the sensing portion 18 with electrodes 20 directly exposed to the user's body fluids via the window
10 22. Further description of the needle 14 and the sensor set 10 are found in U.S. Patent No. 5,586,553, entitled "TRANSCUTANEOUS SENSOR INSERTION SET"; co-pending U.S. Patent Application Serial No. 08/871,831, entitled 'DISPOSABLE SENSOR INSERTION ASSEMBLY'; and co-pending U.S. Patent Application Serial No. 09/161,128, filed September 25, 1998, entitled "A SUBCUTANEOUS IMPLANTABLE SENSOR SET HAVING THE
15 CAPABILITY TO REMOVE OR DELIVER FLUIDS TO AN INSERTION SITE," which are herein incorporated by reference.

Next, the user connects the connection portion 24 of the sensor set 10 to the cable 102 of the telemetered characteristic monitor transmitter 100, so that the sensor 12 can then be used over a prolonged period of time for taking blood chemistry or other characteristic readings, such as
20 blood glucose readings in a diabetic patient. Preferred embodiments of the telemetered characteristic monitor transmitter 100 detect the connection of the sensor 12 to activate the telemetered characteristic monitor transmitter 100. For instance, connection of the sensor 12 may activate a switch or close a circuit to turn the telemetered characteristic monitor transmitter 100 on. The use of a connection detection provides the capability to maximize the battery and
25 shelf life of the telemetered characteristic monitor transmitter prior to use, such as during manufacturing, test and storage. Alternative embodiments of the present invention may utilize an

on/off switch (or button) on the telemetered characteristic monitor transmitter 100.

The transmitter 100 is then affixed to the user's body with an adhesive overdressing. Alternatively, the peel-off strip 34 (see Fig. 1) is removed from the lower case 116, at which time the lower case 116 can be pressed onto and seated upon the patient's skin. The user then
5 activates the transmitter 100, or the transmitter is activated by detection of the connection to the sensor 12 of the sensor set 10. Generally, the act of connecting (and disconnecting) the sensor 12 activates (and deactivates) the telemetered characteristic monitor 100, and no other interface is required. In alternative steps, the sensor set 10 is connected to the transmitter 100 prior to
10 placement of the sensor 12 to avoid possible movement or dislodging of the sensor 12 during attachment of the transmitter 100. Also, the transmitter may be attached to the user prior to attaching the sensor set 10 to the transmitter 100.

The user then programs the characteristic monitor (or it learns) the identification of the transmitter 100 and verifies proper operation and calibration of the transmitter 100. The characteristic monitor 200 and transmitter 100 then work to transmit and receive sensor data to
15 determine characteristic levels. Thus, once a user attaches a transmitter 100 to a sensor set 10, the sensor 12 is automatically initialized and readings are periodically transmitted, together with other information, to the characteristic monitor 200.

After a sensor set 10 has been used for a period of time, it is replaced. The user will disconnect the sensor set 10 from the cable 102 of the telemetered characteristic monitor
20 transmitter 100. In preferred embodiments, the telemetered characteristic monitor transmitter 100 is removed and posited adjacent the new site for a new sensor set 10. In alternative embodiments, the user does not need to remove the transmitter 100. A new sensor set 10 and sensor 12 are attached to the transmitter 100 and connected to the user's body. Monitoring then continues, as with the previous sensor 12. If the user must replace the telemetered characteristic
25 monitor transmitter 100, the user disconnects the transmitter 100 from the sensor set 10 and the user's body. The user then connects a new transmitter 100, and reprograms the characteristic

monitor (or learns) to work with the new transmitter 100. Monitoring then continues, as with the previous sensor 12.

Additional embodiments of the present invention may include a vibrator alarm (or optional indicator such as an L.E.D.) in either or both the telemetered characteristic monitor transmitter 100 and the characteristic monitor 200 to provide a tactile (vibration) alarm to the user, such as sensor set malfunction, improper connection, low battery, missed message, bad data, transmitter interference, or the like. The use of a vibration alarm provides additional reminders to an audio alarm, which could be important with someone suffering an acute reaction, or to have non-audio alarms to preserve and conceal the presence of the telemetered characteristic monitor system 1.

While the description above refers to particular embodiments of the present invention, it will be understood that many modifications may be made without departing from the spirit thereof. The accompanying claims are intended to cover such modifications as would fall within the true scope and spirit of the present invention.

The presently disclosed embodiments are therefore to be considered in all respects as illustrative and not restrictive, the scope of the invention being indicated by the appended claims, rather than the foregoing description, and all changes which come within the meaning and range of equivalency of the claims are therefore intended to be embraced therein.

WHAT IS CLAIMED IS:

1. An external telemetered characteristic monitor system for monitoring a characteristic of a user, the system comprising:

a remotely located data device;

5 a sensor set supporting a sensor for producing a signal indicative of the characteristic of the user;

an external transmitter device coupled to the sensor set including:

a housing;

a sensor connector coupled to the housing and that is connectable to the sensor set

10 to receive signals from the sensor;

a processor within the housing coupled to the sensor connector to process the signals from the sensor for delivery to the remotely located data device;

a transmitter coupled to the processor for wirelessly transmitting the processed signals to the remotely located data device, wherein the remotely located data device

15 utilizes the received processed signals to determine a characteristic reading of the user;

and

a rechargeable battery within the housing to power the transmitter and the sensor;

and

an associated charger that mates with the sensor connector of the external transmitter

20 device to recharge the rechargeable battery of the external transmitter device when needed.

2. The external telemetered characteristic monitor system according to claim 1, wherein the sensor set supports the external transmitter device when coupled to the sensor set.

3. The external telemetered characteristic monitor system according to claim 1,
wherein the sensor is implantable in tissue selected from the group consisting essentially of
subcutaneous, dermal, sub-dermal, intra-peritoneal and peritoneal tissue, and wherein the sensor
5 connector is directly connected to the sensor externally of the body.
4. The external telemetered characteristic monitor system according to claim 1,
wherein the charger detects when the external transmitter device is mated with the charger and
automatically charges the rechargeable battery.
- 10 5. The external telemetered characteristic monitor system according to claim 1,
wherein the charger has an indication device to communicate status of how the charger is
charging the rechargeable battery.
- 15 6. The external telemetered characteristic monitor system according to claim 1,
wherein the charger is battery-powered.
7. The external telemetered characteristic monitor system according to claim 1,
wherein the charger powered by an external power source.
- 20 8. The external telemetered characteristic monitor system according to claim 7,
wherein the external power source is a USB port.
9. The external telemetered characteristic monitor system according to claim 8,
25 wherein the USB port can also act as a communication link between the external transmitter
device and a computer.

10. The external characteristic monitor system according to claim 1, wherein the data device is an RF programmer for a medical device.

5 11. The external telemetered characteristic monitor system according to claim 1, wherein the data device is a characteristic monitor that displays the characteristic reading of the user.

10 12. The external telemetered characteristic monitor system according to claim 1, wherein the data device is a medication delivery device.

13. The external telemetered characteristic monitor system according to claim 12, wherein the medication delivery device is an infusion pump.

15 14. The external telemetered characteristic monitor transmitter device according to claim 1, wherein the telemetered characteristic monitor transmitter is activated by detection of a connection of the sensor to the sensor connector.

20 15. The external telemetered characteristic monitor transmitter device according to claim 1, further including a relay device, between the transmitter and data receiving device, to receive processed signals from the transmitter and relay them to the data receiving device.

25 16. The external telemetered characteristic monitor transmitter device according to claim 15, wherein the relay device increases a maximum distance by amplifying the processed signals from the transmitter to be received by the remotely located data receiving device.

17. The external telemetered characteristic monitor transmitter device according to claim 16, wherein the relay device enables the remotely located data receiving device to be located in a different room than the transmitter.

5

18. The external telemetered characteristic monitor transmitter device according to claim 15, wherein the relay device includes a telecommunication device, and wherein when the transmitter generates an alarm which the telecommunication device transmits the alarm to a remotely located receiving station.

10

ABSTRACT OF THE DISCLOSURE

A telemetered characteristic monitor system includes a remotely located data receiving device, a sensor for producing signal indicative of a characteristic of a user, and a transmitter device. The transmitter device includes a housing, a sensor connector, a processor, and a
5 transmitter. The transmitter receives the signals from the sensor and wirelessly transmits the processed signals to the remotely located data receiving device. The processor coupled to the sensor processes the signals from the sensor for transmission to the remotely located data receiving device. The data receiving device may be a characteristic monitor, a data receiver that provides data to another device, an RF programmer for a medical device, a medication delivery
10 device (such as an infusion pump), or the like.

+

FIG. 1


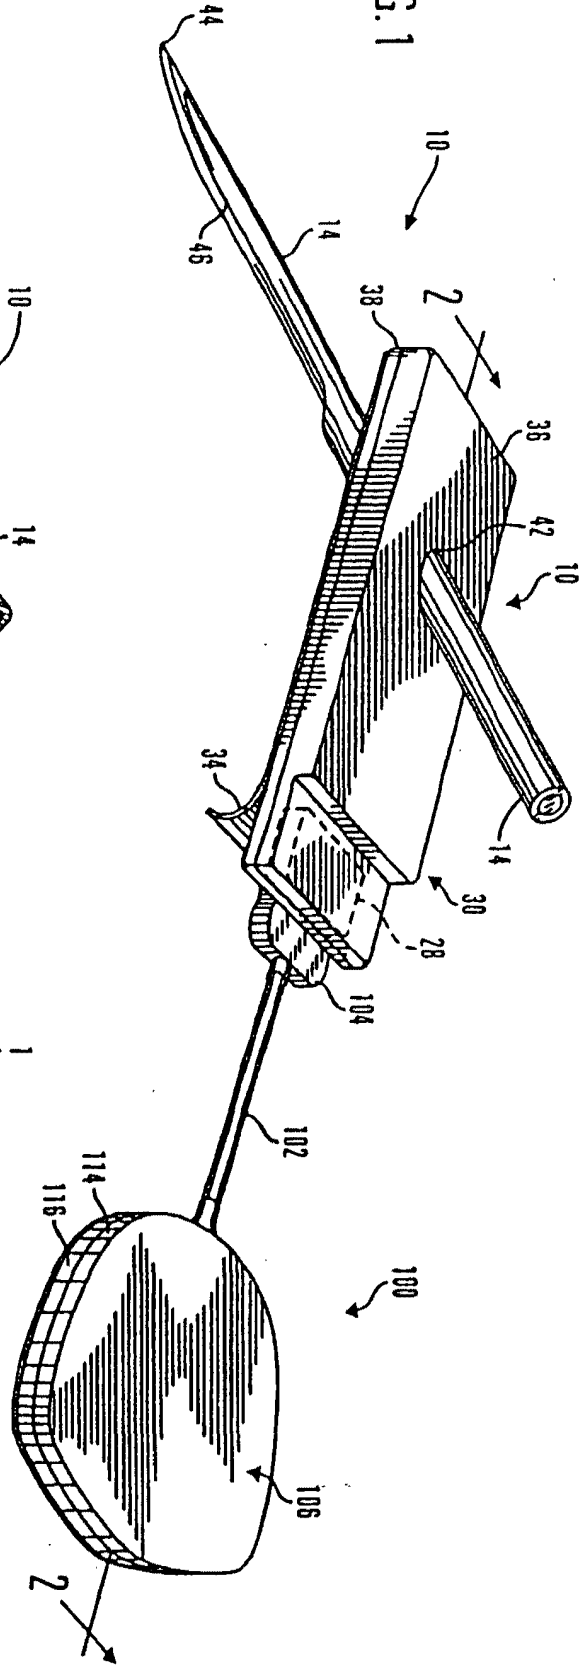


FIG. 2

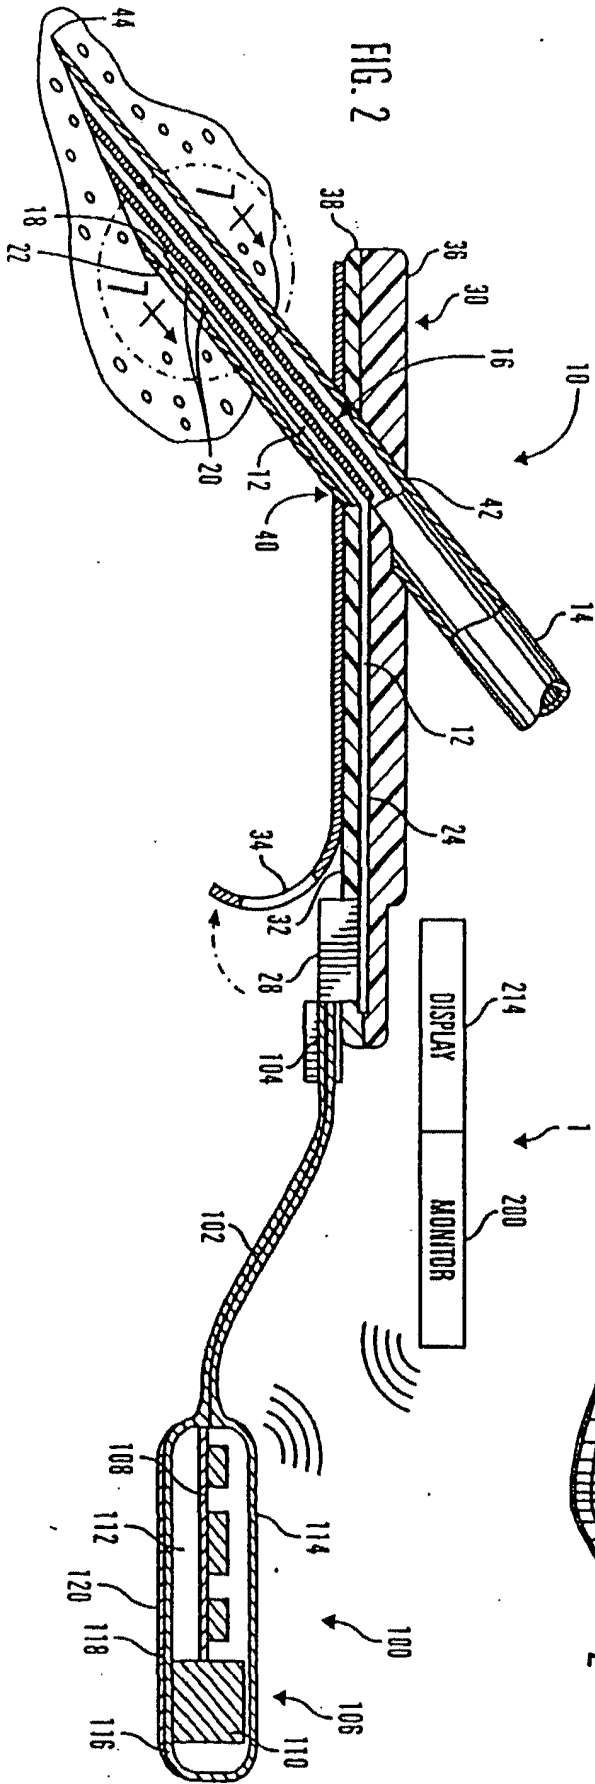

+

+

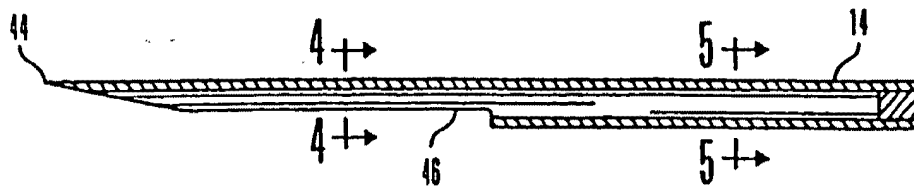


FIG. 3




FIG. 4




FIG. 5

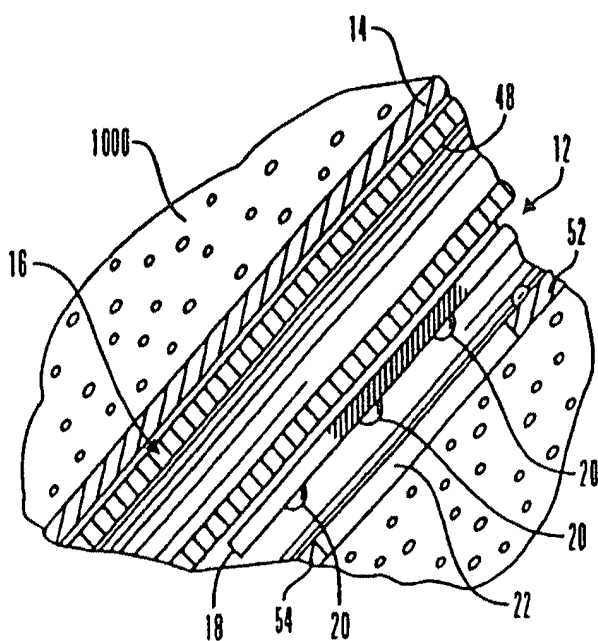


FIG. 6

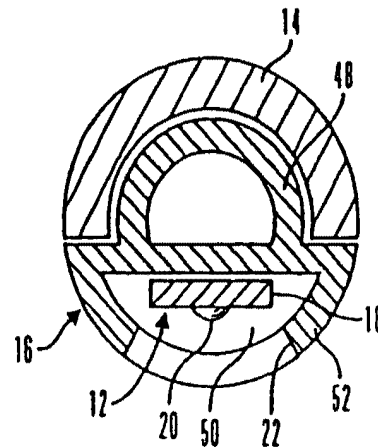


FIG. 7

+

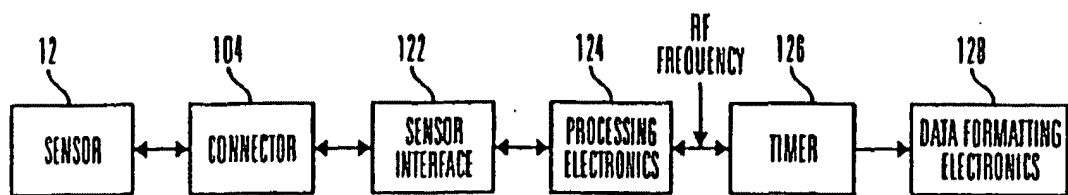
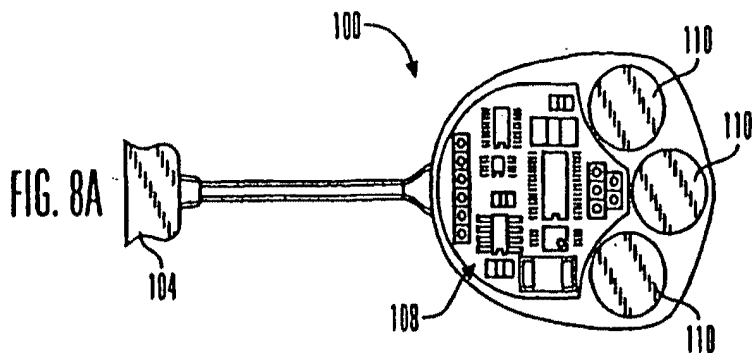


FIG. 8B



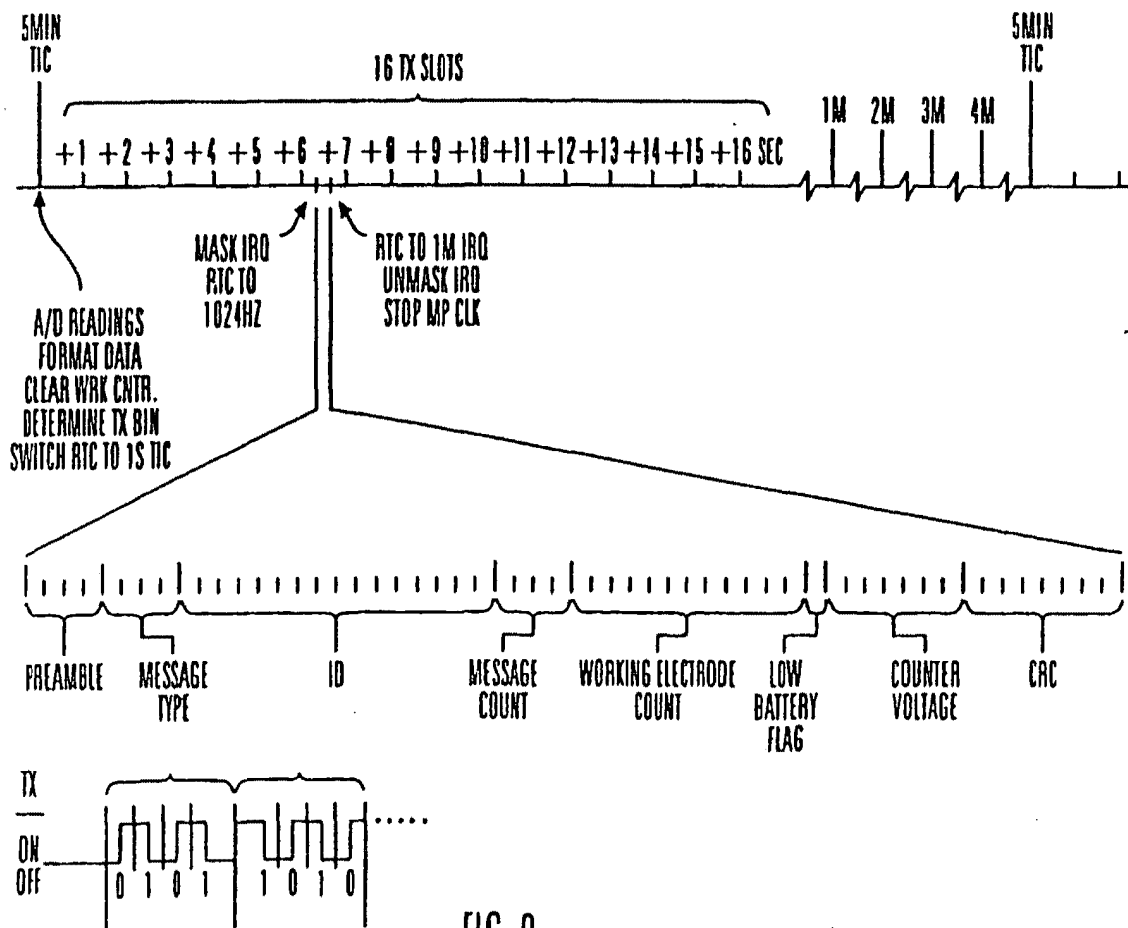


FIG. 9

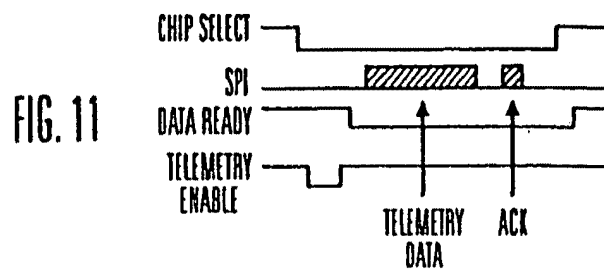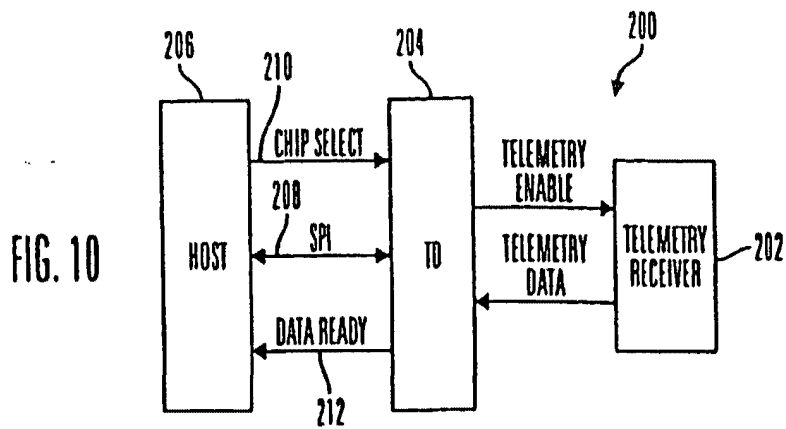

HOST INITIATES RF SESSION

TD WAKES UP
THROUGH RBO / INT

TD SIGNALS DATA READY

HOST SENDS COMMAND

TD SENDS STATUS
DATA TO HOST

TD ENABLES RF RECEIVER

TD COLLECTS RF DATA

HOST TERMINATES
RF SESSION

TD CLOSES OUT
RF SESSION AND
GOES TO SLEEP

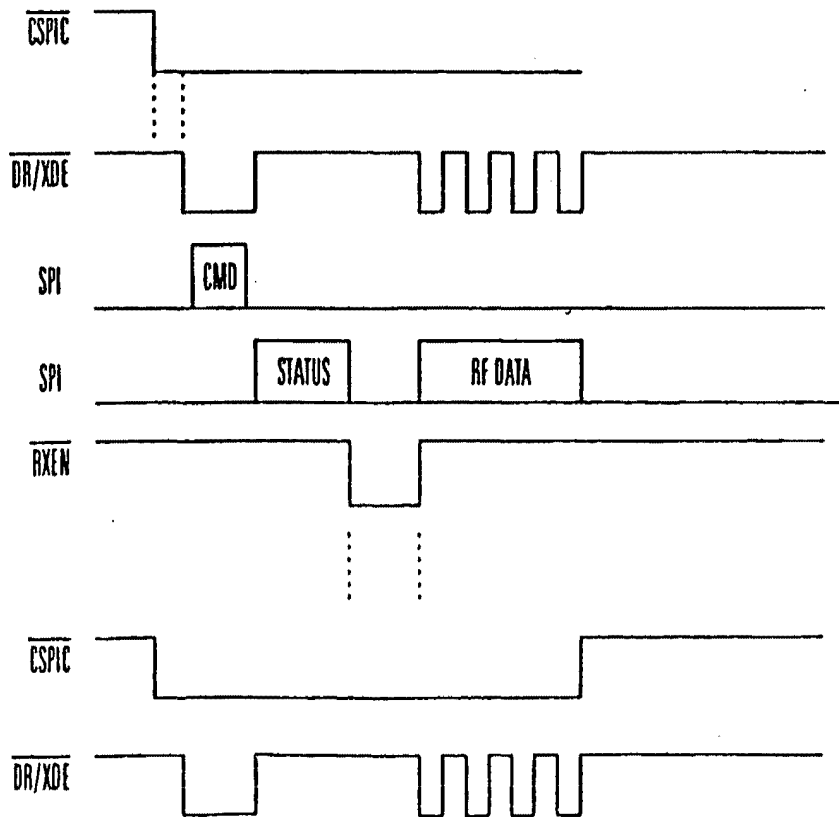


FIG. 12

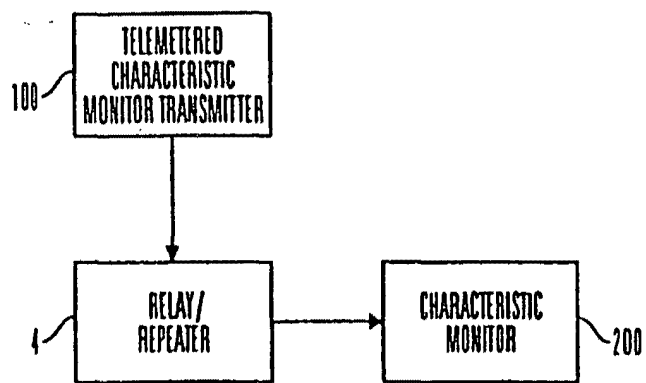


FIG. 13

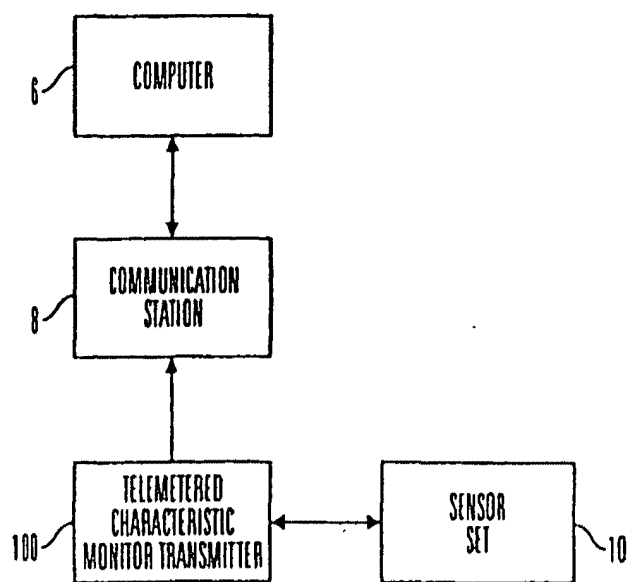


FIG. 14

FIGURE 15


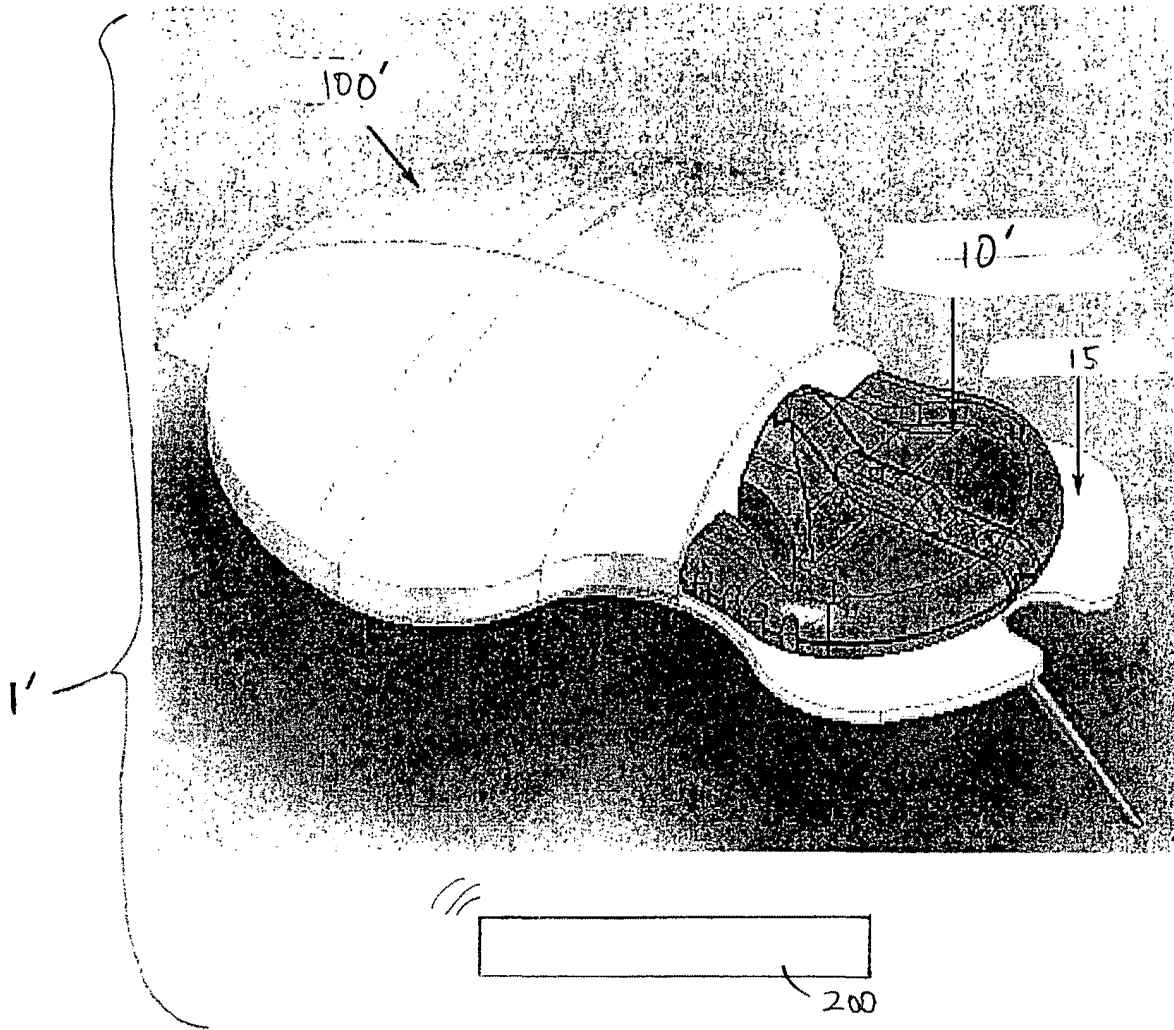


FIGURE 16

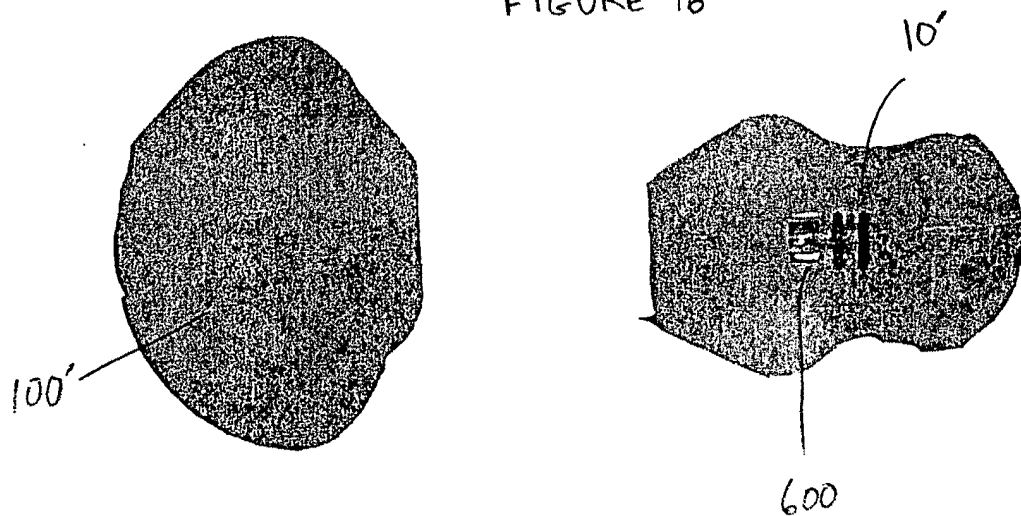

BEST AVAILABLE COPY

100'

FIGURE 17


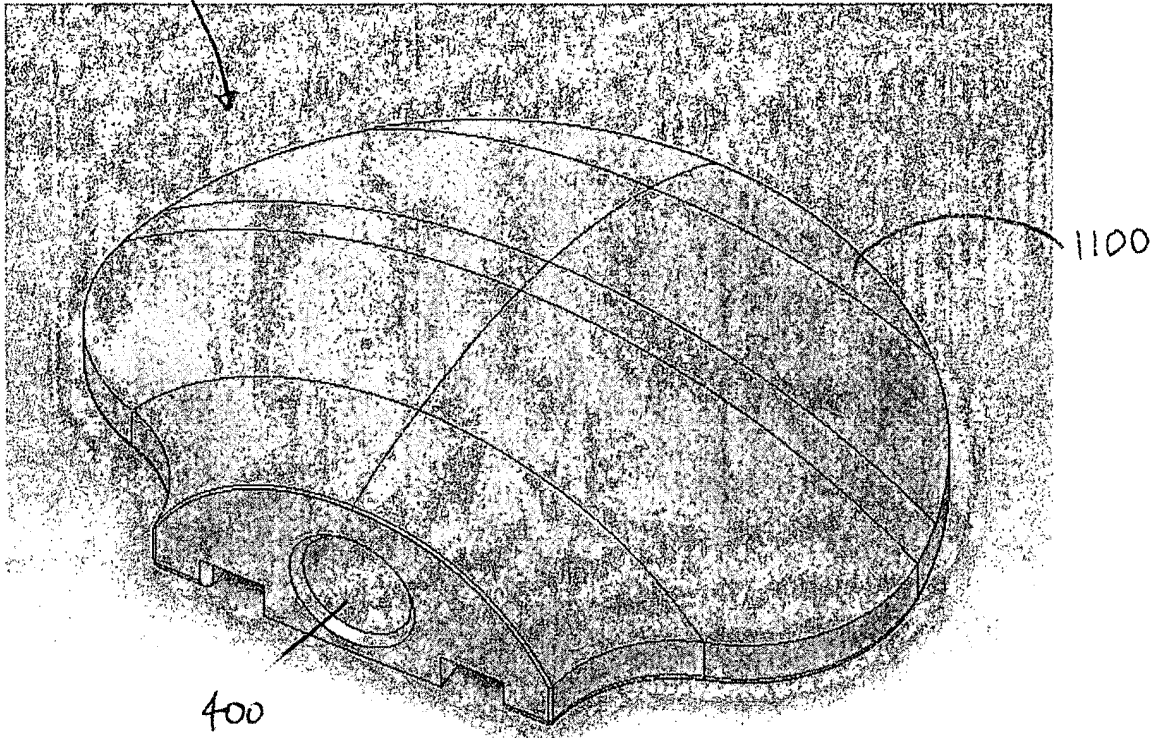


FIGURE 18

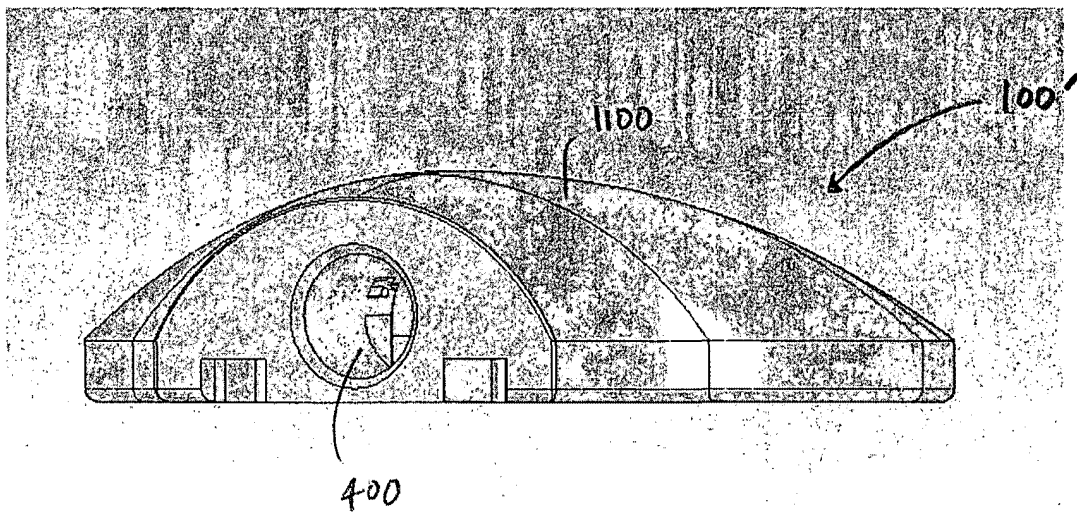

BEST AVAILABLE COPY

FIGURE 19


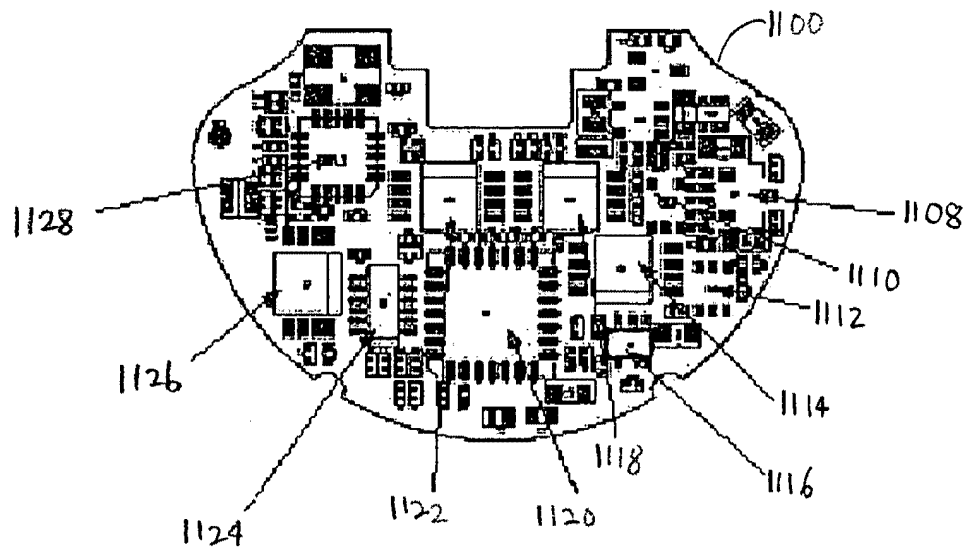


FIGURE 20

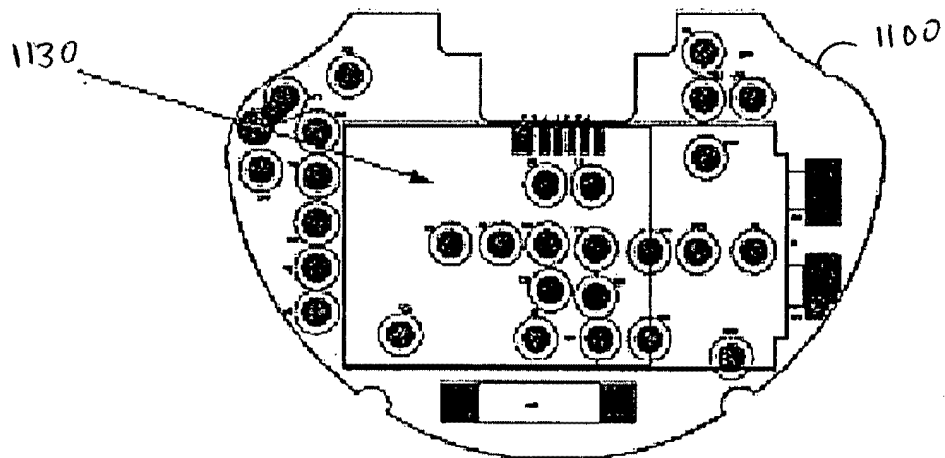

BEST AVAILABLE COPY

FIGURE 21



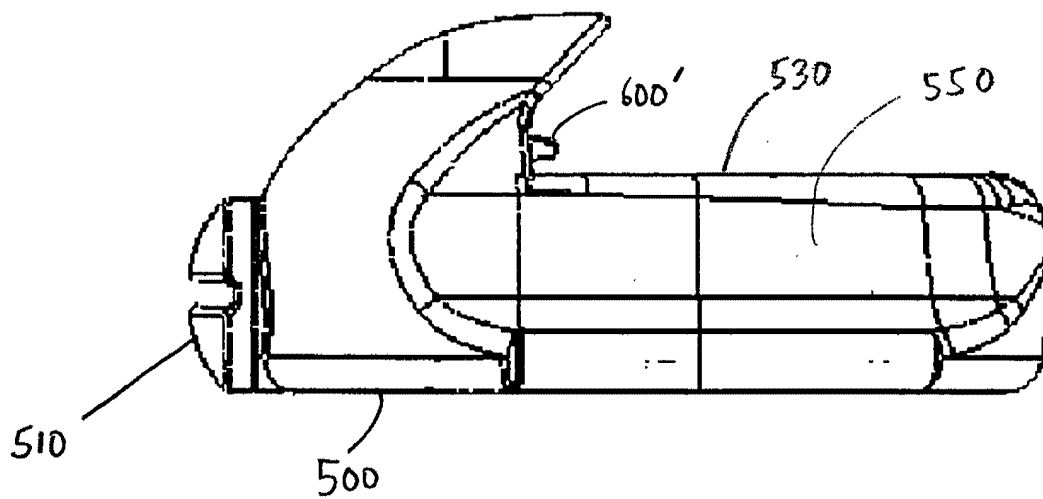


FIGURE 22

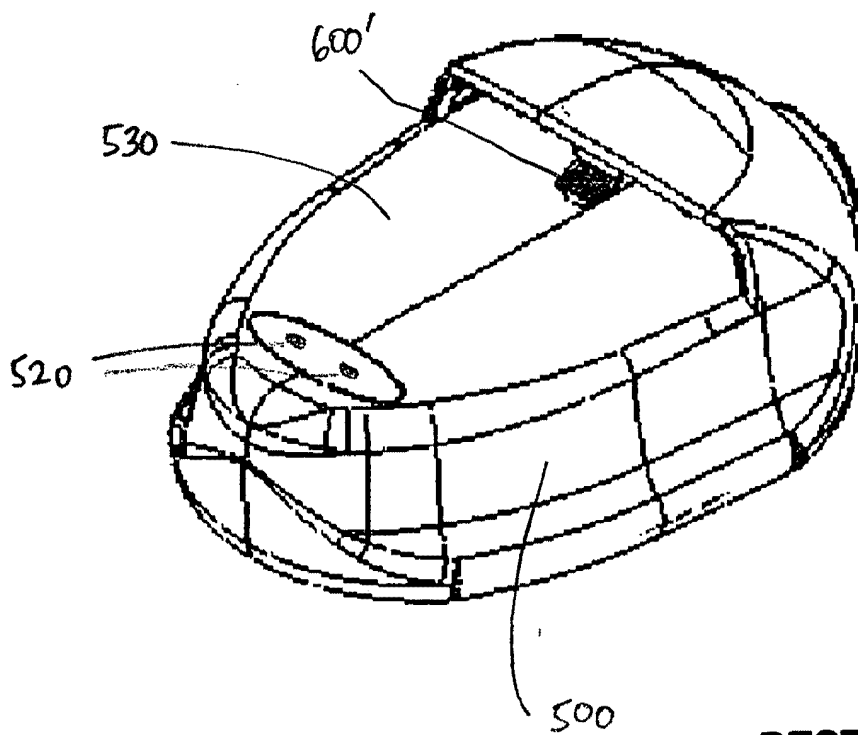

BEST AVAILABLE COPY

FIGURE 23

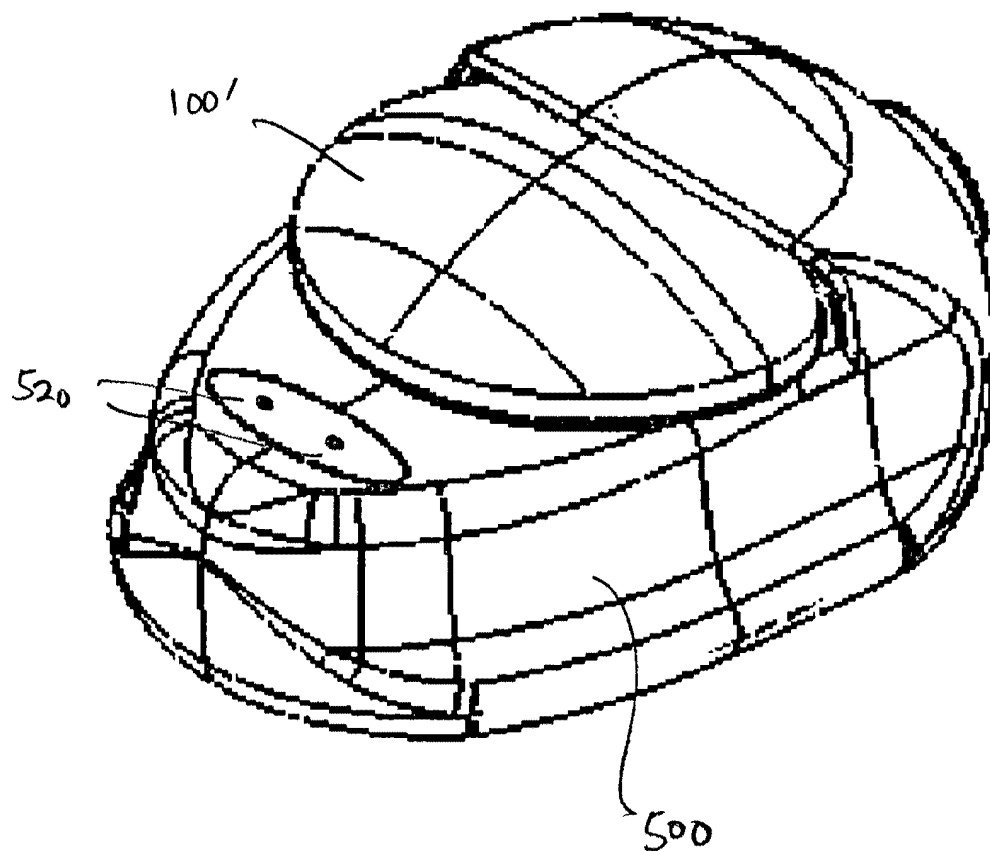

BEST AVAILABLE COPY

FIGURE 24


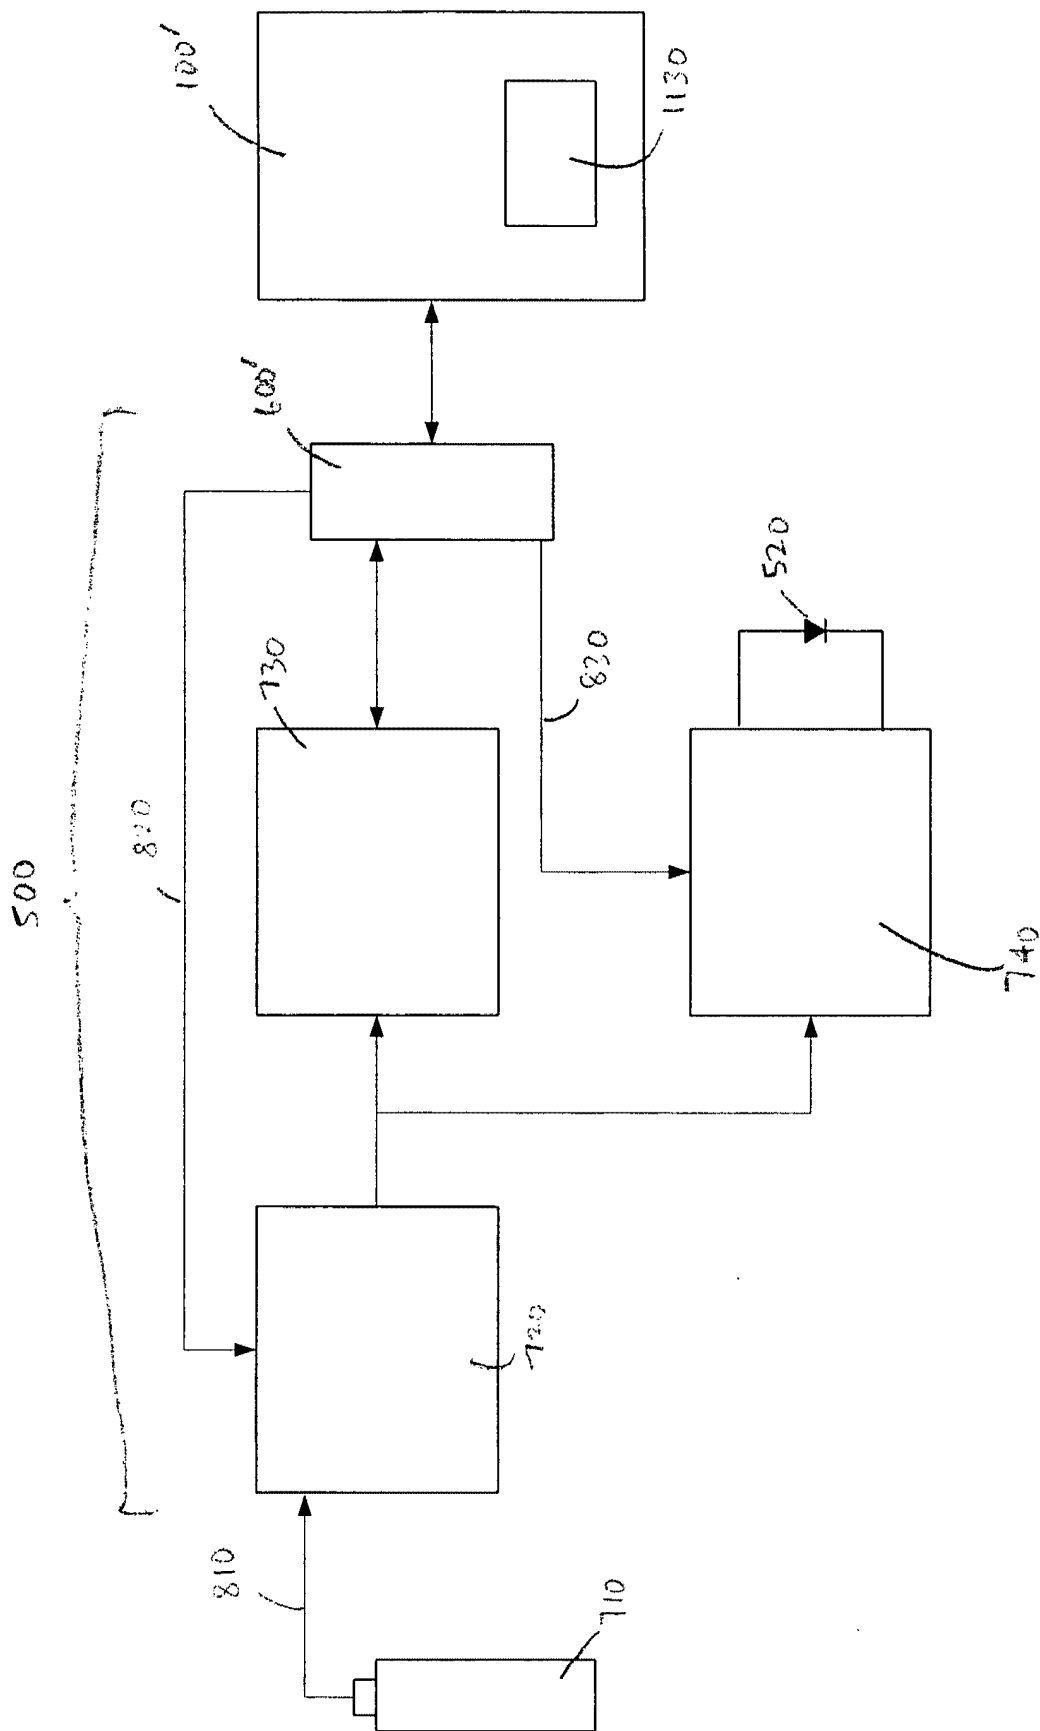


FIGURE 25

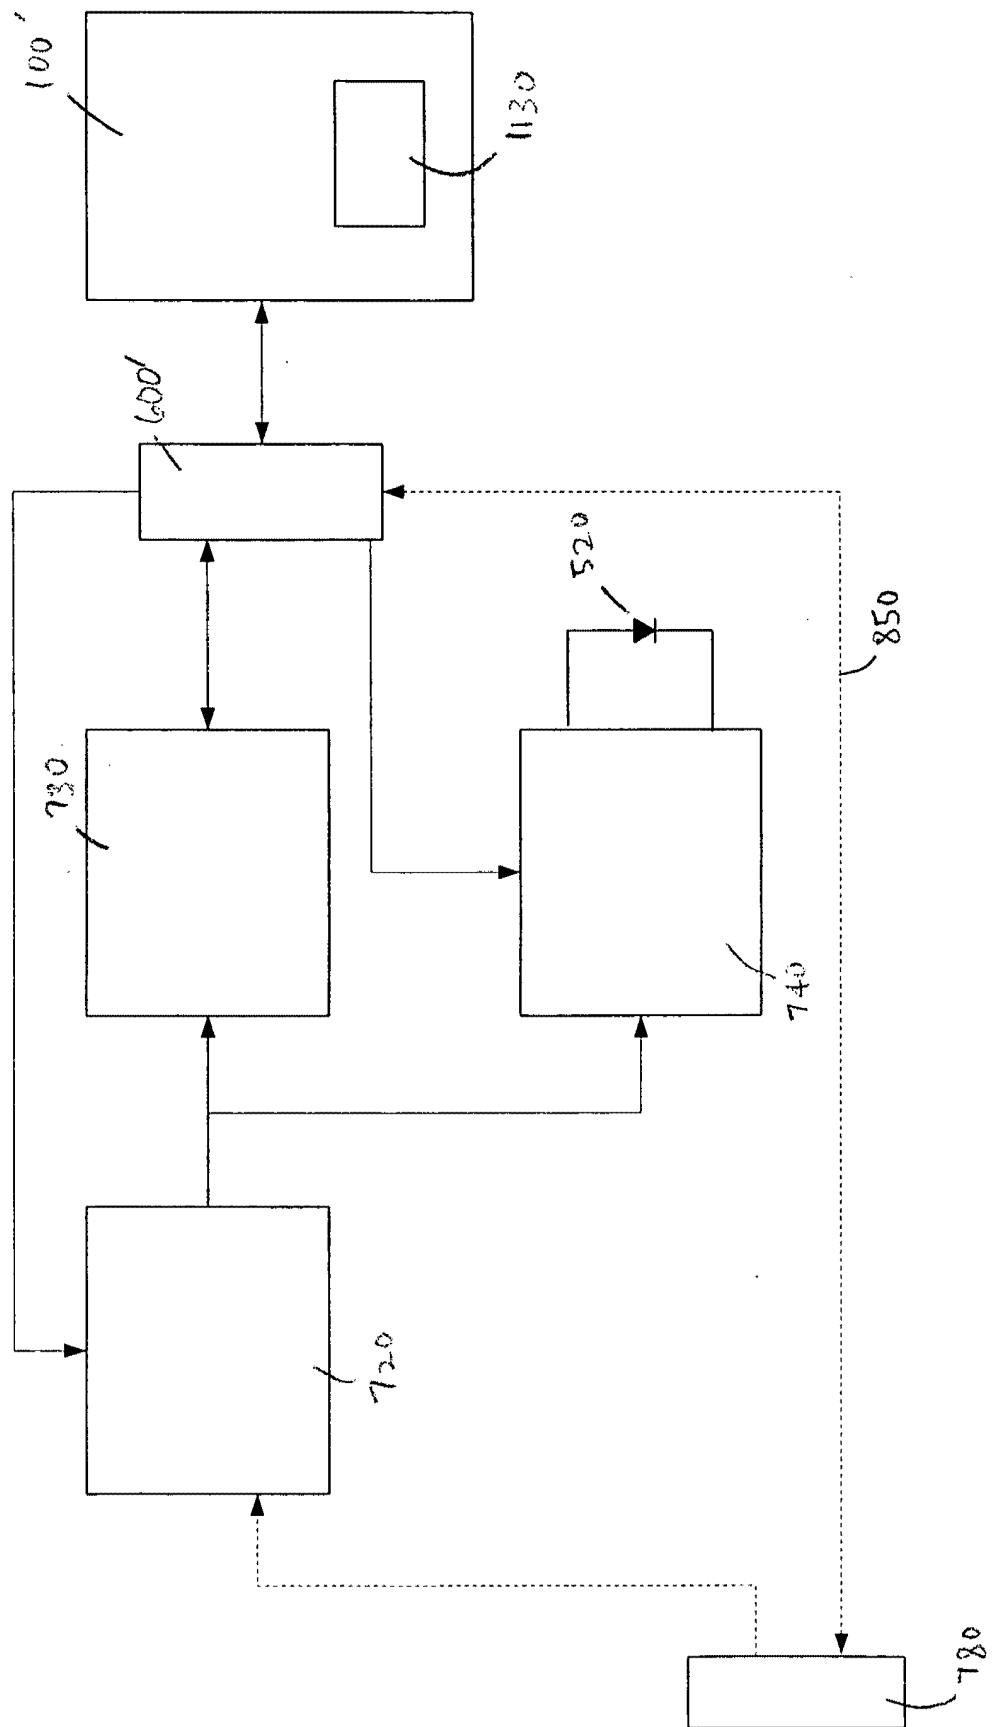

DECLARATION

X ORIGINAL
CONTINUATION-IN-PART
DIVISIONAL

As a below named inventor, I declare that the information given herein is true, that I believe that I am the original, first and sole inventor if only one name is listed at 1 below, or a joint inventor if plural inventors are named below at 1-6, of the invention entitled:

TELEMETERED CHARACTERISTIC MONITOR SYSTEM AND METHOD OF USING THE SAME

Which is described and claimed in:

X the attached specification or
the specification in application Serial No. _____ filed _____
as amended on _____

and for which a patent is sought, and that my residence, post office address and citizenship are as stated below next to my name.

I acknowledge my duty to disclose information, which is material to the examination of this application in accordance with Title 37, Code of Federal Regulations §1.56(a).

I hereby state that I have reviewed and understand the contents of the above-identified specification, including the claims, as amended by any amendment referred to above.

I hereby claim priority benefits under Title 35, United States Code, §119 of any application(s) for patent or inventor's certificate listed below and have also identified below any application for patent or inventor's certificate having a filing date before that of the application on which priority is claimed:

PRIOR
APPLICATION(S)

COUNTRY	APPLICATION NUMBER	DATE OF FILING Month Day Year	PRIORITY CLAIMED UNDER 35 U.S.C. 119
US	60/103,812	October 8, 1998	YES <u>X</u> NO

I hereby claim the benefit under Title 35, United States Code, §120 of any United States application(s) listed below and, insofar as the subject matter of each of the claims of this application is not disclosed in the prior United States application in the manner provided by the first paragraph of Title 35, United States Code §112, I acknowledge the duty to disclose material information as defined in Title 37, Code of Federal Regulations, §1.56(a) which occurred between the filing date of the prior application and the national or PCT international filing date of this application.

10/898,589	July 23, 2004	Pending
10/465,715	December 17, 1999	(Now Issued Patent 6,809,653 Issued 10/24/2004)
09/377,472	October 26, 2005	(Now abandoned)
(Application Serial No.)	(Filing Date)	(Status)

Send correspondence to:
MEDTRONIC MINIMED, INC.
18000 Devonshire Street
Northridge, CA 91325-1219

DIRECT TELEPHONE CALLS TO:
Richard Yoon
(818) 576-4110

1	LAST NAME MASTROTOTARO	FIRST NAME JOHN	MIDDLE NAME J.	Residence: CITY LOS ANGELES	STATE or COUNTRY CALIFORNIA
	Post Office Address 10642 LINDBROOK DRIVE, LOS ANGELES, CA 90024				CITIZENSHIP US
2	LAST NAME CHERNOFF	FIRST NAME EDWARD	MIDDLE NAME	Residence: CITY FRAZIER PARK	STATE or COUNTRY CALIFORNIA
	Post Office Address P.O. BOX 329, FRAZIER PARK, CA 93225				CITIZENSHIP US
3	LAST NAME CHOY	FIRST NAME DAVID	MIDDLE NAME Y.	Residence: CITY SAN GABRIEL	STATE or COUNTRY CALIFORNIA
	Post Office Address 801 MONTECITO DRIVE, SAN GABRIEL, CA 91776				CITIZENSHIP US

4	LAST NAME HENKE	FIRST NAME JAMES	MIDDLE NAME L.	Residence: CITY SIMI VALLEY	STATE or COUNTRY CALIFORNIA
	Post Office Address 5105 E. LOS ANGELES AVENUE, PMB 168, SIMI VALLEY, CA 93063				CITIZENSHIP US
5	LAST NAME PURVIS	FIRST NAME RICHARD	MIDDLE NAME E.	Residence: CITY PASADENA	STATE or COUNTRY CALIFORNIA
	Post Office Address 1478 N. MAR VISTA AVENUE, PASADENA, CA 91104				CITIZENSHIP US
6	LAST NAME HONG	FIRST NAME PETER	MIDDLE NAME I.	Residence: CITY SANTA CLARITA	STATE or COUNTRY CALIFORNIA
	Post Office Address 28030 KENTON LANE, SANTA CLARITA, CA 91350				CITIZENSHIP US

I further declare that all statements made herein of my own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under Section 1001 of Title 18 of the United States Code, and that such willful false statements may jeopardize the validity of the application or any patent issuing thereon.

SIGNATURE OF INVENTOR 1	SIGNATURE OF INVENTOR 2
DATE	DATE
SIGNATURE OF INVENTOR 3	SIGNATURE OF INVENTOR 4
DATE	DATE
SIGNATURE OF INVENTOR 5	SIGNATURE OF INVENTOR 6
DATE	DATE

PATENT APPLICATION SERIAL NO _____

U.S. DEPARTMENT OF COMMERCE
PATENT AND TRADEMARK OFFICE
FEE RECORD SHEET

01/05/2006 KBETEMAI 00000022 500621 11322568

01 FC:1011	300.00 DA
02 FC:1111	500.00 DA
03 FC:1311	200.00 DA

PTO-1556

(5/87)

Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

PATENT APPLICATION FEE DETERMINATION RECORD

Substitute for Form PTO-875 Effective December 8, 2004

Application or Docket Number

113 22568

APPLICATION AS FILED - PART I

(Column 1)

(Column 2)

SMALL ENTITY

OR

OTHER THAN
SMALL ENTITY

FOR	NUMBER FILED	NUMBER EXTRA
BASIC FEE (37 CFR 1.16(a), (b), or (c))	N/A	N/A
SEARCH FEE (37 CFR 1.16(k), (l), or (m))	N/A	N/A
EXAMINATION FEE (37 CFR 1.16(o), (p), or (q))	N/A	N/A
TOTAL CLAIMS (37 CFR 1.16(j))	18 minus 20 =	0
INDEPENDENT CLAIMS (37 CFR 1.16(h))	1 minus 3 =	0
APPLICATION SIZE FEE (37 CFR 1.16(s))	If the specification and drawings exceed 100 sheets of paper, the application size fee due is \$250 (\$125 for small entity) for each additional 50 sheets or fraction thereof. See 35 U.S.C. 41(a)(1)(G) and 37 CFR 1.16(s).	
MULTIPLE DEPENDENT CLAIM PRESENT (37 CFR 1.16(j))		

RATE (\$)	FEE (\$)
N/A	150.00
N/A	\$250
N/A	\$100
X\$ 25 =	
X100 =	
+180=	
TOTAL	

RATE (\$)	FEE (\$)
N/A	300.00
N/A	\$500
N/A	\$200
X\$50 =	
X200 =	
+360=	
TOTAL	1050

* If the difference in column 1 is less than zero, enter "0" in column 2.

APPLICATION AS AMENDED - PART II

(Column 1)

(Column 2)

(Column 3)

SMALL ENTITY

OR

OTHER THAN
SMALL ENTITY

AMENDMENT A	CLAIMS REMAINING AFTER AMENDMENT	HIGHEST NUMBER PREVIOUSLY PAID FOR	PRESENT EXTRA
Total (37 CFR 1.16(j))	0	20	=
Independent (37 CFR 1.16(h))	0	3	=
Application Size Fee (37 CFR 1.16(s))			
FIRST PRESENTATION OF MULTIPLE DEPENDENT CLAIM (37 CFR 1.16(j))			

RATE (\$)	ADDITIONAL FEE (\$)
X\$ 25 =	
X100 =	
+180=	
TOTAL ADD'L FEE	

RATE (\$)	ADDITIONAL FEE (\$)
X\$50 =	
X200 =	
+360=	
TOTAL ADD'L FEE	

(Column 1)

(Column 2)

(Column 3)

AMENDMENT B	CLAIMS REMAINING AFTER AMENDMENT	HIGHEST NUMBER PREVIOUSLY PAID FOR	PRESENT EXTRA
Total (37 CFR 1.16(j))	0	20	=
Independent (37 CFR 1.16(h))	0	3	=
Application Size Fee (37 CFR 1.16(s))			
FIRST PRESENTATION OF MULTIPLE DEPENDENT CLAIM (37 CFR 1.16(j))			

RATE (\$)	ADDITIONAL FEE (\$)
X\$ 25 =	
X100 =	
+180=	
TOTAL ADD'L FEE	

RATE (\$)	ADDITIONAL FEE (\$)
X\$50 =	
X200 =	
+360=	
TOTAL ADD'L FEE	

* If the entry in column 1 is less than the entry in column 2, write "0" in column 3.

** If the "Highest Number Previously Paid For" IN THIS SPACE is less than 20, enter "20".

*** If the "Highest Number Previously Paid For" IN THIS SPACE is less than 3, enter "3".

The "Highest Number Previously Paid For" (Total or Independent) is the highest number found in the appropriate box in column 1.

This collection of information is required by 37 CFR 1.16. The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.14. This collection is estimated to take 12 minutes to complete, including gathering, preparing, and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. SEND TO: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.