



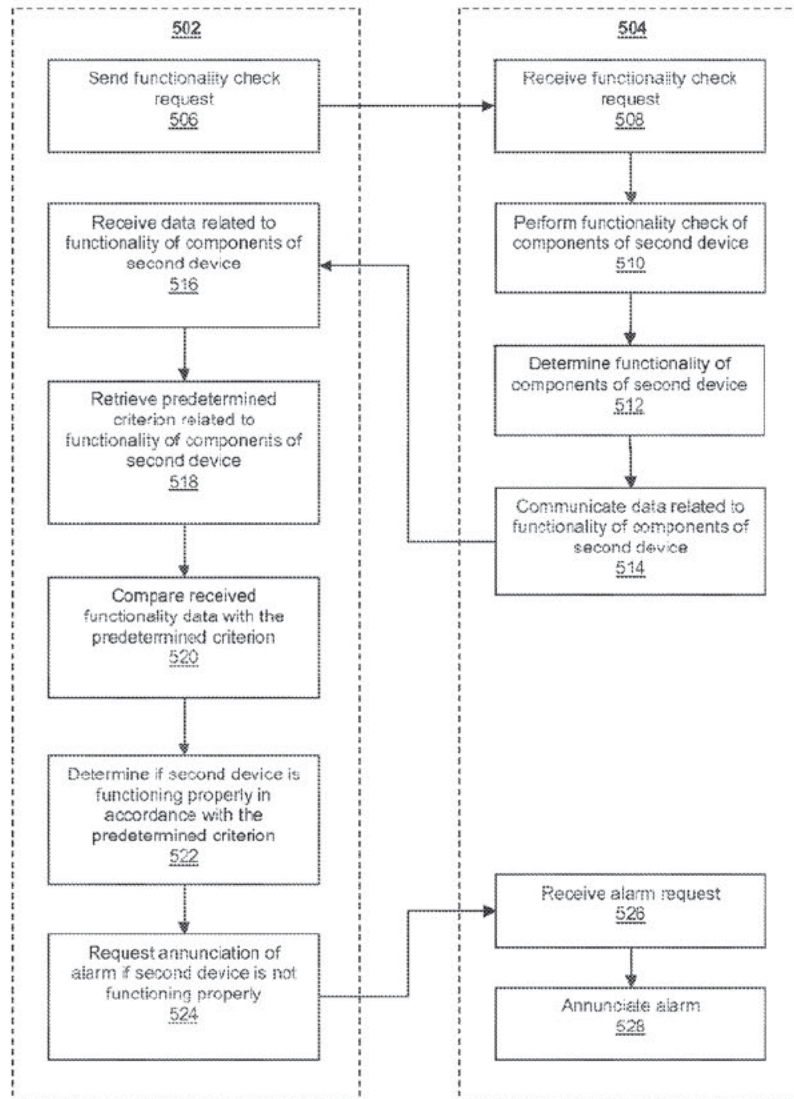


US 20130127627A1

(19) **United States**(12) **Patent Application Publication**
Hayter et al.(10) **Pub. No.: US 2013/0127627 A1**(43) **Pub. Date: May 23, 2013**(54) **MITIGATING SINGLE POINT FAILURE OF
DEVICES IN AN ANALYTE MONITORING
SYSTEM AND METHODS THEREOF**(71) Applicant: **Abbott Diabetes Care Inc.**, Alameda,
CA (US)(72) Inventors: **Gary Alan Hayter**, Oakland, CA (US);
Marc Barry Taub, Mountain View, CA
(US)(73) Assignee: **Abbott Diabetes Care Inc.**, Alameda,
CA (US)(21) Appl. No.: **13/684,078**(22) Filed: **Nov. 21, 2012****Related U.S. Application Data**(60) Provisional application No. 61/563,518, filed on Nov.
23, 2011.**Publication Classification**(51) **Int. Cl.**
G08B 21/18 (2006.01)(52) **U.S. Cl.**
USPC **340/657**(57) **ABSTRACT**Methods, devices, and kits are provided for mitigating single
point failure of at least one device in an analyte monitoring
system.

500

DEXCOM
EXHIBIT 1210

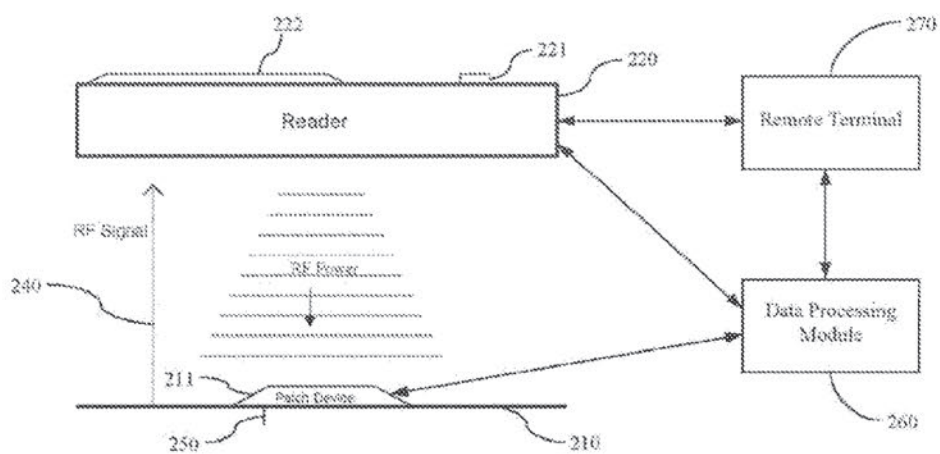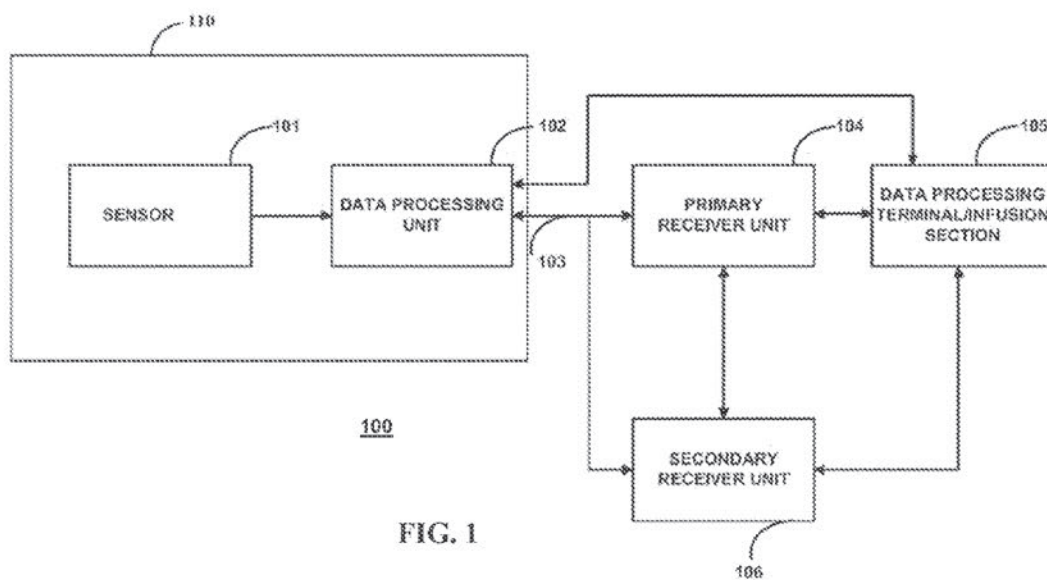

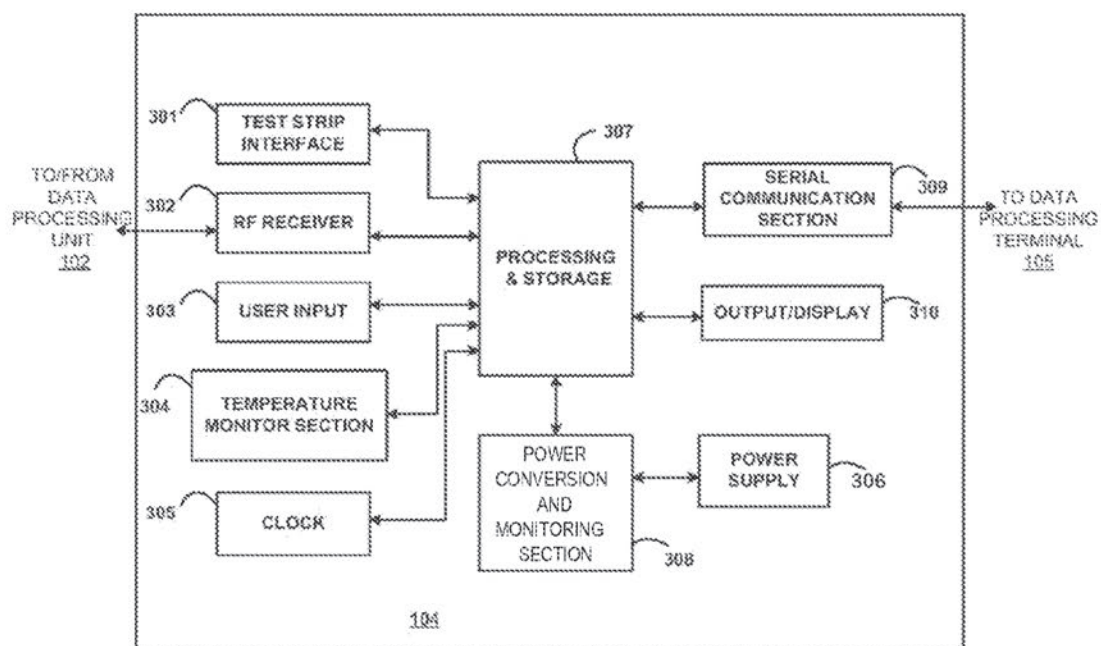


FIG. 3


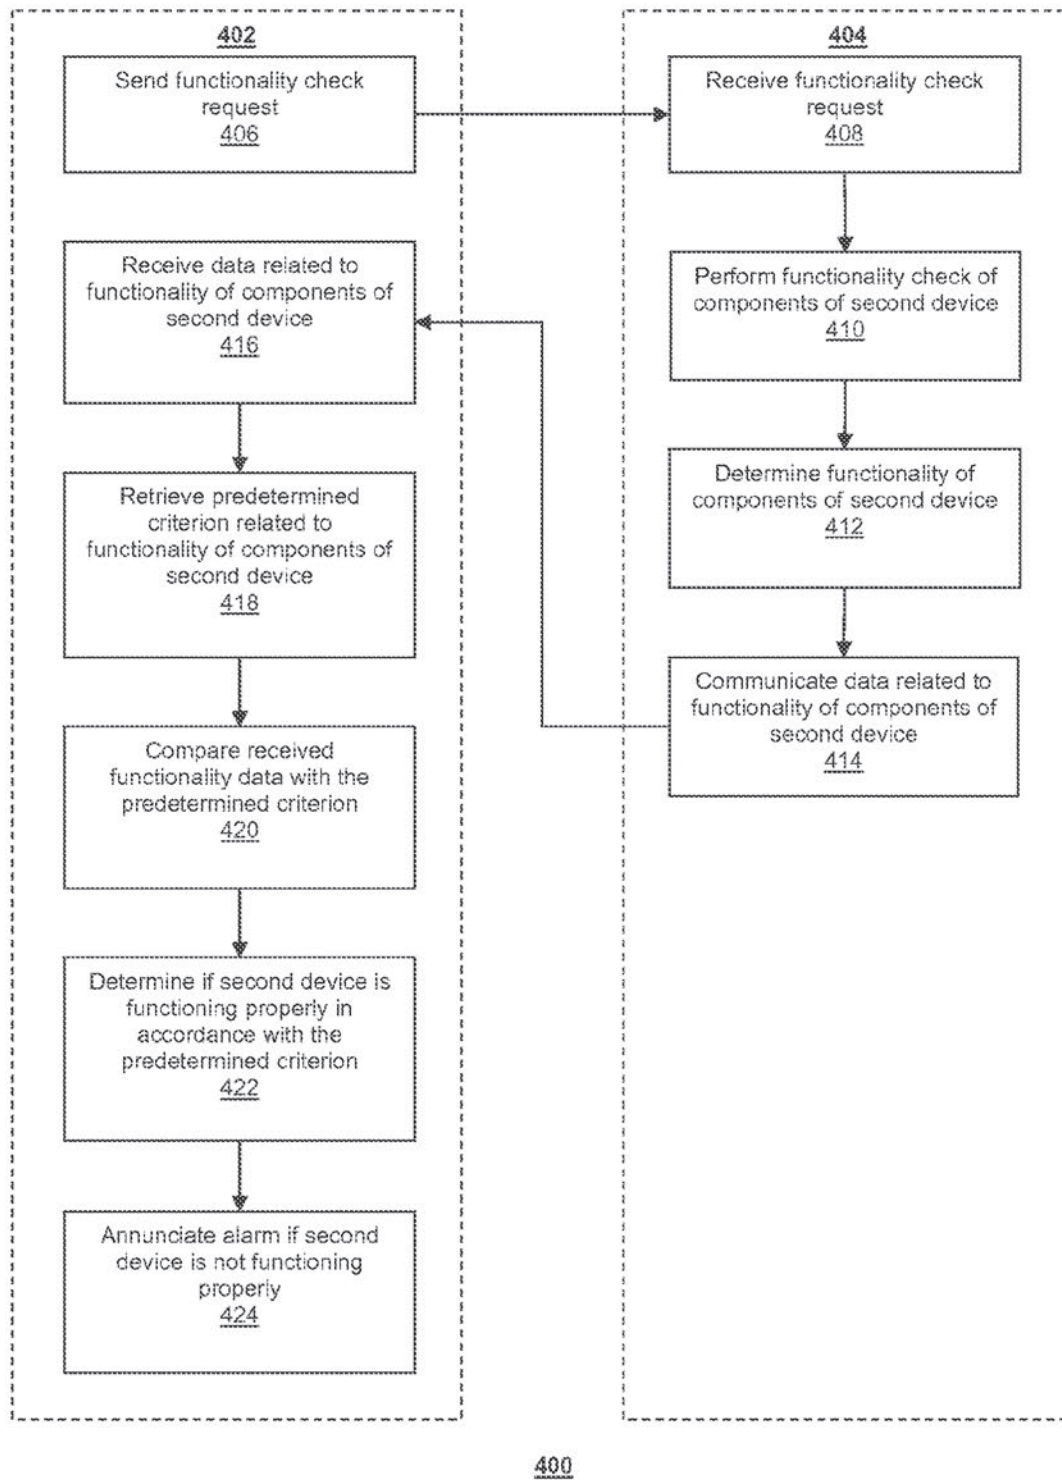


FIG. 4

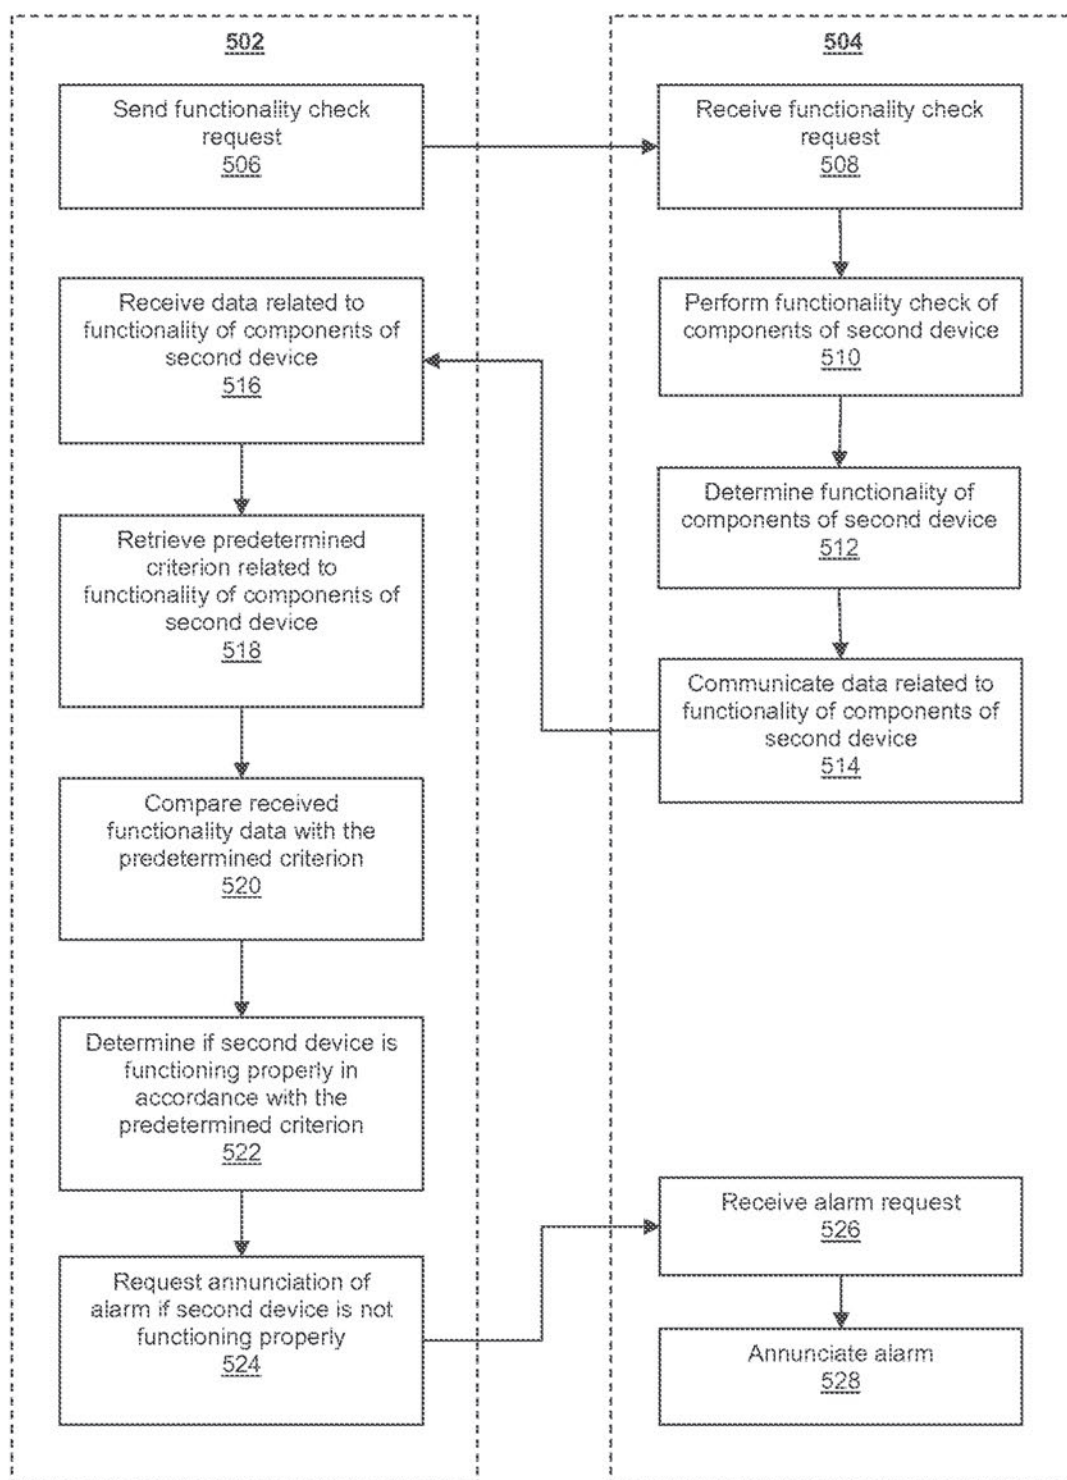

500

FIG. 5

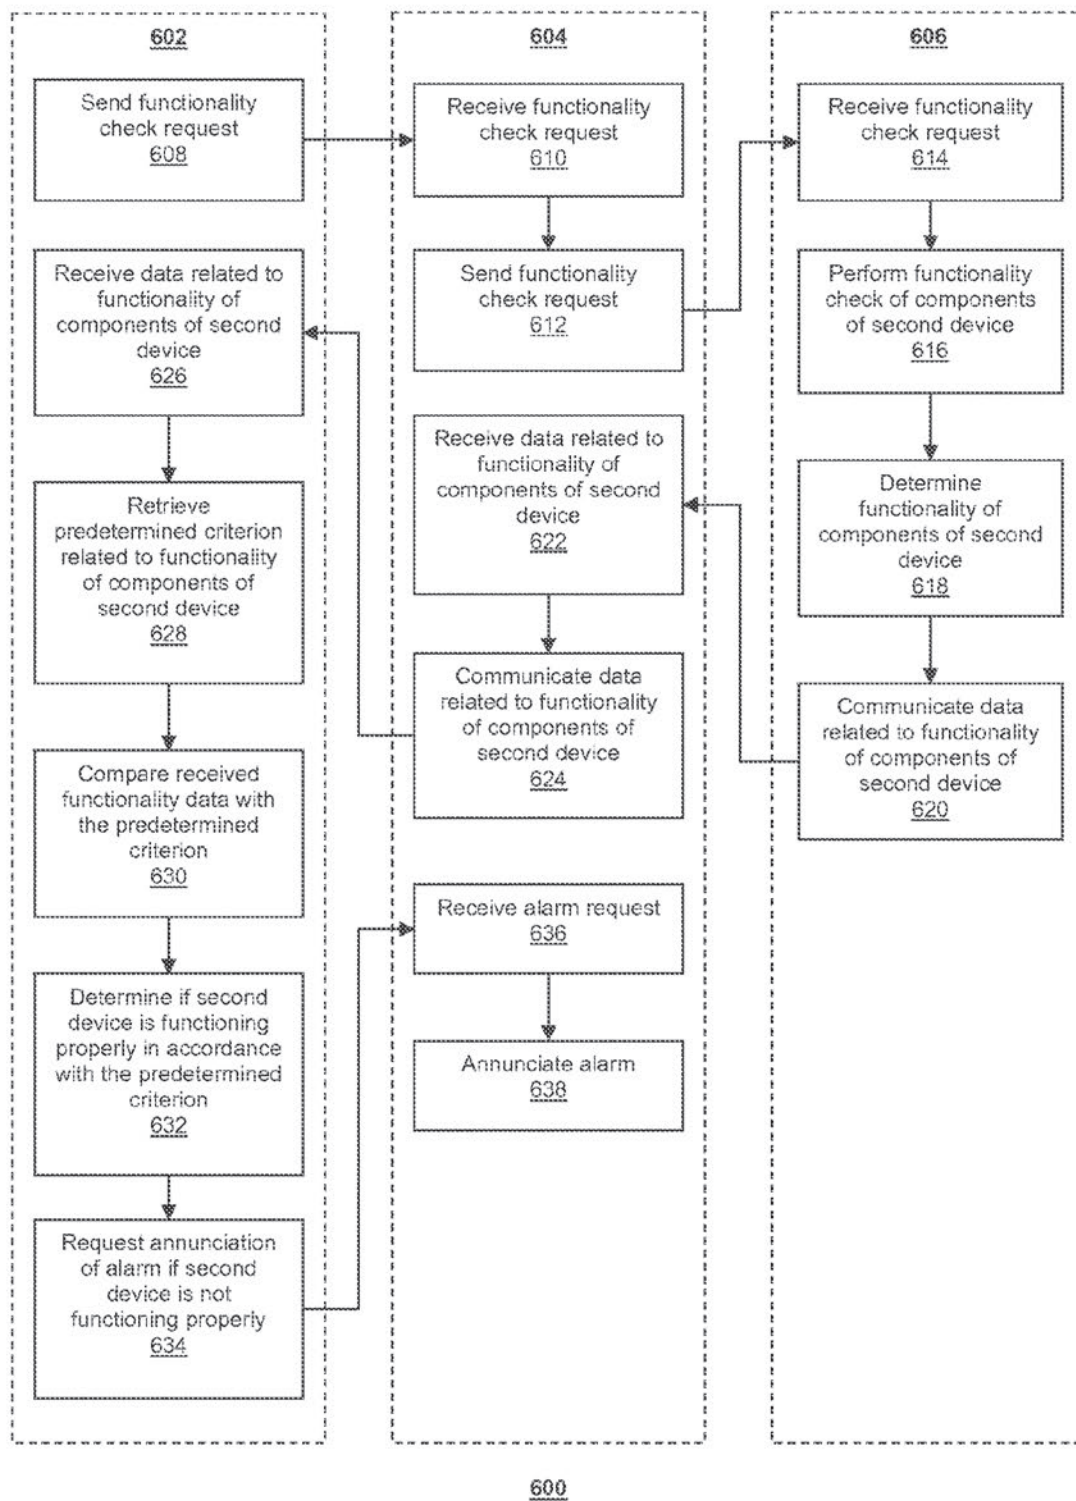


FIG. 6

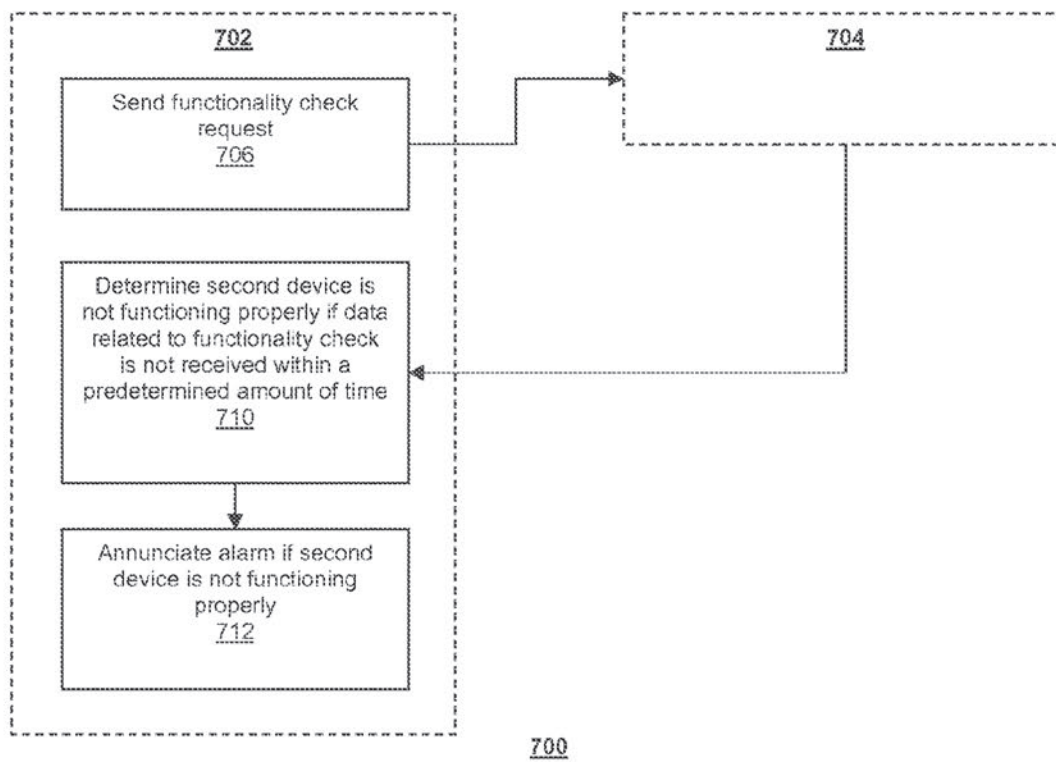


FIG. 7

MITIGATING SINGLE POINT FAILURE OF DEVICES IN AN ANALYTE MONITORING SYSTEM AND METHODS THEREOF

RELATED APPLICATION

[0001] This application claims priority to U.S. provisional application no. 61/563,518, filed Nov. 23, 2011, entitled "Mitigating Single Point Failure of Devices in an Analyte Monitoring System and Methods Thereof", the disclosure of which is incorporated herein by reference in its entirety for all purposes.

BACKGROUND

[0002] The detection of the level of glucose or other analytes, such as lactate, oxygen or the like, in certain individuals is vitally important to their health. For example, the monitoring of glucose is particularly important to individuals with diabetes. Diabetics may need to monitor glucose levels to determine when insulin is needed to reduce glucose levels in their bodies or when additional glucose is needed to raise the level of glucose in their bodies.

[0003] Devices have been developed for continuous or automatic monitoring of analytes, such as glucose, in bodily fluid such as in the blood stream or in interstitial fluid. Some of these analyte measuring devices are configured so that at least a portion of the devices are positioned below a skin surface of a user, e.g., in a blood vessel or in the subcutaneous tissue of a user.

SUMMARY

[0004] Embodiments of the present disclosure include methods for mitigating single point failure of at least one device in an analyte monitoring system. Certain aspects include requesting that a functionality check of one or more components of a first device be performed and that data related to the functionality check of the one or more components of the first device be communicated to a second device, receiving information from the first device that is related to functionality of the one or more components of the first device, communicating the information related to the functionality of the one or more components of the first device to a third device, receiving a request from the third device that an alarm be annunciated if it is determined by the third device that the one or more components of the first device is not functioning in accordance with at least one predetermined criterion and annunciating an alarm to alert a user that the one or more components of the first device is not functioning in accordance with the at least one predetermined criterion.

[0005] Embodiments of the present disclosure include computer-implemented methods for mitigating single point failure of at least one device in an analyte monitoring. Certain aspects include requesting that a functionality check of one or more components of a first device be performed and that data related to the functionality check of the one or more components of the first device be communicated to a second device, receiving the data related to the functionality of the one or more components of the first device, retrieving a list including at least one predetermined criterion related to the functionality of the one or more components of the first device from a storage component of the second device, comparing the data related to the functionality of the one or more components of the first device with the list including the at least one predetermined criterion and determining if the one or more com-

ponents of the first device is functioning in accordance with the at least one predetermined criterion.

[0006] Embodiments of the present disclosure include computer-implemented methods for mitigating single point failure of at least one device in an analyte monitoring. Certain aspects include requesting that a functionality check of one or more components of a first device be performed and that data related to the functionality check of the one or more components of the first device be communicated to a second device and determining that the one or more components of the first device is not functioning properly if the data related to the functionality check of the components of the first device is not received at the second device, wherein an alarm is annunciated from at least one of the second device or a third device to alert a user that one or more components of the first device is not functioning properly.

BRIEF DESCRIPTION OF THE DRAWINGS

[0007] FIG. 1 shows a data monitoring and management system such as, for example, an analyte (e.g., glucose) monitoring system in accordance with certain embodiments of the present disclosure;

[0008] FIG. 2 illustrates a data monitoring and management system for real time glucose measurement data acquisition and processing in one aspect of the present disclosure;

[0009] FIG. 3 is a block diagram of a receiver/monitor unit such as that shown in FIG. 1 in accordance with certain embodiments;

[0010] FIG. 4 is a flowchart illustrating a method for mitigating single point failure of at least one device in an analyte monitoring system in accordance with certain embodiments of the present disclosure;

[0011] FIG. 5 is a flowchart illustrating a method for mitigating single point failure of at least one device in an analyte monitoring system in accordance with certain embodiments of the present disclosure;

[0012] FIG. 6 is a flowchart illustrating a method for mitigating single point failure of at least one device in an analyte monitoring system in accordance with certain embodiments of the present disclosure; and

[0013] FIG. 7 is a flowchart illustrating a method for mitigating single point failure of at least one device in an analyte monitoring system in accordance with certain embodiments of the present disclosure.

DETAILED DESCRIPTION

[0014] Before the present disclosure is further described, it is to be understood that this disclosure is not limited to particular embodiments described, as such may, of course, vary. It is also to be understood that the terminology used herein is for the purpose of describing particular embodiments only, and is not intended to be limiting, since the scope of the present disclosure will be limited only by the appended claims.

[0015] As will be apparent to those of skill in the art upon reading this disclosure, each of the individual embodiments described and illustrated herein has discrete components and features which may be readily separated from or combined with the features of any of the other several embodiments without departing from the scope or spirit of the present disclosure.

[0016] Where a range of values is provided, it is understood that each intervening value, to the tenth of the unit of the lower

limit unless the context clearly dictates otherwise, between the upper and lower limit of that range and any other stated or intervening value in that stated range, is encompassed within the disclosure. The upper and lower limits of these smaller ranges may independently be included in the smaller ranges, and are also encompassed within the disclosure, subject to any specifically excluded limit in the stated range. Where the stated range includes one or both of the limits, ranges excluding either or both of those included limits are also included in the disclosure.

[0017] Unless defined otherwise, all technical and scientific terms used herein have the same meaning as commonly understood by one of ordinary skill in the art to which this disclosure belongs. Although any methods and materials similar or equivalent to those described herein can also be used in the practice or testing of the present disclosure, exemplary methods and materials are now described. All publications mentioned herein are incorporated herein by reference to disclose and describe the methods and/or materials in connection with which the publications are cited.

[0018] As used herein and in the appended claims, the singular forms “a,” “an,” and “the” include plural referents unless the context clearly dictates otherwise. It is further noted that the claims may be drafted to exclude any optional element. As such, this statement is intended to serve as antecedent basis for use of such exclusive terminology as “solely,” “only” and the like in connection with the recitation of claim elements, or use of a “negative” limitation.

[0019] The publications discussed herein are provided solely for their disclosure prior to the filing date of the present application. Nothing herein is to be construed as an admission that the present disclosure is not entitled to antedate such publication by virtue of prior disclosure. Further, the dates of publication provided may be different from the actual publication dates which may need to be independently confirmed.

[0020] FIG. 1 shows a data monitoring and management system such as, for example, an analyte (e.g., glucose) monitoring system in accordance with certain embodiments of the present disclosure. Embodiments of the subject disclosure are described primarily with respect to glucose monitoring devices and systems, and methods of using two or more devices in a glucose monitoring system to reduce the likelihood of a failure of one or more of the devices in the glucose monitoring system going unnoticed by a user.

[0021] Analytes that may be monitored include, but are not limited to, acetyl choline, amylase, bilirubin, cholesterol, chorionic gonadotropin, creatine kinase (e.g., CK-MB), creatine, DNA, fructosamine, glucose, glutamine, growth hormones, hormones, ketones, lactate, peroxide, prostate-specific antigen, prothrombin, RNA, thyroid stimulating hormone, and troponin. The concentration of drugs, such as, for example, antibiotics (e.g., gentamicin, vancomycin, and the like), digitoxin, digoxin, drugs of abuse, theophylline, and warfarin, may also be monitored. In those embodiments that monitor more than one analyte, the analytes may be monitored at the same or different times.

[0022] Referring to FIG. 1, the analyte monitoring system 100 includes a sensor 101, a data processing unit (e.g., sensor electronics) 102 connectable to the sensor 101, and a primary receiver unit 104 which is configured to communicate with the data processing unit 102 via a communication link 103. In aspects of the present disclosure, the sensor 101 and the data processing unit (sensor electronics) 102 may be configured as a single integrated assembly 110. In certain embodiments, the

integrated sensor and sensor electronics assembly 110 may be configured as an on-body patch device. In such embodiments, the on-body patch device may be configured for, for example, RFID or RF communication with a reader device/receiver unit, and/or an insulin pump.

[0023] In certain embodiments, the primary receiver unit 104 may be further configured to transmit data to a data processing terminal 105 to evaluate or otherwise process or format data received by the primary receiver unit 104. The data processing terminal 105 may be configured to receive data directly from the data processing unit 102 via a communication link which may optionally be configured for bi-directional communication. Further, the data processing unit 102 may include a transmitter or a transceiver to transmit and/or receive data to and/or from the primary receiver unit 104, the data processing terminal 105 or optionally the secondary receiver unit 106.

[0024] Also shown in FIG. 1 is an optional secondary receiver unit 106 which is operatively coupled to the communication link and configured to receive data transmitted from the data processing unit 102. The secondary receiver unit 106 may be configured to communicate with the primary receiver unit 104, as well as the data processing terminal 105. The secondary receiver unit 106 may be configured for bi-directional wireless communication with each of the primary receiver unit 104 and the data processing terminal 105. As discussed in further detail below, in certain embodiments the secondary receiver unit 106 may be a de-featured receiver as compared to the primary receiver unit 104, i.e., the secondary receiver unit 106 may include a limited or minimal number of functions and features as compared with the primary receiver unit 104. As such, the secondary receiver unit 106 may include a smaller (in one or more, including all, dimensions), compact housing or embodied in a device such as a wrist watch, arm band, etc., for example. Alternatively, the secondary receiver unit 106 may be configured with the same or substantially similar functions and features as the primary receiver unit 104. The secondary receiver unit 106 may include a docking portion to be mated with a docking cradle unit for placement by, e.g., the bedside for night time monitoring, and/or bi-directional communication device.

[0025] Only one sensor 101, data processing unit 102 and data processing terminal 105 are shown in the embodiment of the analyte monitoring system 100 illustrated in FIG. 1. However, it will be appreciated by one of ordinary skill in the art that the analyte monitoring system 100 may include more than one sensor 101 and/or more than one data processing unit 102, and/or more than one data processing terminal 105.

[0026] The analyte monitoring system 100 may be a continuous monitoring system, or semi-continuous, or a discrete monitoring system. In a multi-component environment, each component may be configured to be uniquely identified by one or more of the other components in the system so that communication conflict may be readily resolved between the various components within the analyte monitoring system 100. For example, unique IDs, communication channels, and the like, may be used.

[0027] In certain embodiments, the sensor 101 is physically positioned in or on the body of a user whose analyte level is being monitored. The sensor 101 may be configured to at least periodically perform a functionality check and convert the results of the functionality check into a corresponding signal for transmission by the data processing unit 102.

[0028] The data processing unit 102 is coupleable to the sensor 101 so that both devices are positioned in or on the user's body, with at least a portion of the analyte sensor 101 positioned transcutaneously. The data processing unit 102 in certain embodiments may include a portion of the sensor 101 (proximal section of the sensor in electrical communication with the data processing unit 102) which is encapsulated within or on the printed circuit board of the data processing unit 102 with, for example, potting material or other protective material. The data processing unit 102 performs data processing functions, where such functions may include but are not limited to, filtering and encoding of data signals, each of which corresponds to a sampled analyte level of the user, for transmission to the primary receiver unit 104 via the communication link 103. In one embodiment, the sensor 101 or the data processing unit 102 or a combined sensor/data processing unit may be wholly implantable under the skin layer of the user.

[0029] In one aspect, the primary receiver unit 104 may include an analog interface section including an RF receiver and an antenna that is configured to communicate with the data processing unit 102 via the communication link 103, and a data processing section for processing the received data from the data processing unit 102 such as data decoding, error detection and correction, data clock generation, and/or data bit recovery.

[0030] In operation, the primary receiver unit 104 in certain embodiments is configured to synchronize with the data processing unit 102 to uniquely identify the data processing unit 102, based on, for example, an identification information of the data processing unit 102, and thereafter, to periodically receive signals transmitted from the data processing unit 102 associated with the monitored analyte levels detected by the sensor 101. That is, when operating in the CGM mode, the receiver unit 104 in certain embodiments is configured to automatically receive data related to the functionality of the sensor from the analyte sensor/sensor electronics when the communication link (e.g., RF range) is maintained between these components.

[0031] Referring again to FIG. 1, the data processing terminal 105 may include a personal computer, a portable data processing devices or computers such as a laptop computer or a handheld device (e.g., personal digital assistants (PDAs), communication devices such as a cellular phone (e.g., a multimedia and Internet-enabled mobile phone such as an iPhone, a Blackberry device, a Palm device such as Palm Pre, Treo, or similar phone), mp3 player, pager, and the like), drug delivery device, insulin pump, each of which may be configured for data communication with the receiver via a wired or a wireless connection. Additionally, the data processing terminal 105 may further be connected to a data network (not shown).

[0032] The data processing terminal 105 may include an infusion device such as an insulin infusion pump or the like, which may be configured to administer insulin to patients, and which may be configured to communicate with the primary receiver unit 104 for receiving, among others, the measured analyte level. Alternatively, the primary receiver unit 104 may be configured to integrate an infusion device therein so that the primary receiver unit 104 is configured to administer insulin (or other appropriate drug) therapy to patients, for example, for administering and modifying basal profiles, as well as for determining appropriate boluses for administration based on, among others, the detected analyte levels

received from the data processing unit 102. An infusion device may be an external device or an internal device (wholly implantable in a user).

[0033] In particular embodiments, the data processing terminal 105, which may include an insulin pump, may be configured to receive the functionality signals from the data processing unit 102, and thus, incorporate the functions of the primary receiver unit 104 including data processing for managing the patient's insulin therapy and analyte monitoring. In certain embodiments, the communication link 103 as well as one or more of the other communication interfaces shown in FIG. 1 may use one or more of an RF communication protocol, an infrared communication protocol, a Bluetooth enabled communication protocol, an 802.11x wireless communication protocol, or an equivalent wireless communication protocol which would allow secure, wireless communication of several units (for example, per HIPPA requirements) while avoiding potential data collision and interference.

[0034] As described in aspects of the present disclosure, the analyte monitoring system may include an on-body patch device with a thin profile that can be worn on the arm or other locations on the body (and under clothing worn by the user or the patient), the on-body patch device including an analyte sensor and circuitry and components for operating the sensor and processing and storing signals, including functionality signals, received from the sensor as well as for communication with the reader device. For example, one aspect of the on-body patch device may include electronics to sample the voltage signal received from the analyte sensor in fluid contact with the body fluid, and to process the sampled voltage signals into the corresponding glucose values and/or store the sampled voltage signal as raw data, or to perform a functionality check of its components, and to process the results of the functionality check into a signal or data.

[0035] In certain embodiments, the on-body patch device includes an antenna such as a loop antenna to receive RF power from an external device such as the reader device/receiver unit described above, electronics to convert the RF power received via the antenna into DC (direct current) power for the on-body patch device circuitry, communication module or electronics to detect commands received from the reader device, and communication component to transmit data to the reader device, a low capacity battery for providing power to sensor sampling circuitry (for example, the analog front end circuitry of the on-body patch device in signal communication with the analyte sensor), one or more non-volatile memory or storage device to store data including raw signals from the sensor or processed data based on the raw sensor signals. More specifically, in the on operation demand mode, the on-body patch device in certain embodiments is configured to transmit real time analyte related data and/or stored historical analyte related data, and/or functionality data when within the RF power range of the reader device. As such, when the reader device is removed or positioned out of range relative to the on-body patch device, the on-body patch device may no longer transmit the analyte related data and/or functionality data.

[0036] In certain embodiments, a data processing module/terminal may be provided in the analyte monitoring system that is configured to operate as a data logger, interacting or communicating with the on-body patch device by, for example, transmitting requests for functionality information to the on-body patch device, and storing the responsive functionality information received from the on-body patch device

in one or more memory components of the data processing module (e.g., repeater unit). Further, data processing module may be configured as a compact on-body relay device to relay or retransmit the received analyte level information from the on-body patch device to the reader device/receiver unit or the remote terminal or both. The data processing module in one aspect may be physically coupled to the on-body patch device, for example, on a single adhesive patch on the skin surface of the patient. Alternatively, the data processing module may be positioned close to but not in contact with the on-body patch device. For example, when the on-body patch device is positioned on the abdomen of the patient, the data processing module may be worn on a belt of the patient or the user, such that the desired close proximity or predetermined distance of approximately 1-5 inches (or about 1-10 inches, for example, or more) between the on-body patch device and the data processing module may be maintained.

[0037] The various processes described above including the processes operating in the software application execution environment in the analyte monitoring system including the on-body patch device, the reader device, data processing module and/or the remote terminal performing one or more routines described above may be embodied as computer programs developed using an object oriented language that allows the modeling of complex systems with modular objects to create abstractions that are representative of real world, physical objects and their interrelationships. The software required to carry out the inventive process, which may be stored in a memory or storage device of the storage unit of the various components of the analyte monitoring system described above in conjunction to the Figures including the on-body patch device, the reader device, the data processing module, various described communication devices, or the remote terminal may be developed by a person of ordinary skill in the art and may include one or more computer program products.

[0038] In one embodiment, an apparatus for bi-directional communication with an analyte monitoring system may comprise a storage device having stored therein one or more routines, a processing unit operatively coupled to the storage device and configured to retrieve the stored one or more routines for execution, a data transmission component operatively coupled to the processing unit and configured to transmit data based at least in part on the one or more routines executed by the processing unit, and a data reception component operatively coupled to the processing unit and configured to receive functionality related data from a remote location and to store the received functionality related data in the storage device for retransmission, wherein the data transmission component is programmed to transmit a query to a remote location, and further wherein the data reception component receives the functionality related data from the remote location in response to the transmitted query when one or more electronics in the remote location transitions from an inactive state to an active state upon detection of the query from the data transmission component.

[0039] FIG. 2 illustrates a data monitoring and management system for functionality related data acquisition and processing in one aspect of the present disclosure. More specifically, as shown in FIG. 2, the on-body patch device 211 including sensor electronics coupled to an analyte sensor 250 is positioned on a skin surface 210 of a patient or a user.

[0040] Referring back to FIG. 2, as shown, when the reader device/receiver unit 220 is positioned or placed in close prox-

imity and within a predetermined range of the on-body patch device 211, the RF power supply in the reader device/receiver unit 220 may be configured to provide the necessary power to operate the electronics in the on-body patch device 211, and the on-body patch device 211 may be configured to, upon detection of the RF power from the reader device/receiver unit 220, perform preprogrammed routines including, for example, transmitting one or more signals 240 to the reader device/receiver unit 220 indicative of the functionality of the components of the analyte sensor 250, or performing functionality check of one or more components of the analyte sensor 250.

[0041] In certain embodiments, the reader device/receiver unit 220 may include an RF power switch that is user activatable or activated upon positioning within a predetermined distance from the on-body patch device 211 to turn on the analyte sensor in the on-body patch device 211. That is, using the RF signal, the analyte sensor coupled to the sensor electronics in the on-body patch device 211 may be initialized or activated. In another embodiment, a passive RFID function may be provided or programmed such that upon receiving a "turn on" signal which, when authenticated, will turn on the electronic power switch that activates the on-body patch device 211. That is, the passive RFID configuration may include drawing energy from the RF field radiated from the reader device/receiver unit 220 so as to prompt for and/or detect the "turn on" signal which, upon authentication, activates the on-body patch device 211.

[0042] In one embodiment, communication and/or RF power transfer between the reader device/receiver unit 220 and the on-body patch device 211 may be automatically initiated when the reader device/receiver unit 220 is placed in close proximity to the on-body patch device 211 as discussed above. Alternatively, the reader device/receiver unit 220 may be configured such that user activation, such as data request initiation and subsequent confirmation by the user using, for example, the display 222 and/or input components 221 of the reader device/receiver unit 220, may be required prior to the initiation of communication and/or RF power transfer between the reader device/receiver unit 220 and the on-body patch device 211. In a further embodiment, the reader device/receiver unit 220 may be user configurable between multiple modes, such that the user may choose whether the communication between the reader device/receiver unit 220 and on-body patch device 211 is performed automatically or requires a user activation and/or confirmation.

[0043] As further shown in FIG. 2, the display 222 of the reader device/receiver unit 220 may be configured to provide the functionalities of a user interface to present information such as alarm or alert notification to the user. In one aspect, the reader device/receiver unit 220 may include other output components such as a speaker, vibratory output component and the like to provide audible and/or vibratory output indication to the user in addition to the visual output indication provided on the display 222.

[0044] As discussed, some or all of the electronics in the on-body patch device 211 in one embodiment may be configured to rely on the RF power received from the reader device/receiver unit 220 to perform functionality data processing and/or transmission of the processed functionality information to the reader device/receiver unit 220. That is, the on-body patch device 211 may be discreetly worn on the body of the user or the patient, and under clothing, for example, and when desired, by positioning the reader device/receiver unit

220 within a predetermined distance from the on-body patch device 211, functionality information may be received by the reader device/receiver unit 220.

[0045] Referring still to FIG. 2, also shown are a data processing module/terminal 260 and a remote terminal 270. In one aspect, data processing module 260 may include a stand alone device configured for bi-directional communication to communicate with the on-body patch device 211, the reader device/receiver unit 220 and/or the remote terminal 270. More specifically, data processing module 260 may include one or more microprocessors or similar data processing components configured to execute one or more software routines for communication, as well as data storage and retrieval to and from one or more memory components provided in the housing of the data processing module 260.

[0046] The data processing module 260 in one embodiment may be configured to communicate with the on-body patch device 211 in a similar manner as the reader device/receiver unit 220 and may include communication components such as antenna, power supply and memory, among others, for example, to allow provision of RF power to the on-body patch device 211 or to request or prompt the on-body patch device 211 to send the functionality related data and optionally stored analyte related data. The data processing module 260 may be configured to interact with the on-body patch device 211 in a similar manner as the reader device/receiver unit 220 such that the data processing module 260 may be positioned within a predetermined distance from the on-body patch device 211 for communication with the on-body patch device 211.

[0047] In one aspect, the on-body patch device 211 and the data processing module 260 may be positioned on the skin surface of the user or the patient within the predetermined distance of each other (for example, within approximately 5 inches or less) such that the communication between the on-body patch device 211 and the data processing module 260 is maintained. In a further aspect, the housing of the data processing module 260 may be configured to couple to or cooperate with the housing of the on-body patch device 211 such that the two devices are combined or integrated as a single assembly and positioned on the skin surface.

[0048] Referring again to FIG. 2, the data processing module 260 may be configured or programmed to prompt or ping the on-body patch device 211 at a predetermined time interval such as once every minute, or once every five minutes or once every 30 minutes or any other suitable or desired programmable time interval to request functionality related data from the on-body patch device 211 which is received and is stored in one or more memory devices or components of the data processing module 260. In another embodiment, the data processing module 260 is configured to prompt or ping the on-body patch device 211 when desired by the patient or the user on-demand, and not based on a predetermined time interval. In yet another embodiment, the data processing module 260 is configured to prompt or ping the on-body patch device 211 when desired by the patient or the user upon request only after a programmable time interval has elapsed. For example, in certain embodiments, if the user does not initiate communication within a programmed time period, such as, for example 5 hours from last communication (or 10 hours from the last communication), the data processing module 260 may be programmed to automatically ping or prompt the on-body patch device 211 or alternatively, initiate an alarm function to notify the user that an extended period of

time has elapsed since the last communication between the data processing module 260 and the on-body patch device 211. In this manner, users, healthcare providers, or the patient may program or configure the data processing module 260 to provide certain compliance with analyte monitoring regimen, to avoid a failure of the analyte sensor device from going unnoticed. Similar functionalities may be provided or programmed in the receiver unit or the reader device in certain embodiments.

[0049] As further shown in FIG. 2, the data processing module 260 in one aspect may be configured to transmit the stored data received from the on-body patch device 211 to the reader device/receiver unit 220 when communication between the data processing module 260 and the reader device/receiver unit 220 is established. More specifically, in addition to RF antenna and RF communication components described above, data processing module 260 may include components to communicate using one or more wireless communication protocols such as, for example, but not limited to, infrared (IR) protocol, Bluetooth protocol, Zigbee protocol, and 802.11 wireless LAN protocol. Additional description of communication protocols including those based on Bluetooth protocol and/or Zigbee protocol can be found in U.S. Patent Publication No. 2006/0193375 incorporated herein by reference for all purposes. The data processing module 260 may further include communication ports, drivers or connectors to establish wired communication with one or more of the reader device/receiver unit 220, on-body patch device 211, or the remote terminal 270 including, for example, but not limited to USB connector and/or USB port, Ethernet connector and/or port, FireWire connector and/or port, or RS-232 port and/or connector.

[0050] In one aspect, the data processing module 260 may be configured to operate as a data logger configured or programmed to periodically request or prompt the on-body patch device 211 to transmit the functionality related information, and to store the received information for later retrieval or subsequent transmission to the reader device/receiver unit 220 or to the remote terminal 270 or both, for further processing and analysis.

[0051] In a further aspect, the functionalities of the data processing module 260 may be configured or incorporated into a memory device such as an SD card, microSD card, compact flash card, XD card, Memory Stick card, Memory Stick Duo card, or USB memory stick/device including software programming resident in such devices to execute upon connection to the respective one or more of the on-body patch device 211, the remote terminal 270 or the reader device/receiver unit 220. In a further aspect, the functionalities of the data processing module 260, including executable software and programming, may be provided to a communication device such as a mobile telephone including, for example, iPhone, iPod Touch, Blackberry device, Palm based device (such as Palm Pre, Treo, Treo Pro, Centro), personal digital assistants (PDAs) or any other communication enabled operating system (such as Windows or Android operating systems) based mobile telephones as a downloadable application for execution by the downloading communication device. To this end, the remote terminal 270 as shown in FIG. 2 may include a personal computer, or a server terminal that is configured to provide the executable application software to one or more of the communication devices described above when communication between the remote terminal 270 and the devices are established.

[0052] Depending upon the user setting or configuration on the communication device, the downloaded application may be programmed or customized using the user interface of the respective communication device (screen, keypad, and the like) to establish or program the desired settings such as a receiver alarm, an insulin pump alarm, sensor replacement alarm, or any other alarm or alert conditions as may be desired by the user. Moreover, the programmed notification settings on the communication device may be output using the output components of the respective communication devices, such as speaker, vibratory output component, or visual output/display. As a further example, the communication device may be provided with programming and application software to communicate with the on-body patch device 211 such that a frequency or periodicity of data acquisition is established. In this manner, the communication device may be configured to conveniently receive functionality information from the on-body patch device 211 at predetermined time periods such as, for example, but not limited to once every minute, once every five minutes, or once every 10 or 15 minutes, and store the received information, as well as to provide a desired or appropriate warning indication or notification to the user or the patient.

[0053] FIG. 3 is a block diagram of a receiver/monitor unit or insulin pump such as that shown in FIG. 1 in accordance with certain embodiments. The primary receiver unit 104 (FIG. 1) includes one or more of: a blood glucose test strip interface 301, an RF receiver 302, an input 303, a temperature detection section 304, and a clock 305, each of which is operatively coupled to a processing and storage section 307. The primary receiver unit 104 also includes a power supply 306 operatively coupled to a power conversion and monitoring section 308. Further, the power conversion and monitoring section 308 is also coupled to the receiver processor 307. Moreover, also shown are a receiver serial communication section 309, and an output 310, each operatively coupled to the processing and storage unit 307. The receiver may include user input and/or interface components or may be free of user input and/or interface components.

[0054] In one aspect, the RF receiver 302 is configured to communicate, via the communication link 103 (FIG. 1) with the data processing unit (sensor electronics) 102, to receive encoded data from the data processing unit 102 for, among others, signal mixing, demodulation, and other data processing. The input 303 of the primary receiver unit 104 is configured to allow the user to enter information into the primary receiver unit 104 as needed. In one aspect, the input 303 may include keys of a keypad, a touch-sensitive screen, and/or a voice-activated input command unit, and the like. The temperature monitor section 304 may be configured to provide temperature information of the primary receiver unit 104 to the processing and control section 307, while the clock 305 provides, among others, real time or clock information to the processing and storage section 307.

[0055] Each of the various components of the primary receiver unit 104 shown in FIG. 3 is powered by the power supply 306 (or other power supply) which, in certain embodiments, includes a battery. Furthermore, the power conversion and monitoring section 308 is configured to monitor the power usage by the various components in the primary receiver unit 104 for effective power management and may alert the user, for example, in the event of power usage which renders the primary receiver unit 104 in sub-optimal operating conditions. The serial communication section 309 in the

primary receiver unit 104 is configured to provide a bi-directional communication path from the testing and/or manufacturing equipment for, among others, initialization, testing, and configuration of the primary receiver unit 104.

[0056] Serial communication section 309 can also be used to upload data to a computer, such as functionality related data. The communication link with an external device (not shown) can be made, for example, by cable (such as USB or serial cable), infrared (IR) or RF link. The output/display 310 of the primary receiver unit 104 is configured to provide, among others, a graphical user interface (GUI), and may include a liquid crystal display (LCD) for displaying information. Additionally, the output/display 310 may also include an integrated speaker for outputting audible signals as well as to provide vibration output as commonly found in handheld electronic devices, such as mobile telephones, pagers, etc. In certain embodiments, the primary receiver unit 104 also includes an electro-luminescent lamp configured to provide backlighting to the output 310 for output visual display in dark ambient surroundings.

[0057] Referring back to FIG. 3, the primary receiver unit 104 may also include a storage section such as a programmable, non-volatile memory device as part of the processor 307, or provided separately in the primary receiver unit 104, operatively coupled to the processor 307. The processor 307 may be configured to perform Manchester decoding (or other protocol(s)) as well as error detection and correction upon the encoded data received from the data processing unit 102 via the communication link 103.

[0058] In further embodiments, the data processing unit 102 and/or the primary receiver unit 104 and/or the secondary receiver unit 106, and/or the data processing terminal/infusion section 105 of FIG. 1 may be configured to receive the blood glucose value wirelessly over a communication link from, for example, a blood glucose meter. In further embodiments, a user manipulating or using the analyte monitoring system 100 (FIG. 1) may manually input the blood glucose value using, for example, a user interface (for example, a keyboard, keypad, voice commands, and the like) incorporated in the one or more of the data processing unit 102, the primary receiver unit 104, secondary receiver unit 106, or the data processing terminal/infusion section 105.

[0059] Additional detailed descriptions are provided in U.S. Pat. Nos. 5,262,035; 5,264,104; 5,262,305; 5,320,715; 5,593,852; 6,175,752; 6,650,471; 6,746, 582, 6,284,478, 7,299,082, and 7,811,231, in application Ser. No. 11/060,365 filed Feb. 16, 2005 titled "Method and System for Providing Data Communication in Continuous Glucose Monitoring And Management System", in application Ser. No. 12/698, 124 filed Feb. 1, 2010 titled "Compact On-Body Physiological Monitoring Devices and Methods Thereof", and in application Ser. No. 12/807,278 filed Aug. 31, 2010 titled "Medical Devices and Methods", each of which is incorporated herein by reference.

[0060] A safety issue with the receiver device, continuous glucose monitors (CGMs), repeater unit, and insulin pumps in an analyte monitoring system is the susceptibility to single point failure associated with each device's microprocessor, power supply, audio annunciators, transmitter, and transceiver. Introducing a power supply monitoring circuit, a microprocessor monitoring circuit, a secondary power supply, and/or audio annunciator (or vibrator) to the device will provide redundancy that will reduce the likelihood of a failure going unnoticed by the user; however, including these com-

ponents is costly in terms of expense and product size. The embodiments of the present disclosure provide additional protection against single point failures in systems made up of two or more devices. Essentially, each device in the analyte monitoring system is monitored by one or more of the other devices in the system.

[0061] In certain integrated CGM and insulin pump system embodiments, where both devices contain at least one microprocessor, power supply, and audio annunciator or other alarm mechanism, in one embodiment, each device can perform a periodic self test and report this to the other device. Each device has a monitoring process that would initiate an alarm if the other device does not report a successful self test. In some embodiments, the monitoring device could poll the other device, and even initiate the self test on the other device. Also, different functionality could be tested and/or reported on different test schedules.

[0062] The applicability of this functionality depends on how necessary periodic communication between the devices is to the function of the system. For instance, in certain embodiments where the receiver device of a continuous analyte monitoring system may not need to be in communication, such as RF communication, range with an insulin pump for the insulin pump to function, this feature could be optional, e.g., configured by the user, a parent of the user, and/or a physician. In other embodiments, such as for a closed loop control system where the control algorithm is maintained in the receiver device, frequent communication is needed between the handheld and the pump, and therefore continuous knowledge of the functionality of both devices is vital.

[0063] FIG. 4 is a flow diagram illustrating steps in an embodiment for mitigating single point failure of at least one device in an analyte monitoring system 400. The first device 402 and the second device 404 in the analyte monitoring system 400 can be at least one of a receiver device, an analyte meter, a glucose monitor, an insulin pump, a continuous analyte monitor, a cellular phone, a personal digital assistant, a personal computer, a laptop computer, and/or a repeater unit. In certain embodiments, a first device 402 sends a request that a functionality check of the components of a second device 404 be performed (406). The request can be sent, for example, wirelessly from the transmitter of the first device 402 to the transceiver of the second device 404. The components of the second device 404 can include at least one of a microprocessor, a power supply, a sensor, an electronic component, and a storage device.

[0064] The second device 404 receives the request to perform a functionality check of the second device 404 from the first device 402 (408) and performs the functionality check of its components (410). In certain embodiments, the second device 404 only performs the functionality check if the second device 404 has the capacity to perform the check. A functionality check, or "self-test", is a standard feature of most electronic devices. The functionality check of the components can include a determination of the current, voltage, and/or resistance that can be measured across an electrical circuit in the one or more components. The functionality check can include component testing that applies an input to the various components being tested, and receives an output based on the input. The functionality check may also include checking digital system components, such as a checksum for a block of memory. Any of a number of common techniques used in electronic devices can be applied to the functionality check of the present disclosure. In addition, some compo-

nents of the devices in the analyte monitoring system may have built in self-test functionality that can be queried. For instance, a power supply module may have a digital self-test status output that can be queried by the processor in order to determine the functionality of the power supply. A device may have electronic circuitry that includes electronic or mechanical switches that allow testing of the electronic circuitry. The switch, for example, could route the current path for functional test across the speaker circuit to test for the proper speaker resistance, in order to detect any open or short circuits.

[0065] Referring still to FIG. 4, the second device 404 determines the functionality of its components based on the outcome of the functionality check (412) and the second device 404 communicates data related to the determined functionality of its components to the first device 402 (414). In certain embodiments the second device 404 determining the functionality of its components (412) is optional and data related to the functionality of the second device 404 can be sent to the first device 402 without a determination of functionality being processed at the second device 404. The data can be communicated, for example, from the transmitter of the second device 404 to the transceiver of the first device 402.

[0066] Still referring to FIG. 4, the data related to the functionality of the components of the second device 404 is received at the first device 402 (416). The first device 402 then retrieves from storage a list that includes at least one predetermined criterion related to the functionality of the components of the second device 404 (418). The predetermined criterion can be, for instance, current, voltage and/or resistance thresholds or ranges used to define the proper operating range. In certain embodiments, for example, the functional check may measure the power supply voltage to determine if it is in an acceptable tolerance. In certain embodiments, the predetermined criterion may be a digital or coded threshold range used to define the proper operating range, whereby, the measured functional test output can be compared to the criterion threshold (e.g., above or below) or compared to the criterion range (e.g., within or outside) to determine functional test status of the component.

[0067] Returning to FIG. 4, the first device 402 compares the data related to the functionality of the second device 404 with the list including the at least one predetermined criterion (420) to determine if the second device 404 is functioning properly (422). In certain embodiments, the first device 402 announces or otherwise communicates an alarm to alert a user if it is determined that the second device 404 is not functioning properly (424). The alarm may be at least one of an audio alarm, a vibratory alarm, and a visual alarm.

[0068] In certain embodiments, the first device 402 does not have to poll the second device 404 to perform the functionality check if the second device 404 automatically performs the functionality check at predetermined intervals and automatically sends a signal or data related to the functionality of the second device 404 to the first device 402. In this manner, in certain embodiments, if the first device 402 does not automatically receive a signal or data related to the functionality of the second device 404 within a predetermined time period, then the first device 402 will announce an alarm to alert the user that the second device 404 is not functioning properly.

[0069] FIG. 5 is a flow diagram illustrating steps in an embodiment for mitigating single point failure of at least one

device in an analyte monitoring system 500. The first device 502 and the second device 504 in the analyte monitoring system 500 can be at least one of a receiver device, an analyte meter, a glucose monitor, an insulin pump, a continuous analyte monitor, a cellular phone, a personal digital assistant, a personal computer, a laptop computer, and/or a repeater unit. Execution of the method begins at process block 506 when a first device 502 sends a request that a functionality check of the components of a second device 504 be performed. The request can be sent, for example, wirelessly from the transmitter of the first device 502 to the transceiver of the second device 504. The components of the second device 504 include at least one of a microprocessor, a power supply, a sensor, an electronic component, and a storage device.

[0070] Referring to FIG. 5, the second device 504 receives the request to perform a functionality check from the first device 502 (508) and the second device 504 performs the functionality check of its components (510). In certain embodiments, the second device 504 only performs the functionality check if the second device 504 has the capacity to perform the check. The functionality check of the components can include a determination of the current, voltage, and/or resistance that can be measured across an electrical circuit in the components. Additionally, the functionality check can include component testing that applies an input to the various components being tested, and receives an output based on the input. The functionality check may also include checking digital system components, such as a checksum for a block of memory. Any of a number of common techniques used in electronic devices can be applied to this invention. In addition, some components of the devices in the analyte monitoring system may have built in self-test functionality that can be queried, for instance, a power supply module may have a digital self-test status output that can be queried by the processor in order to determine the functionality of the power supply. Also, a device may have electronic circuitry that includes electronic or mechanical switches that allow testing of the electronic circuitry. The switch, for example, could route the current path for functional test across the speaker circuit to test for the proper speaker resistance, in order to detect any open or short circuits.

[0071] Referring back to FIG. 5, the second device 504 determines the functionality of its components based on the outcome of the functionality check (512) and communicates data related to the determined functionality of its components to the first device 502 (514). The data can be communicated, for example, from the transmitter of the second device 504 to the transceiver of the first device 502. In certain embodiments, the second device 504 may communicate data related to the functionality of its components to the first device 502 without determining the functionality of the components at the second device 504 itself. The data related to the functionality of the components of the second device 504 is then received at the first device 502 (516) and the first device 502 retrieves from storage a list that includes at least one predetermined criterion related to the functionality of the components of the second device 504 (518). The predetermined criterion can be, for instance, current, voltage and/or resistance thresholds or ranges used to define the proper operating range. In certain embodiments, the functional check may measure the power supply voltage to determine if it is in an acceptable tolerance. In certain embodiments, the predetermined criterion may be a digital or coded threshold range used to define the proper operating range. The measured

functional test output can be compared to the criterion threshold (e.g., above or below) or compared to the criterion range (e.g., within or outside) to determine functional test status of the component.

[0072] Referring still to FIG. 5, the first device 502 compares the data related to the functionality of the second device 504 with the list including the at least one predetermined criterion at process block 520 and determines if the second device 504 is functioning properly (522). If it is determined that the second device 504 is not functioning properly, the first device 502 requests that the second device 504 announce an alarm to alert a user that the second device 504 is not functioning properly (524). The request may be sent from the transmitter of the first device 502 to the transceiver of the second device 504. The second device 504 receives the request from the first device 502 to announce the alarm to alert the user of its lack of proper functionality (526) and then announces the corresponding alarm (528). The alarm may be at least one of an audio alarm, a vibratory alarm, and a visual alarm.

[0073] FIG. 6 is a flow diagram illustrating steps in one embodiment for mitigating single point failure of at least one device in an analyte monitoring system 600 that includes a first device 602, a repeater unit 604, and a second device 606. The first device 602 can include at least one of a receiver unit, an analyte meter, a cellular phone, a personal digital assistant, a personal computer, a laptop computer, and an insulin pump. The repeater unit 604 can be operatively or physically coupled to second device 606. The second device can be an analyte sensor and/or a continuous glucose monitor.

[0074] Referring to FIG. 6, in certain embodiments, the first device 602 sends a request to the repeater unit 604 that the second device 606 perform a functionality check of its components (608). The request can be sent, for example, wirelessly from the transmitter of the first device 602 to the transceiver of the repeater unit 604. The repeater unit 604 receives the request from the first device 602 (610) and sends, to the second device 606, a request to perform a functionality check of the components of the second device 606 (612). The request may be sent, for example, wirelessly from the transmitter of the repeater unit 604 to the transceiver of the second device 606.

[0075] Still referring to FIG. 6, the request to perform a functionality check of its components is received at the second device 606 (614) and, if it is functioning in a high enough capacity, the second device 606 performs the functionality check of one or more of its components (616). In certain embodiments, the functionality check of the components can include a determination of the current, voltage, and/or resistance that can be measured across an electrical circuit in the one or more components. Additionally, the functionality check can include component testing that applies an input to the various components being tested, and receives an output based on the input. The functionality check may also include checking digital system components, such as a checksum for a block of memory. Any of a number of common techniques used in electronic devices can be applied to this invention. In addition, some components of the devices in the analyte monitoring system may have built in self-test functionality that can be queried, for instance, a power supply module may have a digital self-test status output that can be queried by the processor in order to determine the functionality of the power supply. Also, a device may have electronic circuitry that includes electronic or mechanical switches that allow testing

of the electronic circuitry. The switch, for example, could route the current path for functional test across the speaker circuit to test for the proper speaker resistance, in order to detect any open or short circuits.

[0076] Returning to FIG. 6, the second device 606 determines the functionality check of its components based upon the results of the functionality check (618) and data related to the results of the functionality check are then communicated from the second device 606 to the repeater unit 604 (620). The data can be communicated, for example, wirelessly from the transmitter of the second device 606 to the transceiver of the repeater unit 604. The repeater unit 604 receives the data related to the results of the functionality check of the one or more components of the second device 606 (622) and communicates the data related to the results of the functionality check of the second device 606 to the first device 602 (624). The data can be communicated, for example, wirelessly from the transmitter of the repeater unit 604 to the transceiver of the first device 602. The data related to the functionality check of the one or more components of the second device 606 is then received at the first device 602 (626). The first device 602 retrieves from storage a list including at least one predetermined criterion related to the functionality of the one or more components of the second device (628) and compares the data related to the results of the functionality check with the list including the at least one predetermined criterion (630). The predetermined criterion can be, for instance, current, voltage and/or resistance thresholds or ranges used to define the proper operating range. For instance, the functional check may measure the power supply voltage to determine if it is in an acceptable tolerance. Additionally, the predetermined criterion may be a digital or coded threshold range used to define the proper operating range. The measured functional test output can be compared to the criterion threshold (e.g., above or below) or compared to the criterion range (e.g., within or outside) to determine functional test status of the component. The first device 602 then determines if the second device 604 is functioning in accordance with the at least one predetermined criterion (632) and, if it is determined that the second device 606 is not functioning in accordance with the at least one predetermined criterion, requests that the repeater unit 604 announce an alarm (634). The request can be sent, for example, from the transmitter of the first device 602 to the transceiver of the repeater unit 604. The repeater unit 604 receives the request from the first device 602 to announce an alarm to alert a user that the second device 606 is not functioning properly (636) and accordingly an alarm is announced by the repeater unit 604 (638). The alarm may include at least one of an audio alarm, a vibratory alarm, and a visual alarm that is produced at the repeater unit 604.

[0077] In certain embodiments, the first device 602 does not have to send a request to the repeater unit 604 if the repeater unit 604 automatically polls the second device 606 to perform the functionality check or if the second device 606 automatically performs the functionality check at predetermined intervals and then automatically sends this information to the repeater unit 604. In this instance, if the repeater unit 604 does not receive a signal or data related to the functionality of the second device 606, then the repeater unit 604 can announce an alarm to alert the user that the second device 606 is not functioning properly.

[0078] FIG. 7 is a flow diagram illustrating an embodiment for mitigating single point failure of the transmitter of at least one device in an analyte monitoring system 700 that includes

a first device 702 and a second device 704. The first device 702 sends a request to a second device 704 to perform a functionality check of the components of the second device 704 (706). If a signal or data has not been received at the first device 702 within a predetermined amount of time, then the first device 702 determines that at least one of the components of the second device 704 is not functioning properly (710) and announces an alarm to alert a user that the second device 704 is not functioning properly (712).

[0079] In certain embodiments, the first device 702 does not have to request that the second device 704 perform a functionality check of its components, as the second device 704 automatically performs the functionality check at predetermined intervals and then automatically sends data related to the results of the functionality check to the first device 702. In this instance, if the first device 702 does not automatically receive data related to the functionality of the second device 704, then the first device 702 determines that the second device 704 is not functioning properly and announces an alarm at the first device 702 to alert the user.

[0080] In certain embodiments, the analyte monitoring system includes at least one transmitter attached to the continuous analyte sensor, the receiver device, and the insulin pump. In certain embodiments, the receiver device and/or the insulin pump will detect if the transmitter in the continuous analyte sensor stops functioning. In certain embodiments, the insulin pump and/or the continuous analyte sensor will detect if the transmitter in the receiver device stops functioning. In certain embodiments, the receiver device and/or the continuous analyte sensor will detect if the transmitter in the insulin pump stops functioning.

[0081] In certain embodiments, a computer-implemented method for mitigating single point failure of at least one device in an analyte monitoring system includes requesting that a functionality check of one or more components of a first device be performed and that data related to the functionality check of the one or more components of the first device be communicated to a second device, receiving information from the first device that is related to functionality of the one or more components of the first device, communicating the information related to the functionality of the one or more components of the first device to a third device, receiving a request from the third device that an alarm be announced if it is determined by the third device that the one or more components of the first device is not functioning in accordance with at least one predetermined criterion, and announcing an alarm to alert a user that the one or more components of the first device is not functioning in accordance with the at least one predetermined criterion.

[0082] In certain aspects, the first device is a continuous glucose monitor.

[0083] In certain aspects, the second device includes a repeater unit operatively coupled to the continuous glucose monitor.

[0084] In certain aspects, the third device includes one of a receiver device or an insulin pump.

[0085] In certain aspects, the one or more components of the first device include at least one of a microprocessor, a power supply, a sensor, and an electronic component.

[0086] In certain aspects, the alarm includes at least one of an audio alarm, a vibratory alarm, and a visual alarm.

[0087] Certain aspects include receiving a request from the third device that a functionality check of one or more components of a first device be performed and that data related to

the functionality check of the one or more components of the first device be communicated to the third device, wherein the request is received at the second device, the second device being operatively coupled to the first device.

[0088] In certain aspects, the information related to the functionality of the one or more components of the first device includes a lack of data being received from the first device.

[0089] Certain aspects include that the functionality check includes at least one of a determination of a current, a voltage, and a resistance that is measured across an electrical circuit in the one or more components, applying an input to the one or more components and receiving an output from the one or more components, a digital check of the one or more components, a checksum of a memory of the first device, a self-test output check of the one or more components, and an electrical or mechanical test of at least one switch of the one or more components.

[0090] Certain embodiments include the at least one predetermined criterion including at least one of a current, a voltage, and a resistance threshold used to define a proper operating range of the first device, a power supply measurement that defines an acceptable tolerance, and a digital threshold range used to define a proper operating range.

[0091] In certain embodiments, a computer-implemented method for mitigating single point failure of at least one device in an analyte monitoring system includes requesting that a functionality check of one or more components of a first device be performed and that data related to the functionality check of the one or more components of the first device be communicated to a second device, receiving the data related to the functionality of the one or more components of the first device, retrieving a list including at least one predetermined criterion related to the functionality of the one or more components of the first device from a storage component of the second device, comparing the data related to the functionality of the one or more components of the first device with the list including the at least one predetermined criterion, and determining if the one or more components of the first device is functioning in accordance with the at least one predetermined criterion.

[0092] Certain aspects include requesting that an alarm be annunciated at a third device to alert a user if it is determined by the second device that the one or more components of the first device is not functioning in accordance with the at least one predetermined criterion.

[0093] In certain aspects, the third device is operatively coupled to the first device.

[0094] In certain aspects, the request for the functionality check is received by a third device and the third device polls the first device to perform the functionality check.

[0095] Certain aspects include annunciating an alarm operatively coupled to the second device to alert a user if it is determined that the one or more components of the first device is not functioning in accordance with the at least one predetermined criterion.

[0096] In certain aspects, the first device is a continuous glucose monitor.

[0097] In certain aspects, the second device is one of a receiver device or an insulin pump.

[0098] In certain aspects, the third device is a repeater unit operatively coupled to the continuous glucose monitor.

[0099] In certain aspects, the one or more first components of the first device include at least one of a microprocessor, a power supply, a sensor, and an electric component.

[0100] In certain aspects, the alarm includes at least one of an audio alarm, a vibratory alarm, and a visual alarm.

[0101] Certain aspects include that the functionality check includes at least one of a determination of a current, a voltage, and a resistance that is measured across an electrical circuit in the one or more components, applying an input to the one or more components and receiving an output from the one or more components, a digital check of the one or more components, a checksum of a memory of the first device, a self-test output check of the one or more components, and an electrical or mechanical test of at least one switch of the one or more components.

[0102] Certain aspects include that the at least one predetermined criterion includes at least one of a current, a voltage, and a resistance threshold used to define a proper operating range of the first device, a power supply measurement that defines an acceptable tolerance, and a digital threshold range used to define a proper operating range.

[0103] In certain embodiments, a computer-implemented method for mitigating single point failure of at least one device in an analyte monitoring system includes requesting that a functionality check of one or more components of a first device be performed and that data related to the functionality check of the one or more components of the first device be communicated to a second device, and determining that the one or more components of the first device is not functioning properly if the data related to the functionality check of the components of the first device is not received at the second device, wherein an alarm is annunciated from at least one of the second device or a third device to alert a user that one or more components of the first device is not functioning properly.

[0104] Various other modifications and alterations in the structure and method of operation of the embodiments of the present disclosure will be apparent to those skilled in the art without departing from the scope and spirit of the present disclosure. Although the present disclosure has been described in connection with certain embodiments, it should be understood that the present disclosure as claimed should not be unduly limited to such embodiments. It is intended that the following claims define the scope of the present disclosure and that structures and methods within the scope of these claims and their equivalents be covered thereby.

What is claimed is:

1. A computer-implemented method for mitigating single point failure of at least one device in an analyte monitoring system, comprising:

requesting, using a second device, that a functionality check of one or more components of a first device be performed and that data related to the functionality check of the one or more components of the first device be communicated to the second device;

receiving, at the second device, information from the first device that is related to functionality of the one or more components of the first device;

communicating, using the second device, the information related to the functionality of the one or more components of the first device to a third device;

receiving, at the second device, a request from the third device that an alarm be annunciated if it is determined by the third device that the one or more components of the

first device is not functioning in accordance with at least one predetermined criterion; and

annunciating, using the second device, an alarm to alert a user that the one or more components of the first device is not functioning in accordance with the at least one predetermined criterion.

2. The computer-implemented method of claim 1, wherein the first device is a continuous glucose monitor.

3. The computer-implemented method of claim 2, wherein the second device includes a repeater unit operatively coupled to the continuous glucose monitor.

4. The computer-implemented method of claim 1, wherein the third device includes one of a receiver device or an insulin pump.

5. The computer-implemented method of claim 1, wherein the one or more components of the first device include at least one of a microprocessor, a power supply, a sensor, and an electronic component.

6. The computer-implemented method of claim 1, wherein the alarm includes at least one of an audio alarm, a vibratory alarm, and a visual alarm.

7. The computer-implemented method of claim 1, further comprising:

receiving, at the second device, a request from the third device that a functionality check of one or more components of a first device be performed and that data related to the functionality check of the one or more components of the first device be communicated to the third device, wherein the second device is operatively coupled to the first device.

8. The computer-implemented method of claim 1, wherein the information related to the functionality of the one or more components of the first device includes a lack of data being received from the first device.

9. The computer-implemented method of claim 1, wherein the functionality check includes at least one of a determination of a current, a voltage, and a resistance that is measured across an electrical circuit in the one or more components, applying an input to the one or more components and receiving an output from the one or more components, a digital check of the one or more components, a checksum of a memory of the first device, a self-test output check of the one or more components, and an electrical or mechanical test of at least one switch of the one or more components.

10. The computer-implemented method of claim 1, wherein the at least one predetermined criterion includes at least one of a current, a voltage, and a resistance threshold used to define a proper operating range of the first device, a power supply measurement that defines an acceptable tolerance, and a digital threshold range used to define a proper operating range.

11. A computer-implemented method for mitigating single point failure of at least one device in an analyte monitoring system, comprising:

requesting, using a second device, that a functionality check of one or more components of a first device be performed and that data related to the functionality check of the one or more components of the first device be communicated to the second device;

receiving, at the second device, the data related to the functionality of the one or more components of the first device;

retrieving, from the second device, a list including at least one predetermined criterion related to the functionality of the one or more components of the first device;

comparing, using the second device, the data related to the functionality of the one or more components of the first device with the list including the at least one predetermined criterion; and

determining, using the second device, if the one or more components of the first device is functioning in accordance with the at least one predetermined criterion.

12. The computer-implemented method of claim 11, further comprising:

requesting, using the second device, that an alarm be annunciated at a third device to alert a user if it is determined by the second device that the one or more components of the first device is not functioning in accordance with the at least one predetermined criterion.

13. The computer-implemented method of claim 12, wherein the third device is operatively coupled to the first device.

14. The computer-implemented method of claim 11, wherein the request for the functionality check is received by a third device and the third device polls the first device to perform the functionality check.

15. The computer-implemented method of claim 11, further comprising:

annunciating, using the second device, an alarm to alert a user if it is determined that the one or more components of the first device is not functioning in accordance with the at least one predetermined criterion.

16. The computer-implemented method of claim 11, wherein the third device is a repeater unit operatively coupled to the first device.

17. The computer-implemented method of claim 11, wherein the one or more first components of the first device include at least one of a microprocessor, a power supply, a sensor, and an electric component.

18. The computer-implemented method of claim 15, wherein the alarm includes at least one of an audio alarm, a vibratory alarm, and a visual alarm.

19. The computer-implemented method of claim 11, wherein the functionality check includes at least one of a determination of a current, a voltage, and a resistance that is measured across an electrical circuit in the one or more components, applying an input to the one or more components and receiving an output from the one or more components, a digital check of the one or more components, a checksum of a memory of the first device, a self-test output check of the one or more components, and an electrical or mechanical test of at least one switch of the one or more components.

20. The computer-implemented method of claim 11, wherein the at least one predetermined criterion includes at least one of a current, a voltage, and a resistance threshold used to define a proper operating range of the first device, a power supply measurement that defines an acceptable tolerance, and a digital threshold range used to define a proper operating range.

21. A computer-implemented method for mitigating single point failure of at least one device in an analyte monitoring system, comprising:

requesting, using a second device, that a functionality check of one or more components of a first device be performed and that data related to the functionality

check of the one or more components of the first device be communicated to the second device; and
determining, using the second device, that the one or more components of the first device is not functioning properly if the data related to the functionality check of the components of the first device is not received at the second device;
wherein an alarm is annunciated from at least one of the second device or a third device to alert a user that one or more components of the first device is not functioning properly.

* * * * *