

[REDACTED]

[REDACTED]

EXHIBIT 176

[REDACTED]

SERENDIA-00005698

CX-0761C.1



Home > For Providers > SYLFIRM SERIES > Sylfirm X




Sylfirm X

FDA Cleared Pulsed Wave (PW) and Continuous Wave (CW) Radio Frequency Micro Needling device.

BROCHURE DOWNLOAD

At 300 μ m, Papillary Dermis

FDA Cleared Pulsed Wave (PW) and Continuous Wave (CW) Radio Frequency Micro Needling device. Dual wave is subdivided into 8 different modes, which can be customized to individual patients, taking into account the indications, skin conditions, to provide a delicate treatment.

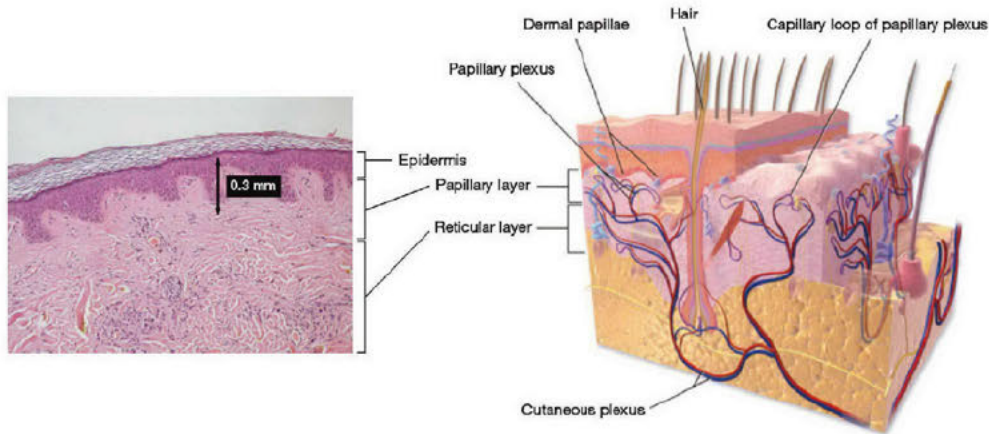

Optimal Skin Rejuvenating Depth

Papillary Dermis contains collagen factors, especially Type III collagen. Compared with older adults, the distribution of Type III collagen in the fetus's skin is higher than that of Type I. Also Type III collagen is present more in papillary dermis than reticular dermis. The density of type III collagen increased after 300 μ m targeted treatment with Sylfirm X.

Regulation of Hyperactive Melanocytes

The senescent fibroblasts, which stimulate melanogenesis, are more distributed in the melasma lesion than in the perilesional area, and more in the papillary dermis than in the reticular dermis. 300 μ m target procedure improves senescent fibroblasts that promote melanin production, strengthens the basement membrane, and helps improve melasma.




FOR PROVIDERS

FOR PATIENTS


NEWS & EVENTS

ABOUT US


CONTACT US

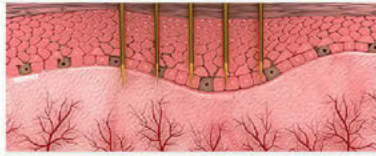

Electrodes inserted into the dermal tissue

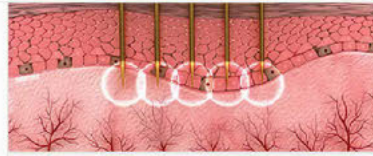

Delivers RF Energy

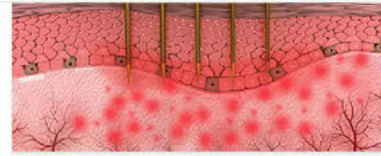

Create Thermal Coagulation Zone

SYLFIRM X, Ultimate Edition

Dual Wave RF Microneedling System

PULSED WAVE (PW) & CONTINUOUS WAVE (CW)

FDA Cleared Pulsed Wave (PW) and Continuous Wave (CW) Radio Frequency Micro Needling device featuring 300 Micron depth targeting both skin laxity. Sylfirm X with its 8 different PW/CW modes has proven its effectiveness and safety through 25+ clinical studies and experiments.

- Minimally Invasive
- Short Treatment Time
- Minimal Downtime
- Safe & Comfortable
- Immediate Results

Bipolar Non-insulated Electrode System

SYLFIRM X adopted bipolar non-insulated micro needle electrodes to cover all dermal layers with uniform electric field and maximize the treatment result specifically for during the Pulsed Wave (PW) modes, and during the Continuous Wave (CW) modes.


Robotic Production System

The micro needles are precisely produced by the robotic system, which brings evenly-leveled electrodes to penetrate an accurate target depth during the treatment.

Two Type X Mode



Accessories



https://violmedical.com/for_providers/product?idx=10

2/25/2023

SERENDIA-00005700

Ex. 2079-003

CX-0761C.3



FOR PROVIDERS

FOR PATIENTS

NEWS & EVENTS

ABOUT US

CONTACT US

5*5(25Pin), 2mm

X-25 Tip (Full Face)

5*5(25Pin), 2mm

XE-25 Tip (Full Face)

5*5(25Pin), 1.5mm

XA-25 Tip (Intensive)

6*3(18Pin), 1.5mm

XW-18 Tip (Narrow Area)

Marketing Materials

DOWNLOAD

Testimonials

Sylfirm X offers the next generation of a radiofrequency (RF) micro-needling device. This new device has replaced my older machines, because it is much more comfortable for patients, and it features two waveform modalities that are specific for individual patients' needs.

Diane Duncan, MD, FACS

Specification

System Type	RF (Radiofrequency)
Power Input	AC 100~240V, 50/60Hz
Electrode Depth	2 Mhz
Mode	8 Modes CW(Continuous Wave) 1~4 PW(Pulsed Wave) 1~4
Max Power	0~12 Level (0: Minimum, RF OFF) (1-12: Maximum, RF ON)
Speed	0.1~1 sec (0.1sec step)



https://violmedical.com/for_providers/product?idx=10

2/25/2023

SERENDIA-00005701

Ex. 2079-004

CX-0761C.4

Viol global website is only for international users.

LOGIN [KOR](#)



[FOR PROVIDERS](#)

[FOR PATIENTS](#)

[NEWS & EVENTS](#)

[ABOUT US](#)

[CONTACT US](#)



[Privacy Policy](#)

[Terms of use](#)

[Log In](#)

Headquarters


808, 809, Bundang Technopark C, 744, Pangyo-ro, Bundang-gu, Seongnam-si, Gyeonggi-do, Republic of Korea('3510)

TEL. +82 31 8017 7893

FAX. +82 31 8016 7894

E-mail. info@scarletf.com

COPYRIGHT © 2022 Viol Co., Ltd. All Rights Reserved.



https://violmedical.com/for_providers/product?idx=10

2/25/2023

SERENDIA-00005702

Ex. 2079-005

CX-0761C.5