



(19) **United States**

(12) **Patent Application Publication**

Bainbridge et al.

(10) **Pub. No.: US 2002/0033370 A1**

(43) **Pub. Date: Mar. 21, 2002**

(54) **EXTRACORPOREAL BLOOD PROCESSING METHODS AND APPARATUS**

Publication Classification

(76) Inventors: **Marlene Bainbridge**, Lakewood, CO (US); **Muriel Keller**, Thornton, CO (US); **Timothy M. Gordon**, Littleton, CO (US); **Michael J. McAteer**, Lakewood, CO (US); **Scott D. Butzke**, Littleton, CO (US)

(51) **Int. Cl.⁷** **C02F 1/38**
(52) **U.S. Cl.** **210/782**

(57) **ABSTRACT**

Methods and apparatus particularly involving the separation of blood into blood components and the collection of such components are disclosed. In one aspect, an extracorporeal method for the collection of plasma and red blood cells is provided, wherein the collection of plasma and red blood cells may occur simultaneously or subsequently utilizing the same dual stage blood processing vessel. The flow of blood to the blood processing vessel and return of uncollected blood components may be provided via a single needle, wherein blood is removed from and returned to a donor/patient during alternating blood removal and blood return submodes. Platelet separation and collection options are also described. In either case, prior to red blood cell collection, a set-up phase may be carried out to set a predetermined hematocrit and AC ratio. Replacement fluid delivery may optionally also be provided either substantially continuously during any collection phase(s) and/or in a bolus mode.

Correspondence Address:
GAMBRO, INC
PATENT DEPARTMENT
10810 W COLLINS AVE
LAKEWOOD, CO 80215 (US)

(21) Appl. No.: **09/803,304**
(22) Filed: **Mar. 9, 2001**

Related U.S. Application Data

(63) Non-provisional of provisional application No. 60/188,133, filed on Mar. 9, 2000.

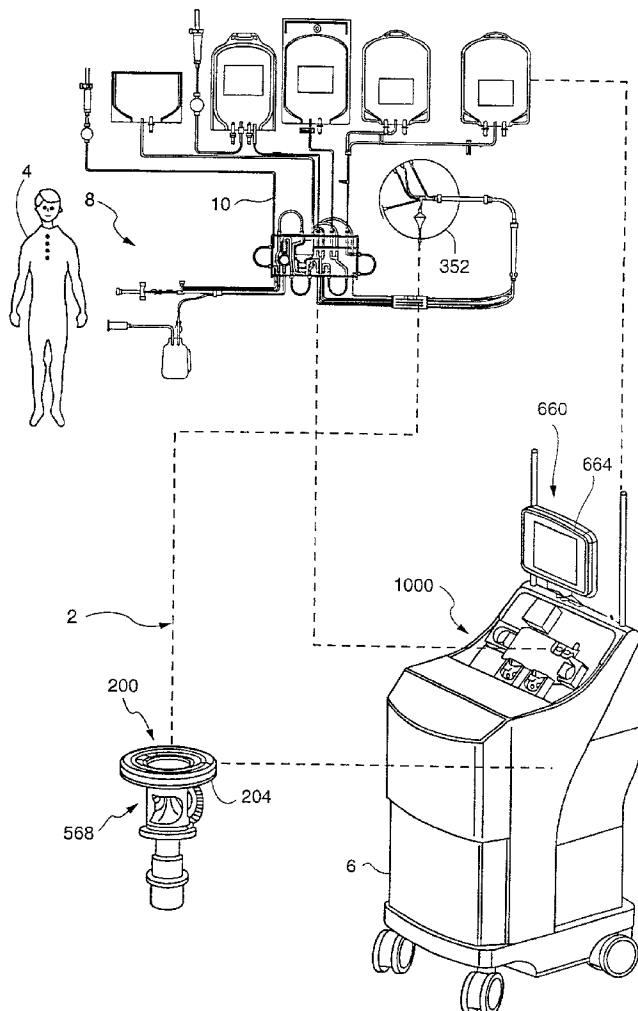
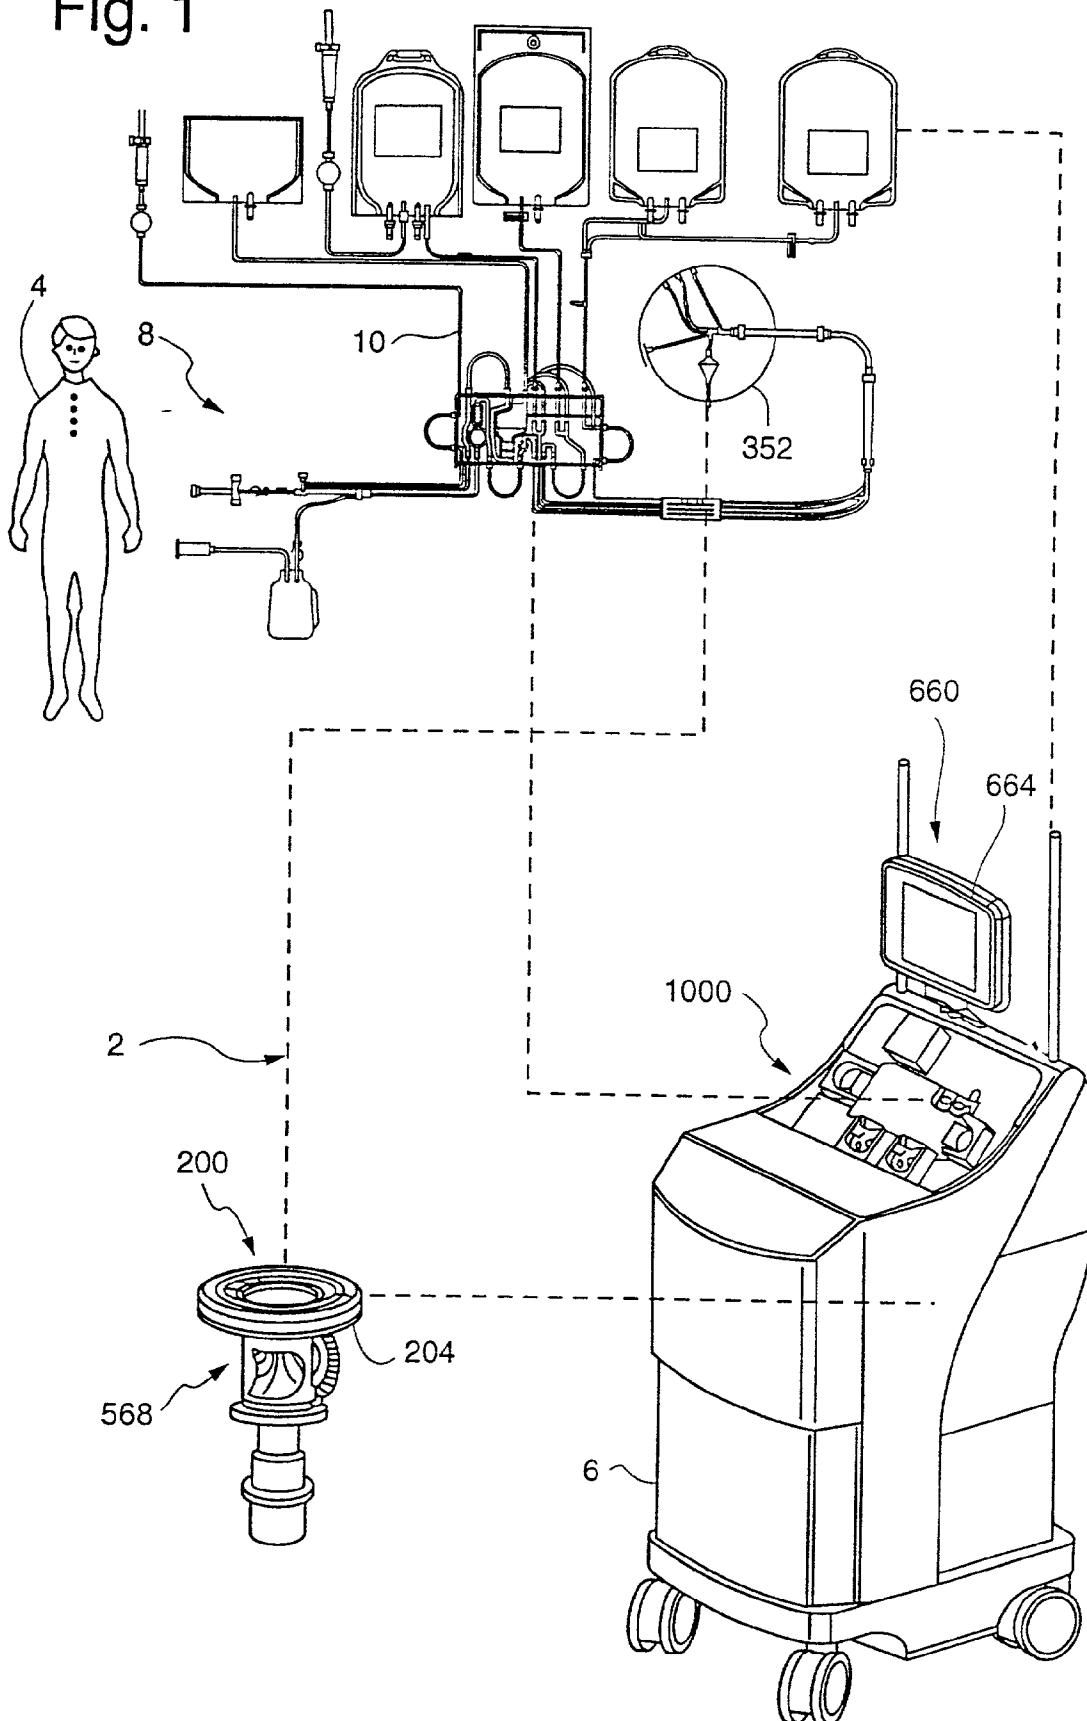
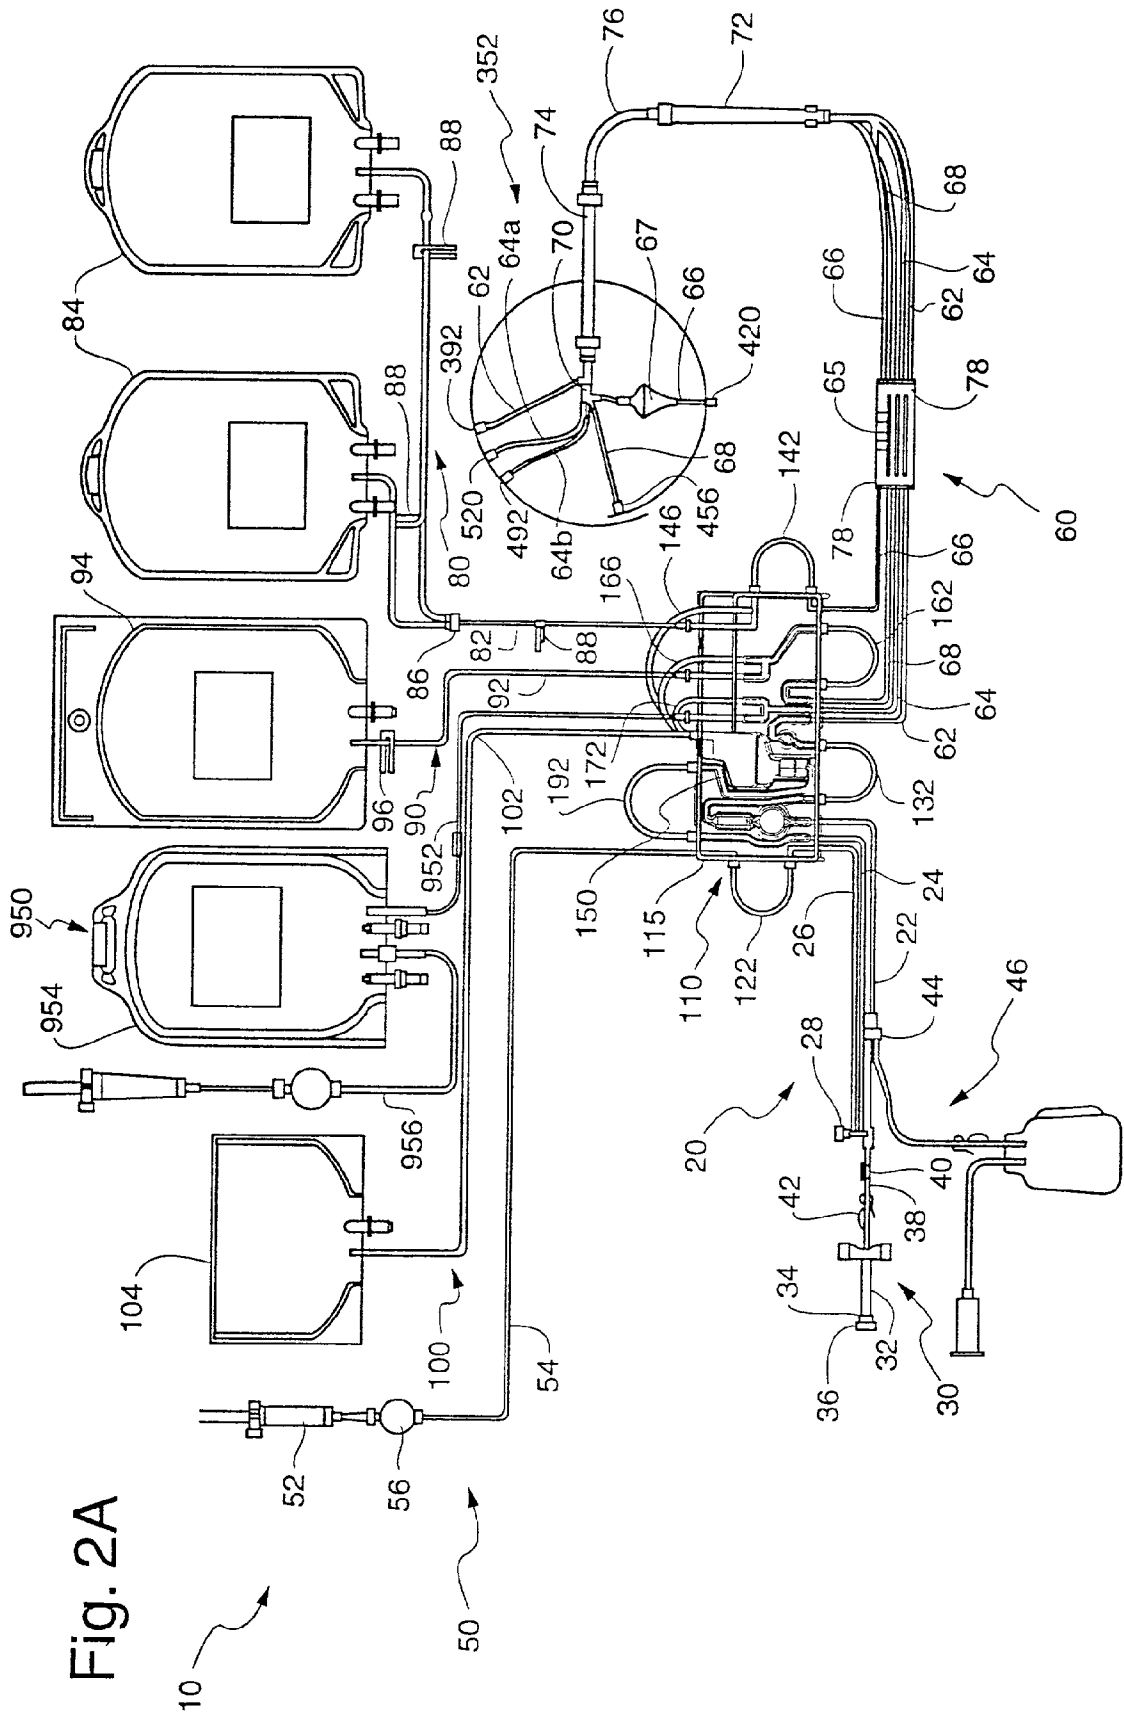


Fig. 1





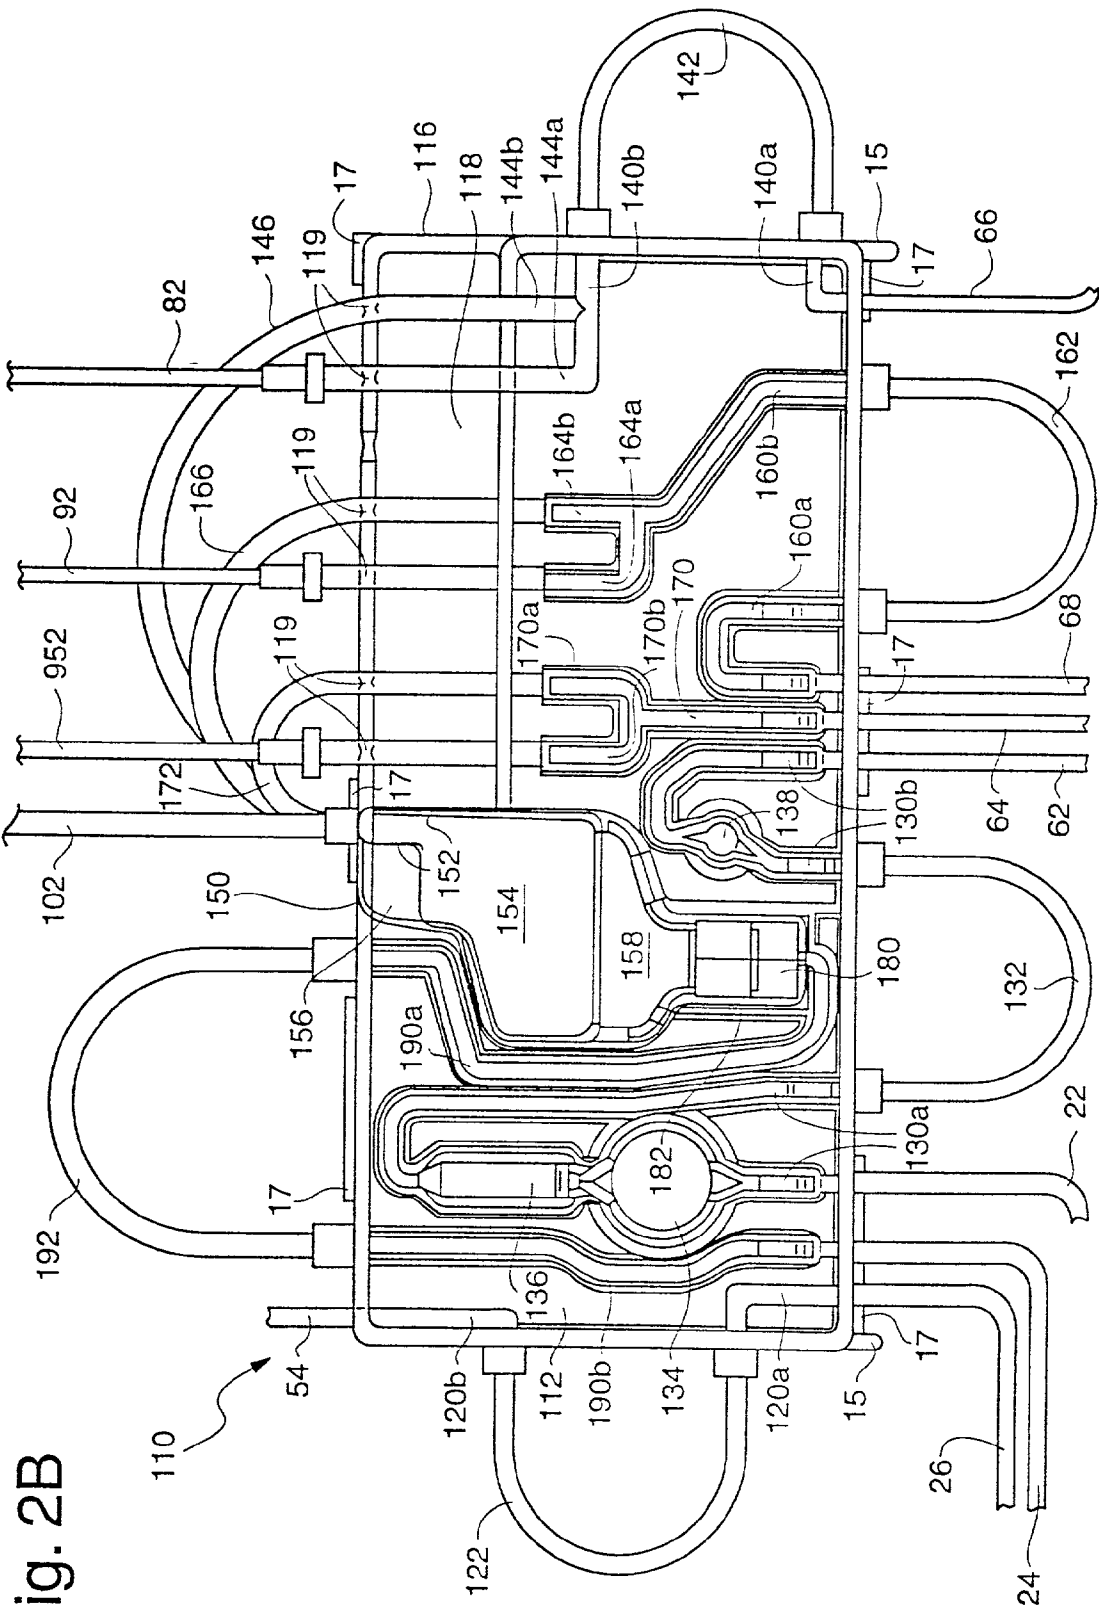


Fig. 2B

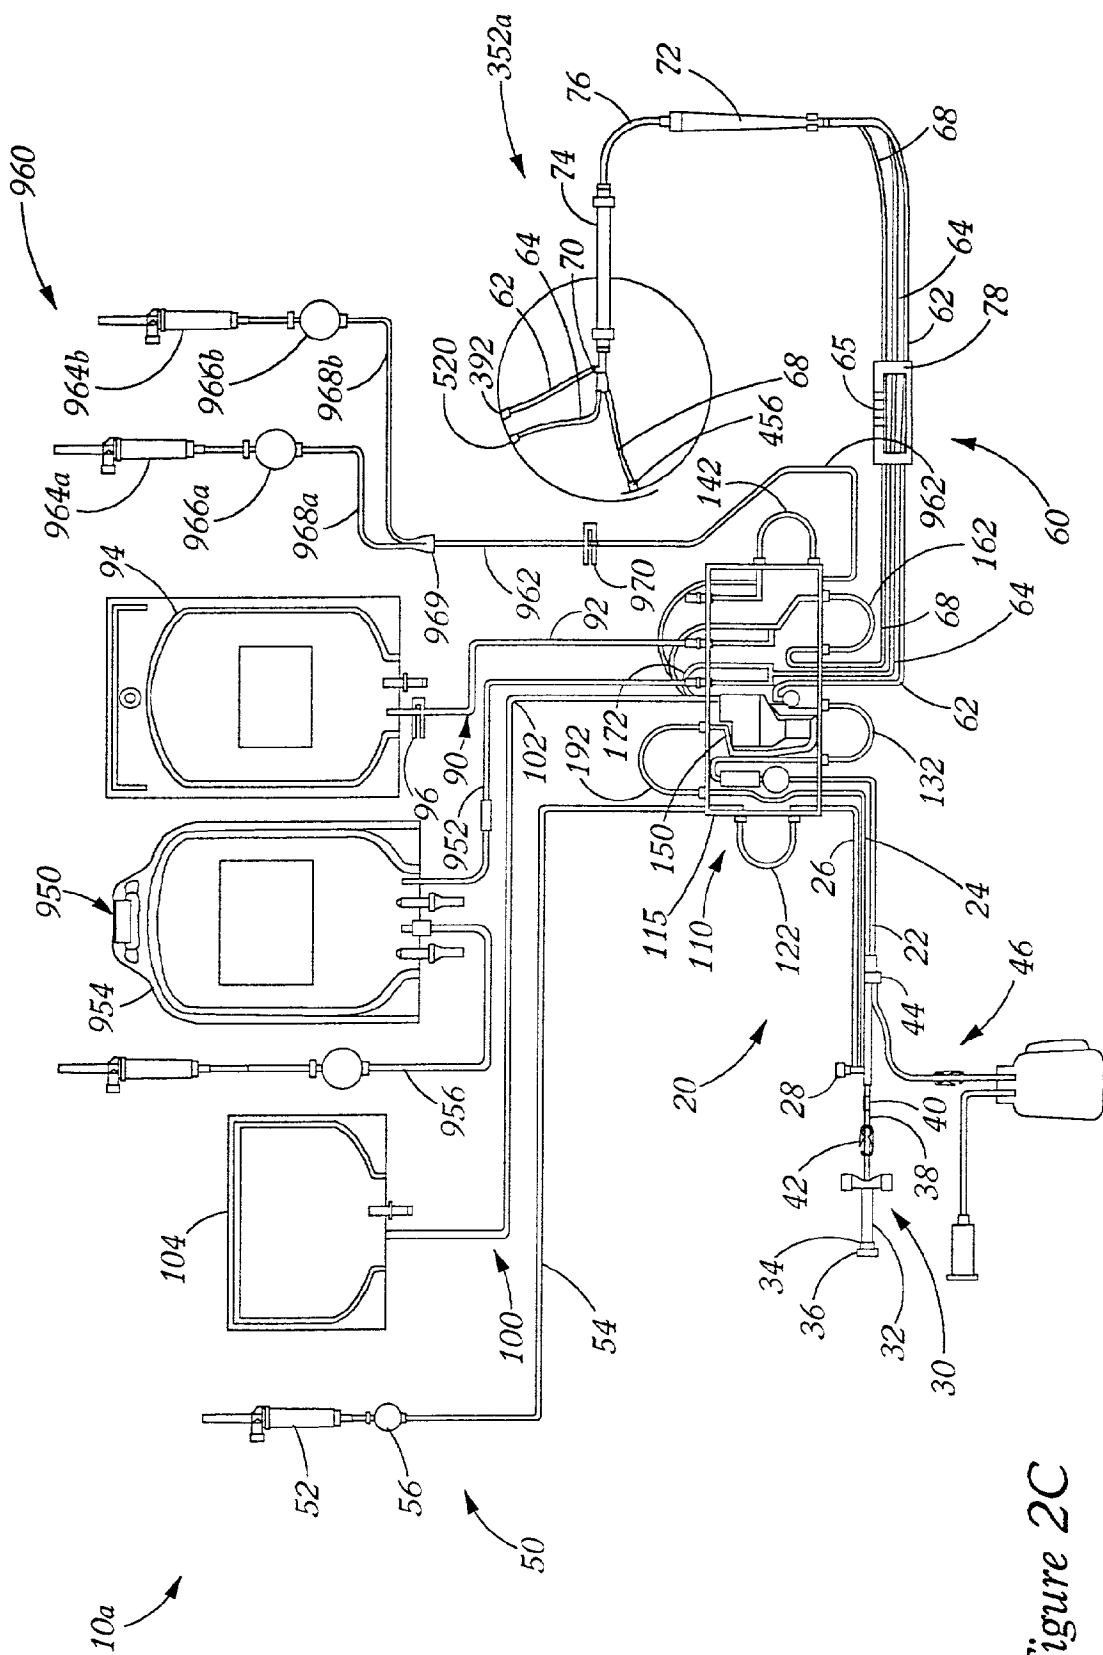
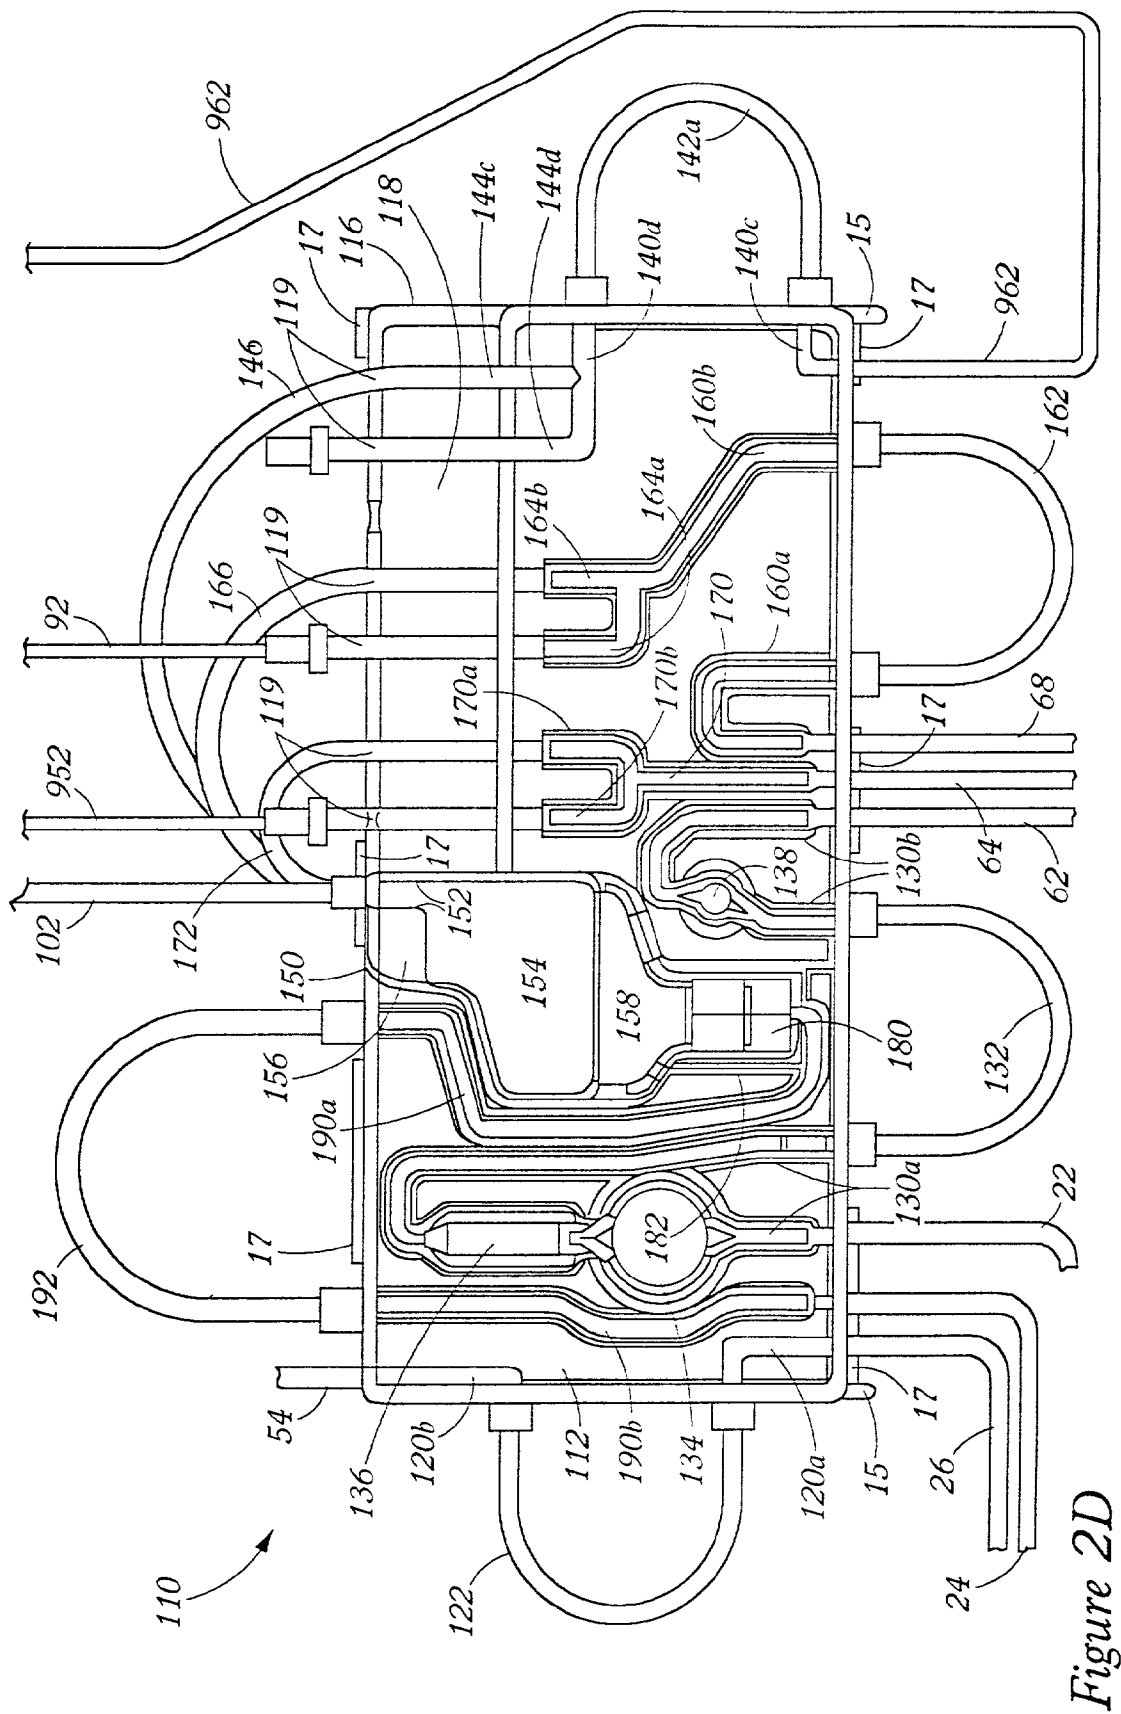
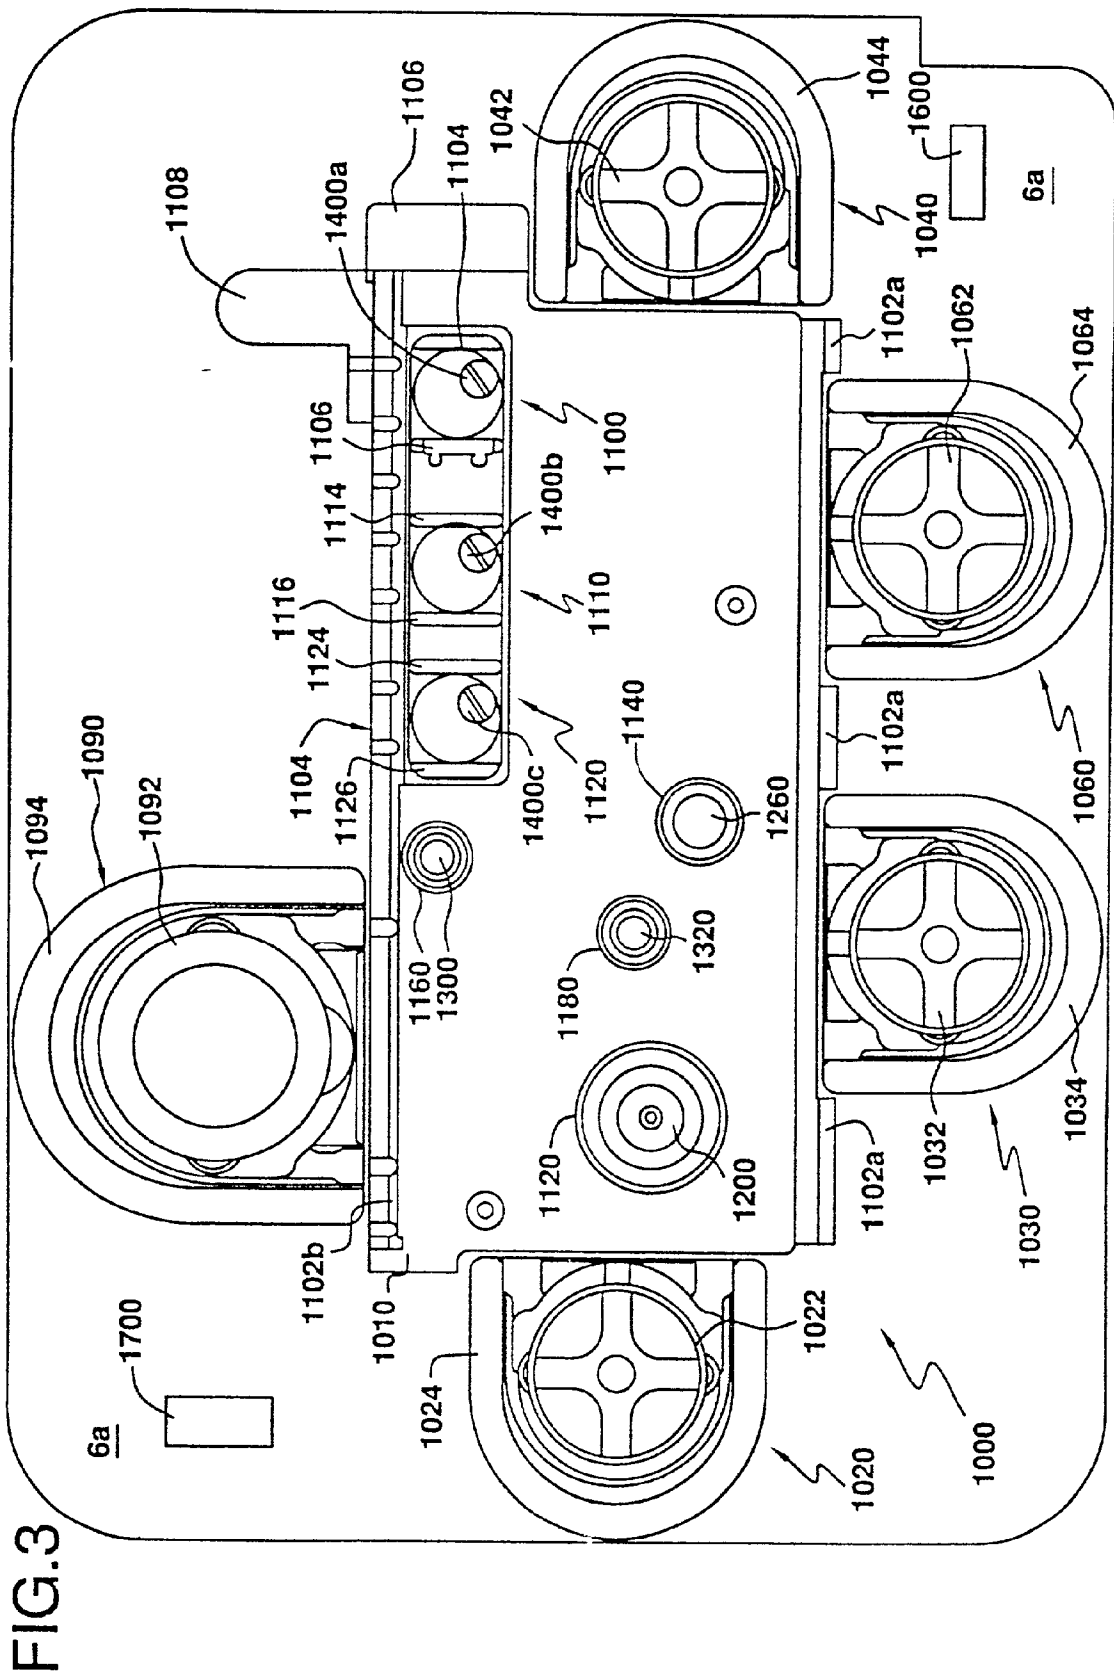


Figure 2C





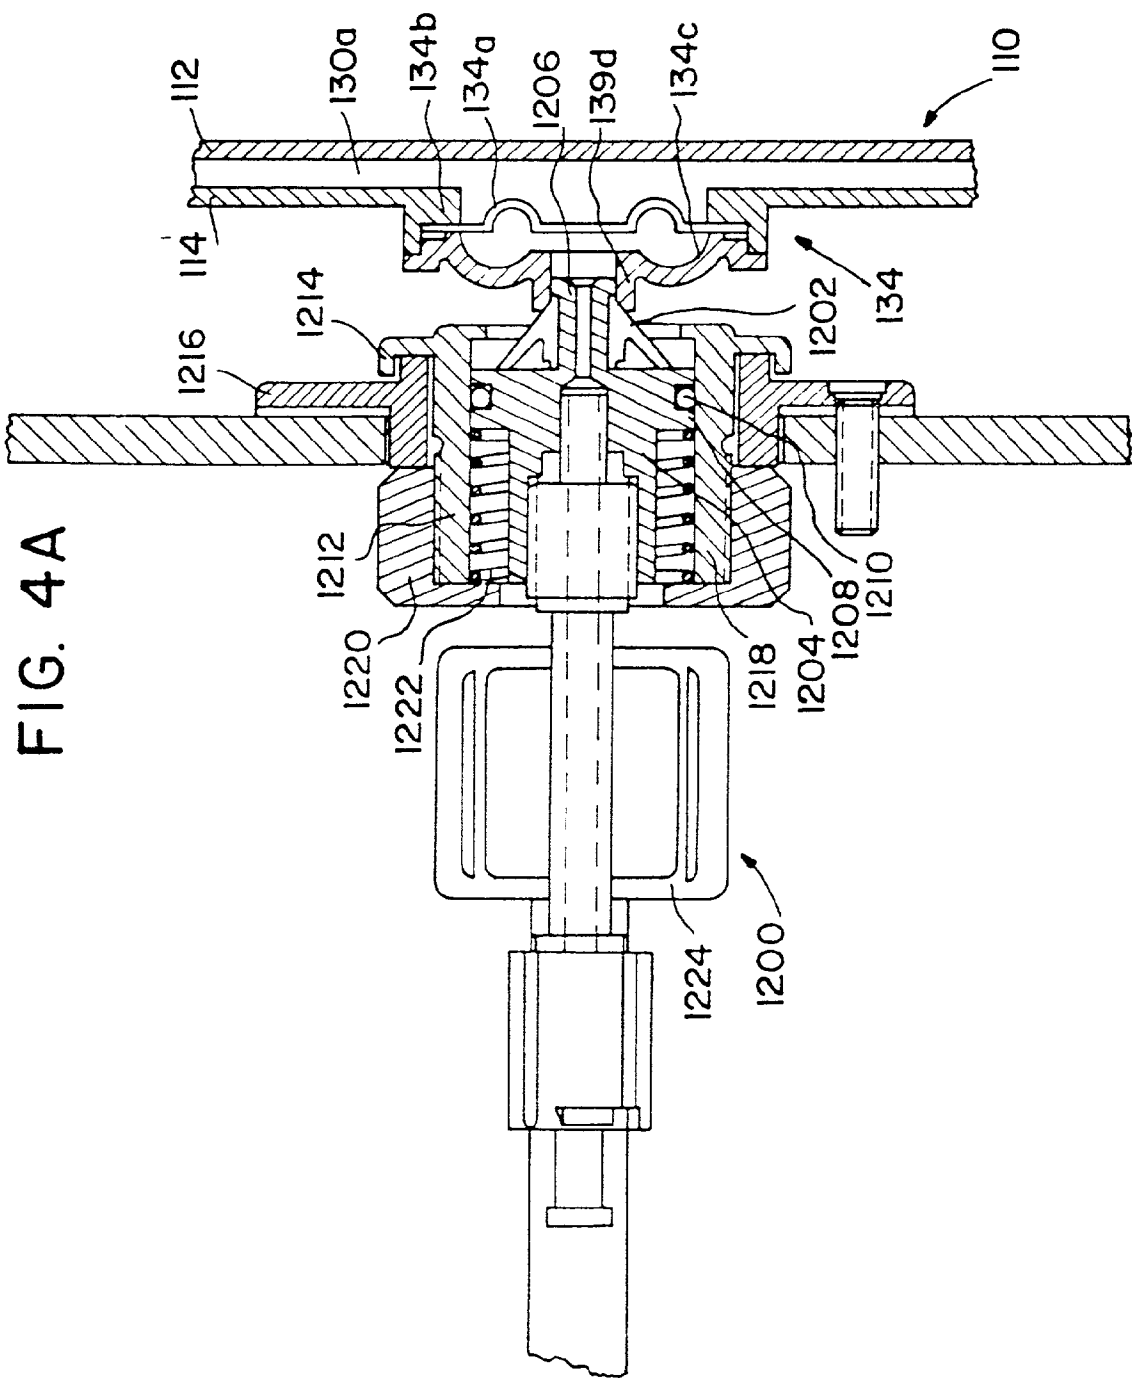
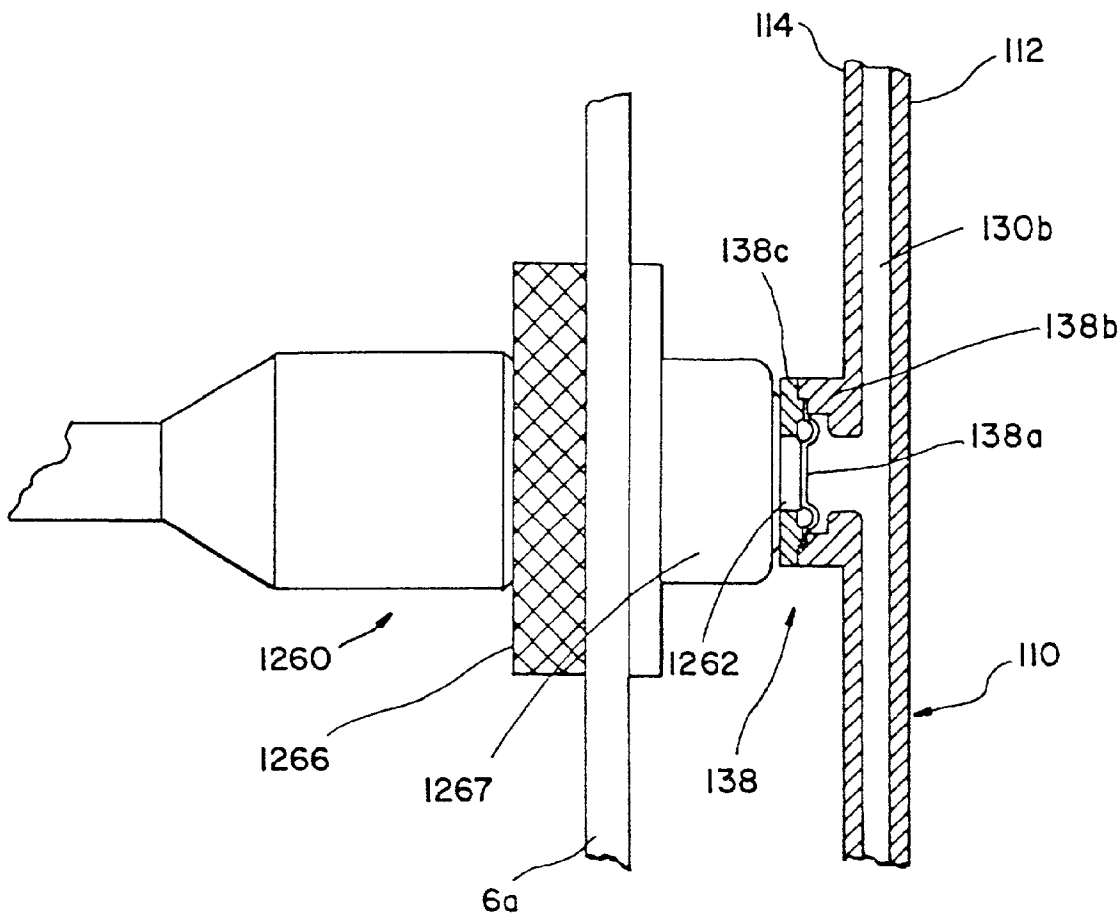


FIG.4B



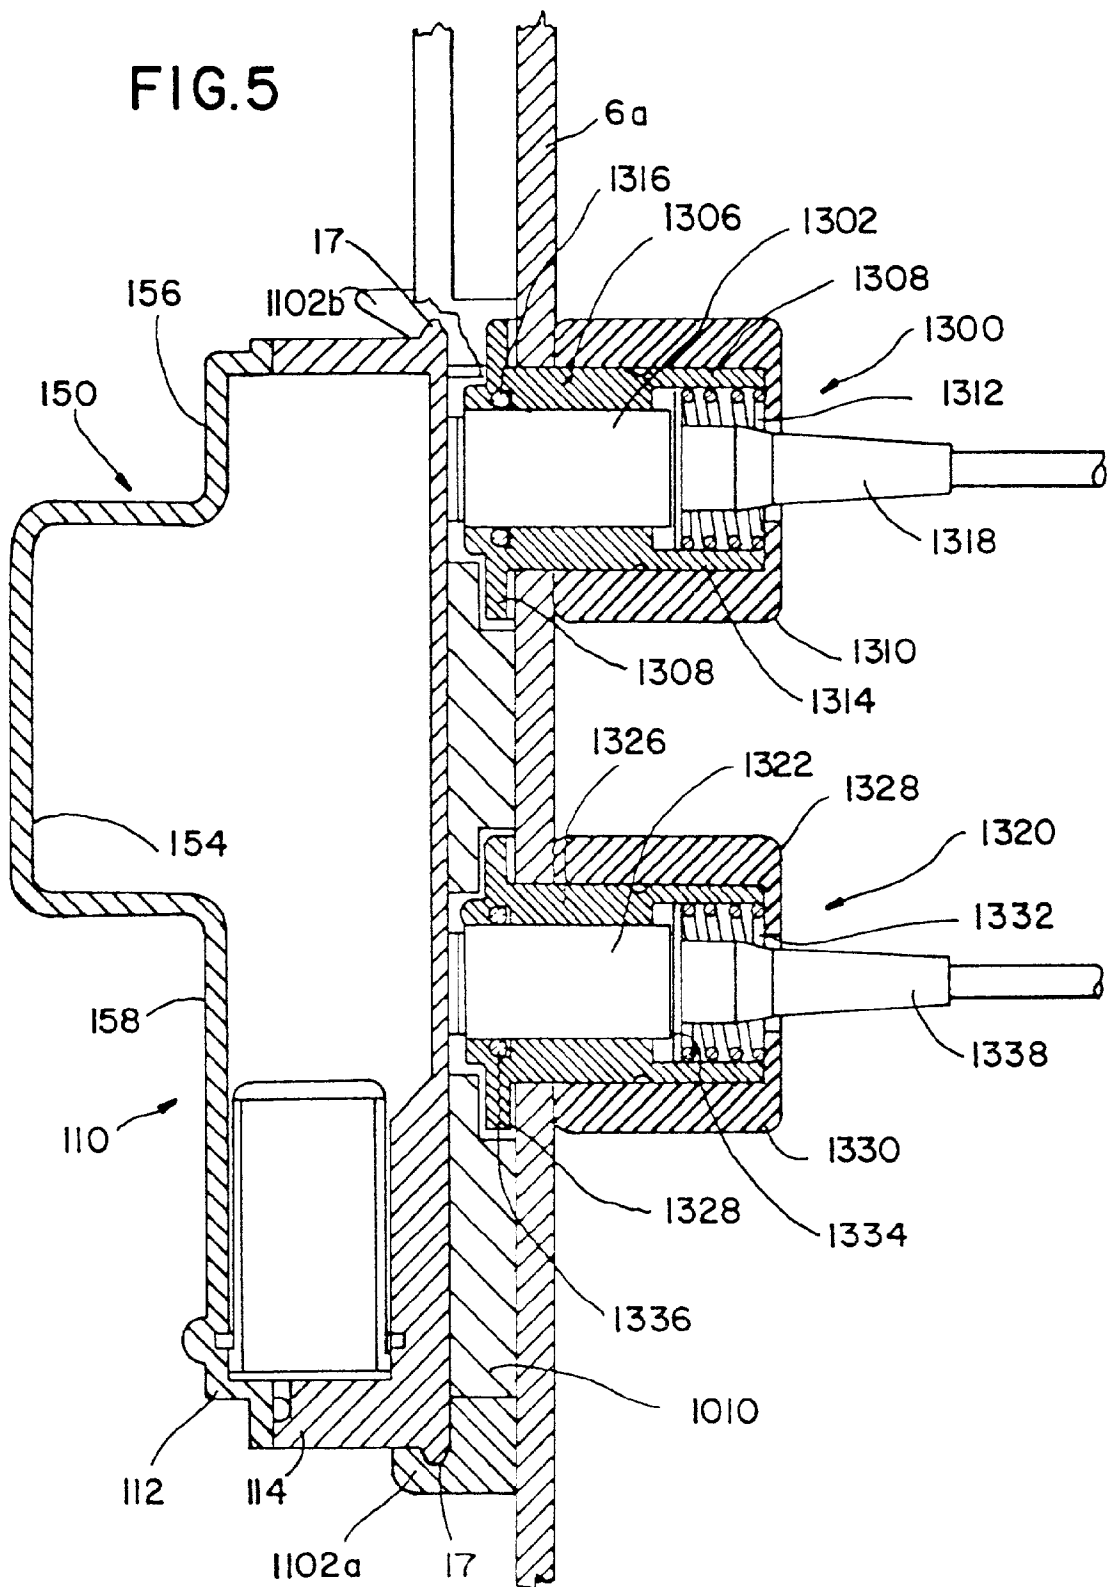
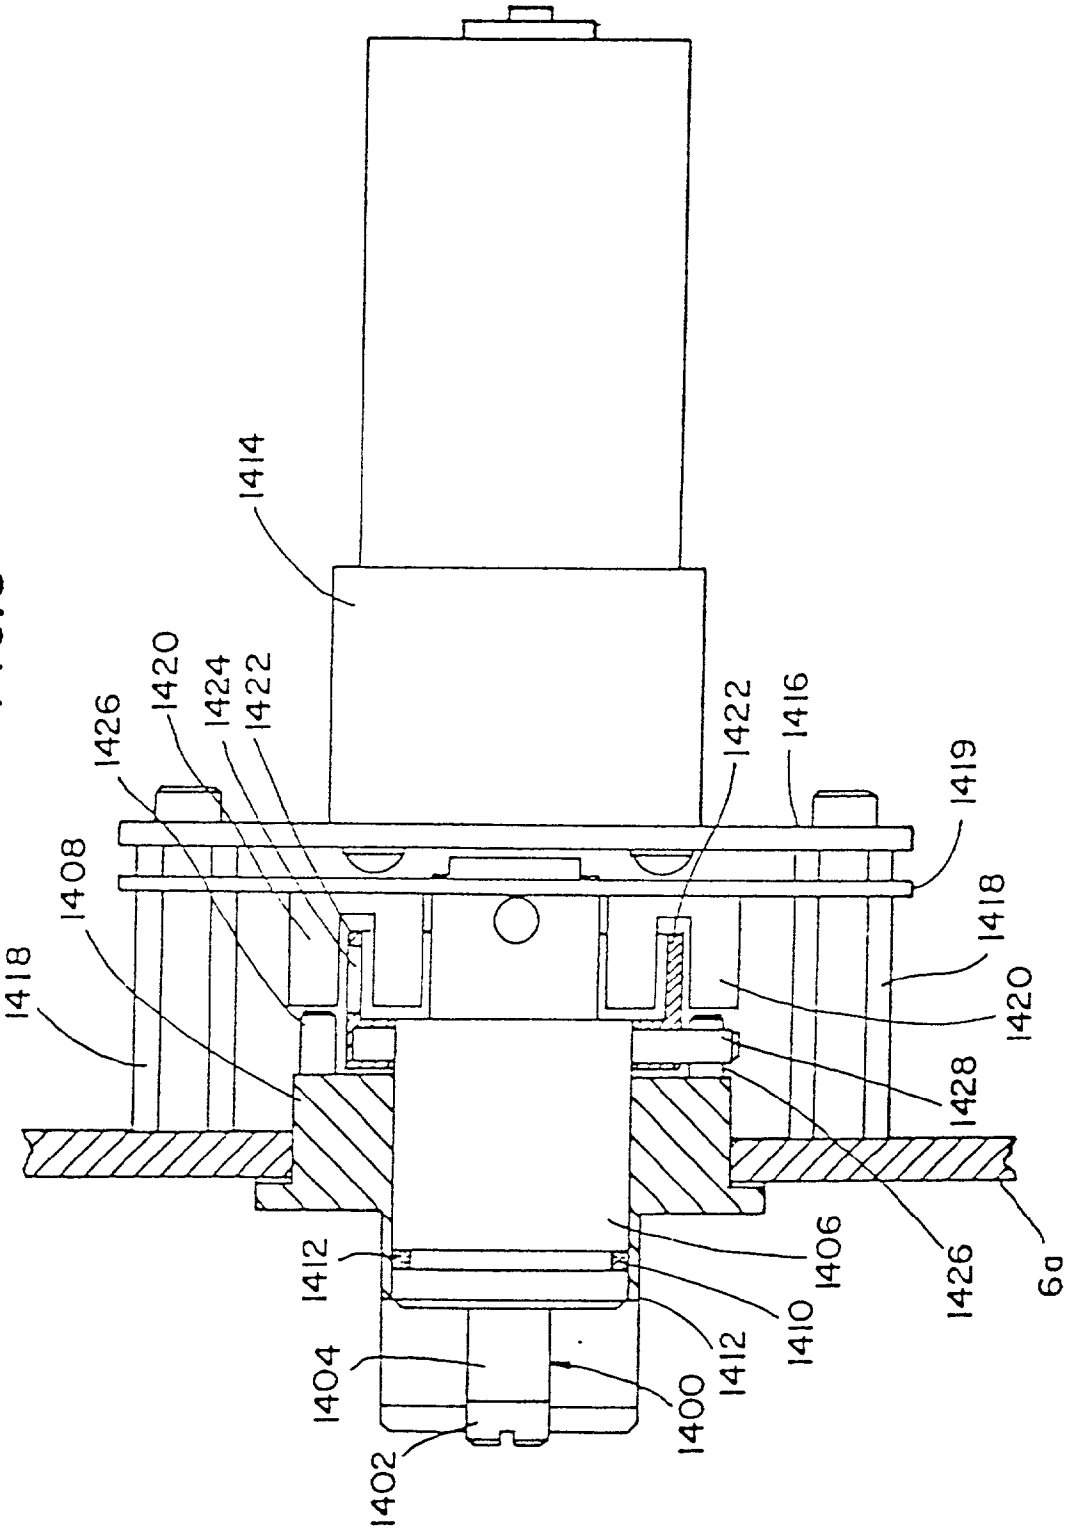
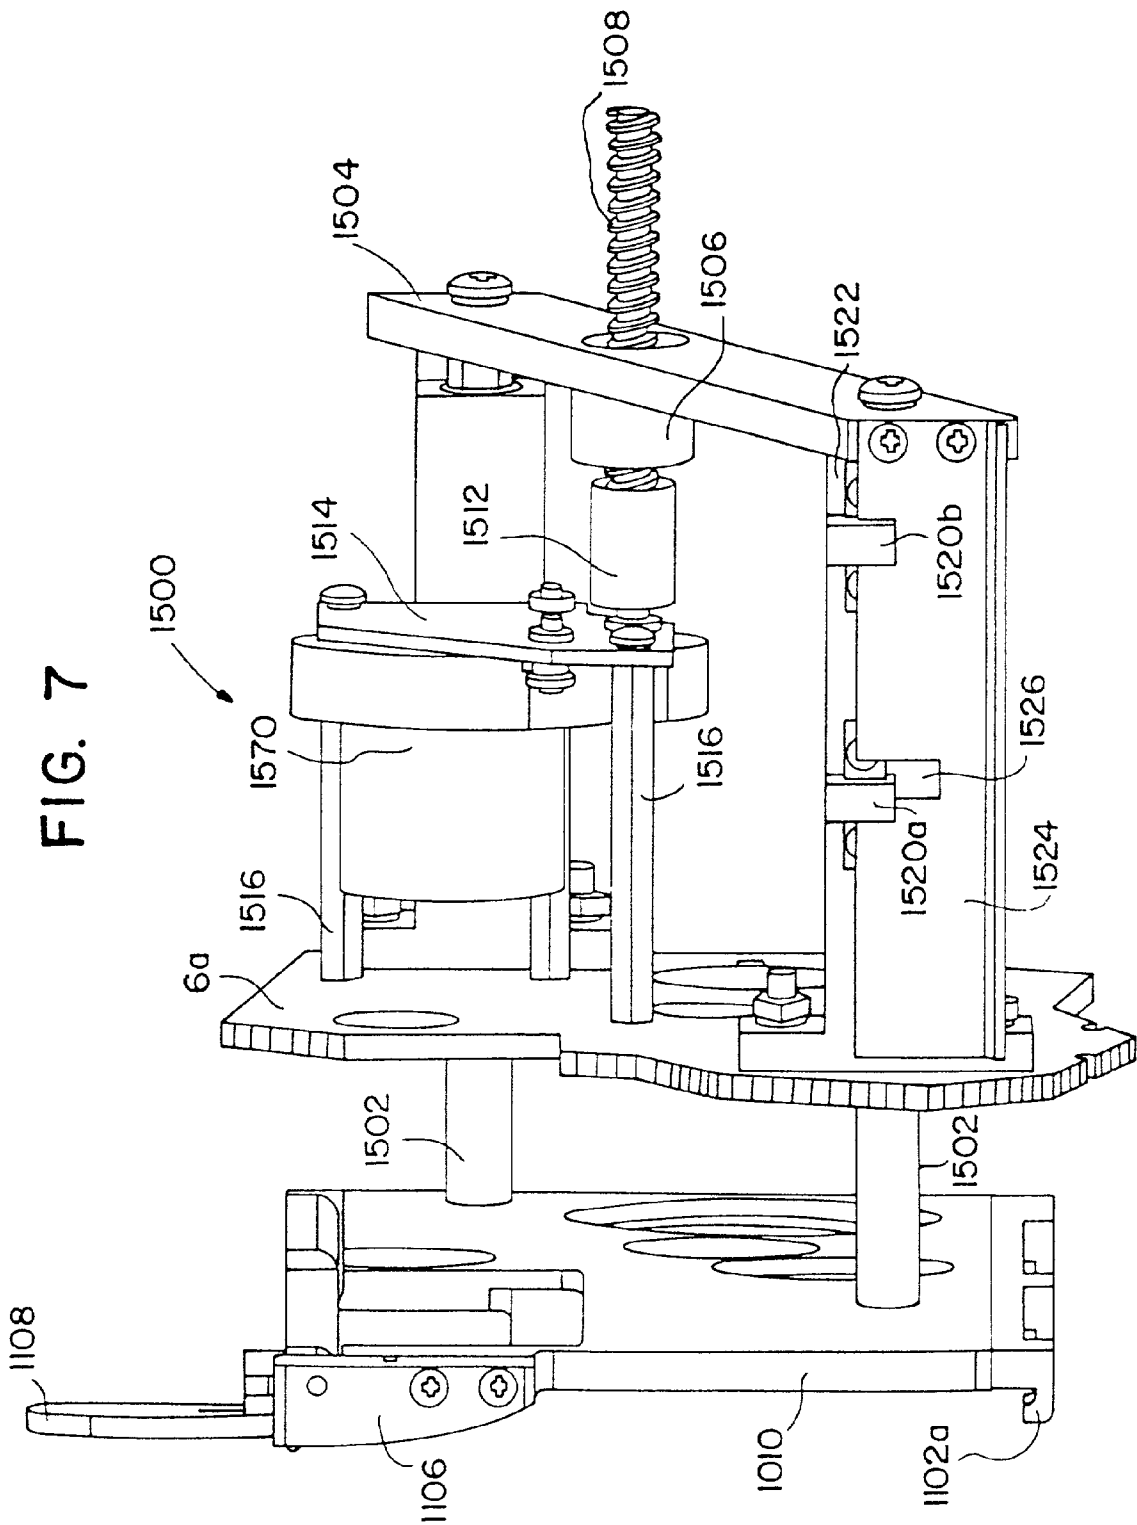


FIG. 6





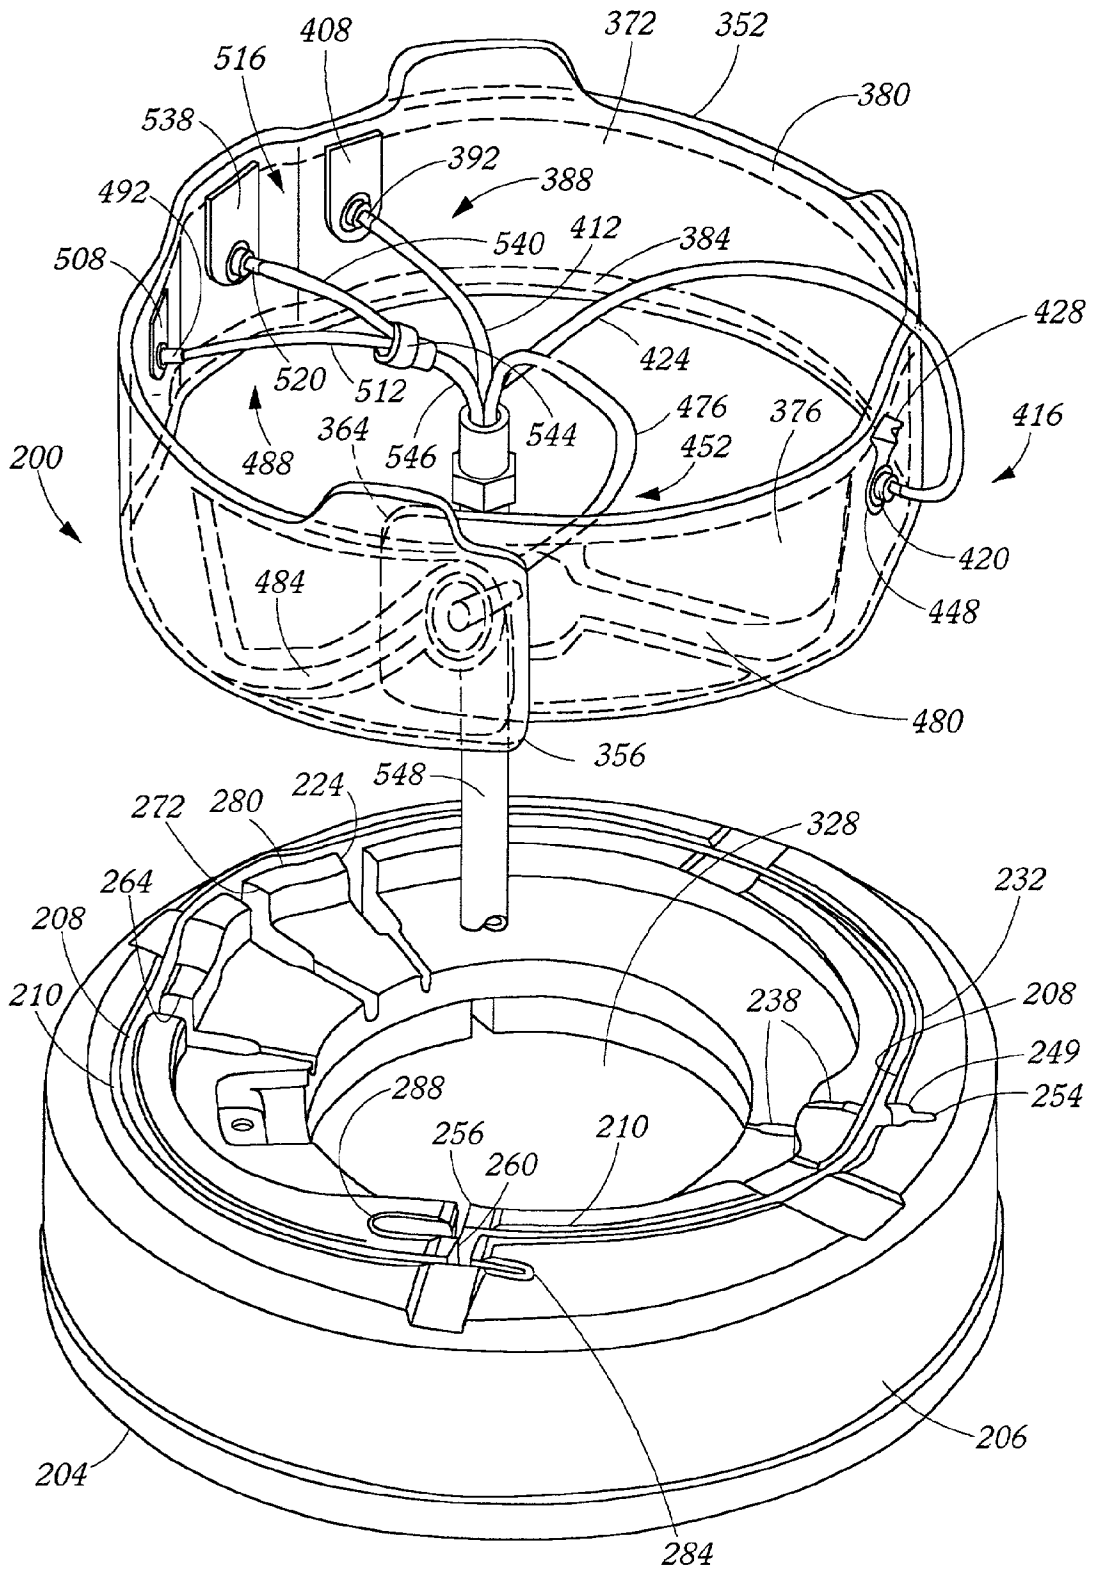


Figure 8A

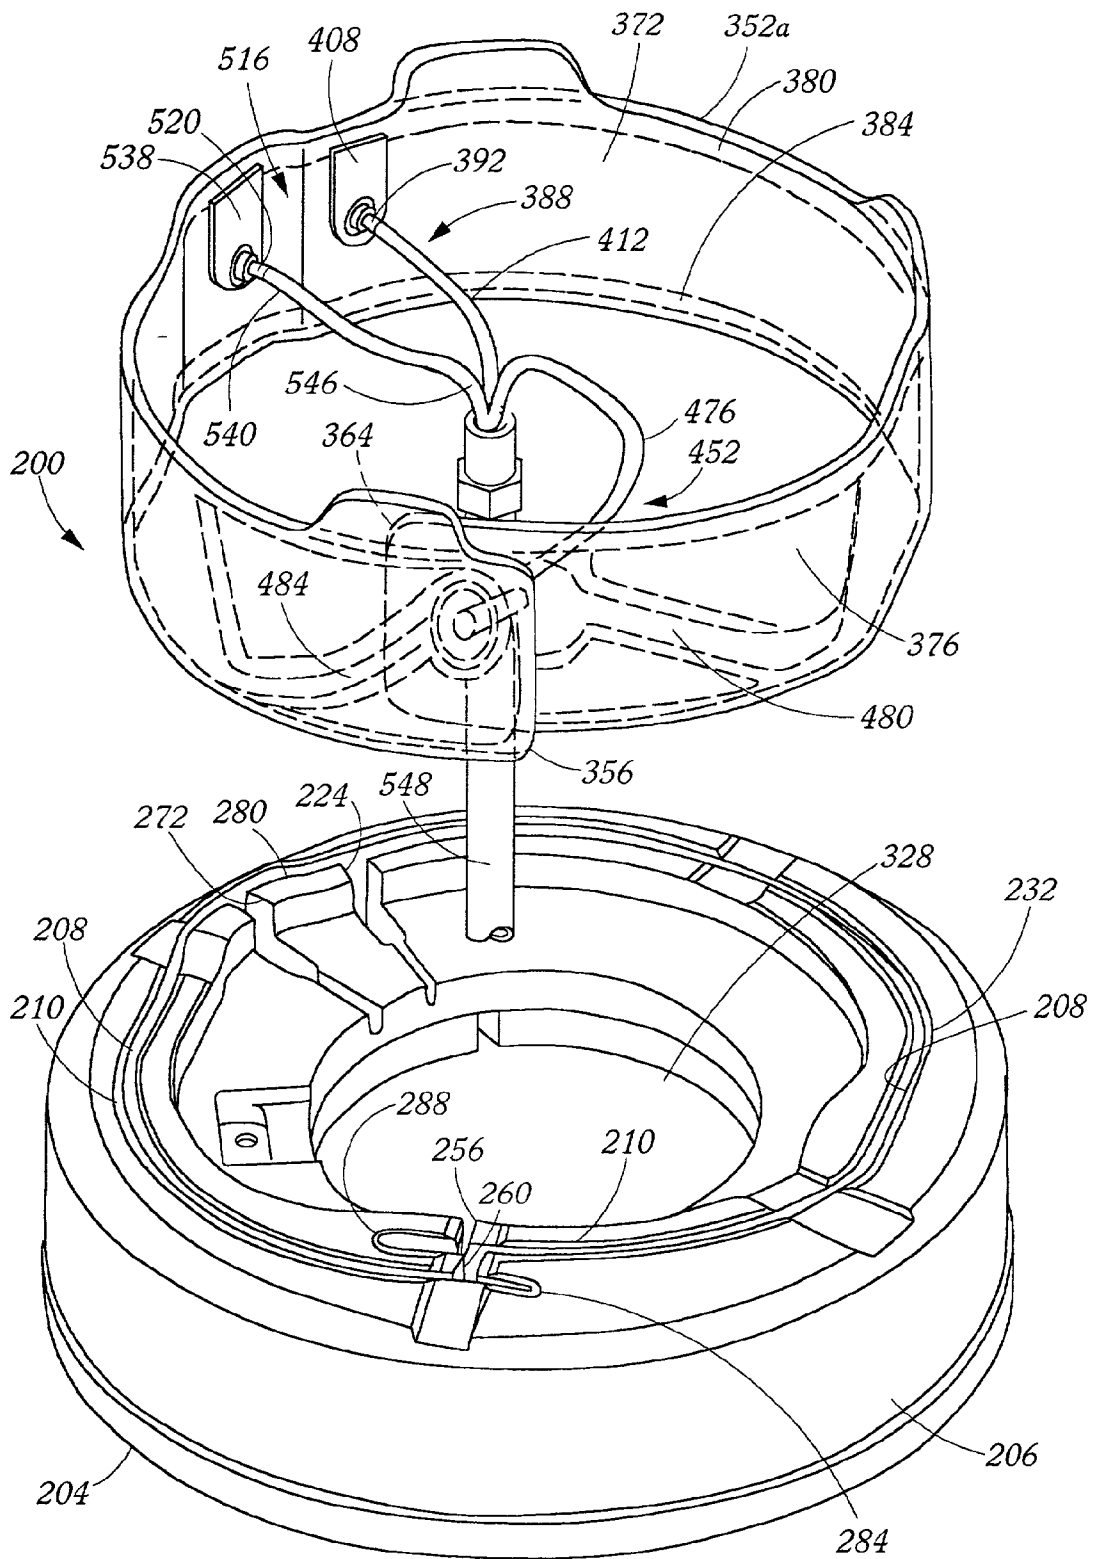
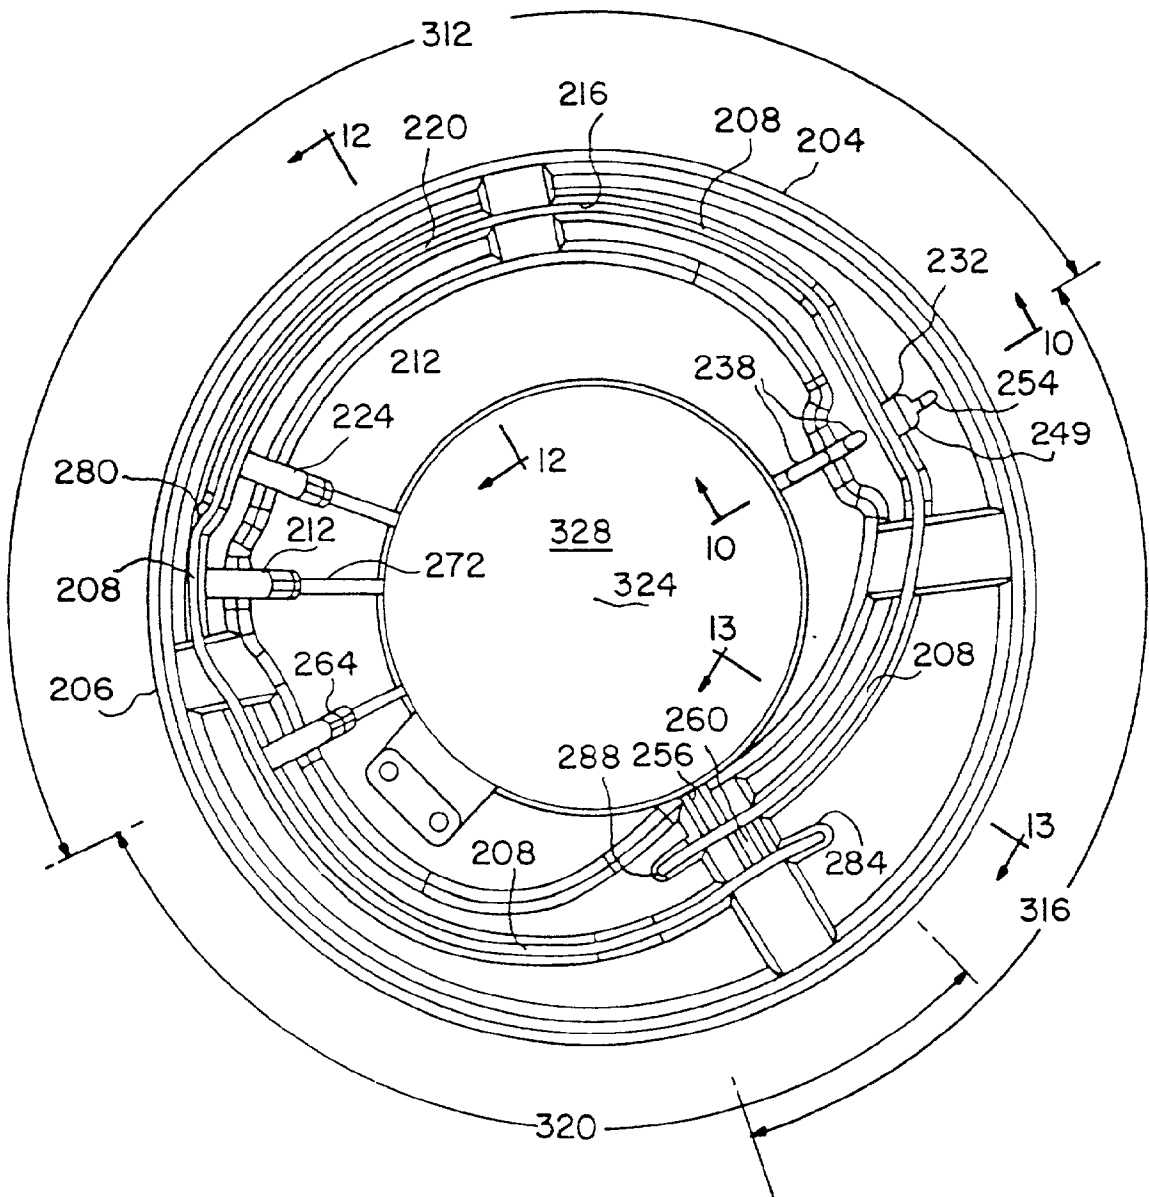


Figure 8B

FIG. 9A



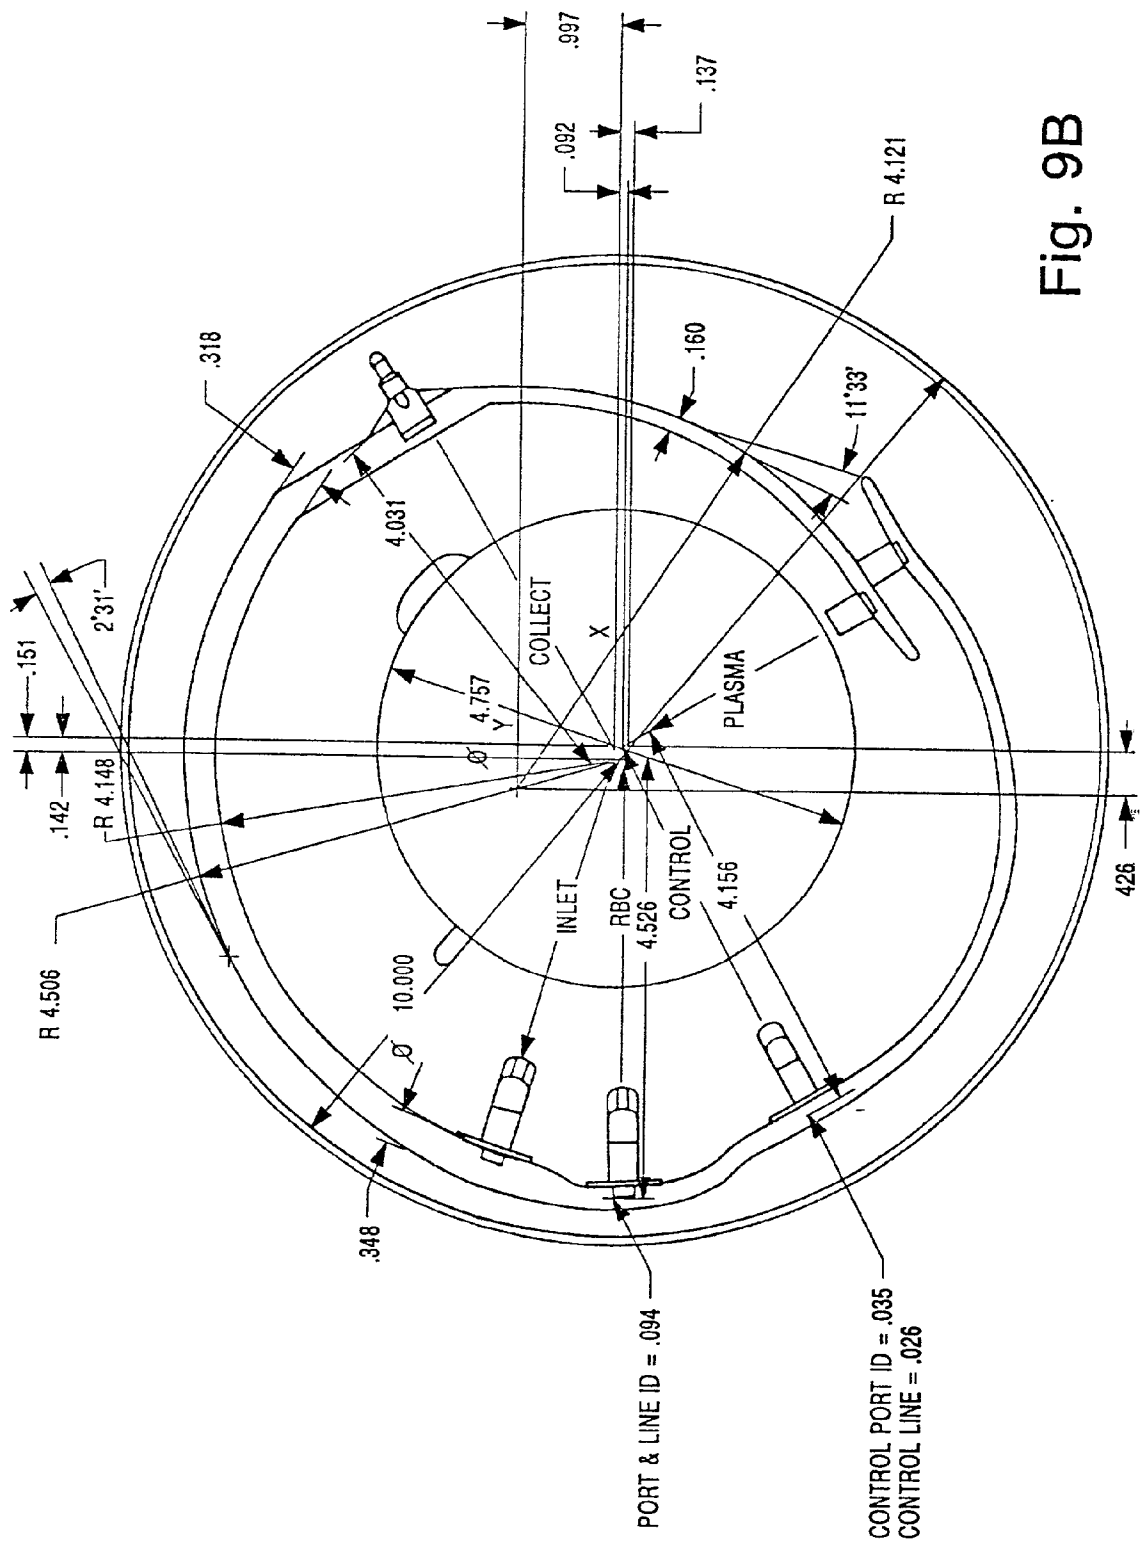


FIG.10

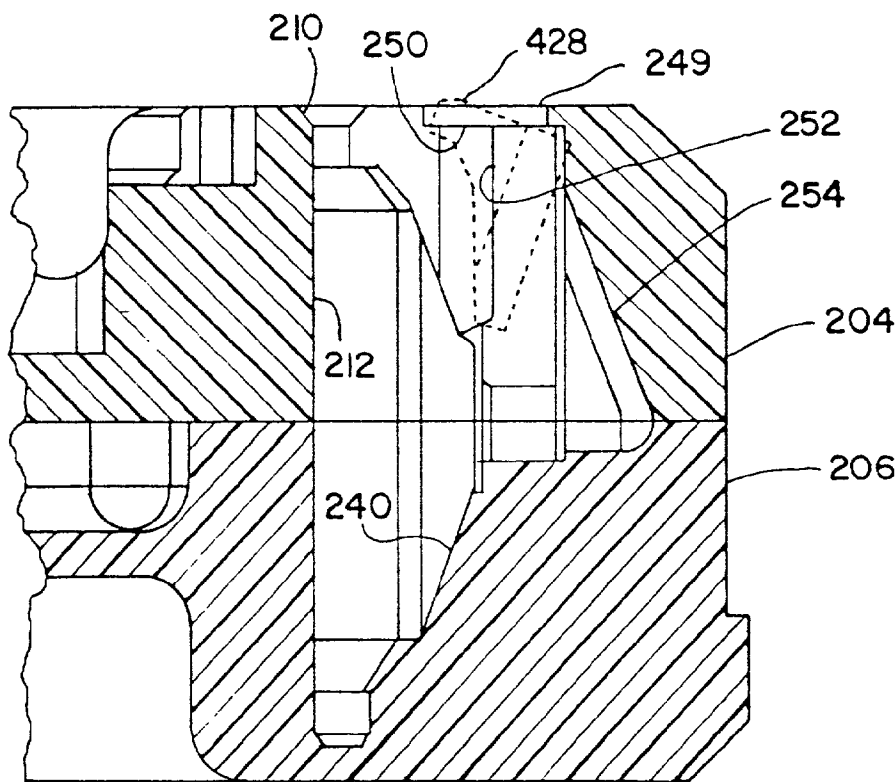


FIG. IIA

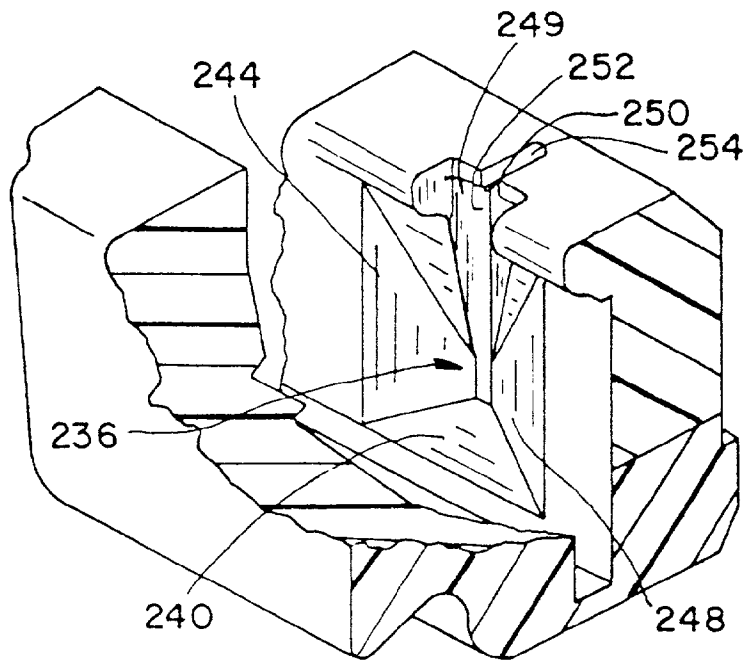


FIG. IIB

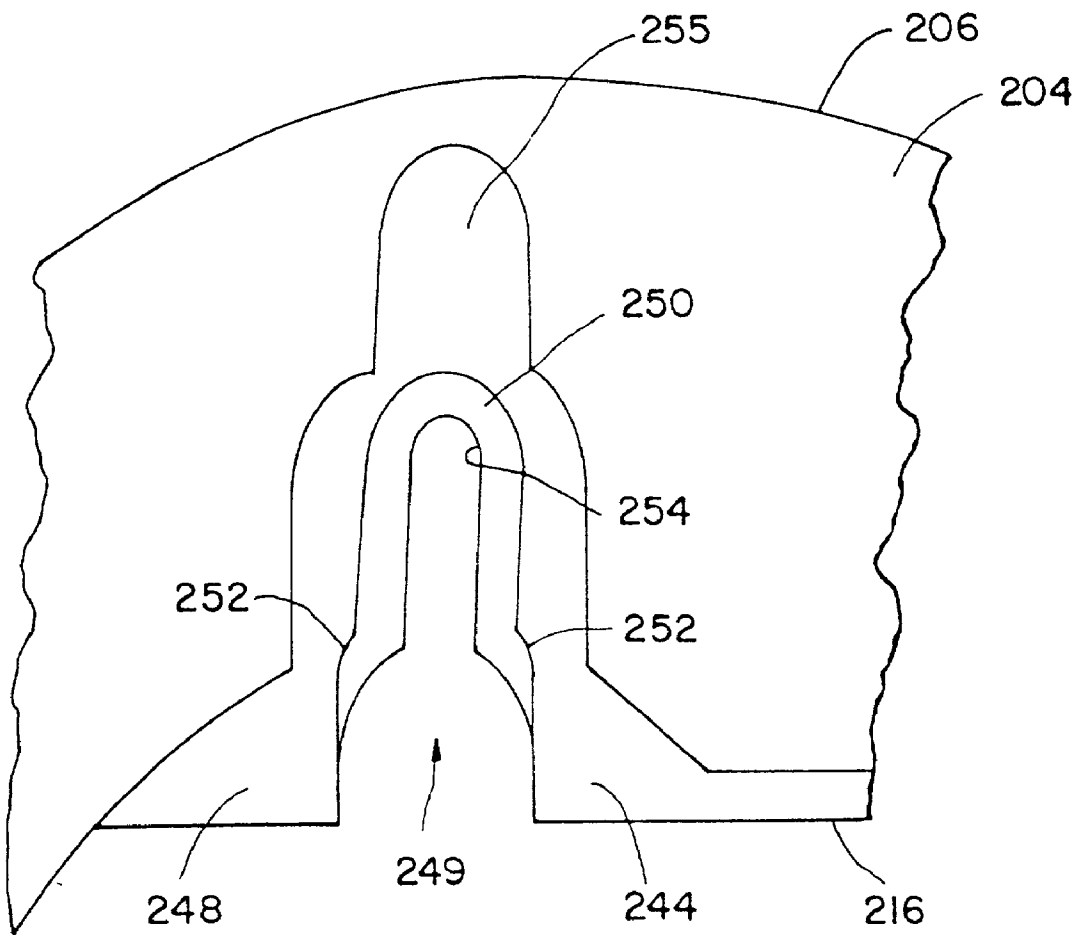


FIG.12

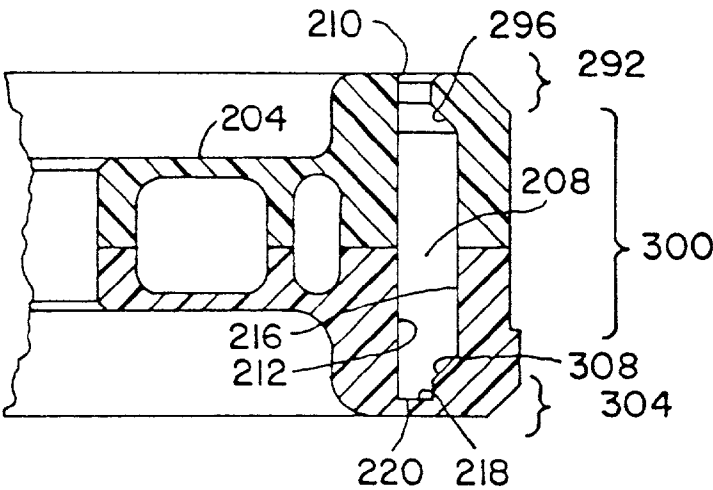


FIG.13

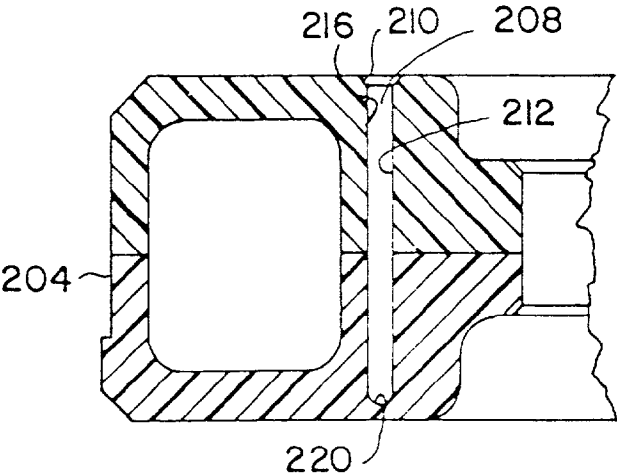


FIG.14C

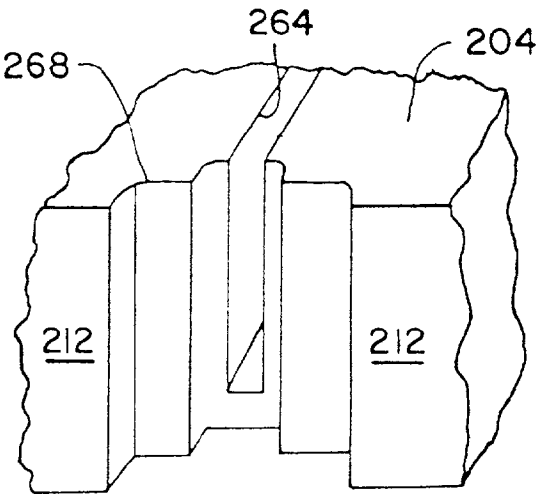


FIG. 14A

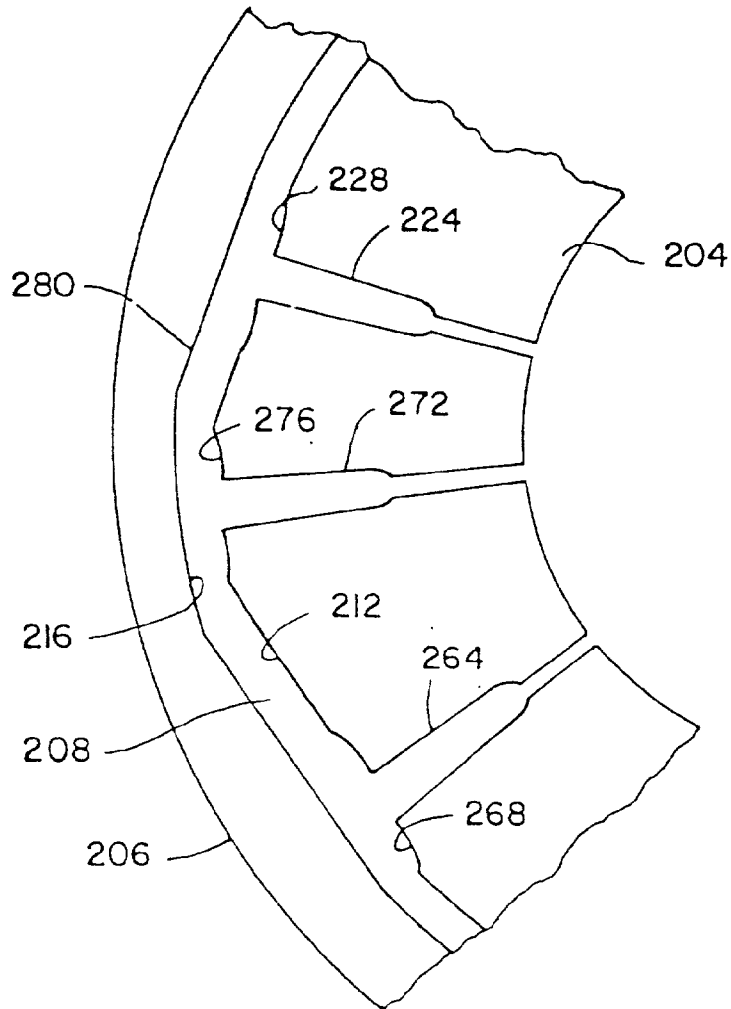


FIG. 14B

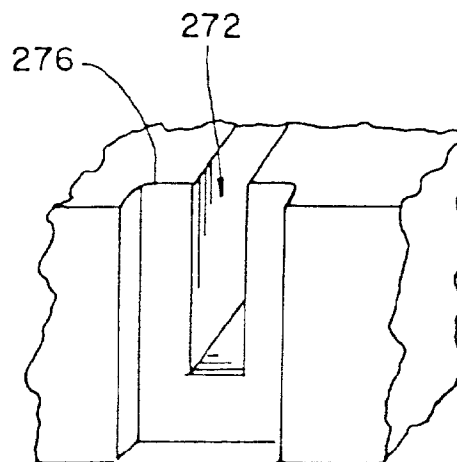
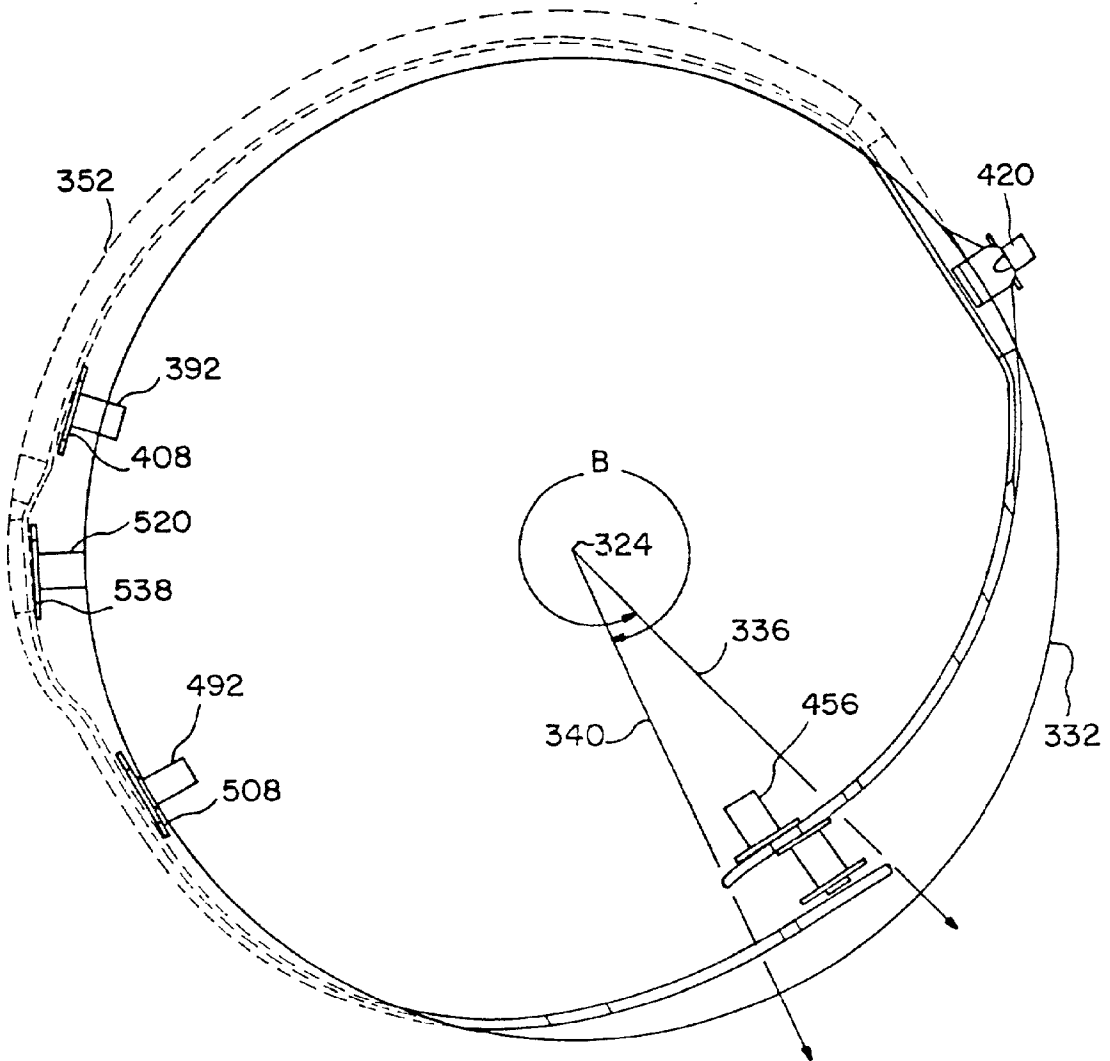


FIG. 15



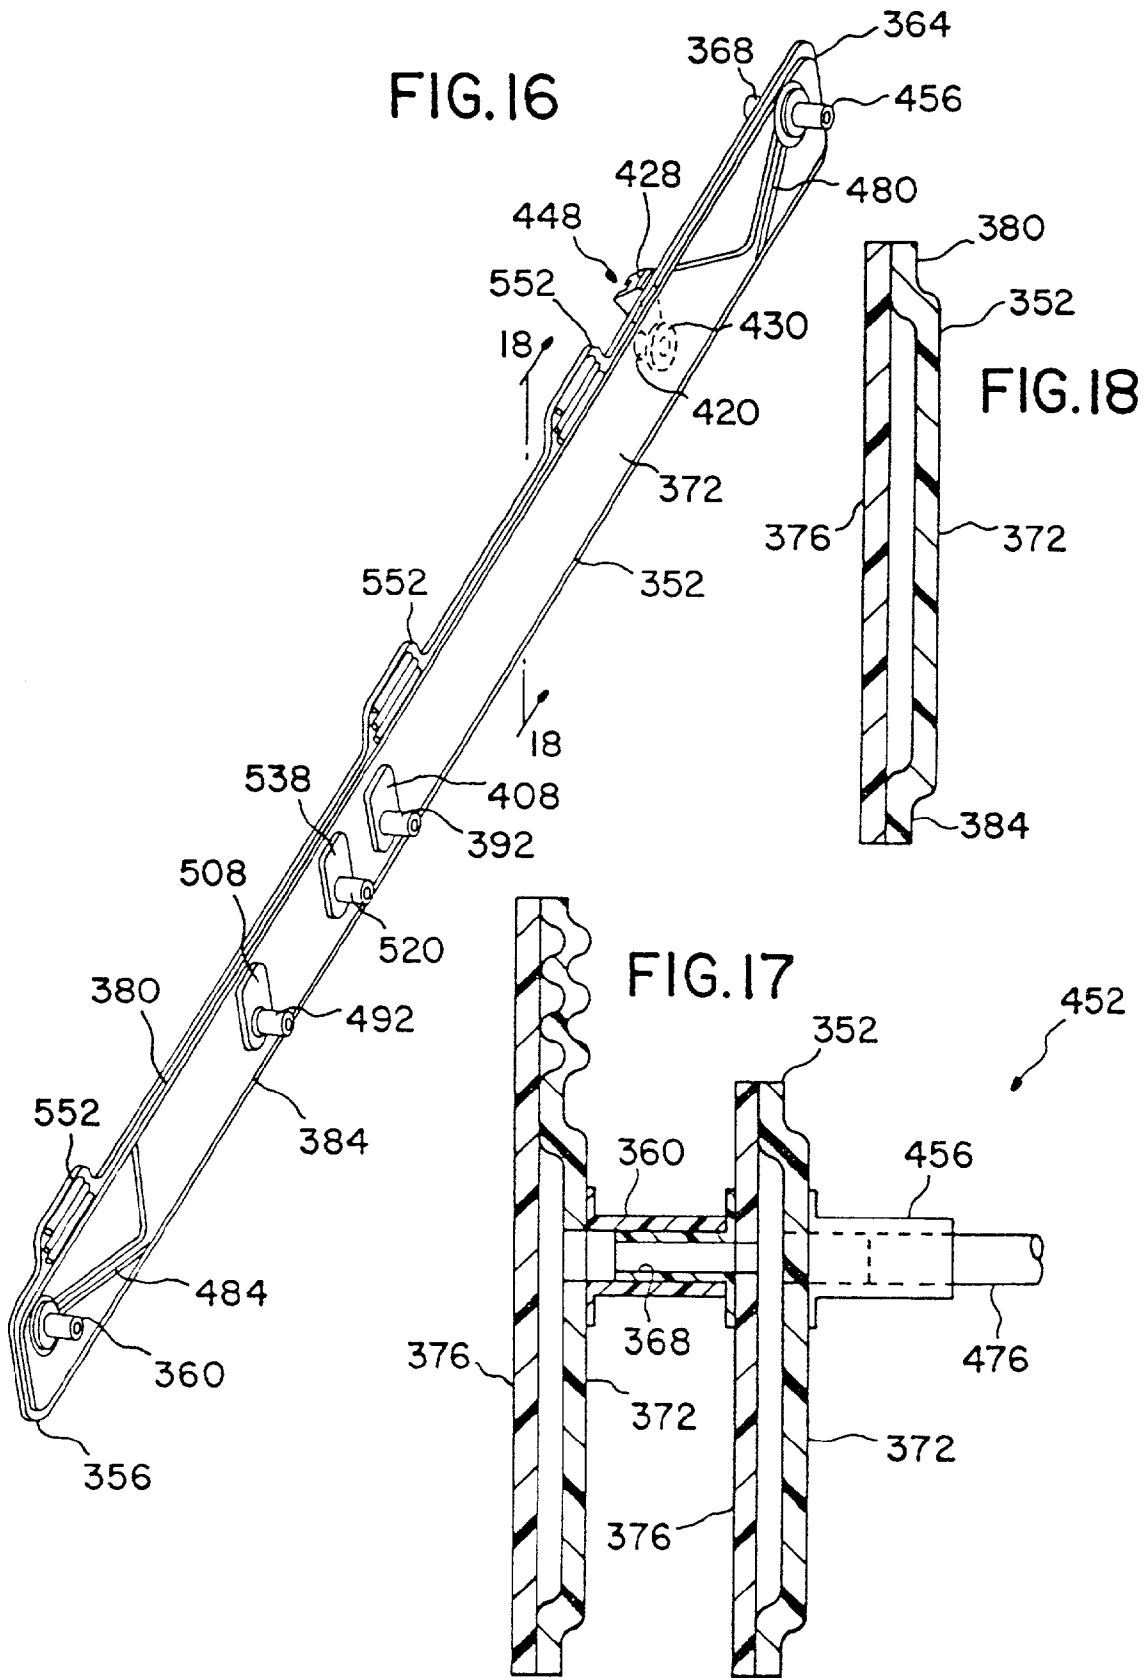


FIG. 19A

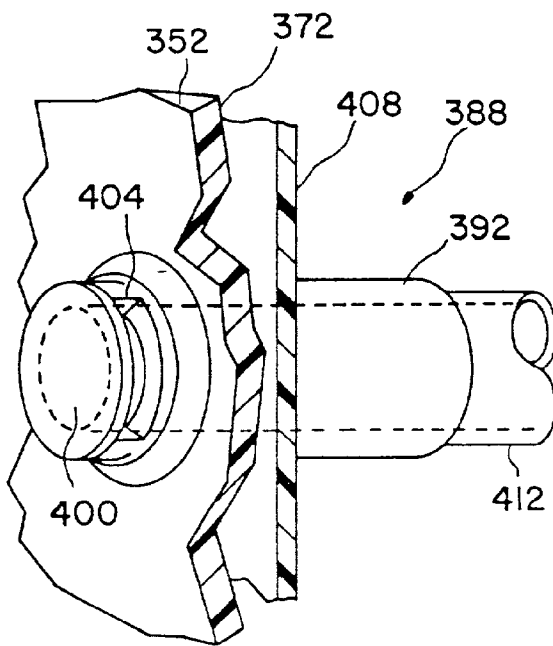


FIG. 19B

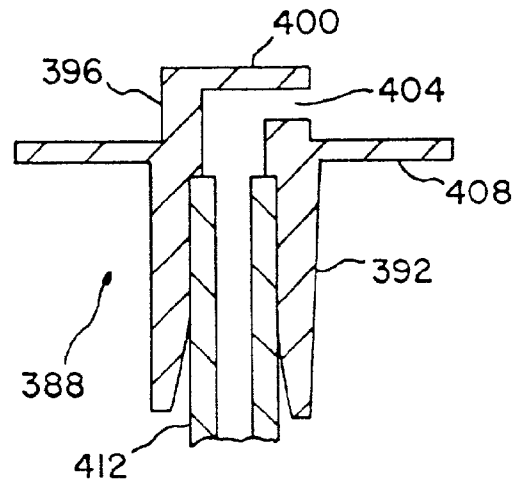


FIG. 19C

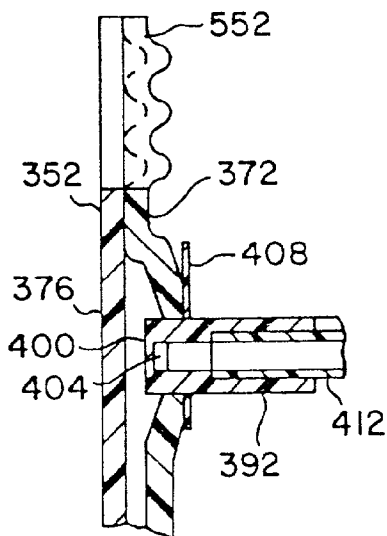


FIG. 19D

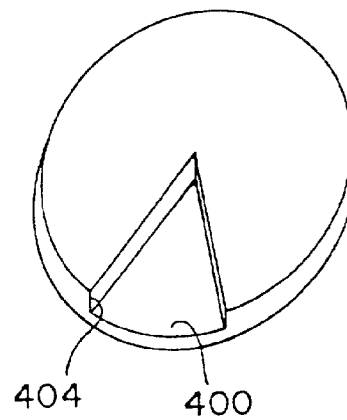


FIG. 19E

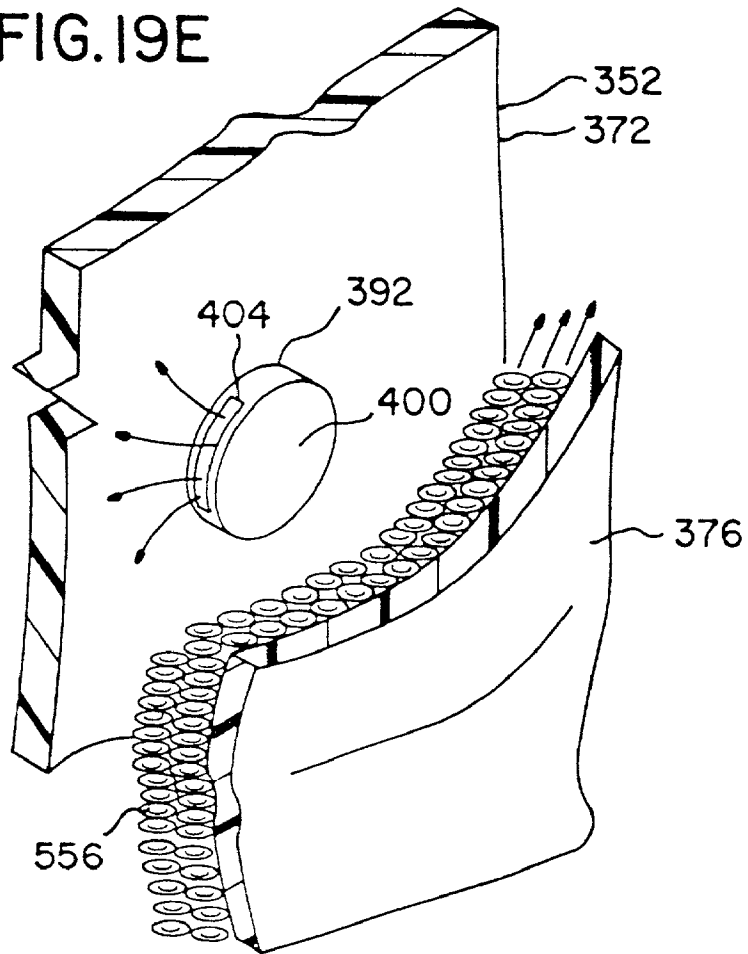
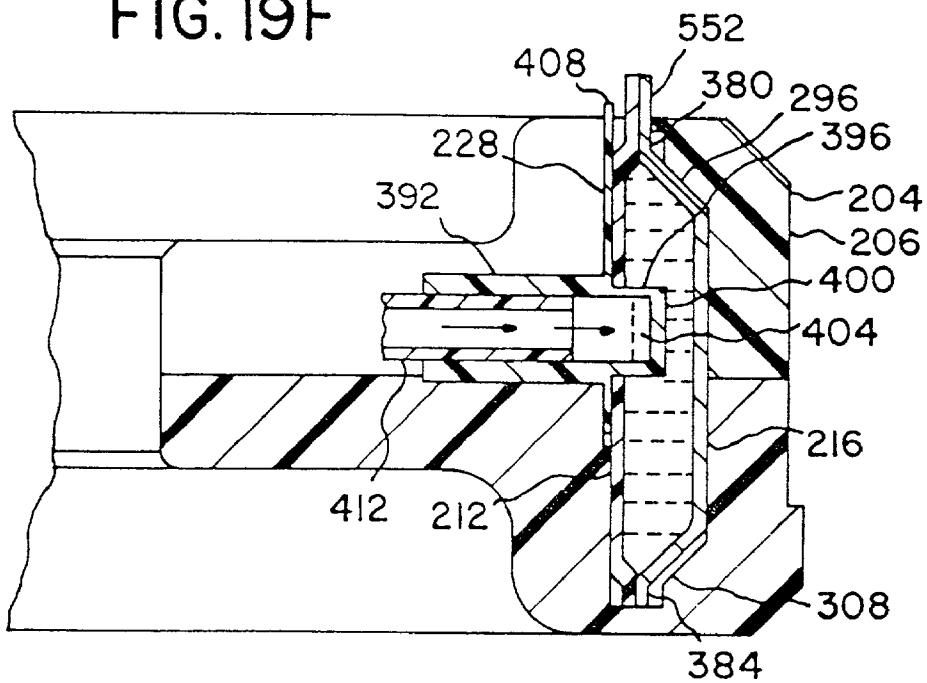


FIG. 19F



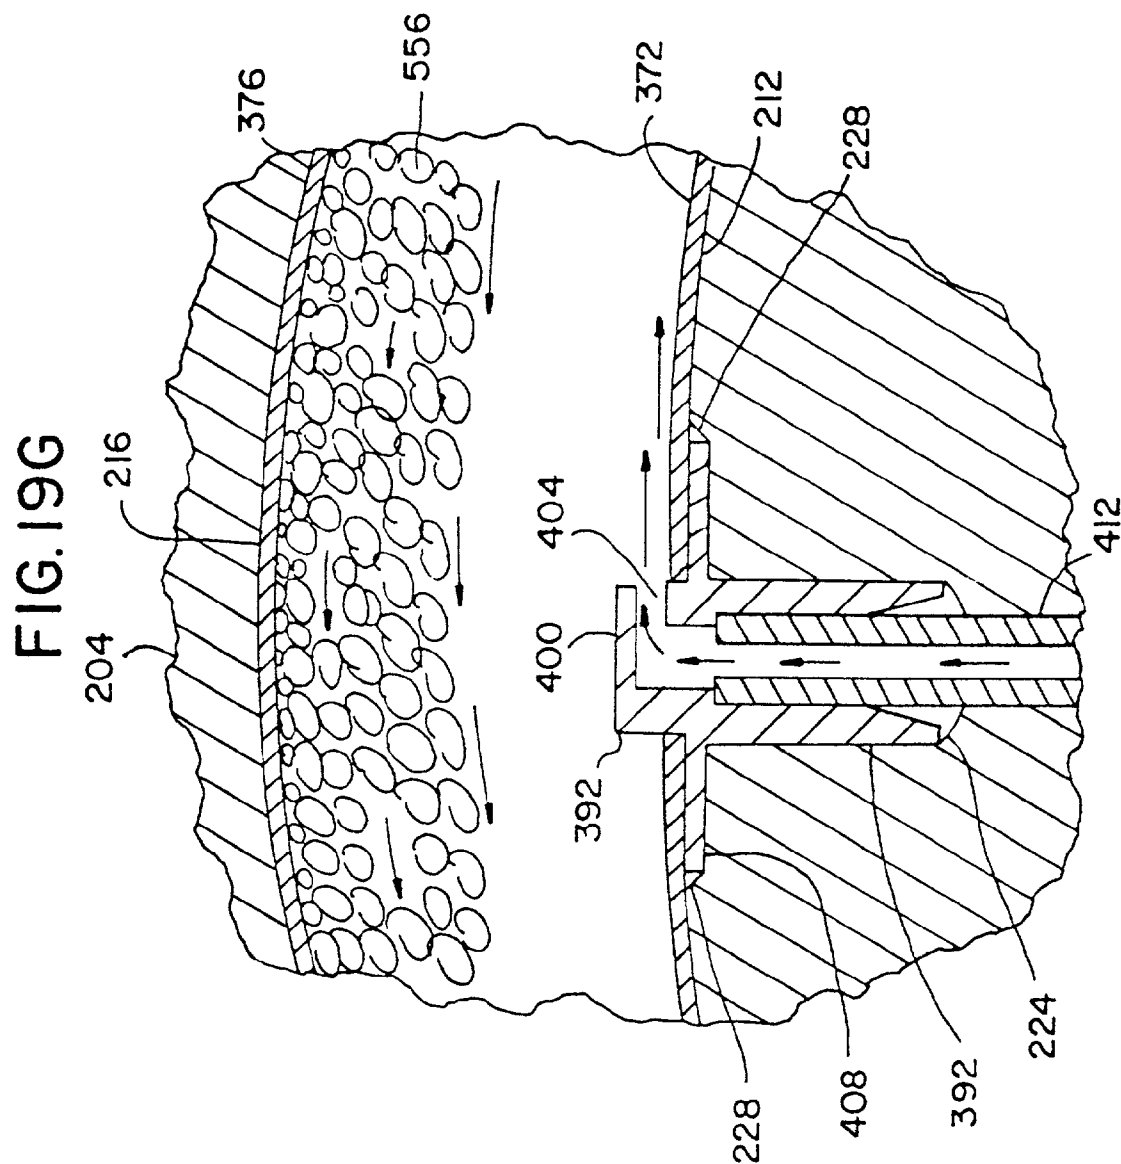


FIG. 20A

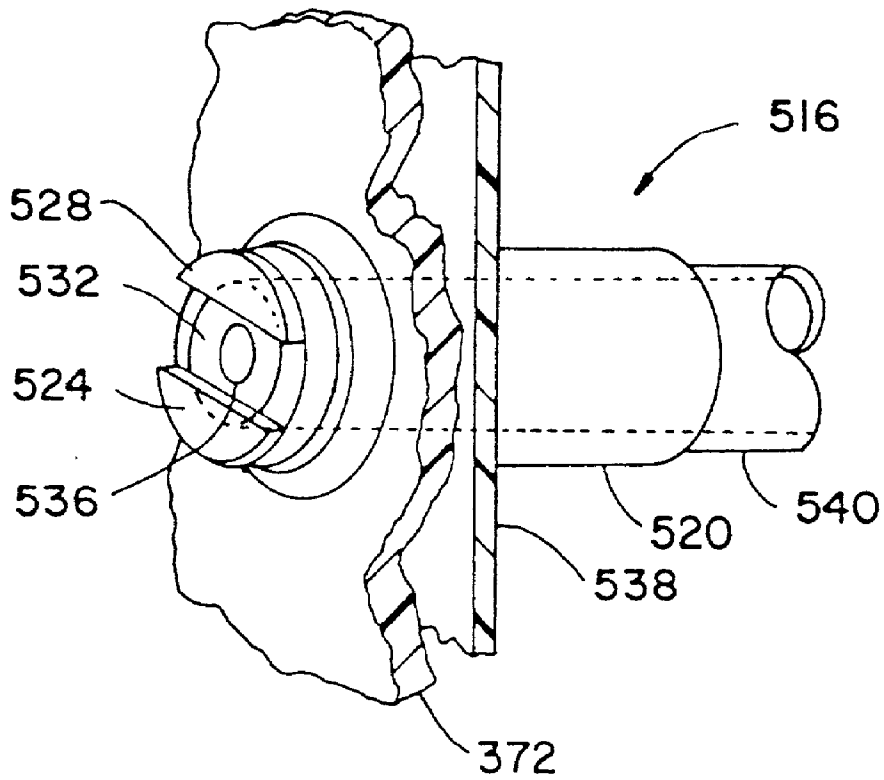


FIG. 20B

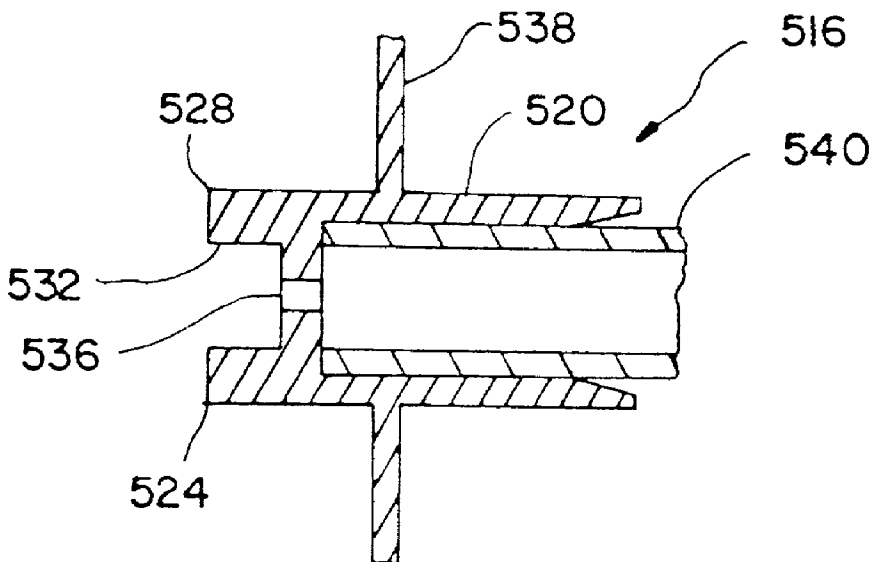


FIG. 20C

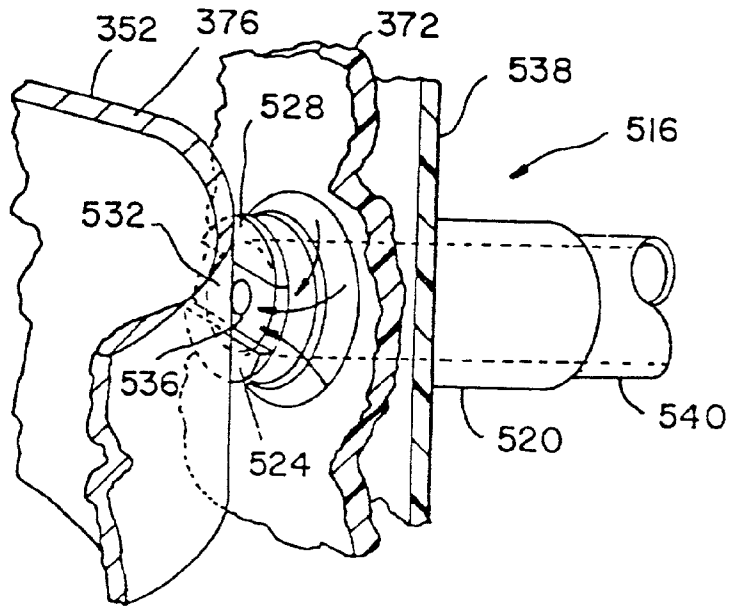


FIG. 20D

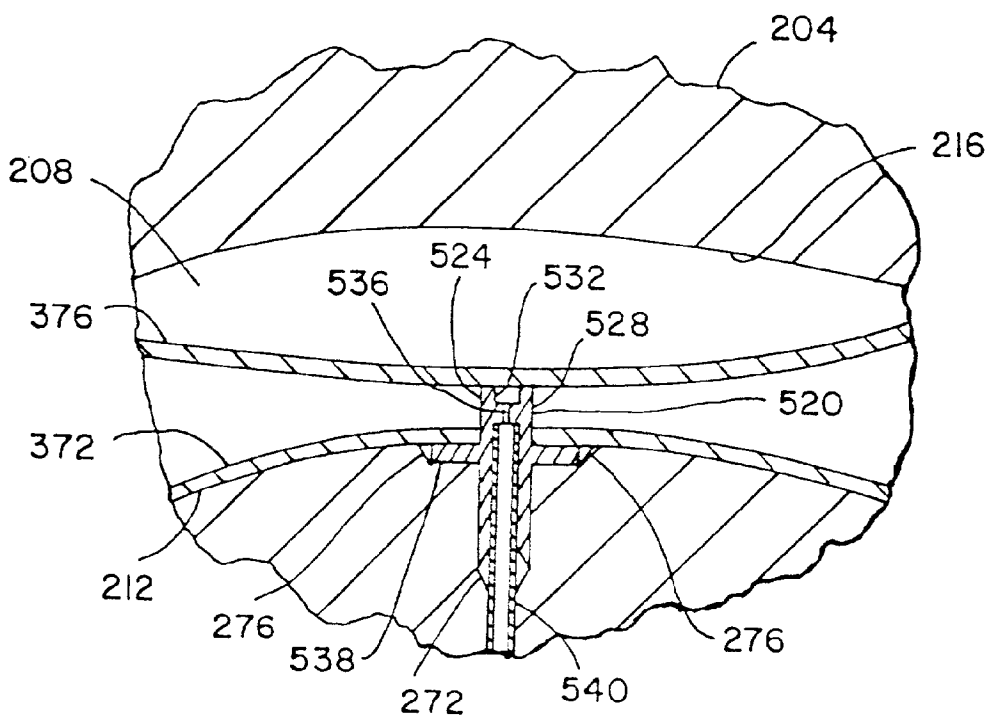


FIG. 21A

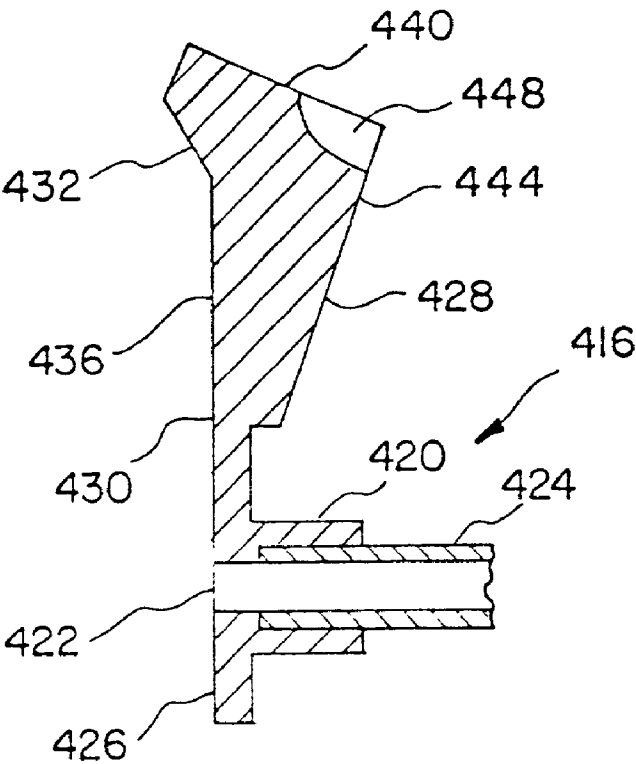


FIG. 21B

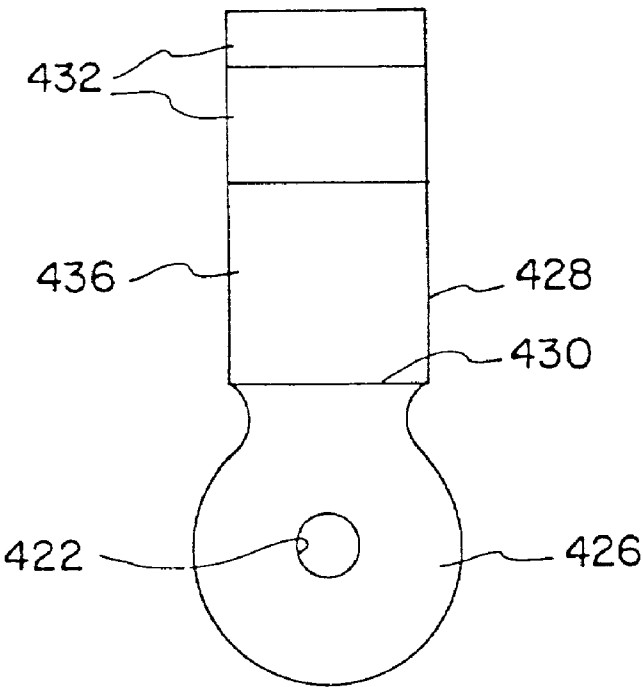


FIG.22

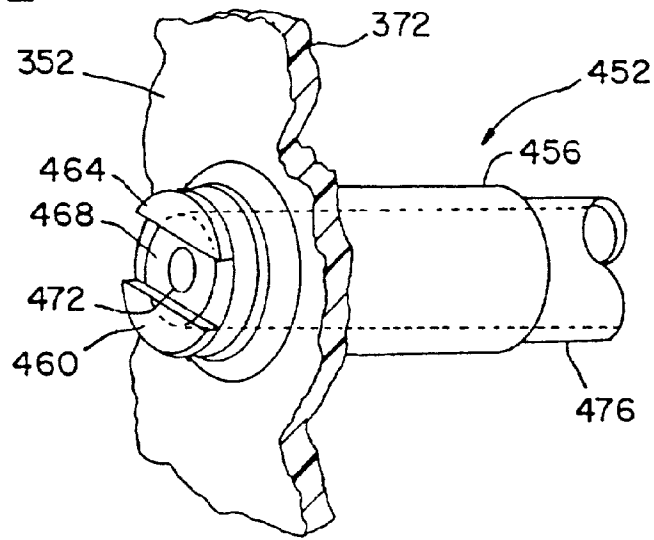


FIG.23A

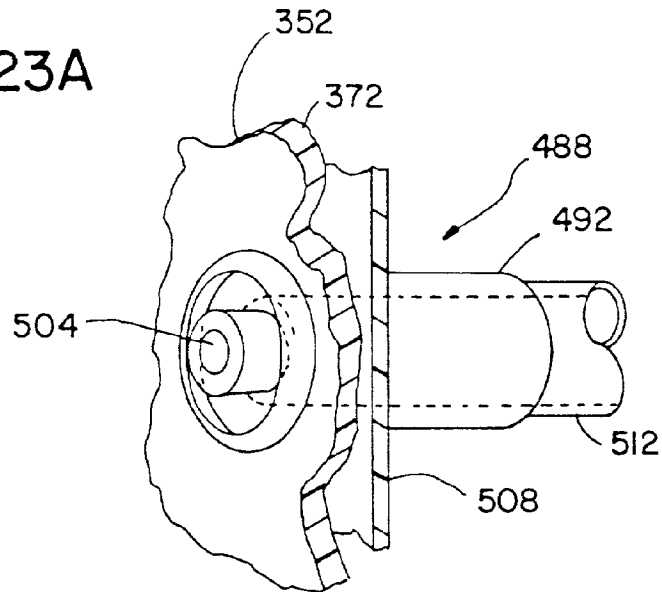


FIG.23B

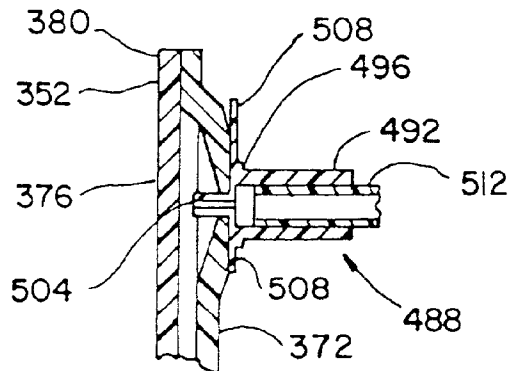


FIG. 24

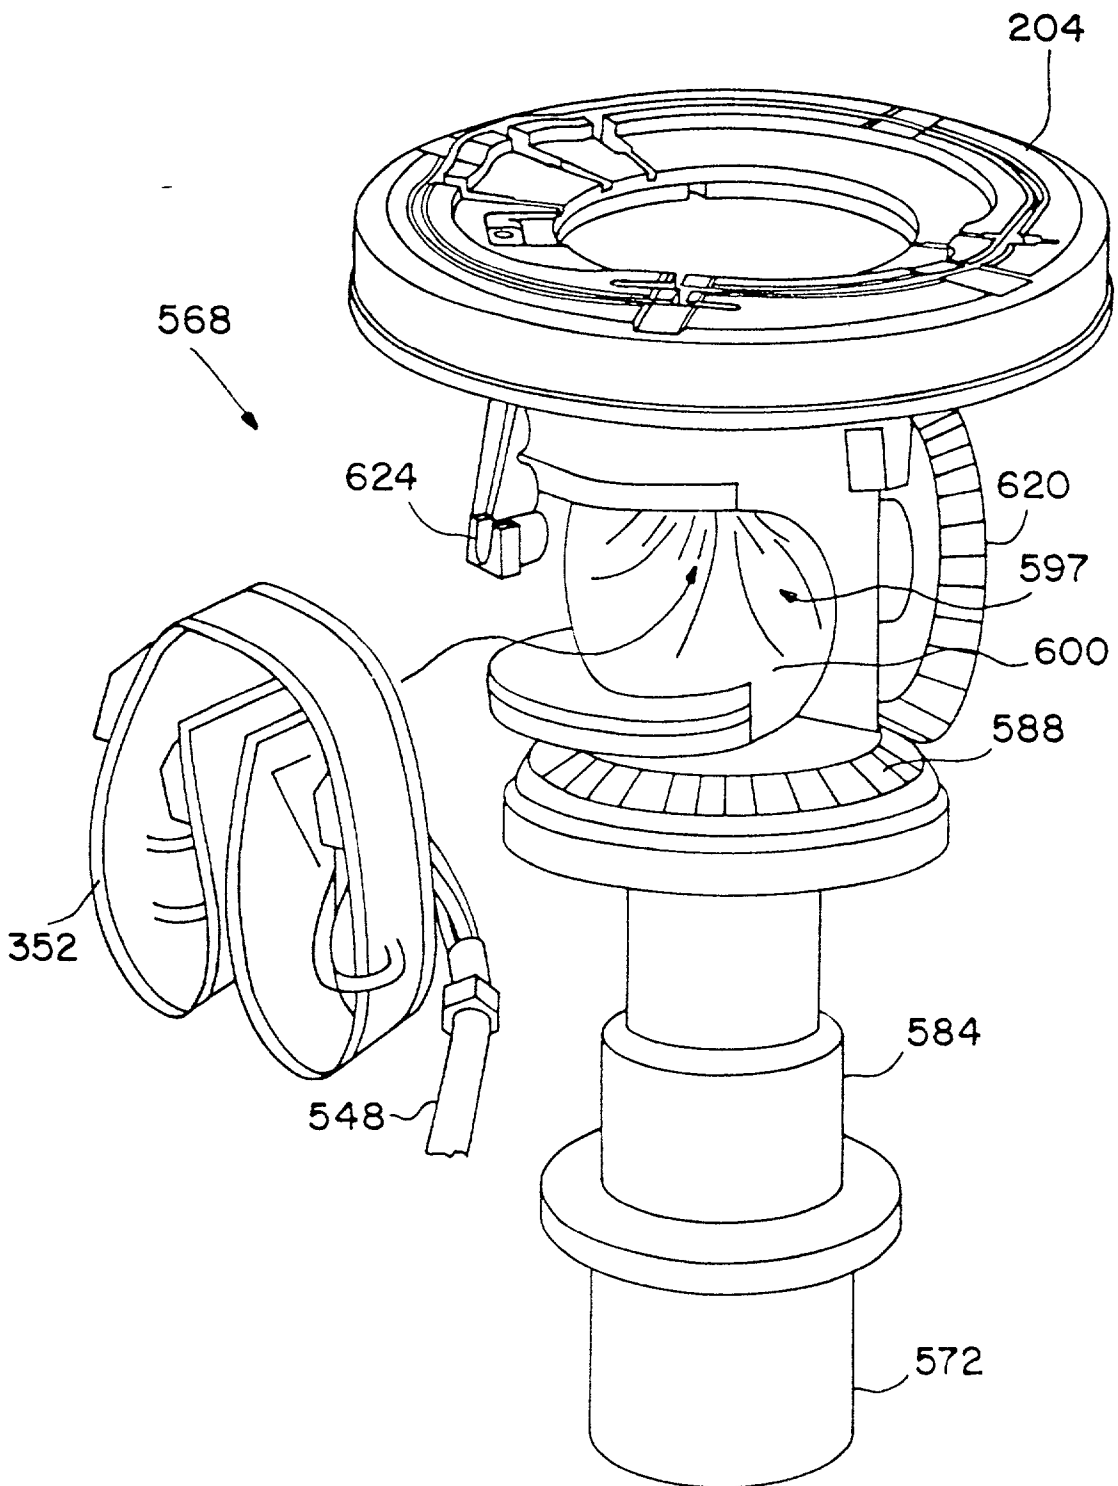


FIG.25A

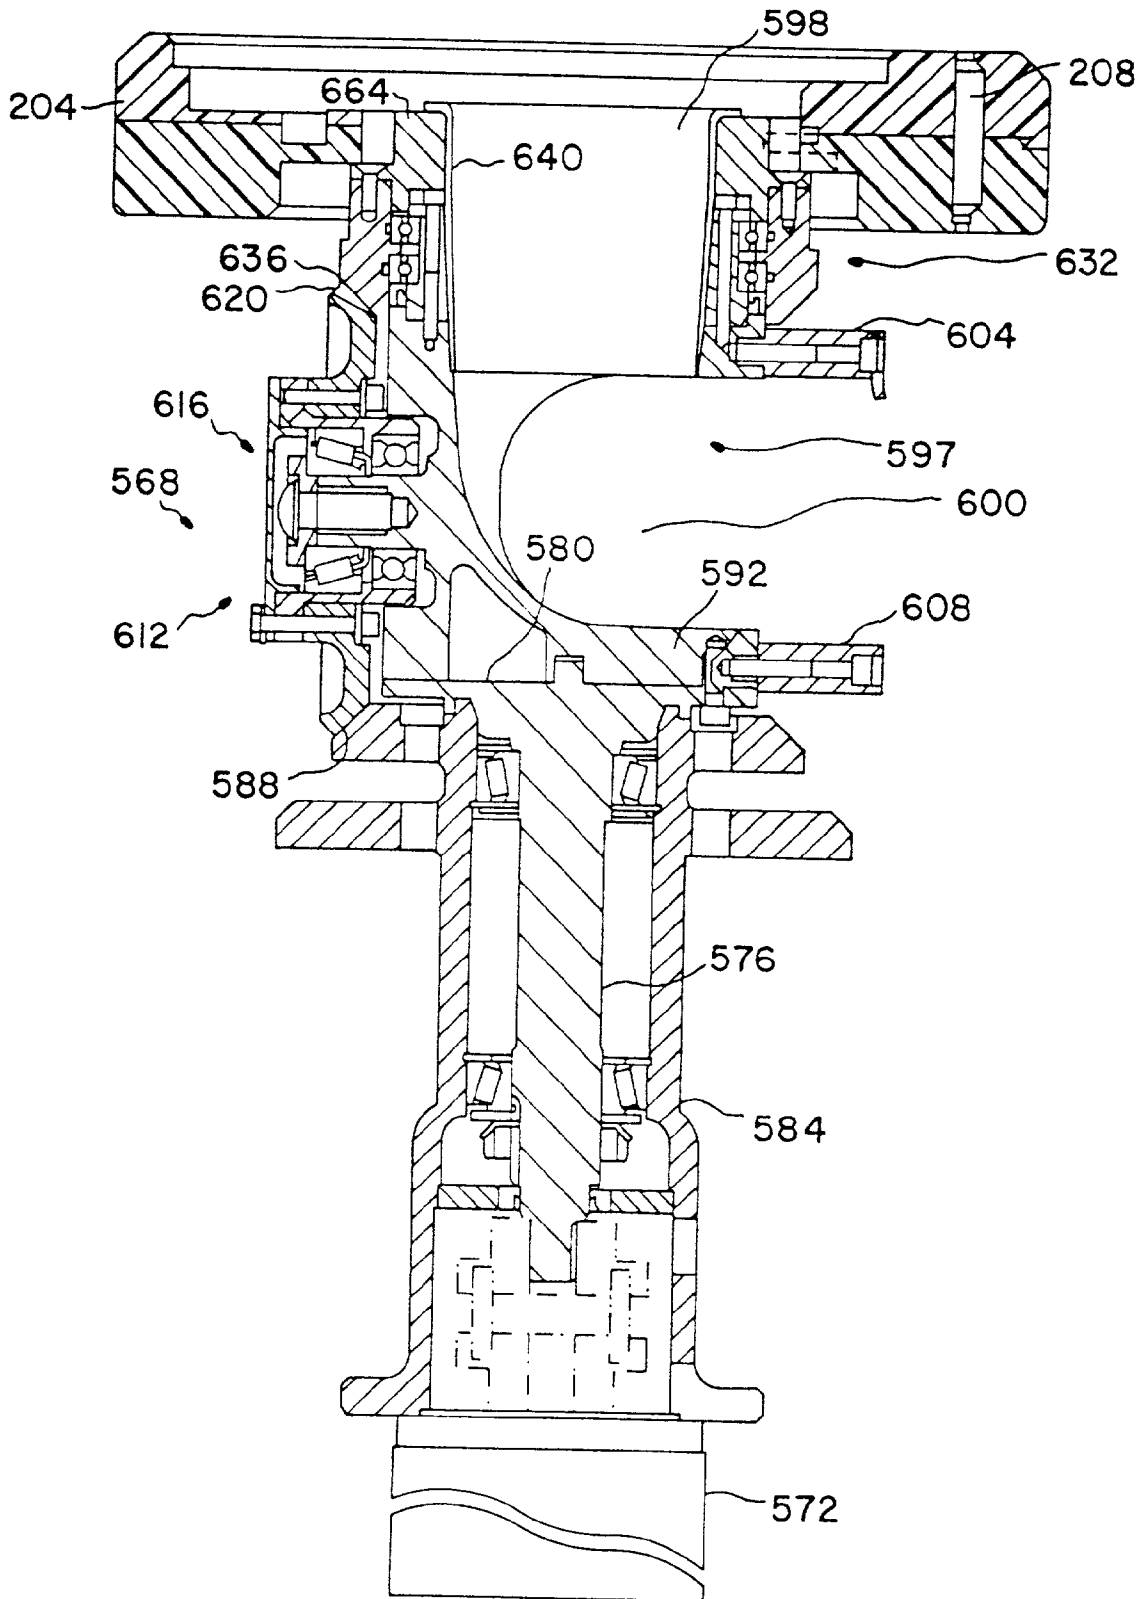


FIG. 25C

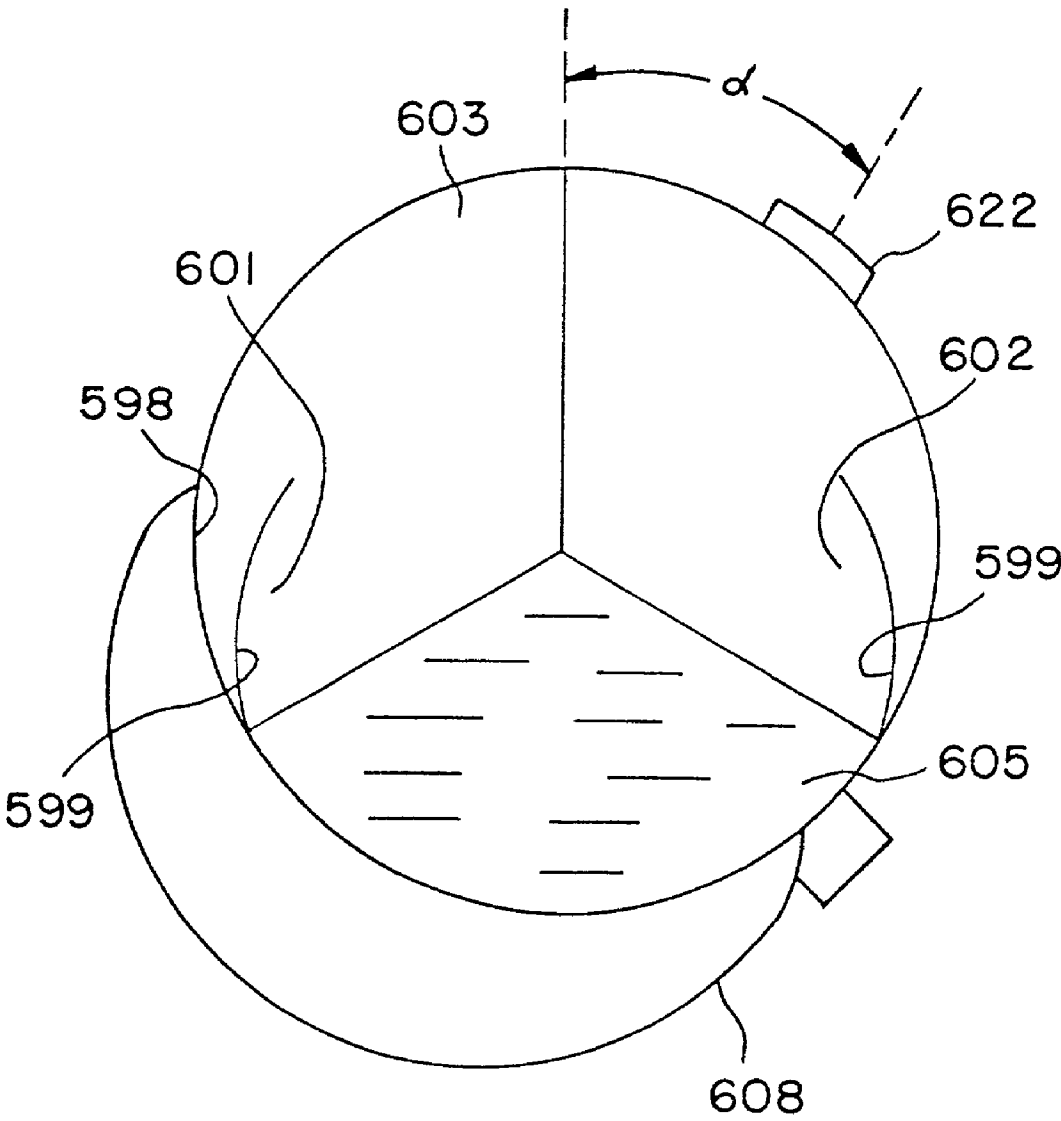


FIG. 25D

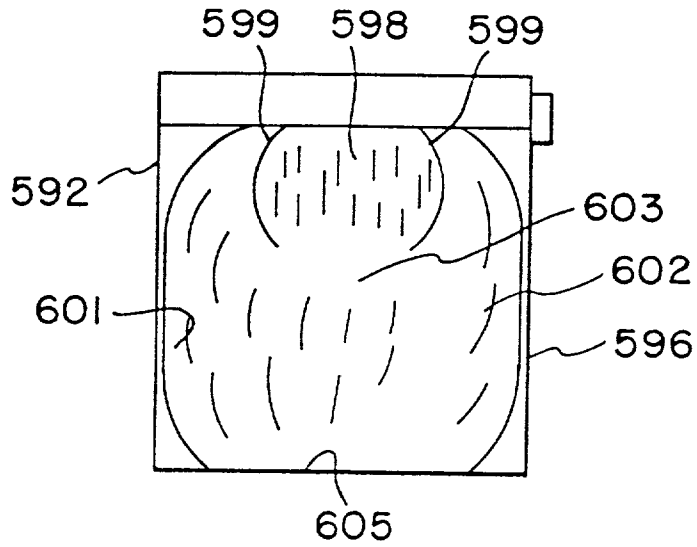


FIG. 25E

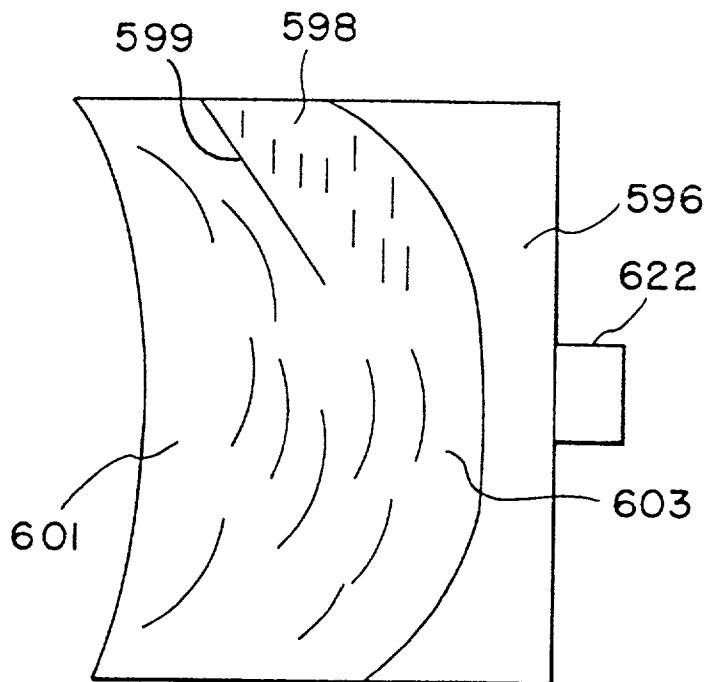
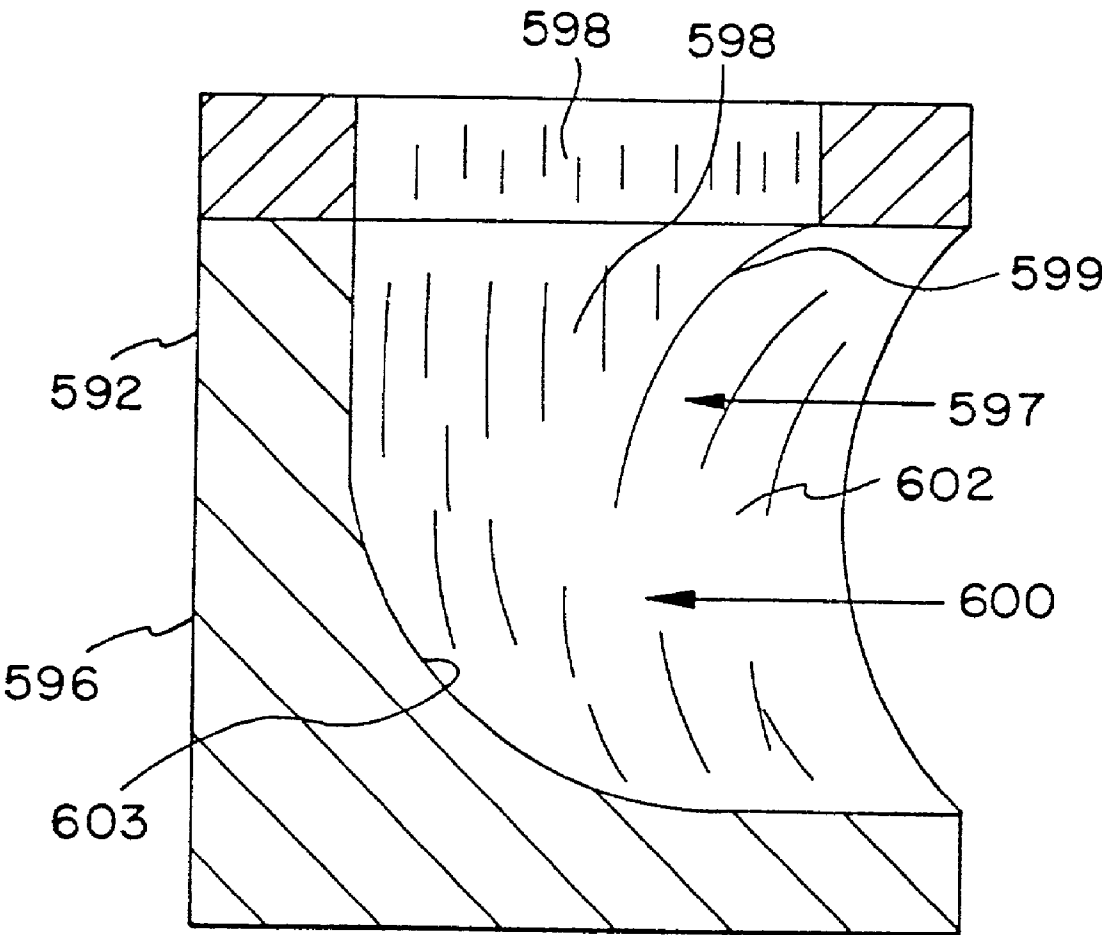
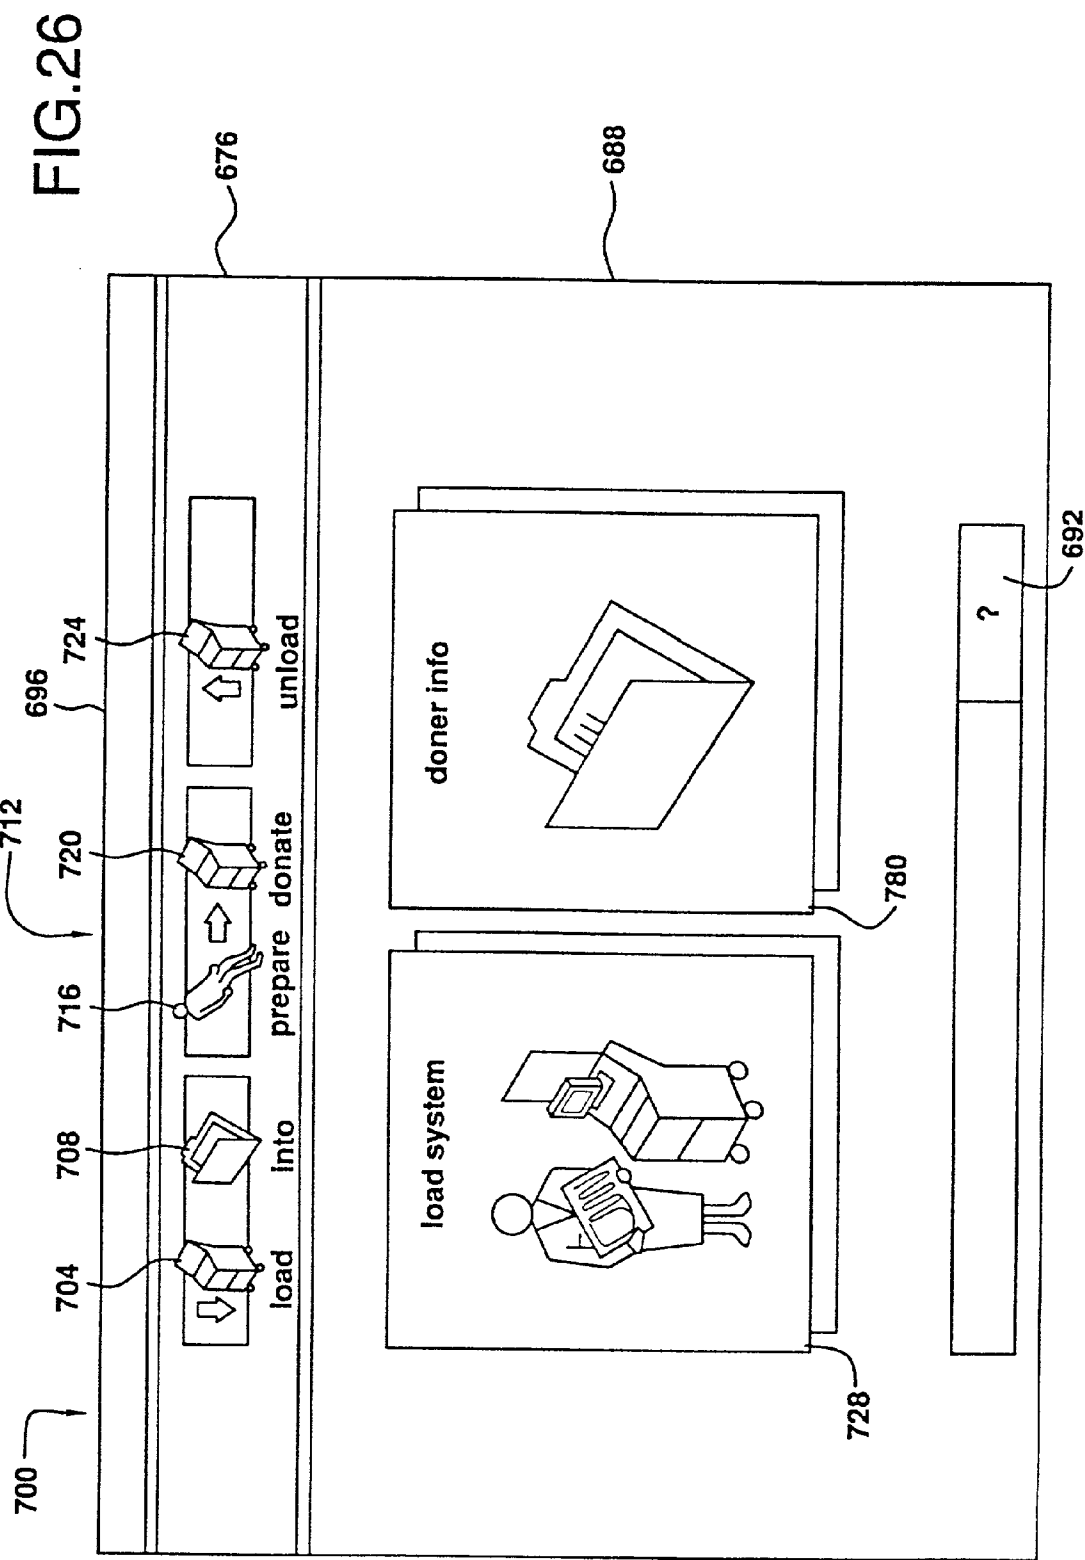
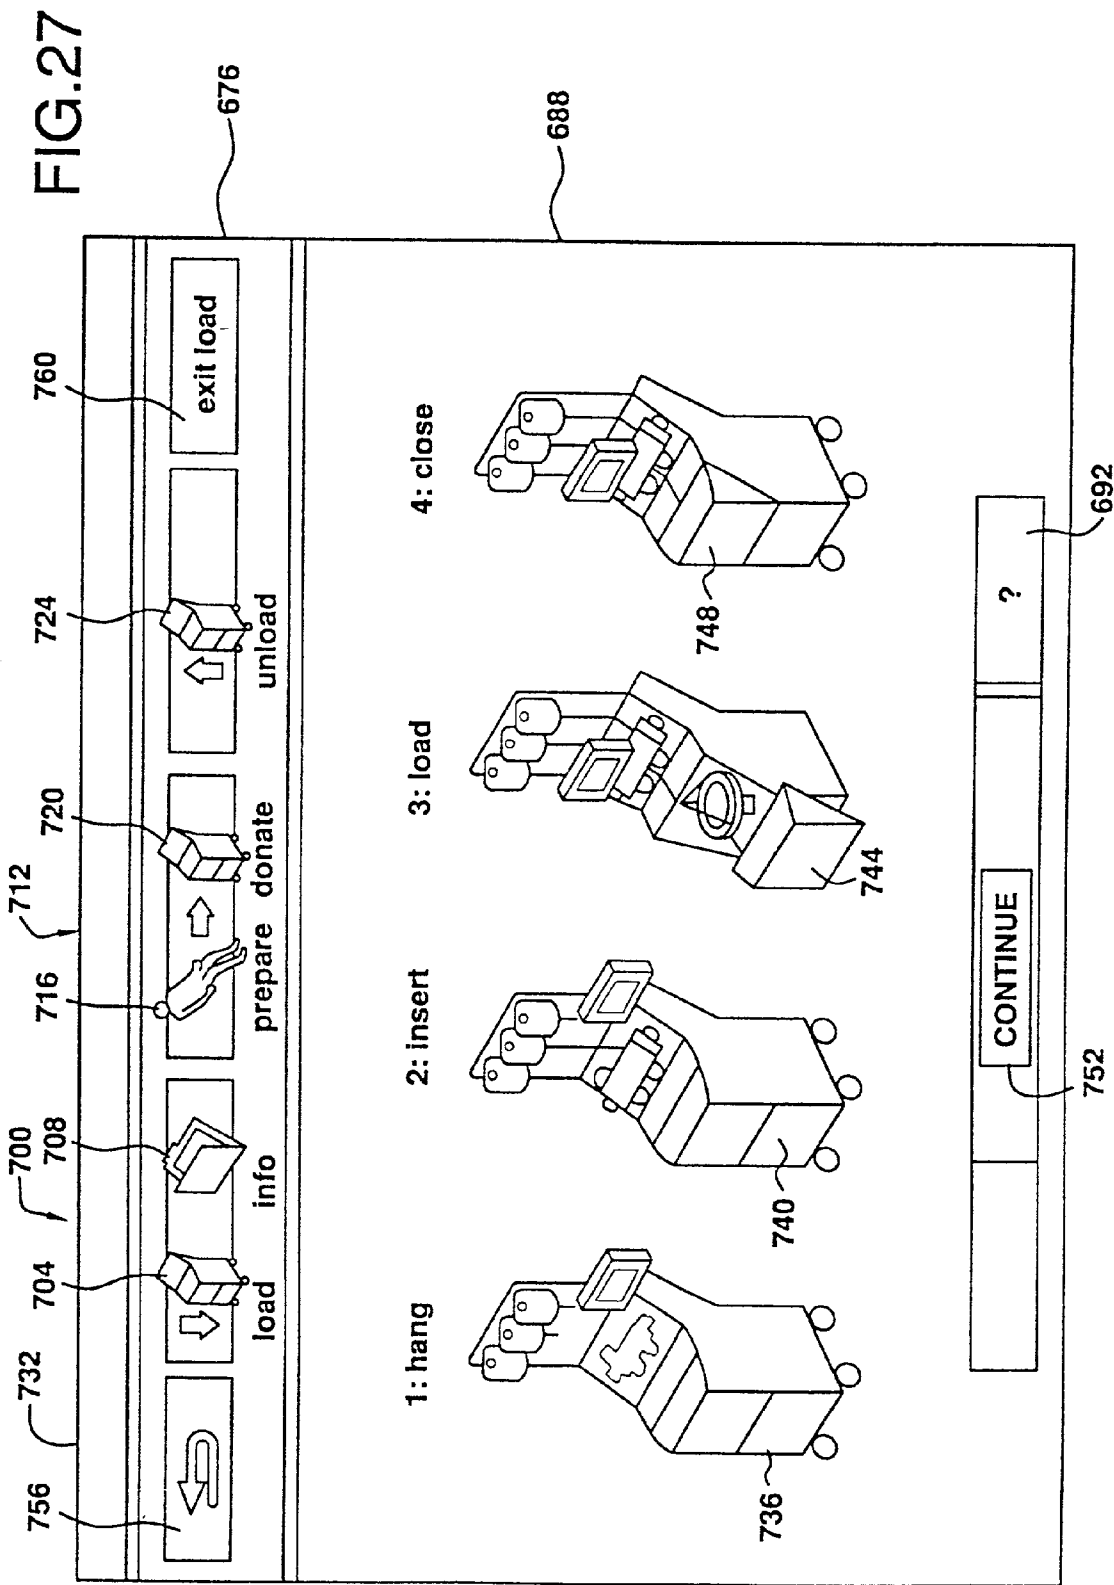
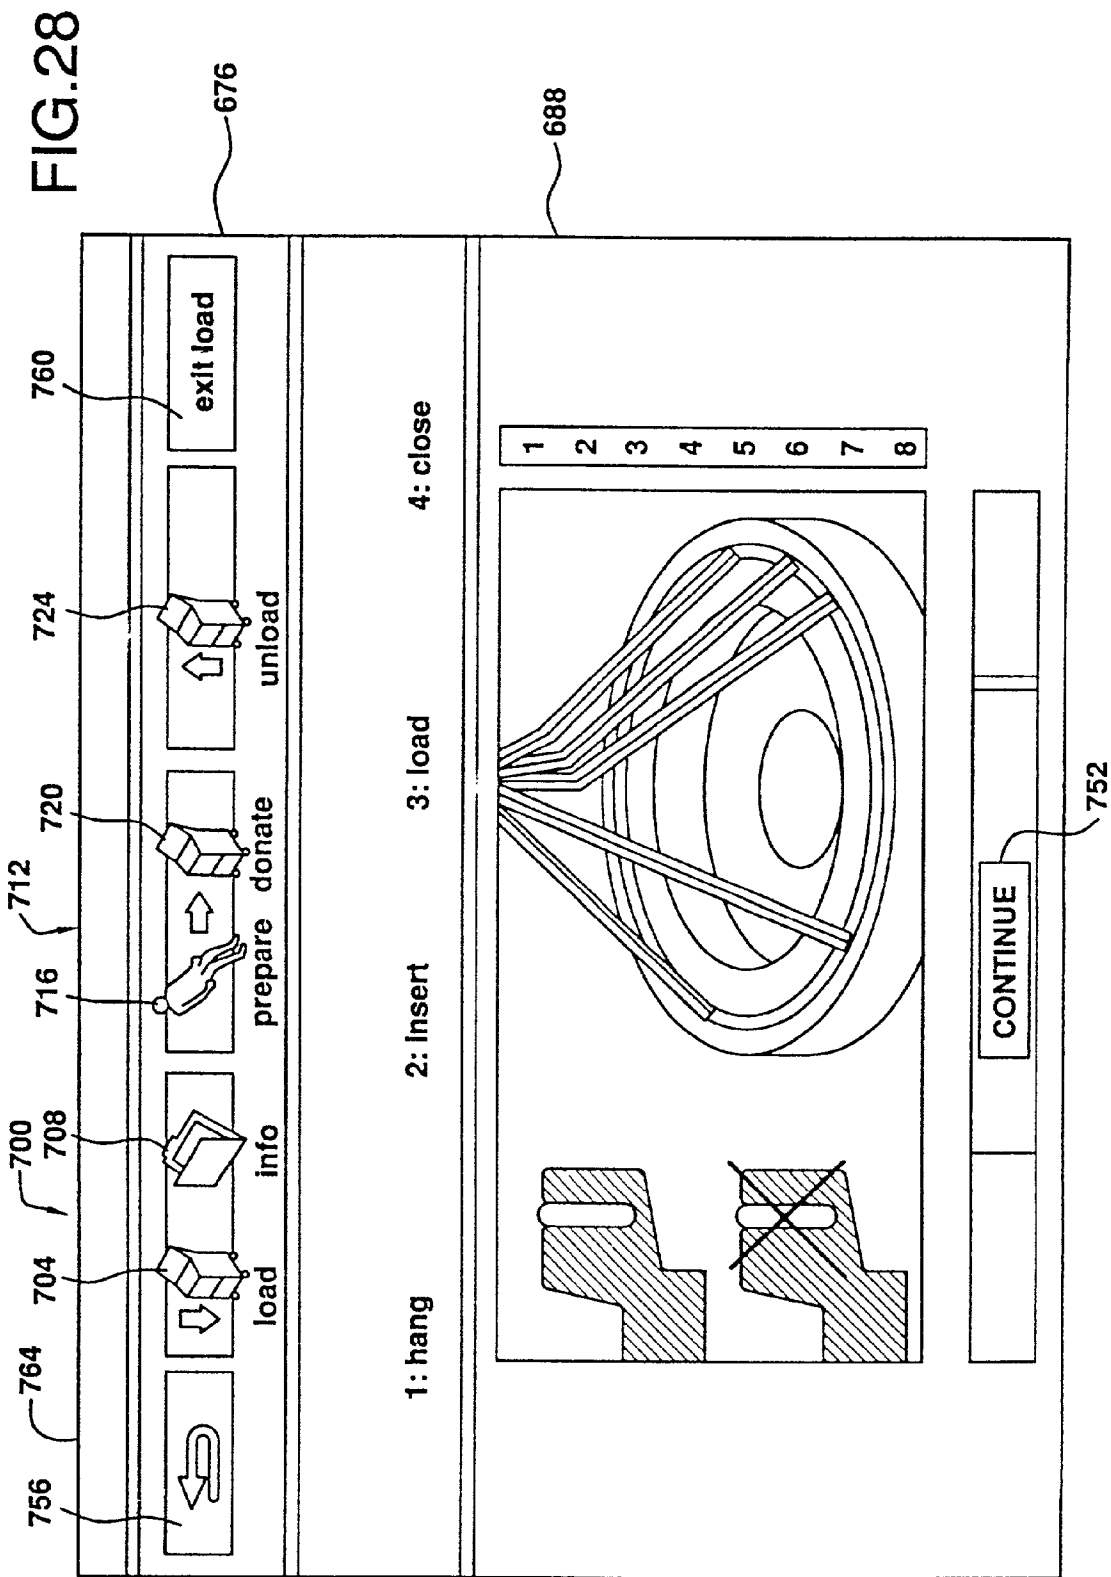


FIG. 25F









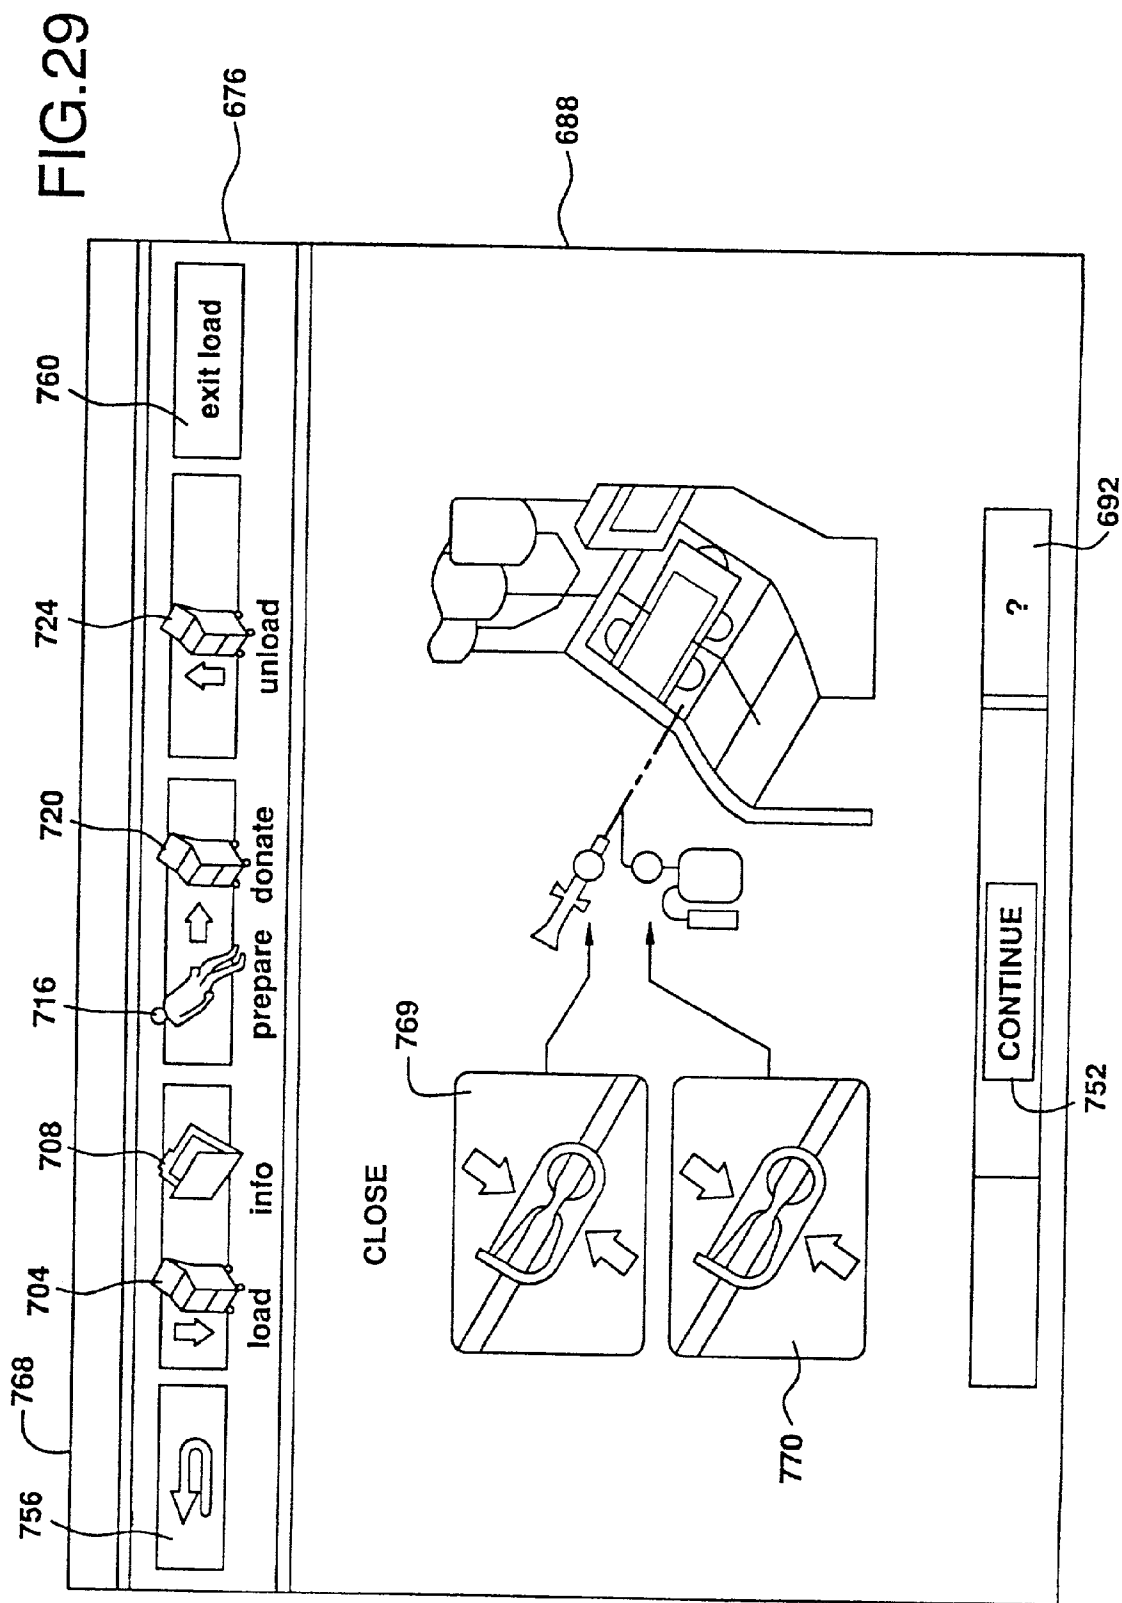
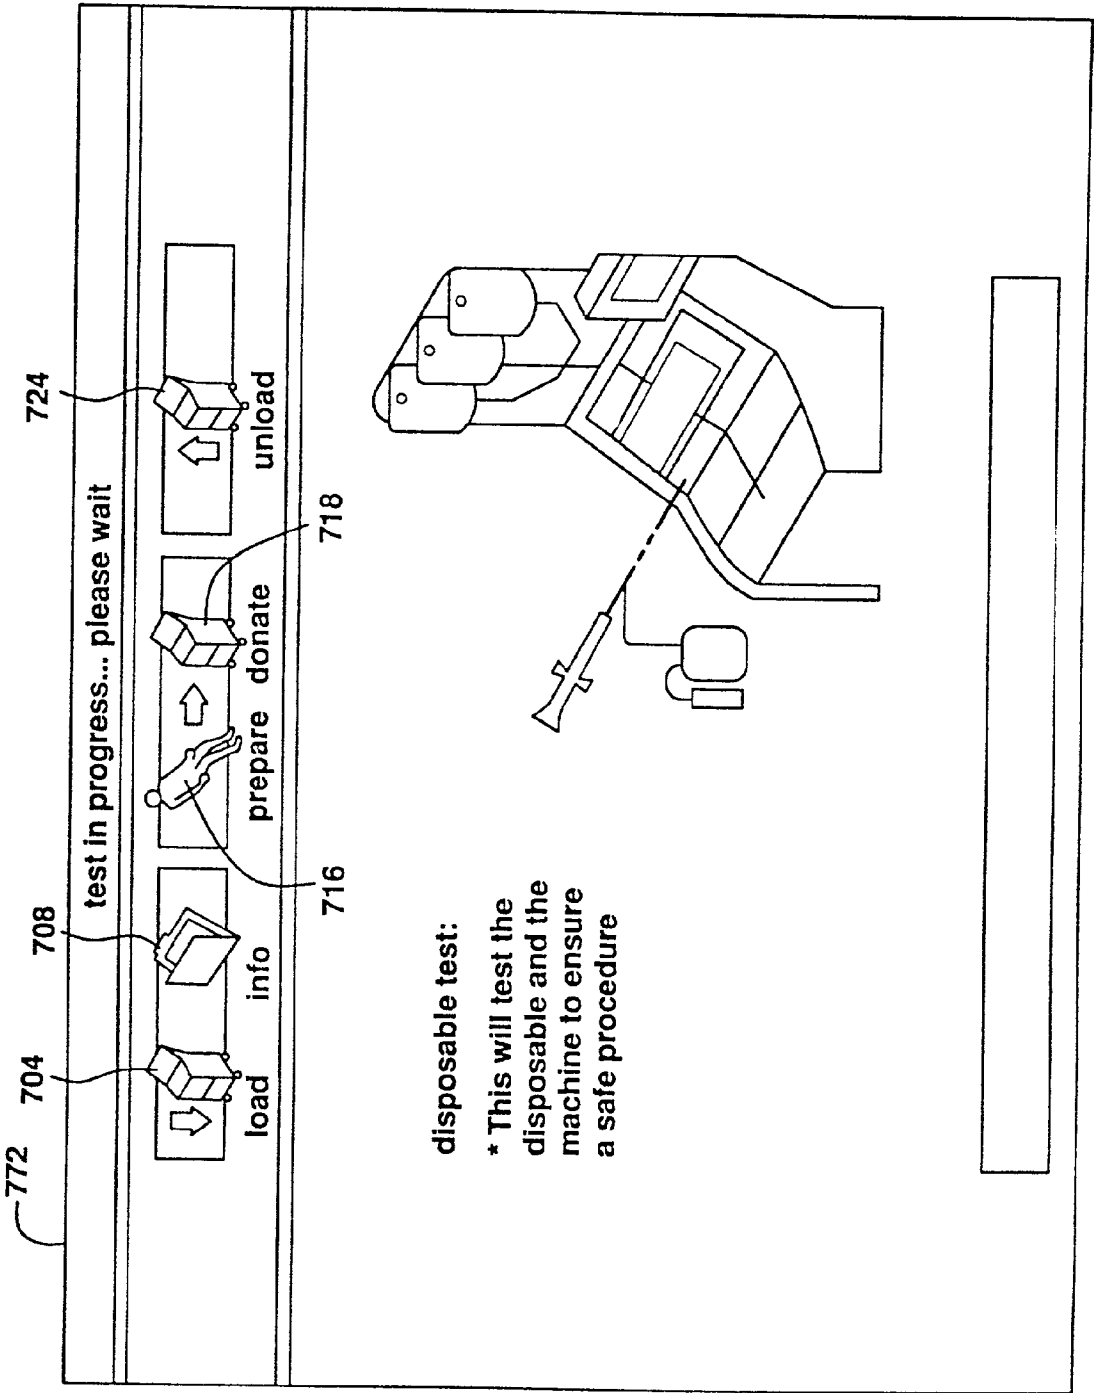


FIG.30



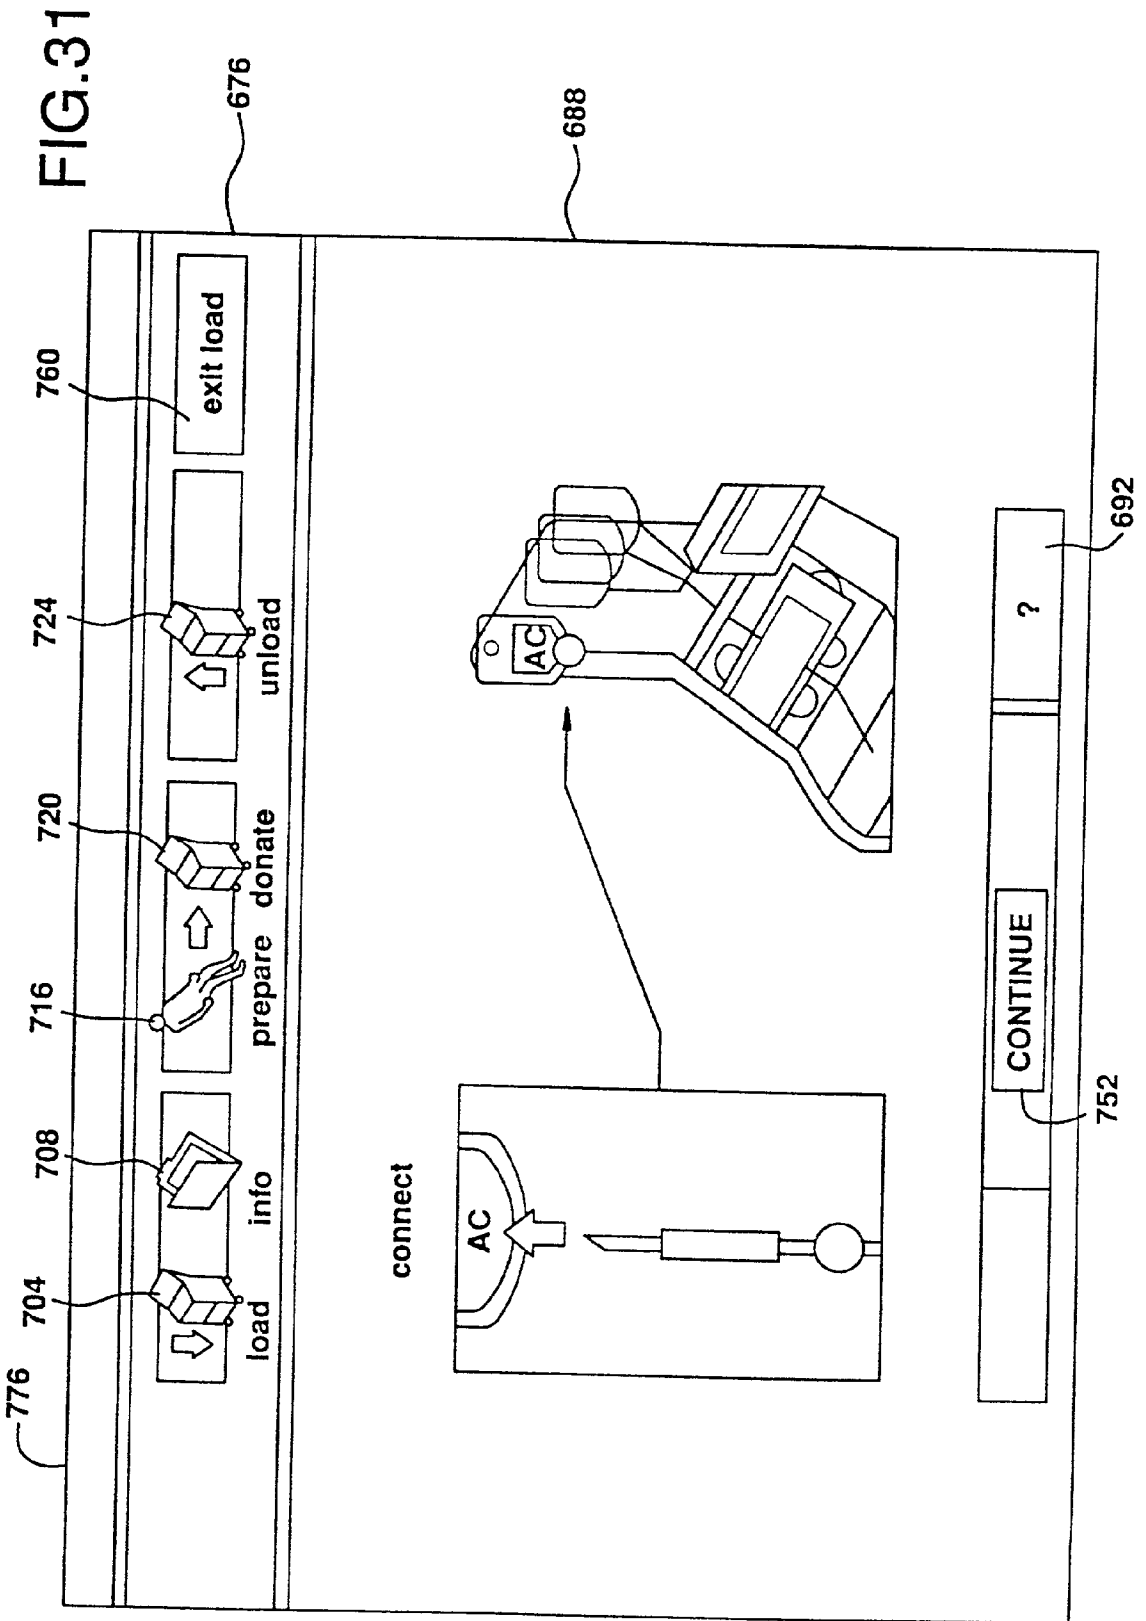
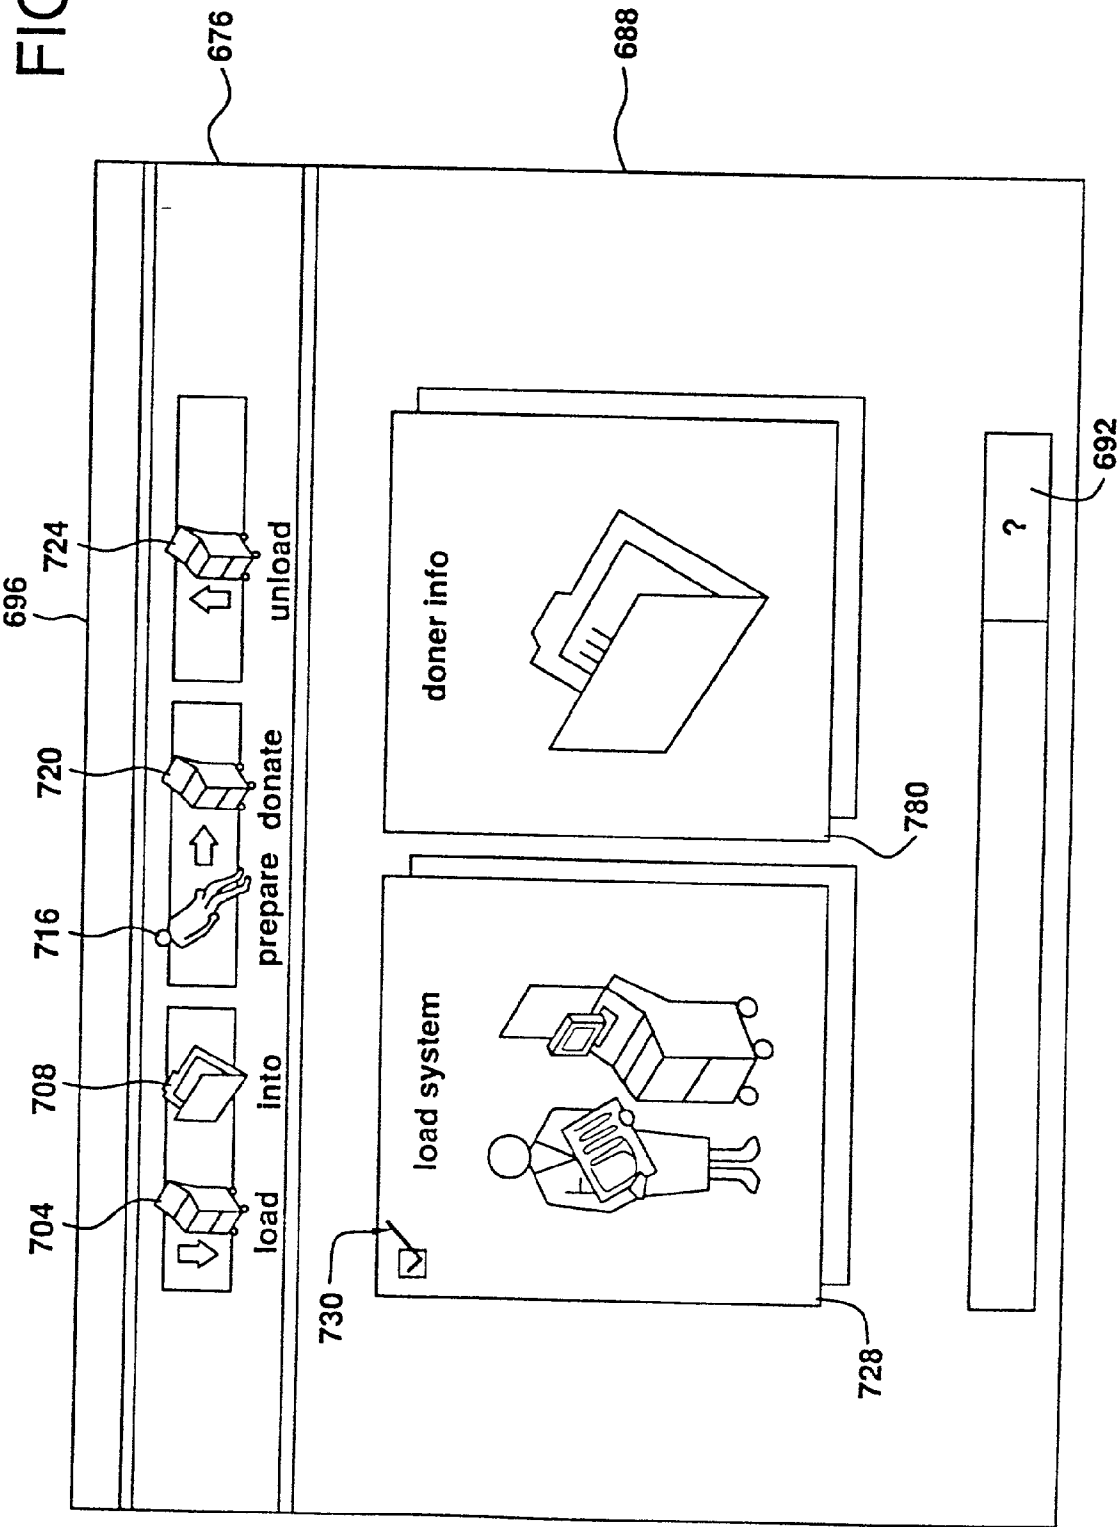


FIG. 32



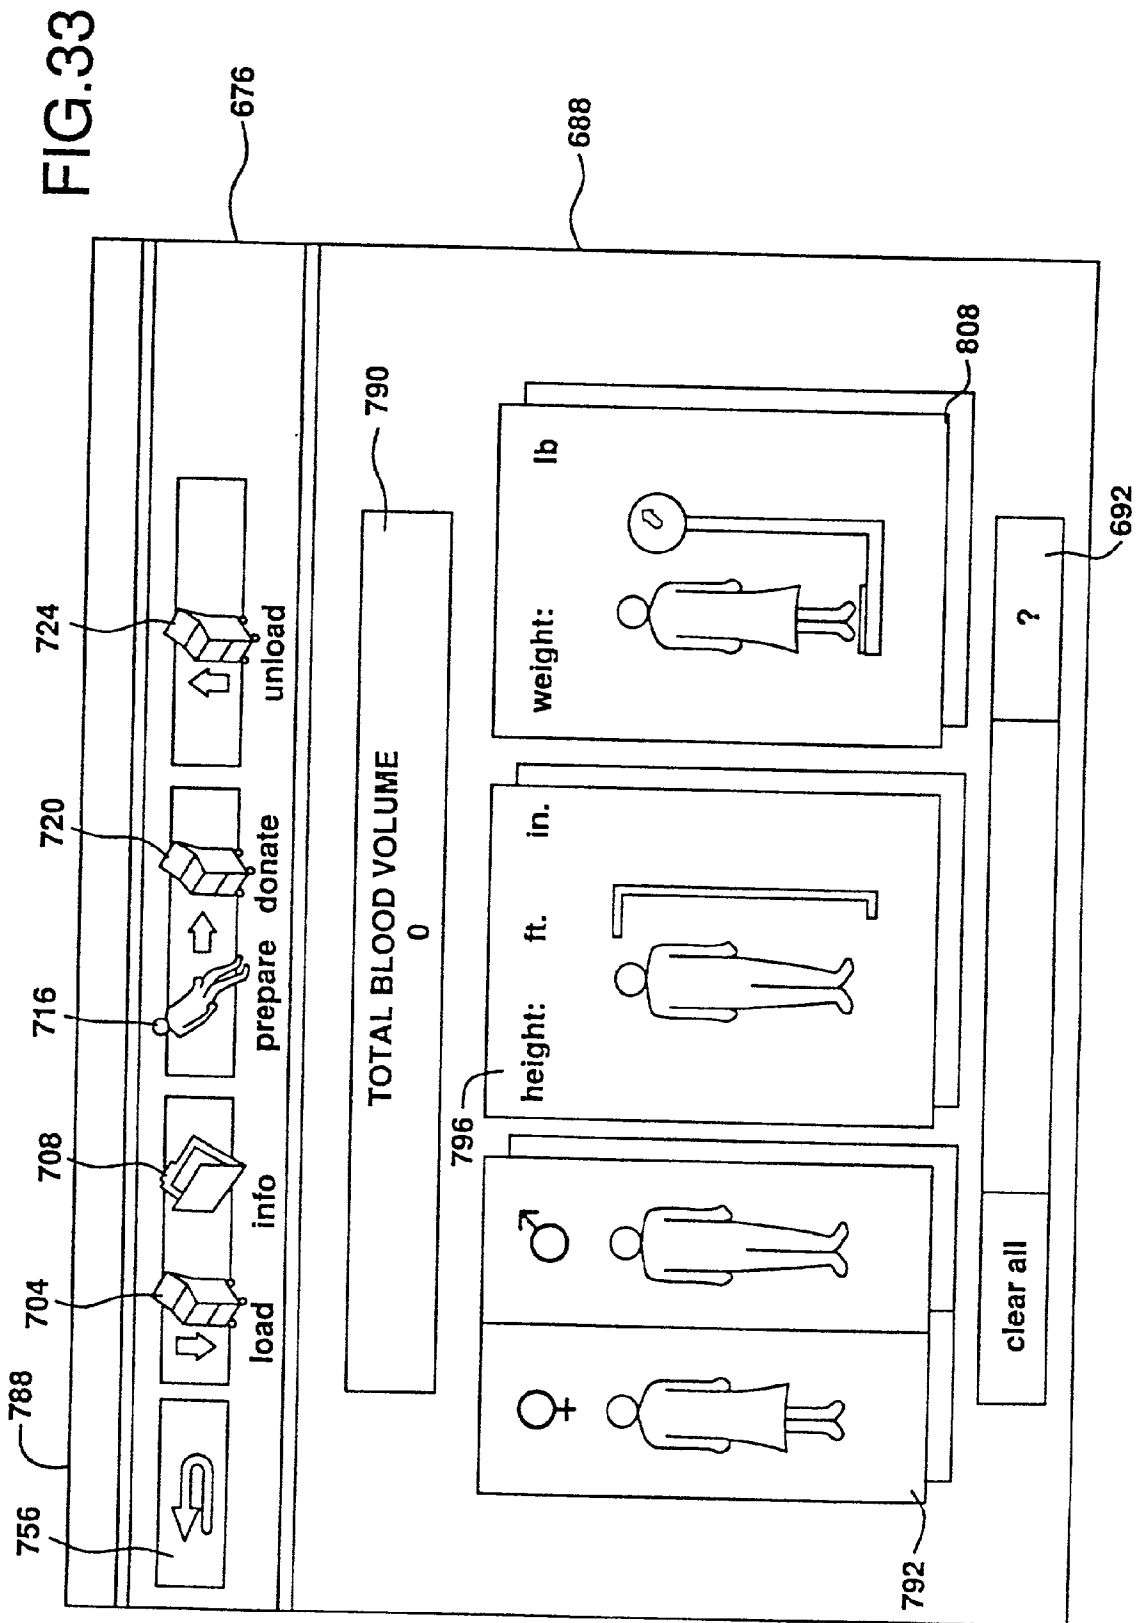


FIG.34

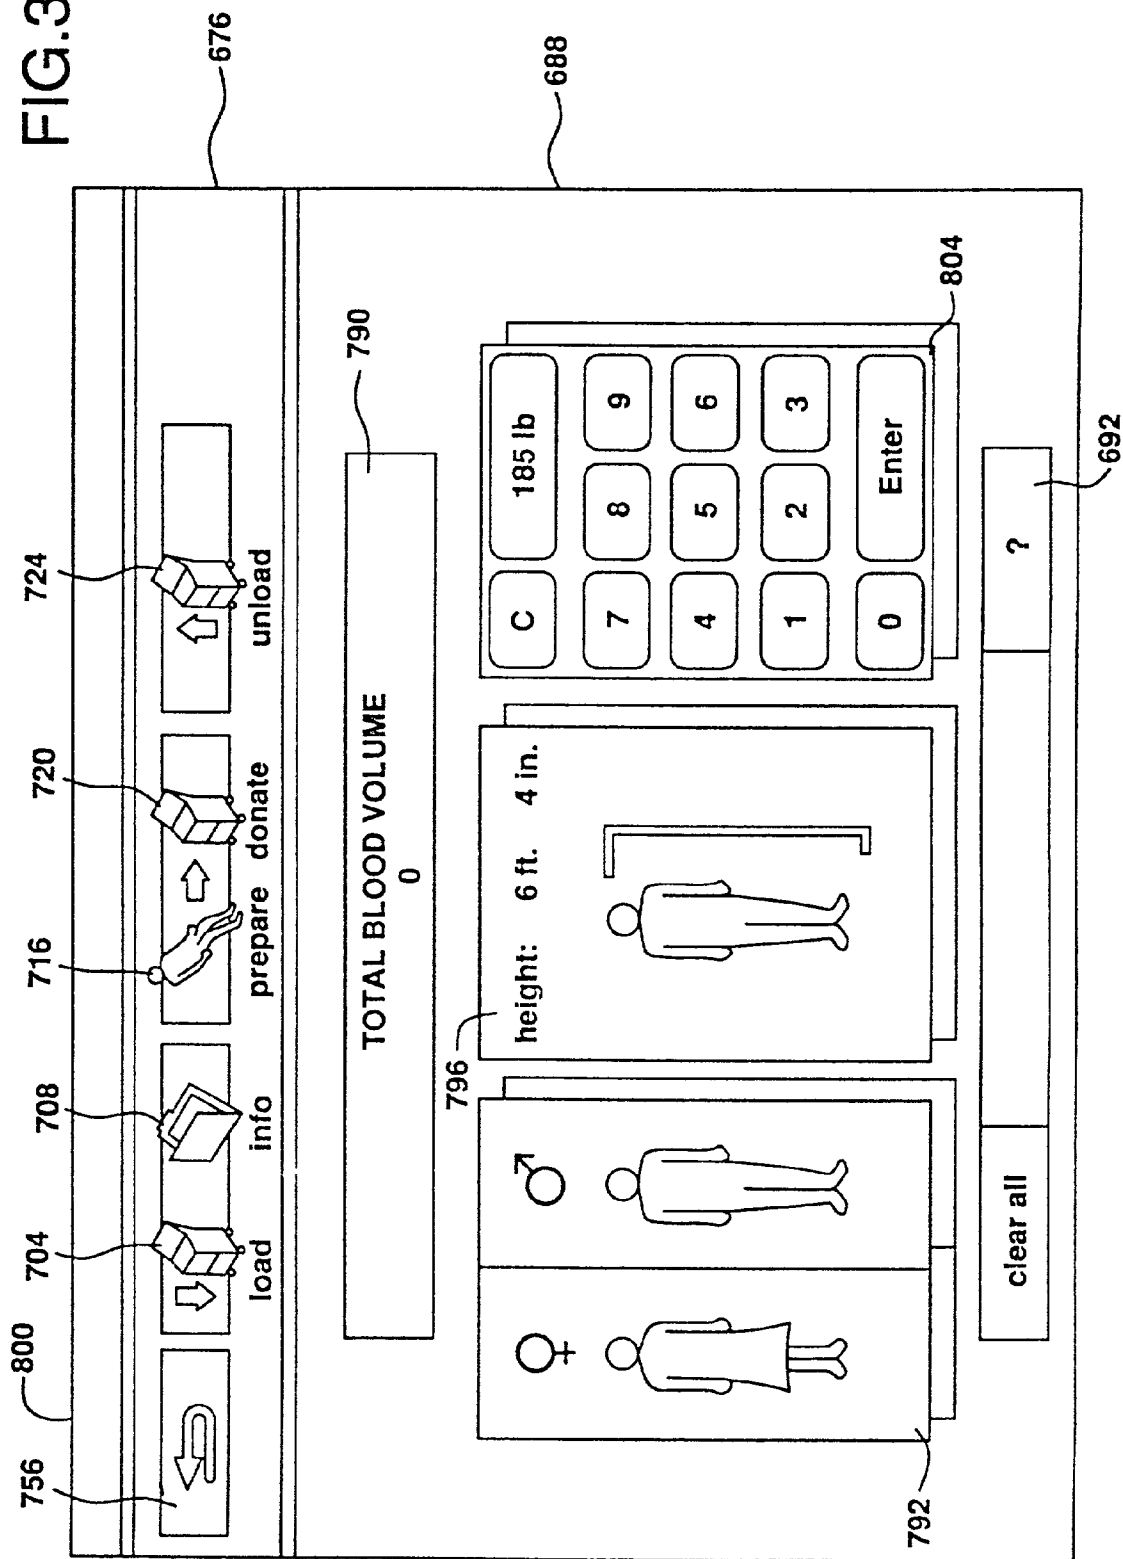


FIG.35

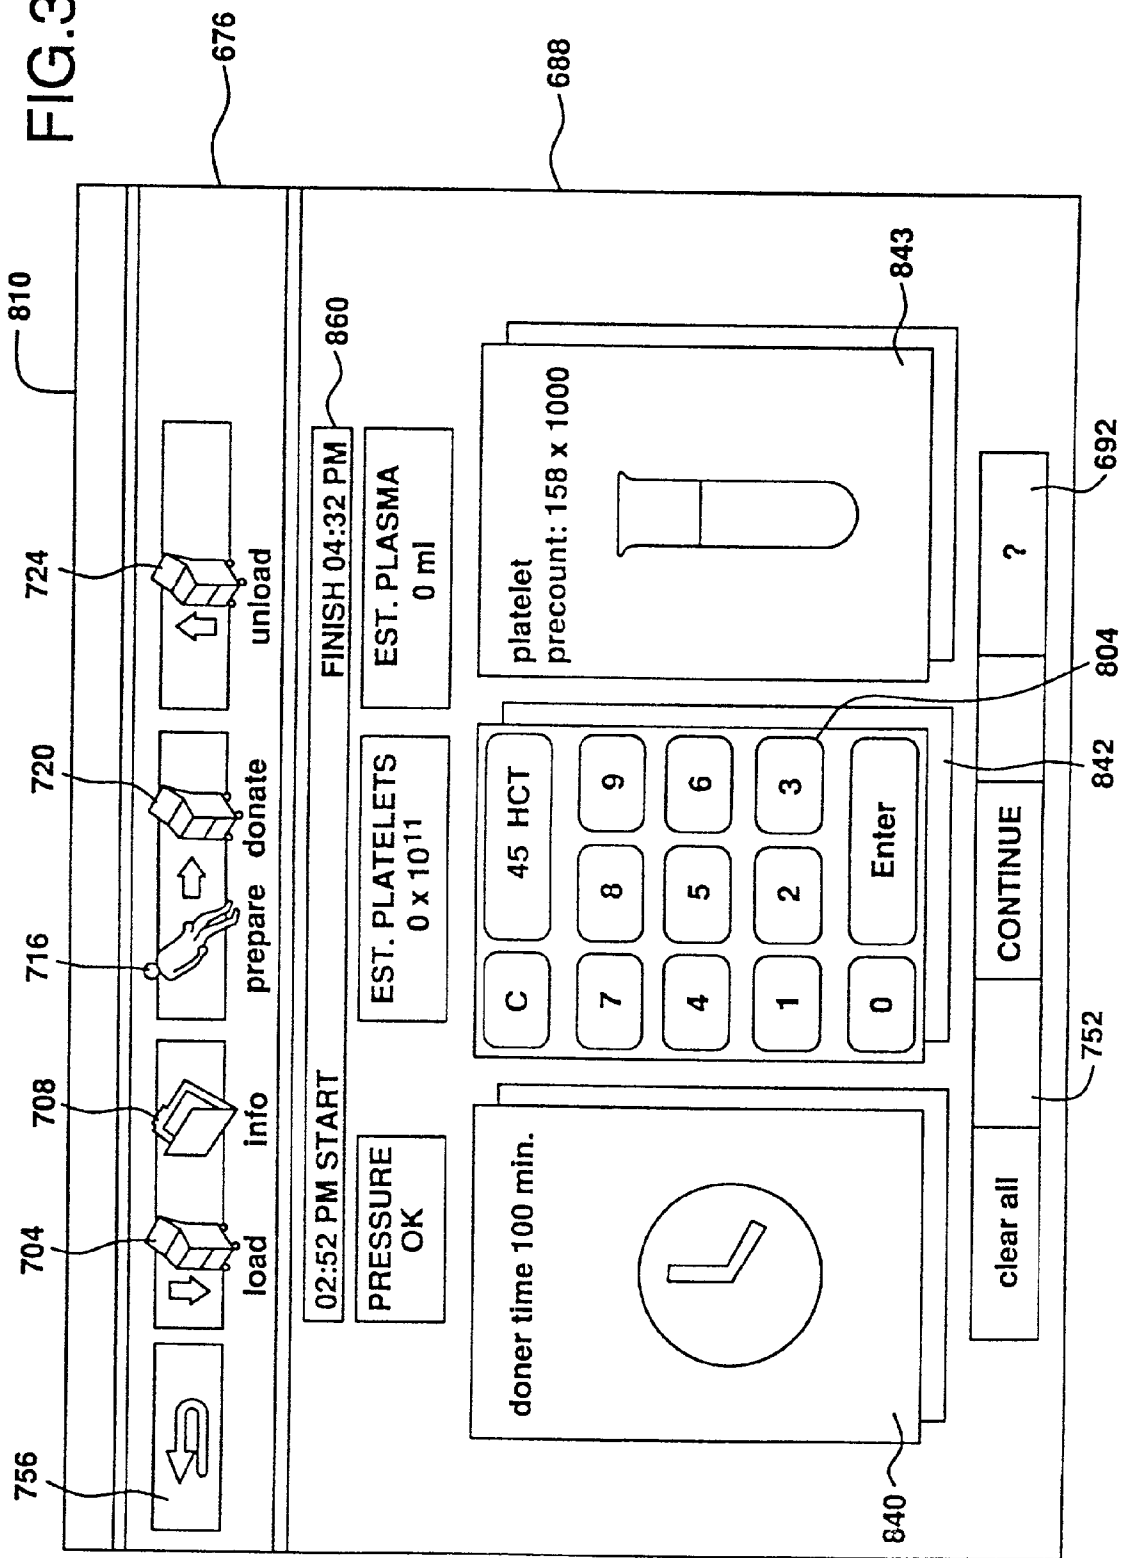
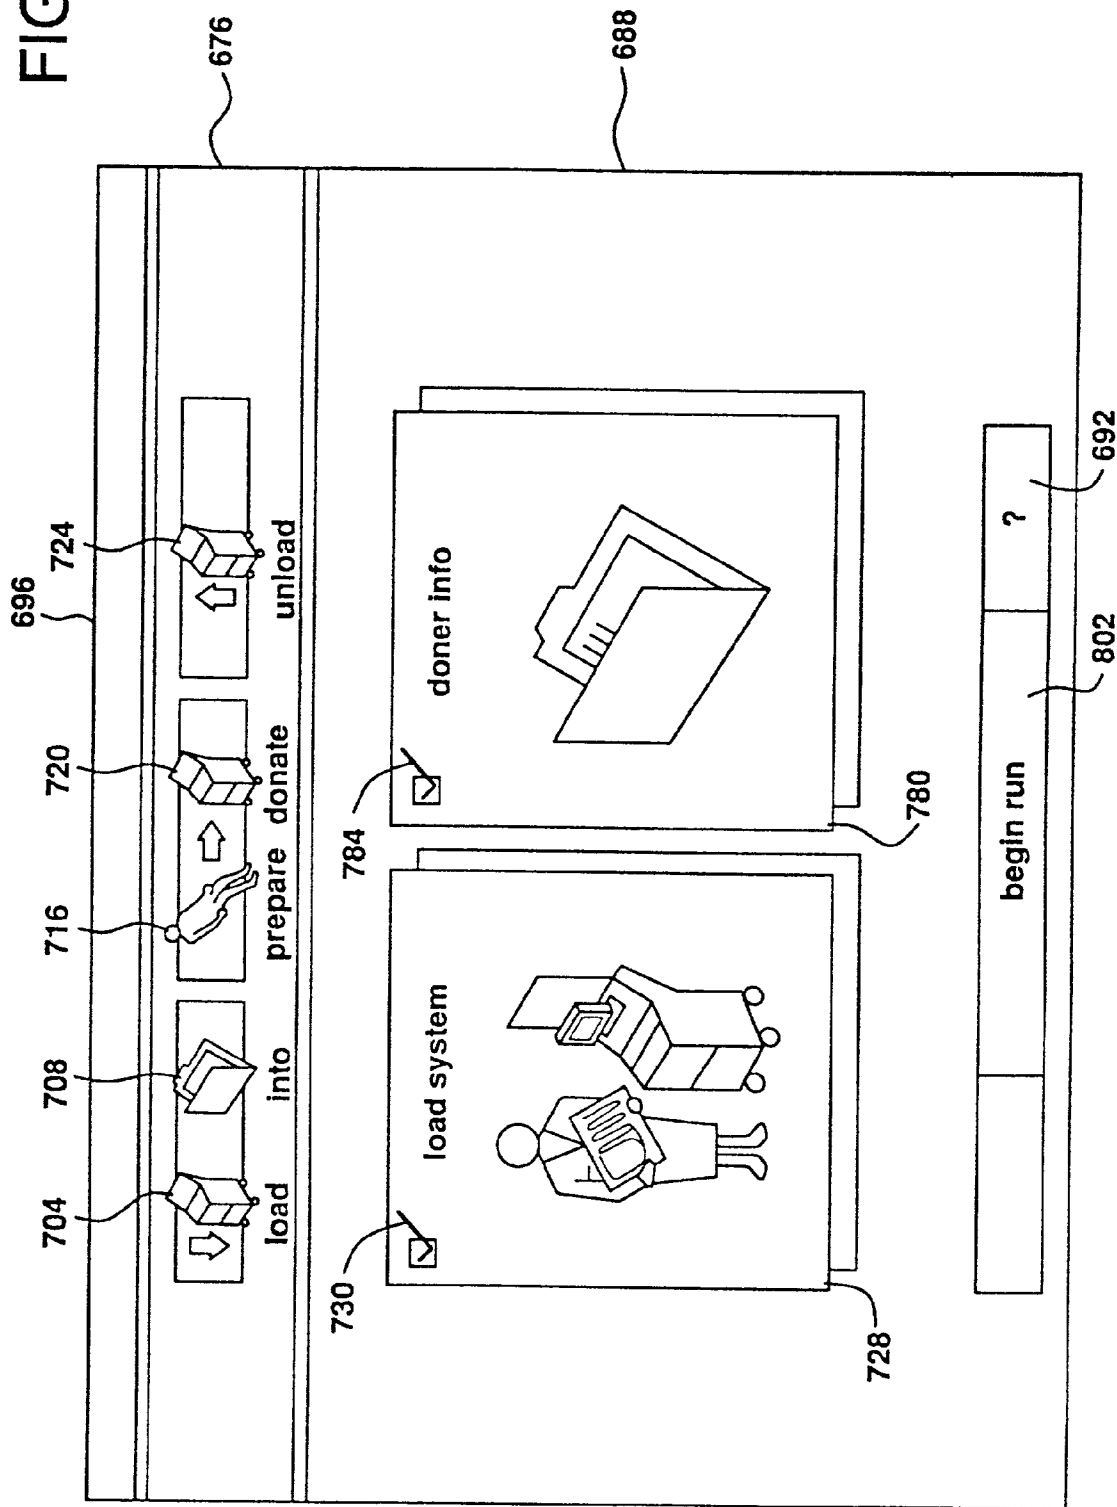
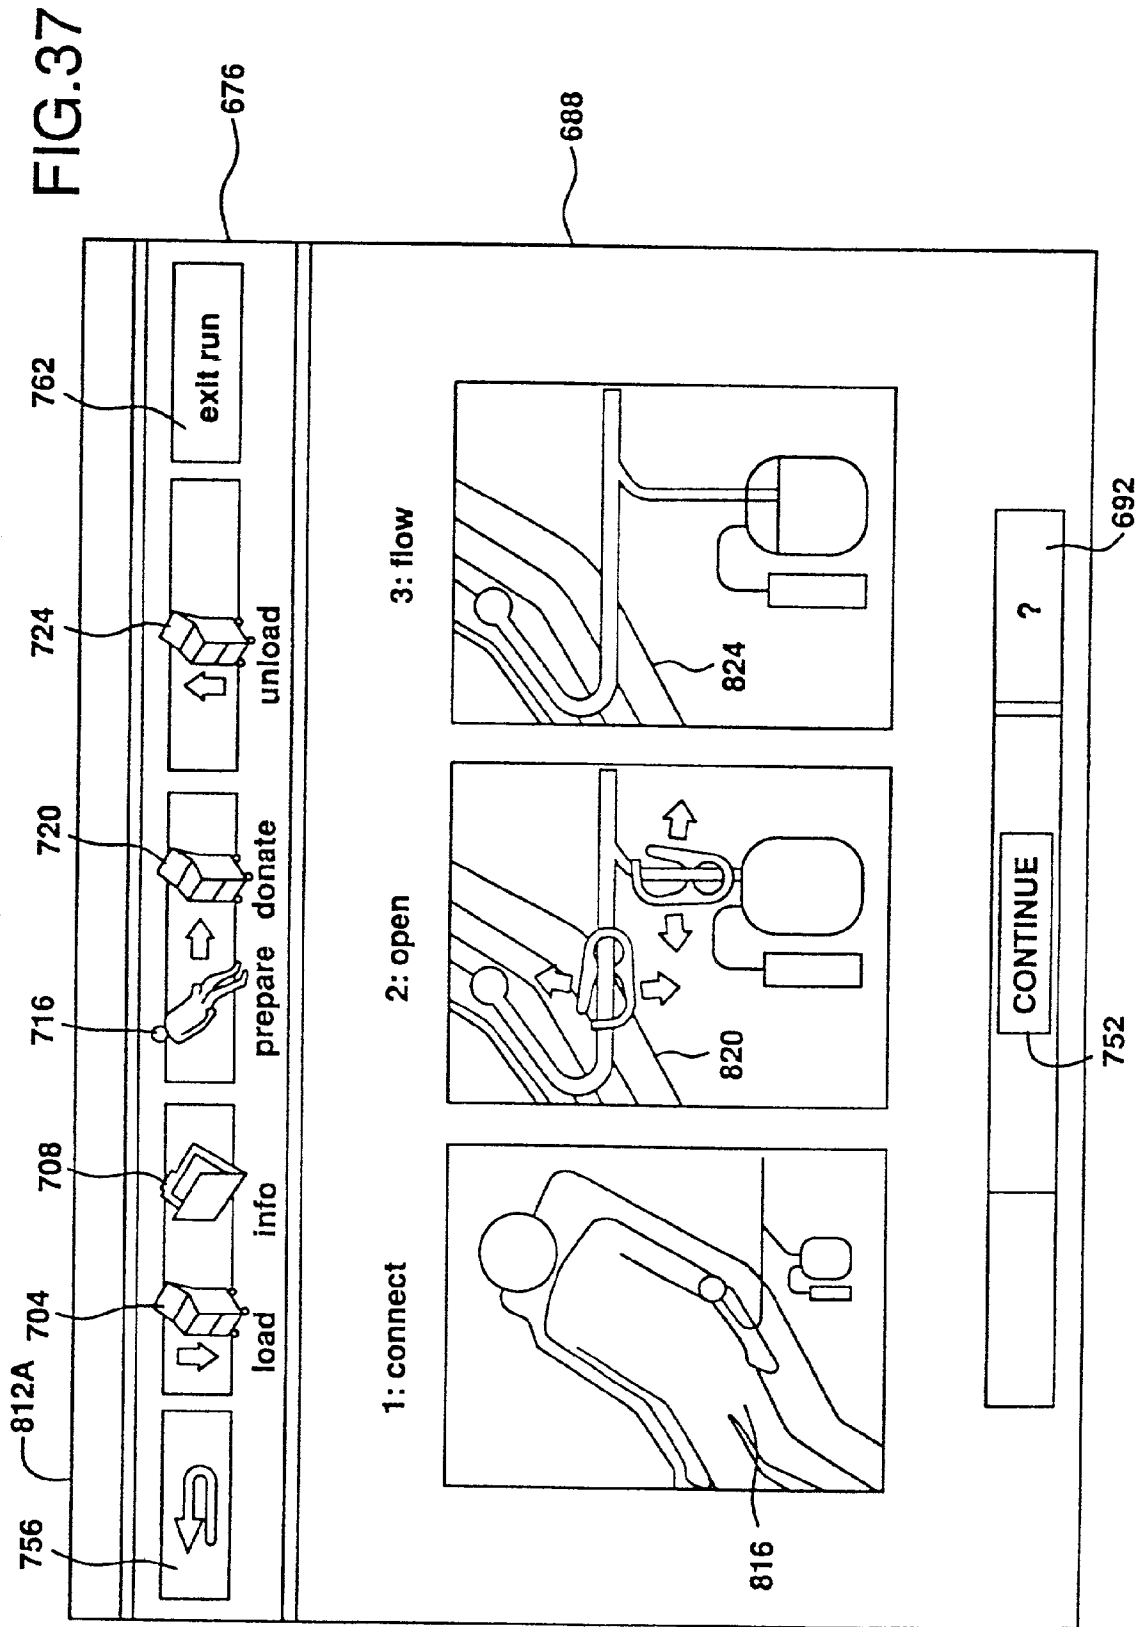
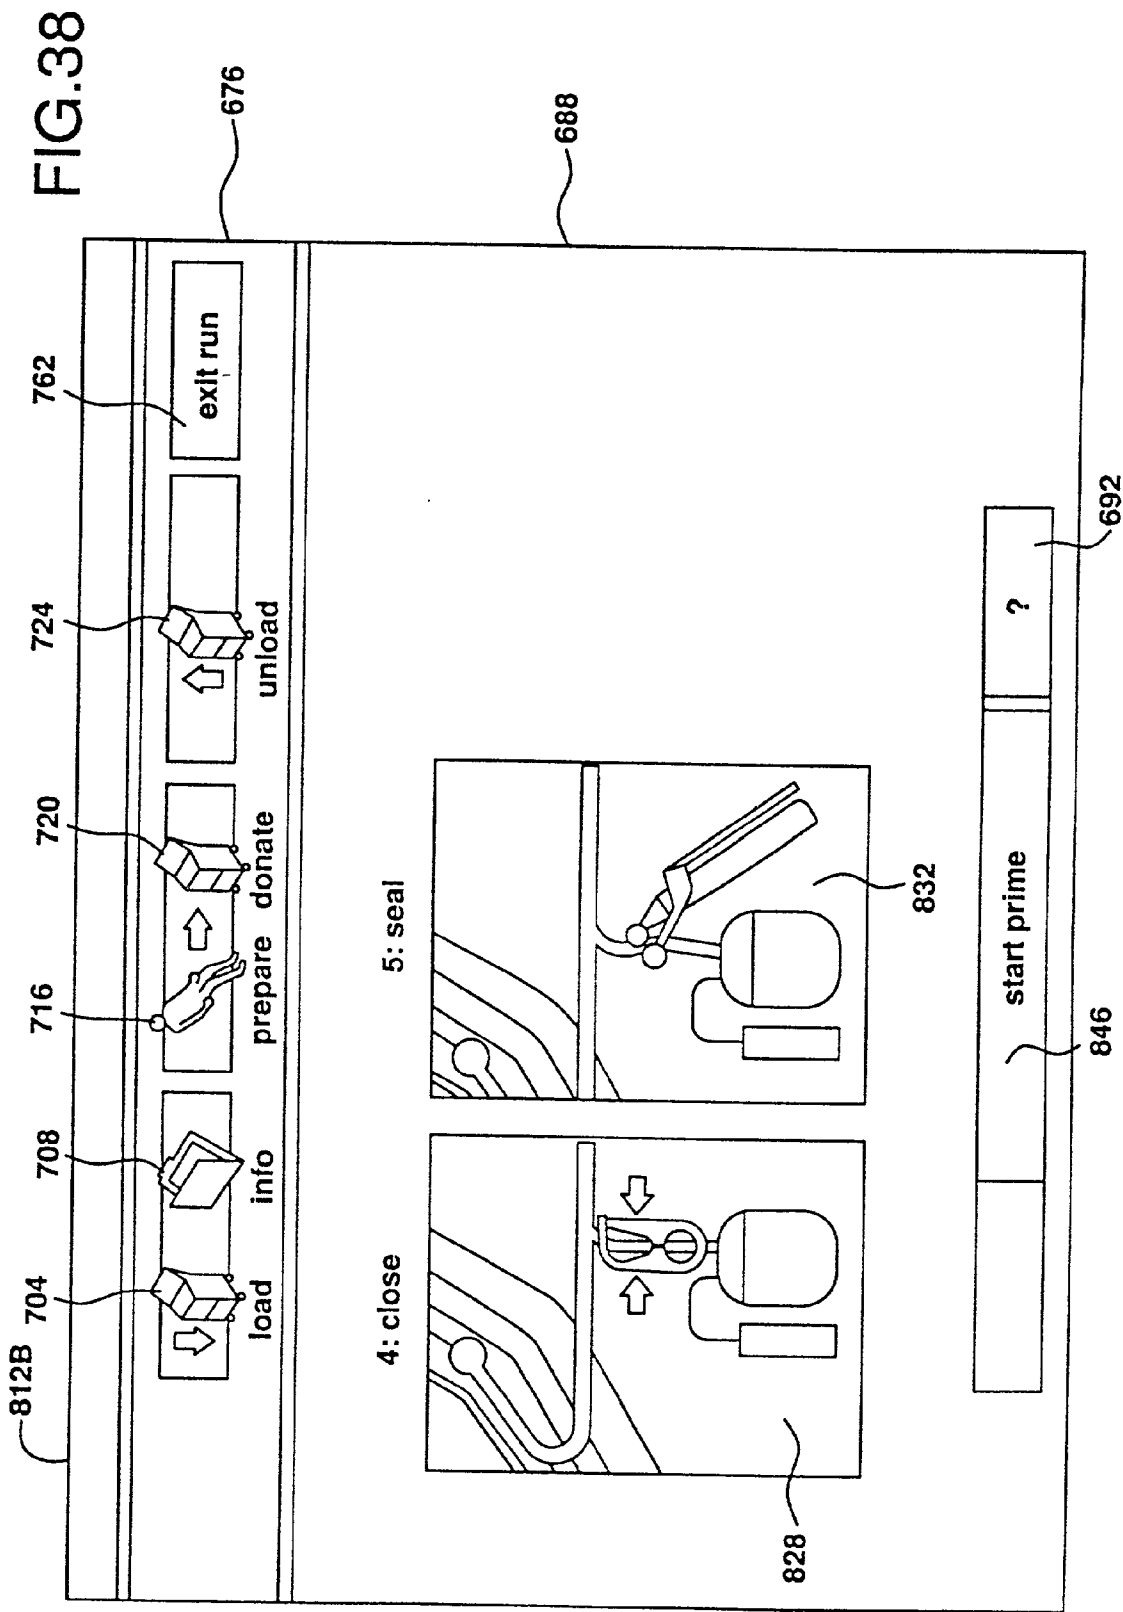


FIG.36







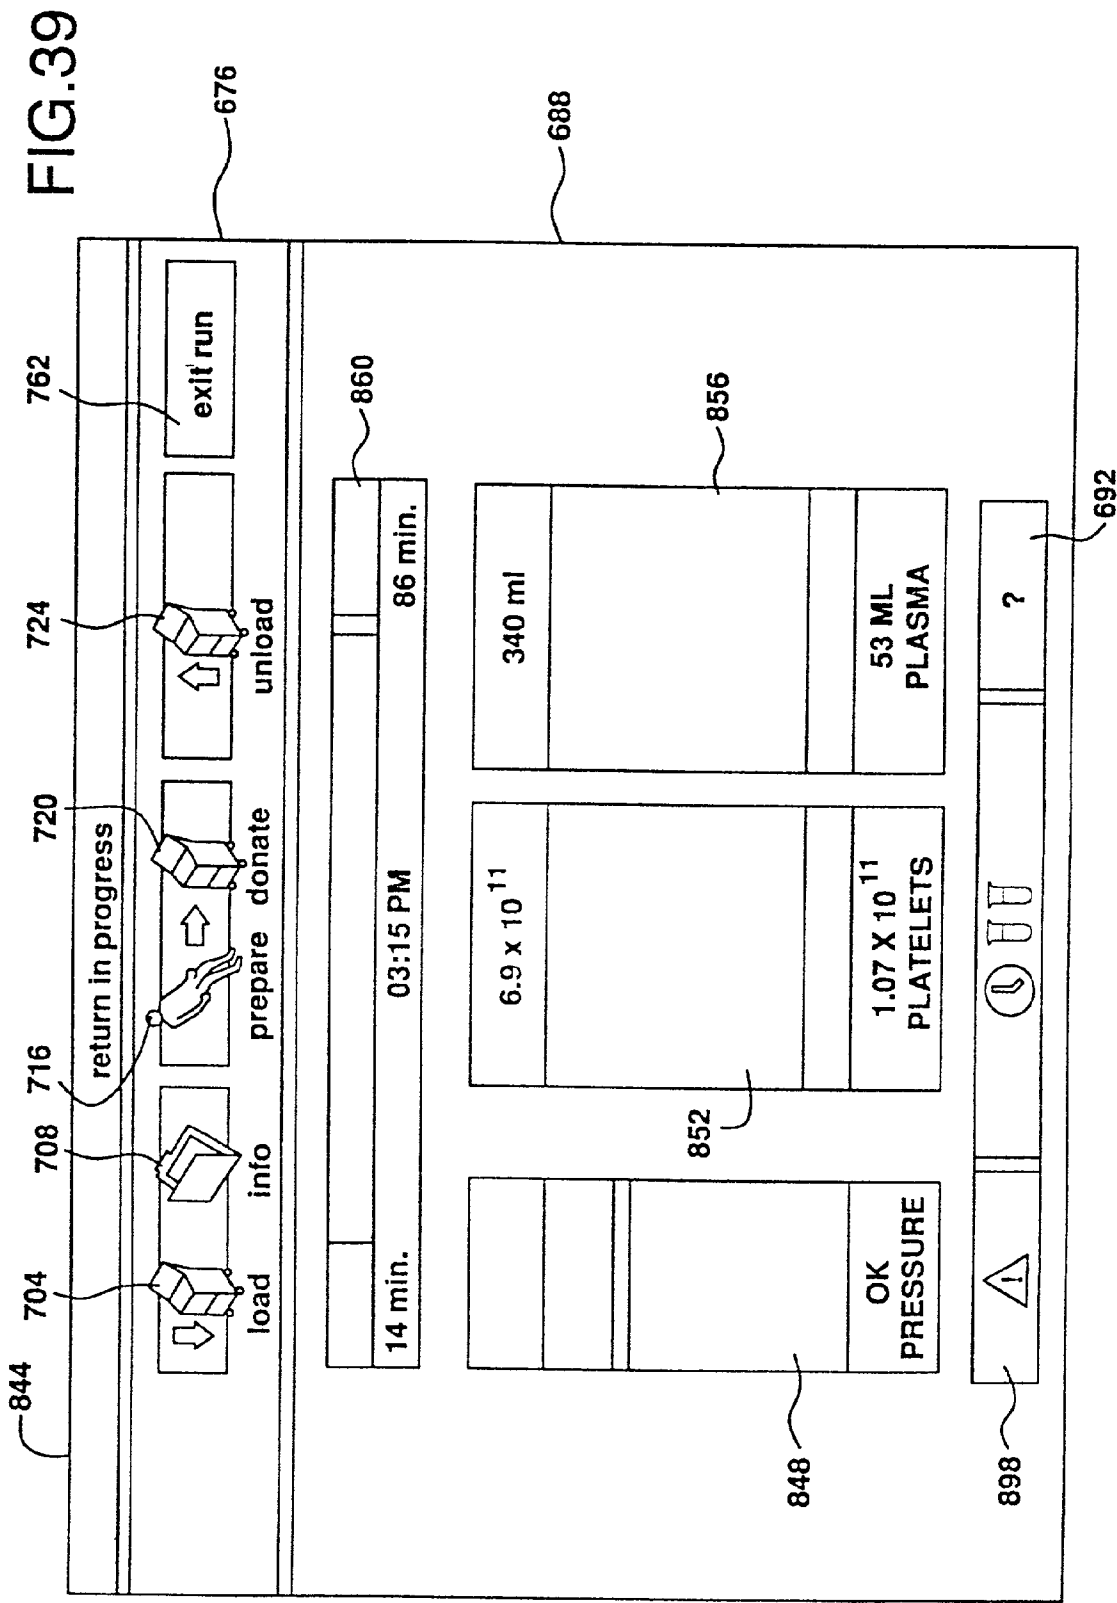
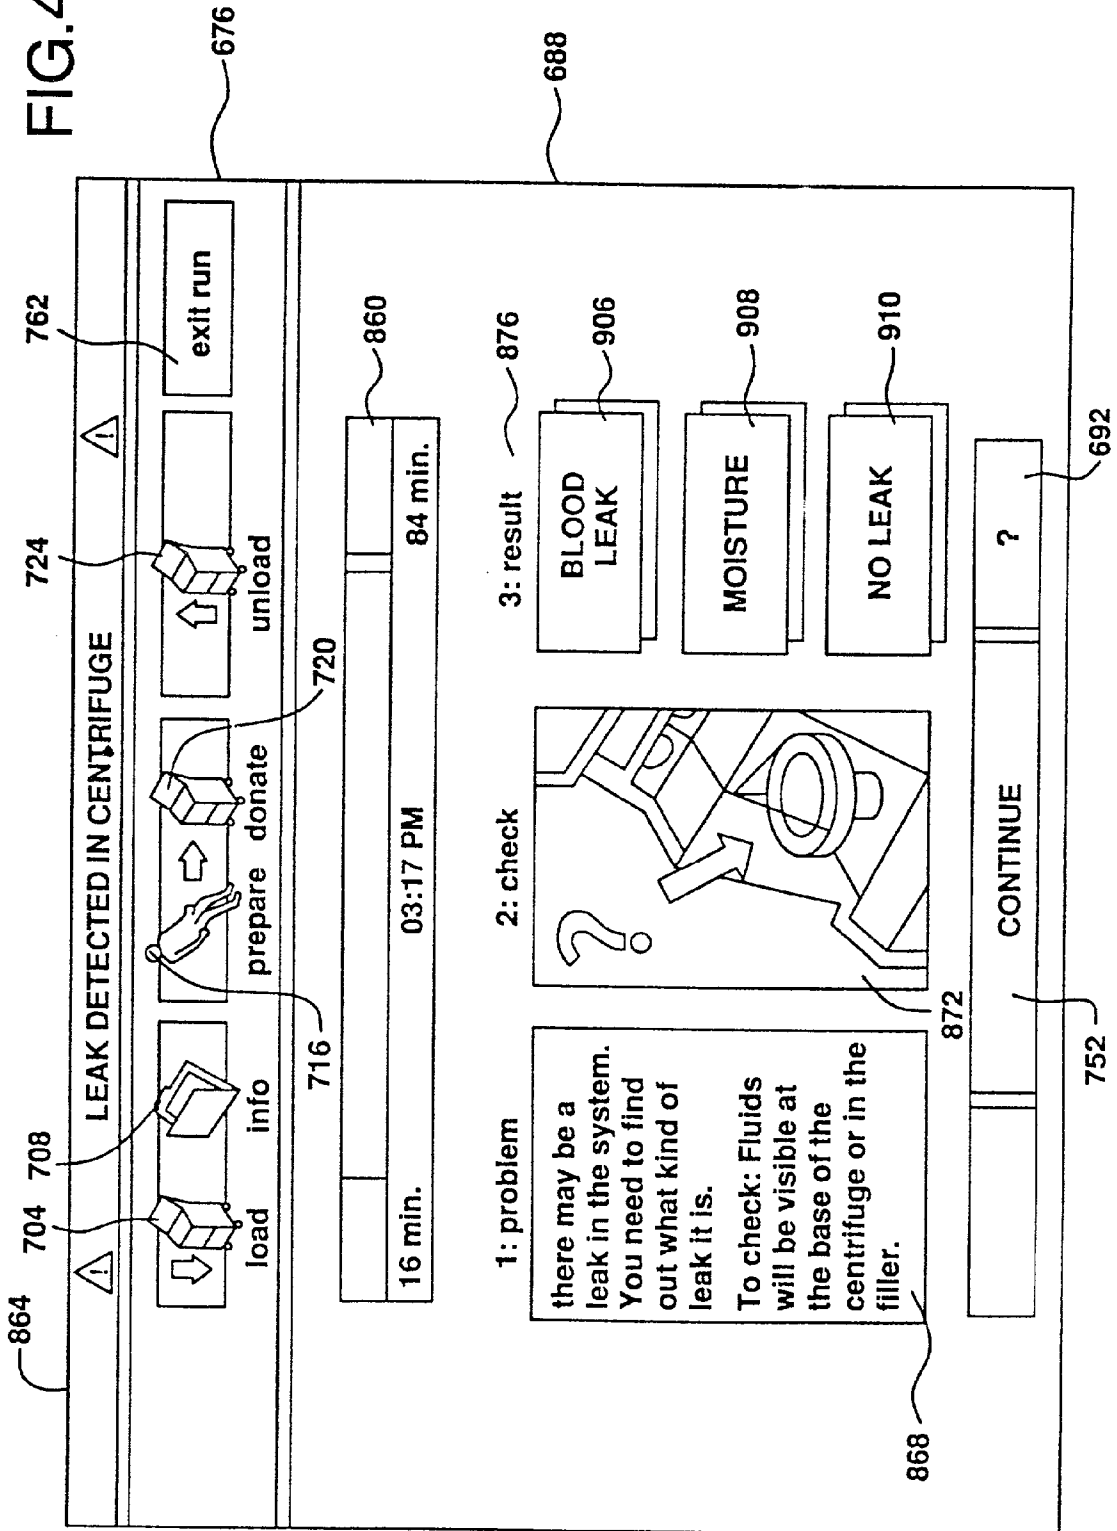
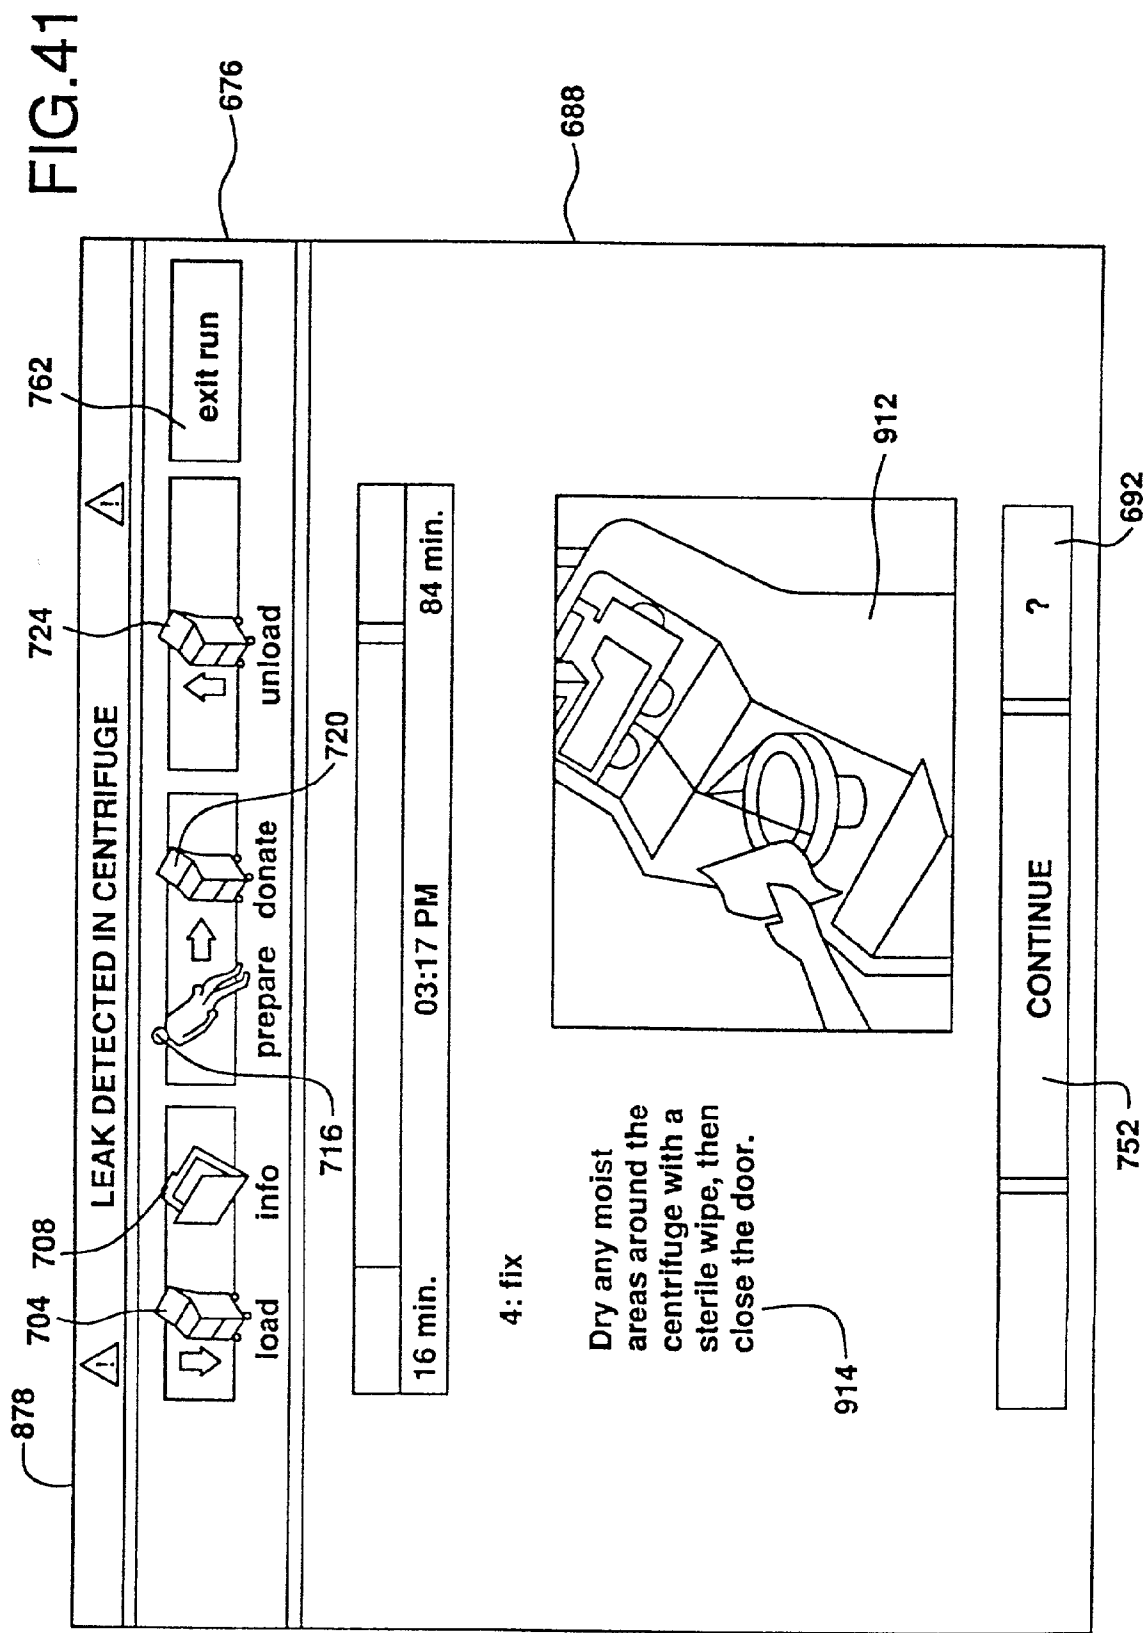
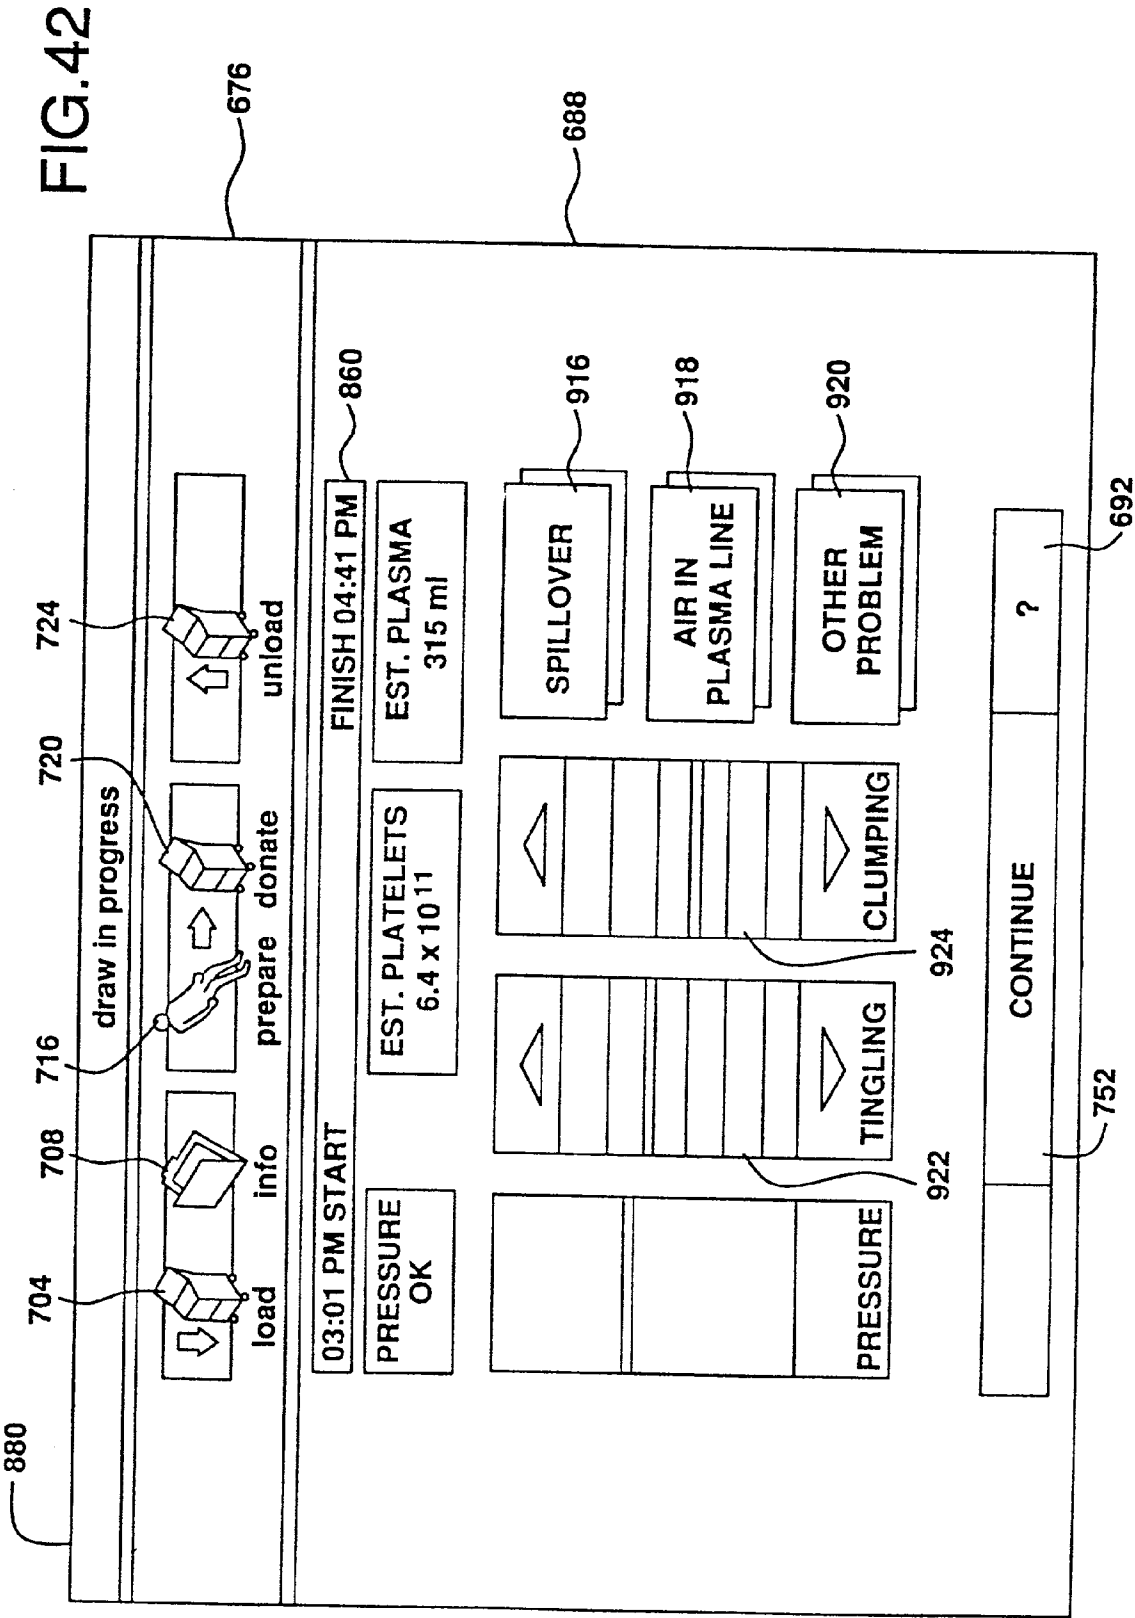
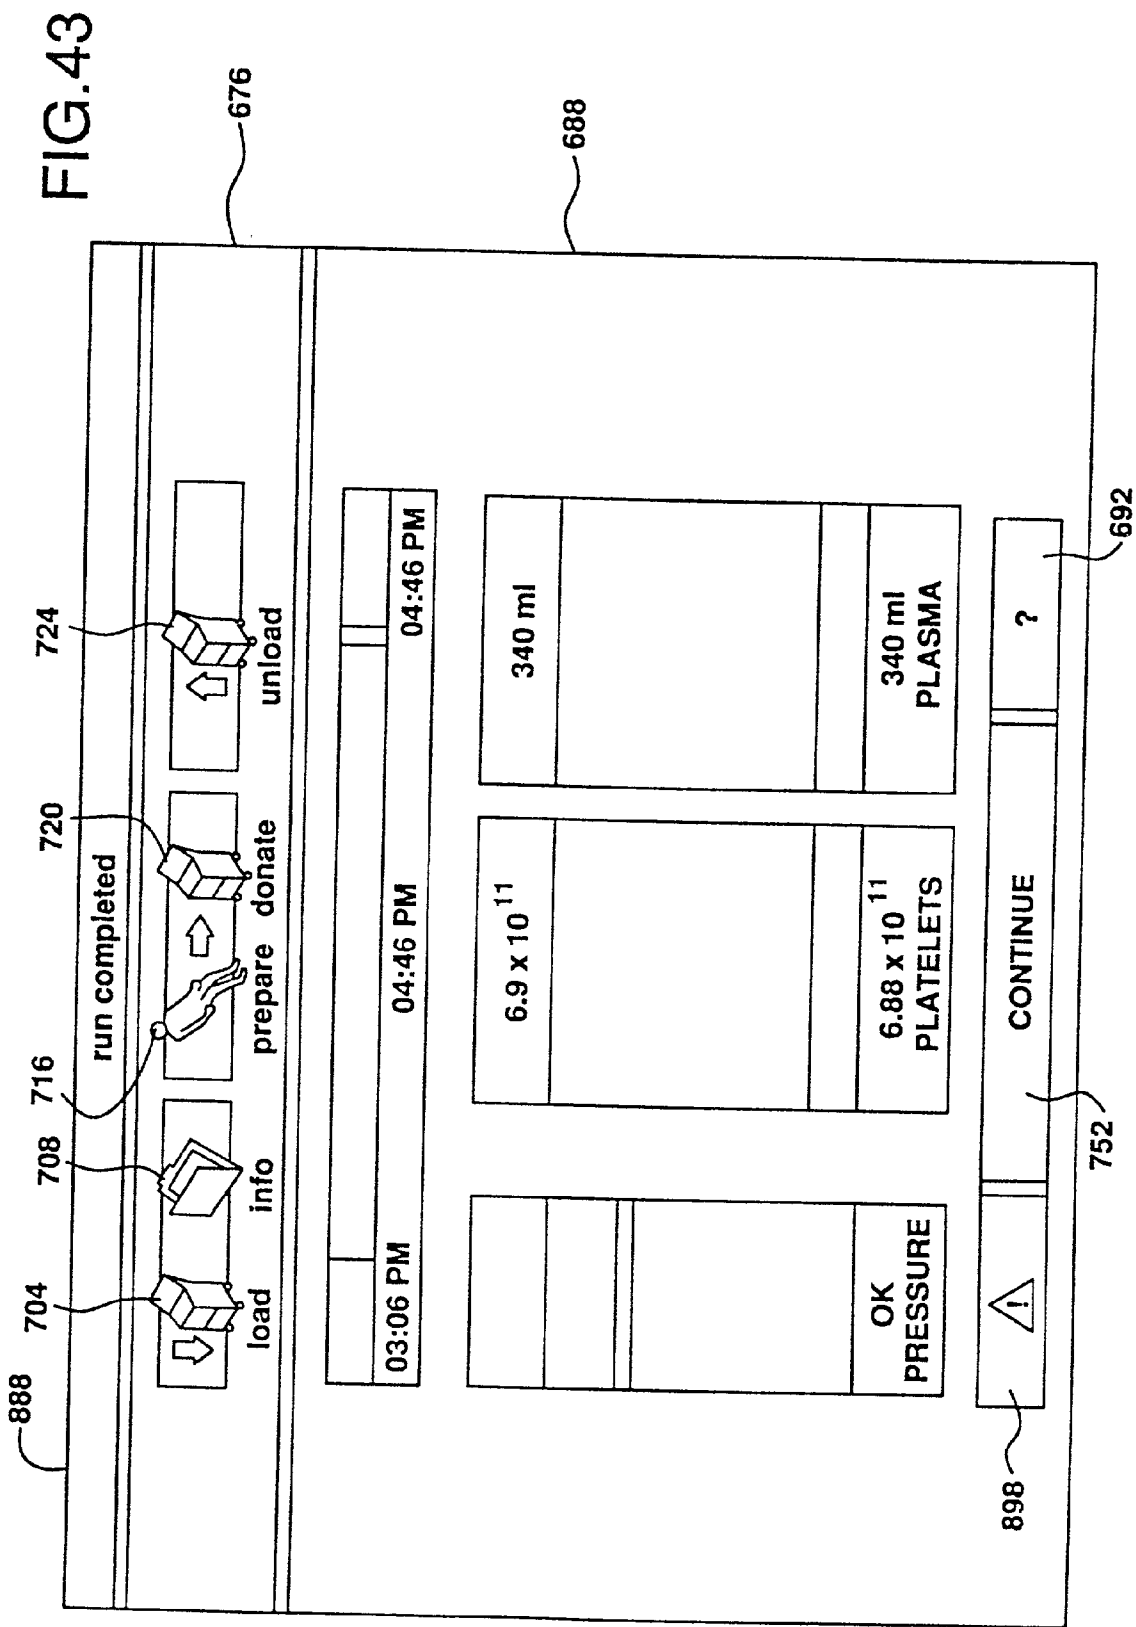


FIG. 40










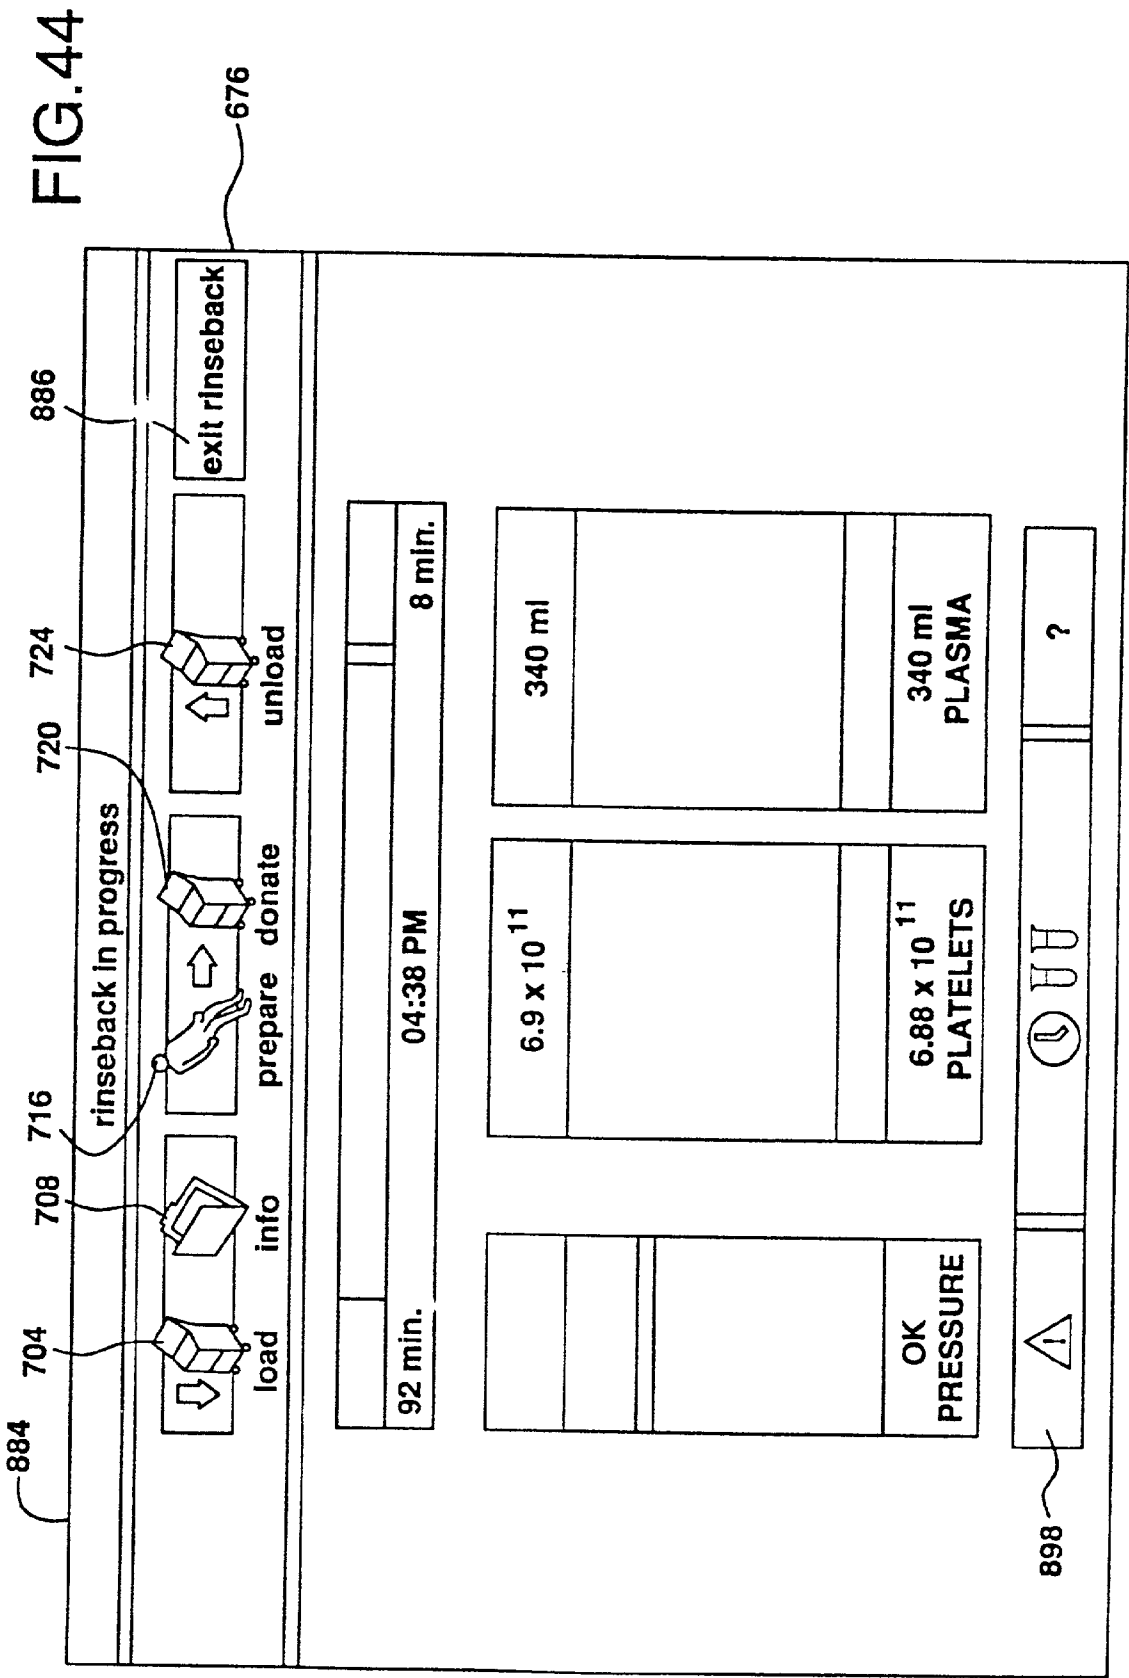


FIG. 45

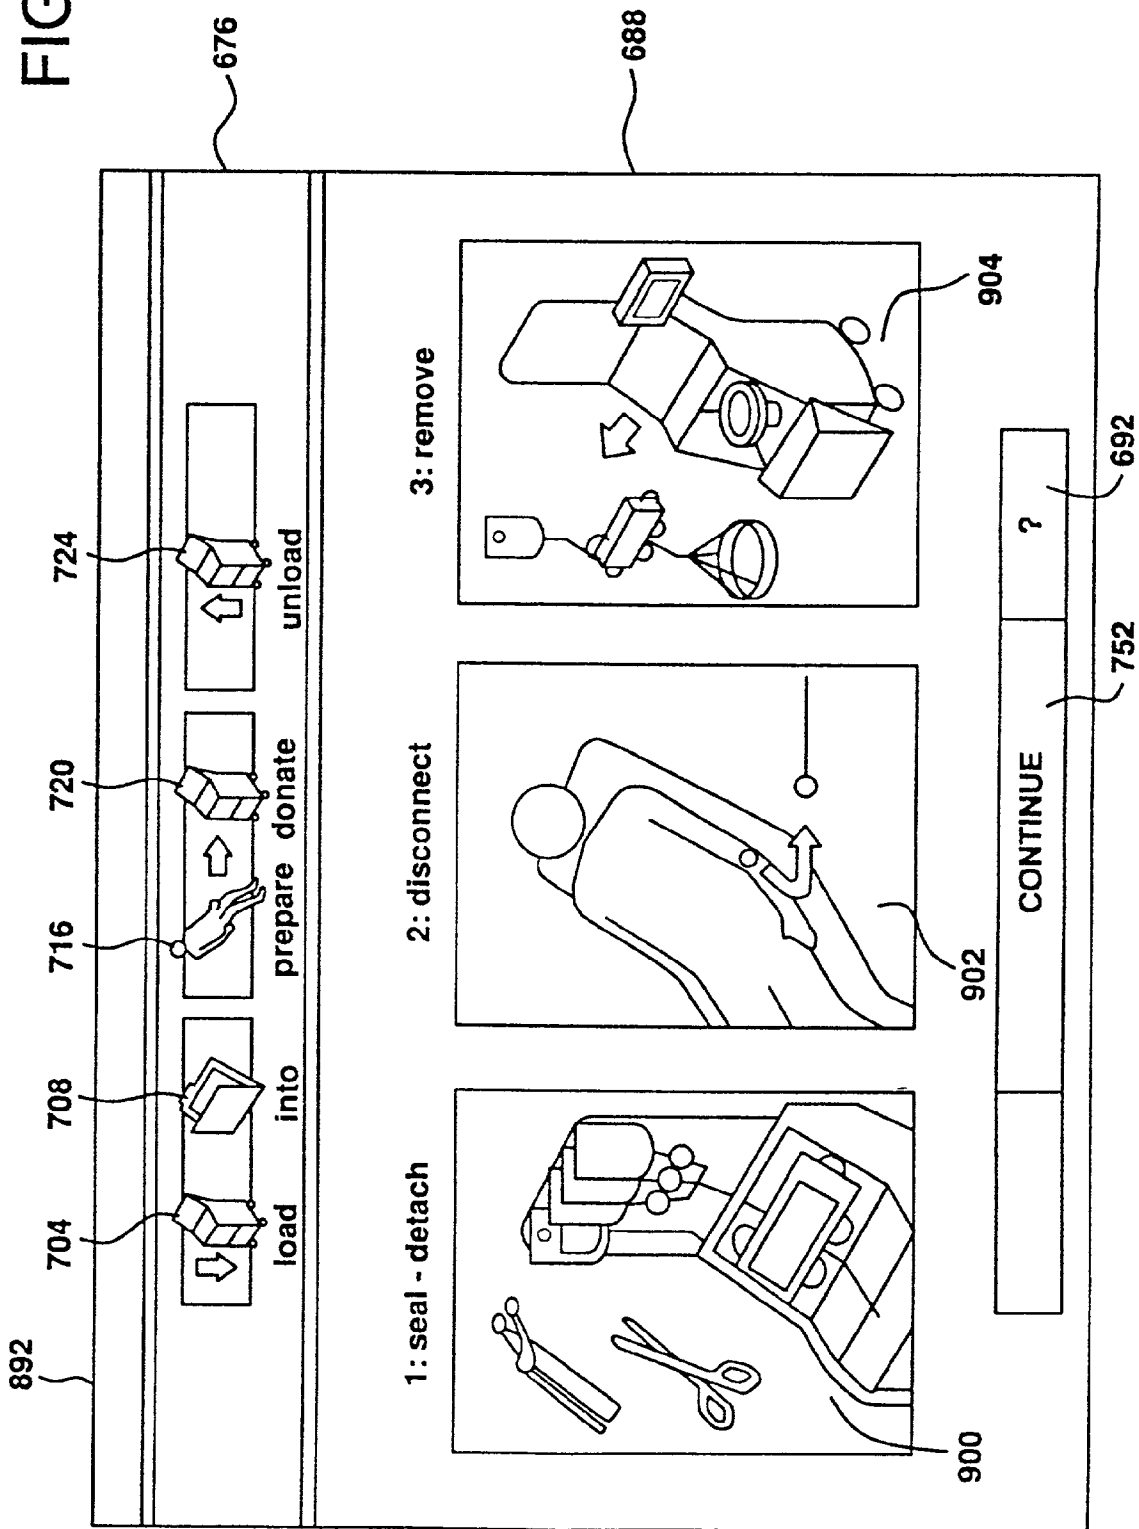

EXTRACORPOREAL BLOOD PROCESSING METHODS AND APPARATUS

[0001] This patent application claims the benefit of U.S. Provisional Patent Application No. 60/188,133; filed Mar. 09, 2000.

FIELD OF THE INVENTION

[0002] The present invention generally relates to the field of extracorporeal blood processing and, more particularly, to methods and apparatus which may be incorporated into an apheresis system useful for blood component collection, or for therapeutic purposes.

BACKGROUND OF THE INVENTION

[0003] One type of extracorporeal blood processing is an apheresis procedure in which blood is removed from a donor or patient (hereafter, donor/patient), directed to a blood component separation device (e.g., centrifuge), and separated into various blood component types (e.g., red blood cells, white blood cells, platelets, plasma) for collection and/or therapeutic purposes. One or more of these blood component types are collected (e.g., for therapeutic transfusion purposes), while the remainder are preferably returned to the donor or donor/patient.

[0004] A number of factors may affect the commercial viability of an apheresis system. One factor relates to the operator of the system, specifically the time and/or expertise required of an individual to prepare and operate the apheresis system. For instance, reducing the time required by the operator to load and unload the disposables, as well as the complexity of these actions, can increase productivity and/or reduce the potential for operator error. Moreover, reducing the dependency of the system on the operator may lead to reductions in operator errors and/or to reductions in the credentials desired/required for the operators of these systems.

[0005] Donor-related factors may also impact the commercial viability of an apheresis system and include donor convenience and donor comfort. For instance, donors typically have a limited amount of time which may be committed to visiting a blood component collection facility for a donation. Consequently, once at the collection facility the amount of the donor's time which is actually spent collecting blood components is another factor which should be considered. This also relates to donor comfort in that many view the actual collection procedure as being somewhat discomforting in that at least one and sometimes two access needles are disposed in the donor throughout the procedure.

[0006] Performance-related factors continue to affect the commercial viability of an apheresis system. Performance may be judged in terms of the "collection efficiency" of the apheresis system, which may in turn reduce the amount of donation time and thus increase donor convenience. The "collection efficiency" of a system may of course be gauged in a variety of ways, such as by the amount of a particular blood component type which is collected in relation to the quantity of this blood component type which passes through the apheresis system. Performance may also be evaluated based upon the effect which the apheresis procedure has on the various blood component types. For instance, it is desirable to minimize the adverse effects on the blood component types as a result of the apheresis procedure (e.g., reduce platelet activation).

SUMMARY OF THE INVENTION

[0007] The present invention generally relates to extracorporeal blood processing. Since each of the various aspects of the present invention may be incorporated into an apheresis system (e.g., whether for blood component collection in which "healthy" cells and/or plasma are removed from the blood or for therapeutic purposes in which "unhealthy" cells and/or plasma are removed from the blood), the present invention will be described in relation to this particular application. However, at least certain of the aspects of the present invention may be suited for other extracorporeal blood processing applications and such are also within the scope of the present invention.

[0008] A typical apheresis system which may embody one or more aspects of the present invention would generally include a blood component separation device; for example, a membrane-based separation device and/or, a rotatable centrifuge element, such as a rotor, which provides the forces required to separate blood into its various blood component types (e.g., red blood cells, white blood cells, platelets, and/or plasma). In one preferred embodiment, the separation device includes a channel which receives a blood processing vessel. Typically, a healthy human donor or a donor/patient suffering from some type of illness (collectively referred to here as a donor/patient) is fluidly interconnected with the blood processing vessel by an extracorporeal tubing circuit, and preferably the blood processing vessel and extracorporeal tubing circuit collectively define a closed, sterile system. When the fluid interconnection is established, blood may be extracted from the donor/patient and directed to the blood component separation device such that at least one type of blood component may be separated and removed from the blood, either for collection or for therapy.

[0009] When the blood processing vessel is loaded into the channel, the blood processing vessel and most of the tubing lines must be primed. In this regard, an aspect of the present invention relates to priming these elements, preferably with blood. A channel associated with a channel housing, which is rotatably interconnected with a centrifuge rotor, preferably includes a first cell separation stage. The channel extends generally curvilinearly about a rotational axis of the channel housing in a first direction. The channel preferably includes, progressing in the first direction, the first cell separation stage, a red blood cell dam, a platelet and/or a plasma collection area, and an interface control region for controlling a radial position of at least one interface between red blood cells (RBCs) and an adjacent blood component type(s) (e.g., plasma and/or a buffy coat of white blood cells (WBCs), lymphocytes, and platelets). Blood introduced into the channel is separated into layers of red blood cells (and/or a buffy coat generally including white blood cells and platelets), and plasma in the first cell separation stage. Preferably, throughout an RBC/plasma apheresis procedure (e.g., a non-platelet procedure) and including the priming of the blood processing vessel, only separated plasma flows beyond the red blood cell dam where the plasma may be removed from the channel in the plasma collection area. This is provided by an interface control mechanism which is disposed in the interface control region of the channel and which maintains the position of the interface between separated red blood cells and the plasma such that this condition is maintained. Note, the buffy coat (platelets and WBCs) is

also preferably kept behind the RBC dam in the RBC/plasma collection procedures. In this embodiment, the buffy coat is generally collected with the RBCs and may be either later filtered out (e.g., the WBCs by leukoreduction filtration) or left in the RBC product (the platelets).

[0010] Although the term “blood prime” may be subject to a variety of characterizations, in each case described herein, blood is the first fluid introduced into the blood processing vessel. One characterization of the blood prime is that separated plasma is provided to the interface control region before any separated red blood cells would ever flow beyond the red blood cell dam into the plasma collection area. Preferably, no RBCs ever flow over the RBC dam. Another characterization is that blood and/or blood component types occupy the entire fluid-containing volume of the blood processing vessel before any separated red blood cells would flow beyond the red blood cell dam into the plasma collection area.

[0011] A further aspect of the present invention relates to blood priming an apheresis system which includes a channel housing having a blood processing channel associated therewith, a blood processing vessel disposed in the channel and which has a blood inlet port and a red blood cell (RBC) outlet port which also acts as an interface control port. The RBC/interface control port is used to control the radial position of at least one interface between separated red blood cells and a blood component type(s), here preferably plasma, disposed adjacent the separated red blood cells.

[0012] Another aspect of the present invention relates to the RBC/control port which assists in automatically controlling (i.e., without operator action) the location of an interface between the separated red blood cells and the separated plasma relative to a red blood cell dam in the processing vessel. The red blood cell dam restricts the flow of separated red blood cells to a plasma collect port. The RBC/control port extends through the blood processing vessel and removes plasma and red blood cells as required in order to reduce the potential for red blood cells flowing “over” the red blood cell dam to the plasma collect port. The capability of “selective” removal of red blood cells from the blood processing vessel through the RBC/control port is based at least in part upon its position within the channel. That is, the automatic control provided at least in part by the control port is predicated upon the control port assuming a predetermined radial position within the channel. In order to facilitate achieving this predetermined radial position within the channel, the disposition of the control port is provided independently of the thickness of the blood processing vessel. Specifically, the position of the control port is not dependent upon the thickness of the materials which form the blood processing vessel.

[0013] Another aspect of the present invention relates to a packing factor associated with the separated blood component types in a separation stage of the blood processing vessel. The packing factor is a number which reflects the degree with which the blood component types are “packed together” in the separation stage and is dependent at least upon the rotational speed of the channel housing and the flow rate into the blood processing vessel. The packing factor may be characterized as a dimensionless “density” of sorts of the respective blood component type in the respective separation stage. One embodiment of this aspect is a

method which includes the steps of rotating the channel housing, providing a flow to the blood processing vessel in the channel housing (e.g., the flow includes blood and typically anticoagulant as well), separating the blood into a plurality of blood component types, and adjusting the rotational speed of the channel housing based upon a certain change in the flow rate. Since the packing factor is dependent upon the rotational speed of the channel housing and the flow rate into the blood processing vessel, the methodology of this aspect may be used to maintain a substantially constant and predetermined packing factor. In this regard, preferably the packing factor is maintained between about 11 and about 15, and preferably about 13 for collection of RBCs alone and preferably about 16 for collection of RBCs contemporaneously with plasma.

[0014] A further aspect of the present invention relates to the extracorporeal collection of both or either plasma and red blood cells utilizing the same blood processing vessel. More particularly, such a method includes flowing blood from a donor/patient to a blood processing vessel and separating plasma from the blood within the blood processing vessel. At least a portion of the plasma is collected in a collection reservoir that is separate from the blood processing vessel. Further, such a method may include separating red blood cells from the blood within the blood processing vessel and collecting at least a portion of the separated red blood cells within a red blood cell collection reservoir that is also separate from blood processing vessel. In one approach, the collection of plasma and red blood cells may be advantageously completed contemporaneously, although they may also be collected during separate time periods. For example, plasma collection may be completed prior to red blood cell collection. Alternatively, red blood cell collection may precede plasma collection. Note, in a continuous apheresis process, the steps of separating and collecting may be performed substantially simultaneously.

[0015] In conjunction with this aspect of the present invention, and prior to the step of collecting red blood cells, the method may further include a set-up phase during which a desired packing factor is established within the separated red blood cells in the blood processing vessel and a desired AC ratio may be established. Preferably, such a packing factor is established to be between about 11 and 21, and most preferably at about 13 for collection of RBCs alone and 16 for collection of RBCs contemporaneously with plasma. Further, it is preferable that the AC ratio be established to be between about 6 and 16, and most preferably at about 8. The method may further include removing blood from a donor/patient and returning uncollected components of the blood to the donor/patient via use of a single needle. Such removing and returning steps may be alternately and repeatedly carried out during blood processing, including during the set-up and collection phases for red blood cell collection. If the collection of plasma alone is desired, the method may further include separating plasma from the blood within the blood processing vessel and collecting at least a portion of the separated plasma in a separate plasma collection reservoir. Most preferably, plasma separation/collection may be completed contemporaneous with the separation/collection of RBCs. Alternatively or additionally, plasma separation/collection may be completed before or after the separation/collection of RBCs. The use of a replacement fluid is also contemplated during collection and/or may be used in a

substantially continuous (including cycled for single needle draw/return alternating applications) or in a bolus form.

[0016] Moreover, another aspect of the present invention involves the presentation of versatility in providing virtually any option for the collection of red blood cell, plasma and/or platelet products. More specifically, the present system can be operated such that upon input of the donor characteristics (e.g., height, weight, hematocrit and platelet pre-count) the present system will return a list optional donations this particular donor can provide. For example, with a sufficient total blood volume (calculated by the body height and weight, e.g.) and hematocrit and platelet pre-count, a donor can produce possibly several alternate and/or a plurality of products; and, the system can determine not only how many and what combinations of products this donor can donate, but also what might be preferred or prioritized by the blood center. A sufficiently large donor may produce one or more red blood cell products and one or more plasma products and/or one or more platelet products. Many variations of product combinations may now be realized. Different tubing and bag set options are also preferably presented for such alternative collection procedures.

[0017] These and other features of the present invention will be made manifest by the detailed description and the attached drawings which are intended to be read in conjunction with each other as set forth below.

BRIEF DESCRIPTION OF THE DRAWINGS

[0018] FIG. 1 is an isometric view of one embodiment of an apheresis system according to the present invention;

[0019] FIGS. 2A-2B illustrate an alternative extracorporeal tubing circuit and cassette assembly thereof for use in the system of FIG. 1;

[0020] FIGS. 2C-2D illustrate another alternative extracorporeal tubing circuit and cassette assembly thereof for use in the system of FIG. 1;

[0021] FIG. 3 is a front view of a pump/valve/sensor assembly for the system of FIG. 1;

[0022] FIGS. 4A-4B are cross-sectional side views of first and second pressure sensing modules of the extracorporeal tubing circuit of FIGS. 2A-2D coupled with corresponding pressure sensors of the pump/valve/sensor assembly of FIGS. 1 and 3;

[0023] FIG. 5 is a cross-sectional side view of the upper and lower ultrasound sensors of the pump/valve/sensor assembly of FIG. 3 coupled with a reservoir of the cassette assembly of the extracorporeal tubing circuit of FIGS. 2A-2D;

[0024] FIG. 6 is a cross-sectional side view of a platelet divert or replacement fluid introduction valve subassembly of the pump/valve/sensor assembly of FIG. 3;

[0025] FIG. 7 illustrates a loading assembly for a cassette mounting plate of the pump/valve/sensor assembly of FIG. 3;

[0026] FIG. 8A is an exploded, isometric view of the channel assembly from the system of FIG. 1 together with a vessel such as that shown in FIGS. 2A-2B;

[0027] FIG. 8B is an exploded, isometric view of a channel assembly as from the system of FIG. 1 together with the vessel of FIGS. 2C-2D;

[0028] FIGS. 9A-9B are top views of the channel housing from the channel assembly of FIG. 8A;

[0029] FIG. 10 is a cross-sectional view taken along line 10-10 of FIG. 9A;

[0030] FIG. 11A is a cutaway, isometric view of the platelet collect well region of the channel housing of FIG. 8A;

[0031] FIG. 11B is a lateral cutaway view, looking upwardly of the platelet collect well region of the channel housing of FIG. 8A;

[0032] FIG. 12 is a cross-sectional view of the channel housing taken along line 12-12 in FIG. 9A;

[0033] FIG. 13 is a cross-sectional view of the channel housing taken along line 13-13 in FIG. 9A;

[0034] FIG. 14A is a top view of the blood inlet port slot, the RBC outlet slot, and the control port slot on the channel housing of FIG. 8A;

[0035] FIG. 14B is a cutaway, isometric view of the whole blood inlet port slot region of the channel housing of FIG. 8A;

[0036] FIG. 14C is a cutaway, isometric view of the control port slot region of the channel housing of FIG. 8A;

[0037] FIG. 15 is a top view of the channel of FIG. 8A illustrating a ratio of the plasma volume to the red blood cell volume;

[0038] FIG. 16 is an isometric view of the blood processing vessel of the channel assembly of FIG. 8A in a disassembled state;

[0039] FIG. 17 is a cross-sectional view of the blood processing vessel at the interconnection;

[0040] FIG. 18 is cross-sectional view of the blood processing vessel taken along lines 18-18 in FIG. 16;

[0041] FIG. 19A is a cutaway, isometric view of the blood inlet port assembly for the blood processing vessel of FIG. 8A;

[0042] FIG. 19B is a longitudinal cross-sectional view of the blood inlet port assembly for the blood processing vessel of FIG. 8A;

[0043] FIG. 19C is a cross-sectional view of the blood inlet port assembly interfacing with the blood processing vessel of FIG. 8A;

[0044] FIG. 19D is an isometric view of the interior of the vane of the blood inlet port of FIG. 19C;

[0045] FIG. 19E is a cutaway, isometric view of blood being introduced into the blood processing vessel of FIG. 8A during an apheresis procedure;

[0046] FIG. 19F is a cross-sectional view of blood being introduced into the blood processing vessel and channel of FIG. 8A during an apheresis procedure;

[0047] FIG. 19G is a cross-sectional view, looking downwardly, of blood being introduced into the blood processing vessel and channel of FIG. 8A during an apheresis procedure;

[0048] FIG. 20A is a cutaway, isometric view of the red blood cell outlet port assembly interfacing with the blood processing vessel of FIG. 8A;

[0049] FIG. 20B is a longitudinal, cross-sectional view of the red blood cell outlet port assembly of FIG. 20A;

[0050] FIG. 20C is a cutaway, isometric view of the red blood cell port assembly interfacing with the blood processing vessel of FIG. 8A during rinseback at the end of an apheresis procedure;

[0051] FIG. 20D is a cross-sectional view, looking downwardly, of the red blood cell outlet port assembly interfacing with the blood processing vessel in the channel of FIG. 8A during rinseback at the end of an apheresis procedure;

[0052] FIG. 21A is a cross-sectional view of the platelet outlet port assembly for the blood processing vessel of FIG. 8A;

[0053] FIG. 21B is a plan view of the platelet outlet port assembly of FIG. 21A from the interior of the channel;

[0054] FIG. 22 is a cutaway, isometric view of the plasma port assembly for the blood processing vessel of FIG. 8A;

[0055] FIG. 23A is a cutaway, isometric view of the control port assembly for the blood processing vessel of FIG. 8A;

[0056] FIG. 23B is a cross-sectional view of the control port assembly interfacing with the blood processing vessel of FIG. 8A;

[0057] FIG. 24 is an isometric view of a centrifuge rotor assembly for the system of FIG. 1;

[0058] FIG. 25A is a longitudinal cross-sectional view of the rotor assembly of FIG. 24;

[0059] FIG. 25B is a top view of the rotor body of the rotor assembly of FIG. 24;

[0060] FIG. 25C is a top view of the rotor body of the rotor assembly of FIG. 24 with the upper counterweight removed so as to illustrate the lower counterweight;

[0061] FIG. 25D is a front view of the rotor body of FIG. 24;

[0062] FIG. 25E is an isometric view of the left side of the blood processing vessel aperture in the rotor body of FIG. 24;

[0063] FIG. 25F is a cross-sectional view of the rotor body of FIG. 24;

[0064] FIG. 26 is a "master screen" for the computer graphics interface of the apheresis system of FIG. 1;

[0065] FIG. 27 is a "loading procedures screen" for the computer graphics interface of the apheresis system of FIG. 1;

[0066] FIG. 28 is one embodiment of a "help screen" for the loading procedures screen of FIG. 27;

[0067] FIG. 29 is a "disposable pressure test screen" for the computer graphics interface of the apheresis system of FIG. 1;

[0068] FIG. 30 is a "pressure test in progress screen" for the computer graphics interface of the apheresis system of FIG. 1;

[0069] FIG. 31 is a "AC interconnect screen" for the computer graphics interface of the apheresis system of FIG. 1;

[0070] FIG. 32 is the "master screen" of FIG. 26 which has been updated to reflect completion of the loading of the disposables;

[0071] FIG. 33 is a "donor/patient data screen" for the computer graphics interface of the apheresis system of FIG. 1;

[0072] FIG. 34 is a "weight input screen" for the computer graphics interface of the apheresis system of FIG. 1;

[0073] FIG. 35 is a "lab data screen" for the computer graphics interface of the apheresis system of FIG. 1;

[0074] FIG. 36 is the "master screen" of FIG. 26 which has been updated to reflect completion of the donor/patient preps;

[0075] FIG. 37 is a first "donor/patient preps screen" for the computer graphics interface of the apheresis system of FIG. 1;

[0076] FIG. 38 is a second "donor/patient preps screen" for the computer graphics interface of the apheresis system of FIG. 1;

[0077] FIG. 39 is a "run screen" for the computer graphics interface of the apheresis system of FIG. 1;

[0078] FIG. 40 is one embodiment of an "alarm screen" for the computer graphics interface of the apheresis system of FIG. 1;

[0079] FIG. 41 is a "supplemental alarm screen" for the alarm screen of FIG. 40;

[0080] FIG. 42 is one embodiment of a "trouble shooting screen" for the computer graphics interface of the apheresis system of FIG. 1;

[0081] FIG. 43 is a "final run data display screen" for the computer graphics interface of the apheresis system of FIG. 1;

[0082] FIG. 44 is a "rinseback screen" for the computer graphics interface of the apheresis system of FIG. 1; and

[0083] FIG. 45 is an "unload screen" for the computer graphics interface of the apheresis system of FIG. 1.

DETAILED DESCRIPTION

[0084] The present invention will be described in relation to the accompanying drawings which assist in illustrating the pertinent features hereof. Generally, all preferred aspects of the present invention relate to improvements in a blood apheresis system, both procedural and structural. However, certain of these improvements may be applicable to other extracorporeal blood processing applications and such are within the scope of the present invention as well.

[0085] A preferred blood apheresis system 2 is illustrated in FIG. 1 and preferably provides for a continuous blood component separation process. Generally, whole blood is withdrawn from a donor/patient 4 and is provided to a blood component separation device 6 where the blood is separated into the various component types and at least one of these separated blood component types is collected by and/or removed from the device 6. These collected blood components may then be provided for subsequent use by another such as by transfusion and/or may be removed in favor of the delivery or infusion of replacement fluid(s) for therapeutic or non-therapeutic purposes, or may undergo a therapeutic treatment and be returned to the donor/patient 4.

[0086] In the blood apheresis system 2, blood is withdrawn from the donor/patient 4 and directed through a disposable set 8 which includes an extracorporeal tubing circuit 10 and a blood processing vessel 352 and which defines a completely closed and sterile system. The disposable set 8 is mounted on the blood component separation device 6 which includes a pump/valve/sensor assembly 1000 for interfacing with the extracorporeal tubing circuit 10, and a channel assembly 200 for interfacing with the disposable blood processing vessel 352.

[0087] The channel assembly 200 includes a channel housing 204 which is rotatably interconnected with a rotatable centrifuge rotor assembly 568 which provides the centrifugal forces required to separate blood into its various blood component types by centrifugation. The blood processing vessel 352 is interfitted with the channel housing 204. Blood thus flows from the donor/patient 4, through the extracorporeal tubing circuit 10, and into the rotating blood processing vessel 352. The blood within the blood processing vessel 352 is separated into various blood component types and at least one of these blood component types (e.g., plasma, red blood cells) may preferably be continually removed from the blood processing vessel 352. Blood components which are not being collected for transfusion to a distinct recipient, or for therapeutic exchange or treatment (e.g., red blood cells, white blood cells, plasma, as described hereinbelow) are also removed from the blood processing vessel 352 and returned to the donor/patient 4 via the extracorporeal tubing circuit 10. A continuous process here preferably includes at least a continuously spinning/rotating vessel 352, and may also include continuous inflow of blood and/or outflow of separated products.

[0088] Operation of the blood component separation device 6 is preferably controlled by one or more processors included therein, and may advantageously comprise a plurality of embedded processors. Such processors may be like those used in personal computers or the like, and/or preferably accommodate interface capabilities with ever-increasing computer user facilities (e.g., CD ROM, modem, audio, networking and other capabilities). Relatedly, in order to assist the operator of the apheresis system 2 with various aspects of its operation, the blood component separation device 6 preferably includes a graphical interface 660 preferably with a touch screen input/output device 664.

[0089] Disposable Set: Extracorporeal Tubing Circuit

[0090] As illustrated in the alternative embodiments shown in FIGS. 2A-2D, a blood-primable extracorporeal tubing circuit 10 preferably includes a cassette assembly 110 and a number of tubing assemblies 20, 50, 60, 80, 90, 100,

950 and/or 960 interconnected therewith. Generally, blood removal/return tubing assembly 20 provides a single needle interface between a donor/patient 4 and cassette assembly 110, and blood inlet/blood component tubing subassembly 60 provides the interface between cassette assembly 110 and blood processing vessel 352. As shown in the embodiment of FIGS. 2A-2B, an anticoagulant tubing assembly 50, platelet collection tubing assembly 80, plasma collection tubing assembly 90, red blood cell collection assembly 950 and vent bag tubing subassembly 100 may be interconnected with cassette assembly 110. As shown alternatively in the embodiment of FIGS. 2C and 2D, a variation of RBC assembly 950 may be included, as well as a replacement fluid assembly 960 substituted generally in place of the platelet assembly 80 of the embodiment of FIGS. 2A and 2B. As will be appreciated, the extracorporeal tubing circuit 10 and blood processing vessel 352/352a are interconnected to combinatively yield a closed disposable assembly 8 for a single use. Note that differences between the two primary alternative tubing sets disclosed herein will be addressed as they arise in the course of the following description. Similarities, on the other hand, are numerous and are not uniformly described as such hereinbelow.

[0091] The blood removal/return tubing assembly 20 includes a needle subassembly 30 interconnected with blood removal tubing 22, blood return tubing 24 and anticoagulant tubing 26 via a common manifold 28. The needle subassembly 30 includes a needle 32 having a protective needle sleeve 34 and needle cap 36, and interconnect tubing 38 between needle 32 and manifold 28. Needle subassembly 30 preferably further includes a D sleeve 40 and tubing clamp 42 positioned about the interconnect tubing 38. Blood removal tubing 22 may be provided with a Y-connector 44 interconnected with a blood sampling subassembly 46.

[0092] Cassette assembly 110 includes front and back molded plastic plates 112 and 114 (see also FIGS. 4A, 4B and 5) that are hot-welded together to define a rectangular cassette member 115 having integral fluid passageways. The cassette assembly 110 further includes a number of outwardly extending tubing loops interconnecting various integral passageways. The integral passageways are also interconnected to the various tubing assemblies.

[0093] Specifically, cassette assembly 110 includes a first integral anticoagulant passageway 120a interconnected with the anticoagulant tubing 26 of the blood removal/return tubing assembly 20. The cassette assembly 110 further includes a second integral anticoagulant passageway 120b and a pump-engaging, anticoagulant tubing loop 122 between the first and second integral anticoagulant passageways 120a, 120b. The second integral anticoagulant passageway 120b is interconnected with anticoagulant tubing assembly 50. The anticoagulant tubing assembly 50 includes a spike drip chamber 52 connectable to an anticoagulant source, anticoagulant feed tubing 54 and a sterilizing filter 56. During use, the anticoagulant tubing assembly 50 supplies anticoagulant to the blood removed from a donor/patient 4 to reduce or prevent any clotting in the extracorporeal tubing circuit 10.

[0094] Cassette assembly 110 also includes a first integral blood inlet passageway 130a interconnected with blood removal tubing 22 of the blood removal/return tubing assembly 20. The cassette assembly 110 further includes a

second integral blood inlet passageway **130b** and a pump-engaging, blood inlet tubing loop **132** between the first and second integral blood inlet passageways **130a**, **130b**. The first integral blood inlet passageway **130a** includes a first pressure-sensing module **134** and inlet filter **136**, and the second integral blood inlet passageway **130b** includes a second pressure-sensing module **138**. The second integral blood inlet passageway **130b** is interconnected with blood inlet tubing **62** of the blood inlet/blood component tubing assembly **60**.

[0095] Blood inlet tubing **62** is also interconnected with input port **392** of blood processing vessel **352** to provide whole blood thereto for processing, as will be described. To return separated blood components to cassette assembly **110**, the blood inlet/blood component tubing assembly **60**, as shown in FIGS. 2A and 2B, further includes red blood cell (RBC)/plasma outlet tubing **64**, platelet outlet tubing **66** and plasma outlet tubing **68** interconnected with corresponding outlet ports **492** and **520**, **456**, and **420** of blood processing vessel **352**. As shown in the alternative embodiment of FIGS. 2C and 2D, there is no platelet outlet tubing, nor a corresponding outlet port **420**. The RBC/plasma outlet tubing **64** of FIGS. 2A and 2B includes a Y-connector **70** to interconnect tubing spurs **64a** and **64b**. Contrarily, there are no spurs in the FIG. 2C embodiment, rather only a single RBC outlet tubing **64**. Thus, there is also no corresponding plasma/control outlet port **492** in this embodiment. The blood inlet tubing **62**, RBC/plasma outlet tubing **64**, and plasma outlet tubing **68** all pass through first and second strain relief members **72** and **74** and a braided bearing member **76** therebetween. This advantageously allows for a sealless interconnection, as taught in U.S. Pat. No. 4,425,112 to Ito. As shown, multi-lumen connectors **78** can be employed for the various tubing lines.

[0096] Instead of a platelet collection assembly **80** (see the description below), the alternative embodiment shown in FIGS. 2C and 2D preferably has a replacement fluid tubing assembly **960** for delivery of replacement fluid(s) such as sterile saline solution(s) (or replacement/exchange RBCs or plasma, e.g.) to the donor/patient **4** as described in further detail below. As shown, the replacement fluid assembly **960** includes at least a replacement fluid inlet tubing line **962** attached to the cassette **110** in fluid communication with an internal replacement fluid passageway **140c** which is in turn connected to a replacement fluid tubing loop **142a** which is connected back to the cassette **110** and an internal replacement fluid passageway **140d**. These passageways **140c**, **140d** and tubing loop **142a** are as shown, preferably similar structurally to the platelet passageways **140a**, **140b** and loop **142** in FIGS. 2A-2B (see below), though they may take other forms as well. Two further internal passageways or spurs **144c** and **144d** and a tubing loop **146** are also shown in the alternative embodiment of FIGS. 2C-2D; these also are shown as similar to the platelet passageways **144a**, **144b** and loop **146** (see below), but again, may take other forms. Indeed, the alternative internal passageway **144d** of the embodiment of FIGS. 2C-2D is preferably blocked off to disallow any fluid flow therein or therethrough. No outlet tubing line is preferably connected thereto. Though similar structurally in many ways, when referring to the embodiment of FIGS. 2C-2D, the component elements thereof will be referred to as replacement fluid elements as opposed to platelet assembly components. This alternative naming convention will also be used for other component elements

which could be referred to in connection with either the platelet assembly or the replacement fluid assembly; for example, the platelet or replacement fluid inlet pump **1040** (described hereinbelow, see FIG. 3) will be referred to in both contexts using each respective nominative prefix, even though it remains a single pump **1040** which may be used alternately in each of these alternative fashions.

[0097] The replacement fluid assembly **960** further preferably includes one or more spike assemblies **964a-964b** with associated sterile barrier devices **966a-966b** and tubing connection lines **968a-968b** which may be connected to tubing line **962** via a Y-connector **969** as shown. One or more slide clamp(s) **970** may also be included.

[0098] Either the platelet outlet tubing **66** (FIGS. 2A-2B), or the replacement fluid inlet line **962** (FIGS. 2C-2D) of either blood input/blood component tubing assembly **60** may include a cuvette **65** for use in the detection of red blood cells (via an interfacing RBC spillover detector provided on blood component separation device **6**) and interconnects with a first integral platelet passageway **140a** or replacement fluid passageway **140c** of cassette assembly **110**. As will be appreciated, a transparent member could alternatively be integrated into cassette assembly **110** in fluid communication with first integral platelet passageway **140a**, or the replacement fluid passageway **140c** or either plasma passageway **160a** or **160b**, to interface with an RBC spillover detector (see, e.g. U.S. Pat. No. 5,936,714). Further in the embodiment of FIGS. 2A-2B, the platelet outlet tubing **66** also includes a chamber **67** positioned in close proximity to platelet collect port **420** of blood processing vessel **352**. During operation a saturated bed of platelets will form within chamber **67** and advantageously serve to retain white blood cells within chamber **67**. The embodiment of FIGS. 2C-2D does not preferably have such a chamber because it does not have a corresponding platelet collection assembly **80**.

[0099] The cassette assembly **110** further includes a pump-engaging, platelet or replacement fluid inlet tubing loop **142** or **142a** interconnecting the first respective integral platelet or replacement fluid passageway **140a** or **140c** and a second integral platelet or replacement fluid passageway **140b** or **140d**. The second integral platelet or replacement fluid passageway **140b** or **140d** includes first and second spurs **144a** and **144b**, or **144c**, **144d** respectively. The first spur **144a** is, in the embodiment of FIGS. A-2B, interconnected with platelet collection tubing assembly **80**. And, as introduced above, the corresponding first spur **144c** of the embodiment of FIGS. 2C-2D is preferably not connected to any external tubing system and preferably does not allow fluid flow therethrough. The platelet collection tubing assembly **80** of FIGS. 2A-2B can receive separated platelets during operation and includes platelet collector tubing **82** and platelet collection bags **84** interconnected thereto via a Y-connector **86**. Slide clamps **88** are provided on platelet collector tubing **82**.

[0100] The second spur **144b** of the second integral platelet passageway **140b** (FIGS. 2A-2B) is interconnected with platelet return tubing loop **146** of the cassette assembly **110** to return separated platelets to a donor/patient **4** (e.g., upon detection of RBC spillover during platelet collection). For such purpose, platelet return tubing loop **146** is interconnected to the top of a blood return reservoir **150** integrally

formed by the molded front and back plates **112**, **114** of cassette member **115**. Similarly, the second spur **144c** of the second replacement fluid passageway **140d** (FIGS. 2C-2D) is interconnected with replacement fluid tubing loop **146** to deliver replacement fluid to the cassette reservoir **150** for ultimate delivery to the donor/patient **4**. As will be further described, one or more types of uncollected blood components, collectively referred to as either return blood and/or replacement fluid, will cyclically accumulate in and be removed from reservoir **150** during use. Back plate **114** of the cassette member **115** also includes an integral frame corner **116** defining a window **118** through a corner of cassette member **115**. The frame corner **116** includes keyhole recesses **119** for receiving and orienting the platelet collector tubing **82** and platelet return tubing or replacement loop **146** in a predetermined spaced relationship within window **118**.

[0101] In both of the above-described embodiments, the plasma outlet tubing **68** of blood inlet/blood component tubing assembly **60** interconnects with a first integral plasma passageway **160a** of cassette assembly **110**. Cassette assembly **110** further includes a pump-engaging, plasma tubing loop **162** interconnecting the first integral plasma passageway **160a** and a second integral plasma passageway **160b**. The second integral plasma passageway **160b** includes first and second spurs **164a** and **164b**. The first spur **164a** is interconnected to the plasma collection tubing assembly **90**. The plasma collection tubing assembly **90** may be employed to collect plasma during use and includes plasma collector tubing **92** and plasma collection bag **94**. A slide clamp **96** is provided on plasma collector tubing **92**.

[0102] The second spur **164b** of the second integral plasma passageway **160b** is interconnected to a plasma return tubing loop **166** to return plasma to donor/patient **4**. For such purpose, the plasma return tubing loop **166** is interconnected to the top of the blood return reservoir **150** of the cassette assembly **110**. Again, keyhole recesses **119** in the frame **116** of cassette assembly **110** are utilized to maintain the plasma collector tubing **92** and plasma return tubing loop **166** in a predetermined spaced relationship within window **118**.

[0103] Similarly, in both embodiments, the RBC/plasma outlet tubing **64** of the blood inlet/blood component tubing assembly **60** is interconnected with integral RBCs/plasma passageway **170** of cassette assembly **110**. The integral RBC/plasma passageway **170** includes first and second spurs **170a** and **170b**, respectively. The first spur **170a** is interconnected with RBC/plasma return tubing loop **172** to return separated RBCs/plasma to a donor/patient **4**. For such purpose, the RBC/plasma return tubing loop **172** is interconnected to the top of blood return reservoir **150** of the cassette assembly **110**. The second spur **170b** may be closed off (in a platelet/plasma collection scenario, not shown), or may be connected with an RBC/plasma collection tubing assembly **950** (as shown in either of the embodiments herein) for collecting RBC/plasma during use. RBC collection tubing assembly **950** includes RBC collector tubing **952**, at least one RBC collection reservoir, or bag **954**, and sterile barrier filter/drip spike assembly **956**. The RBC/plasma return tubing loop **172** and RBC/plasma collector tubing **952** is maintained in a desired orientation within window **118** by keyhole recesses **119** of the frame **116**. One or a larger practical number (not shown) of RBC bag(s) **954**

may be connected to the collector tubing **952**. Moreover, although not shown here one or more white blood cell (WBC) filtration devices and/or RBC storage solution connections and/or bags may also be pre-connected to and/or be included as component parts of the RBC collection tubing assembly **950**.

[0104] Vent bag tubing assembly **100** is also interconnected to the top of blood return reservoir **150** of cassette assembly **110**. The vent bag tubing assembly **100** includes vent tubing **102** and a vent bag **104**. During use, sterile air present since packaging within cassette assembly **110**, and particularly within blood return reservoir **150**, cyclically passes into and back out of vent tubing **102** and vent bag **104**, as will be further described.

[0105] Vent bag **104** may be provided with a sterile, gas pressure-relief valve at a top end (not shown). Further, it should be noted that, as opposed to vent bag tubing assembly **100**, additional integral passageways, integrated chambers and tubing loops could be included in cassette assembly **110** to perform the same functions as the vent bag tubing assembly **100**.

[0106] The platelet return tubing replacement fluid loop **146**, plasma return tubing loop **166** and RBC/plasma return tubing loop **172** are interconnected in a row to the top of blood return reservoir **150** immediately adjacent to forwardly projecting sidewalls **152** thereof so that the blood components or replacement fluid(s) returned thereby will flow down the inner walls of the blood return reservoir **150**. The blood return reservoir **150** includes an enlarged, forwardly projecting mid-section **154**, a reduced top section **156** and reduced bottom section **158** (see also FIG. 5). A filter **180** is disposed in a bottom cylindrical outlet **182** of the blood return reservoir **150**.

[0107] A first integral blood return passageway **190a** is interconnected to the outlet **182** of blood return reservoir **150**, and is further interconnected to a second integral blood return passageway **190b** via a pump-engaging, blood return tubing loop **192**. The second integral blood return passageway **190b** is interconnected with the blood return tubing **24** of the blood removal/return tubing assembly **20** to return blood to the donor/patient **4** via needle assembly **30**. The nominative prefix terminology of "blood return" is intended to also include the alternative of replacement fluid(s) delivery throughout this description, as in the blood return or replacement fluid delivery loop **192**.

[0108] As illustrated in FIGS. 2A-2D, pump-engaging tubing loops **122**, **132**, **142**, **162** and **192** extend from cassette member **115** to yield an asymmetric arrangement thereby facilitating proper mounting of cassette assembly **110** on blood component separation device **6** for use. Relatedly, to further facilitate loading of cassette assembly **110**, it is noted that the back plate **114** of cassette member **115** is preferably molded to present a shallow pan-shaped back having a rim extending around the entire periphery and around window **118**, the edge of the rim being substantially coplanar with the back surface of the top, mid and bottom sections **154**, **156**, **158** of reservoir **150** and further defining a recessed region within which first and second pressure sensing modules **134** and **138** project.

[0109] Tubing assemblies **20**, **50**, **60**, **80**, **90**, **100**, **950** and/or **960** are preferably made of PVC tubing and plastic

components that permit visual observation and monitoring of blood/blood components therewithin during use. Cassette assembly 110 is also made of plastic allowing visual observation. It should be noted that thin-walled PVC tubing (e.g., less than about 0.023 inch) may be employed for approved, sterile docking (i.e., the direct connection of two pieces of tubing) for platelet collector tubing 82, plasma collector tubing 92 and RBC/plasma collector tubing 952. Alternately, thicker-walled PVC tubing (e.g., about 0.037 inch or more) may be employed for approved, sterile docking for platelet collector tubing 82, plasma collector tubing 92 and RBC/plasma collector tubing 952, and is otherwise preferably utilized for pump-engaging tubing loops 132, 142, 162 and 192.

[0110] Pump/Valve/Sensor Assembly

[0111] As noted, cassette assembly 110 is mounted upon and operatively interfaces with the pump/valve/sensor assembly 1000 of blood component separation device 6 during use. The pump/valve/sensor assembly 1000 is angled upward at about 45 degrees (see FIG. 1) and as illustrated in FIG. 3 includes a cassette mounting plate 1010, and a number of peristaltic pump assemblies, flow divert valve assemblies, pressure sensors and ultrasonic level sensors interconnected to face plate 6a of blood collection device 6 for pumping, controlling and monitoring the flow of blood/blood components or replacement fluid(s) through extracorporeal tubing circuit 10 during use.

[0112] More particularly, anticoagulant pump assembly 1020 is provided to receive anticoagulant tubing loop 122, blood inlet pump assembly 1030 is provided to receive blood inlet tubing loop 132, platelet or replacement fluid inlet pump assembly 1040 is provided to receive platelet or replacement fluid tubing loop 142, plasma pump assembly 1060 is provided to receive plasma tubing loop 162, and blood return or replacement fluid delivery pump assembly 1090 is provided to receive blood return or replacement fluid delivery tubing loop 192. Each of the peristaltic pump assemblies 1020, 1030, 1040, 1060, and 1090 includes a rotor 1022, 1032, 1042, 1062 and 1092, and raceway 1024, 1034, 1044, 1064, and 1094 between which the corresponding tubing loop is positioned to control the passage and flow rate of the corresponding fluid.

[0113] Platelet divert or replacement fluid valve assembly 1100 is provided to receive platelet collector tubing 82 and platelet return tubing or replacement fluid loop 146, plasma divert valve assembly 1110 is provided to receive plasma collector tubing 92 and plasma return tubing loop 166, and RBC/plasma divert valve assembly 1120 is provided to receive RBC/plasma return tubing loop 172 and RBC/plasma collector tubing 952. As noted above, each pair of tubings for collection or return or replacement of separated blood components is disposed in a predetermined spaced relationship within window 118 of cassette assembly 110, thereby facilitating loading relative to the corresponding divert valve assemblies. As will be further described, platelet divert or replacement fluid valve assembly 1100, plasma divert valve assembly 1110 and RBC/plasma divert valve assembly 1120 each preferably include a rotary occluding member 1400a, 1400b and 1400c that is selectively positionable between stationary occluding walls 1104 and 1106, 1114 and 1116, and 1124 and 1126, respectively, for diverting fluid flow through one tubing of the corresponding pairs of tubings.

[0114] Pressure sensors 1200 and 1260 (See also FIGS. 4A and 4B) are provided within pump/valve/sensor assembly 1000 to operatively engage the first and second pressure-sensing modules 134 and 138 of cassette assembly 110 through openings 1120 and 1140 of cassette mounting plate 1010. Similarly, ultrasonic level sensors 1300 and 1320 (see also FIG. 5) are provided to operatively engage the blood return reservoir 150 cassette assembly 110 through openings 1160 and 1180 of cassette mounting plate 1010.

[0115] As shown in FIGS. 4A and 4B, the first and second pressure sensing modules 134, 138 of cassette assembly 110 each comprise a circular diaphragm 134a, 138a positioned on a raised cylindrical seat 134b, 138b formed into the back plate 114 of cassette assembly 110 with a ring-shaped, plastic diaphragm retainer 134c, 138c hot-welded to the raised cylindrical seats 134b, 138b to establish a seal therebetween. This arrangement allows the diaphragms 134a, 138a to be directly responsive to the fluid pressures within the first and second integral blood inlet passageways 130a, 130b, respectively, and pressure sensors 1200, 1260 to directly access the diaphragms 134a, 138a through the ring-shaped retainers 134c, 138c. By monitoring the diaphragms 134a, 138a, the pressure sensors 1200, 1260 can monitor the fluid pressure within the first and second integral blood inlet passageways 130a, 130b. In this regard, it should also be noted that since first integral blood inlet passageway 130a is in direct fluid communication with blood removal tubing 22, and since blood removal tubing 22 and blood return tubing 24 are fluidly interconnected via the common manifold 28, the first pressure sensing module 134 will be responsive to and first pressure sensor 1200 will actually sense the substantially common pressure in both the blood removal tubing 22 and blood return tubing 24 during operation.

[0116] With further regard to the first pressure sensing module 134 and first pressure sensor 1200, FIG. 4A illustrates an alternative air coupling arrangement that allows for the sensing of positive and negative pressure changes (i.e., causing outward and inward flexure of diaphragm 134a). To achieve an air seal between the first pressure sensor 1200 and first pressure sensing module 134, the sensor 1200 includes a resilient (e.g., rubber), cone-shaped engaging member 1202. The engaging member 1202 is attached to an air channel member 1204 having a nipple-end 1206 that is received by beveled cylindrical extension 134d of retainer 134c. Air channel member 1204 further includes an outer, annular projecting channel portion 1208 that contains an O-ring 1210 for sealed sliding engagement of the air channel member 1204 within housing 1212. As illustrated, housing 1212 includes ears 1214 which interface with a floating positioning member 1216 secured to the face plate 6a of blood component separation device 6. As shown, a slight clearance is provided in such interface so as to permit slight lateral movement of the engaging member 1202 and air channel member 1204 during loading of the cassette assembly 110. A threaded end 1218 of housing 1212 extends through the face plate 6a of blood component separation device 6 and receives nut 1220 thereupon, while leaving a slight clearance between the nut 1220 and face plate 6a. A spring 1222 is positioned within the housing 1212 and acts upon the annular channel portion 1208 of the air channel member 1204 to provide a spring-loaded interface between the first pressure sensor 1200 and first pressure sensing module 134. Pressure sensing transducer 1224 engages air

channel member **1204** to sense positive and negative pressure changes within sensing module **134** and provide an output signal in response thereto during use. As will be further described, the output signal of pressure transducer **1224** can be employed to control the operation of blood inlet pump **1030** and blood return pump **1090** during operation.

[0117] With regard to the second pressure sensing module **138** and the second pressure sensor **1260**, **FIG. 4B** illustrates a direct contact coupling approach that allows for sensing of positive pressure changes (i.e., causing outward flexure of diaphragm **138a**). Such contact coupling facilitates loading since the precise position of the diaphragm **138a** relative to the second pressure sensor **1260** is not critical. As shown, second pressure sensor **1260** includes a projecting end portion **1262** that is received by the ring retainer **138c** of sensing module **138** to directly contact diaphragm **138a**. Pressure transducer **1264** is mounted relative to the face plate **6a** of the blood component separation device **6** via a ring **1266** that threadingly engages a portion of pressure transducer **1264** extending through the face plate **6a**. Pressure transducer **1264** provides an output signal responsive to positive pressure changes acting upon diaphragm **138a**.

[0118] As shown in **FIG. 5**, when cassette assembly **110** is mounted on pump/valve/sensor assembly **1000**, the ultrasonic level sensors **1300** and **1320** will be positioned to monitor the fluid level in the blood return or replacement fluid reservoir **150**. More particularly, upper ultrasonic level sensor **1300** will be positioned in contact with the reduced top section **156** of blood return or replacement fluid reservoir **150** and lower ultrasonic level sensor **1320** will be positioned in contact with the reduced bottom section **158** of blood return or replacement fluid reservoir **150**.

[0119] Ultrasonic sensors **1300**, **1320** each comprise pulse/echo transducers **1302**, **1322** having a contact surface (e.g., urethane) **1304**, **1324** that facilitates divert dry coupling (i.e., without a gel or other like coupling medium) with the blood return or replacement fluid reservoir **150**. By way of example, ultrasonic sensors may comprise model Z-11405 transducers offered by Zevex Inc. of 5175 Greenpine Drive, Salt Lake City, Utah. Pulse/echo transducers **1302**, **1322** are disposed within housings **1306**, **1326** for interconnection with face plate **6a** of the blood component separation device **6**. Housings **1306**, **1326** include a flange **1308**, **1328** for engaging the front of face plate **6a**, and further include a threaded end **1308**, **1328** that extends through the face plate **6a** to receive corresponding retaining nuts **1310**, **1330**. A slight clearance is provided for between flanges **1308**, **1328** and face plate **6a**. Springs **1312**, **1332** are positioned within housings **1306**, **1326** to act upon the corresponding pulse/echo transducers **1302**, **1322** via E-clips **1314**, **1334** disposed therebetween. Such spring loading of pulse/echo transducers **1302**, **1322** yields a predetermined desired loading pressure for pulse/echo transducers **1302**, **1322** relative to reservoir **150** during operation (e.g., at least about 5 lbs.). O-rings **1316**, **1336** are provided intermediate pulse/echo transducers **1302**, **1322** and housings **1306**, **1326** to provide a sliding seal therebetween. Cables **1318**, **1338** are interconnected to transducers **1302**, **1322** to provide pulsing signals and return detected echo signals.

[0120] By gauging the presence and timing of return ultrasonic echo pulses each of sensors **1300** and **1320** can be

employed to monitor the presence or absence of fluid within their corresponding echo regions within the blood return reservoir **150**, and permit blood component separation device **6** to provide pump control signals in response thereto. More particularly, when return blood or replacement fluid accumulates up into the echo region of upper level sensor **1300** during blood processing, ultrasonic pulses emitted by upper level sensor **1300** will readily pass through the return blood or replacement fluid and reflect off of the opposing reservoir outside sidewall/air interface to yield echo pulses having a predetermined minimum strength that are detected by upper sensor **1300** within a predetermined time period after transmission. When such echo pulses are received, upper sensor **1300** provides a signal that is used by blood component separation device **6** to initiate operation of blood return or replacement fluid delivery pump **1090** so as to remove accumulated return blood or replacement fluid from the blood return or replacement fluid reservoir **150** and transfer the same to the donor/patient **4**.

[0121] When blood return or replacement fluid delivery pump **1090** has removed return blood or replacement fluid from the reservoir **150** down into the lower echo region, ultrasonic pulses emitted by lower level sensor **1320** will not be reflected at the opposing reservoir outside sidewall/air interface to yield echo pulses having a predetermined minimum strength for detection by lower level sensor **1320** within a predetermined time period after transmission. When this occurs, lower level sensor **1320** will fail to provide corresponding signals to blood component separation device **6**, and blood component separation device **6** will automatically stop blood return/replacement fluid delivery pump **1090** to stop further removal of return blood/replacement fluid from the blood return/replacement fluid reservoir **150**, and return blood/replacement fluid will again begin accumulating in reservoir **150**. Thus, in the blood processing mode, blood component separation device **6** will not initiate operation of blood return/replacement fluid delivery pump **1090** unless and until it receives signals from upper ultrasonic sensor **1300** (the provisions of such signals indicating the presence of return blood or replacement fluid in the upper echo region), and will thereafter automatically stop operation of blood return/replacement fluid delivery pump **1090** if it fails to receive signals from ultrasonic sensor **1320** (the failure to receive such signals indicating the absence of return blood or replacement fluid in the lower echo region).

[0122] In a preferable initial blood prime mode, whole blood may be introduced to reservoir **150** from a donor/patient **4** through blood return/replacement fluid delivery tubing **24**, integral passageways **190a**, **190b**, and tubing loop **192** via reverse operation of blood return/replacement fluid delivery pump **1090**. When such whole blood accumulates up into the echo region of lower level sensor **1320**, ultrasonic pulses emitted by lower level sensor **1320** will pass through the blood and reflect off of the opposing reservoir outside sidewall/air interface to yield echo pulses having a predetermined minimum strength that are detected by lower level sensor **1320** within a predetermined time period after transmission. When such echo pulses are received in the blood prime mode, lower level sensor **1320** provides a signal that is used by blood component separation device **6** to turn off blood return/replacement fluid delivery pump **1090** and end the blood prime mode (at least insofar as the priming of the return/replacement tubing **24** and reservoir **150** is con-

cerned). Blood component separation device 6 may then initiate the blood processing mode.

[0123] It is contemplated that ultrasonic sensors 1300, 1320 can be utilized for indicating and/or confirming the desired mounting relationship of cassette member 115 on cassette mounting plate 1010 for blood processing operations. For such purposes, if the desired mounting has been achieved, the sensors 1300, 1320 should be coupled to reservoir 150 so that ultrasonic pulses reflect off the interface between the inside surface of the back sidewall of reservoir 150 (i.e., the sidewall contacted by the sensors 1300, 1320) and contained air within reservoir 150, and be received with a predetermined minimum strength within a predetermined time period after transmission. If such echo pulses are received with respect to both ultrasonic sensors 1300, 1320, the desired loading relationship will be indicated and/or confirmed. Further, it is noted that ultrasonic sensors 1300, 1320 may be employable to sense echo pulses from the interfaces between fluid contained within the reservoir 150 and the inside surface of the outer sidewall of reservoir 150 in the upper and lower echo regions of the reservoir during operation. If such echo pulses are detectable within corresponding, predetermined time windows, corresponding signals provided by ultrasonic sensors 1300, 1320 can provide a further input for blood component separation device 6 to control operation of blood return/replacement fluid delivery pump 1090.

[0124] It should be noted that in the illustrated arrangement, the upper and lower ultrasonic sensors 1300 and 1320 advantageously operate via coupling with reduced cross-sectional portions 156 and 158 of reservoir 150. The reduced upper and lower reservoir portions 154, 158, accommodate reliable detection of echo pulses when fluid is present in the upper and lower echo regions, and the enlarged mid-portion 158 provides satisfactory return blood/replacement fluid holding capabilities.

[0125] FIG. 6 shows the preferred components of each of the platelet divert/replacement fluid valve subassembly 1100, plasma divert valve subassembly 1110 and RBC/plasma divert valve subassembly 1120. Each subassembly includes a rotary occluder member 1400 having a headed shaft member 1402 and barrel sleeve 1404 positioned thereupon and rotatable relative thereto. The subassembly further comprises a main valve shaft 1406 positioned within a valve body 1408 that is secured to face plate 6a of blood component separation device 6. An O-ring 1410 is provided in a recess on the main valve shaft 1406 to provide a sliding seal between main valve shaft 1406 and extensions 1412 of main valve body 1408. The main valve shaft 1406 is driven by a motor 1414 mounted on mount plate 1416 that in turn is mounted to and set off from face plate 6a by standoff legs 1418.

[0126] For positioning rotary occluder member 1400 for occlusion relative to one of the co-acting walls (e.g. 1104 or 1106 of the platelet divert/replacement fluid valve subassembly 1100; see FIG. 3) or for loading/removal of the cassette assembly 110 on the blood component separation device 6, each divert valve subassembly comprises three optical through-beam sensors 1420 (two shown) interconnected to standoff legs 1418 via support layer 1419, and an optical interrupter member 1422 interconnected to the main valve shaft 1406. Each through-beam sensor 1420 is of a

U-shape configuration with a radiation source and radiation receiver disposed on opposing legs. The optical interrupter member 1422 has an inverted cup configuration with its sidewalls interposed and rotatable between the opposing legs of sensors 1420. The optical interrupter member 1422 includes a single window 1424 therethrough. As will be appreciated, the position of the rotary occluder member 1400 relative to the window 1424 of the optical interrupter 1422 is known, such that when the optical window 1424 passes between the opposing radiation source/receiver for a given optical sensor 1420, the optical sensor 1420 will provide a signal in response to the through-beam (indicating the position of the rotary occluder member 1400), and the signal is employed to control the operation of motor 1414 to dispose rotary occluder member 1400 in the desired position. To provide/route such signals, the support layer 1419 may advantageously comprise a printed circuit board. Optical sensors 1420 are preferably positioned slightly "upstream" of predetermined stop regions for occlusion or cassette loading so that motor 1414 will be able to dynamically slow down and position rotary occluder member 1400 within such regions as desired. To insure the desired positioning for occlusion, however, stops 1426 are provided on main valve shaft 1406 to co-act with cross-pin 1428 interconnected to main valve shaft 1406 to insure stop positioning of rotary occluder member 1400 relative to the desired occluding wall.

[0127] Each of the occluding walls 1104 and 1106, 1114 and 1116, and 1124 and 1126, are provided with arcuate recesses (not shown) for receiving the rotatable barrel sleeve 1404 of rotary occluder members 1400a, 1400b and 1400c. By way of example, such arcuate recesses may have an arc length of 20 degrees and provide a tolerance range for positioning the rotary occluder members 1400a, 1400b, 1400c to achieve the desired tubing occlusion. As illustrated in FIG. 3, occluding wall 1106 may be provided with a resilient pad to best accommodate the use of thin-walled PVC tubing for platelet collector tubing 82. Further, and as noted above, thin-walled PVC tubing may be employed for plasma collector tubing 92 and RBC/plasma collector tubing 952, and corresponding resilient pads (not shown) may be provided on occluding walls 1114 and 1124. In this regard, given the relatively high-spring rate of thin-walled PVC tubing, the use of resilient pads in connection therewith increases the wearability of the thin-walled PVC tubing.

[0128] In order to establish an initial predetermined set position of the cassette assembly 110 relative to the pump/valve/sensor assembly 1000, the cassette assembly 110 includes downwardly extending corner positioning tabs 15 and top and bottom edge lips 17 that engage corresponding lower channel projections 1102a on cassette mounting plate 1010 and upper channel projections 1102b on a pivotable spring-loaded interlock member 1104 that extends across the top edge of cassette mounting plate 1010. The interlock member 1104 is spring-loaded to positively engage cassette assembly 110 upon loading via a spring positioned within housing 1106, and is provided with a tab 1108 for pivotable movement during cassette loading against the spring loading pressure. Preferably, interlock member 1104 is disposed relative to the raceway 1094 of return/replacement fluid delivery pump assembly 1090, such that when cassette assembly 110 is fully loaded for operation on blood component separation device 6, raceway 1094 will physically restrict interlock member 1104 from being pivoted, thereby

advantageously restricting removal and/or movement of cassette assembly 110 during use.

[0129] After cassette assembly 110 has been secured on the cassette mounting plate 1010, a loading assembly 1500 retracts the cassette mounting plate 1010 towards face plate 6a of the blood component separation device 6 to establish the above-noted, fully-loaded pump, valve and sensor relationships. As illustrated in FIG. 7, loading assembly 1500 includes two posts 1502 upon which cassette mounting plate 1010 is supportably interconnected. The posts 1502 extend through the face plate 6a of blood collection device 6 and are interconnected to a cross-connect member 1504. A drive nut 1506 is secured to cross-connect member 1504 and engages a drive screw 1508. The drive screw 1508 is in turn rotatably interconnected to a drive motor 1510 via coupling 1512, the drive motor 1510 being mounted on a platform 1514 which is supportively interconnected to face plate 6a via standoff legs 1516. The drive motor 1510 operates to turn drive screw 1508 so as to cause cross-connect member 1504 and posts 1502 to selectively move cassette mounting plate 1010 perpendicularly towards face plate 6a during loading procedures and perpendicularly away from face plate 6a for unloading of the cassette assembly 110.

[0130] To establish the desired position of cassette mounting plate 1010, U-shaped optical through-beam sensors 1520a and 1520b are mounted on post bearing holders 1522 and an optical occluder member 1524 having a window 1526 is interconnected to the cross-connect member 1504. Each of the U-shaped optical sensors 1520a, 1520b includes a radiation source and radiation receiver positioned on opposing extending legs, and the optical occluder member 1524 extends between such legs. Since the relative positions between cassette mounting plate 1010 and optical sensors 1520a, 1520b are known, by detecting the passage of radiation through window 1526 using optical sensors 1520, and providing a signal responsive thereto, the position of cassette mounting plate 1010 for loading and unloading can be automatically established. For example, when a through-beam is received by optical sensor 1520b, a signal will be provided to stop motor 1510 in a position wherein cassette assembly 110 will be fully loaded on the pump/valve/sensor assembly 1000 for operation.

[0131] To confirm such loaded condition, first and second pressure sensors 1200 and 1260 and upper and lower ultrasonic sensors 1300 and 1320 may be employed. For example, predetermined minimum pressure values can be established and actual pressures measured for each of the first and second pressure sensors 1200 and 1260 to confirm the desired loading of cassette assembly 110. Further, and of particular interest, ultrasonic sensors 1300 and 1320 can be advantageously employed to confirm the desired loading, since upon proper coupling to reservoir 150 echo pulses should be reflected off of the internal sidewall/air interface with a predetermined minimum strength within a predetermined time period as noted above.

[0132] It should be noted that drive motor 1510 preferably includes a number of reduction gears with the last gear being operatively associated with a slip clutch plate to limit the maximum amount of force that may be applied by cassette mounting plate 1010 (e.g., to an object between cassette mounting plate 1010 and face plate 6a). Relatedly, it is preferable to include control capabilities wherein during a

load cycle if the window 1526 of optical occluder 1524 has not moved from its position within the first optical pass through sensor 1520a to a position within the second optical pass through sensor 1520b within a predetermined time period, drive motor 1510 will automatically either stop or reverse operations.

[0133] To summarize the loading process, loading assembly 1500 initially disposes cassette mounting plate 1010 in an extended position. With the cassette mounting plate 1010 in such extended position, interlock member 1104 is pivoted away from cassette mounting plate 1010 and cassette assembly 110 is positioned on cassette mounting plate 1010 with bottom edge lips 17 of cassette assembly 110 being received by lower channel projections 1102a of cassette mounting plate 1010 and, upon return pivotal movement of interlock member 1104, top edge lips 17 of cassette assembly 110 being engaged by upper channel projections 1102b on interlock member 1104. Loading assembly 1500 is then operated to retract cassette mounting plate 1010 from its extended position to a retracted position, wherein tubing loops 122, 132, 162, 142, 192 of cassette assembly 110 are automatically positioned within the corresponding peristaltic pump assemblies 1020, 1030, 1060, 1040 and 1090. For such purposes, the rotors of each of the peristaltic pump assemblies are also operated to achieve loaded positioning of the corresponding tubing loops. Further, it should be noted that for loading purposes, the rotary occluder members 1400a, 1400b and 1400c of the divert valve assemblies 1100, 1110 and 1120 are each positioned in an intermediate position so as to permit the corresponding sets of tubing to be positioned on each side thereof.

[0134] Upon retraction of the cassette mounting plate 1010, spring-loaded, ultrasonic sensors 1300 and 1320 will automatically be coupled to reservoir 150 and first and second pressure sensors 1200 and 1260 will automatically couple to first and second pressure sensing modules 134 and 138 of cassette assembly 110. In this fully-loaded, retracted position, the cassette assembly 110 will be restricted from movement or removal by the above-noted physical restriction to pivotal movement of interlock member 1104 provided by raceway 1094 of return pump assembly 1090.

[0135] It is also noted that during loading of cassette assembly 110 on the blood component separation device 6, cuvette 65 (whether disposed in cassette 110 or in line tubing line 66 or 68) is positioned within an RBC spillover detector 1600 (e.g., an optical sensor for detecting the presence of any red blood cells in the separated platelet or plasma fluid stream and providing a signal response thereto) provided on the face plate 6a. Detector 1600 may also be used for set identification as described hereinabove. Similarly, a portion of anticoagulant tubing 54 is positioned within an AC sensor 1700 (e.g., an ultrasonic sensor for confirming the presence of anticoagulant and providing a signal in the absence thereof) also provided in face plate 6a.

[0136] To unload cassette assembly 110 after use, the occluding members 1400a, 1400b and 1400c of each divert valve assembly are again positioned in an intermediate position between the corresponding occluding walls and loading assembly 1500 is operated to move cassette mounting plate 1010 from its retracted position to its extended position. Contemporaneously, the rotors of the various peristaltic pump assemblies are operated to permit the corre-

sponding tubing loops to exit the same. In the extended position, the interlock member **1104** is pivoted out of engagement with cassette assembly **110** and cassette assembly **110** is removed and disposed of.

[0137] Operation of Extracorporeal Tubing Circuit and Pump/Valve/Sensor Assembly

[0138] In an initial blood prime mode of operation, blood return/replacement fluid delivery pump **1090** is operated in reverse as mentioned above, to transfer whole blood from the donor/patient **4** through blood removal/return tubing assembly **20**, integral blood return passageway **190**, blood return/replacement fluid delivery tubing loop **192** and into reservoir **150**. Contemporaneously with and/or prior to the reverse operation of blood return/replacement fluid delivery pump **1090**, anticoagulant peristaltic pump **1020** is operated to prime and otherwise provide anticoagulant from anticoagulant tubing assembly **50**, through anticoagulant integral passageway **120**, and into blood removal tubing **22** and blood return tubing **24** via manifold **28**. When lower level ultrasonic sensor **1320** senses the presence of the whole blood in reservoir **150** a signal is provided and blood component separation device **6** stops blood return/replacement fluid delivery peristaltic pump **1090**. As will be further discussed, during the blood prime mode blood inlet pump **1030** is also operated to transfer blood into blood inlet integral passageway **130**, through blood inlet tubing loop **132** and into blood inlet/blood component tubing assembly **60** to prime the blood processing vessel **352**.

[0139] During the blood prime mode, vent bag assembly **100** receives air from reservoir **150**. Relatedly, the occluding members **1400a**, **1400b**, **1400c** of divert assemblies **1100**, **1110**, **1120** are each preferably positioned to divert flow to the reservoir **150**. It should also be noted that to facilitate blood priming, the cassette assembly **110** is angled upward at about **45** degrees in its loaded position, and the integral passageways of cassette member **115** are disposed so that all blood and blood component and replacement fluid inlet paths provide for a bottom-to-top blood flow.

[0140] In the blood processing mode, the blood inlet peristaltic pump **1030**, platelet/replacement fluid inlet peristaltic pump **1040** and plasma peristaltic pump **1060** are operated generally continuously (except as described hereinbelow in further detail, e.g., when operating with replacement fluids, at least the blood inlet pump **1030** is stopped during delivery of replacement fluids to the donor/patient **4**), and the occluding members **1400a**, **1400b**, **1400c** are positioned for collection or return of corresponding blood components, as desired. During a blood removal submode, blood return/replacement fluid delivery peristaltic pump **1090** is not operated so that whole blood will pass into blood removal/return tubing assembly **20** and transferred to processing vessel **352** via the cassette assembly **110** and blood inlet/blood component tubing assembly **60**. In the blood removal submode, uncollected blood components are transferred from the processing vessel **352** to cassette assembly **110**, and uncollected components are passed into and accumulate in reservoir **150** up to a predetermined level at which upper level ultrasonic sensor **1300** provides signals used by blood component separation device **6** to end the blood removal submode and initiate a blood return or replacement fluid delivery submode. More particularly, a blood return or replacement fluid delivery submode is initiated by forward

operation of blood return/replacement fluid delivery peristaltic pump **1090**. In this regard, it should be appreciated that in the blood return or replacement fluid delivery submode the volume transfer rate of return blood or replacement fluid through blood return/replacement fluid tubing loop **192** utilizing blood return/replacement fluid delivery peristaltic pump **1090** is established by blood component separation device **6**, according to a predetermined protocol, to be greater than the volume transfer rate through blood inlet tubing loop **132** utilizing blood inlet peristaltic pump **1030** (again, in certain red blood cell collection protocols and/or, if using replacement fluid delivery, the blood inlet pump **1030** is stopped when return/delivery pump **1090** is operating). As such, the accumulated blood or replacement fluid in reservoir **150** is transferred into the blood return/replacement fluid delivery tubing of blood removal/return tubing assembly **20** and back into the donor/patient **4**. During the blood processing mode, when the accumulated return blood or replacement fluid in reservoir **150** is removed down to a predetermined level, lower level ultrasonic sensor **1320** will fail to provide signals to blood component separation device **6**, whereupon blood component separation device **6** will automatically stop blood return/replacement delivery peristaltic pump **1090** to end the blood return/replacement delivery submode. This automatically serves to reinitiate the blood removal submode since blood inlet peristaltic pump **1030** continuously operates (or restarts as described herein in replacement delivery use).

[0141] During the blood processing mode, pressure sensor **1200** senses negative/positive pressure changes within the blood removal tubing **22** blood return/replacement delivery tubing **26**, via first integral blood inlet passageway **130a**. Such monitored pressure changes are communicated to blood component separation device **6** which in turn controls blood inlet pump **1030** and return pump **1090** so as to maintain fluid pressures within predetermined ranges during the blood removal and the blood return submodes. Specifically during the blood removal submode, if a negative pressure is sensed that exceeds (i.e., is less than) a predetermined negative limit value, then blood component separation device **6** will slow down operation of blood inlet pump **1030** until the sensed negative pressure is back within an acceptable range. During the blood return/replacement delivery submode, if a positive pressure is sensed that exceeds (i.e., is greater than) a predetermined positive limit value, then blood component separation device **6** will preferably slow down operation of blood return/replacement delivery pump **1090** until the sensed positive pressure is back within an acceptable range.

[0142] Pressure sensor **1260** monitors the positive pressure within the second integral blood inlet passageway **130b** and blood inlet tubing **62**. If such sensed positive pressure exceeds a predetermined maximum value, blood component separation device **6** will initiate appropriate responsive action, including, for example, slowing or stoppage of the centrifuge and peristaltic pumps.

[0143] During the blood processing mode, blood component separation device **6** controls the operation of anticoagulant pump **1020** according to a predetermined protocol and responsive to signals provided by AC sensor **1700** (e.g., indicating a depleted anticoagulant source). Also, blood component separation device **6** also controls the operation of divert assemblies **1100**, **1110**, **1120** according to predeter-

mined instructions and further pursuant to any detect signals provided by RBC spillover detector **1600**. In the latter regard, if an RBC spillover in the separated platelet or plasma stream is detected, blood component separation device **6** will automatically cause occluder member **1400a** to divert the separated platelet or plasma stream to the return reservoir **150** until the RBC spillover has cleared, thereby keeping red blood cells from undesirably passing into the corresponding platelet or plasma collector tubing assembly **80** or **90**. Similarly, if a spillover detector is used with the replacement fluid line **962** and anything other than a replacement fluid is detected (in the embodiment of FIGS. 2C-2D), then the device **6** will take appropriate action, such as halting the procedure (even before it starts, e.g.) and prompting for a change in tubing set or fluid connection, e.g.

[0144] In normal operation, whole blood will pass through needle assembly **30**, blood removal tubing **22**, cassette assembly **110** and blood inlet tubing **62** to processing vessel **352**. As will be further described in detail, the whole blood will then be separated into blood components in vessel **352**. In the embodiment of FIGS. 2A-2B, a platelet stream will pass out of port **420** of the vessel, through platelet tubing **66**, back through cassette assembly **110**, and will then be either collected in platelet collector assembly **80** or diverted to reservoir **150**. Similarly, separated plasma will exit vessel **352** through port **456** to plasma tubing **68** back through cassette assembly **110**, and will then either be collected in plasma tubing assembly **90** or diverted to reservoir **150**. Further, red blood cells (and potentially white blood cells) may pass through ports **492** and **520** of vessel **352** through RBC/plasma tubing **64**, through cassette assembly **110** and into reservoir **150**. Alternatively, during RBC collection procedures as described hereinbelow, separated RBCs will be delivered to RBC/plasma collector tubing assembly **950** for collection. Also, alternatively, according to the embodiment of FIGS. 2C-2D, during product collection, replacement fluid will be passed through inlet tubing line **962**, cassette **110** and into the reservoir **150**, and only RBCs and plasma will be passed out of vessel **352** through corresponding ports **520** and **456** for collection and/or return as described in more detail hereinbelow.

[0145] As noted above, when uncollected platelets, plasma, and RBC/plasma (and potentially white blood cells) and/or replacement fluid(s) have accumulated in reservoir **150** up to upper ultrasonic level sensor **1300**, operation of return/delivery peristaltic pump **1090** will be initiated to remove the noted blood or replacement components from reservoir **150** and transfer the same back to the donor/patient **4** via the return/delivery tubing **24** and needle assembly **20**. When the fluid level in the reservoir **150** drops down to the level of the lower ultrasonic level sensor **1320**, the return/delivery peristaltic pump **1090** will automatically turn off reinitiating the blood removal submode (including restarting the blood inlet pump **1030**, if necessary). The cycle between blood removal and blood return/replacement delivery submodes will then continue until a predetermined amount of platelets, RBCs or other collected blood components have been harvested.

[0146] In one embodiment, reservoir **150** and upper and lower ultrasonic sensors **1300** and **1320** are provided so that, during the blood processing mode, approximately 50 milliliters of return blood/replacement fluid will be removed from reservoir **150** during each blood return/replacement

delivery submode and accumulated during each blood removal submode. Relatedly, in such embodiment, lower and upper level triggering by ultrasonic sensors **1300** and **1320** occurs at fluid volumes of about 15 milliliters and 65 milliliters, respectively, within reservoir **150**. For such embodiment, it is also believed desirable to provide for a volume transfer operating rate range of about 30 to 300 milliliters/minute through blood return/replacement delivery tubing loop **192** utilizing return/delivery pump **1090**, and a volume transfer operating rate range of either zero or about 20 to 140 milliliters/minute through blood inlet tubing loop **132** utilizing blood inlet pump **1030**. Additionally, for such embodiment a negative pressure limit of about -250 mmHg and positive pressure limit of about 350 mmHg is believed appropriate for controlling the speed of inlet pump **1030** and return/delivery pump **1090**, respectively, in response to the pressures sensed in first pressure sensing module **134**. A positive pressure limit of about 1350 mmHg within second sensing module **138** is believed appropriate for triggering slow-down or stoppage of the centrifuge and pumps.

[0147] Channel Housing

[0148] The channel assembly **200** is illustrated in FIGS. 8A-23B and includes a channel housing **204** which is disposed on the rotatable centrifuge rotor assembly **568** (FIGS. 1 and 24) and which receives a disposable blood processing vessel **352** or **352a**. Referring more specifically to FIGS. 8-15, the channel housing **204** has a generally cylindrically-shaped perimeter **206** with a diameter of preferably no more than about 10 inches to achieve a desired size for the blood component separation device **6** (e.g., to enhance its portability). An opening **328** extends longitudinally through the channel housing **204** and contains an axis **324** about which the channel housing **204** rotates. The channel housing **204** may be formed from materials such as delrin, polycarbonate, or cast aluminum and may include various cut-outs or additions to achieve weight reductions and/or rotational balance.

[0149] The primary function of the channel housing **204** is to provide a mounting for the blood processing vessel **352** or **352a** such that the blood may be separated into the blood component types in a desired manner. In this regard, the channel housing **204** includes a generally concave channel **208** in which the blood processing vessel **352** or **352a** is positioned. The channel **208** is principally defined by an inner channel wall **212**, an outer channel wall **216** which is radially spaced from the inner channel wall **212**, and a channel base **220** which is positioned therebetween. The channel **208** also extends from a first end **284** generally curvilinearly about a rotational axis **324** of the channel housing **204** to a second end **288** which overlaps with the first end **284** such that a continuous flow path is provided about the rotational axis **324**. That is, the angular disposition between the first end **284** of the channel **208** and the second end **288** of the channel **208** is greater than 360 degrees and up to about 390 degrees, and in the illustrated embodiment is about 380 degrees. Referring to FIG. 15, this angular disposition is measured by the angle B (beta), along a constant radius arc, between a first reference ray **336** which extends from the rotational axis **324** to the first end **284**, and a second reference ray **340** which extends from the rotational axis **324** to the second end **288** of the channel **208**.

[0150] The blood processing channel vessel **352** or **352a** is disposed within the channel **208**. Generally, the channel **208**

desirably allows blood to be provided to the blood processing vessel **352/352a** during rotation of the channel housing **204**, to be separated into its various blood component types by centrifugation, and to have various blood component types removed from the blood processing vessel **352/352a** during rotation of the channel housing **204**. For instance, the channel **208** is configured to allow for the use of high packing factors (e.g., generally a value reflective of how “tightly packed” the red blood cells and other blood component types are during centrifugation and as will be discussed in more detail below). Moreover, the channel **208** also desirably interacts with the blood processing vessel **352/352a** during centrifugation (e.g., by retaining the blood processing vessel **352/352a** in the channel **208** and by maintaining a desired contour of the blood processing vessel **352/352a**). In addition, the channel **208** allows for a blood priming of the blood processing vessel **352/352a** (i.e., using blood as the first liquid which is provided to the blood processing vessel **352/352a** in an apheresis procedure).

[0151] The above-identified attributes of the channel **208** are provided primarily by its configuration. In this regard, the channel housing **204** includes a blood inlet slot **224** which is generally concave and which intersects the channel **208** at its inner channel wall **212** in substantially perpendicular fashion (e.g., the blood inlet slot **224** interfaces with the inner channel wall **212**). A blood inlet port assembly **388** to the interior of the blood processing vessel **352/352a** is disposed in this blood inlet slot **224** such that blood from the donor/patient **4** may be provided to the blood processing vessel **352/352a** when in the channel **208**. In order to retain a substantially continuous surface along the inner channel wall **212** during an apheresis procedure and with the blood processing vessel **352/352a** being pressurized, namely by reducing the potential for the blood inlet port assembly **388** deflecting radially inwardly within the blood inlet slot **224**, a recess **228** is disposed on the inner channel wall **212** and contains the end of the blood inlet slot **224** (e.g., FIG. 14A). This recess **228** receives a shield **408** which is disposed about the blood inlet port assembly **388** on the exterior surface of the blood processing vessel **352/352a** as will be discussed in more detail below.

[0152] As illustrated in FIGS. 8-9, an RBC dam **232** of the channel **208** is disposed in a clockwise direction from the blood inlet slot **224** and whose function is to preclude RBCs and other large cells such as WBCs from flowing in a clockwise direction beyond the RBC dam **232**. Generally, the surface of the RBC dam **232** which interfaces with the fluid containing volume of the blood processing vessel **352/352a** may be defined as a substantially planar surface or as an edge adjacent the collect well **236**. At least in that portion of the channel **208** between the blood inlet port **224** and the RBC dam **232**, blood is separated into a plurality of layers of blood component types including, from the radially outermost layer to the radially innermost layer, red blood cells (“RBCs”), white blood cells (“WBCs”), platelets, and plasma. The majority of the separated RBCs are removed from the channel **208** through an RBC outlet port assembly **516** which is disposed in an RBC outlet slot **272** associated with the channel **208**, although at least some RBCs may be removed from the channel **208** through a control port assembly **488** which is disposed in a control port slot **264** associated with the channel **208**.

[0153] The RBC outlet port slot **272** is disposed in a counterclockwise direction from the blood inlet slot **224**, is generally concave, and intersects the channel **208** at its inner channel wall **212** in substantially perpendicular fashion (e.g., the RBC outlet slot **272** interfaces with the inner channel wall **212**). An RBC outlet port assembly **516** to the interior of the blood processing vessel **352/352a** is disposed in this RBC outlet slot **272** such that separated RBCs from the apheresis procedure may be continually removed from the blood processing vessel **352/352a** when in the channel **208** (e.g., during rotation of the channel housing **204**). In order to retain a substantially continuous surface along the inner channel wall **212** during an apheresis procedure and with the blood processing vessel **352/352a** being pressurized, namely by reducing the potential for the RBC outlet port assembly **516** deflecting radially inwardly within the RBC outlet slot **272**, a recess **276** is disposed on the inner channel wall **212** and contains the end of the RBC outlet slot **272** (e.g., FIGS. 14A, 14B). This recess **276** receives a shield **538** which is disposed about the RBC outlet port assembly **516** on the exterior surface of the blood processing vessel **352/352a** as will be discussed in more detail below. These above elements are preferably substantially similar in both of the alternative embodiments as shown in FIGS. 8A and 8B.

[0154] In the embodiment of FIG. 8A, there is a control port slot **264** is disposed in a counterclockwise direction from the RBC outlet slot **272**, is generally concave, and intersects the channel **208** at its inner channel wall **212** in substantially perpendicular fashion (e.g., the control port slot **264** interfaces with the inner channel wall **212**). A control port assembly **488** to the interior of the blood processing vessel **352** (see FIG. 8A) is disposed in the control port slot **264** (e.g., FIGS. 14A and C). In order to retain a substantially continuous surface along the inner channel wall **212** during an apheresis procedure and with the blood processing vessel **352** being pressurized, namely by reducing the potential for the control port assembly **488** deflecting radially inwardly within the control port slot **264**, a recess **268** is disposed on the inner channel wall **212** and contains the end of the control port slot **264**. This recess **268** receives a shield **508** which is disposed about the control port assembly **488** on the exterior surface of the blood processing vessel **352** as will be discussed in more detail below.

[0155] In the embodiment of FIG. 8B, the RBC outlet port **520** acts also as the interface control outlet port, and there is thus no corresponding control port assembly **488** in this embodiment. The interface control features hereof will be described further below.

[0156] The portion of the channel **208** extending between the control port slot **264** and the RBC dam **232** may be characterized as the first stage **312** of the channel **208**. The first stage **312** is configured to remove primarily RBCs from the channel **208** by utilizing a reverse flow in relation to the flow of platelet-rich and/or platelet-poor plasma (depending upon the corresponding use of respective vessels **352** or **352a**) through the channel **208** which is in a clockwise direction. In this regard, the outer channel wall **216** extends along a curvilinear path from the RBC dam **232** to the blood inlet slot **224** generally progressing outwardly away from the rotational axis **324** of the channel housing **204**. That is, the radial disposition of the outer channel wall **216** at the

RBC dam 232 is less than the radial disposition of the outer channel wall 216 at the blood inlet slot 224. The portion of the RBC outlet slot 272 interfacing with the channel 208 is also disposed more radially outwardly than the portion of the blood inlet slot 224 which interfaces with the channel 208.

[0157] In the first stage 312, blood is separated into a plurality of layers of blood component types including, from the radially outermost layer to the radially innermost layer, red blood cells ("RBCs"), white blood cells ("WBCs"), platelets, and plasma. As such, the RBCs sediment against the outer channel wall 216 in the first stage 312. By configuring the RBC dam 232 such that it is a section of the channel 210 which extends further inwardly toward the rotational axis 324 of the channel housing 204, this allows the RBC dam 232 to retain separated RBCs and other large cells as noted within the first stage 312. That is, the RBC dam 232 functions to preclude RBCs from flowing in a clockwise direction beyond the RBC dam 232. And, in the embodiment of FIGS. 2C-2D and 8B, it is preferable that, as described below, all blood components except platelet-poor plasma are precluded from flowing in a clockwise direction beyond the RBC dam 232.

[0158] Separated RBCs and other large cells as noted are removed from the first stage 312 utilizing the above-noted configuration of the outer channel wall 216 which induces the RBCs and other large cells as noted to flow in a counterclockwise direction (e.g., generally opposite to the flow of inlet blood into and through the first stage 312). Specifically, separated RBCs and other large cells as noted flow through the first stage 312 counter clockwise along the outer channel wall 216, past the blood inlet slot 224 and the corresponding blood inlet port assembly 388 on the blood processing vessel 352/352a, and to an RBC outlet slot 272. In the embodiment of FIG. 8A, in order to reduce the potential for counterclockwise flows other than separated RBCs being provided to the control port assembly 488 disposed in the control port slot 264 (e.g., such that there is a sharp demarcation or interface between RBCs and plasma proximate the control port slot 264 as will be discussed in more detail below), a control port dam 280 of the channel 208 is disposed between the blood inlet slot 224 and the RBC outlet slot 272. That is, preferably no WBCs, nor any portion of a buffy coat, disposed radially adjacent to the separated RBCs, is allowed to flow beyond the control port dam 280 and to the control port slot 264. The "buffy coat" includes primarily WBCs, lymphocytes, and the radially outwardmost portion of the platelet layer. As such, substantially only the separated RBCs and plasma are removed from the channel 208 in the FIG. 8A embodiment via the RBC control slot 264 to maintain interface control as noted. Contrarily, in the embodiment of FIGS. 2C-2D and 8B, all of these layers (except the platelet poor plasma) are retained behind the dam 232 and are also flowed back counter clockwise to the RBC/control outlet 520 where all such components, even the platelet poor plasma flowing thereto in a clockwise direction from the second stage (see below), is removed through the RBC/control outlet 520. Preferably, as will be described below, the RBC/plasma interface is maintained at the radial level of the RBC/control outlet 520; and thus, the dam 280 does not foreclose any separated component flow thereto.

[0159] The flow of RBCs to the control port assembly 488 in the embodiment of FIGS. 2A-2B and 8A, is typically

relatively small. Nonetheless, the ability for this flow is highly desired in that the control port assembly 488 functions in combination with the RBC outlet port assembly 516 to automatically control the radial position of an interface between separated RBCs and the "buffy coat" in relation to the RBC dam 232 by controlling the radial position of an interface between separated RBCs and plasma in relation to the control port assembly 488. The control port assembly 488 and RBC outlet port assembly 516 automatically function to maintain the location of the interface between the separated RBCs and the buffy coat at a desired radial location within the channel 208 which is typically adjacent the RBC dam 232 such that there is no spillover of RBCs or the buffy coat beyond the RBC dam 232. This function is provided by removing separated RBCs from the channel 208 at a rate which reduces the potential for RBCs and the other large cells as noted flowing beyond the RBC dam 232 and contaminating the platelet collection.

[0160] Separated platelets, again in the embodiment of FIGS. 2A-2B and 8A, which are disposed radially inwardly of the RBC layer and more specifically radially inwardly of the buffy coat, flow beyond the RBC dam 232 with the plasma (e.g., via platelet-rich plasma) in a clockwise direction. In the FIG. 8B embodiment, there is no platelet collection performed, and, preferably only platelet-poor plasma flows over the dam 232. Forcing the interface further radially outwardly by making the RBC port 520 also act as the control port achieves this restriction. I.e., the platelets do not get close enough to the dam 232 to flow thereover in this other embodiment. However, in the embodiment of FIG. 8A, a generally funnel-shaped platelet collect well 236 is disposed in a clockwise direction from the RBC dam 232 and is used to remove platelets from the channel 208 in the platelet-rich plasma. The configuration of the platelet collect well 236 is defined by only part of the outer channel wall 216. The portion of the platelet collect well 236 defined by the configuration of the outer channel wall 216 includes a lower face 240, a left side face 244, and a right side face 248. These faces 240, 244, 248 are each substantially planar surfaces and taper generally outwardly relative to the rotational axis 324 and inwardly toward a central region of the platelet collect well 236.

[0161] The remainder of the platelet collect well 236 (FIG. 8A) is defined by the blood processing vessel 352 when loaded in the channel 208, namely a generally triangular-shaped 428 which is disposed above the platelet outlet port assembly 416 to the interior of the blood processing vessel 352 and discussed in more detail below. A platelet support recess 249 extends further radially outwardly from those portions of the platelet collect well 236 defined by the configuration of the outer channel wall 216 and primarily receives the support 428 associated with the platelet collect port assembly 416. Generally, the upper portion of the support 428 is disposed below and engages an upper lip 252 of the platelet support recess 249, while portions of the fourth face 444 of the support 428 are seated against the two displaced shoulders 252. This positions the support 428 when the blood processing vessel 352 is pressurized to direct platelets toward the platelet collect port assembly 416.

[0162] The outer channel wall 216 is further configured to receive the platelet collect tube 424. An upper platelet collect tube recess 254 and a lower platelet collect tube

recess 255 are disposed yet further radially outwardly from the platelet support recess 249 to provide this function. As such, the platelet collect tube 424 may extend radially outwardly from the outer sidewall 376 of the blood processing vessel 352, extend upwardly through the lower platelet collect tube recess 255 and the upper platelet collect tube recess 254 behind or radially outwardly from the support 428, and extend above the channel housing 204.

[0163] Platelet-poor plasma continues to flow in a clockwise direction through the channel 208 after the platelet collect well 236 (FIG. 8A), or after the dam 232 (in the embodiment of FIG. 8B), and may be removed from the channel 208. In this regard, the channel 208 further includes a generally concave plasma outlet slot 256 (FIGS. 8A and 8B) which is disposed proximate the second end 288 of the channel 208 and intersects the channel 208 at its inner channel wall 212 in substantially perpendicular fashion (e.g., the plasma outlet slot 256 interfaces with the inner channel wall 212). A plasma outlet port assembly 452 to the interior of the blood processing vessel 352 is disposed in this plasma outlet slot 256 such that plasma may be continually removed from the blood processing vessel 352/352a during an apheresis procedure (e.g., during continued rotation of the channel housing 204). This plasma may be collected and/or returned to the donor/patient 4 as described in further detail below.

[0164] In order to increase the number of platelets that are separated and removed from the vessel 352 in the embodiment of FIG. 8A, in a given apheresis procedure, the configuration of the channel 208 between the platelet collect well 236 and the plasma outlet slot 256 may be such that platelets which separate from plasma in this portion of the channel 208 actually flow in a counterclockwise direction back towards the platelet collect well 236 for removal from the channel 208. This may be provided by configuring the outer channel wall 216 such that it extends generally curvilinearly about the rotational axis 324 from the platelet collect well 236 to the plasma outlet slot 256 progressing generally inwardly toward the rotational axis 324 of the channel housing 204. Consequently, the portion of the channel 208 including the platelet collect well 236 and extending from the platelet collect well 236 to the second end 288 may be referred to as a second stage 316 of the channel 208. In the embodiment of FIGS. 2C-2D and 8B where there is no platelet collect well, the second stage 316 extends from the top of the dam 232 to the plasma outlet port 456 (see FIG. 2C).

[0165] The channel 208 is also configured to provide platelet-poor plasma to the control port slot 264 in the FIG. 8A embodiment, and to the RBC/control port slot 272 in the FIG. 8B embodiment. Thus platelet-poor plasma flows to the control port assembly 488 (FIG. 8A) or RBC/control port 520 (FIG. 8B) in order to assist in automatically controlling the interface between the RBCs and the buffy coat or plasma in relation to the RBC dam 232. In this regard, the first end 284 of the channel 208 is interconnected with the second end 288 of the channel 208 by a connector slot 260. With the first connector 360 and second connector 368 of the blood processing vessel 352/352a being joined, they may be collectively disposed in this connector slot 260. As such, a continuous flowpath is provided within the blood processing vessel 352/352a and, for purposes of the automatic interface control feature, RBCs may flow to the

control port slot 264 (FIG. 8A) in a counterclockwise direction and plasma may flow to the control port slot 264 (FIG. 8A) or RBC/control port slot 272 (FIG. 8B) in a clockwise direction. The portion of the channel 208 extending from the first end 284 to the respective control port slots 264/272 may be referred to as a third stage 320 of the channel 208.

[0166] As noted above, the configuration of the channel 208 is desirable/important in a number of respects. As such, the dimensions of one embodiment of the channel 208 are provided herein and which may contribute to the functions of the channel 208 discussed below. The dimensions for one embodiment of the channel 208 are identified on FIG. 9B. All radius and thicknesses, etc., are expressed in inches.

[0167] One of the desired attributes of the channel 208 is that it facilitates the loading of the blood processing vessel 352/352a therein. This is provided by configuring the channel 208 to include a chamfer 210 on both sides of the channel 208 along the entire extent thereof. Generally, the chamfer 210 extends downwardly and inwardly toward a central portion of the channel 208 as illustrated, for instance, in FIGS. 12-13. In embodiment, the angle of this chamfer 210 ranges from about 30 degrees to about 60 degrees relative to horizontal, and preferably is about 45 degrees. Moreover, the configuration of the channel 208 retains the blood processing vessel 352/352a within the channel 208 throughout the apheresis procedure. This is particularly relevant in that the channel housing 254 is preferably rotated a relatively high rotational velocities, such as about 3,000 RPM.

[0168] Another desirable attribute of the channel 208 is that it provides a self-retaining function for the blood processing vessel 352/352a. The configuration of the channel 208 in at least the first stage 312, and preferably in the region of the platelet collect well 236 (FIG. 8A) and in the region of the RBC dam 232 as well, is configured such that the upper portion of the channel 208 includes a restriction (e.g., such that the upper part of the channel 208 in this region has a reduced width in relation to a lower portion thereof). Although this configuration could also be utilized in the portion of the second stage 316 disposed between the platelet collect well 236 or dam 232 and the plasma outlet slot 256, in the illustrated embodiment the width or sedimentation distance of the channel 208 in this region is less than the width or sedimentation distance of the channel 208 throughout the entire first stage 312. This use of a "reduced width" can itself sufficiently retain the blood processing vessel 352/352a in the channel 208 in the "reduced-width" portion of the second stage 316 such that the inner channel wall 212 and outer channel wall 216 in this portion of the second stage 316 may be generally planar and vertically extending surfaces.

[0169] In the illustrated embodiment and as best illustrated in FIG. 12, the noted "restriction" in the channel 208 is provided by configuring the outer channel wall 216 with a generally C-shaped profile. In this portion of the channel 208, the channel 208 includes an upper channel section 292 having a first width, a mid-channel section 300 having a second width greater than the first width, and a lower channel section 304 having a width less than that of the mid-channel section 300 and which is typically equal to that of the upper channel section 292. This profile is provided by an upper lip 296 which extends radially inwardly from the

outer channel wall **216** toward, but displaced from, the inner channel wall **212**, and by a lower lip **308** which extends radially inwardly from the outer channel wall **216** toward, but displaced from, the inner channel wall **212**. This lower lip **308** actually defines a portion of the channel base **220** but does extend entirely from the outer channel wall **216** to the inner channel wall **212** such that it defines a notch **218**.

[0170] When the blood processing vessel **352/352a** is loaded into the channel **208**, the fluid-containing volume of the coinciding portion of the blood processing vessel **352/352a** is disposed below the upper channel section **292** and is principally contained within the mid-channel section **300**. That is, the upper lip **296** "hangs over" the fluid-containing volume of the blood processing vessel **352/352a** over at least a portion of its length. The upper lip **296** thereby functions to retain the blood processing vessel **352/352a** within the channel **208** during rotation of the channel housing **204**. Moreover, the upper lip **296** reduces the potential for creep by supporting the vessel **352/352a** proximate the upper seal **380**. The upper channel section **292** and the lower channel section **304** are multi-functional in that they also serve to receive and support an upper seal **380** and lower seal **384** of the blood processing vessel **352/352a** to a degree such that the stresses induced on these portions of the blood processing vessel **352/352a** during an apheresis procedure are reduced as will be discussed in more detail below. As can be appreciated, a similarly configured upper lip and lower lip could extend outwardly from the inner channel wall **212** toward, but displaced from, the outer channel wall **216**, alone or in combination with the upper lip **296** and lower lip **308**, and still retain this same general profile for the channel **208** to provide the noted functions.

[0171] Another desirable attribute of the channel **208** is that it allows for the use of blood as the liquid which primes the blood processing vessel **352/352a** versus, for instance, saline solutions. Priming with blood allows for the actual collection of blood components to begin immediately (i.e., blood used in the prime is separated into blood component types, at least one of which may be collected). Blood priming is subject to a number of characterizations in relation to the apheresis system **2** and is based primarily upon the configuration of the channel **208**. For instance, the configuration of the channel **208** allows for blood to be the first liquid introduced into the blood processing vessel **352/352a** which is loaded in the channel **208**. Moreover, the configuration of the channel **208** allows separated plasma to flow in a clockwise direction through the channel **208** and to reach the control port slot **264** (FIG. 8A) (and thus the control port assembly **488** of the blood processing vessel **352**) before any separated RBCs or any of the other noted large cells flow in the same clockwise direction beyond the RBC dam **232** and thus into the second stage **316** (i.e., a spillover condition). That is, blood priming may be utilized since control of the interface between the separated RBCs and the buffy coat is established before any RBCs or WBCs spill over into the second stage **316**. Blood priming may also be characterized as providing blood and/or blood components to the entire volume of the blood processing vessel **352/352a** prior to any RBCs or any of the other noted large cells flowing beyond the RBC dam **232** and into the second stage **316**.

[0172] In order to achieve this desired objective of priming the blood processing vessel **352/352a** with blood, gen-

erally the volume of the channel **208** which does not have RBCs to the volume of the channel **208** which does have RBCs must be less than one-half of one less than the ratio of the hematocrit of the RBCs leaving the channel **208** through the RBC outlet port assembly **516** to the hematocrit of the blood being introduced into the channel **208** through the blood inlet port assembly **388**. This may be mathematically expressed as follows:

$$V_2/V_1 < (H_{RP}/H_{IN} - 1)/2,$$

[0173] where:

[0174] V_2 =the volume of the channel **208** containing only plasma or platelet-rich plasma;

[0175] V_1 =the volume of the channel **208** containing RBCs of the first stage **312** and third stage **320**;

[0176] H_{RP} =the hematocrit of the packed RBCs leaving the channel **208** through the RBC outlet port assembly **516**; and

[0177] H_{IN} =the hematocrit of the blood entering the channel **208** through the blood inlet port assembly **388**.

[0178] This equation assumes that the hematocrit in the RBC volume and is calculated as $(H_{IN} + H_{RP})/2$. In the case where the H_{IN} is equal to 0.47 and H_{RP} is equal to 0.75, this requires that the ratio of V_1/V_2 be less than 0.30 in order for a blood prime to be possible.

[0179] The noted ratio may be further characterized as the ratio of that portion of the channel **208** which may be characterized as containing primarily plasma (e.g., V_{PL}) to the volume of that portion of the channel **208** which may be characterized as containing primarily RBCs (e.g., V_{RBC}). Referring to FIG. 15, these respective volumes may be defined by a reference circle **332** which originates at the rotational axis **324** and which intersects the RBC dam **232** at the illustrated location which would be at the border of a spillover condition. Portions of the channel **208** which are disposed outside of this reference circle **232** are defined as that portion of the channel **208** which includes primarily RBCs or which defines V_{RBC} (e.g., about 77.85 cc in the illustrated embodiment), while those portions of the channel **208** which are disposed inside of the reference circle **232** are defined as that portion of the channel **208** which includes primarily plasma or which defines V_{PL} (e.g., about 19.6 cc in the illustrated embodiment). In the illustrated embodiment, the ratio of V_{PL}/V_{RBC} is about 0.25 which is less than that noted above for the theoretical calculation for the blood prime (i.e., 0.30 based upon comparison of the hematocrits). In order to further achieve the noted desired ratio, the width and height of the channel **208** throughout that portion of the second stage **316** disposed in a clockwise direction from the platelet collect well **236** (FIG. 8A) or the dam **232** (FIG. 8B), also in third stage **320**, are each less than the width and height of the channel **208** throughout the entire first stage **312**.

[0180] Another important feature relating to the configuration of the channel **208** is that the radially inwardmost portion of the inner channel wall **212** is at the interface with the plasma outlet slot **256**. That is, the entirety of the inner channel wall **212** slopes toward the plasma outlet slot **256**. This allows any air which is present in the blood processing vessel **352/352a** during priming to be removed from the

blood processing vessel **352/352a** through the plasma outlet slot **256** and more specifically the plasma outlet port assembly **452** since the air will be the least dense fluid within the blood processing vessel **352/352a** at this time.

[0181] Another desirable attribute of the channel **208** is that it contributes to being able to utilize a high packing factor in an apheresis procedure. A “packing factor” is a dimensionless quantification of the degree of packing of the various blood component types in the first stage **312** and is thus reflective of the spacings between the various blood component types. The packing factor may thus be viewed similarly to a theoretical density of sorts (e.g., given a quantity of space, what is the maximum number of a particular blood component type that can be contained in this space).

[0182] The packing factor is more specifically defined by the following equation:

$$PF=\omega^2\times R\times (v_{RBC}/W)\times V/Q_{IN},$$

[0183] where:

- [0184] PF=packing factor;
- [0185] ω =rotational velocity;
- [0186] R=the average radius of the outer channel wall **216** in the first cell separation stage **312**;
- [0187] V_{RBC} =the sedimentation velocity of RBCs at 1 G;
- [0188] V=the functional volume of the first cell separation stage **312**;
- [0189] W=the average sedimentation distance or width of the channel **208**; and
- [0190] Q_{IN} =the total inlet flow to the channel **208**.

[0191] Consequently, the packing factor as used herein is dependent upon not only the configuration of the channel **208**, particularly the first stage **312**, but the rotational velocities being used in the apheresis procedure as well as the inlet flow to the blood processing vessel **352/352a**. The following are packing factors associated with the blood processing channel **208** having the above-described dimensions:

	N (rpm)	Q _{in} ml/mi	V (ml)	PF	G @R _{avg}	P@R1st (psi)
FF8 SLOPE = .02	0	0	62.8	0.0	0.0	0.0
	905	5	62.8	13.0	100.1	8.1
	1279	10	62.8	13.0	200.2	16.2
	1567	15	62.8	13.0	300.2	24.3
	1809	20	62.8	13.0	400.3	32.5
	2023	25	62.8	13.0	500.4	40.6
	2216	30	62.8	13.0	600.5	48.7
	2394	35	62.8	13.0	700.6	56.8
	2559	40	62.8	13.0	800.6	64.9
	2714	45	62.8	13.0	900.7	73.0
	2861	50	62.8	13.0	1100.9	81.1
	3001	55	62.8	13.0	1100.9	89.3
	3001	60	62.8	11.9	1100.9	89.3
	3001	65	62.8	11.0	1100.9	89.3
	3001	70	62.8	10.2	1100.9	89.3
	3001	75	62.8	9.5	1100.9	89.3
	3001	80	62.8	8.9	1100.9	89.3
	3001	85	62.8	8.4	1100.9	89.3

-continued					
N (rpm)	Q _{in} ml/mi	V (ml)	PF	G @R _{avg}	P@R1st (psi)
3001	90	62.8	7.9	1100.9	89.3
3001	95	62.8	7.5	1100.9	89.3
3001	100	62.8	7.1	1100.9	89.3
3001	105	62.8	6.8	1100.9	89.3
3001	110	62.8	6.5	1100.9	89.3
3001	115	62.8	6.2	1100.9	89.3
3001	120	62.8	6.0	1100.9	89.3
3001	125	62.8	5.7	1100.9	89.3
3001	130	62.8	5.5	1100.9	89.3
3001	135	62.8	5.3	1100.9	89.3
3001	140	62.8	5.1	1100.9	89.3

[0192] Note the G forces are listed for the various rotational speeds at the middle of the first stage **312** and for a 10 inch outer diameter for the channel housing **204**. At about 2,560 RPM, the G force is about 800 G, while at about 3,000 RPM the G force is about 1,100 Gs.

[0193] Increasing the packing factor beyond a certain point produces diminishing returns regarding the collection of blood component types. That is, further increases in packing factor may not produce correspondingly increased collection efficiencies and may in fact impede the collection of blood component types. It is believed that a packing factor ranging from about 4 to about 21, preferably from about 11 to 16, and more preferably about 13, is optimum for collection of most blood component types. It has been observed, however, that during red blood cell collection, an increased packing factor (i.e., >13) may prove desirable to lower the level of white blood cells in the collected RBC product. A packing factor of 16 has been found preferable in collecting RBCs and plasma simultaneously with the embodiment of FIGS. 2C-2D and 8B (see below). The rotational velocity of the channel housing **204** may be adjusted based upon the inlet flows being provided to the blood processing vessel **352** or **352a** to maintain the desired packing factor. For instance, the desired operating speed for the centrifuge housing **204** during the normal course of an apheresis procedure is preferably about 3,000 RPM. However, this rotational speed may be reduced to “match” the inlet flow to the blood processing vessel **352** or **352a** in order to retain the desired packing factor. Similarly, the rotational speed of the channel housing **204** may be increased to “match” an increased inlet flow to the blood processing vessel **352/352a** in order to retain the desired packing factor.

[0194] Due to constraints regarding the blood processing vessel **352/352a**, more specifically the various tubes interconnected therewith (e.g., which provide the seal-less loop), the above-noted desired packing factors of about 13 may be realized for inlet flows of up to about 55 ml/min. (instantaneous). Beyond 55 ml/min., the rotational speed would have to be increased above 3000 RPM to maintain the desired packing factor of about 13. Although tubes exist which will withstand those rotational speeds, presently they are not approved for use in an apheresis system. With the presently approved tubing, the packing factor may be maintained at a minimum of about 10, and preferably at least about 10.2, or even 11, for inlet flows (instantaneous) of about 40-70 ml/min. For the packing factor preference of 16 for the collection of RBCs and plasma together (FIGS. 2C-2D), a maximum 3000 RPM rotational speed would indicate that a

slower inlet flow would be necessary. The higher packing factor of 16 provides a purer plasma separation (i.e., fewer platelets) over the RBC dam; and thus, a purer plasma product. However, a packing factor of 16 is also slower because of the lower inlet flow. Thus, after collecting plasma and RBCs together (until a minimum desired amount of plasma is collected, for instance), then the packing factor would preferably be reduced to about 13 to collect RBCs at a faster rate.

[0195] The packing factor may also be related to the resulting hematocrit achieved by the system. A target hematocrit of 80, for example, has been readily achievable with a packing factor of preferably between 11 and 16, and again preferably about 13. Note, the resulting hematocrit is also dependent on the amount of separated plasma which is remixed with the separated RBCs in the interface control outlets, as described herein.

[0196] At the above noted increased rotational speeds, the channel 208 not only provides for achieving an increased packing factor, but reduces the impact of this high packing factor on the collection efficiency regarding platelet collection. Specifically, the configuration of the channel 208 is selected to reduce the number of platelets that are retained within the first stage 312 (in FIG. 8A embodiment). The configuration of the channel 208 in the first stage 208 utilizes a progressively reduced width or sedimentation distance progressing from the blood inlet slot 224 to the RBC dam 232. That is, the width of the channel 208 proximate the blood inlet slot 224 is less than the width of the channel 208 proximate the RBC dam 232. This configuration of the channel 208 in the first stage 312 reduces the volume of the "buffy coat" or more specifically layer between the RBCs and platelets to be collected. As noted, this buffy coat includes primarily WBCs and lymphocytes, as well as the radially outwardmost portion of the platelet layer. The "buffy coat" is preferably retained in the first stage 312 during an apheresis procedure. Since the volume of the "buffy coat" is reduced by the reduced width of the channel 208 proximate the RBC dam 232, this reduces the number of platelets which are retained in the first stage 312 (FIG. 8A), and thus increases the number of platelets which flow to the platelet collect well 236 (FIG. 8A).

[0197] Disposable Set: Blood Processing Vessel

[0198] The blood processing vessel 352 (or 352a in the FIG. 2C, 8B embodiment) is disposed within the channel 208 for directly interfacing with and receiving a flow of blood in an apheresis procedure. The use of the blood processing vessel 352/352a alleviates the need for sterilization of the channel housing 204 after each apheresis procedure and the vessel 352/352a may be discarded to provide a disposable system. There are initially two important characteristics regarding the overall structure of the blood processing vessel 352/352a. The blood processing vessel 352/352a is constructed such that it is sufficiently rigid to be free-standing in the channel 208. Moreover, the blood processing vessel 352/352a is also sufficiently rigid so as to be loaded in the channel 208 having the above-identified configuration (i.e., such that the blood processing vessel 352/352a must be directed through the reduced width upper channel section 292 before passage into the larger width mid-channel section 300). However, the blood processing

vessel 352/352a must also be sufficiently flexible so as to substantially conform to the shape of the channel 208 during an apheresis procedure.

[0199] In order to achieve the above-noted characteristics, the blood processing vessel 352/352a may be constructed as follows. Initially, materials for the blood processing vessel 352/352a include PVC, PETG, and polyolefins, with PVC being preferred. Moreover, the wall of thickness of the blood processing vessel 352/352a will typically range between about 0.030" and 0.040". Furthermore, the durometer rating of the body of the blood processing vessel 352/352a will generally range from about 50 Shore A to about 90 Shore A.

[0200] Referring primarily to FIGS. 16-23B, the blood processing vessel 352/352a includes a first end 356 and a second end 364 which overlaps with the first end 356 and is radially spaced therefrom. A first connector 360 is disposed proximate the first end 356 and a second connector 368 is disposed proximate the second end 364. When the first connector 360 and second connector 368 are engaged (typically permanently), a continuous flow path is available through the blood processing vessel 352/352a. This construction of the blood processing vessel 352/352a facilitates loading in the channel 208 in the proper position and as noted also contributes to the automatic control of the interface between the separated RBCs and the buffy coat or plasma relative to the RBC dam 232.

[0201] The blood processing vessel 352/352a includes an inner sidewall 372 and an outer sidewall 376. In the illustrated embodiment, the blood processing vessel 352/352a is formed by sealing two pieces of material together (e.g., RF welding). More specifically, the inner sidewall 372 and outer sidewall 376 are connected along the entire length of the blood processing vessel 352/352a to define an upper seal 380 and a lower seal 384. Seals are also provided on the ends of the vessel 352/352a. The upper seal 380 is disposed in the reduced width upper channel section 292 of the channel 208, while the lower seal 384 is disposed in the reduced width lower channel section 304 of the channel 208 (e.g., FIG. 19F). This again reduces the stresses on the upper seal 380 and lower seal 384 when a flow of blood is provided to the blood processing vessel 352/352a and pressurizes the same. That is, the upper seal 380 and lower seal 384 are effectively supported by the channel 208 during an apheresis procedure such that a resistance is provided to a "pulling apart" of the upper seal 380 and lower seal 384. By utilizing two separate sheets to form the blood processing vessel 352/352a, a "flatter" profile may also be achieved. This type of profile is beneficial during rinseback, and also facilitates loading and unloading of the vessel 352/352a relative to the channel 208.

[0202] Blood is introduced into the interior of the blood processing vessel 352/352a through a blood inlet port assembly 388 which is more particularly illustrated in FIGS. 19A-G. Initially, the port 392, as all other ports, is welded to the blood processing vessel 352/352a over a relatively small area. This results in less movement of materials due to the welding procedure which provides a smoother surface for engagement by the blood and/or blood component types.

[0203] The blood inlet port assembly 388 includes a blood inlet port 392 and a blood inlet tube 412 which is fluidly interconnected therewith exteriorly of the blood processing vessel 352/352a. The blood inlet port 392 extends through and beyond the inner sidewall 372 of the blood processing

vessel **352/352a** into an interior portion of the blood processing vessel **352/352a**. Generally, the blood inlet port assembly **388** is structured to allow blood to be introduced into the blood processing vessel **352/352a** during an apheresis procedure without substantially adversely affecting the operation of the apheresis system **2**.

[0204] The blood inlet port **392** includes a substantially cylindrical sidewall **396**. A generally vertically extending slot **404** is disposed proximate an end of the sidewall **396** of the blood inlet port **392** such that the slot **404** is substantially parallel with the inner sidewall **372** and outer sidewall **376** of the blood processing vessel **352/352a**. The slot **404** projects in the clockwise direction, and thus directs the flow of blood in the channel **208** generally toward the RBC dam **232**. A vane **400** is positioned on the end of the cylindrical sidewall **396**, is disposed to be substantially parallel with the inner sidewall **372**, and thereby directs the flow of blood out through the slot **404**. As illustrated in FIG. 19D, the vane **400** includes a generally V-shaped notch on the interior of the blood inlet port **392**, the arcuate extent of which defines the "height" of the slot **404**.

[0205] The desired manner of flow of blood into the blood processing vessel **352/352a** during an apheresis procedure is subject to a number of characterizations, each of which is provided by the above-described blood inlet port assembly **388**. Initially, the flow of blood into the blood processing vessel may be characterized as being at an angle of less than 90 degrees relative a reference line which is perpendicular to the inner sidewall **372** of the blood processing vessel **352/352a**. That is, the blood is injected in a direction which is at least partially in the direction of the desired flow of blood through the blood processing vessel **352/352a**. Moreover, the desired flow of blood into the blood processing vessel **352/352a** may be characterized as that which reduces the effect on other flow characteristics within blood processing vessel **352/352a** at the blood inlet port **392**.

[0206] Separated RBCs **556** again flow along the outer sidewall **376** of the blood processing vessel **352/352a** adjacent the outer channel wall **216**, past the blood inlet port **392**, and to the RBC outlet port assembly **516** as illustrated in FIGS. 19E and 19G. The desired flow of blood into the blood processing vessel **352/352a** may then be further characterized as that which is substantially parallel with at least one other flow in the region of the blood inlet port **392** (e.g., inject the blood substantially parallel with the flow of RBCs **556**). This manner of introducing blood into the blood processing vessel **352/352a** may then be further characterized as that which does not significantly impact at least one other flow in the region of the blood inlet port **392**.

[0207] As noted above, the blood inlet port assembly **388** interfaces with the inner sidewall **372** of the blood processing vessel **352/352a** in a manner which minimizes the discontinuity along the inner channel wall **212** in the region of the blood inlet slot **224** in which the blood inlet port **392** is disposed. Specifically, a shield **408** may be integrally formed with and disposed about the blood inlet port **392**. The shield **408** is disposed on an exterior surface of the blood processing vessel **352/352a** and interfaces with its inner sidewall **372**. The shield **408** is at least in partial overlapping relation with the inner sidewall **372**. Moreover, in the case where the shield **408** is integrally formed with the port **392**, it need not be attached to the inner sidewall **372**. The port

392 is installed asymmetrical relative to the shield **408** which is beneficial for manufacturability. All shields and their blood-related ports discussed below also include this feature.

[0208] Generally, the shield **408** is more rigid than the inner sidewall **372** of the blood processing vessel **352/352a**. This increased rigidity may be provided by utilizing a more rigid material for the shield **408** than is used for the inner sidewall **372**. For instance, the durometer rating of the material forming the shield **408** may range from about 90 Shore A to about 130 Shore A, while the durometer rating of the material forming the inner sidewall **372** of the blood processing vessel **352/352a** again ranges from about 50 Shore A to about 90 Shore A in one embodiment. This durometer rating (when the shield **408** and port **392** are integrally formed) also enhances the seal between the port **392** and the tube installed therein.

[0209] When the blood inlet port **392** is disposed in the blood inlet slot **224** when loading the blood processing vessel **352/352a** in the channel **208**, the shield **408** is positioned within the recess **228** formed in the inner channel wall **212**. Again, the blood inlet slot **224** intersects with the inner channel wall **212**, and more specifically the recess **228**. That is, the recess **228** contains and is disposed about one end of the blood inlet slot **224**. Preferably, the thickness of the shield **408** is substantially equal to the depth or thickness of the recess **228** such that the amount of discontinuity along the inner channel wall **212** in the region of the blood inlet slot **224** is reduced or minimized. Due to the increased rigidity of the shield **408** in comparison to the materials forming the blood processing vessel **352/352a**, when the blood processing vessel **352/352a** is pressurized during an apheresis procedure the shield **408** restricts movement of the blood processing vessel **352/352a** and/or the blood inlet port **392** into the blood inlet slot **224**. That is, the shield **408** restricts and preferably minimizes any deflection of the blood processing vessel **352/352a** into the blood inlet slot **224** during the procedure. Moreover, with the shield **408** being integrally formed with the blood inlet port **392**, the radial position of the vertical slot **404** in the blood inlet port **392** is not dependent upon the thickness of the materials forming the blood processing vessel **352/352a**.

[0210] In the first stage **312**, blood which is provided to the blood processing vessel **352/352a** by the blood inlet port assembly **388** is separated into at least RBCs, and plasma. The RBCs, as well as most of the WBCs, are retained within the first stage **312** and are preferably precluded from flowing in a clockwise direction past the RBC dam **232** into the second stage **316** or, in the FIG. 8A embodiment, into the platelet collect well **236**. Instead, the RBCs and WBCs are induced to flow along the outer channel wall **216** in a counterclockwise direction past the blood inlet port **392** and toward the RBC outlet port assembly **516** of the blood processing vessel **352/352a**. That is, the RBC outlet port assembly **516** is disposed in a counterclockwise direction from the blood inlet port assembly **388**. However, as noted above, in the FIG. 8A embodiment, the control port dam **280** impedes the flow to the buffy coat control port assembly **488** to provide a sharp interface between the separated RBCs and the plasma proximate the control port assembly **488** such that this may be used to control the radial position of the interface between the RBCs and the buffy coat in the area of the RBC dam **232**. In the FIG. 8B embodiment on the

other hand, the interface is established proximate the RBC/control port **520** as described hereinbelow.

[0211] The RBC outlet port assembly **516** is more specifically illustrated in FIGS. **20A-D** and generally includes an RBC outlet port **520** and an RBC outlet tube **540** fluidly interconnected therewith exteriorly of the blood processing vessel **352/352a**. The RBC outlet port **520** extends through and beyond the inner sidewall **372** of the blood processing vessel **352/352a** into an interior portion of the blood processing vessel **352/352a**. In addition to removing separated RBCs from the blood processing vessel **352/352a** during an apheresis procedure, the RBC outlet port assembly **516** also functions in combination with the control port assembly **488** (FIG. **8A**) or by itself (FIG. **8B**) to automatically control the radial position of the interface between separated RBCs and the buffy coat or plasma relative to the RBC darn **232** (e.g., to prevent RBCs from flowing beyond the RBC dam **232**) in a manner discussed in more detail below.

[0212] The RBC outlet port **520** is also configured to reduce the potential for the flow therethrough being obstructed during rinseback (i.e., during the evacuation of the blood processing vessel **352/352a** upon completion of blood component separation and collection process so as to provide as much of the contents thereof back to the donor/patient **4**). During rinseback, the rotation of the channel housing **204** is terminated and a relatively significant drawing action (e.g., by pumping) is utilized to attempt to remove all contents from the blood processing vessel **352/352a**. The end of the RBC outlet port **520** includes a first protrusion **524** and a second protrusion **528** displaced therefrom, with a central recess **532** being disposed therebetween which contains the noted orifice **536** for the blood outlet port **520**. The first protrusion **524** and the second protrusion **528** each extend further beyond the inner sidewall **372** of the blood processing vessel **352/352a** a greater distance than the central recess **532/352a**. As such, during rinseback if the outer sidewall **376** attempts to contact the inner sidewall **372**, the first protrusion **524** and second protrusion **528** will displace the central recess **532** and its orifice **536** away from the outer sidewall **376**. This retains the orifice **536** in an open condition such that the flow therethrough is not obstructed during rinseback.

[0213] As noted above, the RBC outlet port assembly **516** interfaces with the inner sidewall **372** of the blood processing vessel **352/352a** in a manner which minimizes the discontinuity along the inner channel wall **212** in the region of the RBC outlet **272** in which the RBC outlet port **520** is disposed. Specifically, a shield **538** is integrally formed with and disposed about the RBC outlet port **520**. The shield **538** is disposed on an exterior surface of the blood processing vessel **352/352a** and interfaces with its inner sidewall **372**. The shield **538** is at least in partial over-lapping relation with the inner sidewall **372**. Moreover, in the case where the shield **538** is integrally formed with the port **520**, it need not be attached to the inner sidewall **372**. Generally, the shield **538** is more rigid than the inner sidewall **372**. This increased rigidity may be provided by utilizing a more rigid material for the shield **538** than is used for the inner sidewall **372**. For instance, the durometer rating of the material forming the shield **538** may range from about 90 Shore A to about 130 Shore A, while the durometer rating of the material forming the inner sidewall **372** of the blood processing vessel **352/**

352a again ranges from about 50 Shore A to about 90 Shore A in one preferred embodiment.

[0214] When the RBC outlet port **520** is disposed in the RBC outlet slot **272** when loading the blood processing vessel **352/352a** in the channel **208**, the shield **538** is positioned within the recess **276** formed in the inner channel wall **212**. Again, the RBC outlet slot **272** intersects with the inner channel wall **212**, and more specifically the recess **276**. That is, the recess **276** contains and is disposed about one end of the RBC outlet slot **272**. Preferably, the thickness of the shield **538** is substantially equal to the depth or thickness of the recess **276** such that the amount of discontinuity along the inner channel wall **212** in the region of the RBC outlet slot **272** is reduced or minimized. Due to the increased rigidity of the shield **538** in comparison to the materials forming the blood processing vessel **352/352a**, when the blood processing vessel **352/352a** is pressurized during an apheresis procedure, the shield **538** restricts movement of the blood processing vessel **352/352a** and/or the RBC outlet port **520** into the RBC outlet slot **272**. That is, the shield **538** restricts and preferably minimizes any deflection of the blood processing vessel **352/352a** into the RBC outlet slot **272**. Moreover, with the shield **538** being integrally formed with the RBC outlet port **520**, the radial position of the orifice **536** is not dependent upon the thickness of the materials forming the blood processing vessel **352/352a**.

[0215] Separated platelets in the embodiment of FIG. **8A**, are allowed to flow beyond the RBC dam **232** and into the second stage **316** of the channel **208** in platelet-rich plasma. The blood processing vessel **352** (FIG. **8A**) includes a platelet collect port assembly **416** to continually remove these platelets from the vessel **352** throughout an apheresis procedure and such is more particularly illustrated in FIGS. **8A**, **16**, and **21A-B**. Generally, the platelet collect port assembly **416** is disposed in a clockwise direction from the blood inlet port assembly **388**, as well as from the RBC dam **232** when the blood processing vessel **352** is loaded into the channel **208**. Moreover, the platelet collect port assembly **416** interfaces with the outer sidewall **376** of the blood processing vessel **352**.

[0216] The platelet collect port assembly **416** (FIG. **8A**) is disposed in the platelet support recess **249** and the platelet outlet tube recess **254** which are disposed radially outwardly from the portion of the platelet collect well **236** defined by the outer channel wall **216** of the channel **208**. The platelet collect port assembly **416** generally includes a platelet collect port **420** and a platelet collect tube **424** which is fluidly interconnected therewith exteriorly of the blood processing vessel **352**. The orifice **422** of the port **420** may be substantially flush with the interior surface of the outer sidewall **376** of the blood processing vessel **352**. Moreover, the radial position of the orifice **422** is established by engagement of part of the platelet collect port **420** with boundaries of the recess **249** and/or **254**.

[0217] The platelet collect port **420** (FIG. **8A**) is welded to the blood processing vessel **352**. The thickness of the overlapping portions of the port **420** and vessel **352** are substantially equal. The weld area is overheated such that there is a mixing of the two materials. This results in the platelet collect port **420** being able to flex substantially against the outer channel wall **216** when the vessel **352** is pressurized.

[0218] The blood processing vessel 352 (FIG. 8A) and the outer channel wall 216 of the channel 210 collectively define the platelet collect well 236. The contribution of the blood processing vessel 352 to the platelet collect well 236 is provided by a substantially rigid support 428 which is disposed vertically above the platelet collect port 420 and hingedly interconnected at location 430 with the outer sidewall 376 and/or a mounting plate 426 of the platelet collect port 420. The contoured support 428 includes a first face 432 and a second face 436 which interface with the exterior surface of the outer sidewall 376 of the blood processing vessel 352 (i.e., the support overlaps with the sidewall 376 of the blood processing vessel 352 and need not be attached thereto over the entire interface therewith) and which are disposed in different angular positions. The upper portion of the first face 432 extends over the top of the blood processing vessel 352, while the lower portion of the first face 432 generally coincides with the upper seal 380 on the blood processing vessel 352. The second face 436 interfaces with the outer sidewall 376 in a region of the fluid-containing volume of the blood processing vessel 352 and is the primary surface which directs platelets toward the platelet collect port 420.

[0219] When the blood processing vessel 352 (FIG. 8A) is pressurized, the support 428 moves into a predetermined position defined by portions of the platelet collect recess 252. Specifically, a third face 440 is retained under an upper lip 254 on the upper perimeter of the platelet support recess 249, and the two sides of a fourth face 444 seat against a shoulder 252 disposed on each side of the platelet support recess 249. A platelet tubing notch 448 is formed in the support 428 at generally the intersection between the third face 440 and the fourth face 444. The platelet collect tube 426 thus may extend out from the platelet collect port 420, up the platelet collect tube recess 254, against the platelet tube notch 448 if necessary, and above the channel housing 204 to pass down through the central opening 328 therein.

[0220] In order to increase the purity of platelets that are collected, a platelet purification system as described in U.S. patent application Ser. Nos. 08/423,578 and corresponding U.S. Pat. Nos. 5,674,173; 5,906,570; inter alia, and Ser. No. 08/423,583 may be disposed in the platelet collect tube 424 of the embodiment of FIGS. 2A-2B and 8A, and the entire disclosures of these patent documents are incorporated by reference in their entirety herein.

[0221] Platelet-poor plasma flows beyond the platelet collect well 236 (FIG. 8A) and/or beyond the dam 232 (FIG. 8B) and to the plasma outlet port assembly 452. Here, some of the platelet-poor plasma may be removed from the blood processing vessel 352/352a and collected, although this "separated" plasma may also be returned the donor/patient 4 in some instances. The plasma port 456 is also used in the blood priming of the vessel 352/352a in that air is removed from the vessel 352/352a through the plasma port 456. Referring to FIG. 22, the plasma outlet port assembly 452 includes a plasma outlet port 456 and a plasma outlet tube 476 which is fluidly interconnected therewith exteriorly of the blood processing vessel 352/352a. The plasma outlet port 456 extends through and beyond the inner sidewall 372 of the blood processing vessel 352/352a into an interior of the blood processing vessel 352/352a. The plasma outlet

port 456 is disposed between the second end 364 of the blood processing vessel 352/352a and the second connector 368.

[0222] The plasma outlet port 456 is configured to reduce the potential for the flow therethrough being obstructed during rinseback (i.e., during evacuation of the blood processing vessel 352/352a upon completion of an apheresis procedure so as to provide as much of the contents thereof back to the donor/patient 4). During rinseback, the rotation of the channel housing 204 is terminated and a relatively significant drawing action (e.g., by pumping) is utilized to attempt to remove all contents from the blood processing vessel 352/352a. The end of the plasma outlet port 456 includes a first protrusion 460 and a second protrusion 464 displaced therefrom, with a central recess 468 being disposed therebetween which contains an orifice 472 for the plasma outlet port 456. The first protrusion 460 and the second protrusion 464 each extend further beyond the inner sidewall 372 of the blood processing vessel 352/352a a greater distance than the central recess 468. As such, during rinseback if the outer sidewall 376 attempts to contact the inner sidewall 372, the first protrusion 460 and second protrusion 464 will displace the central recess 468 and its orifice 472 away from the outer sidewall 376. This retains the orifice 472 in an open condition such that the flow therethrough is not obstructed during rinseback.

[0223] In order to further assist in withdrawal from the blood processing vessel 352/352a after completion of an apheresis procedure and thus during rinseback, a first passageway 480 and a second passageway 484 (see FIGS. 8A, 8B and 16) are formed in the blood processing vessel 352/352a (e.g., via heat seals, RF seals) and generally extend downwardly from the plasma outlet port 456 toward a lower portion of the blood processing vessel 352/352a. The first passageway 480 and second passageway 484 are disposed on opposite sides of the plasma outlet port 456. With this configuration, a drawing action through the plasma outlet port 456 is initiated in a lower portion of the blood processing vessel 352/352a at two displaced locations.

[0224] Some of the separated plasma is also utilized to automatically control the location of the interface between separated RBCs and the buffy coat or plasma in the first stage 312, specifically the radial position of this interface relative to the RBC dam 232. Plasma which provides this interface control function is removed from the blood processing vessel 352 by a control port assembly 488 in the embodiment of FIGS. 2A-2B and 8A, and which is illustrated in FIGS. 23A-B. (Again, the embodiment of FIGS. 2C-2D and 8B does not preferably have a control port assembly 488.) The control port assembly 488 is disposed in a clockwise direction from the plasma outlet port assembly 452 and proximate the RBC outlet port assembly 516, and thus between the first end 284 of the channel 208 and the RBC outlet port assembly 516. This plasma thus flows from the second stage 316 and into the third stage 320 to provide this function.

[0225] The control port assembly 488 (FIG. 8A) generally includes a control port 492 and control port tube 512 which is fluidly interconnected therewith exteriorly of the blood processing vessel 352. The control port 492 extends through and beyond the inner sidewall 372 of the blood processing vessel 352 into an interior portion of the blood processing

vessel 352. The radial positioning of the orifice 504 of the control port 492 is not dependent upon the thickness of the material forming the blood processing vessel 352. Instead, the control port 492 includes a shoulder 496 which engages or seats upon structure within the control port slot 264 to accurately place the orifice 504 at a predetermined radial position within the channel 208. Moreover, this predetermined radial position is substantially maintained even after the blood processing vessel is pressurized. In this regard, the control port assembly 488 interfaces with the inner sidewall 372 of the blood processing vessel 352 in a manner which minimizes the discontinuity along the inner channel wall 212 in the region of the control port slot 264 in which the control port 492 is disposed. Specifically, a shield 508 is integrally formed with and disposed about the control port 492. The shield 508 is disposed on an exterior surface of the blood processing vessel 352 and interfaces with its inner sidewall 372. The shield 508 is at least in partial overlapping relation with the inner sidewall 372. Moreover, in the case where the shield 508 is integrally formed with the port 492, it need not be attached to the inner sidewall 372. Generally, the shield 508 is more rigid than the inner sidewall 372 and this assists in maintaining the orifice 504 of the control port 492 at the desired radial position within the channel 208. This increased rigidity may be provided by utilizing a more rigid material for the shield 508 than is used for the inner sidewall 372. For instance, the durometer rating of the material forming the shield 508 may range from about 90 Shore A to about 130 Shore A, while the durometer rating of the material forming the inner sidewall 372 of the blood processing vessel 352 again ranges from about 50 Shore A to about 90 Shore A in one embodiment.

[0226] The control port assembly 488 (FIG. 8A) and/or the RBC outlet port assembly 516 (by itself in the FIG. 8B embodiment) function in combination to control the radial position of the interface between separated RBCs and the buffy coat or plasma relative to the RBC dam 232. In the FIG. 8A embodiment, two structural differences between the RBC outlet port assembly 516 and the control port assembly 488 contribute to achieving this automatic control. Initially, the orifice 536 to the RBC outlet port 520 is disposed further into the interior of the blood processing vessel 352 than the control port 492. In one embodiment, the orifice 536 of the RBC outlet port 520 is disposed more radially outwardly than the orifice 504 of the control port 492. Moreover, the diameter of the RBC outlet tube 540 is greater than that of the control port tube 512. In one embodiment, the inner diameter of the RBC outlet tube 54 is about 0.094", while the inner diameter of the control port tube 512 is about 0.035". The control port tube 512 and RBC outlet tube 540 also join into a common return tube 546 via a three-way tubing jack 544 which further assists in providing the automatic interface control feature.

[0227] The automatic interface position control is provided as follows utilizing the RBC outlet port assembly 516 and the control port assembly 488 in FIG. 8A. Initially, there are two interfaces in the channel 208 of significance with regard to this automatic interface position control feature. One of these interfaces is the RBC/buffy coat interface in relation to the RBC dam 232. However, there is also an RBC/plasma interface in the region of the control port assembly 488 which again is available through use of the control port dam 280. The control port dam 280 allows

substantially only RBCs to flow to the control port assembly 488 in a counterclockwise direction.

[0228] In the event that the interface between the RBCs and plasma moves radially inwardly toward the rotational axis 324, RBCs will begin flowing out the control port tube 512 in addition to the RBC outlet tube 540. This decreases the flow through the smaller diameter control port tube 512 due to the higher viscosity and density of the RBCs compared to the plasma which typically flows through the control port tube 512. Consequently, the flow through the larger diameter RBC outlet tube 540 must increase since the flow through the return tube 546 must remain the same. This removes more RBCs from the first stage 312 such that both the interface between the RBCs and the buffy coat in relation to the RBC dam 232 and the interface between the RBCs and the plasma both move radially outwardly. That is, this changes the radial position of each of these interfaces. As such, the potential for RBCs flowing beyond the RBC dam 232 and into the platelet collect well 236 is reduced.

[0229] In the event that the location of the interface between the RBCs and plasma progresses radially outward, the flow through the control port tube 512 will increase since the quantity of RBCs exiting the blood processing vessel 352 through the control port 512 will have decreased. Since the flow through the return tube 546 must remain the same, this results in a decrease in the flow of RBCs through the RBC outlet tube 540. This reduces the number of RBCs being removed from the channel 208 such that both the interface between the RBCs and the buffy coat in relation to the RBC dam 232 and the interface between the RBCs and the plasma both move radially inwardly. That is, this changes the radial position of each of these interfaces.

[0230] The above-described tubes which interface with the blood processing vessel 352 of the embodiment of FIGS. 2A-2B and 8A, namely the blood inlet tube 412, the platelet collect tube 424, the plasma outlet tube 476, the return tube 546, each pass downwardly through the central opening 328 in the channel housing 204. A tubing jacket 548 is disposed about these various tubes and protects such tubes during rotation of the channel housing 204. These tubes are also fluidly interconnected with the extracorporeal tubing circuit 10 which again provides for fluid communication between the donor/patient 4 and the blood processing vessel 352.

[0231] The blood processing vessel 352/352a also includes features for loading and unloading the same from the channel 208. Referring back to FIG. 16, the vessel 352/352a includes at least one and preferably a plurality of tabs 552. The tabs 552 may be integrally formed with the blood processing vessel 352/352a (e.g., formed by the seal which also forms the upper seal 380). However, the tabs 552 may also be separately attached. The tabs 552 nonetheless extend vertically above the fluid-containing volume of the blood processing vessel 352/352a, preferably a distance such that the tabs 552 actually project above the channel housing 204. The tabs 552 thereby provide a convenient non-fluid-containing structure for the operator to grasp and load/remove the blood processing vessel 352/352a into/from the channel 208 (i.e., they provide structure for the operator to grasp which has had no blood-related flow therethrough during the apheresis procedure). The tabs 552 are particularly useful since there may be resistance provided to a loading and an unloading of the blood processing vessel 352/352a into/from the channel 208.

[0232] Centrifuge Rotor Assembly

[0233] The channel assembly **200** is mounted on the centrifuge rotor assembly **568** which rotates the channel assembly **200** to separate the blood into the various blood component types by centrifugation. The centrifuge rotor assembly **568** is principally illustrated in FIGS. **24-25** and generally includes a lower rotor housing **584** having a lower gear **588**. An input or drive shaft **576** is disposed within the lower rotor housing **584** and is rotatably driven by an appropriate motor **572**. The input/drive shaft **576** includes a platform **580** mounted on an upper portion thereof and a rotor body **592** is detachably interconnected with the platform **580** such that it will rotate therewith as the input/drive shaft **576** is rotated by the motor **572**.

[0234] The centrifuge rotor assembly **568** further includes an upper rotor housing **632** which includes a mounting ring **644** on which the channel housing **204** is positioned. In order to allow the channel housing **204** to rotate at twice the speed of the rotor body **592**, the upper rotor housing **632** and lower rotor housing **584** are rotatably interconnected by a pinion assembly **612**. The pinion assembly **612** is mounted on the rotor body **592** and includes a pinion mounting assembly **616** and a rotatable pinion **620**. The pinion **620** interfaces with the lower gear **588** and a driven gear **636** which is mounted on the mounting ring **644**. The gear ratio is such that for every one revolution of the rotor body **592**, the upper rotor housing **632** rotates twice. This ratio is desired such that no rotary seals are required for the tubes interfacing with the blood processing vessel **352/352a**. In one embodiment, the lower gear **588**, the pinion **620**, and the driven gear **636** utilize straight bevel gearing.

[0235] The centrifuge rotor assembly **568** is also configured for easy loading of the blood processing vessel **352/352a** in the channel **208** of the channel housing **204**. In this regard, the rotor body **592** includes a generally L-shaped blood processing vessel loading aperture **597**. The aperture **597** includes a lower aperture **600** which extends generally horizontally into the rotor body **592** through its sidewall **596** of the rotor body **592**, but only partially therethrough. The perimeter of the lower aperture **600** is defined by a left concave wall **601**, a back concave wall **603**, and a right concave wall **602**.

[0236] The loading aperture **597** also includes an upper aperture **598** which intersects with the lower aperture **600** at **599** and extends upwardly through an upper portion of the rotor body **592**. The upper aperture **598** is aligned with a generally vertically extending central opening **640** in the upper rotor housing **632**. As noted above, the channel housing **204** also includes a central opening **328**. As such, a blood processing vessel **352/352a** may be folded if desired, inserted into the lower aperture **600**, deflected upwardly by the back concave wall **603**, through the upper aperture **598**, through the central opening **640** in the upper rotor housing **632**, and through the central opening **328** of the channel housing **204**. The operator may then grasp the blood processing vessel **352/352a** and load the same in the channel **208**.

[0237] The centrifuge rotor assembly **568** includes a number of additional features to facilitate the loading of the blood processing vessel **352/352a** in the channel **208**. Initially, the pinion **620** is radially offset in relation to the lower aperture **600** of the rotor body **592**. In one embodiment, a

reference axis laterally bisects the lower aperture **600** and may be referred to as the "zero axis". The axis about which the pinion **620** rotates is displaced from this "zero axis" by an angle α of about 40 degrees in the illustrated embodiment (see FIG. **25A**). An angle α of -40 degrees could also be used. Positioning the pinion **620** at an angle of "greater" than ± 40 degrees will result in the pinion **620** beginning to interfere with the access to the loading aperture **597**. Although the angle α may be less than 40 degrees and may even be 0 degrees, having the pinion **620** at 0 degrees will result in the counterweights **608** potentially interfering with the access to the loading aperture **597**. Based upon the foregoing, in FIG. **25** the pinion assembly **612** has therefore been rotated about the axis which the centrifuge rotor assembly **568** rotates for ease of illustration.

[0238] Since only a single drive gear is utilized to rotate the upper rotor housing **632** relative to the rotor body **592**, an upper counterweight **604** and lower counterweight **608** are disposed or detachably connected to the rotor body **592** proximate the upper and lower extremes of the lower aperture **600**. Due to the offset positioning of the pinion **620** in relation to the lower aperture **600**, the upper and lower counterweights **604**, **608** are also radially offset in relation to the lower aperture **600**. That is, the upper and lower counterweights **604**, **608** are "off to the side" in relation to the lower aperture **600** such that access thereto is not substantially affected by the counterweights **604** and **608**. A tube mounting arm **624** is also appropriately attached to the rotor body **592** and engages the tubing jacket **548**. The tubing mounting arm **624** serves to further the rotational balance of the rotor body **592**.

[0239] Another feature of the centrifuge rotor assembly **568** which contributes to the loading of the blood processing vessel **352/352a** upwardly through the rotor body **592** is the size of the lower aperture **600**. As illustrated in FIG. **25B**, the "width" of the lower aperture may be defined by an angle θ which may range from about 70 degrees to about 90 degrees, and in the illustrated embodiment is about 74 degrees. The back wall **603**, left wall **601**, and right wall **602** are also defined by a radius ranging from about 1.75" to about 2.250", and in the illustrated embodiment this radius is between about 2.008" and about 2.032".

[0240] Apheresis Protocol

[0241] A first alternative protocol which may be followed for performing an apheresis procedure on a donor/patient **4** utilizing the above-described system **2** will now be summarized. Initially, an operator loads the cassette assembly **110** onto the pump/valve/sensor assembly **1000** of the blood component separation device **6** and hangs the various bags (e.g., bags **104**, **94**, **84**, and/or **954**) on the blood component separation device **6**. The operator then loads the blood processing vessel **352** (e.g., FIGS. **2A**, **2B** and **8A**) within the channel **208** which is disposed on the channel housing **204** which is in turn mounted on the centrifuge rotor assembly **568**, particularly the mounting ring **644**. More specifically, the operator may fold the blood processing vessel **352** and insert the same into the blood processing vessel loading aperture **597** on the rotor body **592**. Due to the arcuately-shaped, concave configuration of the loading aperture **597**, specifically the lower aperture **600**, the blood processing vessel **352** is deflected upwardly through the upper aperture **598**, the central opening **640** in the upper

rotor housing, and the central opening **328** in the channel housing **294**. The operator then grasps the blood processing vessel **352** and pulls it upwardly away from the channel housing **204**.

[0242] Once the blood processing vessel **352** has been installed up through the centrifuge rotor assembly **568**, the operator loads the blood processing vessel **352** into the channel **208** on the channel housing **204**. The operator generally aligns the blood processing vessel **352** relative to the channel **208** (e.g., such that the blood inlet port **392** is vertically aligned with the blood inlet slot **224**, such that the platelet collect port **420** is vertically aligned with the platelet support recess **249** and the platelet collect tube recess **254** (in the embodiment of FIGS. 2A-2B), such that the plasma outlet port **456** is vertically aligned with the plasma outlet slot **256**, such that the control port **492** is vertically aligned with the control port slot **264** (also per FIGS. 2A-2B), and such that the RBC outlet port **520** is vertically aligned with the RBC outlet slot **272**). Once again, the interconnection of the first connector **360** and second connector **368**, which is preferably fixed, facilitates the loading of the blood processing vessel **352**, as well as the existence of the chamfer **210**.

[0243] With the blood processing vessel **352** properly aligned, the operator directs the blood processing vessel **352** through the reduced width upper channel section **292** of the channel **208** until the blood processing vessel **352** hits the channel base **220**. In this case, the longitudinal extent of the blood processing vessel **352** located in the portion of the channel **208** which includes the first stage **312**, the RBC dam **232**, and the platelet/plasma collect or second stage **316** will be disposed as follows: 1) the upper seal **380** will be disposed in the upper channel section **292**; 2) the fluid-containing volume of the blood processing vessel **352** will be disposed in the mid channel section **300**; and 3) the lower seal **384** will be disposed in the lower channel section **304**. The above-noted ports will also be disposed in their respective slots in the channel housing **204** by the operator at this time. Moreover, the shield **408** associated with the blood inlet port assembly **388** will be disposed in the recess **228** associated with the blood inlet slot **224**. Similarly, the shield **538** associated with the RBC outlet port assembly **516** will be disposed in the recess **276** associated with the RBC outlet slot **272**. Furthermore, the shield **508** associated with the control port assembly **488** will be disposed in the recess **268** associated with the control port slot **264** (according to the embodiment of FIGS. 2A-2B).

[0244] With the extracorporeal tubing circuit **10** and the blood processing vessel **352** loaded in the above-described manner, the circuit **10** and vessel **352** may first be pressure-tested to verify that there are no leaks. The donor/patient **4** is then fluidly interconnected with the extracorporeal tubing circuit **10** (by inserting an access needle **32** into the donor/patient **4**). Moreover, the anticoagulant tubing **54** is primed between the anticoagulant supply (which interfaces with the spike drip member **52**) and the manifold **48**. Furthermore, blood return/replacement delivery tubing **28** is primed with blood from the donor/patient **4** by running the blood return/replacement delivery peristaltic pump **1090** pump in reverse to draw blood from the donor/patient **4**, through the blood return tubing **28**, and into the reservoir **150** until blood is detected by the low level sensor **1320**.

[0245] The blood processing vessel **352** must also be primed for the apheresis procedure. In one embodiment, a

blood prime may be utilized in that blood will be the first liquid introduced into the blood processing vessel **352**. The flow of blood from the donor/patient **4** to the extracorporeal tubing circuit **10** is initiated with the centrifuge rotor assembly **568** rotating the channel housing **204** at a rotational velocity of from about 150 RPM to about 250 RPM for a rotor diameter of about 10", and typically about 200 RPM. This lower rotational velocity not only reduces the potential for air locks developing in the blood processing vessel **352**, but also minimizes any preheating of the blood processing vessel **352**. The rotational velocity in this "first stage" need not be fixed, but may vary.

[0246] Once the flow of blood reaches the blood processing vessel **352**, the rotational speed of the channel housing **204** is increased from about 1,500 RPM to about 2,500 RPM for a rotor diameter of about 10", preferably about 2000 RPM, such that blood being provided to the blood processing vessel **352** will be separated into the various blood component types even during the priming procedure. Once again, in this "second stage", the rotational velocity need not be fixed, but may vary. In order for a blood prime to be successful in the first embodiment, a flow must be provided to the control port assembly **488** before any RBCs flow beyond the RBC dam **232** in a clockwise direction. This is again provided by the configuration of the channel **208**. When there is no control port assembly **488** (see FIGS. 2C-2D), a plasma flow first desirably reaches the RBC/control port **520** before RBCs flow over or beyond the RBC dam **232** (although this is less important in this embodiment as described below).

[0247] Importantly, during this "second stage" of the blood priming procedure, air present in the blood processing vessel **352** is removed from the blood processing vessel **352** and due to the noted rotational velocities in this "second stage", the potential for air locks is also reduced. More specifically, air which is present in the blood processing vessel **352** is less dense than the whole blood and all of its blood component types. As noted above, the radially inward-most portion of the inner channel wall **212** is at the intersection between the plasma outlet slot **256** and the inner channel wall **212**. Consequently, the air present in the blood processing vessel **352** collects near the plasma outlet port **456** and is removed from the blood processing vessel **352** through the plasma outlet tubing **476**, and is provided to the vent bag **104**.

[0248] When the blood processing vessel **352** contains blood and/or blood components throughout its entirety, the rotational velocity of the channel housing **204** is increased to its normal operation speed from about 2,750 RPM to about 3,250 RPM for a rotor diameter of about 10", and preferably about 3,000 RPM. This completes the blood priming procedure.

[0249] During the above-noted blood priming procedure, as well as throughout the remainder of the apheresis procedure, blood component types are separated from each other and removed from the blood processing vessel **352** on a blood component type basis. At all times during the apheresis procedure, the flow of whole blood is provided to the blood processing vessel **352** through the blood inlet port assembly **416** and is directed to the first stage **312**. The control port dam **280** again reduces the potential for blood flowing in a counterclockwise direction in the channel **208**

in the FIG. 8A embodiment. Other detailed differences of blood priming between the embodiments disclosed herein will be further addressed below.

[0250] In the first stage 312, blood is separated into a plurality of layers of blood component types including, from the radially outermost layer to the radially innermost layer, RBCs, WBCs, platelets, and plasma. As such, the RBCs sediment against the outer channel wall 216 in the first cell separation stage 312. By configuring the RBC dam 232 such that it is a section of the channel 210 which extends further inwardly toward the rotational axis 324 of the channel housing 204, this allows the RBC dam 232 to retain separated red blood cells in the first stage 312.

[0251] Separated RBCs are removed from the first stage 312 utilizing the above-noted configuration of the outer channel wall 216 which induces the RBCs to flow in a counterclockwise direction (e.g., generally opposite to the flow of blood through the first cell separation stage 312). That is, the portion of the channel 208 proximate the RBC outlet port assembly 516 is disposed further from the rotational axis 324 of the channel housing 204 than that portion of the channel 210 proximate the RBC dam 232. As such, separated RBCs flow through the first stage 312 in a counterclockwise direction along the outer channel wall 216, past blood inlet port assembly 388 on the blood processing vessel 352, and to an RBC outlet port assembly 516. Since the vertical slot 404 of the blood inlet port 392 is substantially parallel with the inner channel wall 212, the outer channel wall 216, the inner sidewall 372 of the blood processing vessel 352 and the outer sidewall 376 of the blood processing vessel 352, since it directs the flow of blood in a clockwise direction in the channel 208 and thus toward the RBC dam 232, and since it is disposed proximate the inner channel wall 212, the introduction of blood into the blood processing vessel 352 does not substantially affect the flow of RBCs along the outer channel wall 216. Consequently, RBCs effectively flow undisturbed past the blood inlet port 392 and to the RBC outlet port assembly 516 for removal from the blood processing vessel 352. These RBCs may either be collected and/or provided back to the donor/patient 4.

[0252] An embodiment such as the first embodiment described herein (corresponding to FIGS. 2A-2B and FIG. 8A) may make use of the fact that platelets are less dense than RBCs and are thus able to flow beyond the RBC dam 232 when the RBC/buffy coat interface is disposed sufficiently close to the dam 232 (i.e., sufficiently radially inwardly disposed to be near the top of the dam 232). These platelets would then flow to the platelet collect well 236 in platelet-rich plasma where they are removed from the blood processing vessel 352 by the platelet collect port assembly 416. Again, the blood processing vessel 352 via the support 428 and the outer channel wall 216 would collectively define the platelet collect well 236 when the blood processing vessel 352 is pressurized. That is, part of the platelet collect well 236 is defined by the lower face 240 and side faces 244, 248 formed in the outer channel wall 216, while the remainder thereof is defined by the second face 436 of the support 428 when the support 428 is moved into a predetermined position within and against portions of platelet support recess 249 upon pressurization of the blood processing vessel 352.

[0253] Platelet-poor plasma is less dense than the platelets and would continue to flow in a clockwise direction through the second stage 316 to the plasma outlet port assembly 452 where at least some of the plasma is removed from the blood processing vessel 352. This plasma may be collected and/or returned to the donor/patient 4. However, some of the plasma flow continues in the clockwise direction into and through the third stage 320 to the control port assembly 488 to provide for automatic control of the location of the interface between the RBCs and platelets in the above-described manner. As described further below, preferably all of the plasma which flows over the RBC dam 232 in the second embodiment herein (FIGS. 2C-2D) would be platelet-poor and flow to the plasma outlet port assembly 452 as above, as well as to the RBC/control outlet port 520 even though there is no control port assembly 488.

[0254] Platelet/RBC (and potential Plasma) Collection

[0255] As noted, a preferred blood apheresis system 2 provides for contemporaneous separation of a plurality of blood components during blood processing, including the separation of red blood cells (RBCs), platelets and plasma. In turn, such separated blood components may be selectively collected in corresponding storage reservoirs (or bags) or immediately returned to the donor/patient 4 during a blood return submode. In this regard, and in one approach where at least platelets and/or both platelets and RBCs (and/or potentially plasma) are to be collected (see the embodiment of FIGS. 2A-2B), blood apheresis system 2 may be advantageously employed to collect platelets, and if desired separated plasma, during a time period(s) separate from the collection of red blood cells. In this manner, the collection of both high quality platelet units and high quality red blood cell units can be realized.

[0256] Moreover, the procedures described herein are preferably carried out using blood priming of extracorporeal tubing circuit 10 and blood processing vessel 352. Also, the preferred blood processing here provides for the collection of platelets in reservoir 84 during a first period and the collection of red blood cells in reservoir 954 during a second period (FIGS. 2A-2B). Plasma collection in reservoir 94 may also be selectively completed during the first period. During the platelet blood processing period and successive RBC collection procedure, blood component separation device 6 will control the initiation and termination of successive blood removal and blood return submodes, as described hereinabove. Additionally, blood component separation device 6 will control the platelet and RBC collection processes according to a predetermined protocol, including control over the divert valve assemblies 1100, 1110 and 1120 of the pump/valve/sensor assembly 1000.

[0257] More particularly, following blood priming, blood separation control device 6 provides control signals to pump/valve/sensor assembly 1000 so that in the embodiment of FIGS. 2A-2B, platelet divert valve assembly 1100 diverts the flow of separated platelets pumped through platelet outlet tubing 66 and platelet tubing loop 142 into platelet collection tubing 82 for collection in reservoir 84. If plasma collection is desired, blood component separation device 6 also provides control signals so that plasma divert valve assembly 1110 diverts the flow of separated plasma pumped through plasma outlet tubing 68 and plasma tubing loop 162 into plasma collector tubing 92 for collection in

reservoir **94**. Additionally, RBC/plasma divert valve assembly **1120** will continue to divert the flow of separated RBCs flowing through outlet tubing **64** through return tubing loop **172** and into blood return reservoir **150**. Platelet collection is carried out as previously discussed hereinabove, with a packing factor in the second stage of vessel **352** maintained at between about 4 and 15, and most preferably at about 13. When the desired volumes of platelets and plasma have been collected, blood component separation device **6** will selectively control divert assemblies **1100** and **1110** to divert the flow of platelets and plasma into reservoir **150**.

[0258] Preferably following completion of platelet and plasma collection (in the embodiment of FIGS. 2A-2B), the RBC collection procedure is initiated via control signals provided by blood collection device **6**. Such RBC collection procedure includes a setup phase and a collection phase. During the setup phase, the blood apheresis system **2** is adjusted to establish a predetermined hematocrit in those portions of the blood processing vessel **352** and extracorporeal tubing circuit **10** through which separated RBCs will pass for collection during the RBC collection phase.

[0259] More particularly, during the setup phase, and in order to realize a predetermined hematocrit of at least about 75%, for example, and more preferably at about 80%, the packing factor in the first stage **312** of the blood processing vessel **352** is established at between about 11 and about 21, and most preferably at about 13. Additionally, the AC ratio (i.e. the ratio between the inlet flow rate to vessel **352** (including whole blood plus anticoagulant AC) and the AC flow rate into tubing circuit **10**) will be established within the range of about 6 to 16, and most preferably at about 8.14 (particularly in the U.S.). Further, the total uncollected plasma flow rate through blood processing vessel **352** and extracorporeal tubing circuit **10** will be established at a predetermined level. These adjustments are carried out in simultaneous fashion to establish the desired hematocrit in an expeditious manner. As will be appreciated, the adjusted AC ratio and predetermined hematocrit should be maintained during the subsequent RBC collection phase.

[0260] During the set-up phase, blood component separation device **6** provides appropriate control signals to the pump/valve/sensor assembly **1000** such that all separated blood components flowing out of processing vessel **352** will pass to return reservoir **150**. Also, blood component separation device **6** will continue operation of blood inlet pump assembly **1030**, including operation during each blood return submode.

[0261] In order to establish the desired packing factor, the operating speed of centrifuge rotor assembly **568** may be selectively established via control signals from blood component separation device **6**, and the blood inlet flow rate to vessel **352** may be selectively controlled via control by blood component separation device **6** over pump assembly **1030**. More particularly, as mentioned above, increasing the rpms of centrifuge rotor assembly **568** and/or decreasing the inlet flow rate will tend to increase the packing factor, while decreasing the rpms and increasing the flow rate will tend to decrease the packing factor. As can then be appreciated, the blood inlet flow rate to vessel **352** is effectively limited by the desired packing factor.

[0262] To establish the desired AC ratio, blood component separation device **6** provides appropriate control signals to

anticoagulant peristaltic pump **1020** so as to introduce anticoagulant into the blood inlet flow at a predetermined rate, as previously described hereinabove. Relatedly, in this regard, it should be noted that the inlet flow rate of anticoagulated blood to blood processing vessel **352** is limited by a predetermined, maximum acceptable anticoagulant infusion rate (ACIR) to the donor/patient **4**. As will be appreciated by those skilled in the art, the predetermined ACIR may be established on a donor/patient-specific basis (e.g. to account for the particular total blood volume of the donor/patient **4**).

[0263] To establish the desired total uncollected plasma flow rate out of blood processing vessel **352**, blood collection device **6** provides appropriate control signals to plasma pump assembly **1060** and platelet pump assembly **1040**. Relative to platelet collection, such control signals will typically serve to increase plasma flow through plasma outlet port **456**, and thereby reduce plasma flow with RBCs through RBC outlet port **520**. This serves to increase the hematocrit in the separated RBCs. Additionally, it is preferable for blood processing device **6** to provide control signals to platelet pump assembly **1040** so as to establish a predetermined flow rate wherein platelets and some plasma pass together through platelet port **420**, thereby reducing platelet clumping downstream in tubing circuit **10**. In this regard, such predetermined rate will be limited by the diameter of the platelet outlet tubing **66** and the size of the internal channels (e.g. **140a**, **140b**) within molded cassette **110**.

[0264] In one embodiment, where centrifuge rotor assembly **568** defines a rotor diameter of about 10 inches, and where a blood processing vessel **352** (FIGS. 2A-2B) is utilized, as described hereinabove, it has been determined that channel housing **204** can be typically driven at a rotational velocity of about 3000 rpms to achieve the desired hematocrit during the setup and blood collection phases. Correspondingly, the blood inlet flow rate to vessel **352** should be established at or below about 64.7 ml/min. The desired hematocrit can be reliably stabilized by passing about two whole blood volumes of either reservoir **150** (in cassette **110**) or reservoir **352** through the respective reservoir before the RBC collection phase is initiated.

[0265] To initiate the RBC collection phase, blood component separation device **6** provides an appropriate control signal to RBC/plasma divert valve assembly **1120** so as to direct the flow of RBCs removed from blood processing vessel **352** into RBC collection reservoir **954**. Both the platelet divert valve assembly **1100** and plasma divert valve assembly **1110** remain in a position to direct flow into reservoir **150** for return to donor/patient **4** during blood return submodes. In the later regard, it is preferable that, during blood return submodes of the RBC collection phase, blood collection device **6** provide appropriate control signals so as to stop the operation of all pump assemblies other than return pump assembly **1090**. In this regard, stoppage of inlet pump assembly **1030** avoids recirculation of uncollected blood components into vessel **352** and resultant dilution of separated RBC components within vessel **352**.

[0266] As will be appreciated, in the present invention separated RBCs are not pumped post-separation out of vessel **352** for collection, but instead are pushed out vessel **352** and through extracorporeal tubing circuit **10** by the

pressure of the blood inlet flow to vessel **352**. Consequently, trauma to the collected RBCs is minimized.

[**0267**] During the RBC collection phase, the inlet flow into vessel **352** is limited by the above-noted maximum acceptable ACIR to the donor/patient **4**. The desired inlet flow rate is also limited by that necessary to maintain the desired packing factor, as also discussed. In this regard, it will be appreciated that, relative to the setup phase, the inlet flow rate may be adjusted slightly upwards during the RBC collection phase since not all anticoagulant is being returned to the donor/patient **4**. That is, a small portion of the AC remains with the plasma that is collected with the RBCs in RBC reservoir **954**.

[**0268**] Following collection of the desired quantity of red blood cells, blood separation device **6** may provide a control signal to divert assembly **1120**, so as to divert RBC flow to reservoir **150**. Additionally, if further blood processing is not desired, rinseback procedures may be completed. Additionally, the red blood cell reservoir **954** may be disconnected from the extracorporeal tubing circuit **10**. A storage solution may then be added. Such storage solution may advantageously facilitate storage of the RBCs for up to about 42 days at a temperature of about 1-6 degrees C. In this regard, acceptable storage solutions include a storage solution generically referred to in the United States as Additive Solution 3 (AS-3), available from Medsep Corp. located in Covina, Calif.; and a storage solution generically referred to in Europe as (SAGM), available from MacoPharma located in Tourcoing, France.

[**0269**] The storage solution may be contained in a separate storage solution bag that can be selectively interconnected to the RBC collection bag **954**. Such selective interconnection may be provided via sterile-docking tubing utilizing a sterile connecting device. By way of example, one such sterile connecting device to interconnect tubing is that offered under the trade name "SCD 312" by Terumo Medical Corporation located in Somerset, N.J. Alternatively, selective interconnection may be established utilizing the sterile barrier filter/spike assembly **956**. The use of assembly **956** facilitates the maintenance of a closed system, thereby effectively avoiding bacterial contamination. By way of example, the mechanical, sterile barrier filter in assembly **956** may include a porous membrane having 0.2 micron pores.

[**0270**] In order to ensure the maintenance of RBC quality, the RBC collection bag **954**, the storage solution and the anticoagulant used during blood processing should be compatible. For example, RBC collection reservoir **954** may comprise a standard PVC DEHP reservoir (i.e. polyvinyl chloride-diethylhexylphthalate) offered by Medsep Corporation. Alternatively, a citrated PVC reservoir may be employed. Such reservoir may utilize a plasticizer offered under the trade name "CITRIFLEX B6" by Moreflex located in Commerce, Calif. Further, the anticoagulant utilized in connection with the above-described platelet collection and red blood cell collection procedures may be an acid citrate dextrose-formula A (ACD-A).

[**0271**] After the storage solution has been added to the collected red blood cells in RBC reservoir **954**, selective filtering may be desired to remove white blood cells. More particularly, for example, leukoreduction may be desired to establish a white blood cell count at $<5 \times 10^8$ white blood

cells/unit (e.g. about 250 ml.) to reduce any likelihood of febrile nonhemolytic transfusion reactions. Further, such filtering may be desirable to achieve a white blood cell count of $<5 \times 10^6$ white blood cells/unit to reduce any risk of HLA (i.e. human leukocyte A) sensitization. If such leukoreduction is deemed appropriate, the red blood cell/storage solution mixture can be connected to a commercially available red cell filter/bag assembly so that red blood cells are gravity transferred from the collection bag **954** through a filter and into a new storage bag. Such commercially available red cell filter/bag kits include those available under the trade names "LEUKONET" or "rLS" from Hemosure, Inc. located in Marlborough, Mass., and "RC 100", "RC50" and "BPF4" from Pall Corp. located in Glencove, N.Y.

[**0272**] Several advantages can be realized utilizing the above-described procedure for red blood cell collection. Such advantages include: consistency in final RBC product volume and hematocrit; reduced exposure of a recipient if multiple units of blood products are collected from a single donor/patient and transfused to a single recipient; reduced time requirements for RBC collection and for collection of double units of red blood cells if desired.

[**0273**] While one approach for platelet and RBC collection has been described above, other approaches using the embodiment of FIGS. 2A-2B will be apparent. By way of primary example, the described RBC collection procedure may be carried out following blood priming, and prior to platelet collection. Such an approach would advantageously allow RBC collection to occur in the course of AC ramping, thereby reducing total processing time requirements. That is, since AC ramping up to a predetermined level (e.g. increasing the AC ratio up to about 13) is typically, gradually completed prior to the start of a platelet collection procedure (e.g. so as to maintain an acceptable ACIR), completing RBC collection procedures in the course of AC ramping would reduce the overall processing time for RBC and platelet collection. The RBC collection procedure could be completed when AC ramping reaches about 8.14, with AC ramping continuing thereafter. Alternately, RBC collection could occur in tandem with AC ramping, wherein the target AC ratio of about 8.14 would be established as an average effective ratio for the RBCs and plasma collected and mixed within reservoir **954**.

[**0274**] Further, and as noted above, plasma collection could occur contemporaneous with RBC collection. Additionally, in this regard, plasma collection could occur during both platelet and RBC collection procedures, depending upon the volume of plasma product desired. Finally, it has been recognized that the present invention of embodiment of FIGS. 2A-2B may also be employable to simultaneously separate and collect both red blood cells and platelets, and if desired, plasma.

[**0275**] RBC/Plasma (Generally Non-Platelet) Collection

[**0276**] As noted, a preferred blood apheresis system **2** also provides for continuous separation of red blood cells (RBCs) and plasma with various alternative collection options. For example, continuous separation may be provided with contemporaneous collection of both RBCs and plasma and/or with collection of either RBCs or plasma separately (see e.g., the embodiment of FIGS. 2C-2D and **8B**). In the preferred system, all the non-collected components are re-

infused into the donor. Moreover, the separated blood components, RBCs and/or plasma (in the embodiments of FIGS. 2C-2D, e.g.), may be selectively collected, as described above, in corresponding storage reservoirs or immediately returned to the donor/patient **4** during a blood return/replacement fluid delivery submode. Note, the buffy coat components; namely platelets and WBCs are not collected separately in this embodiment (FIGS. 2C-2D). Rather, these components preferably remain with the RBCs throughout these procedures and may either be filtered out subsequently, e.g., the WBCs through a leukoreduction filter (e.g. "COBE rLS" filter) or the like; or may remain with the RBC product(s) as the platelets likely will, albeit without any deleterious effect. Preferably, the plasma product(s) hereof will remain platelet-poor and contain no WBCs (or at least within promulgated minimum safety ranges).

[0277] In the present embodiment (FIGS. 2C-2D and 8B), any of three options is primarily available, the collection of RBCs and plasma contemporaneously, or RBCs alone, or plasma alone (in either "alone" case, the collection may mean no other product is ever collected during that procedure, or no other product is collected at the same time; previous or subsequent collection is also possible). And in one approach where both plasma and RBCs are to be collected, blood apheresis system **2** may preferably be advantageously employed to collect RBCs and plasma contemporaneously for a first time period, and then collect either plasma or red blood cells for a second period. In this manner, the collection of both high quality plasma units and high quality red blood cell units can be realized. Target yields for both components are thus also preferably achieved or achievable. This may thus include double red blood cell products, for example. Note, a double product quantity is preferably configurable by the user; however, suggestions have been made for red blood cell products to be targeted at about 180 or 200 milliliters in pure form, which would be 225 or 250 ml at 80 hematocrit (i.e., including 20% plasma in the end product). Thus, a double RBC product under these suggestions would be about 360 or about 400 ml. in pure form and 450 to 500 at 80 hematocrit. Note, the 180 ml. suggestion may be based upon an understood concept of a whole blood donation unit of 450 ml. $\pm 10\%$ which would provide about 60 grams of hemoglobin (Hb) or an average 180 ml. hematocrit (Ht) (see U.S. Federal Food and Drug Administration (FDA) suggestions). Other sizes can also be configured and collected based upon donor ability.

[0278] Replacement fluid(s) are preferably also optionally administrable within the procedures of the present invention using the embodiment of FIGS. 2C-2D. Sterile saline solution(s) and/or replacement/exchange plasma (and/or replacement/exchange red blood cells) are optional replacement fluids, inter alia, considered for use herein. Thus, if/when large fluid amounts of plasma and/or RBCs are taken from a donor/patient, replacement fluid(s) may be delivered in return to leave the donor/patient adequately hydrated. I.e., replacement fluids may, in certain situations, qualify more product options from a given donor. For example, a particular donor may not qualify for a certain donation (e.g., a double RBC product) under normal conditions; however, with a replacement fluid infusion, that donor may then qualify for that donation.

[0279] Also, replacement fluids may also be used to avoid hypovolemia and like reactions. Bolus deliveries are also

preferably deliverable herewithin. Exchange fluids (plasma and/or RBCs) may be used for therapeutic purposes as well. These alternatives are detailed further hereinbelow. Note first however that it is preferable that the one or more replacement fluid spike assembly(ies) **964** (**964a/964b**) are/ may be similar structurally and/or functionally to the anticoagulant spike assembly **50/52** shown and described hereinabove; but it is preferable that there be some distinction therebetween for safety reasons. For example, if a plastic spike is used for the anticoagulant line(s), it would then be preferable to include a metal or distinctly colored or shaped spike or spikes for the replacement fluid line(s) so that the operator will not confuse them and accidentally run anticoagulant into the replacement fluid system and thereby potentially seriously overload the donor/patient with anticoagulant.

[0280] The general set-up or initiation procedures described hereinabove for any and/or all other apheresis procedures are likewise and/or similarly carried out here to provide blood priming of extracorporeal tubing circuit **10a** (FIGS. 2C-2D) and blood processing vessel **352a** (FIG. 8B) (distinctions are described herein). The initiation of blood processing thereafter then provides for the collection of plasma in one or more reservoir(s) **94** and/or the collection of red blood cells in one or more reservoir(s) **954**. Alternatively, either RBC collection in reservoir(s) **954** or plasma collection in reservoir(s) **94** may also be selectively completed in separate procedures. During either collection procedure, blood component separation device **6** preferably controls the initiation and termination of successive blood removal and blood return submodes, as described for example, in the preferred embodiment hereinabove (from and to the donor through level control in the cassette reservoir **150** using the two ultrasound fluid level detectors **1300, 1320**, e.g.). Additionally, blood component separation device **6** will control the plasma and RBC collection processes according to predetermined protocols, preferably including control over the preferred valve assemblies **1100, 1110** and **1120** of the pump/valve/sensor assembly **1000**, and/or the appropriate pumps **1020, 1030, 1040, 1060** and/or **1090**.

[0281] Initially, blood priming is carried out generally as described hereinabove. However, as described here, a further step during priming is preferably instituted prior to starting component collection. During blood priming, it is still desirable that the component separation begin even during the priming stage, and that plasma flows over the RBC dam **232** and continues around to the plasma outlet port **456** and still further around to the RBC/control outlet **520** (see FIG. 8B); while RBCs build up behind the RBC dam **232** and flow in a counterflow direction back to the RBC/control outlet **520**. (Note that the buffy coat elements preferably remain behind the dam **232** as well and flow to the RBC outlet port **520** with the RBCs; however, even though not preferred, sufficient functionality may nevertheless likely be retained even if some RBCs and/or buffy coat components flow over the dam **232** during priming. Potential WBC contamination of platelet collection apparatus is not here in issue, though it may be an issue for the plasma collection assembly, as well). The further priming step here is to then shut the plasma pump **1060** off for a period and thereby force a greater quantity of separated plasma toward the RBC/control outlet port **520**, and thereby force the high hematocrit separated RBCs out of the vessel **352a** through

the RBC/control outlet **520** until the plasma/RBC interface moves radially outward toward the orifice **536** of the outlet port **520**. Eventually, plasma reaches the orifice **536** and spills therein and flows out through the outlet port **520**. This plasma spilling into port **520** suggests it may also be called a spill port **520**. Note, a greater quantity of plasma also fills the first stage **312** thus also contributing to the forcing of the RBC/plasma interface radially outward. Then, when the interface is established at or sufficiently adjacent the RBC orifice **536**, as preferred here, the plasma pump may be automatically turned back on by the separation device **6** at a rate which maintains the RBC/plasma interface at or sufficiently adjacent the radial level of the RBC/control outlet orifice **536**. In particular, it is desirable that the interface be maintained at this location such that a mixed flow of RBCs and plasma is maintained continuously through the RBC/control outlet port **520** such that the mixed flow of RBCs and plasma has reached and continues at a target hematocrit, here preferably at about **80**. Maintenance by the device **6** of a particular relationship of the rate of plasma outflow generated by the plasma pump **1060** relative to the inlet rate of blood flow generated by the blood inlet pump **1030** provides for continuing the target output hematocrit of the RBC/plasma mixed flow through the RBC/control outlet port **520**.

[0282] Following and/or contemporaneously with the blood priming phase as described hereinabove, blood separation control device **6** provides control signals to pump/valve/sensor assembly **1000** so that the replacement fluid lines may also be primed. In particular, replacement fluid valve assembly **1100** is opened and replacement fluid inlet pump **1040** is switched on to provide for the pumping of saline solution (or other replacement fluid(s)) through replacement fluid inlet tubing **962** and the replacement fluid tubing loop **142a** into replacement fluid introduction tubing line **146** for initial collection in cassette reservoir **150**, though this initial priming collection will likely and preferably does constitute a small amount of replacement fluid(s).

[0283] After priming is completed, yet still during the set-up phase, blood component separation device **6** may provide appropriate control signals to the pump/valve/sensor assembly **1000** such that all separated blood components flowing out of processing vessel **352a** will first pass to return/delivery reservoir **150**. Optionally, one or more cycles (preferably two) of separation and return of all blood components back to the donor may be performed before collection(s) and/or regular replacement fluid deliveries begin (this may be performed in order to stabilize the hematocrit in the first stage of vessel **352a**). Any replacement fluid(s) collected in reservoir **150** during priming (again, likely very small amounts) may also be delivered to the donor/patient at this time. Also, blood component separation device **6** may continue operation of blood inlet pump assembly **1030** during one or more these initial blood component return submodes.

[0284] Then, the process of collection may begin. If plasma collection is not desired, plasma divert assembly **1110** maintains the flow of separated plasma from the vessel **352a** to the reservoir **150** for return to the donor/patient **4**. However, if plasma collection is desired (either alone or contemporaneously with RBCs), blood component separation device **6** may provide control signals so that plasma divert valve assembly **1110** switches to divert the flow of

separated plasma pumped from vessel **352a** through plasma outlet tubing **68** and plasma tubing loop **162** into plasma collector tubing **92** for collection in one or more plasma reservoir(s) **94**. Additionally, if plasma is to be collected alone, RBC divert valve assembly **1120** will continue to maintain the flow of separated RBCs flowing from vessel **352a** through outlet tubing **64** through return tubing loop **172** and into blood return reservoir **150**. However, if RBCs are to be collected, alone or contemporaneously with plasma, then the RBC divert valve assembly **1120** switches to divert the flow of separated RBCs flowing from tubing **64** to and through spur **170b** (of cassette **110**) and into and through tubing line **952** to the one or more RBC collection reservoir(s) **954**. No platelet collection is preferably carried out in this embodiment as previously discussed hereinabove.

[0285] Preferably during any of the collection processes involved with this embodiment (FIGS. 2C-2D), one or more replacement fluid(s) are also delivered to the donor/patient **4**. Thus, whenever either divert valve assembly **1110** or **1120** is switched by the separation device **6** into a collection mode, then the replacement fluid inlet valve assembly **1100** may also be opened and the replacement fluid pump **1040** started to flow replacement fluids from the fluid source (not shown) through tubing line **962**, cassette passageways **140c** and **140d**, and tubing loops **142a** and **146** into the reservoir **150** (FIGS. 2C-2D). As a basic premise, the replacement fluid flow rate is equal to the total collection flow rate multiplied by the percentage of fluid desired to be given back to the donor/patient **4**. This last factor is called a fluid balance percentage. Preferably, the rate of replacement fluid flow (Q_{rf}) is governed by the relationship of the total collection flow rate (Q_{tot}) minus the flow rate of the anticoagulant inflow (Q_{ac}) multiplied by the total fluid balance percentage (FB) ultimately delivered back to the donor/patient **4**. In mathematical form;

$$Q_{rf} = [Q_{tot} - Q_{ac}] * FB;$$

[0286] Preferably, the fluid balance percentage is chosen within a limited range of 80% and 120% (e.g., 80% representing the lessened amount of fluid the donor/patient **4** is given back, or has received at the end of the procedure relative to the donor/patient's donation amount, and 120% representing the additional amount of fluid given to the donor/patient **4** over the donation amount; thus, if 80% is chosen for example, then the donor/patient **4** ends the procedure with 80% of the donated fluid volume).

[0287] Note, a farther option of fluid bolus infusion may be offered with a replacement fluid assembly such as that described herein. For example, a procedure for bolus infusion may be made available at any desired point in a procedure. As such, it may involve stopping all pumps except at least the replacement fluid inlet pump **1040** which delivers replacement fluid to the reservoir **150** at a selected infusion rate, then (with perhaps a slight delay to ensure a minimum level of fluid is present in the reservoir **150** prior to fluid return/delivery to the donor/patient), the return/delivery pump **1090** may be started to deliver the replacement fluid from the reservoir **150** to the donor/patient **4**. A bolus button for initiating such a procedure may be permanently disposed on the separation device **6**, and/or it may preferably be disposed on one or more selected touch screen(s) (see generally below) which may be displayed on

the computer graphical interface **660**. This may appear on an adjustment or troubleshooting screen, for example (see description(s) below).

[0288] When RBCs are collected contemporaneously with plasma, a packing factor in the first stage of vessel **352a** is maintained preferably at 16. If RBCs are collected alone, then the packing factor is set between about 4 and 15, more preferably between 11 and 15, and most preferably at about 13. When the desired volumes of RBCs and/or plasma have been collected, blood component separation device **6** will preferably selectively control divert assemblies **1110** and **1120** to divert the respective flow of RBCs and/or plasma (whichever has reached its desired collected volume) into reservoir **150**.

[0289] Following contemporaneous RBC and plasma collection (if this procedure is chosen), at which point either the target RBC volume/yield or the target plasma volume/yield (or both) has been reached, then the respective divert valve assembly **1110** or **1120** (or both) of the respective component whose target volume/yield has been reached is switched to divert flow of that separated component to flow to the reservoir **150**. Thus, if and when the target volume/yield of RBCs has been reached, then the divert valve assembly **1120** may be switched to return flow of separated RBCs to the reservoir **150**, independent of and/or even if the plasma target volume/yield has not yet been reached. The same may be true in reverse, if and when the plasma target volume/yield has been reached, even if this occurs before the RBC target is reached, then the plasma divert valve assembly **1110** may be switched to flow the still in-coming separated plasma to the reservoir **150**. Then, collection of the other component is preferably continued until its target volume/yield is reached. Note, though either separated component may be collected first, and then the other components collected after the target volume/yield of the first component has been reached, it is preferable to start the procedure collecting both RBCs and plasma contemporaneously (assuming that a quantity of both products are desired from a given donor), and then switch to collecting only the component whose target volume/yield has not yet been reached when the other target has been reached.

[0290] Control over these switching steps after achieving either the RBC or the plasma target collection volumes/yields is initiated via control signals provided by blood collection/separation device **6** to the respective divert valve assemblies **1110** and **1120**. Note also that the separation device **6** may make further adjustments as well upon switching from the contemporaneous collection of RBCs and plasma to the collection of only one such component. For example, the packing factor has been noted as preferably kept at 16 with a target hematocrit of 80 during collection of both RBCs and plasma contemporaneously. However, when the target volume/yield of one or the other blood component has been reached and then collection of only one component is continued, then the separation device **6** preferably adjusts to the preferred packing factor or hematocrit value as discussed herein. Specifically, if the plasma target has been reached, but RBC collection is to continue, the separation device preferably lowers the packing factor to the range disclosed herein, preferably to 11-15, or set even more preferably at 13 while maintaining a target hematocrit of 80. If, on the other hand, collection of plasma is instead to be continued after the target for RBCs has been reached, then

the separation device **6** may reset the target hematocrit to approximately 55, for example, without concern for the resulting or actually occurring packing factor at this point.

[0291] Such RBC and/or plasma collection procedures may also include a setup phase and a collection phase. During a setup phase, the blood apheresis system **2** may be adjusted to establish a predetermined hematocrit in those portions of the blood processing vessel **352a** and extracorporeal tubing circuit **10a** through which separated RBCs will pass for collection during the RBC collection phase. More particularly, during the setup phase, and in order to realize a predetermined hematocrit of about 80%, the packing factor in the first stage **312** of the blood processing vessel **352a** is established at between about 11 and about 21, and most preferably at about 16 for contemporaneous RBC and plasma collections, or 13 for RBC collections, alone. These are the preferred packing factors for collection phases of RBCs and plasma simultaneously, and RBCs alone, see discussions throughout. Additionally, the AC ratio (i.e. the ratio between the inlet flow rate to vessel **352a** (including whole blood plus anticoagulant AC) and the AC flow rate into tubing circuit **10**) will be established within the range of about 6 to 16, and most preferably at about 8.14 (in the United States) and/or 11 (in other countries). Further, the total uncollected plasma flow rate through blood processing vessel **352a** and extracorporeal tubing circuit **10** may be established at a predetermined level. These adjustments are preferably carried out by controlling the speeds of the respective pumps and/or the centrifuge which may be adjusted in simultaneous fashion to establish the desired hematocrit in an expeditious manner. As will be appreciated, this adjusted AC ratio and predetermined hematocrit should be maintained during the subsequent RBC and plasma collection phase(s).

[0292] These adjustments will not affect the other collection control parameters where again, when collecting RBCs alone, the target hematocrit remains at 80, but the packing factor is preferably reduced to, for example, 11-13. This is similar to the RBC packing factor preference described above for the collection phase of RBCs after platelet collection has ceased (for the platelet/plasma/RBC embodiment; e.g., FIGS. 2A-2B, and corresponding description, above). Further still, when collecting plasma alone, the target hematocrit is preferably dropped to 55, and the packing factor in the first stage is not an issue (also as described hereinabove).

[0293] In order to establish the desired packing factor, the operating speed of centrifuge rotor assembly **568** may be selectively established via control signals from blood component separation device **6**, and/or the blood inlet flow rate to vessel **352a** may be selectively controlled via control by blood component separation device **6** over pump assembly **1030**, and/or the plasma flow rate out through port **456** may similarly be controlled by device **6** through pump **1060**. More particularly, increasing the rpms of centrifuge rotor assembly **568** and/or decreasing the inlet flow rate will tend to increase the packing factor, while decreasing the rpms and/or increasing the flow rate will tend to decrease the packing factor. As can be appreciated, the blood inlet flow rate to vessel **352a** is effectively limited by the desired packing factor.

[0294] To establish the desired AC ratio, blood component separation device **6** provides appropriate control signals to

anticoagulant peristaltic pump **1020** so as to introduce anticoagulant into the blood inlet flow at a predetermined rate, as previously described hereinabove. Relatedly, in this regard, it should be noted that the inlet flow rate of anticoagulated blood to blood processing vessel **352a** is limited by a predetermined, maximum acceptable anticoagulant infusion rate (ACIR) to the donor/patient **4**. As will be appreciated by those skilled in the art, the predetermined ACIR may be established on a donor/patient-specific basis (e.g., to account for the particular total blood volume of the donor/patient **4**).

[0295] To establish the desired total uncollected plasma flow rate out of blood processing vessel **352a**, it should be noted that when RBCs and plasma are collected simultaneously/contemporaneously, there is no uncollected plasma. Further, when plasma is collected alone, the uncollected plasma is that portion of the RBC/plasma outflow (i.e., that plasma flowing out RBC outlet port **520** with the RBC's through line **64**) which may be determined by the hematocrit thereof. With a target hematocrit of about 55 in RBC line **64** during plasma collection alone, the uncollected plasma will constitute about 45% of that outflow. In either event, the blood collection device **6** provides appropriate control signals to plasma pump assembly **1060** to establish the desired total plasma flow rate, uncollected or collected. Relative to RBC collection, on the other hand, such control signals will typically serve to increase plasma flow through plasma outlet port **456**, and thereby reduce plasma flow with RBCs through RBC outlet port **520**. This serves to increase the hematocrit in the separated RBCs, to the target hematocrit of 80.

[0296] In one embodiment, where centrifuge rotor assembly **568** defines a rotor diameter of about 10 inches, and where a blood processing vessel **352a** (see FIGS. 2C-2D and 8B) is utilized, as described hereinabove, it has been determined that channel housing **204** can be typically driven at a rotational velocity of about 3000 rpms to achieve the desired hematocrit during the both the setup and component collection phases. Correspondingly, the blood inlet flow rate to vessel **352a** should preferably be established at below about 64.7 ml/min. The desired hematocrit can be reliably stabilized by passing about two whole blood volumes of vessel **352a** through vessel **352a** before the RBC and/or plasma collection phases are initiated.

[0297] To initiate an RBC collection phase, blood component separation device **6** provides an appropriate control signal to RBC divert valve assembly **1120** so as to direct the flow of RBCs removed from blood processing vessel **352a** into RBC collection reservoir **954**. In an RBC only collection, plasma divert valve assembly **1110** remains in a position to direct flow into reservoir **150** for return of the separated plasma to donor/patient **4** during blood return/replacement fluid delivery submodes. Upon and/or simultaneously with initiation of RBC collection, replacement fluid valve assembly **1100** also preferably is switched to provide replacement fluid flow also into the reservoir **150**. In all RBC collection and/or replacement fluid operational phases, it is preferable that, during blood component return/replacement fluid delivery submodes of the RBC collection phase, blood collection and separation device **6** provides appropriate control signals so as to stop the operation of all pump assemblies other than return/delivery pump assembly **1090**. In this regard, stoppage of inlet pump assembly **1030** avoids

recirculation of uncollected blood components and/or replacement fluid(s) into vessel **352a** and resultant dilution of separated RBC components within vessel **352a**.

[0298] As will be appreciated, and as was also true in the previously described above, in the present invention separated RBCs are not pumped post-separation out of vessel **352a** through line **64** for collection, but instead are moved out of vessel **352a** and through extracorporeal tubing circuit **10a** by the relative pressure of the blood inlet flow to vessel **352a** (as this may be modified by the plasma outlet pressure through the plasma outlet port **456**). Consequently, trauma to the separated and collected RBCs is minimized.

[0299] During the RBC and/or plasma collection phases, the inlet flow into vessel **352a** is limited as described above by the above-noted maximum acceptable ACIR to the donor/patient **4**. The desired inlet flow rate is also limited by that necessary to maintain the desired packing factor, as also discussed. In this regard, it will be appreciated that, relative to the setup phase, the inlet flow rate may be adjusted slightly upwards during the RBC and/or plasma collection phases since not all anticoagulant is being returned to the donor/patient **4**. That is, a portion of the anticoagulant remains with the collected plasma and/or the plasma that is collected with the RBCs in RBC reservoir(s) **954**.

[0300] Following collection of the desired quantity of red blood cells and/or plasma, and after blood separation device **6** has provided control signals to divert assemblies **1110** and **1120**, so as to divert the respective separated plasma and separated RBC flows to reservoir **150**, if further blood processing is not desired, rinseback procedures may then be completed as generally described above. However, here (in the embodiment of FIGS. 2C-2D) where there is no platelet pump splitting the rinseback flow, the plasma pump **1060** is set at the full plasma rate equal to rate of the return/delivery pump **1090** for rinseback. Note again, that the replacement fluid inlet pump **1040** is stopped here also as in all (non-bolus) instances when no RBCs or plasma are being collected.

[0301] Additionally, at the end of the procedures, the plasma bag(s) **94** and the red blood cell reservoir(s) **954** may be disconnected from the extracorporeal tubing circuit **10** in fashions like those described above. Storage solutions may also be added, also as described above. Post-collection filtration may also be performed. For example, leukoreduction/white blood cell filtration from the collected RBCs in a fashion as described above, before or after the option of adding a storage solution. The storage solutions and/or filtration devices and corresponding final storage reservoir(s) (not shown) may, as described hereinabove, be preconnected to the collection reservoirs herein, or attached subsequently via sterile connection or spike and sterile barrier connections, also as described hereinabove.

[0302] Note, a further beneficial feature of the present invention is that it is preferred that the system **2** be able to monitor or model the hematocrit (and/or platelet count) and the total blood volume of the donor/patient **4** during the overall procedure. For example, the machine **6** can continuously and instantaneously monitor the quantity of RBCs collected, the plasma collected, the anticoagulant (AC) collected with either or both the RBCs and/or plasma as well as the AC delivered to the donor/patient **4**, and, if used, the saline/replacement solution delivered to the donor/patient **4**

to determine the instantaneous hematocrit (and/or platelet count and/or the total blood volume) of the donor/patient **4**. If for example, a donor started with a 45 hematocrit and a total blood volume of 5 liters (roughly equivalent to about 2.25 liters of RBCs), and the equivalent of 0.5 liters of whole blood were removed, and say a 0.5 liters of replacement fluid were added, then a result would be 2.02 liters of RBCs with a total blood volume of 5 liters and a resulting hematocrit of 40. Most desirably, this drop of hematocrit during a procedure may be instantaneously modeled so that the target hematocrit of the resulting products can continue to met. This may mean adjustments to certain flow rates such as the plasma pump rate to ensure that the target amount of separated plasma reaches and exits with the RBCs through the RBC exit port to provide the target hematocrit. Double red blood cell products and/or replacement fluid options will have greater impact on and/or be more greatly impacted by the instantaneous hematocrit of the donor/patient. Thus, this modeling provides better ensurance that the target hematocrit will be reached even in a double red blood cell product.

[0303] Note further that instantaneous platelet and/or total blood volume monitoring may also be performed in similar fashions, and can also be used to ensure the quality of the platelet and/or plasma products by feed back adjustment control over certain flow rates. Moreover, these and similar procedures may be used to mode for ending or post hematocrit, platelet count and/or total blood volumes as protection measures for the donor/patient. For example, an ending total blood volume (or instantaneous such volume) may be pre-set as a maximum removal from the body in total (or at any time during the procedure); then, the machine **6** will be pre-disposed to disallow the start of any procedures (or stop a progressing procedure) which would ever remove in total (or at anytime during a procedure) any amount more than this pre-set maximum. An example maximum might be 15% of the donor's starting total volume (calculated preferably using height and weight). A user could choose other percentage options as well, as for example a more conservative 13%, inter alia. Similarly, post hematocrit and platelet post-count limits may also be pre-set (or configurable per each donor). Examples might be 30 or 32 post hematocrits, and/or 50,000 or 100,000 platelet post-counts. Maximum procedure times might also be used in such donor safety areas; e.g., 120 or 150 minute maximum procedure times.

[0304] As above, several advantages can be realized utilizing these procedures for red blood cell and/or plasma collections. Such advantages include: consistency in final RBC product volume and hematocrit; reduced exposure of a recipient if multiple units of blood products are collected from a single donor/patient and transfused to a single recipient; reduced time requirements for RBC and/or plasma collections and for collection of double units of red blood cells if desired.

[0305] Various approaches for plasma and RBC collection have been described above, and other approaches may also be beneficial. By way of an example, the described RBC collection procedure may be carried out following blood priming, but prior to plasma collection. Such an approach may advantageously allow RBC collection to occur in the course of AC ramping, thereby perhaps reducing total processing time requirements. That is, since AC ramping up to a predetermined level (e.g. increasing the AC ratio up to about 13), may be gradually completed prior to the start of

a plasma collection procedure (e.g. so as to maintain an acceptable ACIR), completing RBC collection procedures in the course of AC ramping may reduce the overall processing time for both RBC and plasma collection. The RBC collection procedure could be completed when AC ramping reaches about 8.14 (in the U.S.) or 11 (in other countries), with AC ramping continuing thereafter. Alternatively, RBC collection could occur in tandem with AC ramping, wherein the target AC ratio of about 8.14 or 11 would be established as an average effective ratio for the RBCs and plasma collected and mixed within reservoir(s) **954**.

[0306] Further alternative procedures are available, for example in therapeutic exchanges of RBCs or plasma, such that the exchange RBCs or plasma is the replacement fluid to be delivered through the replacement fluid tubing assembly **960** to the donor/patient **4** while the corresponding RBCs or plasma is removed from the donor/patient as described hereinabove. Collected components may similarly be therapeutically treated upon collection and then returned to the patient through the replacement fluid tubing assembly **960**.

[0307] Alternative Collections

[0308] As mentioned, the present invention provides for the selection of various alternative component products to be collected. At least two discrete tubing and processing vessel sets have been described to achieve these options. The primary advantage is that any of these and other options may be obtained on the same platform or system. For example, extracorporeal blood processing system **2** (see generally **FIG. 1**) may be used to separate blood in various components and provide for the selection of collections of platelets (single, double or triple products, e.g.), alone or in combination with other products such as RBCs (single or double) and/or plasma (various quantities). More directly, given a particular donor ability (through blood volume, hematocrit and platelet count, e.g.), an operator of the present system may be presented with various options of donation combinations. Then, the operator may choose the most desirable option, and load the appropriate tubing set (see e.g., **FIGS. 2A-2B** vs. **2C-2D**) on the machine **6**, and then collect the desired component products. The system **2**/machine **6** would operate the appropriate protocols as described hereinabove.

[0309] Note, other options are foreseeable as well. For example, though not explicitly shown above (not as preferred), platelets could be collected on a tubing set having a replacement fluid option such as that described relative to **FIGS. 2C-2D**. However, the vessel would be like vessel **325** (**FIGS. 2A-2B**, with the platelet outlet line running to and through the plasma pump **1060**, e.g.) and the protocol preferably as described for the RBC/platelet option above (preferably platelet collection first, with RBCs to follow). Or, such a platelet/RBC with replacement fluids option could be formed of the tubing set of **FIGS. 2A-2B** with the replacement fluids run through the plasma pump **1060** with no plasma collection reservoirs then available. The limiting factor in the shown system is a further pump. In other words, if a further pump were added (not shown) to the machine **6**, then a platelet/plasma/RBC tubing set such as that shown in **FIGS. 2A-2B** could be used with an additional pump and tubing line set running to and through the added pump to flow to the reservoir **150**. A further limiting factor is that during platelet collections, replacement fluids are generally not necessary. Larger collections, such as double red blood

cell products more often indicate a desirability for replacement fluids. Along this line, a further red blood cell container could be added to the tubing set of FIGS. 2A-2B; however, again, the preference would be to have a replacement fluid option available (though not necessary in all cases) for double red blood cell collections.

[0310] In either case, substantially all practical options are presently available using the two tubing sets shown and described herein. Moreover, other sets are also available, as for example a platelet/plasma set such as is shown and described in U.S. Pat. No. 5,653,887 to Wahl et al.; inter alia (assigned to the assignee of the present document). Such sets (as described therein) may also be used with the system of the present invention, and provide a further option to the users hereof.

[0311] Graphical Computer Interface

[0312] In order to assist an operator in performing the various steps of the protocol being used in an apheresis procedure with the apheresis system 2, the apheresis system 2 further includes a computer graphical interface 660 illustrated in FIG. 1. The following description describes an interface for use by an English language speaking operator. For other operations and/or languages, the textual portions of the interface would, of course, be adapted accordingly. The graphical interface 660 includes a computer display 664 which has "touch screen" capabilities. Other appropriate input devices (e.g., keyboard) may also be utilized alone or in combination the touch screen. For example, a pump pause and a centrifuge stop button of the well known membrane type may be provided. The graphics interface 660 not only allows the operator to provide the necessary input to the apheresis system 2 such that the parameters associated with operation of the apheresis system may be determined (e.g., data entry to allow determination of various control parameters associated with the operation of the apheresis system 2), but the interface 660 also assists the operator by providing pictorials of at least certain steps of the apheresis procedure. Moreover, the interface 660 also effectively conveys the status of the apheresis procedure to the operator. Furthermore, the interface 660 also may be used to activate standardized corrective actions (i.e., such that the operator need only identify the problem and indicate the same to the interface 660 which will then direct the apheresis system 2 to correct the same).

[0313] Referring to FIG. 26, at the start of an apheresis procedure a master screen 696 is displayed to the operator on the display 664. The master screen 696, as well as each of the screens displayed to the operator by the interface 600, includes a status bar 676. The status bar 676 includes a system prep icon set 700. The system prep icon set 700 includes a load icon 704 (representing the shape of blood component separation device 6) with a downwardly extending arrow which collectively pictorially conveys to the operator that the disposable set 8 must be loaded onto the blood component separation device 6. The word "LOAD" is also positioned below the load icon 704 to provide a short textual instruction to the operator of the required action(s).

[0314] The system prep icon set 700 also includes an information icon 708 (representing the shape of an open filing folder) which pictorially conveys to the operator that certain information relating to the donor/patient 4, the procedure protocol, and/or the blood component separation

device 6 must be obtained and entered. This information may be utilized by the apheresis system 2 to calculate one or more of the parameters associated with the apheresis procedure (e.g., inlet flow rate to the blood processing vessel 352) and/or to generate predicted yields of one or more blood component types (e.g., the amount of a certain blood component type which is anticipated to be collected based upon certain parameters such as donation time). The word "INFO" is also positioned below the information icon 708 to provide a short textual instruction to the operator of the required action(s). The information icon 708 is also positioned to the right of the load icon 704 to indicate to the operator that it is preferred, although not required, to perform the step(s) associated with the information icon 708 after the step(s) associated with the load icon 704 have been completed.

[0315] The status bar 676 also includes a collection icon set 712. The collection icon set 712 includes a donor/patient prep icon 716 (representing the shape of the donor/patient 4) which pictorially conveys to the operator that the donor/patient 4 must now be fluidly interconnected with the blood component separation device 6. The word "PREPARE" is also positioned below the donor/patient prep icon 716 to provide a short textual instruction to the operator of the required action(s). The donor/patient prep icon 716 is also positioned to the right of the information icon 708 to indicate to the operator that the step(s) associated with the donor/patient prep icon 716 may only be performed after the step(s) associated with the load icon 704 and the information icon 708 have been completed.

[0316] The collection icon set 712 also includes a donate icon 720 with a laterally extending arrow which collectively pictorially conveys to the operator that the actual collection procedure may be initiated and that the step(s) to initiate this action should now be performed. The word "DONATE" is also positioned below the donate icon 720 to provide a short textual instruction to the operator of the required action(s). The donate prep icon 720 is also positioned to the right of the donor/patient prep icon 716 to indicate to the operator that the step(s) associated with the donate icon 720 must be performed after the step(s) associated with the donor/patient prep icon 716 have been completed.

[0317] The status bar 676 also includes an unload icon 724 (representing the shape of the blood component separation device 6) and a generally upwardly extending arrow which collectively pictorially convey to the operator that the disposable set must now be removed from the blood component separation device 6. The word "UNLOAD" is also positioned below the unload icon 724 to provide a short textual instruction to the operator of the required action(s). The unload icon 724 is also positioned to the right of the donate icon 720 to indicate to the operator that the step(s) associated with the unload icon 724 must be performed after the step(s) associated with the donate icon 720 have been completed.

[0318] The system preparation icon set 700, collection icon set 712, and unload icon 724 in the status bar 676 sequentially set forth certain basic steps for the apheresis procedure. That is, the left to right positioning of the various icons conveys to the operator the desired/required order in which the step(s) associated with the icons should/must be performed. Moreover, the individual icons 704, 708, 716, 720, and 724 are also utilized to convey the status of the

apheresis procedure to the operator via three-way color differentiation (i.e., one status per color) and/or by three-way shade differentiation. "Shades" includes variations of a given color and also encompasses using variations based upon being "lighter" and/or "darker" (e.g., using light gray, medium gray, and dark gray). That is, a "gray-scale" technique may also be utilized and is encompassed by use of color and/or shade differentiation.

[0319] The first status conveyed to the operator by the icons in the status bar 676 is that the step(s) associated with respective icon are not ready to be performed. That is, the performance of this step(s) would be premature. This first status is conveyed to the operator by displaying the associated icon in a first color, such as white. The corresponding textual description may also be presented in this first color as well. As noted, a first "shade" may also be utilized to convey this first status as well.

[0320] The second status conveyed to the operator by the icons in the status bar 676 is that the step(s) associated with the respective icon is either ready for execution or is in fact currently being executed. That is, an indication is provided to the operator that performance of this step(s) of the apheresis procedure is now timely. This second status is conveyed to the operator by displaying the associated icon in a second color, such as yellow. The corresponding textual description may also be presented in this second color as well. As noted, second "shade" may also be utilized to convey this second status as well.

[0321] The third status conveyed to the operator by the icons in the status bar 676 is that the step(s) associated with the respective icon has been executed. That is, an indication is provided to the operator that performance of this step(s) of the apheresis procedure has been completed. This third status is conveyed to the operator by displaying the associated icon in a third color, such as gray. The corresponding textual description may also be presented in this third color as well. As noted, third "shade" may also be utilized to convey this third status as well.

[0322] Based upon the foregoing, it will be appreciated that significant information is conveyed to the operator by merely viewing the status bar 676. For instance, the operator is provided with a pictorial graphic indicative of the fundamental steps of an apheresis procedure. Moreover, the operator is provided with a textual graphic indicative of the fundamental steps of an apheresis procedure. Furthermore, the operator is provided with a desired/required order in which these steps should/must be performed. Finally, the operator is provided with the status of the apheresis procedure via the noted three-way color/shade differentiation.

[0323] The master screen 696, as well all other screens displayed to the operator by the interface 660 during an apheresis procedure, also include a work area 688. The work area 688 provides multiple functions. Initially, the work area 688 displays additional information (pictorially and textually in some instances) on performing the apheresis procedure to the operator (e.g., certain additional substeps of the apheresis procedure, addressing certain "conditions" encountered during the apheresis procedure). Moreover, the work area 688 also displays additional information on the status of the apheresis procedure to the operator. Furthermore, the work area 688 also provides for operator interaction with the computer interface 660, such as by allowing/requiring the operator to input certain information.

[0324] Continuing to refer to FIG. 26, the work area 688 of the master screen 696 displays a load system button 728 and a donor/patient info button 780. The operator may touch either of these buttons 728, 780 (i.e., since the display 696 has "touch screen" capabilities) to generate further screens for providing information to the operator and/or to facilitate the inputting of information to the computer interface 660. The operator may initially touch either the load system button 728 or the donor/patient info button 780 at the start of an apheresis procedure. That is, the order in which the step(s) associated with the load system button 728 are performed in relation to the apheresis step(s) associated with the donor/patient info button 780 are performed is not generally important (i.e., the steps associated with the load system button 728 may be performed before or after the steps associated with the donor/patient info button 780). The apheresis procedure will be described with regard to the operator electing to initially activate the load system button 728 via the touch screen feature.

[0325] However, as described below, it has become more preferable to perform the donor/patient information step(s) before loading the disposable assembly because alternative disposable assemblies are now available (see e.g., the alternative forms of cassette and vessel assemblies in FIGS. 2A, 2B relative to those of FIGS. 2C, 2D). Thus, by performing the donor information step (FIGS. 32-36, below) first, a selection of which cassette and/or vessel assembly (e.g., vessel 325 or 325a of respective FIGS. 2A, 2B or 2C, 2D) might be preferred for a given donor. This option will be described further below.

[0326] Whether before or after donor information has been entered (see description of FIGS. 32-36, below), activation of the load system button 728 generates a loading procedure screen 732 on the computer display 664 which is illustrated in FIG. 27. The loading procedure screen 732 displays multiple pictorials to the operator in the work area 688 which relate to the steps which need to be performed to prepare the blood component separation device 6 for an apheresis procedure. Initially, a hang pictorial 736 is displayed which pictorially conveys to the operator that the various bags (e.g., an AC bag(s) (not shown), plasma collect bag(s) 94 platelet collect bag(s) 84) need to be hung on the blood component separation device 6 and generally how this step may be affected by the operator. The word "HANG" is also positioned above the hang pictorial 736 to provide a short textual instruction to the operator of the required action(s). Consequently, there are two different types of graphical representations provided to the operator relating to a specific operator action which is required to prepare the blood component separation device 6 for the apheresis procedure. Moreover, the hang pictorial 736 is disposed on the left side of the loading procedure screen 732 which indicates that this is the first step or substep associated with the load icon 704. In order to provide further indications of the desired order to the operator, the number "1" is also disposed adjacent to the word "HANG."

[0327] A focus color (e.g., yellow) or shade may be used to direct the operator's attention to specific areas of the machine or screen. The loading procedure screen 732 also displays an insert pictorial 740 to the operator in the work area 688. The insert pictorial 740 pictorially conveys to the operator that the cassette assembly 110 needs to be mounted on the pump/valve/sensor assembly 1000 of the blood

component separation device **6** and generally how this step may be affected by the operator. The word "INSERT" is also positioned above the insert pictorial **740** to provide a short textual instruction to the operator of the required action(s). The insert pictorial **740** is also positioned to the right of the hang pictorial **736** to indicate to the operator that it is preferred, although not required, to perform the step(s) associated with the insert pictorial **740** after the step(s) associated with the hang pictorial **736** have been completed. In order to provide further indications of the desired order to the operator, the number "2" is also disposed adjacent to the word "INSERT."

[0328] The loading procedure screen **732** also displays a load pictorial **744** to the operator in the work area **688**. The load pictorial **744** pictorially conveys to the operator that the blood processing vessel **352** needs to be loaded into the channel **208** of the channel housing **204** on the centrifuge rotor assembly **568** and generally how this step may be affected by the operator. The word "LOAD" is also positioned above the load pictorial **744** to provide a short textual instruction to the operator of the required action(s). The load pictorial **744** is also positioned to the right of the insert pictorial **740** to indicate to the operator that it is preferred, although not required, to perform the step(s) associated with the load pictorial **744** after the step(s) associated with the insert pictorial **740** have been completed. In order to provide further indications of the desired order to the operator, the number "3" is also disposed adjacent to the word "LOAD."

[0329] Finally, the loading procedure screen **732** displays a close pictorial **748**. The close pictorial **748** pictorially conveys to the operator that the door of the blood component collection device housing the centrifuge rotor assembly **568** needs to be closed and generally how this step may be affected by the operator. The word "CLOSE" is also positioned above the close pictorial **748** to provide a short textual instruction to the operator of the required action(s). The close pictorial **748** is also positioned to the right of the load pictorial **744** to indicate to the operator that it is required to perform the step(s) associated with the close pictorial **748** after the step(s) associated with the load pictorial **744** have been completed. In order to provide further indications of the desired order to the operator, the number "4" is also disposed adjacent to the word "CLOSE."

[0330] In summary, the work area **688** of the loading procedure screen **732** not only conveys to the operator what type of steps must be performed for this aspect of the apheresis procedure and generally how to perform these steps, the work area **688** of the loading procedure screen **732** also specifies the order in which these steps should be performed by two "methods." Initially, the pictorial graphics **736**, **740**, **744** and **748** are sequentially displayed in left-to-right fashion to specify the desired/required order of performance. Moreover, the four steps are also numerically identified next to their associated one-word textual description.

[0331] In the event that the operator requires additional guidance with regard to any of the steps presented on the loading procedure screen **732**, the operator may touch the help button **692** provided on the loading procedure screen **732**. This may display a menu of screens which the operator may view and/or may sequentially present a number of help screens associated with the loading procedure screen **732**.

FIG. 28 illustrates a help screen **764** which relates to the loading of the blood processing vessel **352** into the channel **208** on the channel housing **204**. Note that in the case of the help screen **764** the upper portion of the work area **688** of the loading procedure screen **732** is retained (i.e., the one word textual descriptions of the four basic steps and the associated numerical ordering identifier). Moreover, the help screen **764** provides the operator with more detail, in the nature of additional pictorials, regarding one or more aspects of the particular step(s) or substep or in this case on the loading of the blood processing vessel **352** in the channel **208**. Once the operator exits the help screen **764** via touching the continue button **752** on the help screen **764**, the operator is returned to the loading procedure screen **732** of **FIG. 27**. Various other screens in the graphics interface **660** may include a help button **692** to provide this type of feature.

[0332] When the operator has completed each of the four steps or substeps presented on the loading procedure screen **732**, the operator touches the continue button **752** on the bottom of the loading procedure screen **732**. In the event that during the time in which the operator is performing the steps or substeps associated with the loading procedure screen **732** the operator wants to return to the begin operations screen **696**, the operator may touch the display screen **664** in the area of the return button **756**. The return button **756** may be provided on various of the screens to return the operator to the previous screen when acceptable. Moreover, in the event that during the time in which the operator is performing the steps or substeps associated with the loading procedure screen **732** the operator wants to terminate the loading procedure, the operator may touch the display screen **664** in the area of the exit load or cancel button **760**. The exit load or cancel button **760** may be provided on various of the other screens to provide the operator with the option to exit the loading procedure where appropriate.

[0333] When the operator touches the continue button **752** on the loading procedure screen **732**, a disposable pressure test screen **768** is produced on the display **664**, one embodiment of which is illustrated in **FIG. 29**. Generally, the disposable pressure test screen **768** pictorially conveys to the operator that certain steps must be undertaken to allow for pressure testing of the disposable set **8** and how this may be affected by the operator. In this regard, a donor/patient access line clamp pictorial **769** pictorially conveys to the operator that the blood removal/return tubing assembly **20**, specifically the interconnect tubing **38**, to the donor/patient **4** must be sealed off. A donor/patient sample line clamp pictorial **770** pictorially conveys to the operator that the sample line of the sample subassembly **46** must also be sealed off as well. When the operator has completed these steps, the operator touches the continue button **752** and a test in progress screen **772** is displayed to the operator to pictorially and textually convey to the operator that the testing procedure is underway and such is illustrated in **FIG. 30**.

[0334] After the pressure test of the disposable set **8** is complete, an AC interconnect screen **776** is produced on the display **664** and one embodiment of which is illustrated in **FIG. 31**. The AC interconnect screen **776** pictorially conveys to the operator that the anticoagulant tubing assembly **50**, specifically the spike drip member **52**, of the extracorporeal tubing circuit **10** needs to be fluidly interconnected with the AC bag (not shown), as well as generally how this

step may be affected by the operator. When this step has been completed by the operator, the operator touches the continue button **752** on the display **664**.

[0335] The AC interconnect is the last of the steps associated with the load icon **704** such that the operator is returned to the master screen **696**. The master screen **696** now reflects the current status of the apheresis procedure and is illustrated in **FIG. 32**. That is, the color or shade of the load icon **704** is changed from the second color/shade to the third color/shade to that which indicates that all steps associated with the load icon **704** have been completed by the operator. Moreover, a status check **730** appears on the load system button **728** in the work area **688** as well. The load system button **728** is grayed out for the duration of the procedure and thus indicates that the system setup may not be repeated. Consequently, two different types of indications are provided to the operator of the current status regarding the loading procedure. The change in status of the donor/patient data entry portion of the apheresis procedure is also updated by presenting the information icon **708** in the status bar **676** in the second color/shade which indicates to the operator that it is now appropriate to begin this aspect of the apheresis procedure.

[0336] Whether after loading the disposable assembly as just described, or prior thereto, as mentioned above as preferred herein, the operator may then enter donor information to assist in determining which products will be the subject of this donation. The operator enters the information entry portion of the apheresis procedure by touching the info button **780** on the display **664** of the master screen **696**. This produces a donor/patient data screen **788** on the display **664**, one embodiment of which is illustrated in **FIG. 33**. The donor/patient data screen **788** which includes a sex-type button **792**, a height button **796**, and a weight button **808**. The operator may indicate the sex of the donor/patient **4** by touching the relevant portion of the split sex-type button **792** and the selected sex may be displayed to the operator (e.g., via color differentiation). Moreover, the operator may enter the height and weight of the donor/patient **4** by touching the height button **796** and the weight button **808**, respectively. When the height button **796** and weight button **808** are engaged by the operator, a keypad **804** is superimposed over the button whose information is to be entered as illustrated in **FIG. 34**. The keypad **804** may be used to enter the height and weight of the donor/patient **4** and this information may also be displayed to the operator.

[0337] The information entered by the operator on the donor/patient data screen **788** is used to calculate, for instance, the total blood volume of the donor/patient **4** which is presented in a total blood volume display **790** on the donor/patient data screen **788**. The total blood volume of the donor/patient **4** may be utilized in the determination of various parameters associated with the apheresis procedure and/or in the estimation of the number and types of blood components which are anticipated to be collected in the procedure. When the operator has completed these data entry procedures, the operator touches the continue button **752** which will be displayed on the bottom of the donor/patient data screen **788** after all requested information has been input.

[0338] A lab data entry screen **810** may also be generated on the computer display **664** after the steps associated with

the donor/patient data screen **788** have been completed and as indicated by the operator, one embodiment of which is illustrated in **FIG. 35**. The lab data entry screen **810** requests the operator to enter the time for the collection procedure by touching a donation time button **840** which results in the keypad **804** being superimposed over the donation time button **832** (not shown). The donation time entered by the operator will be displayed on a time display **860**, which specifies the duration for the procedure. Moreover, the donation time entered by the operator may also be displayed on the donation time button **840**. The donation time is used, for instance, in the prediction of the number of the blood component(s) (e.g., red blood cells, platelets, and/or plasma) which are anticipated to be collected during the procedure.

[0339] The lab data screen **810** also prompts the operator to enter the hematocrit of the donor/patient **4** by touching a hematocrit button **842**. This results in the keypad **804** being superimposed over the hematocrit button **842**. The operator may then enter the hematocrit of the donor/patient **4** (e.g., as determined via laboratory analysis of a blood sample from the donor/patient **4**) and such may be displayed on the hematocrit button **842**. The hematocrit of the donor/patient **4** is also utilized by one or more aspects of the apheresis procedure.

[0340] The lab data screen **810** also prompts the operator to enter the platelet precount of the donor/patient **4** by touching a platelet precount button **843**. This results in the keypad **804** being superimposed over the platelet precount button **843**. The operator may then enter the platelet precount of the donor/patient **4** (e.g., as determined via laboratory analysis of a blood sample from the donor/patient **4**) and such may be displayed on the platelet precount button **843**. The platelet precount of the donor/patient **4** is also utilized by one or more aspects of the apheresis procedure.

[0341] Once the operator has entered all of the requested information, the operator touches the continue button **752** which then displays a procedure listing (not shown) depicting which donation procedures this donor is qualified to undergo, and hence which blood component product or products this donor may donate. Preferably, such a listing will present preferred donation options (configurable by the blood center), such as blood center preferences and/or prioritizations for particular products (e.g., platelet products first, RBCs second; or vice versa), including whether double products may be favored. Then, if a particular donor is qualified to give certain products (as determined by the machine **6** based upon the donor information entered as just described), then this listing will so indicate with the preferences also presented. Moreover, other procedures may also be listed with information such as whether such procedures may not be qualified for this particular donor no matter the circumstances, or perhaps certain other procedures may be listed with indications that certain further products might be qualified if certain variable information were changeable (e.g., if more time were allowed for a procedure). Thus, such procedures may then indicate to the operator to return to screen **810** and change the variable information (e.g., allot more time) to then qualify that particular procedure. Also alternatively, certain procedures may be indicated as available if a certain amount of replacement fluid would be used with a tubing set according to the embodiment of FIGS. 2C-2D, for example. Thus, a selection of which tubing set to be used will also be alternatively

available at this point in the overall procedure. Then, when all such selections procedure (including priority and/or variable changes, if any) and tubing set, e.g.) are made, the operator can then continue to the next step; preferably loading the chosen tubing set on the machine 6 in the fashion described above (see description relative to FIGS. 26-31).

[0342] Then, a further continue button touch (not shown) may then return the operator to the master screen 696 which now reflects the current status of the apheresis procedure and as illustrated in FIG. 36. Since all of the steps associated with the information icon 708 have now been completed, the color/shade of the information icon 708 is changed from the second color/shade to the third color/shade to convey to the operator that all associated steps have been completed. Moreover, a status check 784 appears on the donor/patient info button 780 in the work area 688 as well. Consequently, two different types of indications are provided to the operator of the current status of this aspect of the apheresis procedure. Moreover, the change in status of the collection icon set 712 of the apheresis procedure is updated by changing the color/shade of the donor/patient prep icon 716 in the status bar 676 from the first color/shade to the second color/shade. A run button 802 is also now presented on the master screen 696 such that the steps associated with the collection icon set 712 may now be undertaken and further such that pictorial representations of the same may be provided to the operator.

[0343] The initial screen for steps associated with the collection icon set 712 is a donor/patient prep screen 812A which is illustrated in FIG. 37. The donor/patient prep screen 812A pictorially conveys to the operator the steps which must be undertaken in relation to the donor/patient 4 being fluidly interconnected with the blood component separation device. Initially, a donor/patient connect pictorial 816 is displayed which pictorially conveys to the operator that an access needle 32 must be installed on the donor/patient 4, as well as generally how this step may be affected by the operator. The word "CONNECT" is also positioned above the donor/patient connect pictorial 816 to provide a short textual instruction to the operator of the required action(s). The donor/patient connect pictorial 816 is disposed on the left side of the donor/patient prep screen 812A which indicates that this is the first step or substep associated with the donor/patient prep icon 716. In order to provide further indications of the desired order to the operator, the number "1" is also disposed adjacent the word "CONNECT."

[0344] The donor/patient prep screen 812A also displays an open pictorial 820 on the display 664. The open pictorial 820 pictorially conveys to the operator that the clamps 42 in the interconnect tubing 38 and the clamp in the tubing of the sample subassembly 46 must be removed, as well as generally how these steps may be affected by the operator. The word "OPEN" is also positioned above the open flow pictorial 820 to provide a short textual instruction to the operator of the required action(s). The open pictorial 820 is disposed to the right of the donor/patient connect pictorial 816 which indicates that the step(s) associated with the open pictorial 820 should be performed only after the step(s) associated with the donor/patient connect pictorial 816 have been completed. In order to provide further indications of the desired order to the operator, the number "2" is also disposed adjacent the word "OPEN."

[0345] The donor/patient prep screen 812A also displays a flow pictorial 824 on the display 664. The flow pictorial 824 pictorially conveys to the operator that there should now be a flow of blood from the donor/patient 4 into the blood removal/return tubing assembly 20, specifically the blood removal tubing 22, and in the sample tubing of the sample subassembly 46. The word "FLOW" is also positioned above the flow pictorial 824 to provide a short textual description to the operator of what should be occurring at this time. The flow pictorial 824 is disposed to the right of the open pictorial 820 which indicates that the conditions associated with the flow pictorial 824 should occur only after the step(s) associated with the open pictorial 820 have been completed. In order to provide further indications of the desired order to the operator, the number "3" is also disposed adjacent the word "FLOW."

[0346] In summary, the work area 688 of the donor/patient prep screen 812A not only conveys to the operator what type of steps must be performed for this aspect of the apheresis procedure and how to generally perform these steps, but also specifies the order in which these steps should be performed by two methods. Initially, the pictorial graphics 816, 820, and 824 are sequentially displayed in left-to-right fashion. Moreover, the three steps are also numerically identified next to their associated one-word textual description.

[0347] Once the operator completes all of the steps associated with the donor/patient prep screen 812A, the operator touches the continue button 752 which results in the display of a second donor/patient prep screen 812B as illustrated in FIG. 38. The donor/patient prep screen 812B includes a close pictorial 828 which pictorially conveys to the operator to terminate the flow of blood from the donor/patient 4 to the sample bag of the sample subassembly 46 by clamping the sample line and generally how this step may be affected by the operator. The word "CLOSE" is also positioned above the close pictorial 828 to provide a short textual instruction to the operator of the required action(s). The close pictorial 828 is disposed on the left side of the donor/patient prep screen 812B which indicates that this is the first step or substep associated with the donor/patient prep screen 812B. In order to provide an indication that this is in fact, however, the fourth step associated with the donor/patient preps, the number "4" is also disposed adjacent the word "CLOSE."

[0348] The donor/patient prep screen 812B also displays a seal pictorial 832 on the display 664. The seal flow pictorial 832 pictorially conveys to the operator that the sample line of the sample subassembly 46 should now be sealed off and generally how this step may be affected by the operator. The word "SEAL" is also positioned above the seal pictorial 832 to provide a short textual instruction to the operator of the required action(s). The seal pictorial 832 is disposed to the right of the close pictorial 828 which indicates that the step(s) associated with the seal pictorial 832 should be performed only after the step(s) associated with the close pictorial 828 have been completed. In order to provide further indications of the desired order to the operator, the number "5" is also disposed adjacent the word "SEAL" to indicate that this is actually the fifth step associated with the donor/patient preps.

[0349] In summary, the work area 688 of the donor/patient prep screen 812B not only conveys to the operator what type of steps must be performed for this aspect of the apheresis

procedure and how to generally perform these steps, the work area **688** of the donor/patient prep screen **812B** also specifies the order in which these steps should be performed by two methods. Initially, the pictorials **828**, **832**, and **836** are sequentially displayed in left-to-right fashion. Moreover, the four steps are also numerically identified next to their associated one-word textual description.

[**0350**] Once the operator completes all of the donor/patient preps, the operator may touch the start prime button **846** on the donor/patient prep screen **812B** which initiates the above-described blood prime of the extracorporeal tubing circuit **10** and blood processing vessel **352** and which results in the display of the run screen **844** illustrated in **FIG. 39**. The run screen **844** primarily displays information to the operator regarding the apheresis procedure. For instance, the run screen **844** includes a blood pressure display **848** (i.e., to convey to the operator the donor/patient's extracorporeal blood pressure), a platelet collect display **852** (i.e., to convey to the operator an estimate of the number of platelets which have been currently collected), a plasma collect display **856** (i.e., to convey to the operator the amount of plasma which has been currently collected), and a time display **860** (e.g., both the amount of time which has lapsed since the start of the collection procedure (the left bar graph and noted time), as well as the amount of time remaining in the collection procedure (the right bar graph and noted time). A control button (not shown) may be provided to toggle between the time remaining display and the start and stop time display.

[**0351**] The run screen **844** may also display, in the case of a single needle procedure (i.e., where only one needle is utilized to fluidly interconnect the donor/patient **4** with the blood component separation device **6**), whether blood is being withdrawn from the donor/patient **4** (e.g., by displaying "draw in progress") or is being returned to the donor/patient **4** (e.g., by displaying "return in progress"). This information may be useful to the donor/patient **4** in that if the donor/patient **4** is attempting to maintain a certain blood pressure by squeezing an article to assist in removal of blood from the donor/patient **4**, the donor/patient **4** will be provided with an indication to suspend these actions while blood is being returned to the donor/patient **4**.

[**0352**] During the apheresis procedure, certain conditions may be detected by the apheresis system **2** which would benefit from an investigation by the operator. If one of these types of conditions is detected, an appropriate alarm screen is displayed to the operator. One embodiment of an alarm screen **864** is illustrated in **FIG. 40**. Initially, the alarm screen **864** textually conveys a potential problem with the system **2** via a problem graphic **868**. The text may be useful in ensuring that the operator understands the problem. The alarm screen **864** also includes an action pictorial **872** which graphically conveys to the operator the action which should be taken in relation to the problem. These are actions which may be difficult or impossible for the system **2** to take itself. Finally, the alarm screen includes an inspection results array **876** which allows the operator to indicate the results of the inspection. In the illustrated embodiment, the array **876** includes a blood leak button **906**, a moisture button **908**, and a no leak button **910**.

[**0353**] Depending upon the selection made by the operator on the inspection results array **876**, additional questions may be posed to the operator in further screens which require

further investigation and/or which specify the desired remedial action. For instance, the supplemental alarm screen **878** of **FIG. 41** may be generated by the operator touching the moisture button **908** on the alarm screen **864**. The supplemental alarm screen **878** includes a remedial action pictorial **912** and remedial action text **914** to convey to the operator how to correct the identified problem.

[**0354**] The computer interface **660** may also allow the operator to initiate some type of corrective action based upon observations made by and/or conveyed to the operator. For instance, various screens of the interface **660** may include a trouble shooting button **898** which will generate one or more trouble shooting screens. These trouble shooting screens may include menus or the like to allow the operator to indicate what type of potential problem exists.

[**0355**] One embodiment of a trouble shooting screen **880** is presented in **FIG. 42**. The trouble shooting screen **880** includes a donor/patient tingling button **922**. This button **922** would be utilized by the operator to attempt to remedy the effects of AC on the donor/patient **4** in response to the donor/patient indicating a "tingling sensation" or, alternatively, "AC reaction." When the operator hits the "down arrow" of the donor/patient tingling button **922**, the system **2** attempts to correct the condition in a predetermined manner (i.e., a predetermined protocol is employed preferably this protocol does not require operator actions or decisions). Once the tingling sensation no longer exists, the operator may use the "up arrow" button to return the bar on the donor/patient tingling button **922** to its original position.

[**0356**] The trouble shooting screen **880** also includes a clumping button **924**. This button **924** would be utilized by the operator if any undesired clumping of the collected product (e.g., platelets) was observed. When the operator hits the "down arrow" of the clumping button **924**, the system **2** attempts to correct the condition in a predetermined manner (i.e., a predetermined protocol is employed and preferably this protocol does not require operator actions or decisions). Once the clumping is no longer observed by the operator, the operator may use the "up arrow" button to return the bar on the clumping button **924** to its original position.

[**0357**] The trouble shooting screen **880** may also include a spillover button **916** and an "air in plasma line" button **918**. The spillover button **916** would be engaged by the operator if red blood cells were observed in the platelet outlet tubing **66**, in the platelet collect bag **84**, and/or flowing beyond the RBC dam **232**. Activation of the spillover button **916** via the touch screen capabilities would result in the system **2** using a predetermined and preferably automatic protocol is performed by the system **2** to correct this condition. Similarly, if the operator observes air in the plasma line **918** and engages the button **918**, the system **2** again will preferably automatically employ a predetermined protocol to correct this condition.

[**0358**] The "other problem button" **920** may be utilized to generate further trouble shooting screens to list further problems which may occur in the apheresis procedure. Again, preferably upon the operator touching the associated button indicative of a particular problem, a predetermined protocol will be preferably automatically employed to attempt to correct the same.

[**0359**] Upon completion of the collection portion of the apheresis procedure, the rinseback screen **884** is produced

on the display 664 which indicates that the rinseback procedure will now be performed and which is illustrated in FIG. 44. Once the rinseback is completed, the color/shade of the donate icon 720 changes from the second color to the third color/shade to indicate that all steps associated with this aspect of the apheresis procedure have been completed. Moreover, the color/shade of the unload icon 724 will also change from the first color/shade to the second color/shade to indicate to the operator that the step(s) associated therewith may now be performed.

[0360] Upon completion of the rinseback, a run finish screen may be produced on the display 664 to provide the final collection data as illustrated in FIG. 43 (e.g., the associated yields of platelets and plasma collected during the procedure) as well as the fact that the procedure is over (e.g., by displaying "run completed"). The operator may then touch the continue button 752.

[0361] Once the rinseback procedure is completed, an unload screen 892 will be presented on the display 664 and is illustrated in FIG. 45. The unload screen 892 may sequentially display a number of pictorials to the operator to convey the steps which should be completed to terminate the procedure. For instance, a seal/detach pictorial 900 may be initially displayed on the unload screen 892 to pictorially convey to the operator that the tubes leading to the platelet, plasma and/or RBC collect bag(s) 84, 94 and 954 should each be sealed such that the platelet, plasma and/or RBC collect bag(s) 84, 94 and 954, respectively, may be removed. Once the operator touches the continue button 752, a disconnect pictorial 902 may be presented on the unload screen 892 to pictorially convey to the operator that the access needle 32 should be removed from the donor/patient 4. Once the operator touches the continue button 752, a remove pictorial 904 is presented on the unload screen 892 to pictorially convey to the operator that the disposable set 8 should be removed from the blood component separation device 6 and disposed of properly.

[0362] The computer interface 660 provides a number of advantages. For instance, the computer interface 660 utilizes a three-way color/shade differentiation to conveniently convey the status of the apheresis procedure to the operator. An icon is presented in one color/shade if the step(s) associated with the icon are not yet ready to be performed, while the icon is presented in another color/shade if the step(s) associated with the icon are ready to be performed or are being performed, while the icon is presented in yet another color/shade if the step(s) associated with the icon have been completed. Moreover, the computer interface 660 provides pictorials to the operator of at least certain of the steps of the apheresis procedure. Furthermore, the desired/required ordering of at least the fundamental steps of the apheresis procedure is conveyed to the operator. Finally, the interface 660 allows for correction of certain conditions, which after appropriate operator input, are remedied by the system 2 in accordance with a predetermined protocol.

[0363] The foregoing description of the present invention has been presented for purposes of illustration and description. Furthermore, the description is not intended to limit the invention to the form disclosed herein. Consequently, variations and modifications commensurate with the above teachings, and skill and knowledge of the relevant art, are within the scope of the present invention. The embodiments

described hereinabove are further intended to explain best modes known of practicing the invention and to enable others skilled in the art to utilize the invention in such, or other embodiments and with various modifications required by the particular application(s) or use(s) of the present invention. It is intended that the appended claims be construed to include alternative embodiments to the extent permitted by the prior art.

What is claimed is:

1. A method for extracorporeal separation and collection of blood components from a donor/patient, comprising:

flowing blood into a centrifugal dual stage blood processing vessel, said processing vessel including a first stage and a second stage, the second stage being separated from said first stage by a dam, a blood inlet for communicating blood into the first stage, a plasma outlet disposed in the second stage and a red blood cell outlet disposed in the first stage;

centrifugally separating the blood into separated blood components including;

separating plasma from said blood within said centrifugal dual stage blood processing vessel to establish separated plasma, whereby a portion of the separated plasma flows over the dam in the processing vessel to the plasma outlet in the second stage of the processing vessel;

separating red blood cells from said blood within said centrifugal dual stage blood processing vessel to establish separated red blood cells whereby the separated red blood cells remain in the first stage of the processing vessel and flow to the red blood cell outlet;

collecting at least a portion of at least one separated blood component including;

collecting as a double red blood cell product at least a portion of said separated red blood cells in a red blood cell collection reservoir separate from said blood processing vessel to establish collected red blood cells.

2. A method according to claim 1 in which said collecting step further includes a step for collecting at least a portion of the separated plasma in a plasma collection reservoir separate from said blood processing vessel to establish collected plasma; and wherein said plasma collection step is performed at least partially contemporaneously with said red blood cell collection step.

3. A method as recited in claim 2, wherein said plasma collection step is performed prior to said red blood cell collection step.

4. A method as recited in claim 2, wherein said plasma collection step is performed at least partially after said red blood cell collection step.

5. A method as recited in claim 2, wherein said red blood cell collection step is performed at least partially after said plasma collection step.

6. A method according to claim 2 which farther includes establishing a packing factor of at least about 13 for the separated red blood cells within said blood processing vessel.

7. A method according to claim 6 in which the packing factor is about 16.

8. A method according to claim 6 which further includes establishing an AC ratio in the blood processing vessel of between about 6 and about 16.

9. A method according to claim 5 in which the packing factor is about 16 during the contemporaneous collection of separated plasma and separated red blood cells and the packing factor is then reduced to about 13 during the at least partial step of collecting separated red blood cells after the performance of the collection of separated plasma.

10. A method according to claim 1 which further comprises the step of delivering a replacement fluid to the donor/patient.

11. A method according to claim 10 in which said step of delivering a replacement fluid includes flowing replacement fluid at a rate equal to the total flow rate of collected blood components multiplied by the desired fluid balance percentage resulting within the donor/patient.

12. A method according to claim 10 which further includes a step of adding anticoagulant to the blood flowing into the centrifugal dual stage blood processing vessel; and in which said step of delivering a replacement fluid includes flowing replacement fluid at a rate equal to the total flow rate of collected blood components minus the flow rate of anticoagulant multiplied by the desired fluid balance percentage resulting in the donor/patient.

13. A method according to claim 10 in which a replacement fluid is flowed from a source first to an intermediate reservoir prior to ultimate delivery to the donor/patient.

14. A method according to claim 10 in which a replacement fluid is delivered to the donor/patient in a substantially continuous fashion.

15. A method according to claim 10 in which a replacement fluid is delivered to the donor/patient in a bolus.

16. A method according to claim 1 in which said double volume of collected red blood cells totals substantially about 400 milliliters contained in two substantially separate reservoirs.

17. A method as recited in claim 1, further comprising a set-up step prior to said collecting step, said set-up step including:

flowing the separated blood components out of said blood processing vessel, wherein substantially all of said separated blood components flowing out of the blood processing vessel are accumulated for re-infusion to a donor/patient during the set-up step.

18. A method as recited in claim 1, further comprising:

removing said blood from a donor/patient through a single needle;

returning uncollected separated blood components of said blood to said donor/patient through said single needle.

19. A method as recited in claim 18, wherein said removing and returning steps are alternately and repeatedly performed.

20. A method as recited in claim 18, wherein during said plasma collection step, said method further comprises:

recirculating a portion of the uncollected separated blood components into said blood processing vessel; and,

wherein during said red blood cell collection step, said method includes:

returning substantially all of the uncollected separated blood components to said donor/patient.

21. A method as recited in claim 17, wherein said blood is flowed into said blood processing vessel at an inlet flow rate, and said set-up step comprises:

reducing said inlet flow rate.

22. A method as recited in claim 17, wherein said blood processing vessel is rotated at an rpm rate, and wherein said set-up step comprises:

increasing said rpm rate.

23. A method as recited in claim 17, said set-up step including:

maintaining a predetermined anticoagulant infusion rate to said donor/patient.

24. A method as recited in claim 17, said set-up step including:

removing the separated red blood cells and a portion of the separated plasma together through the RBC outlet from said blood processing vessel to establish the interface between the separated RBCs and the separated plasma at the RBC outlet in the first stage of the blood processing vessel.

25. A method as recited in claim 1, further comprising:

adding a storage solution to said separated red blood cells collected in said red blood cell collection reservoir.

26. A method as recited in claim 25, wherein said storage solution is added through an assembly having a sterile barrier filter.

27. A method as recited in claim 1, further comprising:

leukoreduction filtering of said separated red blood cells collected in said red blood cell collection reservoir.

28. A method for extracorporeal collection of blood components from a donor/patient comprising:

removing blood from a donor/patient through a single needle;

flowing said blood into a dual stage blood processing vessel;

separating plasma from said blood within said blood processing vessel;

collecting at least a portion of said plasma in a plasma collection reservoir separate from said blood processing vessel;

separating red blood cells from said blood within said dual stage blood processing vessel;

collecting at least a portion of said separated red blood cells in a red blood cell collection reservoir separate from said blood processing vessel, wherein said plasma separation and collection steps are completed at least partially contemporaneously with said red blood cell separation and collection steps;

returning uncollected blood components of said blood to said donor/patient through said single needle; and

replacing fluid volume in said donor/patient by flowing a replacement fluid to said donor/patient through said single needle.

29. A method as recited in claim 28, whereby the red blood cell collecting step provides for obtaining a double volume of collected red blood cells.

30. A method as recited in claim 28, wherein said plasma collection step is completed at least partially separately from said red blood cell collection step.

31. A method as recited in claim 28, wherein prior to said red blood cell collection step, and separate from said plasma collection step, said method further comprises a red blood cell collection set-up phase including:

establishing a hematocrit of at least about 80 within said separated red blood cells within said blood processing vessel and an AC ratio within said blood at about 8.

32. A method as recited in claim 31, further comprising maintaining said hematocrit and AC ratio during said red blood cell separation and collection steps.

33. A method according to claim 28 in which said step of delivering a replacement fluid includes flowing replacement fluid at a rate equal to the total flow rate of collected blood components multiplied by the desired fluid balance percentage resulting within the donor/patient.

34. A method according to claim 33 in which said step of delivering a replacement fluid includes pumping replacement fluid at a rate equal to the total flow rate of collected fluids minus the inlet flow rate of anticoagulant multiplied by the desired fluid balance percentage resulting within the donor/patient.

35. A method according to claim 33 in which a replacement fluid is pumped from a source first to an intermediate reservoir prior to ultimate delivery to the donor/patient.

36. A method according to claim 33 in which a replacement fluid is delivered to the donor/patient in a bolus.

37. A method according to claim 33 in which a replacement fluid is delivered to the donor/patient in a substantially continuous fashion.

38. A device for extracorporeal separation and collection of blood components from a donor/patient, comprising:

a centrifugal blood processing channel into which blood from a donor/patient is adapted to be flowed, and in which said blood is separated into at least separated plasma and separated red blood cells; said centrifugal dual stage blood processing channel including a first stage and a second stage, the second stage being separated from said first stage by a dam, a blood inlet for communicating blood into the first stage, a plasma outlet disposed in the second stage and a red blood cell outlet disposed in the first stage; said centrifugal blood processing channel being adapted to be used with:

a removable plasma collection reservoir operably connected to said centrifugal blood processing channel, whereby into which at least a portion of said separated plasma is collected;

a removable red blood cell collection reservoir operably connected to said blood processing channel whereby a portion of said separated red blood cells are collected in said red blood cell collection reservoir; and

a replacement fluid assembly which is operably connectable to the donor/patient;

wherein said replacement fluid assembly is adapted to deliver replacement fluid to the donor/patient.

39. A disposable blood tubing set adapted to be used with a device for extracorporeal separation and collection of blood components from a donor/patient, said disposable blood tubing set comprising:

a disposable centrifugal dual stage blood processing vessel into which blood from a donor/patient is adapted to be flowed, and in which said blood is separated into at least separated plasma and separated red blood cells; said centrifugal dual stage blood processing vessel including a first stage and a second stage, the second stage being separated from said first stage by a dam, a blood inlet for communicating blood into the first stage, a plasma outlet disposed in the second stage and a red blood cell outlet disposed in the first stage;

a plasma collection reservoir operably connected to said centrifugal blood processing vessel, whereby into which said plasma collection reservoir at least a portion of said separated plasma is collected;

a red blood cell collection reservoir operably connected to said blood processing vessel whereby a portion of said separated red blood cells are collected in said red blood cell collection reservoir; and

a disposable fluid flow cassette assembly operably interconnected to said centrifugal blood processing vessel, said cassette assembly having an intermediate reservoir disposed therein, said intermediate reservoir being adapted to receive separated uncollected blood components from said centrifugal blood processing vessel; and

a replacement fluid assembly which is operably connected to said fluid flow cassette and said intermediate reservoir; wherein said replacement fluid assembly is adapted to deliver replacement fluid to said intermediate reservoir for subsequent infusion of the replacement fluid into a donor/patient.

40. A method for extracorporeal collection of a blood component from a donor/patient, comprising:

using a donor/patient characteristic to determine a blood component to be collected;

generating a list having at least one blood component collection option;

using the list in selecting a blood component to be collected;

removing blood from a donor/patient;

flowing the blood into a centrifugal blood processing vessel;

separating the blood into separated blood components within said centrifugal blood processing vessel, said separated blood components including at least separated plasma and separated red blood cells;

collecting at least a portion of at least one of said blood components from said centrifugal blood processing vessel in a blood component collection reservoir separate from said centrifugal blood processing vessel;

returning at least a portion of the uncollected separated blood components from said blood processing vessel to said donor/patient.

41. A method for extracorporeal collection of a blood component from a donor/patient according to claim 40 in which said method uses an extracorporeal blood processing system having an extracorporeal blood processing machine and a plurality of tubing and bag set options available for use

with said machine, said method further comprising loading an appropriate tubing and bag set on said machine.

42. A method as recited in claim 40, wherein said method uses an extracorporeal blood processing system having an extracorporeal blood processing machine, whereby said machine generates said list of at least one component collection option.

43. A method according to claim 42 wherein said donor/patient characteristic is input into said machine, and said machine uses said donor/patient characteristic to generate said list.

44. A method according to claim 42 wherein said donor/patient characteristic includes the height and weight of the donor/patient.

45. A method according to claim 42 wherein said donor/patient characteristic includes the hematocrit of the donor/patient.

46. A method according to claim 42 wherein said donor/patient characteristic includes the platelet count of the donor/patient.

47. A method according to claim 40 wherein said list of blood component options includes at least one option selected from the group consisting essentially of platelets, red blood cells, and plasma.

48. A method according to claim 40 wherein said list of blood component options includes at least one option selected from the group consisting essentially of single platelets, double platelets, triple platelets, red blood cells, double red blood cells, and plasma.

49. A method according to claim 40 wherein said list of blood component options includes at least two options as a combination of collectible products selected from the group consisting essentially of single platelets, double platelets, triple platelets, red blood cells, double red blood cells, and plasma.

50. A system for extracorporeal collection of a blood component from a donor/patient, comprising:

an extracorporeal blood processing machine, said machine being adapted to use a donor/patient characteristic to determine a blood component to be collected and to generate a list having at least one blood component collection option;

said machine being adapted to receive an input selection of a blood component to be collected;

said machine being adapted to receive blood removed from a donor/patient;

said machine having a centrifugal blood processing vessel to receive the blood and separate the blood into separated blood components within said centrifugal blood processing vessel, said separated blood components including at least separated plasma and separated red blood cells;

said machine being adapted to collect at least a portion of at least one of said blood components from said centrifugal blood processing vessel in a blood component collection reservoir separate from said centrifugal blood processing vessel;

said machine being adapted to return at least a portion of the uncollected separated blood components from said blood processing vessel to said donor/patient.

51. A system for extracorporeal collection of a blood component from a donor/patient according to claim 50 in which said extracorporeal blood processing machine is adapted to use a plurality of tubing and bag set options.

52. A system as recited in claim 50, whereby said machine generates said list of at least one component collection option.

53. A system according to claim 52 wherein said donor/patient characteristic is input into said machine, and said machine uses said donor/patient characteristic to generate said list.

54. A system according to claim 52 wherein said donor/patient characteristic includes the height and weight of the donor/patient.

55. A system according to claim 52 wherein said donor/patient characteristic includes the hematocrit of the donor/patient.

56. A system according to claim 52 wherein said donor/patient characteristic includes the platelet count of the donor/patient.

57. A system according to claim 50 wherein said list of blood component options includes at least one option selected from the group consisting essentially of platelets, red blood cells, and plasma.

58. A system according to claim 50 wherein said list of blood component options includes at least one option selected from the group consisting essentially of single platelets, double platelets, triple platelets, red blood cells, double red blood cells, and plasma.

59. A system according to claim 50 wherein said list of blood component options includes at least two options as a combination of collectible products selected from the group consisting essentially of single platelets, double platelets, triple platelets, red blood cells, double red blood cells, and plasma.

60. A system as recited in claim 50, wherein said machine is adapted to deliver a replacement fluid to said donor/patient.

61. A method as recited in claim 60 wherein said machine is adapted to deliver said replacement fluid to said donor/patient in a substantially continuous fashion.

* * * * *