8638249

THE UNITED STATES OF AMERICA

TO ALL TO WHOM THESE PRESENTS SHALL COME:

UNITED STATES DEPARTMENT OF COMMERCE

United States Patent and Trademark Office

September 23, 2025

THIS IS TO CERTIFY THAT ANNEXED IS A TRUE COPY FROM THE RECORDS OF THIS OFFICE OF THE FILE WRAPPER AND CONTENTS OF:

APPLICATION NUMBER: ***15/994,559***
FILING DATE: ***May 31, 2018***
PATENT NUMBER: ***10143412***
ISSUE DATE: ***December 04, 2018***

Certified by

DIRECTOR OF THE UNITED STATES PATENT AND TRADEMARK OFFICE

PTO/AIA/15 (10-17)
Approved for use through 11/30/2020. OMB 0651-0032
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995 no persons are required to respond to a collection of information unless it displays a valid OMB control number.

UTILITY PATENT APPLICATION TRANSMITTAL

(Only for new nonprovisional applications under 37 CFR 1.53(b))

Attorney Docket No.	251102.000027.KURIN2CON2
First Named Inventor	Bobby E. ROGERS
Title	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD
Priority Mail Express® Label No.	

APPLICATION ELEMENTS

See MPEP chapter 600 concerning utility patent application contents.

1. [✔] **Fee Transmittal Form** (PTO/SB/17 or equivalent)
2. [ ] **Applicant asserts small entity status.** See 37 CFR 1.27
3. [ ] **Applicant certifies micro entity status.** See 37 CFR 1.29. Applicant must attach form PTO/SB/15A or B or equivalent.
4. [✔] **Specification** [*Total Pages* 39] Both the claims and abstract must start on a new page. *(See MPEP § 608.01(a) for information on the preferred arrangement)*
5. [✔] **Drawing(s)** (35 U.S.C. 113) [*Total Sheets* 50]
6. **Inventor's Oath or Declaration** [*Total Pages* 3] *(including substitute statements under 37 CFR 1.64 and assignments serving as an oath or declaration under 37 CFR 1.63(e))*
   a. [ ] Newly executed (original or copy)
   b. [✔] A copy from a prior application (37 CFR 1.63(d))
7. [✔] **Application Data Sheet** ** See note below.* See 37 CFR 1.76 (PTO/AIA/14 or equivalent)
8. **CD-ROM or CD-R** in duplicate, large table, or Computer Program (*Appendix*)
   [ ] Landscape Table on CD
9. **Nucleotide and/or Amino Acid Sequence Submission** (*if applicable, items a. – c. are required*)
   a. [ ] Computer Readable Form (CRF)
   b. [ ] Specification Sequence Listing on:
      i. [ ] CD-ROM or CD-R (2 copies); or
      ii. [ ] Paper
   c. [ ] Statements verifying identity of above copies

ADDRESS TO:

Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

ACCOMPANYING APPLICATION PAPERS

10. [ ] **Assignment Papers** (cover sheet & document(s))
    Name of Assignee _____
11. [ ] **37 CFR 3.73(c) Statement** (*when there is an assignee*) [✔] **Power of Attorney**
12. [ ] **English Translation Document** (*if applicable*)
13. [✔] **Information Disclosure Statement** (PTO/SB/08 or PTO-1449)
    [ ] Copies of citations attached
14. [ ] **Preliminary Amendment**
15. [ ] **Return Receipt Postcard** (*MPEP § 503*) (*Should be specifically itemized*)
16. [ ] **Certified Copy of Priority Document(s)** (*if foreign priority is claimed*)
17. [ ] **Nonpublication Request** Under 35 U.S.C. 122(b)(2)(B)(i). Applicant must attach form PTO/SB/35 or equivalent.
18. [✔] **Other:** Certification and Request for Prioritized Examination

Note*: (1) Benefit claims under 37 CFR 1.78 and foreign priority claims under 1.55 **must be included in an Application Data Sheet (ADS).
(2) For applications filed under 35 U.S.C. 111, the application must contain an ADS specifying the applicant if the applicant is an assignee, person to whom the inventor is under an obligation to assign, or person who otherwise shows sufficient proprietary interest in the matter. See 37 CFR 1.46(b).

19. CORRESPONDENCE ADDRESS

[✔] The address associated with Customer Number: 153290 **OR** [ ] Correspondence address below

Name					
Address					
City		State		Zip Code	
Country		Telephone		Email	

Signature	/David Devernoe/	Date	May 31, 2018
Name (Print/Type)	David Devernoe	Registration No. (Attorney/Agent)	50,128

This collection of information is required by 37 CFR 1.53(b). The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.11 and 1.14. This collection is estimated to take 12 minutes to complete, including gathering, preparing, and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. **SEND TO: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.**

If you need assistance in completing the form, call 1-800-PTO-9199 and select option 2.

BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a Continuation of U.S. Application No. 15/140,448, filed on April 27, 2016, which claims the benefit of U.S. Provisional Application Serial No. 62/196,797, filed on July 24, 2015 and titled "BLOOD CULTURE IMPROVEMENT SYSTEM AND METHOD"; U.S. Provisional Application Serial No. 62/238,636, filed on October 7, 2015 and titled "BLOOD SEQUESTRATION SYSTEM FOR NON-CONTAMINATED BLOOD SAMPLING"; and U.S. Provisional Application Serial No. 62/318,194, filed on April 4, 2016 and titled "BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD," the disclosures of which are incorporated by reference in their entirety.

BACKGROUND

[0002] Bacteraemia is the presence of microorganisms in the blood. Sepsis, on the other hand, is bacteraemia in the presence of clinical symptoms and signs such as fever, tachycardia, tachypnea and hypotension. Bacteraemia and sepsis are associated with a high mortality and an increased incidence and duration of hospital stay and associated costs. Many bacteraemias, sepsis, fungaemias and other pathogens actually occur within a hospital or other healthcare settings with catheters and venipunctures being a source of contamination as potential carriers of these pathogens.

[0003] Blood cultures are the standard test used to detect microbial pathogens related to bacteraemia and sepsis in a patient's blood. The term blood culture refers to a single venipuncture, either from a peripheral site or central or arterial line, with the blood inoculated into one or more blood culture bottles or containers. One bottle is considered a blood culture where two or more are considered a set. Multiple sets may be obtained from multiple venipunctures and are associated with different sites on the patient.

[0004] These methods allow for microbial identification and susceptibility testing to be performed, which is a critical component to managing sepsis, however the lack of rapid results and decreased sensitivity for fastidious pathogens has led to the development of improved systems and adjunctive molecular or proteomic testing.

[0005] Collection of blood samples for conducting blood cultures is a critical component of modern patient care and can either positively affect the patient outcome by providing an accurate diagnosis, or can adversely affect the outcome by prolonging unnecessary antimicrobial therapy, the length of hospital stays, and increasing costs.

[0006] One outcome of collection of blood cultures is contamination. Blood culture contamination can lead to a false positive culture result and/or significant increase in healthcare related costs. Sources of blood culture contamination include improper skin antisepsis, improper collection tube disinfection, and contamination of the initial blood draw which may then skew results.

[0007] Blood culture collection kits generally consist of a "butterfly" set, infusion set, or other type of venipuncture device as offered by companies like BD, Smiths, B. Braun and others, and aerobic and anaerobic blood culture bottles. Various different bottles are also available depending on the test requirements. These bottles are specifically designed to optimize recovery of both aerobic and anaerobic organisms. In conventional kits, a bottle used is known generally as a "Vacutainer," which is a blood collection tube formed of a sterile glass or plastic tube with a closure that is evacuated to create a vacuum inside the tube to facilitate the draw of a predetermined volume of liquid such as blood.

[0008] False positive blood cultures are typically a result of poor sampling techniques. They cause the use of antibiotics when not needed, increasing hospital costs and patient anxiety. Blood cultures are drawn from a needlestick into the skin, and then a Vacutainer is attached to capture a sample of blood. Contamination may occur from improper or incomplete disinfection of the skin area in and around the puncture site. It may also occur from the coring of the skin by the needle during insertion, with the cored skin cells and any associated contamination being pulled into the sample.

[0009] Blood flow through a hypodermic needle is laminar, and as such, a velocity gradient can be developed over the flow tube as a pressure drop is applied to the hypodermic needle. Either forceful aspiration of blood, or using a very small hypodermic needle, can cause lysis and a release of potassium from the red blood cells, thereby rendering the blood samples abnormal.

[0010] In other instances, some patients have delicate veins that can collapse under a pressure drop or vacuum, particularly as applied by a syringe's plunger that is drawn too quickly for the patient's condition. Since such condition is impossible to know beforehand, such vein collapses are a risk and very difficult to control.

[0011] Various strategies have been implemented to decrease blood culture contamination rates, e.g. training staff with regard to aseptic collection technique, feedback with regard to contamination rates and implementation of blood culture collection kits. Although skin antisepsis can reduce the burden of contamination, 20% or more of skin organisms are located deep within the dermis and are unaffected by antisepsis. Changing needles before bottle inoculation is not advisable as it increases the risk to acquire needle stick injuries without decreasing contamination rates.

[0012] Some conventional systems and techniques for reducing blood culture contamination include discarding the initial aliquot of blood taken from central venous catheters, venipunctures, and other vascular access systems. However, these systems require the user to mechanically manipulate an intravascular device, or require a complex series of steps that are difficult to ensure being followed.

SUMMARY

[0013] This document presents systems and methods for reducing blood culture contamination, lysing of cells, and vein collapse. In some implementations, a system and method can eliminate user variability in disinfection, and also eliminate the risk of skin cells getting into the blood culture sample. The systems and methods disclosed herein do not require a change in existing clinical processes, other than to potentially indicate when a vacutainer or other blood collection device (i.e., syringe) should be attached for drawing contaminant-free blood samples.

[0014] In some implementations of the systems and methods disclosed herein the withdrawal of blood is accomplished passively by use of the patient's own blood pressure, thereby reducing the risk of vein collapse and eliminating any additional user steps over current practice. The systems and methods can be applied to accommodate short-path direct stick or butterfly venipuncture systems. They can also be used with samples drawn through a catheter.

[0015] In one aspect, a blood sequestration device is presented. The blood sequestration device includes an inlet port and an outlet port. The blood sequestration device further includes a sequestration chamber connected with the inlet port, the sequestration chamber having a vent comprising an air permeable blood barrier. The blood sequestration device further includes a sampling channel having a proximal end connected with the inlet port and a distal end connected with the outlet port.

[0016] In another aspect, a blood sequestration device connected with a blood sampling pathway is described. The blood sampling pathway has a patient needle and a sample collection device. The blood sequestration device includes an inlet port connected with the patient needle, and a sequestration chamber connected with the inlet port, the sequestration chamber having a vent comprising an air permeable blood barrier. The blood sequestration device further includes a sampling channel having a proximal end connected with the inlet port, and an outlet port connected with a distal end of the sampling channel and with the sample collection device.

[0017] In yet another aspect, a blood sequestration device connected with a blood sampling system is described. The blood sampling system includes a patient needle for accessing a blood sample from a patient, and a sample needle that is sealed and adapted for receiving an evacuated blood collection tube. The blood sequestration device includes an inlet port connected with the patient needle to receive the blood sample from the patient. The blood sequestration device further includes a sequestration chamber connected with the inlet port and having a vent comprising an air permeable blood barrier, the sequestration chamber for receiving and sequestering a first portion of the blood sample prior to the sample needle being unsealed by the evacuated blood collection tube. The blood sequestration device further includes a sampling channel having a proximal end connected with the inlet port, the

sampling channel for conveying a subsequent portion of the blood sample once the sample needle is unsealed by the evacuated blood collection tube. The blood sequestration device further includes an outlet port connected with a distal end of the sampling channel for conveying the subsequent portion of the blood sample to the sample needle.

[0018] In yet another aspect, a blood sample optimization system is disclosed and described. The blood sample optimization system includes a blood sampling system for accessing and acquiring one or more samples of a patient's blood, and a blood sequestration device for receiving and sequestering a first portion of the one or more samples of the patient's blood which might be contaminated by a venipuncture process and which could result in a false positive identification of a pathogen in the patient's blood.

[0019] The blood sampling system includes a patient needle configured for a venipuncture of a patient to access a sample of blood of a patient, a blood sampling pathway connected with the patient needle for conveying the sample of blood, and a sample needle configured for receiving an evacuated blood collection container to collect and contain a subsequent portion of the sample of blood.

[0020] In yet another aspect, a blood sequestration device is disclosed and described. In some implementations, the blood sequestration device can include an inlet port, an outlet port connected with the inlet port, and a sequestration chamber connected with the inlet port. The sequestration chamber can have a vent comprising an air permeable blood barrier.

[0021] The blood sequestration device is connected along the blood sampling pathway between the patient needle and the sample needle, and includes an inlet port for receiving the sample of blood. The blood sequestration device further includes a sequestration chamber connected with the inlet port for receiving a first amount of the sample of blood, the sequestration chamber having a vent comprising an air permeable blood barrier for sequestering at least a first portion of the first amount of the sample of blood. The blood sequestration device may further include a sampling channel having a proximal end connected with the inlet port, the sampling channel conveying a subsequent amount of the sample of blood to the evacuated blood collection container upon the sequestration chamber sequestering at least the first portion of the first amount of the sample of blood. The blood

sequestration device further includes an outlet port connected with a distal end of the sampling channel, the outlet port for outputting the subsequent amount of the sample of blood.

[0022] The details of one or more embodiments are set forth in the accompanying drawings and the description below. Other features and advantages will be apparent from the description and drawings, and from the claims.

BRIEF DESCRIPTION OF THE DRAWINGS

[0023] These and other aspects will now be described in detail with reference to the following drawings.

[0024] FIG. 1 illustrates a blood sample optimization system.

[0025] FIG. 2 illustrates a blood sample optimization system in accordance with an alternative implementation.

[0026] FIG. 3 illustrates a blood sample optimization system in accordance with another alternative implementation.

[0027] FIG. 4 illustrates a blood sample optimization system in accordance with another alternative implementation.

[0028] FIG. 5 illustrates a blood sample optimization system in accordance with another alternative implementation.

[0029] FIG. 6 illustrates a blood sample optimization system in accordance with an alternative implementation.

[0030] FIG. 7 is a flowchart of a method for optimizing a quality of a blood culture.

[0031] FIGS. 8A – 8E illustrate a blood sequestration system for non-contaminated blood sampling, in accordance with some implementations.

[0032] FIG. 9 illustrates a pathway splitter for use in a blood sequestrations system.

[0033] FIGS. 10A – 10D illustrate a blood sequestration system for non-contaminated blood sampling, in accordance with alternative implementations.

[0034] FIGS. 11A – 11E illustrate a blood sequestration system for non-contaminated blood sampling, in accordance with other alternative implementations.

[0035] FIGS. 12A-12D illustrate a blood sample optimization system including a blood sequestration device in accordance with yet other alternative implementations.

[0036] FIGS. 13A-13D illustrate a blood sample optimization system 1300 in accordance with yet another alternative implementations.

[0037] FIGS. 14A-14E illustrate yet another implementation of a blood sampling system to sequester contaminates of an initial aliquot or sample to reduce false positives in blood cultures or tests performed on a patient's blood sample.

[0038] FIGS. 15A-15G illustrate a blood sequestration device and method of using the same, in accordance with yet another implementation.

[0039] FIGS. 16A-16D illustrate a blood sequestration device in accordance with yet another implementation.

[0040] FIGS. 17A – 17D illustrate a bottom member of a housing for a blood sequestration device.

[0041] FIGS. 18A – 18F illustrate a top member of a housing for a blood sequestration device.

[0042] FIGS. 19A and 19B illustrate a blood sequestration device having a top member mated with a bottom member.

[0043] FIG. 20 shows a blood sample optimization system including a blood sequestration device.

[0044] FIG. 21 illustrates a non-vented blood sequestration device using a wicking material chamber.

[0045] FIGS. 22A and 22B illustrate a material makeup of a filter for sequestering blood in a sequestration chamber of a blood sequestration device.

[0046] FIGS. 23A and 23B illustrate another implementation of a blood sequestration device that uses a vacuum force from a blood collection device.

[0047] Like reference symbols in the various drawings indicate like elements.

DETAILED DESCRIPTION

[0048] This document describes blood sample optimization systems and methods for reducing or eliminating contaminates in collected blood samples, which in turn reduces or eliminates false positive readings in blood cultures or other testing of collected blood samples. In some implementations, a blood sample optimization system includes a patient needle for vascular access to a patient's bloodstream, a sample needle for providing a blood sample to a blood collection container, such as an evacuated blood collection container or tube like a Vacutainer™ or the like, or other sampling device, and a blood sequestration device located between the patient needle and the sample needle. The blood sequestration device includes a sequestration chamber for sequestering an initial, potentially contaminated aliquot of blood, and may further include a sampling channel that bypasses the sequestration chamber to convey likely uncontaminated blood between the patient needle and the sample needle after the initial aliquot of blood is sequestered in the sequestration chamber.

[0049] FIG. 1 illustrates a blood sample optimization system in accordance with some implementations. The system includes a patient needle 1 to puncture the skin of a patient to access the patient's vein and blood therein. The system further includes a sample needle (i.e., a resealably closed needle for use with Vacutainers™ or the like) 5, which may be contained within and initially sealed by a resealable boot 10, a Luer activated valve, or another collection interface or device. The resealable boot 10 can be pushed aside or around the sample needle 5 by application of a Vacutainer™ bottle (not shown) for drawing the patient's blood. The system can further include a low volume chamber 30 that leads to the sample needle 5, but also includes an orifice or one or more channels 45 that lead to a sequestration chamber 55 formed by a housing 50.

[0050] The sequestration chamber 55 is a chamber, channel, pathway, lock, or other structure for receiving and holding a first aliquot of the patient's blood, which may be in a predetermined or measured amount, depending on a volume of the sequestration chamber 55. The first draw of blood typically contains or is more susceptible to containing organisms that cause bacteraemia and sepsis or other pathogens than subsequent blood draws. The sequestration chamber 55 can be a vessel encased in a solid housing, formed in or defined by the housing itself, or can be implemented as tubing or a lumen. The sequestration chamber 55, regardless how formed and implemented, may have a predetermined volume. In some implementations, the predetermined volume may be based on a volume of the patient needle, i.e. ranging from less than the volume of the patient needle to any volume up to or greater than 20 times or more of the volume of the patient needle. The predetermined volume of the sequestration chamber 55 may also be established to economize or minimize an amount of blood to be sequestered and disposed of.

[0051] The sequestration chamber 55 can be formed, contained or housed in a chamber housing 50, and can be made of plastic, rubber, steel, aluminum or other suitable material. For example, the sequestration chamber 55 could be formed of flexible tubing or other elastomeric materials. The sequestration chamber 55 further includes an air permeable blood barrier 20 that allows air to exit the sequestration chamber 55. As used herein the term "air permeable blood barrier" means an air permeable but substantially blood impermeable substance, material, or structure. Examples may include hydrophobic membranes and coatings, a hydrophilic membrane or coating combined with a hydrophobic membrane or coating, mesh, a filter, a mechanical valve, antimicrobial material, or any other means of allowing air to be displaced from the sequestration chamber 55 as it is filled with blood. In various exemplary embodiments, an air permeable blood barrier may be formed by one or more materials that allow air to pass through until contacted by a liquid, such material then becomes completely or partially sealed to prevent or inhibit the passage of air and/or liquid. In other words, prior to contact with liquid, the material forms a barrier that is air permeable. After contact with a liquid, the material substantially or completely prevents the further passage of air and/or liquid.

[0052] The orifice or channel 45 can be any desired length, cross-sectional shape or size, and/or can be formed to depart from the low volume chamber 30 at any desired angle or

orientation. The orifice or channel 45 may also include a one-way flap or valve 60 that maintains an initial aliquot of blood sample within the sequestration chamber 55. In some specific implementations, the orifice or channel 45 can include a "duck bill" or flapper valve 60, or the like, for one-way flow of blood from low volume chamber 30 to the sequestration chamber 55. The air permeable blood barrier 20 can also be constructed of a material that allows air to exit but then seals upon contact with blood, thereby not allowing external air to enter sequestration chamber 55. This sealing would eliminate the need for a valve.

[0053] Valve 60 can be any type of valve or closing mechanism. Chamber 30 is designed to hold virtually no residual blood, and can be designed to be adapted to hold or allow pass-through of a particular volume or rate of blood into sequestration chamber 55. Likewise, sequestration chamber 55 may also include any type of coating, such as an anti-microbial coating, or a coating that aids identification and/or diagnosis of components of the first, sequestered blood draw.

[0054] Housing 50 and 40 can be formed of any suitable material, including plastic, such as acrylonitrile butadiene styrene (ABS) or other thermoplastic or polymeric material, rubber, steel, or aluminum. The air permeable blood barrier 20 can include a color-providing substance, or other signaling mechanism, that is activated upon contact with blood from the initial blood draw, or when air displacement is stopped, or any combination of events with blood in the sequestration chamber 55. The air permeable barrier may also include an outer layer such as a hydrophobic membrane or cover that inhibits or prevents the inadvertent or premature sealing of the filter by an external fluid source, splash etc. Sequestration chamber 55 can also be translucent or clear to enable a user to visually confirm the chamber is filled.

[0055] FIG. 2 illustrates a blood sample optimization system in accordance with some alternative implementations. In the implementation shown in FIG. 2, a sequestration chamber 55, or waste chamber, surrounds the patient needle 1, with an open-ended cuff or housing connected with the waste chamber and encircling the sample needle housing base and housing. The patient needle 1 and sample needle 5 are connected together by a boot 56, which forms a continuous blood draw channel therethrough. The boot 56 includes a single orifice or channel leading from the blood draw channel into sequestration chamber 55. The device can include more than one single orifice or channel, in other implementations. Each

orifice or channel can include a one-way valve, and can be sized and adapted for predetermined amount of blood flow.

[0056] The sequestration chamber 55 includes an air permeable blood barrier. The filter can further include a sensor or indicator to sense and/or indicate, respectively, when a predetermined volume of blood has been collected in the sequestration chamber 55. That indication will alert a user to attach an evacuated blood collection tube or bottle, such as a Vacutainer™ to the sample needle 5. The housing for the sequestration chamber 55 can be any size or shape, and can include any type of material to define an interior space or volume therein. The interior space is initially filled only with air, but can also be coated with an agent or substance, such as a decontaminate, solidifying agent, or the like. Once evacuated blood collection tube is attached to the sample needle 5, blood will flow automatically into the patient needle 1, through the blood draw channel and sample needle 5, and into the bottle. The sample needle 5 is covered by a resealable boot, coating or membrane that seals the sample needle when a blood collection bottle is not attached thereon or thereto.

[0057] FIG. 3 illustrates a blood sample optimization system in accordance with some alternative implementations. In the implementation shown, a sample needle 5 is surrounded by a resealable boot or membrane, and is further connected with a patient needle 1. A blood flow channel is formed through the sample needle and the patient needle. The connection between the sample needle and patient needle includes a "T" or "Y" connector 102, which includes a channel, port or aperture leading out from the main blood flow channel to a sequestration chamber 104.

[0058] The T or Y connector 102 may include a flap or one-way valve, and have an opening that is sized and adapted for a predetermined rate of flow of blood. The sequestration chamber 104 can be formed from tubing, or be formed by a solid housing, and is initially filled with air. The sequestration chamber 104 will receive blood that flows out of a patient automatically, i.e. under pressure from the patient's own blood pressure. The sequestration chamber 104 includes an air permeable blood barrier 106, preferably at the distal end of tubing that forms the sequestration chamber 104, and which is connected at the proximal end to the T or Y connector 102. The T or Y connector 102 can branch off at any desired angle for most efficient blood flow, and can be formed so as to minimize an interface

between the aperture and channel and the main blood flow channel, so as to minimize or eliminate mixing of the initial aliquot of blood with main blood draw samples.

[0059] In some alternative implementations, the sample needle may be affixed to a tubing of any length, as shown in FIG. 4, connecting at its opposite end to the T or Y connector 102. The sequestration chamber 104 can be any shape or volume so long as it will contain a predetermined amount of blood sample in the initial aliquot. The T or Y connector 102 may also include an opening or channel that is parallel to the main blood flow channel. The air permeable blood barrier may further include an indicator 107 or other mechanism to indicate when a predetermined amount of blood has been collected in the sequestration chamber, or when air being expelled reaches a certain threshold, i.e. to zero. The tubing can also include a clip 109 that can be used to pinch off and prevent fluid flow therethrough.

[0060] Once the air permeable blood barrier and primary chamber are sealed the initial aliquot of blood is trapped in the sequestration chamber 104, an evacuated blood collection tube, such as a Vacutainer™ bottle may be attached to the sample needle 5 to obtain the sample. The blood collection tube can be removed, and the sample needle 5 will be resealed. Any number of follow-on blood collection tubes can then be attached for further blood draws or samples. Upon completion of all blood draws, the system can be discarded, with the initial aliquot of blood remaining trapped in the sequestration chamber 104.

[0061] FIG. 5 illustrates a blood sample optimization system in accordance with some alternative implementations. In the implementation shown, a sample needle 5 is connected with a patient needle by tubing. A "T" or "Y" connector 120 is added along the tubing at any desired location, and includes an aperture, port or channel leading to a sequestration chamber 204, substantially as described above.

[0062] FIG. 6 illustrates a blood sample optimization system in accordance with some alternative implementations, in which a sequestration chamber 304, formed as a primary collection channel, receives an initial aliquot of blood, and is provided adjacent to the blood sampling channel. The sequestration chamber 304 can encircle the blood sampling channel, the patient needle 1, and/or the sample needle 5. The primary collection channel can include a T or Y connector 120, or other type of aperture or channel. The sequestration

chamber 304 includes an air permeable blood barrier, which can also include an indicator of being contacted by a fluid such as blood, as described above.

[0063] In some implementations, either the patient needle 1 or the sample needle 5, or both, can be replaced by a Luer lock male or female connector. However, in various implementations, the connector at a sample needle end of the blood sample optimization system is initially sealed to permit the diversion of the initial aliquot of blood to the sequestration chamber, which is pressured at ambient air pressure and includes the air outlet of the air permeable blood barrier. In this way, the system passively and automatically uses a patient's own blood pressure to overcome the ambient air pressure of the sequestration chamber to push out air through the air permeable blood barrier and displace air in the sequestration chamber with blood.

[0064] FIG. 7 is a flowchart of an exemplary method for optimizing the quality of a blood culture. At 702, a clinician places a needle into a patient's vein. At 704, blood then flows into a sequestration chamber, pushing the air in the sequestration chamber out of the sequestration chamber through an air permeable blood barrier. In some implementations, the volume of the sequestration chamber is less than 0.1 to more than 5 cubic centimeters (cc's), or more. The sequestration chamber is sized and adapted to collect a first portion of a blood sample, which is more prone to contamination than secondary and other subsequent portion of the blood sample or subsequent draws. Since the sequestration chamber has an air-permeable blood barrier through which air can be displaced by blood pushed from the patient's vein, such blood will naturally and automatically flow into the sequestration chamber before it is drawn into or otherwise enters into a Vacutainer or other bottle for receiving and storing a blood sample.

[0065] When the sequestration chamber fills, the blood will gather at or otherwise make contact with the air permeable blood barrier, which will inhibit or prevent blood from passing therethrough. At 706, when the blood comes into contact with the entire internal surface area of the air permeable blood barrier, the air permeable blood barrier is then closed and air no longer flows out or in. At 708, the clinician may be provided an indictor or can see the full chamber, to indicate the evacuated blood collection tube, such as a Vacutainer™ can be attached. The indicator can include visibility into the primary chamber to see whether

it is full, the blood barrier changing color, for example, or other indicator. The fill time of the sequestration chamber may be substantially instantaneous, so such indicator, if present, may be only that the sequestration chamber is filled.

[0066] Prior to an evacuated blood collection tube being attached, communication between the needle, sampling channel, and the sequestration chamber is restricted by the sealing of the sequestration chamber blood barrier thereby not permitting air to reenter the system through the sequestration. Sealing the communication path could also be accomplished with a mechanical twist or other movement, a small orifice or tortuous pathway, eliminating the need for a separate valve or mechanical movement or operation by the clinician. At 710, once the evacuated blood collection tube is removed, the self-sealing membrane closes the sample needle, and at 712, additional subsequent evacuated blood collection tubes may be attached. Once samples have been taken, at 714 the device is removed from the patient and discarded.

[0067] FIGS. 8A – 8E illustrate an exemplary blood sample optimization system 800 for non-contaminated blood sampling, in accordance with some implementations. The blood sample optimization system 800 includes an inlet port 802 that can be connected to tubing, a patient needle (or both), or other vascular or venous access device, and a pathway splitter 804 having a first outlet to a sequestration chamber tubing 806 and a second outlet to sample collection tubing 808. One or both of the sequestration chamber tubing 806 and the sample collection tubing 808 can be formed of tubing. In some implementations, the sequestration chamber tubing 806 is sized so as to contain a particular volume of initial blood sample. The sample collection tubing 808 will receive a blood sample once the sequestration chamber tubing 806 is filled. The sample collection tubing 808 can be connected to a Vacutainer™ base or housing 810, or other blood sample collection device.

[0068] The blood sequestration system 800 further includes a blood sequestration device 812 which, as shown in more detail in FIGS. 8B – 8D, includes a housing 818 that includes a sampling channel 820 defining a pathway for the non-contaminated sample collection tubing 808 or connected at either end to the non-contaminated sample collection tubing 808. The sampling channel 820 can be curved through the housing 818 so as to better

affix and stabilize the housing 818 at a location along the non-contaminated sample collection tubing 808.

[0069] The blood sequestration device 812 further includes a sequestration chamber 822 connected with the sequestration chamber tubing 806 or other chamber. The sequestration chamber 822 terminates at an air permeable blood barrier 824. The air permeable blood barrier 824 can also include a coloring agent that turns a different color upon full contact with blood, as an indicator that the regular collection of blood samples (i.e. the non-contaminated blood samples) can be initiated. Other indicators may be used, such as a small light, a sound generation mechanism, or the like. In some implementations, the air permeable blood barrier is positioned at a right angle from the direction of sequestration chamber 822, but can be positioned at any distance or orientation in order to conserve space and materials used for the housing 818. The housing 818 and its contents can be formed of any rigid or semi-rigid material or set of materials.

[0070] FIG. 9 illustrates a pathway splitter 900 for use in a blood sequestrations system, such as those shown in FIGS. 8A – 8E, for example. The pathway splitter 900 includes an inlet port 902, a main line outlet port 904, and a sequestration channel outlet port 906. The inlet port 902 can be connected to main tubing that is in turn connected to a patient needle system, or directly to a patient needle. The main line outlet port 904 can be connected to main line tubing to a blood sampling system, such as a vacutainer base or housing, or directly to such blood sampling system. The sequestration channel outlet port 906 can be connected to sequestration tubing for receiving and sequestering a first sample of blood, up to a measured amount or predetermined threshold. Alternatively, the sequestration channel outlet port 906 can be connected to a sequestration chamber. The sequestration channel outlet port 906 is preferably 20-70 degrees angled from the main line outlet port 904, which in turn is preferably in-line with the inlet port 902. Once the predetermined amount of initial blood sample is sequestered in the sequestration tubing or chamber, in accordance with mechanisms and techniques described herein, follow-on blood samples will flow into the inlet port 902 and directly out the main line outlet port 904, without impedance.

[0071] FIGS. 10A – 10D illustrate a blood sequestration device 1000 in accordance with alternative implementations. The blood sequestration device 1000 includes an inlet port

1002, a main outlet port 1004, and a sequestration channel port 1006. The inlet port 1002 can be connected to a patient needle or related tubing. The main outlet port 1004 can be connected to a blood sample collection device such as a Vacutainer, associated tubing, or a Luer activated valve, or the like. The sequestration channel port 1006 splits off from the main outlet port 1004 to a sequestration chamber 1008. In some implementations, the sequestration chamber 1008 is formed as a helical channel within a housing or other container 1001.

[0072] The sequestration chamber 1008 is connected at the distal end to an air permeable blood barrier 1010, substantially as described above. Air in the sequestration chamber 1008 is displaced through the air permeable blood barrier 1010 by an initial aliquot of blood that is guided into the sequestration channel port 1006. Once the sequestration chamber 1008 is filled, further blood draws through the main outlet port 1004 can be accomplished, where these samples will be non-contaminated.

[0073] FIGS. 11A – 11E illustrate a blood sequestration device 1100 in accordance with other alternative implementations. The blood sequestration device 1100 includes an inlet port 1102, similar to the inlet ports described above, a main outlet port 1104, and a sequestration channel port 1106 that splits off from the main outlet port 1104 and inlet port 1102. The sequestration channel port is connected to a sequestration chamber 1108. In the implementation shown in FIGS. 11A – 11E, the blood sequestration device includes a base member 1101 having a channel therein, which functions as the sequestration chamber 1108. The channel can be formed as a tortuous path through the base member 1101, which is in turn shaped and formed to rest on a limb of a patient.

[0074] A portion of the sequestration chamber 1108 can protrude from the base member or near a top surface of the base member, just before exiting to an air permeable blood barrier 1110, to serve as a blood sequestration indicator 1109. The indicator 1109 can be formed of a clear material, or a material that changes color when in contact with blood.

[0075] In some implementations, the blood sequestration device 1100 can include a blood sampling device 1120 such as a normally closed needle, Vacutainer™ shield or other collection device. The blood sampling device 1120 can be manufactured and sold with the

blood sequestration device 1100 for efficiency and convenience, so that a first aliquot of blood that may be contaminated by a patient needle insertion process can be sequestered. Thereafter, the blood sampling device 1120 can draw non-contaminated blood samples to reduce the risk of false positive testing and ensure a non-contaminated sample.

[0076] FIGS. 12A-12D illustrate a blood sample optimization system 1200 in accordance with yet other alternative implementations. The system 1200 includes a blood sequestration device 1202 for attaching to a blood sampling device 1204, such as a Vacutainer™ or other collection and sampling device. The blood sequestration device 1202 is configured and arranged to receive, prior to a Vacutainer™ container or vial being attached to a collection needle of the blood sampling device 1204, a first aliquot or amount of blood, and sequester that first aliquot or amount in a sequestration channel of the blood sequestration device 1202.

[0077] In some implementations, the blood sequestration device 1202 can include an inlet port 1212, a main outlet port, and a sequestration channel port. The inlet port 1212 can be connected to a patient needle or related tubing. The main outlet port 1214 can be connected to a normally closed needle or device to enable connection with an evacuated blood collection container or other collection device such as a Vacutainer™, associated tubing, luer connectors, syringe, a Luer activated valve, or the like. The sequestration channel port splits off from the main outlet port to a sequestration chamber 1218.

[0078] In some implementations, the sequestration chamber 1218 is formed as a channel within the body of a sequestration device 1202. The sequestration chamber 1218 can be a winding channel, such as a U-shaped channel, an S-shaped channel, a helical channel, or any other winding channel. The sequestration device 1202 can include a housing or other containing body, and one or more channels formed therein. As shown in FIGS. 12A and 12B, the sequestration device 1202 includes a main body 1206 and a cap 1208. The main body 1206 is formed with one or more cavities or channels, which are further formed with one or more arms 1210 that extend from the cap 1208, and which abut the cavities or channels in the main body 1206 to form the primary collection port and main outlet port.

[0079] FIGS. 13A-13D illustrate a blood sample optimization system 1300 in accordance with yet other alternative implementations. The system 1300 includes a blood sequestration device 1302 for attaching to a blood sampling device 1304, such as a Vacutainer or other bodily fluid collection and sampling device. The blood sequestration device 1302 is configured and arranged to receive, prior to a Vacutainer container or vial being attached to a collection needle of the blood sampling device 1304, a first aliquot or amount of blood, and to sequester that first aliquot or amount of blood or other bodily fluid in a sequestration channel of the blood sequestration device 1302.

[0080] The blood sequestration device 1302 includes a housing 1301 having an inlet port 1314, a main outlet port 1312, and a sequestration channel port 1316. The inlet port 1314 can be connected to a patient needle or associated tubing. The main outlet port 1312 can be connected to a normally closed needle or device to enable connection with an evacuated blood collection container or other collection device such as a Vacutainer™, associated tubing, luer connectors, syringe, a Luer activated valve, or the like. The sequestration channel port 1316 splits off from the main inlet port 1314 to a sequestration chamber 1318.

[0081] In the implementation shown in FIGS. 13A-D, the sequestration chamber 1318 is formed as a cavity or chamber within housing 1301 or formed by walls that define housing 1301. The sequestration chamber 1318 can be a winding channel, such as a U-shaped channel, an S-shaped channel, a helical channel, or any other winding channel, that is defined by the cooperation and connection of housing 1301 with cap 1307 which cap 1307 can include a protrusion 1305 that provides one or more walls or directors for the winding channel in the sequestration chamber 1318. The protrusion 1305 from the cap 1307 can be straight or curved, and may have various channels, apertures or grooves embedded therein, and can extend from the cap 1307 any angle or orientation. When the cap 1307 is connected with the housing 1301 to complete the formation of the sequestration chamber 1318, the protrusion 1305 forms at least part of the winding channel to sequester a first aliquot or amount of blood or other bodily fluid in a sequestration channel formed in the sequestration chamber 1318 and by the winding channel.

[0082] The sequestration chamber 1318 includes an air permeable blood barrier 1310, substantially as described above. Air in the sequestration chamber 1318 is displaced through the air permeable blood barrier 1310 by an initial aliquot of blood that is provided into the sequestration chamber 1318 by the blood pressure of the patient. Once the sequestration chamber 1318 is filled and the air in the sequestration chamber 1318 displaced, the blood pressure of the patient will be insufficient to drive or provide further blood into the blood sequestration device 1302, and in particular the outlet port 1312, until a force such as a vacuum or other pressure, such as provided by the blood sample collection device like Vacutainer is provided to draw out a next aliquot or amount of blood or bodily fluid. Further blood draws through the main outlet port 1312 can be accomplished, where these samples will be non-contaminated since any contaminants would be sequestered in the sequestration chamber 1318 with the first aliquot of blood.

[0083] FIGS. 14A-14E illustrate yet another implementation of a blood sampling system 1400 to sequester contaminates of an initial aliquot or sample to reduce false positives in blood cultures or tests performed on a patient's blood sample. The blood sampling system 1400 includes a blood sequestration device 1401 that can be connected between a blood sample collection device 1403 and a patient needle (not shown). The blood sample collection device 1403 can be a Vacutainer or the like. The blood sequestration device 1401 includes an inlet port 1402 that can be connected with a patient needle that is inserted into a patient's vascular system for access to and withdrawing of a blood sample. The inlet port 1402 may also be connected with tubing or other conduit that is in turn connected with the patient needle.

[0084] The inlet port 1402 defines an opening into the blood sequestration device 1401, which opening can be the same cross sectional dimensions as tubing or other conduit connected with the patient needle or the patient needle itself. For instance, the opening can be circular with a diameter of approximately 0.045 inches, but can have a diameter of between 0.01 inches or less to 0.2 inches or more. The blood sequestration device 1401 further includes an outlet port 1404, which defines an opening out of the blood sequestration device 1401 and to the blood sample collection device 1403. The outlet port 1404 may also be connected with tubing or other conduit that is in turn connected with the blood sequestration device 1403. The outlet port 1404 can further include a connector device such

as a threaded cap, a Luer connector (male or female), a non threaded interference or glue joint fitting for attachment of various devices including but not limited to tubing, or the like.

[0085] The blood sequestration device 1401 further includes a sampling channel 1406 between the inlet port 1402 and the outlet port 1404, and which functions as a blood sample pathway once a first aliquot of blood has been sequestered. The sampling channel 1406 can be any sized, shaped or configured channel, or conduit. In some implementations, the sampling channel 1406 has a substantially similar cross sectional area as the opening of the inlet port 1402. In other implementations, the sampling channel 1406 can gradually widen from the inlet port 1402 to the outlet port 1404.

[0086] The blood sequestration device 1401 further includes a sequestration chamber 1408 that is connected to and split off or diverted from the sampling channel 1406 at any point between the inlet port 1402 and the outlet port 1404, but preferably from a proximal end of the sampling channel 1406 near the inlet port 1402. The sequestration chamber 1408 is at first maintained at atmospheric pressure, and includes an air outlet 1412 at or near a distal end of the sequestration chamber 1408 opposite the diversion point from the sampling channel 1406. The air outlet 1412 includes an air permeable blood barrier 1412. As shown in FIG. 14B, the air permeable blood barrier 1412 can be overlaid with a protective cover 1416. The protective cover 1416 can be sized and configured to inhibit a user from touching the air permeable blood barrier 1412 with their finger or other external implement, while still allowing air to exit the air permeable blood barrier 1412 as the air is displaced from the sequestration chamber 1408 by blood being forced into the sequestration chamber 1408 by a patient's own blood pressure. In addition the protective cover 1416 can be constructed to inhibit or prevent accidental exposure of the air permeable blood barrier to environmental fluids or splashes. This can be accomplished in a variety of mechanical ways including but not limited to the addition of a hydrophobic membrane to the protective cover.

[0087] As shown in FIGS. 14C and 14D, the sampling channel 1406 can be cylindrical or frusto-conical in shape, going from a smaller diameter to a larger diameter, to minimize a potential to lyse red blood cells. Likewise, the sampling channel 1406 is formed with a minimal amount of or no sharp turns or edges, which can also lyse red blood cells. The sampling channel 1406 splits off to the sequestration chamber 1408 near the inlet port

1402 via a diversion pathway 1409. The diversion pathway 1409 can have any cross-sectional shape or size, but is preferably similar to the cross-sectional shape of at least part of the inlet port 1402.

[0088] In some implementations, the sampling channel 1406 and the sequestration chamber 1408 are formed by grooves, channels, locks or other pathways formed in housing 1414. The housing 1414 can be made of plastic, metal or other rigid or semi-rigid material. The housing 1414 can have a bottom member that sealably mates with a top member. One or both of the bottom member and the top member can include the sampling channel 1406 and the sequestration chamber 1408, as well as the diversion pathway 1409, the inlet port 1402, and the outlet port 1404. In some other implementations, one or more of the diversion pathway 1409, the inlet port 1402, and/or the outlet port 1404 can be at least partially formed by a cap member that is connected to either end of the housing 1414. In some implementations, the top member and the bottom member, as well as the cap member(s), can be coupled together by laser welding, heat sealing, gluing, snapping, screwing, bolting, or the like. In other implementations, some or all of the interior surface of the diversion pathway 1409 and/or sequestration chamber 1408 can be coated or loaded with an agent or substance, such as a decontaminate, solidifying agent, or the like. For instance, a solidifying agent can be provided at the diversion pathway 1409 such that when the sequestration chamber 1408 is filled and the initial aliquot of blood backs up to the diversion pathway 1409, that last amount of sequestered blood could solidify, creating a barrier between the sequestration chamber 1408 and the sampling channel 1406.

[0089] FIGS. 15A-15G illustrate a blood sequestration device 1500. The blood sequestration device 1500 can be connected to a normally closed needle or device to enable connection with an evacuated blood collection container or other collection device such as a Vacutainer™, associated tubing, luer connectors, syringe, a Luer activated valve, or the like.

[0090] The blood sequestration device 1500 includes an inlet port 1502 that can be connected with a patient needle that is inserted into a patient's vascular system for access to and withdrawing of a blood sample. The inlet port 1502 may also be connected with tubing or other conduit that is in turn connected with the patient needle. The inlet port 1502 defines an opening into the blood sequestration device 1500, which opening may be the same cross

sectional dimensions as tubing or other conduit connected with the patient needle or the patient needle itself. For instance, the opening can be circular with a diameter of approximately 0.045 inches, but can have a diameter of between 0.01 inches or less to 0.2 inches or more.

[0091] The inlet port 1502 can also include a sealing or fluid-tight connector or connection, such as threading or Luer fitting, or the like. In some implementations, tubing or other conduit associated with the patient needle can be integral with the inlet port 1502, such as by co-molding, gluing, laser weld, or thermally bonding the parts together. In this manner, the blood sequestration device 1500 can be fabricated and sold with the patient needle as a single unit, eliminating the need for connecting the patient needle to the blood sequestration device 1500 at the time of blood draw or sampling.

[0092] The blood sequestration device 1500 further includes an outlet port 1504, which defines an opening out of the blood sequestration device 1500 and to the blood sample collection device. The outlet port 1504 may also be connected with tubing or other conduit that is in turn connected with the blood sequestration device, and may also include a sealing or fluid-tight connector or connection, such as threading or Luer fitting, or the like. Accordingly, as discussed above, the blood sequestration device 1500 can be fabricated and sold with the patient needle and/or tubing and the blood sample collection device as a single unit, eliminating the need for connecting the patient needle and the blood sample collection device to the blood sequestration device 1500 at the time of blood draw or sampling.

[0093] The blood sequestration device 1500 further includes a sampling channel 1506 between the inlet port 1502 and the outlet port 1504, and which functions as a blood sample pathway once a first aliquot of blood has been sequestered. The sampling channel 1506 can be any sized, shaped or configured channel or conduit. In some implementations, the sampling channel 1506 has a substantially similar cross sectional area as the opening of the inlet port 1502. In other implementations, the sampling channel 1506 can gradually widen from the inlet port 1502 to the outlet port 1504.

[0094] The blood sequestration device 1500 further includes a sequestration chamber 1508 that is connected to and split off or diverted from the sampling channel 1506 at any

point between the inlet port 1502 and the outlet port 1504, but preferably from a proximal end of the sampling channel 1506 near the inlet port 1502. In some implementations, the diversion includes a Y-shaped junction. The sequestration chamber 1508 is preferably maintained at atmospheric pressure, and includes a vent 1510 at or near a distal end of the sequestration chamber 1508. The vent 1510 includes an air permeable blood barrier 1512. FIG. 15C illustrates the blood sequestration device 1500 with the sequestration chamber 1508 filled with a first aliquot or sample of blood from the patient.

[0095] The air permeable blood barrier 1512 can be covered with a protective cover 1516. The protective cover 1516 can be sized and configured to inhibit a user from touching the air permeable blood barrier 1512 with their finger or other external implement, while still allowing air to exit the air permeable blood barrier 1512 as the air is displaced from the sequestration chamber 1508 by blood being forced into the sequestration chamber 1508 by a patient's own blood pressure. The protective cover 1516 can be constructed to inhibit or prevent accidental exposure of the filter to environmental fluids or splashes. This can be accomplished in a variety of mechanical ways including but not limited to the addition of a hydrophobic membrane to the protective cover.

[0096] FIG. 15B is a perspective view of the blood sequestration device 1500 from the outlet port 1504 and top side of a housing 1501 of the blood sequestration device 1500 that includes the vent 1510, and illustrating an initial aliquot of blood filling sequestration chamber 1508 while the sampling channel 1506 is empty, before a sample collection device is activated. FIG. 15G is a perspective view of the blood sequestration device 1500 from the outlet port 1504 and bottom side of the housing 1501 of the blood sequestration device 1500, and illustrating the initial aliquot of blood filling sequestration chamber 1508 while the sampling channel 1506 is empty, before the sample collection device is activated. FIG. 15C is another perspective view of the blood sequestration device 1500 from the inlet port 1502 and top side of a housing 1501 of the blood sequestration device 1500 that includes the vent 1510, and illustrating blood now being drawn through sampling channel 1506 while the sequestered blood remains substantially in the sequestration chamber 1508.

[0097] FIG. 15D is a cross section of the blood sequestration device 1500 in accordance with some implementations, showing the housing 1501 that defines the sampling

channel 1506 and the sequestration chamber 1508. FIGS. 15E and 15F illustrate various form factors of a housing for a blood sequestration device, in accordance with one or more implementations described herein.

[0098] The sequestration chamber 1508 can have a larger cross-sectional area than the sampling channel 1506, and the cross-sectional area and length can be configured for a predetermined or specific volume of blood to be sequestered or locked. The sampling channel 1506 can be sized to be compatible with tubing for either or both of the patient needle tubing or the blood collection device tubing.

[0099] The housing 1501 can be formed of multiple parts or a single, unitary part. In some implementations, and as illustrated in FIG. 15D, the housing 1501 includes a top member 1520 and a bottom member 1522 that are mated together, one or both of which having grooves, channels, locks, conduits or other pathways pre-formed therein, such as by an injection molding process or by etching, cutting, drilling, etc. The top member 1520 can be connected with the bottom member 1522 by any mating or connection mechanism, such as by laser welding, thermal bonding, ultrasonic welding, gluing, using screws, rivets, bolts, or the like, or by other mating mechanisms such as latches, grooves, tongues, pins, flanges, or the like.

[00100] In some implementations, such as shown in FIG. 15D, the top member 1520 can include the grooves, channels, locks, conduits or other pathways, while the bottom member 1522 can include a protrusion 1524 that is sized and adapted to fit into at least one of the grooves, channels, locks or other pathways of the top member 1520. The protrusion 1524 can provide a surface feature, such as a partial groove or channel, for instance, to complete the formation of either the sampling channel 1506 and/or the sequestration chamber 1508. In some implementations, the protrusion 1524 can be formed with one or more angled sides or surfaces for a tighter fit within the corresponding groove, channel, lock or other pathway. In yet other implementations, both the top member 1520 and the bottom member can include grooves, channels, locks or other pathways, as well as one or more protrusions 1524.

[00101] In some implementations, the sampling channel 1506 and the sequestration chamber 1508 are formed by grooves, channels, locks or other pathways formed in housing

1501. The housing 1501 can be made of any suitable material, including rubber, plastic, metal or other material. The housing 1501 can be formed of a clear or translucent material, or of an opaque or non-translucent material. In other implementations, the housing 1501 can be mostly opaque or non-translucent, while the housing surface directly adjacent to the sampling channel 1506 and/or the sequestration chamber 1508 is clear or translucent, giving a practitioner a visual cue or sign that the sequestration chamber 1508 is first filled to the extent necessary or desired, and/or then a visual cue or sign that the sequestered blood remains sequestered while a clean sample of blood is drawn through the sampling channel 1506. Other visual cues or signs of the sequestration can include, without limitation: the air permeable blood barrier 1512 turning a different color upon contact, saturation, or partial saturation with blood; a color-coded tab or indicator at any point along or adjacent to the sequestration chamber; an audible signal; a vibratory signal; or other signal.

[00102] After a venipuncture by a patient needle of a patient (not shown), which could gather a number of pathogens from the patient's skin, a first amount of the patient's blood with those pathogens will make its way into the input port 1502 blood sequestration device 1500 and flow into the sequestration chamber 1508 by following the path of least resistance, as the patient's own blood pressure overcomes the atmospheric pressure in the sequestration chamber 1508 to displace air therein through the air permeable blood barrier 1512. The patient's blood pressure will not be sufficient to overcome the air pressure that builds up in the sealed sampling channel 1506. Eventually, the sequestration chamber 1508, which has a predetermined volume, is filled with blood that displaces air through the air permeable blood barrier 1512. Once the blood hits the air permeable blood barrier, the blood interacts with the air permeable blood barrier 1512 material to completely or partially seal the vent 1510. A signal or indication may be provided that the practitioner can now utilize the Vacutainer capsule or other blood sample collection device to acquire a next amount of the patient's blood for sampling. The blood in the sequestration chamber 1508 is now effectively sequestered in the sequestration chamber.

[00103] Upon filling the blood sequestration pathway 1508 but prior to use of the Vacutainer or other blood sample collection device, the patient's blood pressure may drive compression of the air in the sampling channel 1506, possibly resulting in a small amount of blood moving past the diversion point to the sequestration chamber 1508 and into the

sampling channel 1506, queuing up the uncontaminated blood to be drawn through the sampling channel 1506.

[00104] FIGS. 16-19 illustrate yet another implementation of a blood sequestration device. FIGS. 16A-16D illustrate a blood sequestration device 1600 that can be connected between a blood sample collection device, such as an evacuated blood collection container like a Vacutainer™ (not shown), and a patient needle (not shown) and/or associated tubing. FIG. 17 illustrates a bottom member of the blood sequestration device, and FIG. 18 illustrates a top member of the blood sequestration device, which top member and bottom member can be mated together to form an input port, and output port, a sequestration chamber and a sampling channel, as explained more fully below. FIGS. 19A and B show the top member and bottom member mated together. It should be understood that FIGS. 16-19 illustrate one exemplary manner of constructing a blood sequestration device as described herein, and other forms of construction are possible.

[00105] Referring to FIGS. 16A – D, the blood sequestration device 1600 includes an inlet port 1602 that can be connected with a patient needle that is inserted into a patient's vascular system for access to and withdrawing of a blood sample. The inlet port 1602 may also be connected with tubing or other conduit that is in turn connected with the patient needle. The inlet port 1602 defines an opening into the blood sequestration device 1600, which opening can be the same cross sectional dimensions as tubing or other conduit connected with the patient needle or the patient needle itself. For instance, the opening can be circular with a diameter of approximately 0.045 inches, but can have a diameter of between 0.01 inches or less to 0.2 inches or more.

[00106] The inlet port 1602 can also include a sealing or fluid-tight connector or connection, such as threading or Luer fitting, or the like. In some implementations, tubing or other conduit associated with the patient needle can be integral with the inlet port 1602, such as by co-molding, gluing, laser weld, or thermally bonding the parts together. In this manner, the blood sequestration device 1600 can be fabricated and sold with the patient needle and/or tubing as a single unit, eliminating the need for connecting the patient needle to the blood sequestration device 1600 at the time of blood draw or sampling.

[00107] The blood sequestration device 1600 further includes an outlet port 1604, which defines an opening out of the blood sequestration device 1600 and to the blood sample collection device. The outlet port 1604 may also be connected with tubing or other conduit that is in turn connected with the blood sequestration device, and may also include a sealing or fluid-tight connector or connection, such as threading or Luer fitting, or the like. Accordingly, as discussed above, the blood sequestration device 1600 can be fabricated and sold with the patient needle and/or tubing and the blood sample collection device as a single unit, eliminating the need for connecting the patient needle and the blood sample collection device to the blood sequestration device 1600 at the time of blood draw or sampling.

[00108] The blood sequestration device 1600 further includes a sampling channel 1606 between the inlet port 1602 and the outlet port 1604, and a sequestration chamber 1608 that is connected to and split off or diverted from the sampling channel 1606 at any point between the inlet port 1602 and the outlet port 1604. The sampling channel 1606 functions as a blood sampling pathway once a first aliquot of blood has been sequestered in the sequestration chamber 1608. The sampling channel 1606 can be any sized, shaped or configured channel, or conduit. In some implementations, the sampling channel 1606 has a substantially similar cross sectional area as the opening of the inlet port 1602. In other implementations, the sampling channel 1606 can gradually widen from the inlet port 1602 to the outlet port 1604. The sequestration chamber 1608 may have a larger cross section to form a big reservoir toward the sequestration channel path so that the blood will want to enter the reservoir first versus entering a smaller diameter on the sampling channel 1606, as is shown more fully in FIGS. 17 and 19.

[00109] In some exemplary implementations, the diversion between the sampling channel 1606 and the sequestration chamber 1608 is by diverter junction 1607. Diverter junction 1607 may be a substantially Y-shaped, T-shaped, or U-shaped. In some preferred exemplary implementations, and as shown in FIG. 17A – 17B, the diverter junction 1607 is configured such that the flow out of the inlet port 1602 is preferentially directed toward the sequestration chamber 1608. The sequestration chamber 1608 may also include or form a curve or ramp to direct the initial blood flow toward and into the sequestration chamber 1608.

[00110] The sequestration chamber 1608 is preferably maintained at atmospheric pressure, and includes a vent 1610 at or near a distal end of the sequestration chamber 1608. The vent 1610 may include an air permeable blood barrier 1612 as described above.

[00111] The blood sequestration device 1600 can include a housing 1601 that can be formed of multiple parts or a single, unitary part. In some implementations, and as illustrated in FIGS. 17A – 17D and FIGS. 18A – 18F, the housing 1601 includes a top member 1620 and a bottom member 1622 that are mated together. The blood sequestration device 1600 can also include a gasket or other sealing member (not shown) so that when the top member 1620 is mechanically attached with the bottom member 1622, the interface between the two is sealed by the gasket or sealing member. The FIGS. 17A – 17D illustrate a bottom member 1622 of a housing for a blood sequestration device 1600. The bottom member 1622 can include grooves, channels, locks, conduits or other pathways pre-formed therein, such as by an injection molding process or by etching, cutting, drilling, etc., to form the sampling channel 1606, the sequestration chamber 1608, and diverter junction 1607.

[00112] The sequestration chamber 1608 may have a larger cross section than the sampling channel 1606 so that the blood will preferentially move into the sequestration chamber first versus entering a smaller diameter on the sampling channel 1606.

[00113] FIGS. 18A – 18F illustrate the top member 1620, which can be connected with the bottom member 1622 by any mating or connection mechanism, such as by laser welding, thermal bonding, gluing, using screws, rivets, bolts, or the like, or by other mating mechanisms such as latches, grooves, tongues, pins, flanges, or the like. The top member 1620 can include some or all of the grooves, channels, locks, conduits or other pathways to form the sampling channel 1606, the sequestration chamber 1608, and the diverter junction 1607. In yet other implementations, both the top member 1620 and the bottom member 1622 can include the grooves, channels, locks or other pathways.

[00114] In some implementations, the sampling channel 1606 and the sequestration chamber 1608 are formed by grooves, channels, locks or other pathways formed in housing 1601. The housing 1601 can be made of rubber, plastic, metal or any other suitable material. The housing 1601 can be formed of a clear or translucent material, or of an opaque or non-

translucent material. In other implementations, the housing 1601 can be mostly opaque or non-translucent, while the housing surface directly adjacent to the sampling channel 1606 and/or the sequestration chamber 1608 may be clear or translucent, giving a practitioner a visual cue or sign that the sequestration chamber 1608 is first filled to the extent necessary or desired, and/or then a visual cue or sign that the sequestered blood remains sequestered while a clean sample of blood is drawn through the sampling channel 1606. Other visual cues or signs of the sequestration can include, without limitation: the air permeable blood barrier 1612 turning a different color upon contact, saturation, or partial saturation with blood; a color-coded tab or indicator at any point along or adjacent to the sequestration chamber; an audible signal; a vibratory signal; or other signal.

[00115] As shown in FIGS. 18A – 18F, the air permeable blood barrier 1612 can be covered with, or surrounded by, a protective member 1616. The protective member 1616 can be sized and configured to inhibit a user from touching the air permeable blood barrier 1612 with their finger or other external implement, while still allowing air to exit the air permeable blood barrier 1612 as the air is displaced from the sequestration chamber 1608. In some implementations, the protective member 1616 includes a protrusion that extends up from a top surface of the top member 1620 and around the air permeable blood barrier 1612. The protective cover 1616 can be constructed to inhibit or prevent accidental exposure of the filter to environmental fluids or splashes. This can be accomplished in a variety of mechanical ways including but not limited to the addition of a hydrophobic membrane to the protective cover.

[00116] In use, the blood sequestration device 1600 includes a sampling channel 1606 and a sequestration chamber 1608. Both pathways are initially air-filled at atmospheric pressure, but the sampling channel 1606 is directed to an output port 1604 that will be initially sealed by a Vacutainer or other such sealed blood sampling device, and the sequestration chamber 1608 terminates at a vent 1610 to atmosphere that includes an air permeable blood barrier 1612.

[00117] After a venipuncture by a patient needle of a patient (not shown), which could gather a number of pathogens from the patient's skin, a first amount of the patient's blood with those pathogens will pass through input port 1602 of blood sequestration device 1600.

This initial volume of potentially contaminated blood will preferentially flow into the sequestration chamber 1608 by finding the path of least resistance. The patient's own blood pressure overcomes the atmospheric pressure in the vented sequestration chamber 1608 to displace air therein through the air permeable blood barrier 1612, but is not sufficient to overcome the air pressure that builds up in the sealed sampling channel 1606. In various exemplary embodiments, the sequestration chamber 1608 and sampling channel 1606 can be configured such that the force generated by the patient's blood pressure is sufficient to overcome any effect of gravity, regardless of the blood sequestration device's orientation.

[00118] Eventually, the sequestration chamber 1608 fills with blood that displaces air through the air permeable blood barrier 1612. Once the blood contacts the air permeable blood barrier, the blood interacts with the air permeable blood barrier 1612 material to completely or partially seal the vent 1610. A signal or indication may be provided that the practitioner can now utilize the Vacutainer or other blood sampling device.

[00119] Upon filling the blood sequestration pathway 1608 but prior to use of the Vacutainer or other blood sample collection device, the patient's blood pressure may drive compression of the air in the sampling channel 1606, possibly resulting in a small amount of blood moving past the diversion point into the sampling channel 1606, queuing up the uncontaminated blood to be drawn through the sampling channel 1606.

[00120] FIG. 19A is a side view, and FIG. 19B is a cross-sectional view, of the blood sequestration device 1600, illustrating the top member 1620 mated with the bottom member 1622.

[00121] FIG. 20 shows a blood sample optimization system 2000 that includes a patient needle 2002 for vascular access to a patient's bloodstream, a blood sample collection device 2004 to facilitate the collecting of one or more blood samples, and a conduit 2006 providing a fluid connection between the patient needle 2002 and the blood sample collection device 2004. In some implementations, the blood sample collection device 2004 includes a protective shield that includes a sealed collection needle on which a sealed vacuum-loaded container is placed, which, once pierced by the collection needle, draws in a blood sample under vacuum pressure or force through the conduit 2006 from the patient needle 2002.

[00122] The blood sample optimization system 2000 further includes a blood sequestration device 2008, located at any point on the conduit 2006 between the patient needle 2002 and the blood sample collection device 2004 as described herein.

[00123] FIG. 21 illustrates a non-vented blood sequestration device 2100 using a wicking material chamber. The blood sequestration device 2100 includes a housing 2101 that has a sampling channel 2104 that is at least partially surrounded or abutted by a sequestration chamber 2102 that is filled with a wicking material. An initial aliquot of blood is drawn in from the patient needle into the sampling channel 2104 where it is immediately wicked into the wicking material of the sequestration chamber 2102. The wicking material and/or sequestration chamber 2102 is sized and adapted to receive and hold a predetermined amount of blood, such that follow-on or later blood draws pass by the wicking material and flow straight through the sampling channel 2104 to a sampling device such as a Vacutainer. The wicking material can include a substance such as a solidifier, a decontaminate, or other additive.

[00124] As described herein, an air permeable blood barrier may be created using a wide variety of different structures and materials. As shown in FIGS. 22A and B, an air permeable blood barrier 2202 of a blood sequestration device 2200 can include a polymer bead matrix 2204, in which at least some beads are treated to make them hydrophilic. The air permeable blood barrier 2202 further includes a self-sealing material 2206, such as carboxymethyl cellulose (CMC) or cellulose gum, or other sealing material. The air permeable blood barrier 2202 can further include voids 2208 that permit air flow before contact or during partial contact with a fluid such as blood. As shown in FIG. 22B, contact with a fluid causes the self-sealing material 2206 to swell and close off the voids 2208, occluding air flow through the voids 2208 and creating a complete or partial seal.

[00125] FIGS. 23A and B illustrate yet another implementation of a blood sequestration device 2300, having an inlet port 2302 to connect with a patient needle, an outlet port 2304 to connect with a blood sample collection device, a sequestration chamber 2306, and a sampling channel 2308 that bypasses the sequestration chamber 2306 once the sequestration chamber is filled to an initial aliquot of potentially contaminated blood to be sequestered. The sequestration chamber 2306 includes a hydrophobic plug 2312 at a distal

end of the sequestration chamber 2306 that is farthest from the inlet port 2302. A vacuum or other drawing force applied from the outlet port 2304, such as from a Vacutainer or the like, draws in blood into the inlet port 2302 and directly into the sequestration chamber 2306, where the initial aliquot of blood will contact the hydrophobic plug 2312 and cause the initial aliquot of blood to back up into the sequestration chamber 2306 and be sequestered there. A small amount of blood may make its way into the sampling channel 2308, which is initially closed off by valve 2308. Upon release of the valve 2308, and under further force of the vacuum or other force, follow-on amounts of blood will flow into inlet port 2302, bypass the sequestration chamber 2306, and flow into and through sampling channel 2308 toward the outlet port 2304 and to the collection device.

[00126] The sampling channel 2308 can have any suitable geometry and can be formed of plastic tubing or any other suitable material. Valve 2308 can be a clip or other enclosing device to pinch, shunt, bend or otherwise close off the sampling channel before the initial aliquot of blood is sequestered in the sequestration chamber 2306.

[00127] Although a variety of embodiments have been described in detail above, other modifications are possible. Other embodiments may be within the scope of the following claims.

CLAIMS

1. A blood sequestration device comprising;

an inlet port;

an outlet port;

a sequestration chamber having a vent that includes an air permeable blood barrier; and

a sampling channel having a distal end connected with the outlet port;

each of the sequestration chamber and the sampling channel being connected with the inlet port via a junction that is sized and configured such that a first portion of blood flows into the sequestration chamber to displace air therein through the air permeable blood barrier and to be sequestered in the sequestration chamber, and a second portion of blood is allowed to bypass the sequestration chamber and the first portion of blood sequestered therein to be directed into the sampling channel toward the outlet port.

2. The blood sequestration device in accordance with claim 1, wherein the air permeable blood barrier includes an air permeable material that seals at least partially upon contact with blood.

3. The blood sequestration device in accordance with claim 1, further comprising a housing that defines a part of each of the inlet port, the outlet port, the sequestration chamber, and the sampling channel.

4. The blood sequestration device in accordance with claim 3, wherein the sequestration chamber includes a sequestration channel defined in the housing.

5. The blood sequestration device in accordance with claim 2, wherein the housing comprises a bottom member mated with a top member, each of the bottom

member and the top member defining a part of each of the inlet port, the outlet port, the sequestration chamber, and the sampling channel.

6. A blood sequestration device connected with a blood sampling pathway having a patient needle and a sample collection device, the blood sequestration device comprising:

an inlet port connected with the patient needle;

an outlet port connected with the sample collection device;

a sequestration chamber having a vent that includes an air permeable blood barrier; and

and a sampling channel having a distal end connected with the outlet port;

each of the sequestration chamber and the sampling channel being connected with the inlet port via a junction that is sized and configured such that a first portion of blood flows into the sequestration chamber to displace air therein through the air permeable blood barrier and to be sequestered in the sequestration chamber, and a second portion of blood is allowed to bypass the sequestration chamber and the first portion of blood sequestered therein to be directed into the sampling channel toward the outlet port and the sample collection device.

7. The blood sequestration device in accordance with claim 6, further comprising a housing that houses and defines the inlet port, the outlet port, the sequestration chamber, and the sampling channel.

8. The blood sequestration device in accordance with claim 6, wherein the inlet port is connected with the patient needle via a first portion of the blood sampling pathway.

9. The blood sequestration device in accordance with claim 6, wherein the outlet port is connected with the sample collection device via a second portion of the blood sampling pathway.

10. The blood sequestration device in accordance with claim 6, wherein the air permeable blood barrier includes an air permeable material that seals at least partially upon contact with blood.

11. The blood sequestration device in accordance with claim 7, wherein the sequestration chamber includes a sequestration channel defined in the housing.

12. The blood sequestration device in accordance with claim 11, wherein the sequestration channel has a proximal end connected with the inlet port, and a distal end having the vent comprising an air permeable blood barrier.

13. A bodily fluid sequestration device comprising;

an inlet port;

an outlet port connected with the inlet port;

a sequestration chamber connected with the inlet port via a junction, the sequestration chamber having a vent that includes an air permeable bodily fluid barrier; and

a housing that houses and defines the inlet port, the outlet port, and the sequestration chamber, the sequestration chamber and the junction configured to direct a first portion of bodily fluid from the inlet port into the sequestration chamber toward the air permeable bodily fluid barrier, the air permeable bodily fluid barrier including an air permeable material that forms a barrier to bodily fluids upon contact with the bodily fluids,

whereupon formation of the barrier enables sequestration of the first portion of bodily fluid in the sequestration chamber, and enables a second portion of bodily fluid from the inlet port to bypass the sequestration chamber via the junction and the first portion of bodily fluid, toward the outlet port.

14. The bodily fluid sequestration device in accordance with claim 13, wherein the air permeable bodily fluid barrier includes an air permeable material that seals upon contact with the bodily fluids.

15. The bodily fluid sequestration device in accordance with claim 13, wherein the sequestration chamber includes a sequestration channel defined in the housing.

16. The bodily fluid sequestration device in accordance with claim 13, further comprising a sampling pathway connected with the inlet port, wherein the sampling pathway conveys the second portion of bodily fluid from the inlet port to the outlet port via the junction.

17. The bodily fluid sequestration device in accordance with claim 13, wherein the housing comprises a bottom member mated with a top member, each of the bottom member and the top member defining a part of each of the inlet port, the outlet port, and the sequestration chamber.

18. The bodily fluid sequestration device in accordance with claim 13, further comprising a sampling channel having a proximal end connected with the inlet port via the junction.

19. The blood sequestration device in accordance with claim 18, wherein the housing comprises a bottom member mated with a top member, each of the bottom member and the top member defining a part of each of the inlet port, the outlet port, the sequestration chamber, and the sampling channel.

20. A blood sequestration system comprising:

a blood sampling pathway having a patient needle and a sample collection device; and

a blood sequestration device, the blood sequestration device comprising:

an inlet port connected with the patient needle;

an outlet port connected with the sample collection device;

a sequestration chamber having a vent that includes an air permeable blood barrier; and

and a sampling channel having a distal end connected with the outlet port;

each of the sequestration chamber and the sampling channel being connected with the inlet port via a junction that is sized and configured such that a first portion of blood flows into the sequestration chamber to displace air therein through the air permeable blood barrier and to be sequestered in the sequestration chamber, and a second portion of blood is allowed to bypass the sequestration chamber and the first portion of blood sequestered therein to be directed into the sampling channel toward the outlet port and the sample collection device.

21. The blood sequestration system in accordance with claim 20, further comprising a housing that houses and defines the inlet port, the outlet port, the sequestration chamber, and the sampling channel.

22. The blood sequestration system in accordance with claim 20, wherein the inlet port is connected with the patient needle via a first portion of the blood sampling pathway.

23. The blood sequestration system in accordance with claim 20, wherein the outlet port is connected with the sample collection device via a second portion of the blood sampling pathway.

24. The blood sequestration system in accordance with claim 20, wherein the air permeable blood barrier includes an air permeable material that seals at least partially upon contact with blood.

25. The blood sequestration system in accordance with claim 24, wherein the sequestration chamber includes a sequestration channel defined in the housing.

26. The blood sequestration device in accordance with claim 25, wherein the sequestration channel has a proximal end connected with the inlet port, and a distal end having the vent comprising an air permeable blood barrier.

ABSTRACT

Blood sample optimization systems and methods are described that reduce or eliminate contaminates in collected blood samples, which in turn reduces or eliminates false positive readings in blood cultures or other testing of collected blood samples. A blood sample optimization system can include a blood sequestration device located between a patient needle and a sample needle. The blood sequestration device can include a sequestration chamber for sequestering an initial, potentially contaminated aliquot of blood, and may further include a sampling channel that bypasses the sequestration chamber to convey likely uncontaminated blood between the patient needle and the sample needle after the initial aliquot of blood is sequestered in the sequestration chamber.

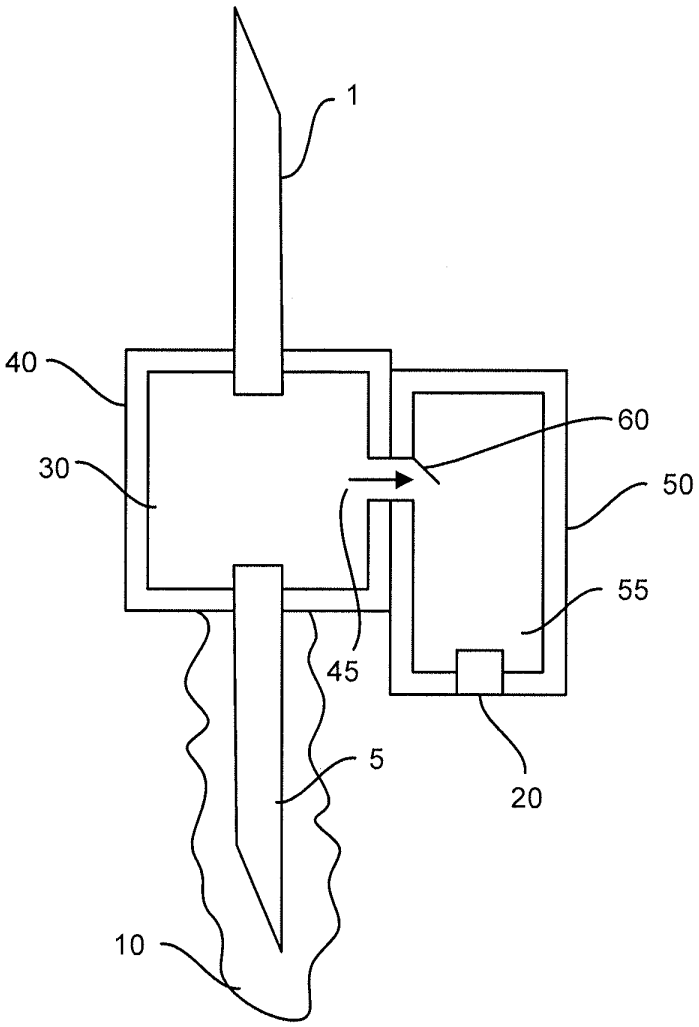


FIG. 1

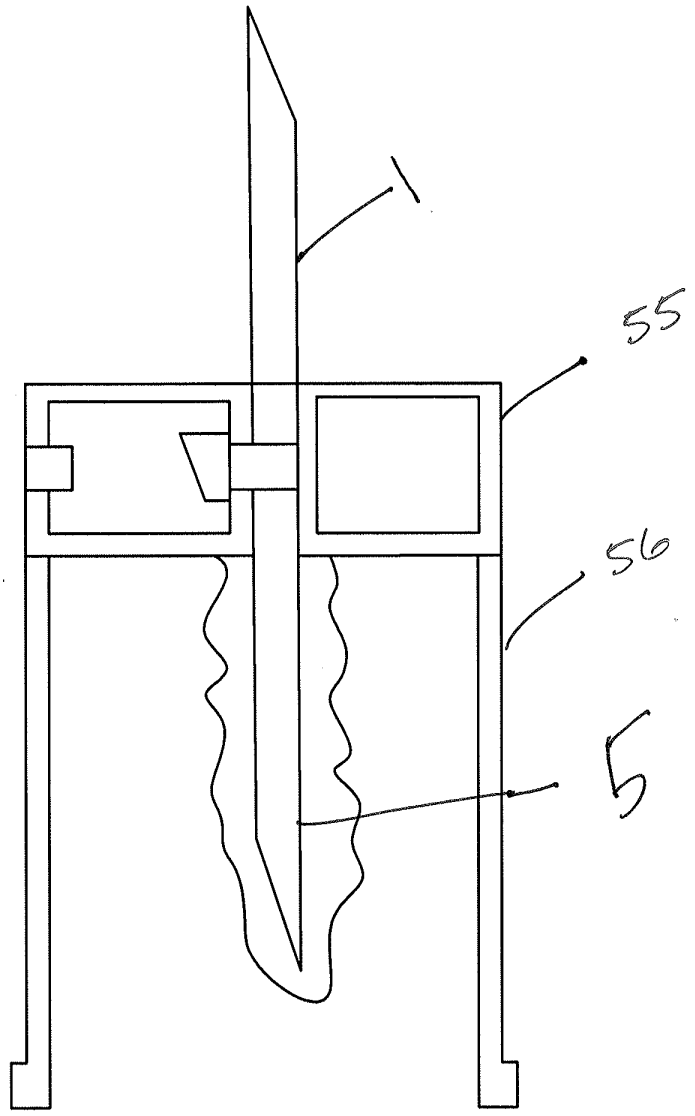


FIG. 2

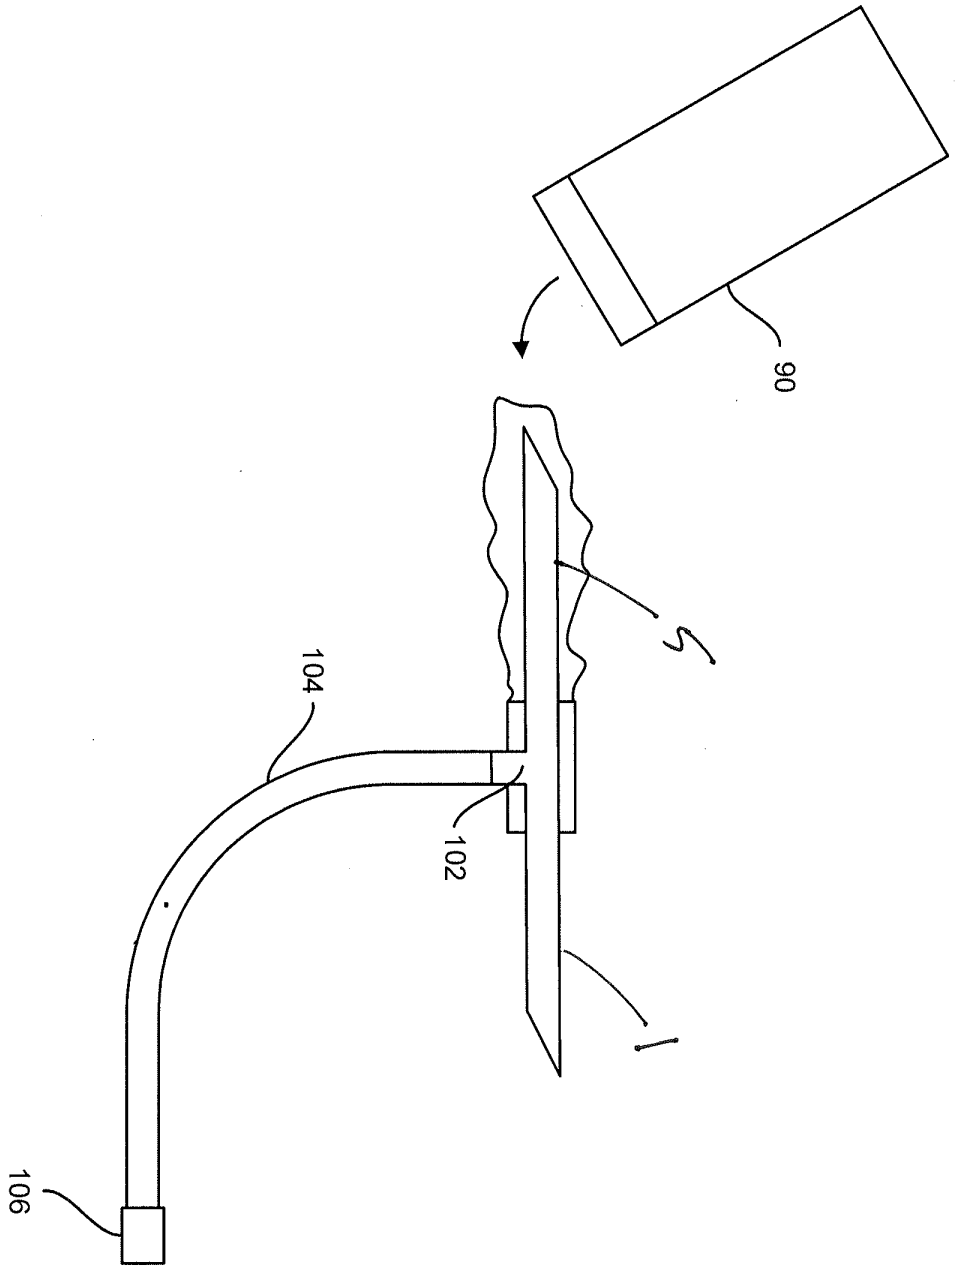


FIG. 3

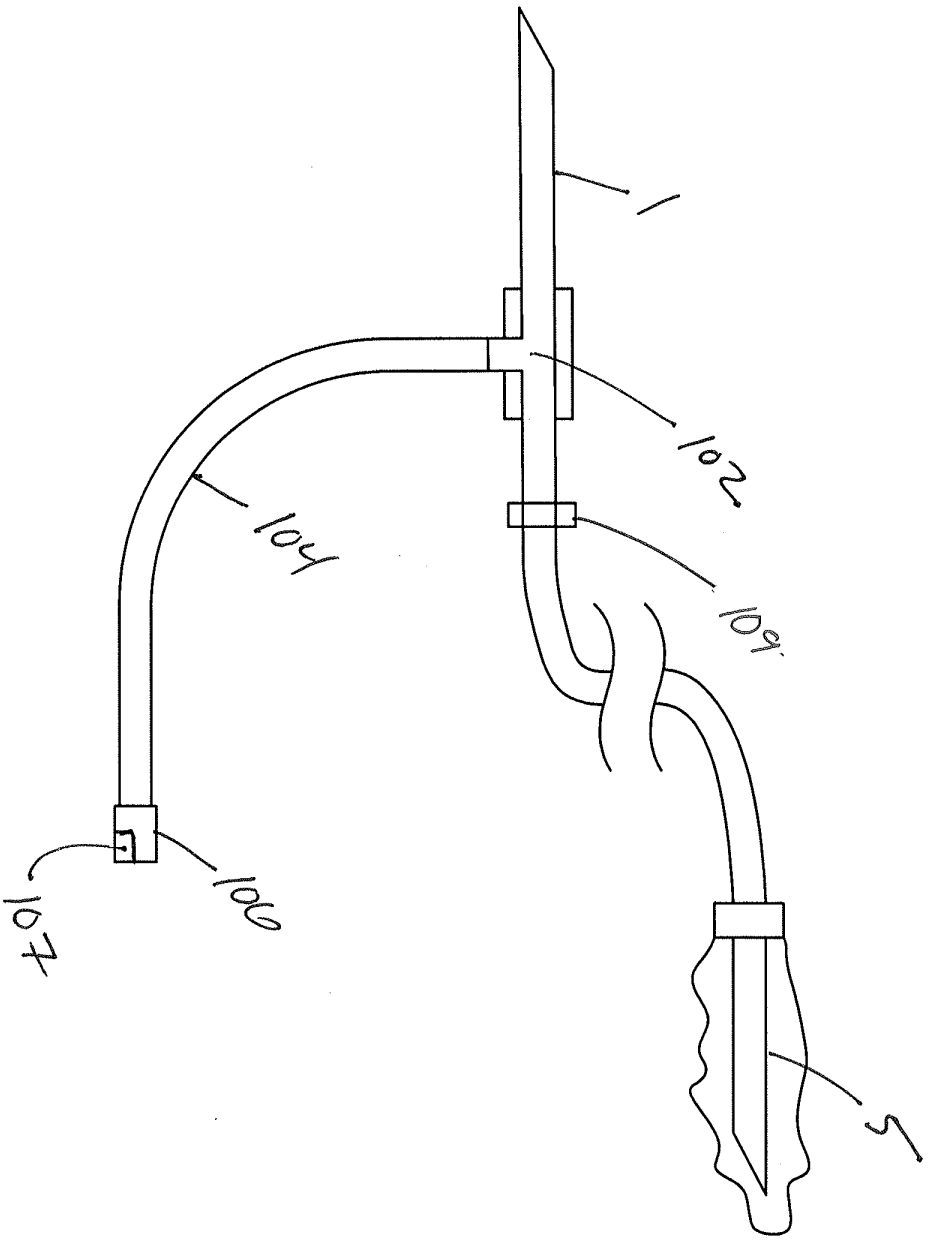


FIG. 4

FIG. 5


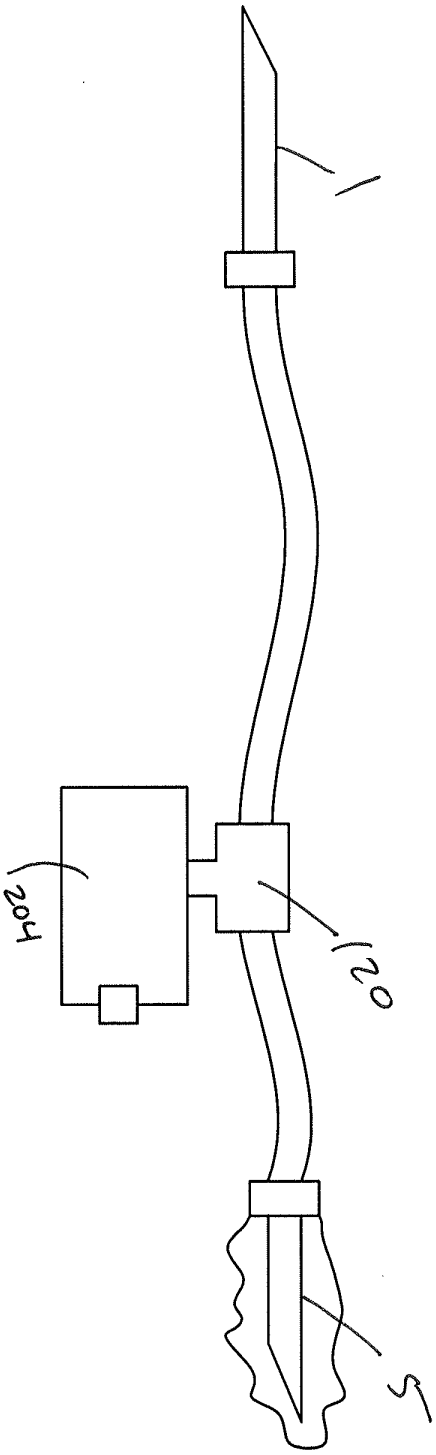


FIG. 6

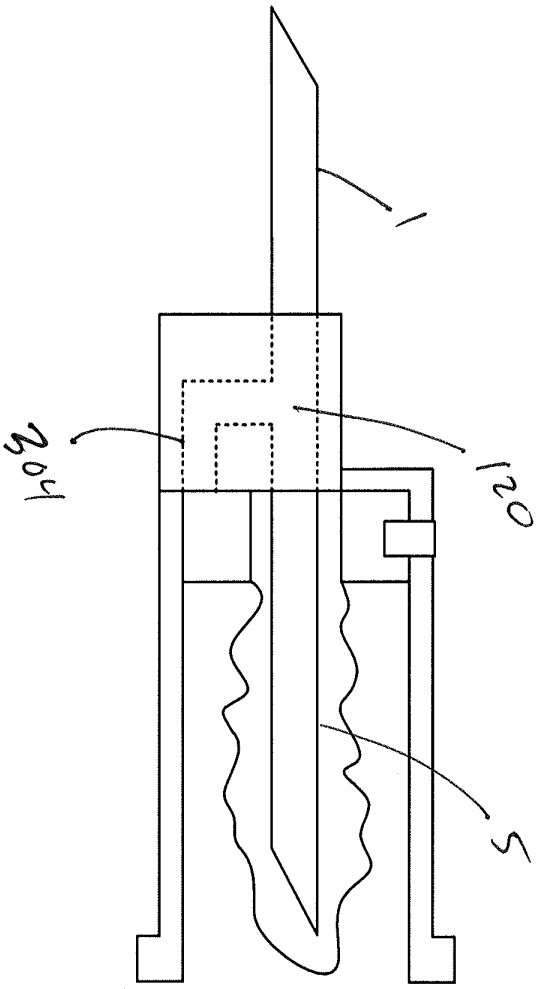

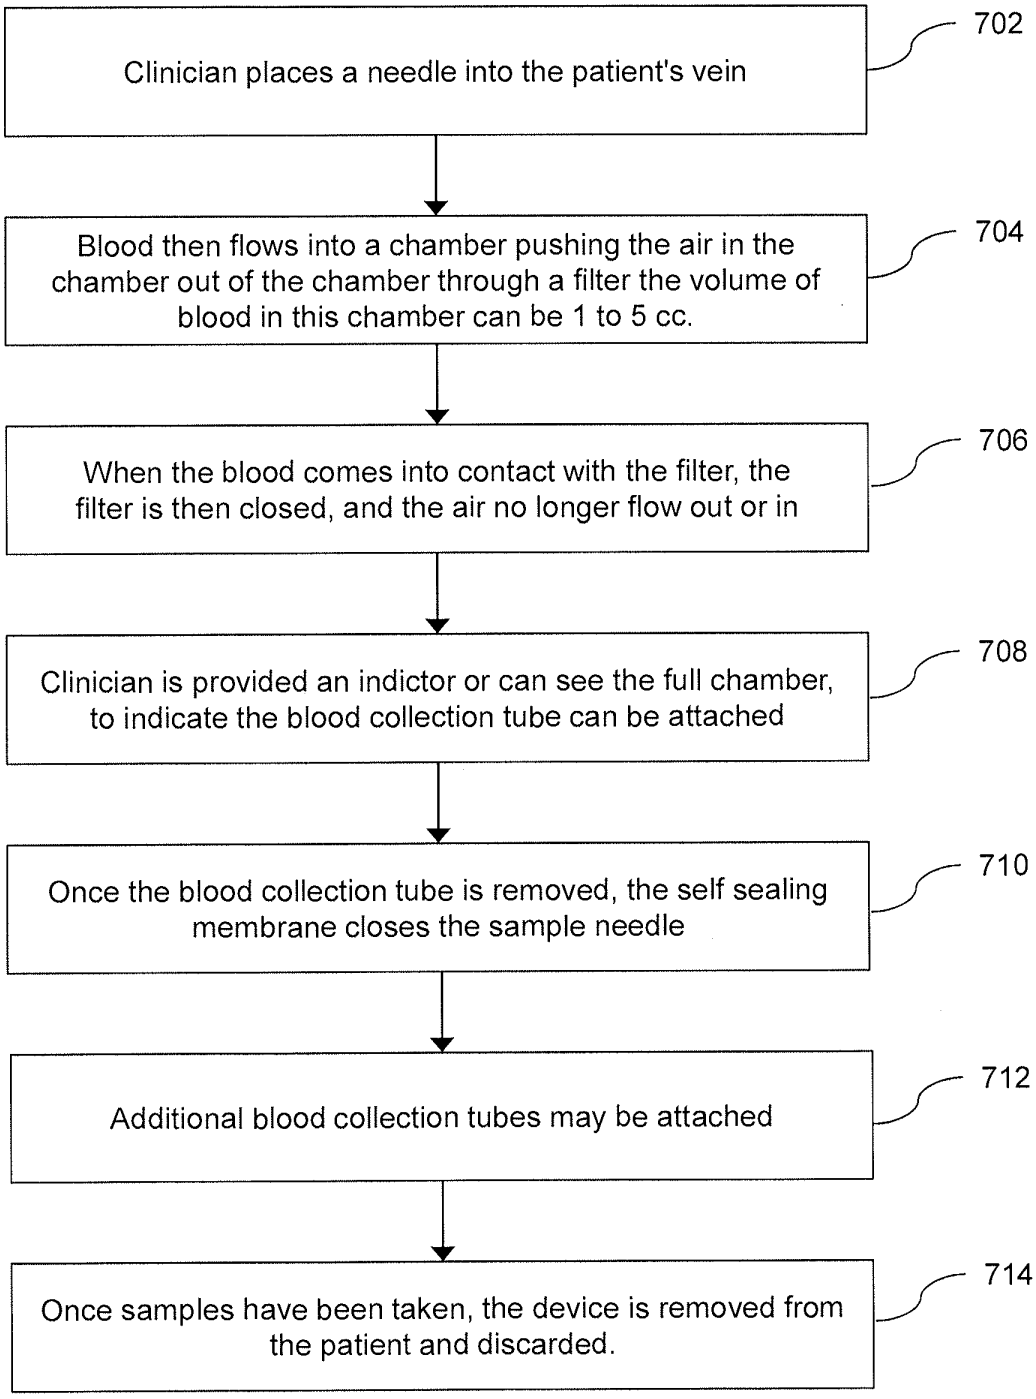

Clinician places a needle into the patient's vein
702
Blood then flows into a chamber pushing the air in the chamber out of the chamber through a filter the volume of blood in this chamber can be 1 to 5 cc.
704
When the blood comes into contact with the filter, the filter is then closed, and the air no longer flow out or in
706
Clinician is provided an indictor or can see the full chamber, to indicate the blood collection tube can be attached
708
Once the blood collection tube is removed, the self sealing membrane closes the sample needle
710
Additional blood collection tubes may be attached
712
Once samples have been taken, the device is removed from the patient and discarded.
714

FIG. 7

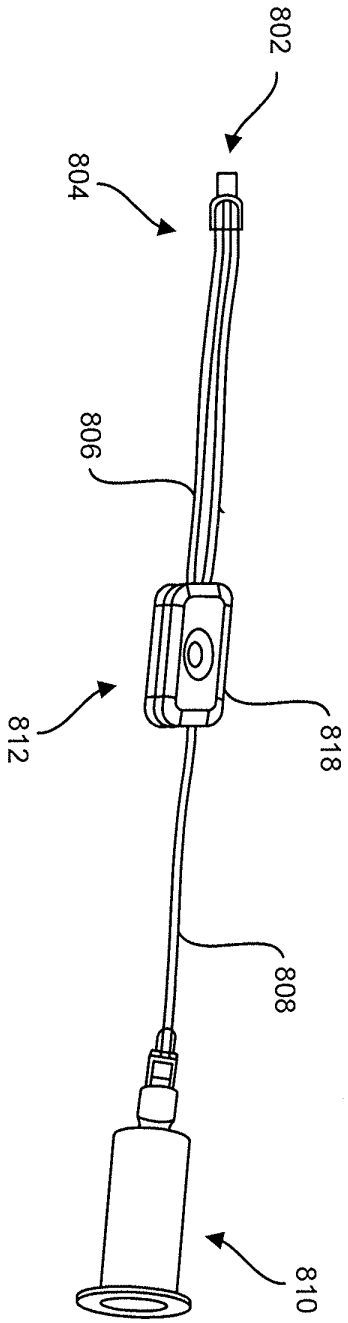


FIG. 8A

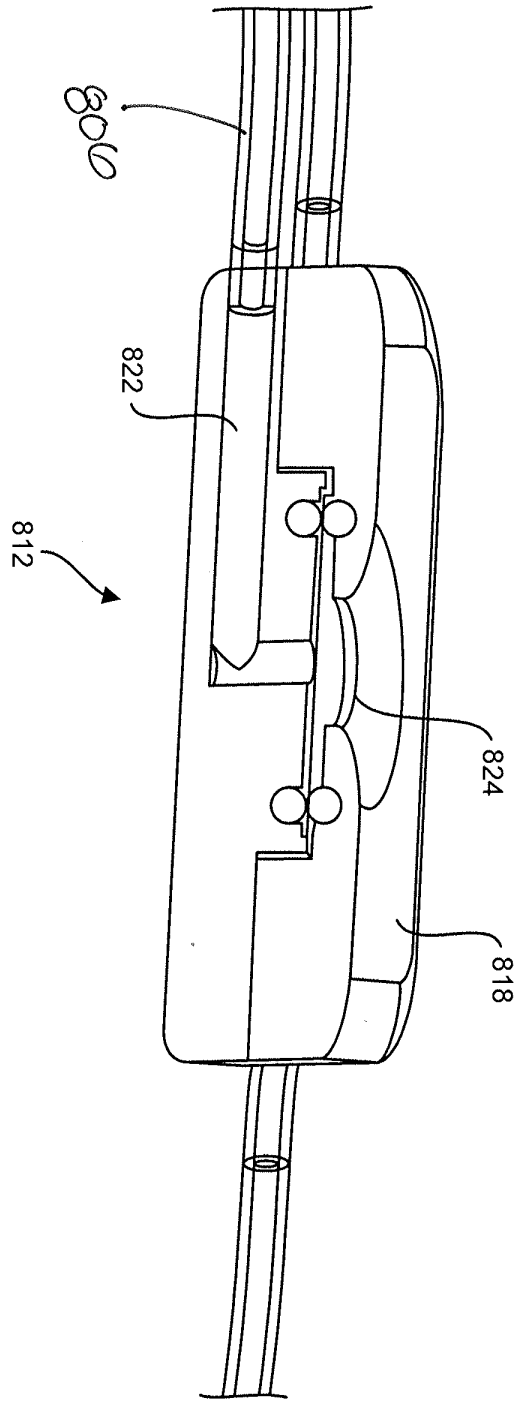


FIG. 8B

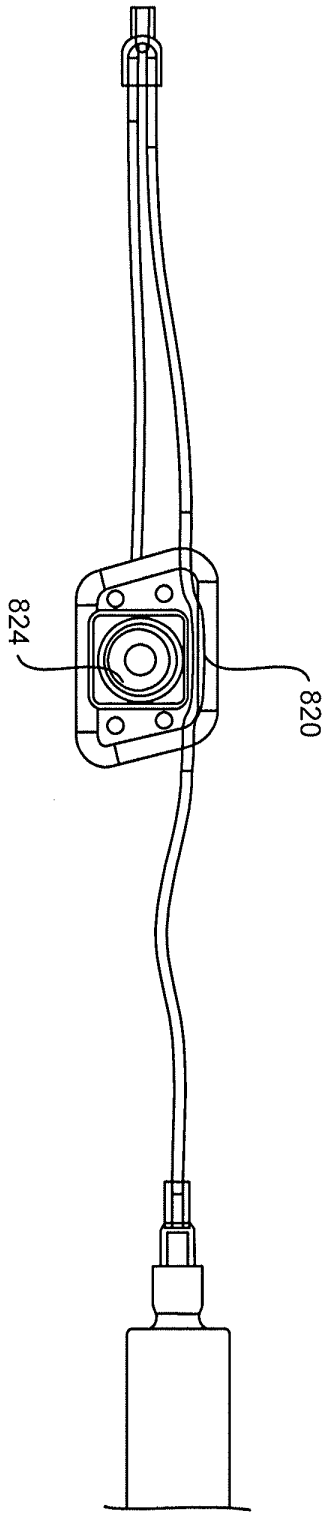


FIG. 8C

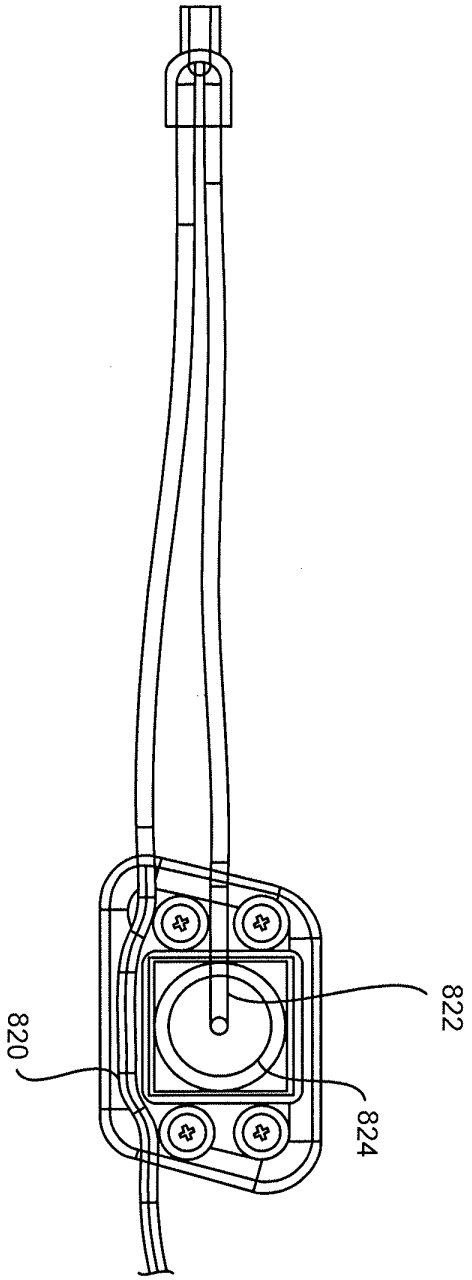


FIG. 8D

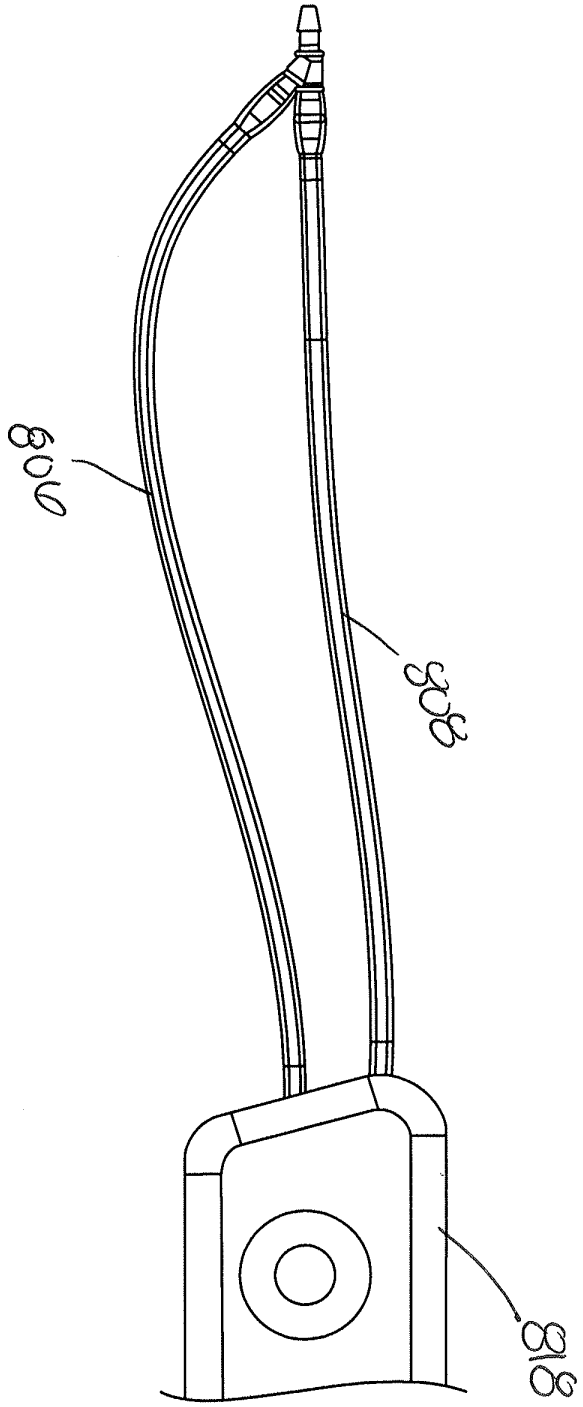
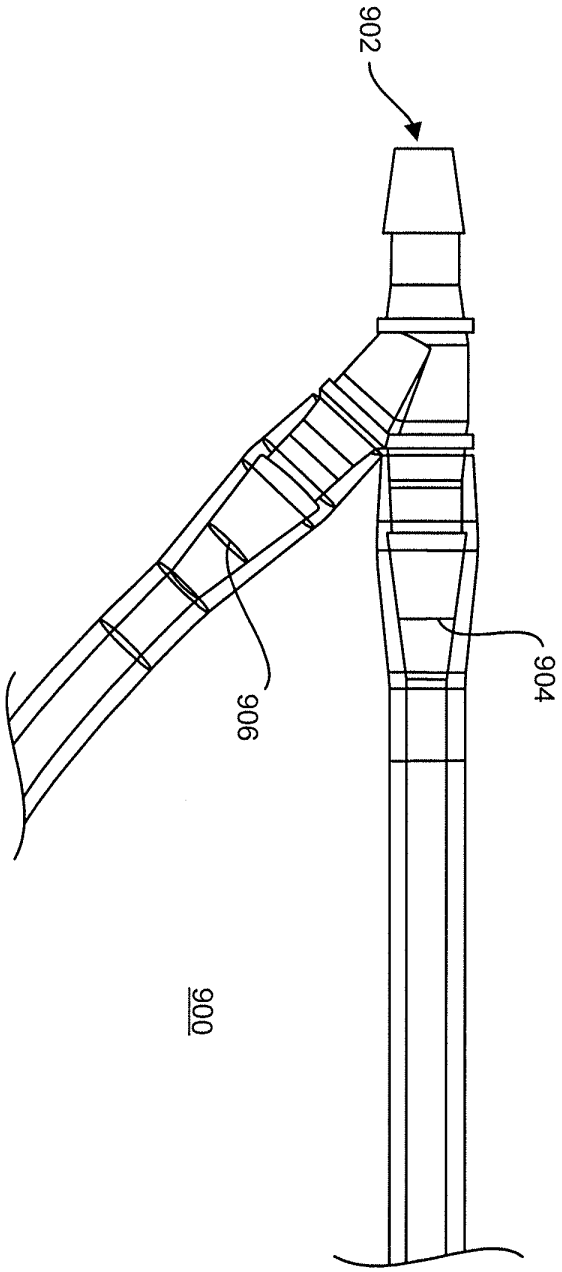


FIG. 8E

FIG. 9



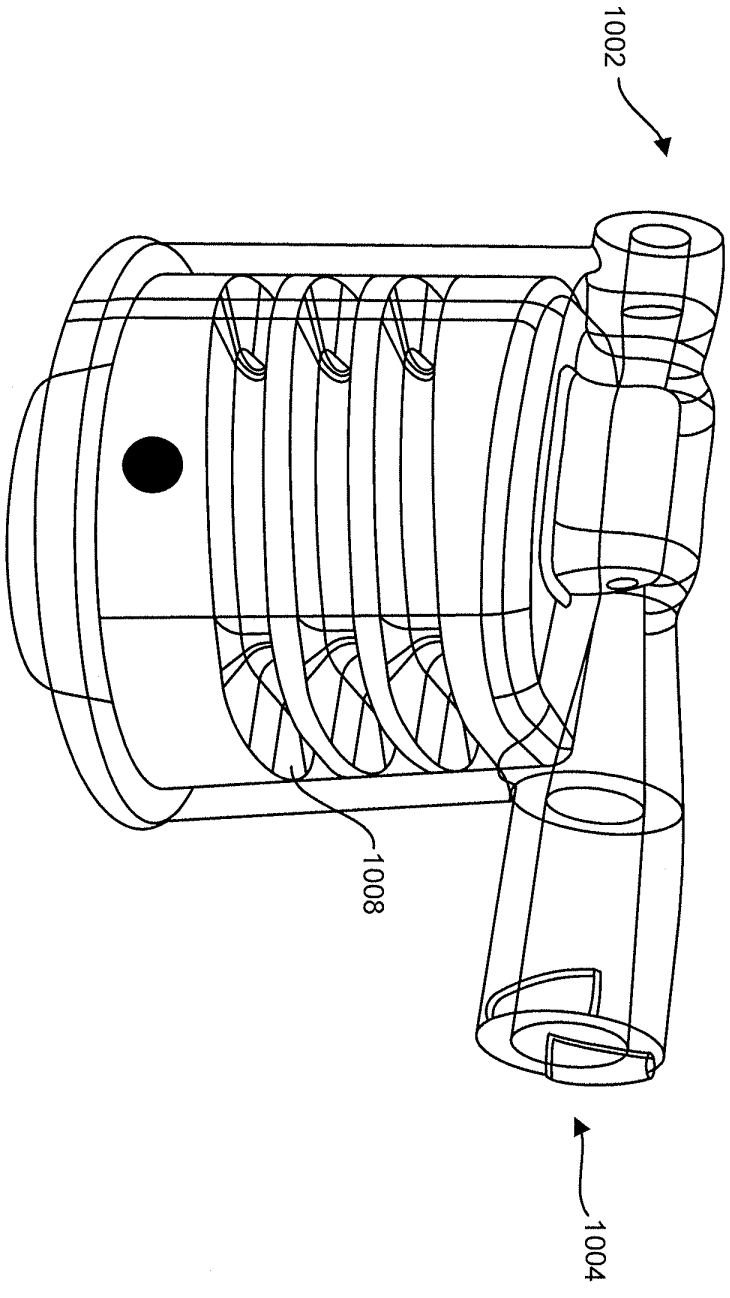


FIG. 10A

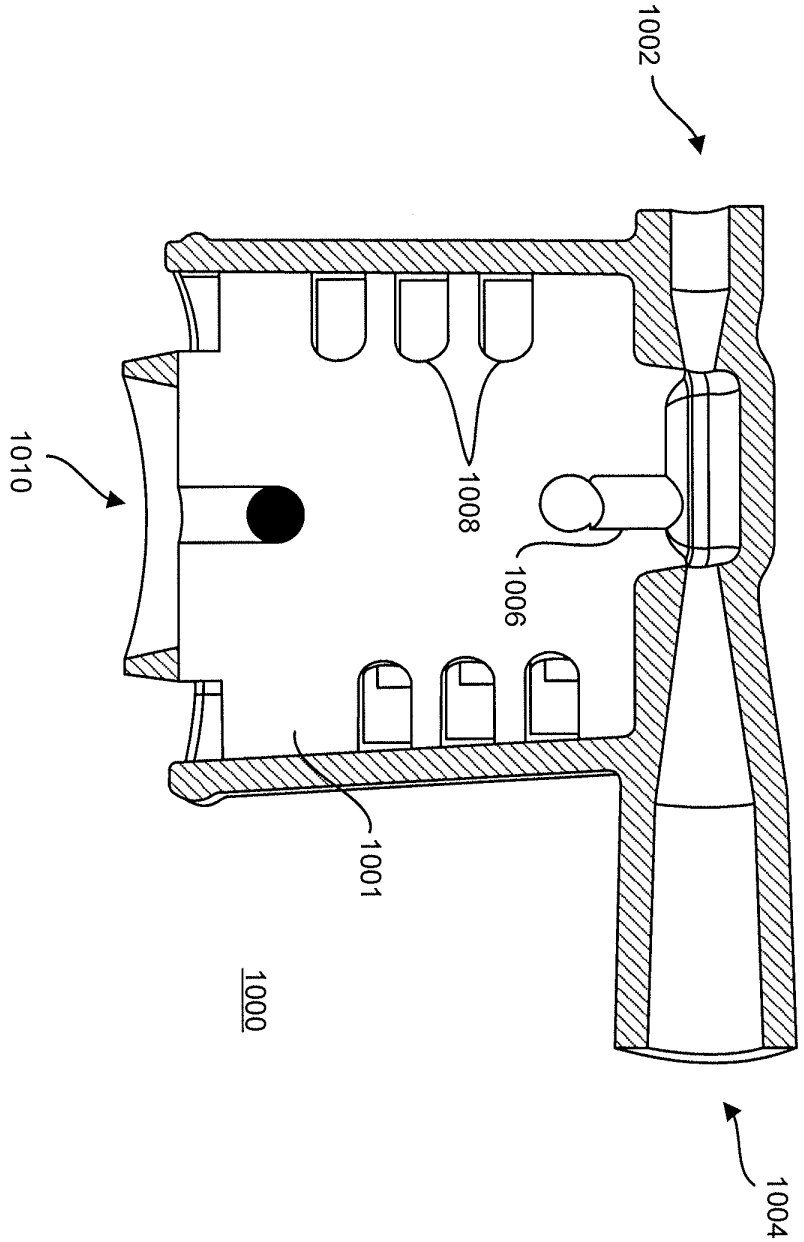


FIG. 10B

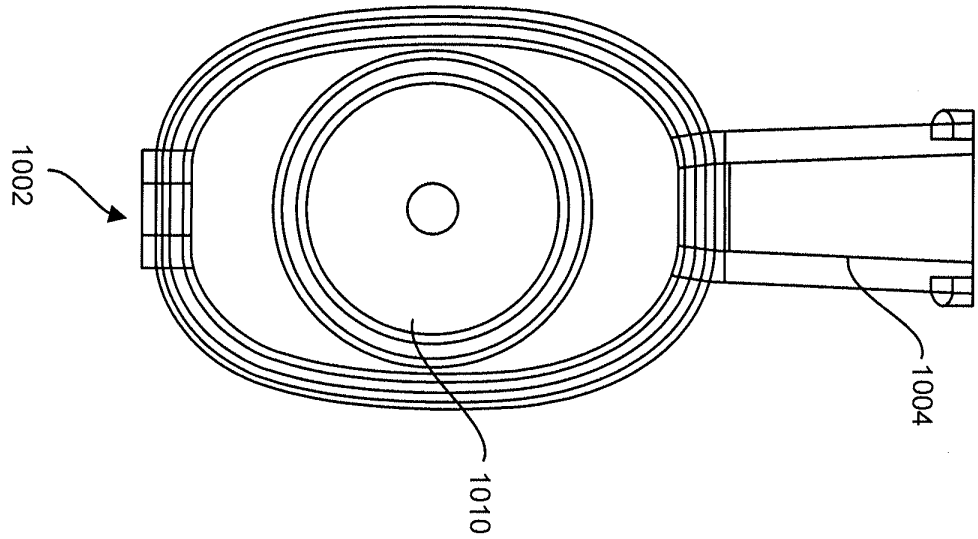
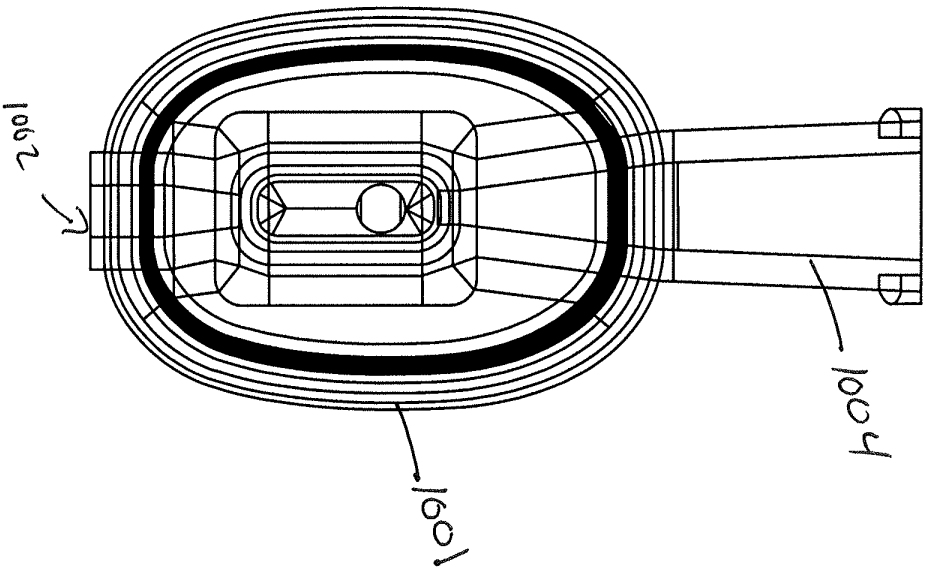


FIG. 10C

FIG. 10D



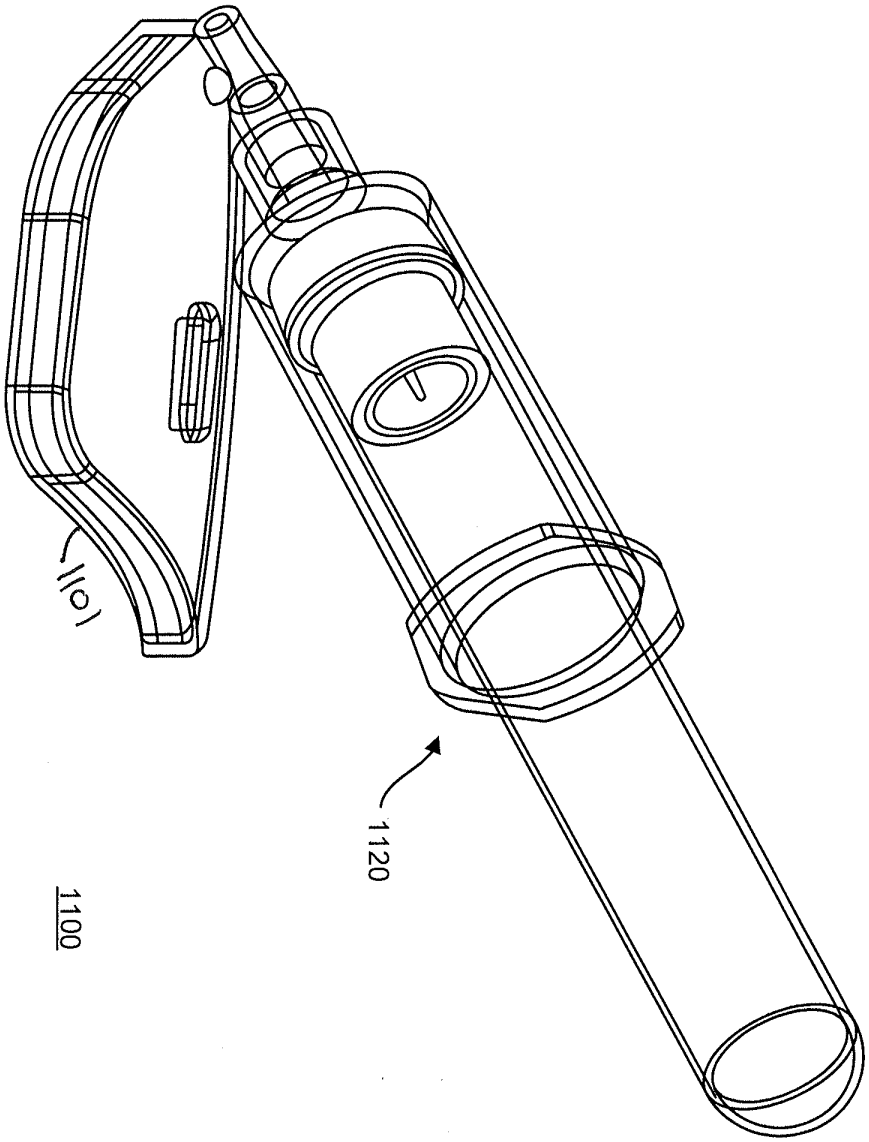


FIG. 11A

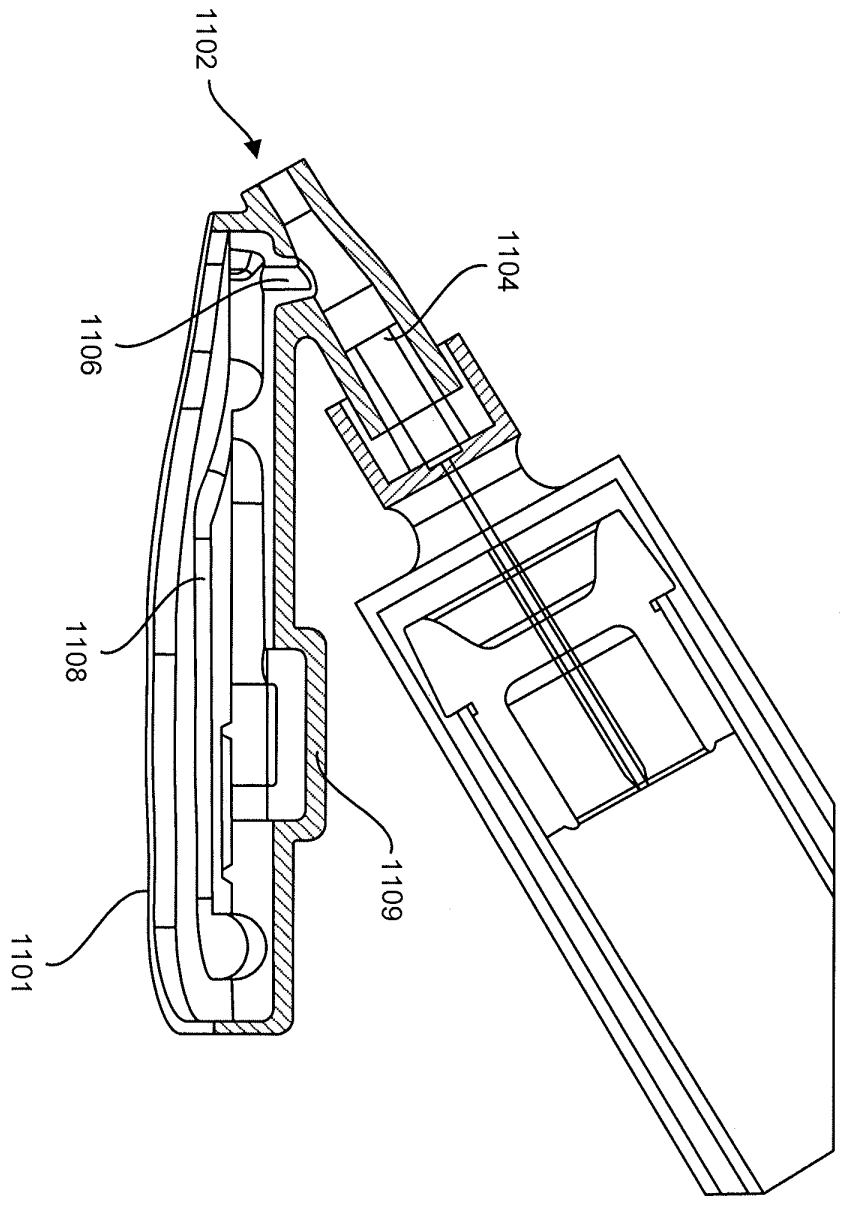


FIG. 11B

FIG. 11C

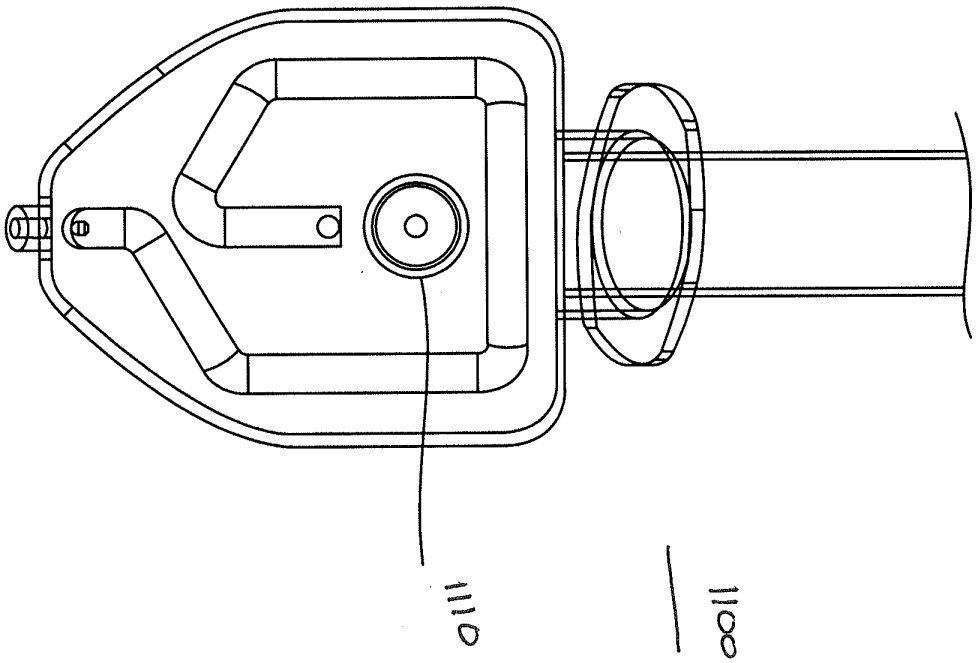
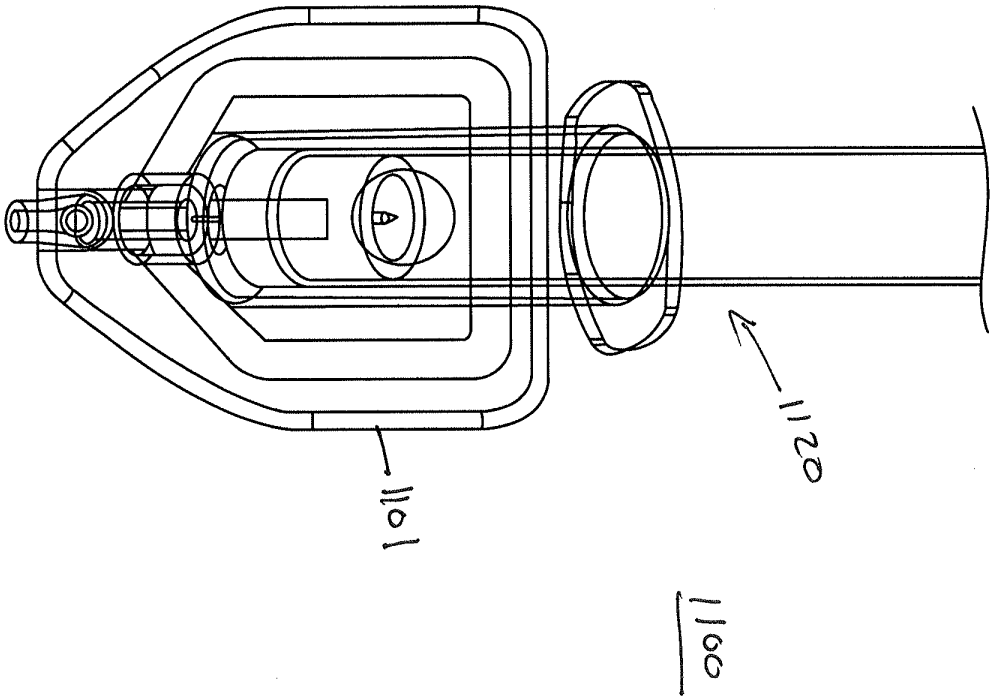


FIG. 11D



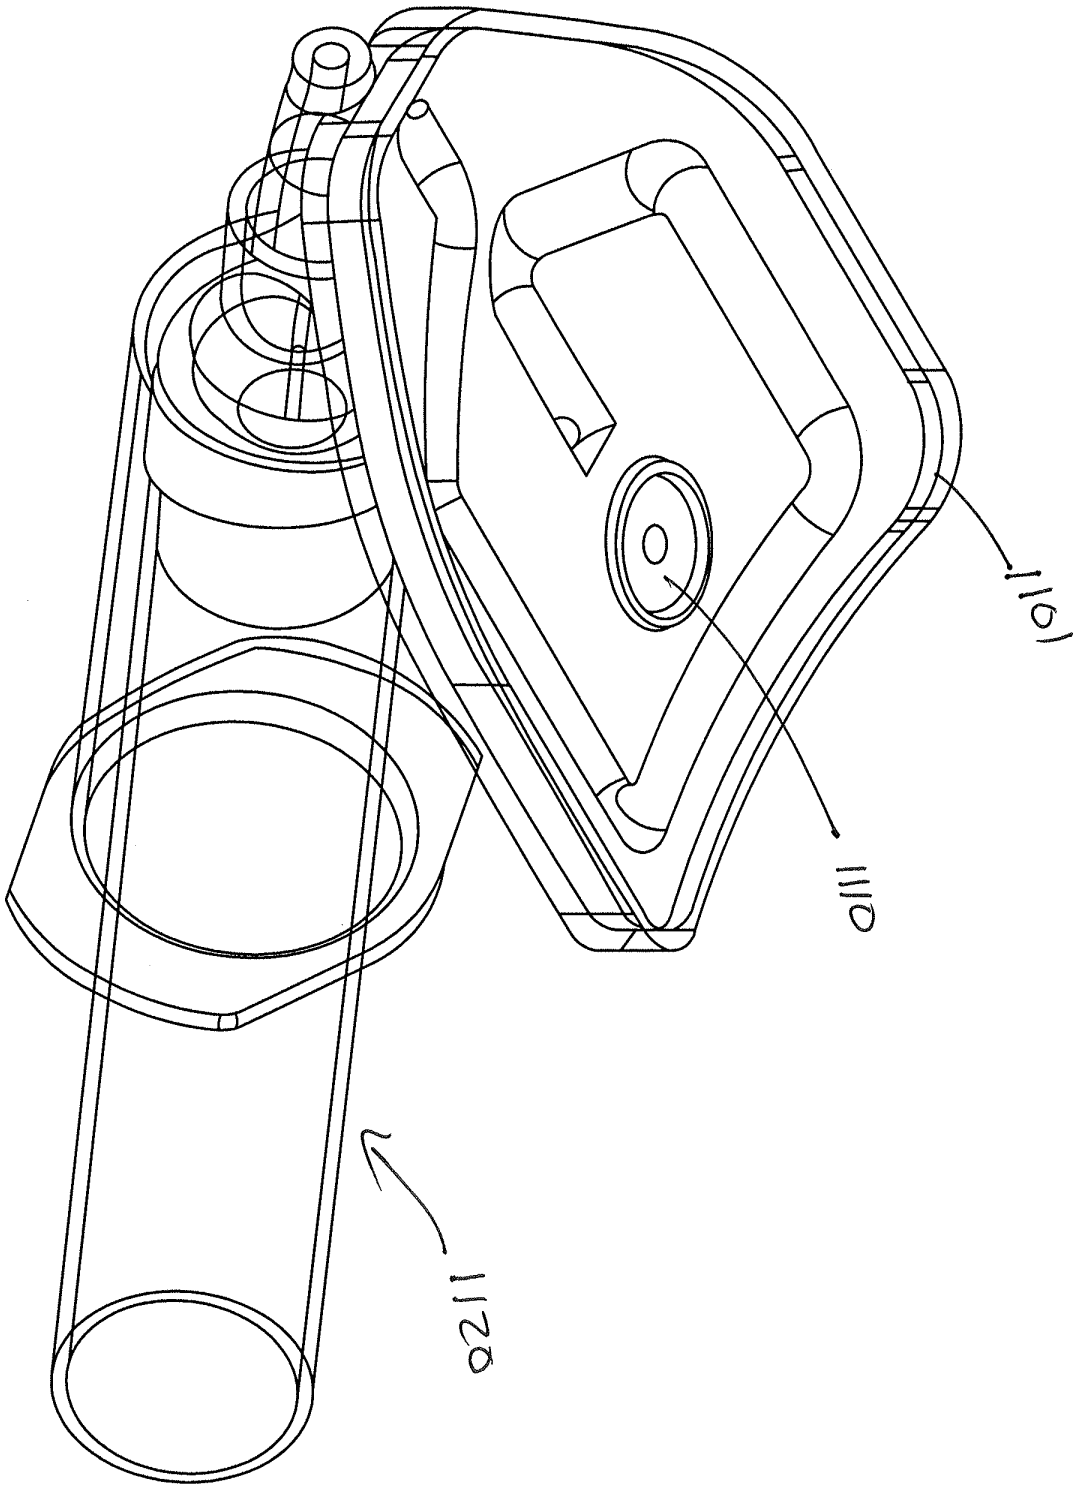


FIG. 11E

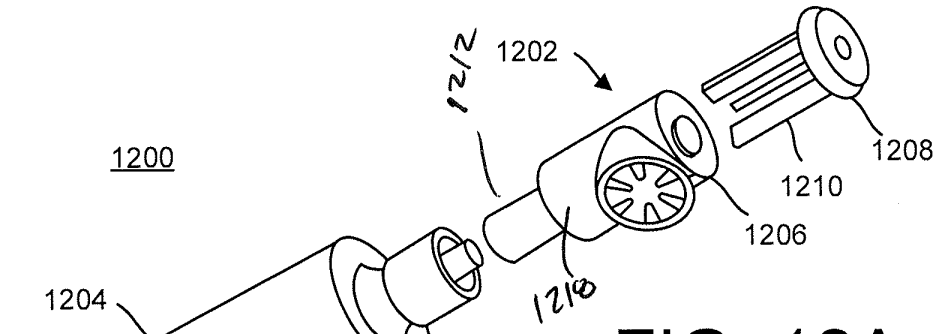


FIG. 12A

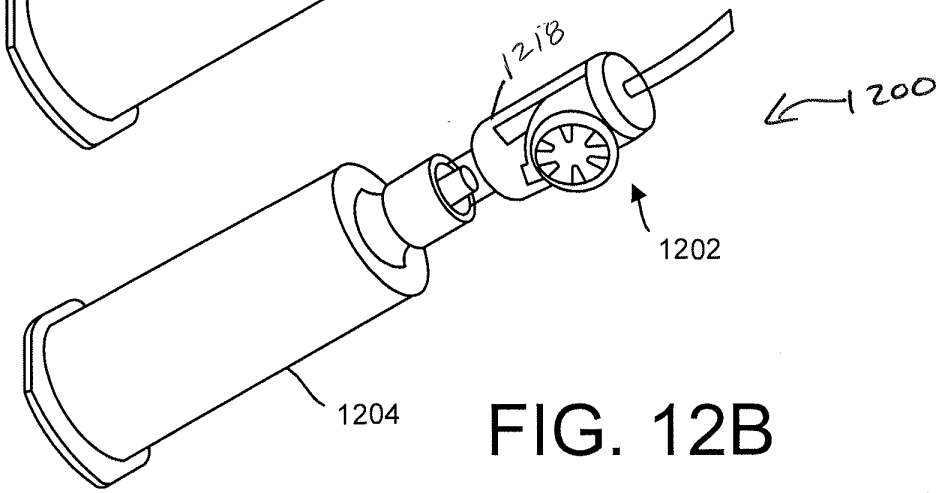


FIG. 12B

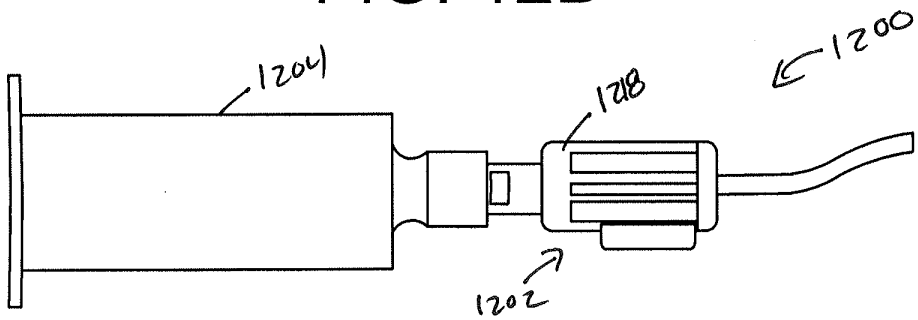


FIG. 12C

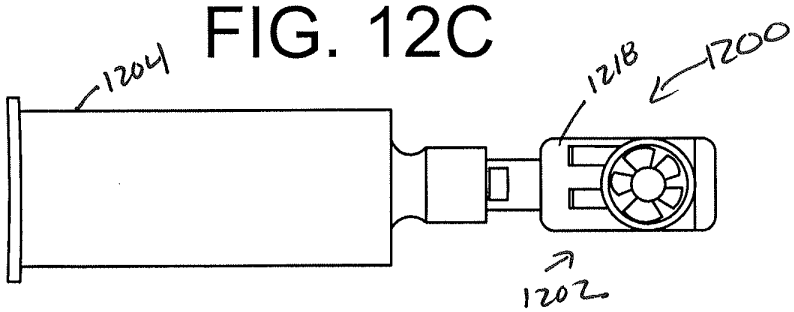


FIG. 12D

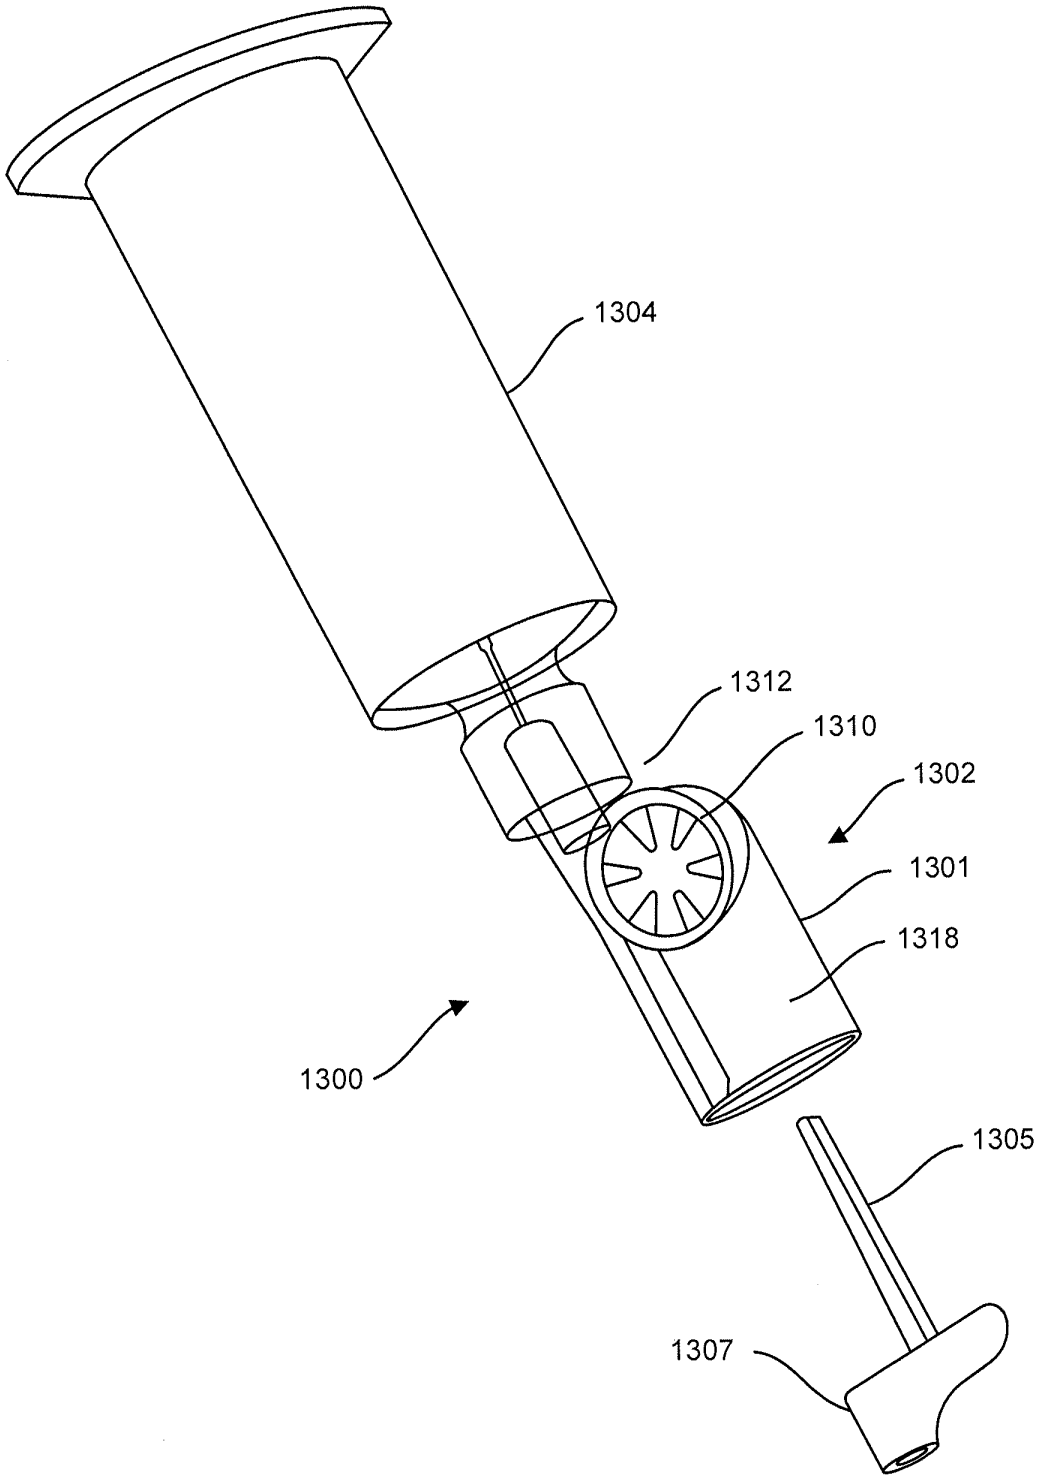


FIG. 13A

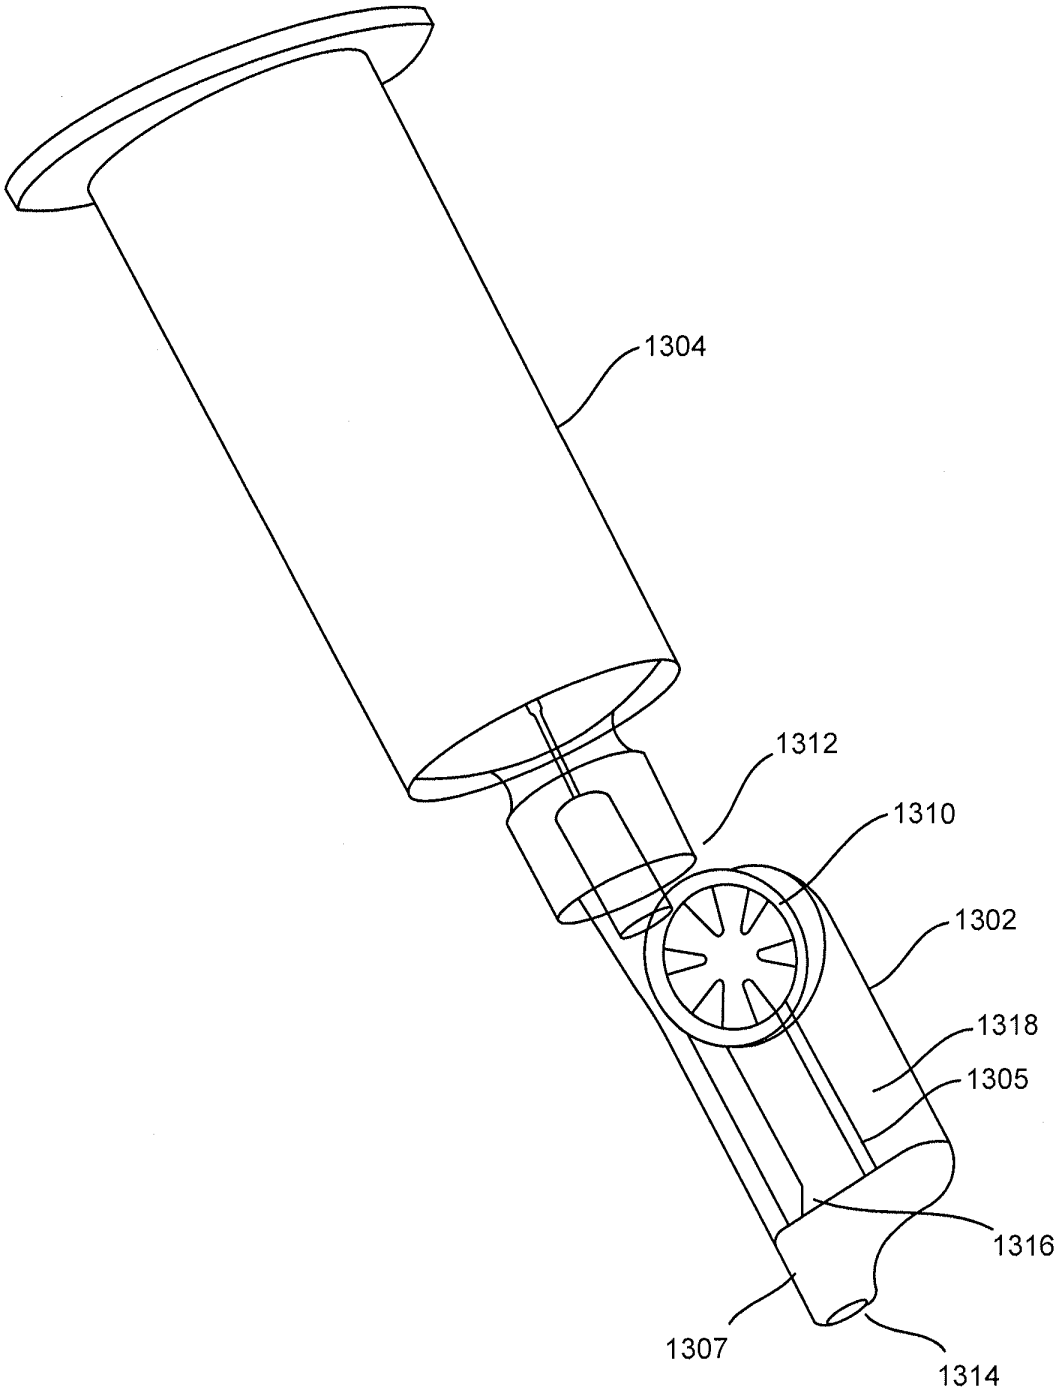


FIG. 13B

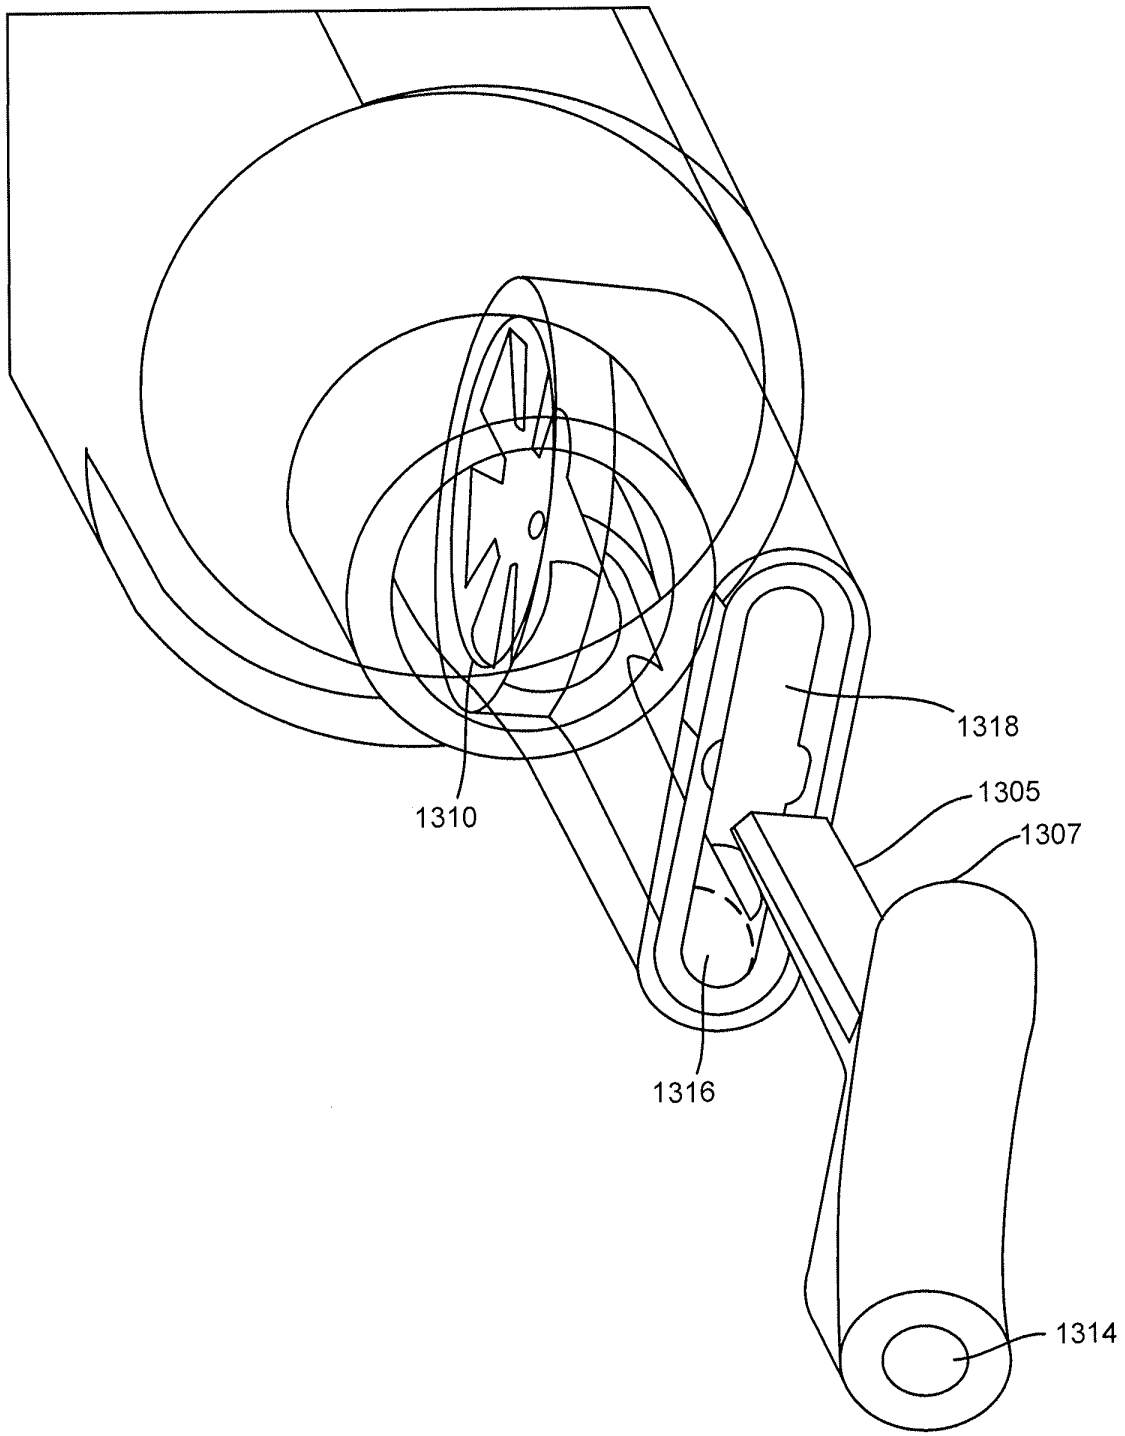


FIG. 13C

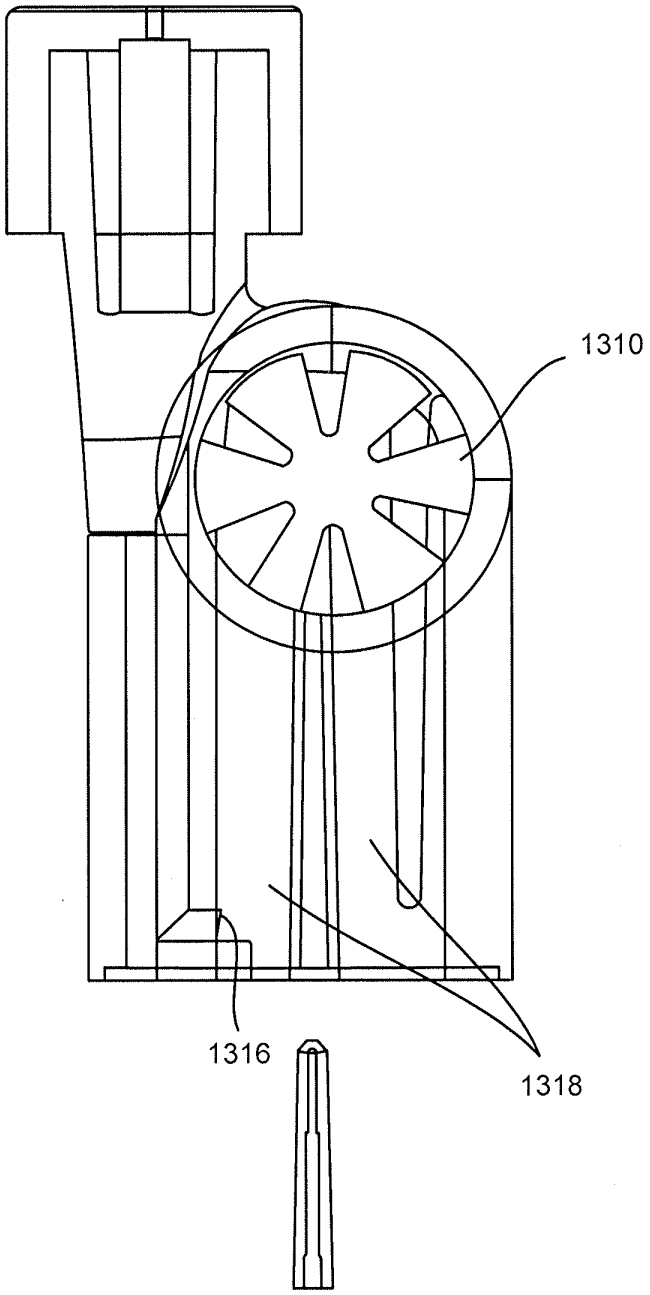


FIG. 13D

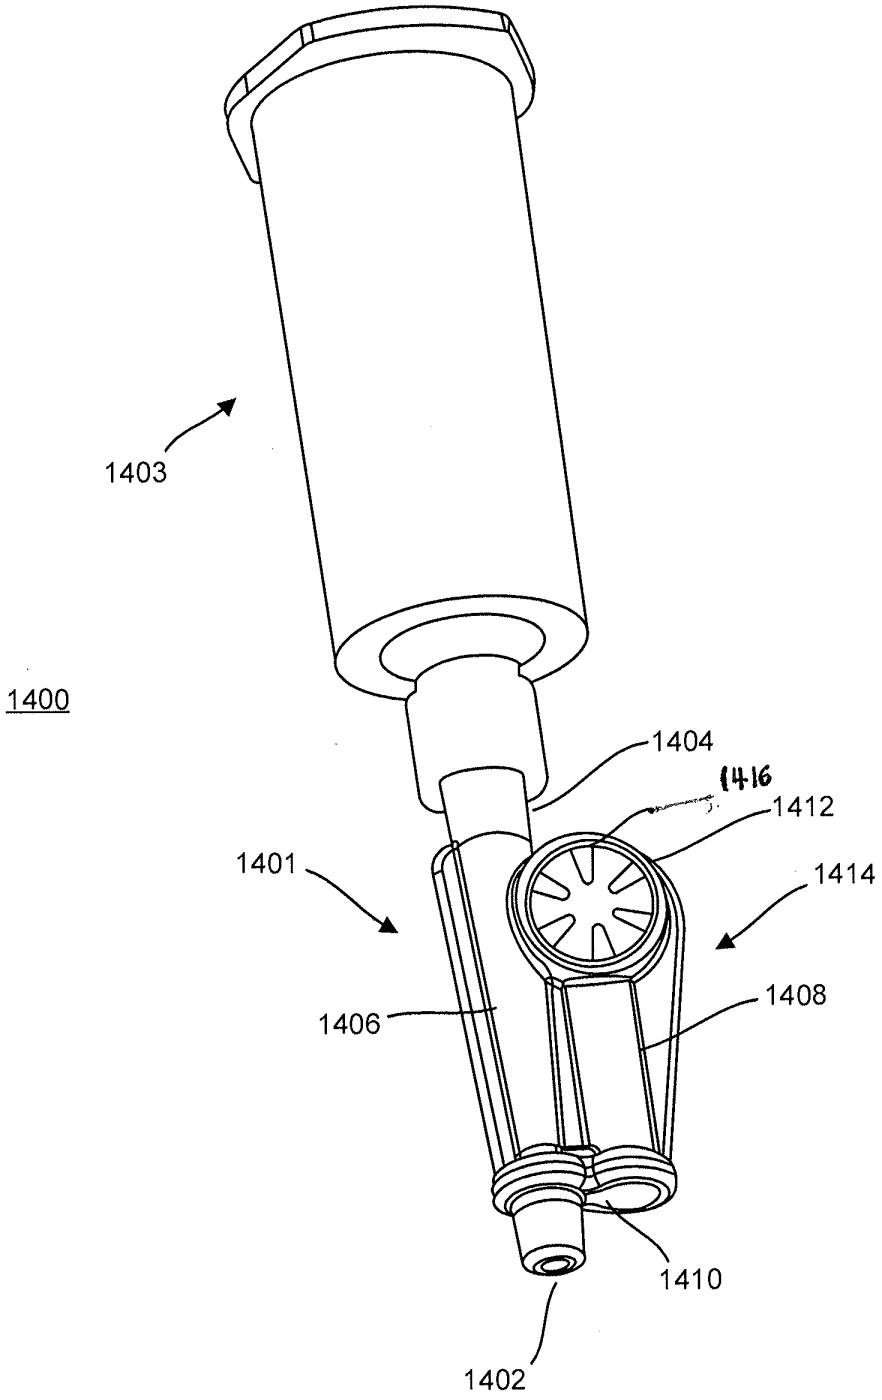


FIG. 14A

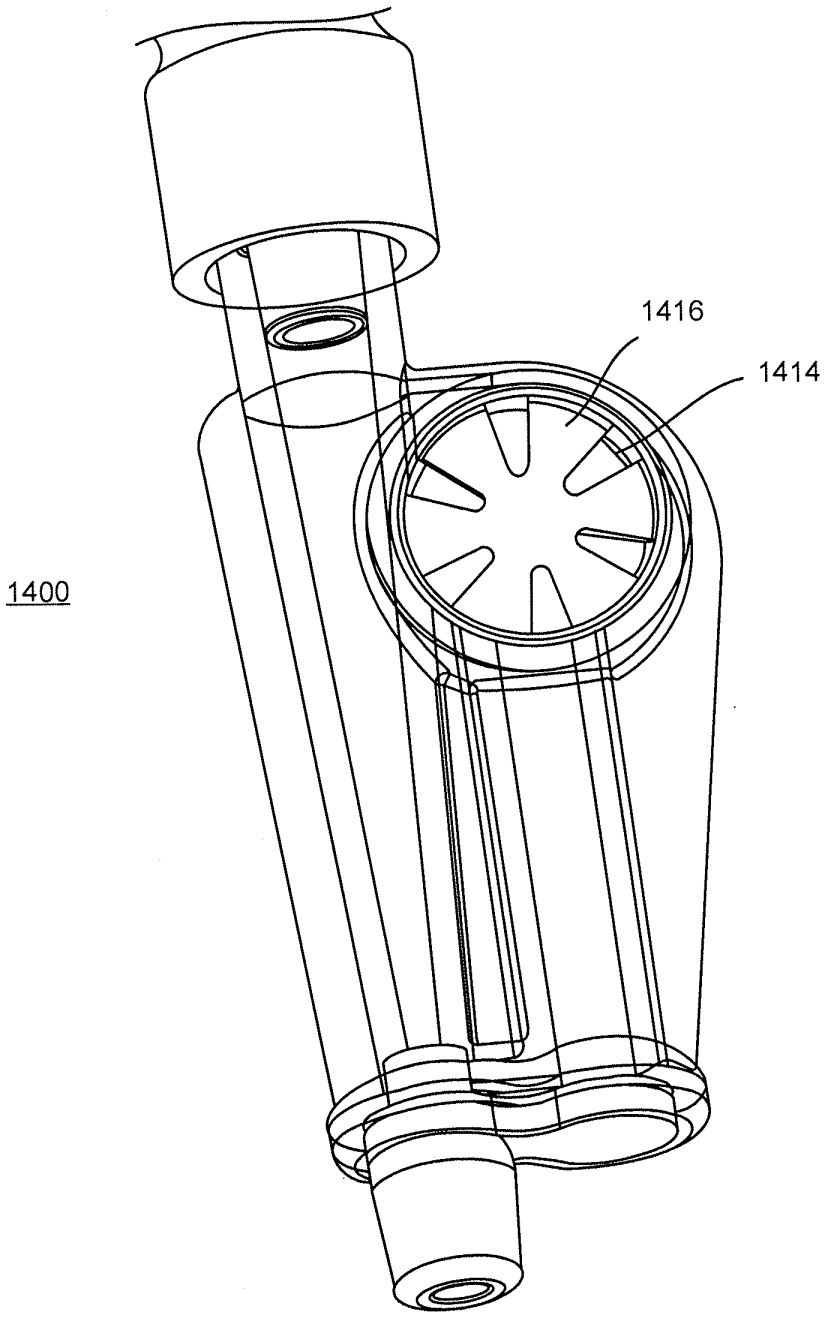


FIG. 14B

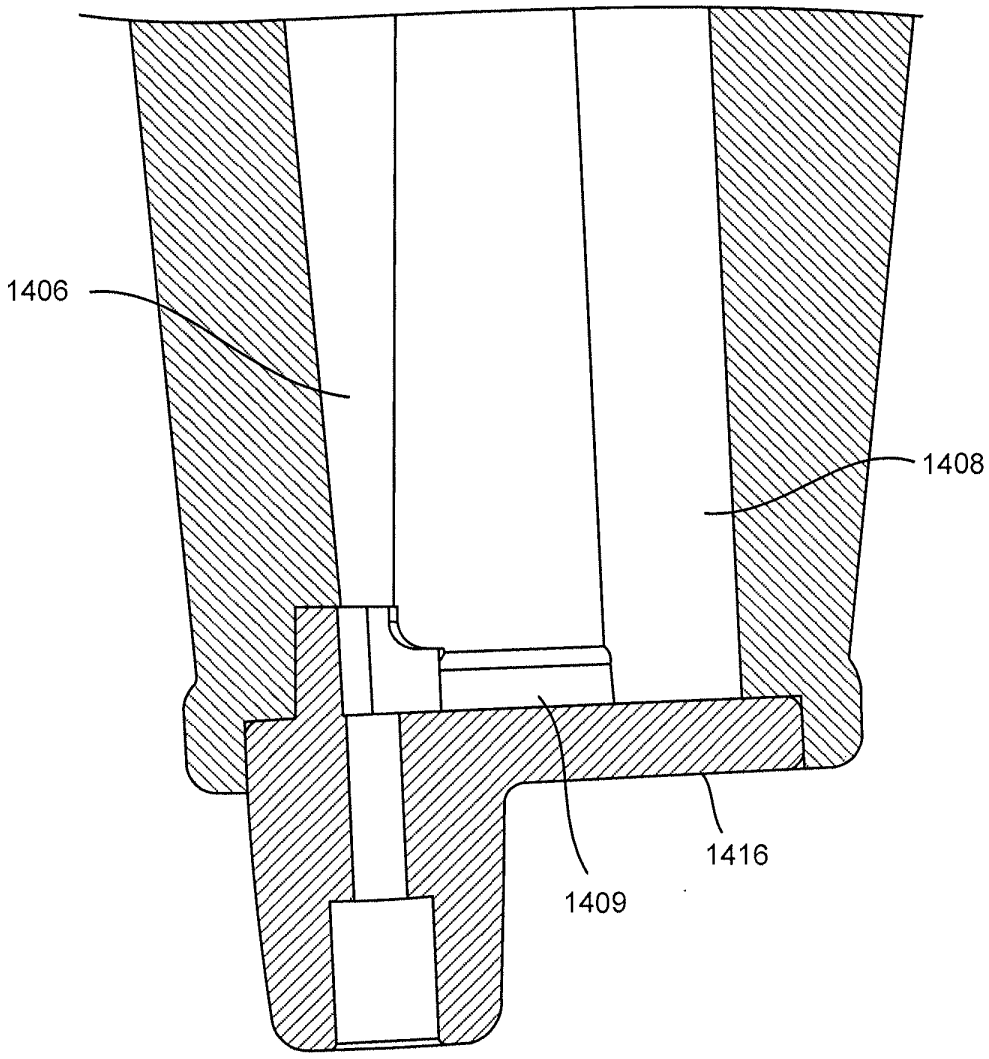


FIG. 14C

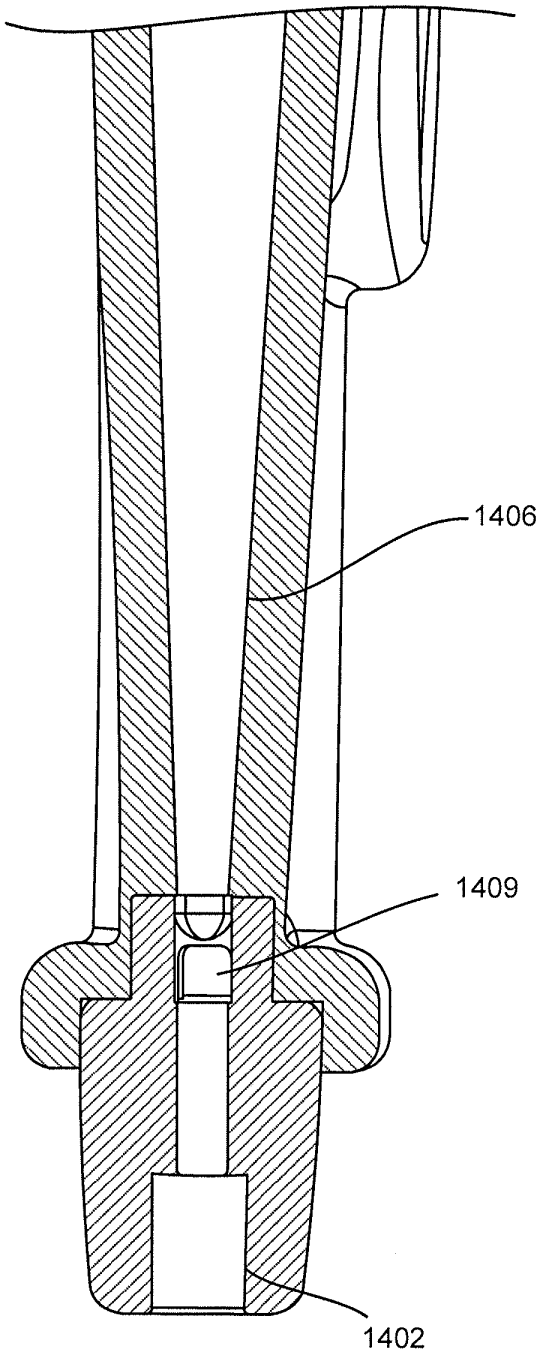


FIG. 14D

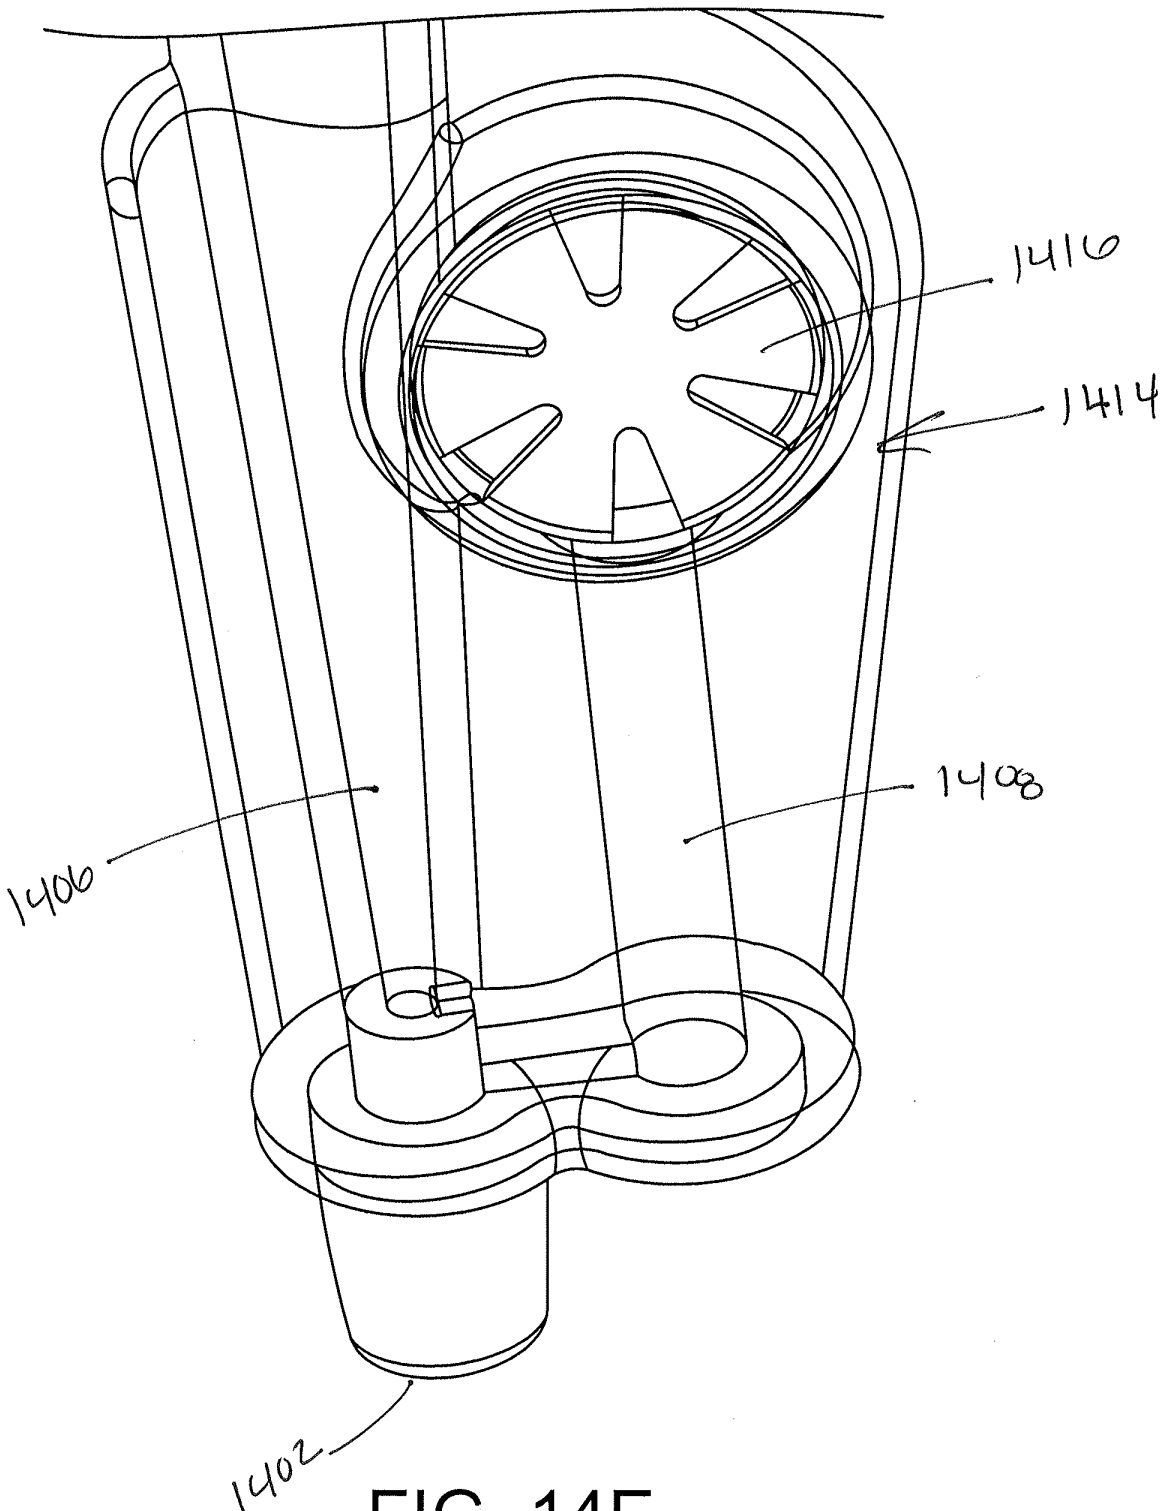


FIG. 14E

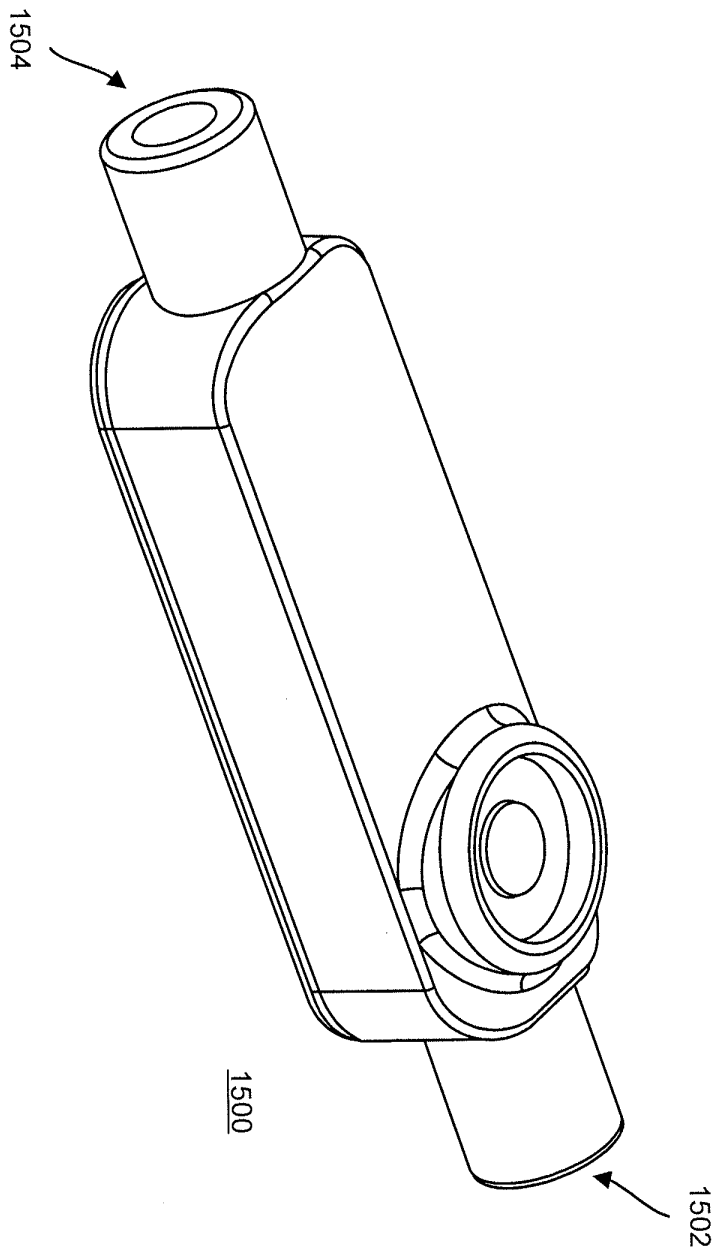


FIG. 15A

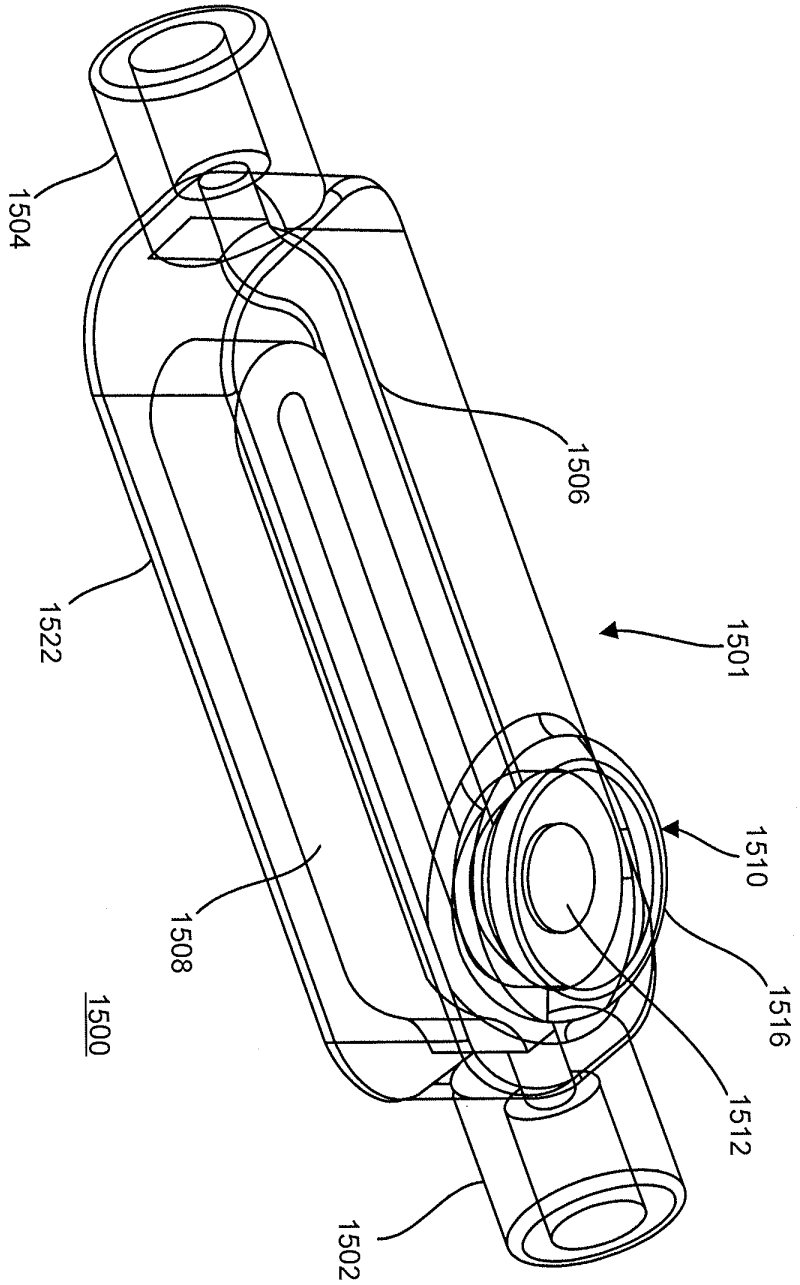


FIG. 15B

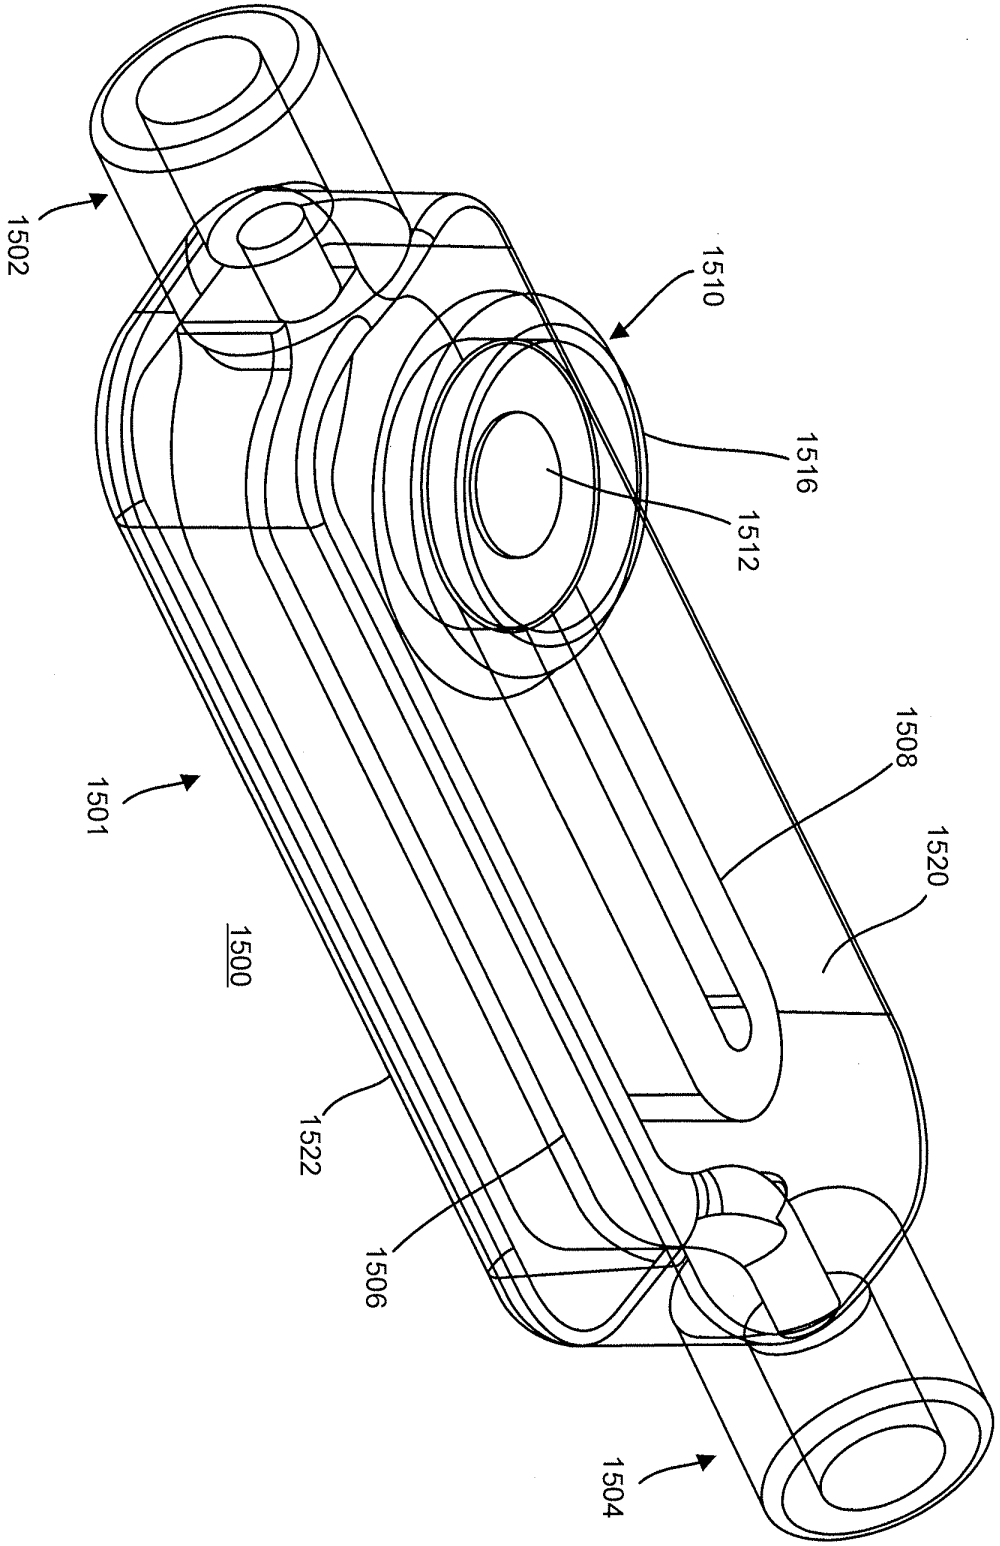


FIG. 15C

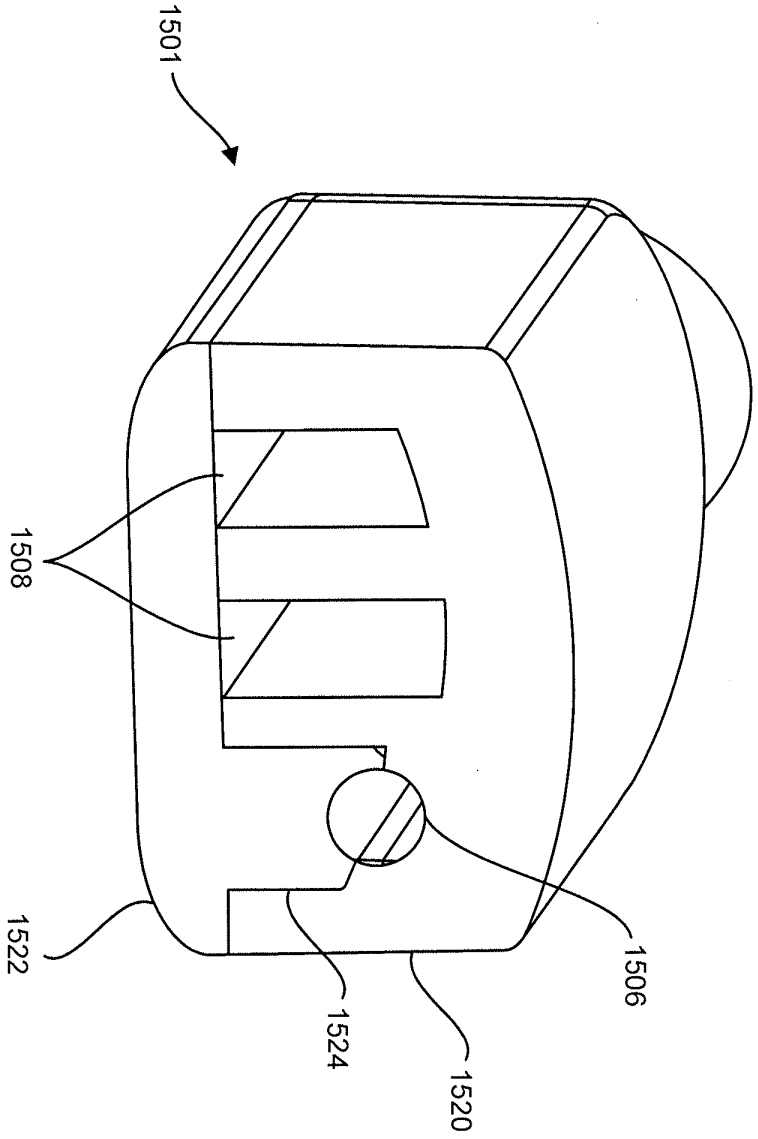


FIG. 15D

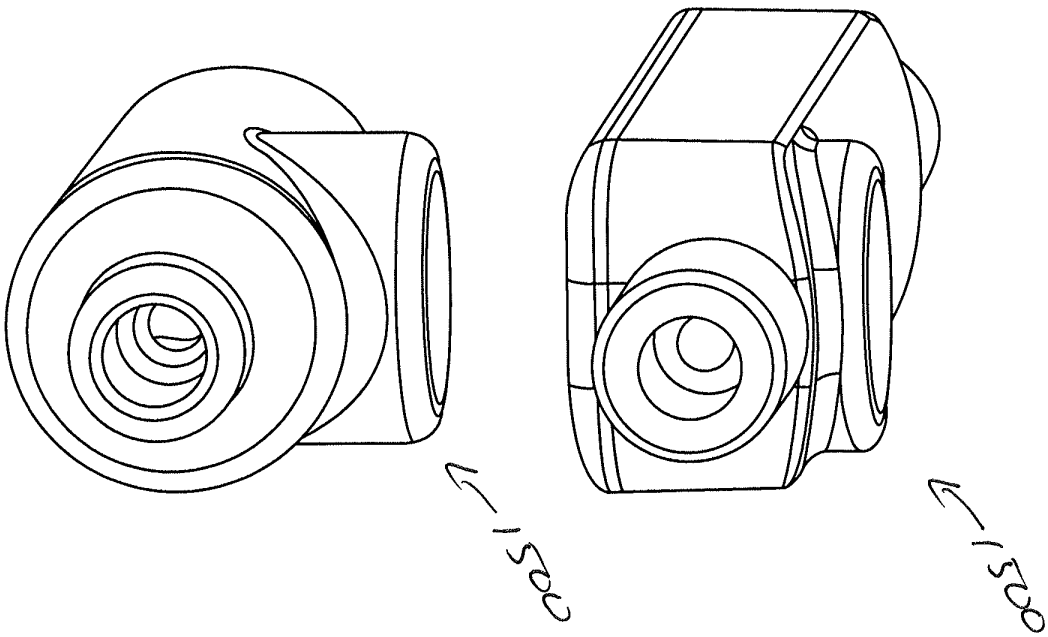


FIG. 15E

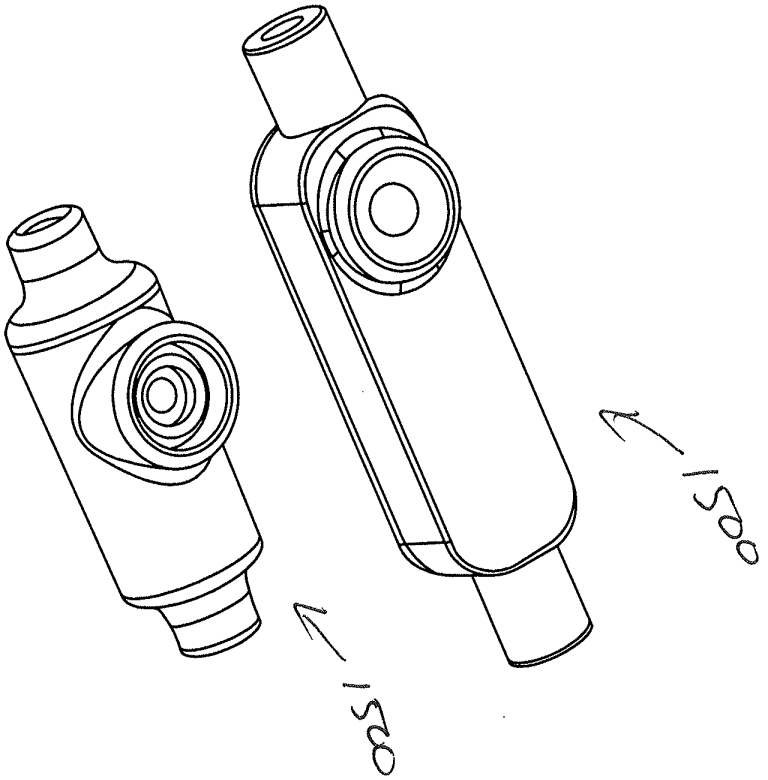


FIG. 15F

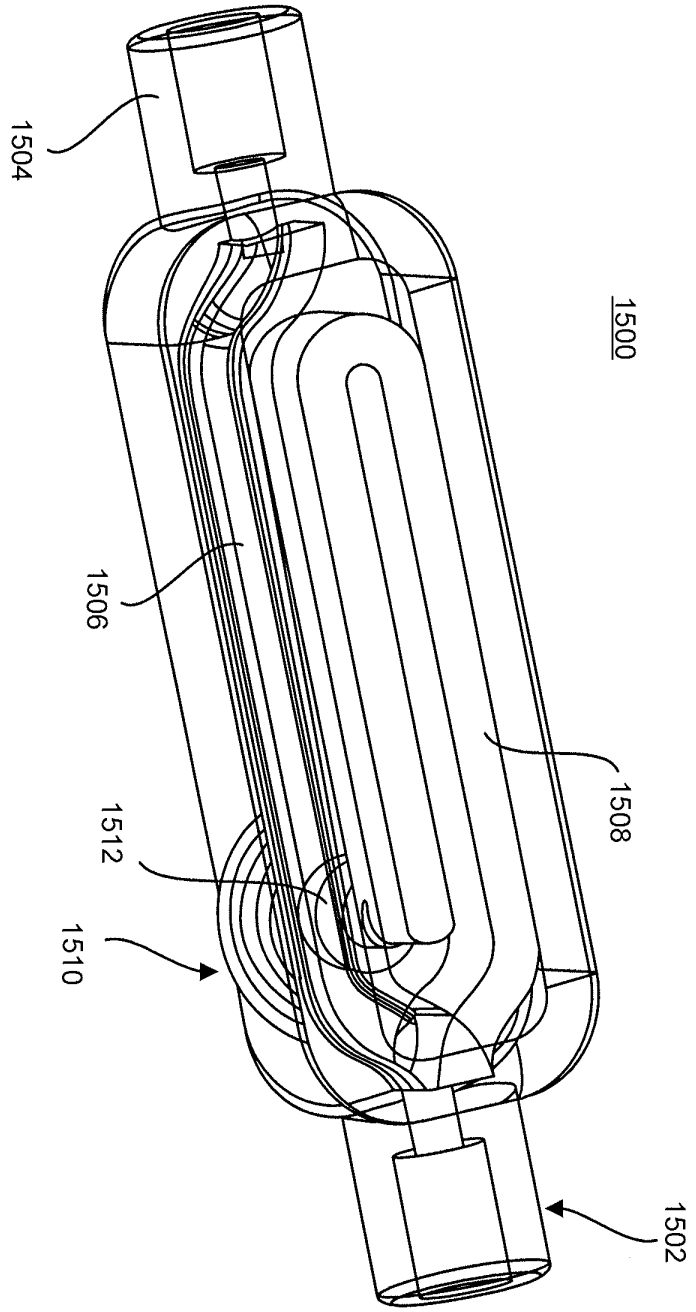


FIG. 15G

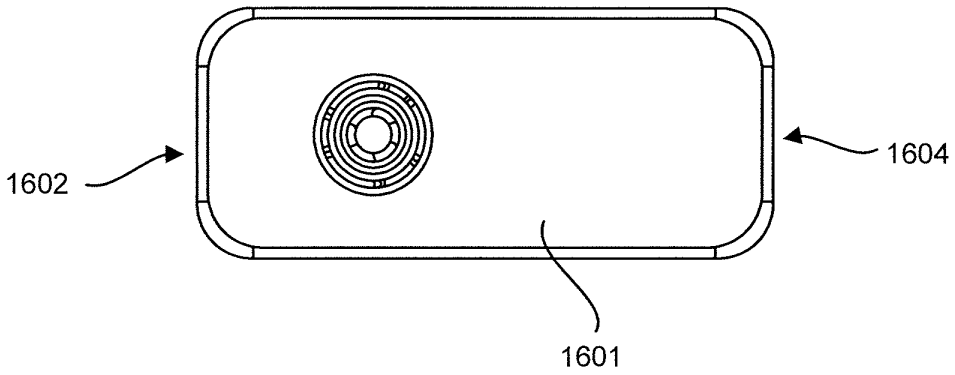


FIG. 16A

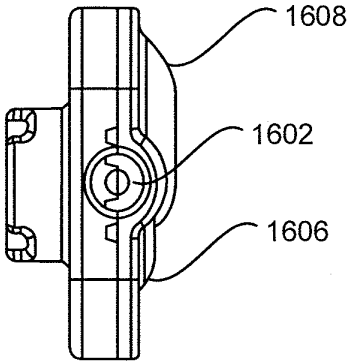


FIG. 16C

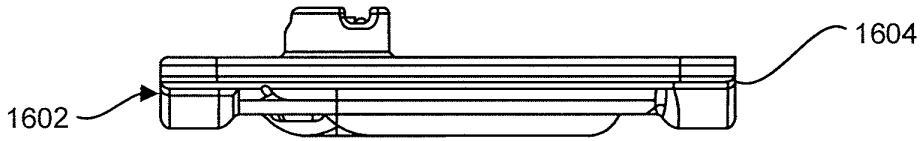


FIG. 16B

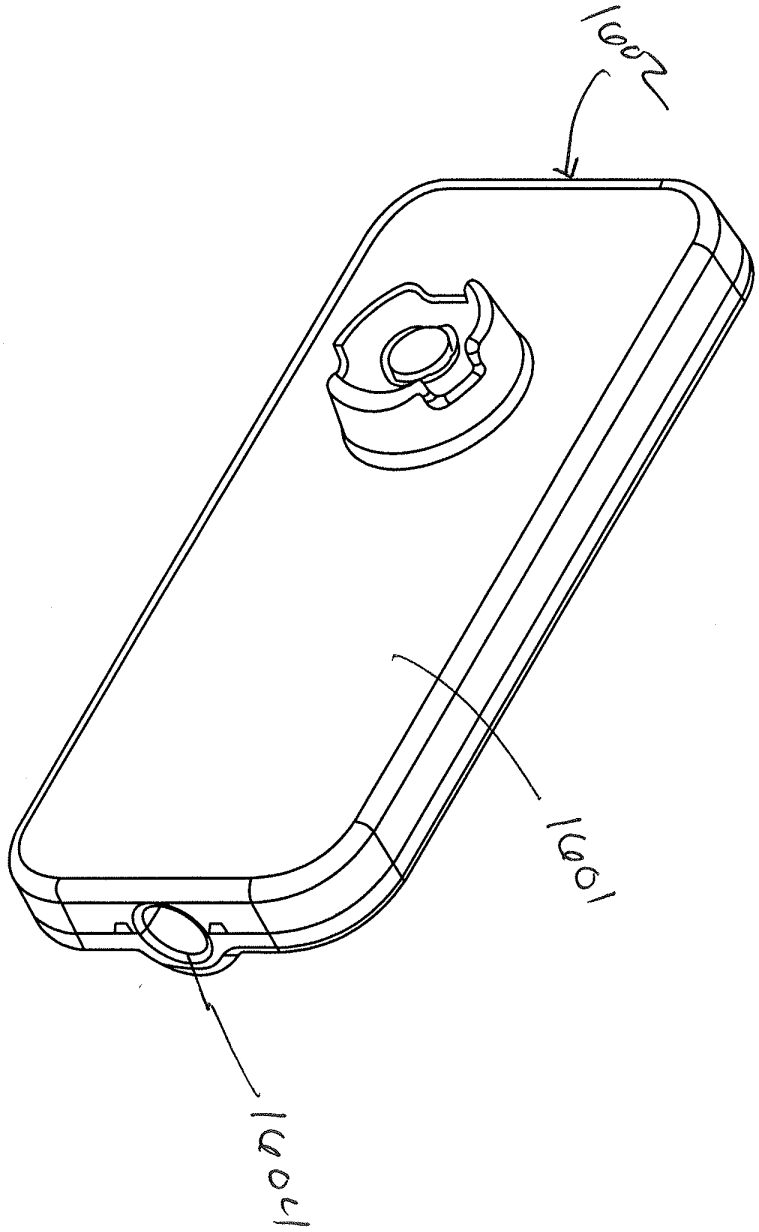


FIG. 16D

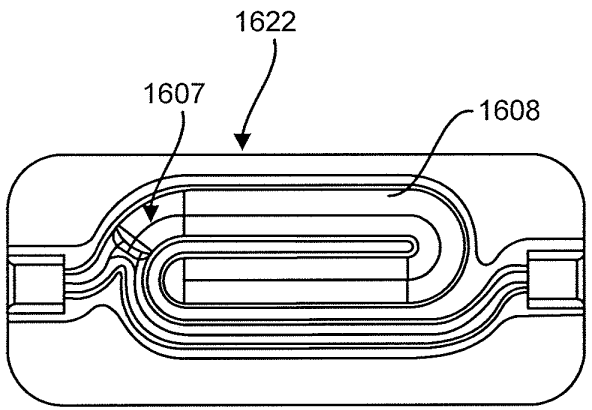


FIG. 17A

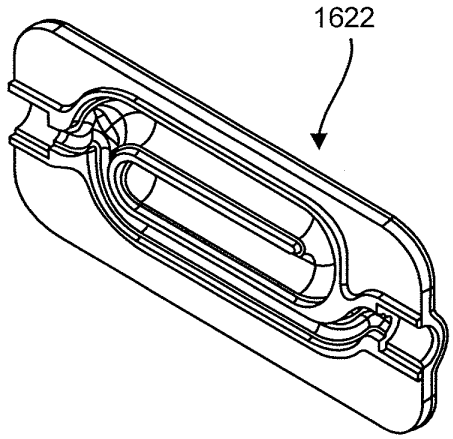


FIG. 17B

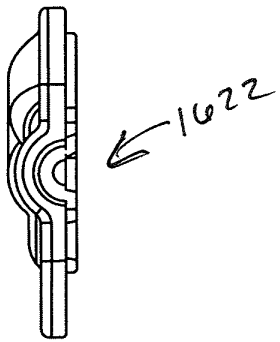


FIG. 17C

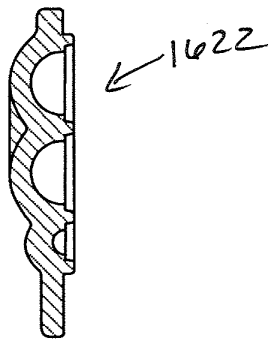


FIG. 17D

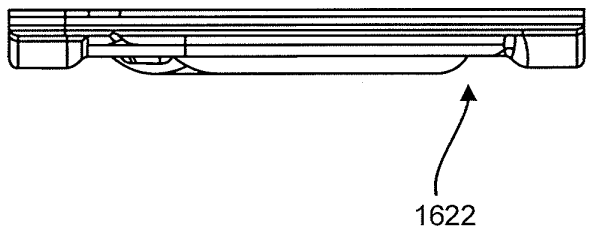


FIG. 17E

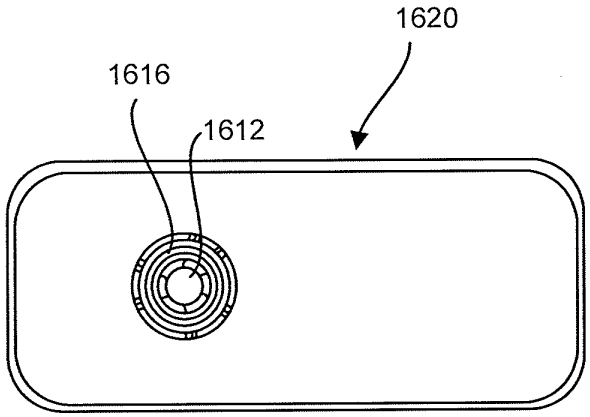


FIG. 18A

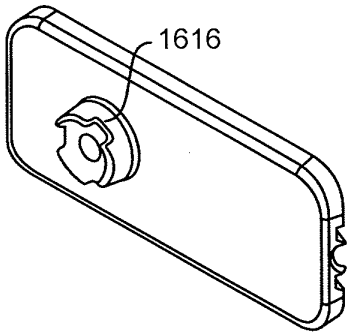


FIG. 18B

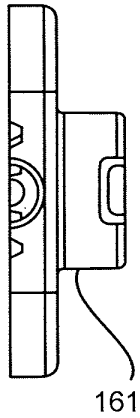


FIG. 18C

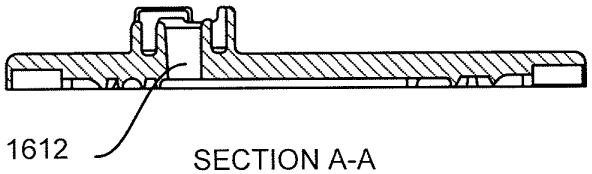


FIG. 18D

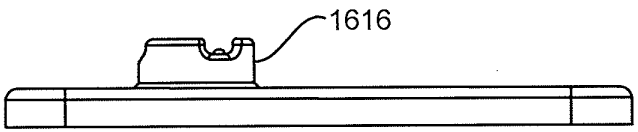


FIG. 18E

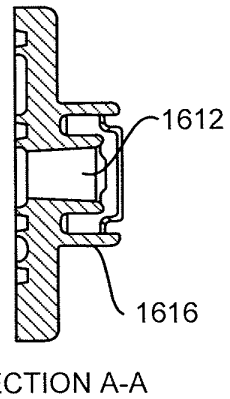


FIG. 18F

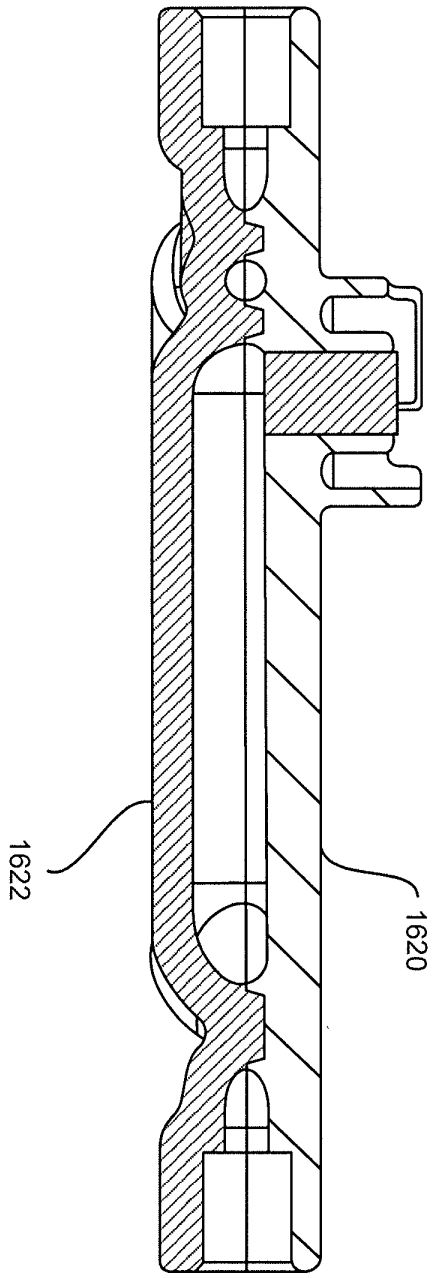


FIG. 19A

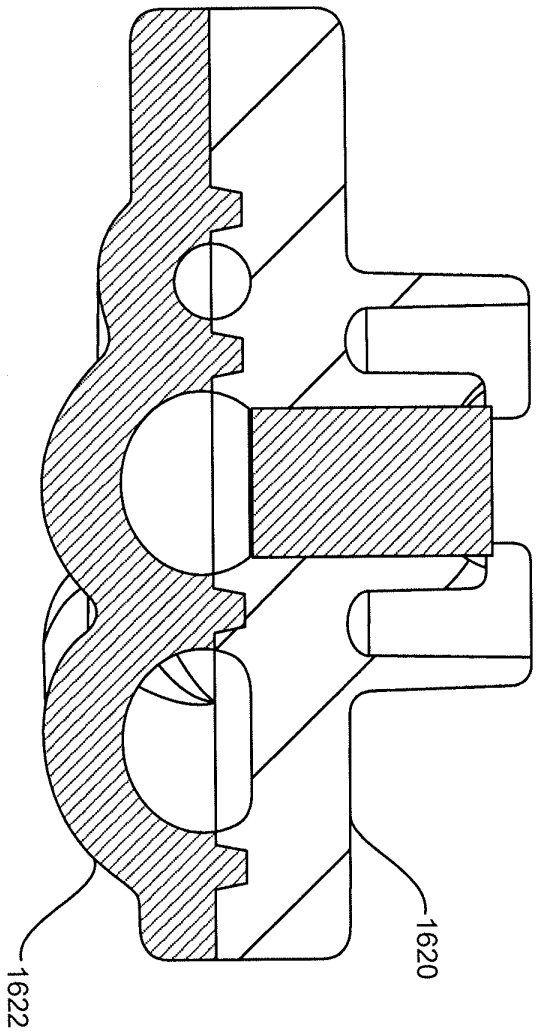


FIG. 19B

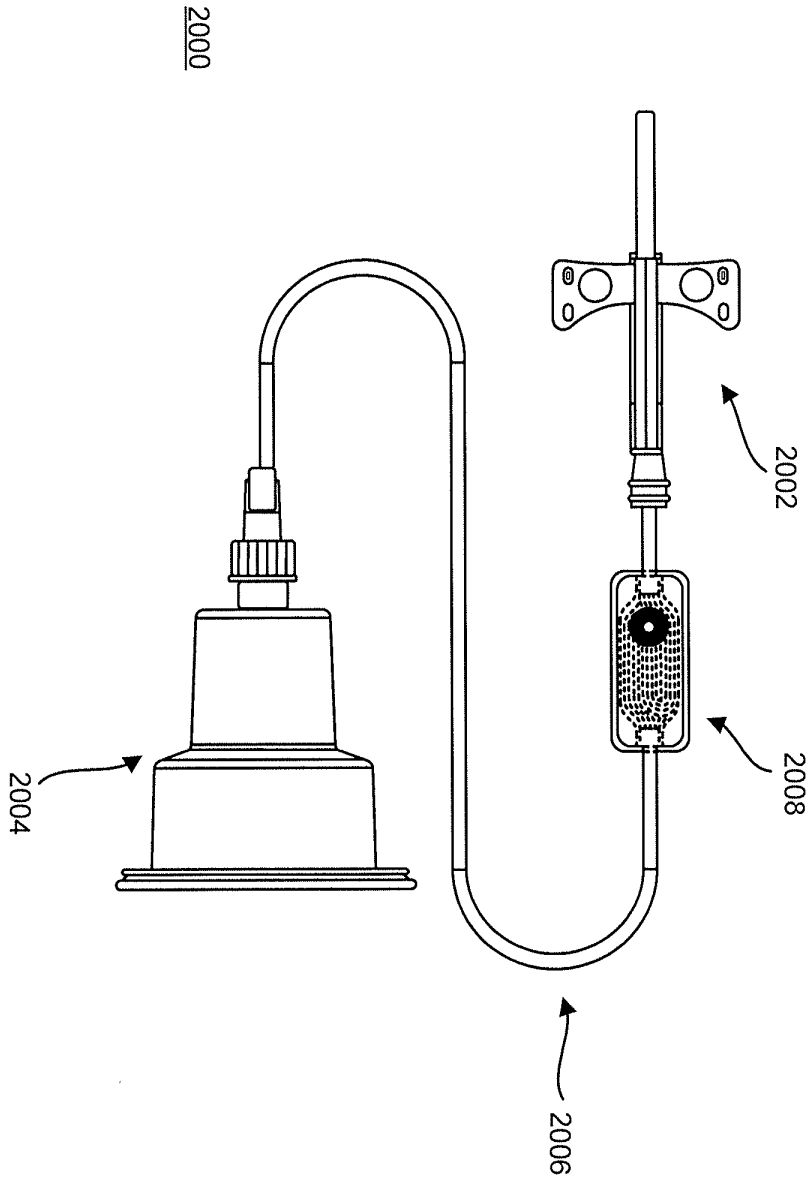


FIG. 20

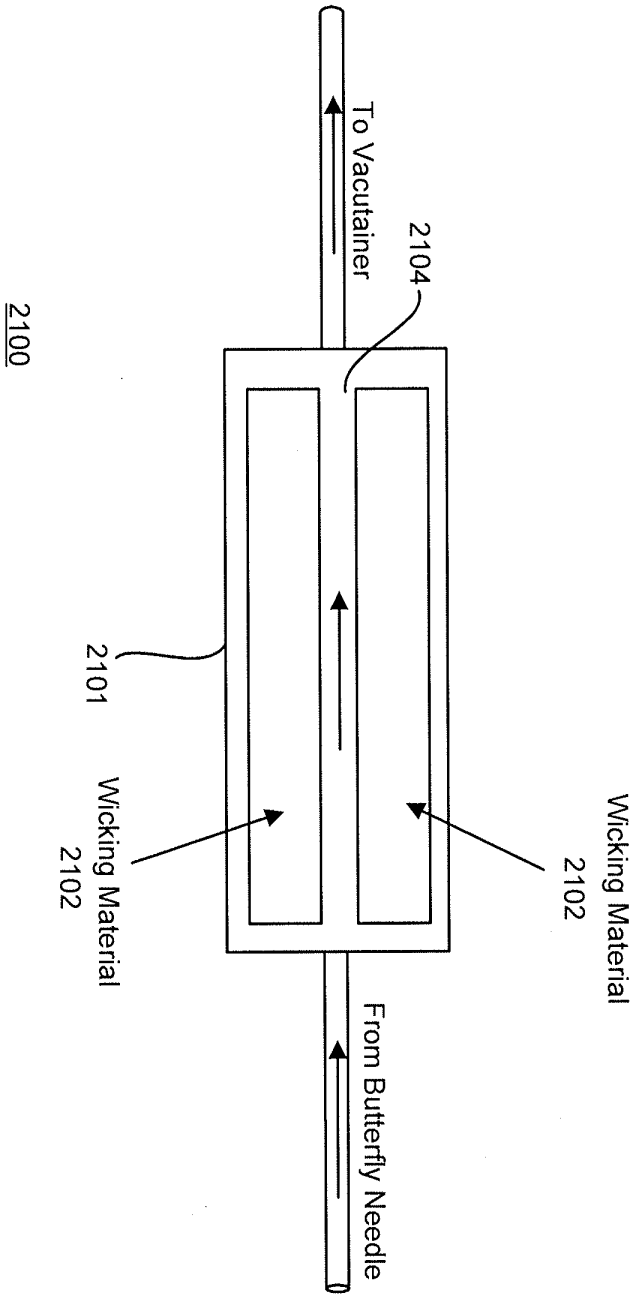

2100
To Vacutainer
2104
2101
Wicking Material
2102
Wicking Material
2102
From Butterfly Needle

FIG. 21

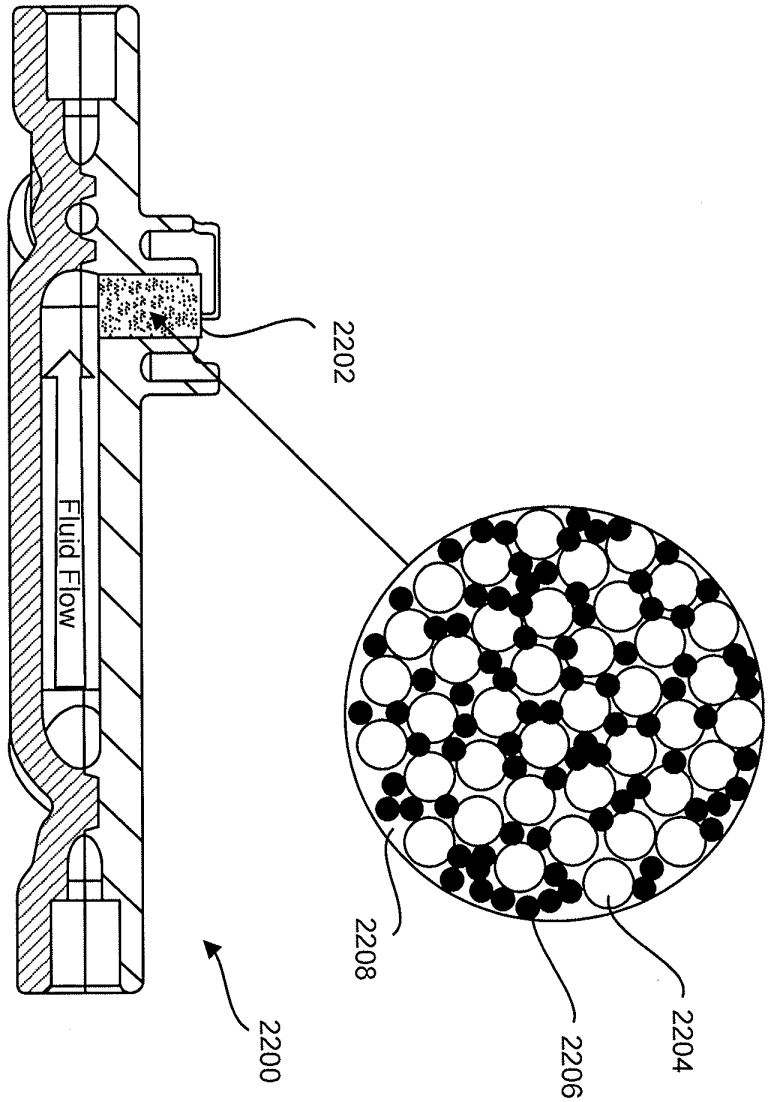


FIG. 22A

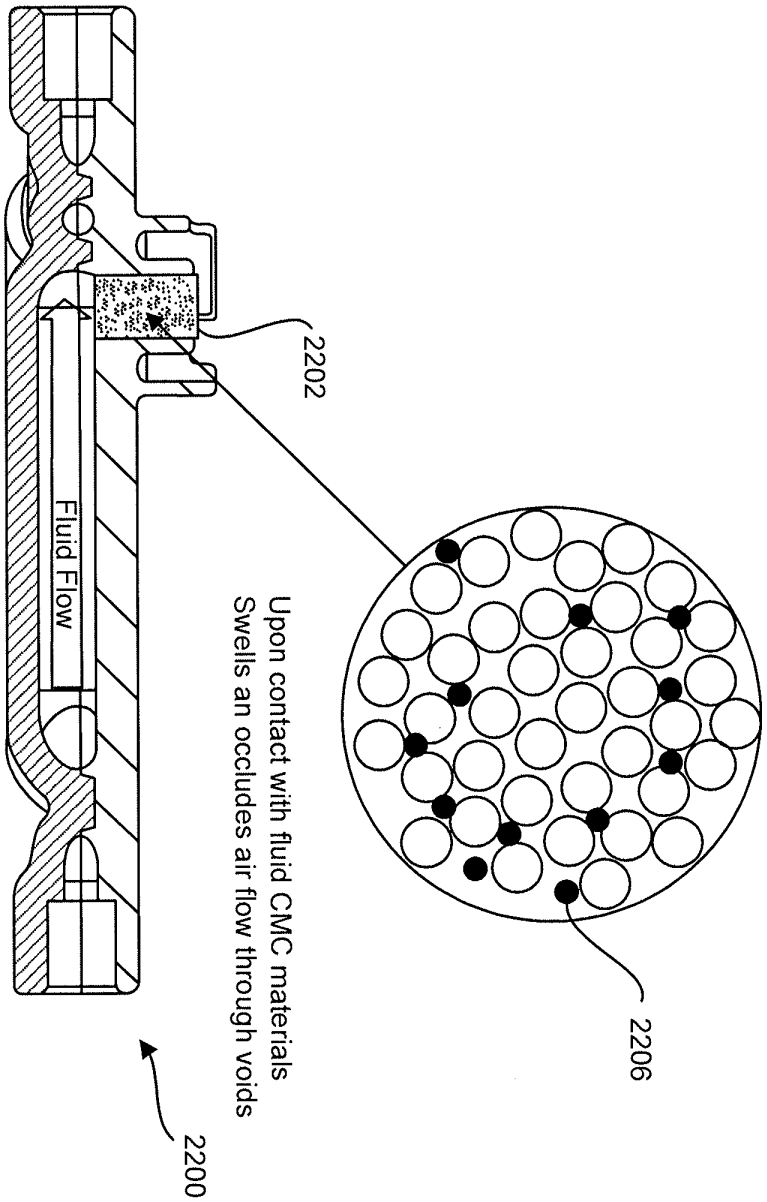

2202
Fluid Flow
Upon contact with fluid CMC materials
Swells an occludes air flow through voids
2206
2200

FIG. 22B

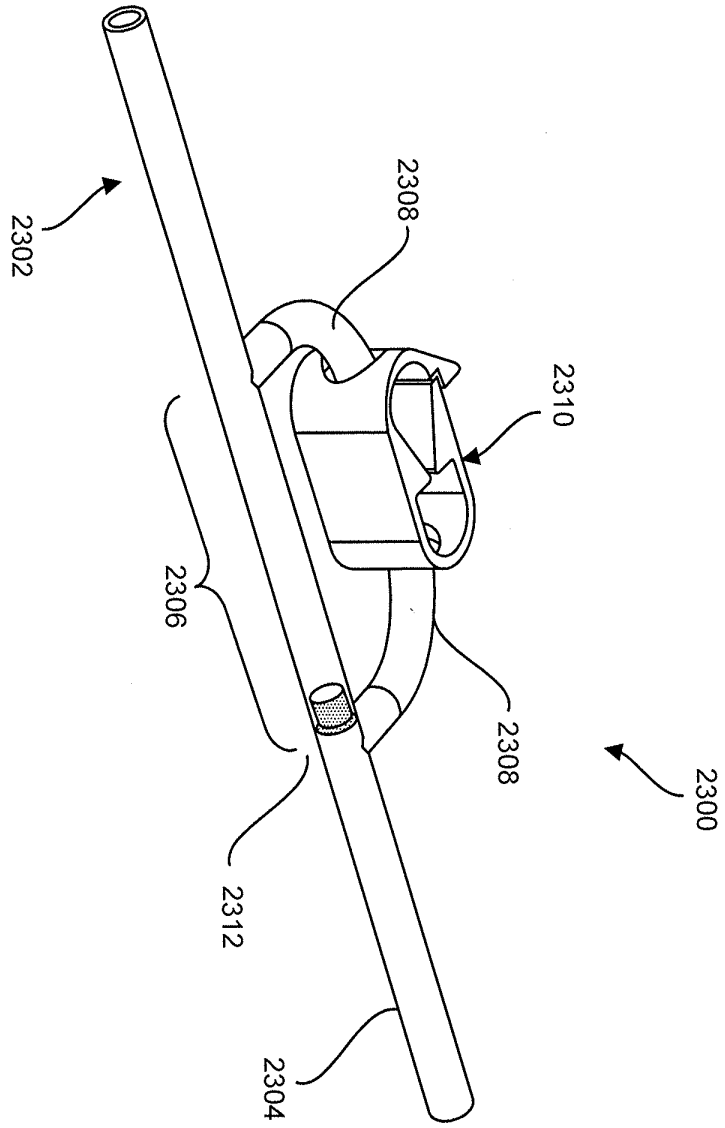


FIG. 23A

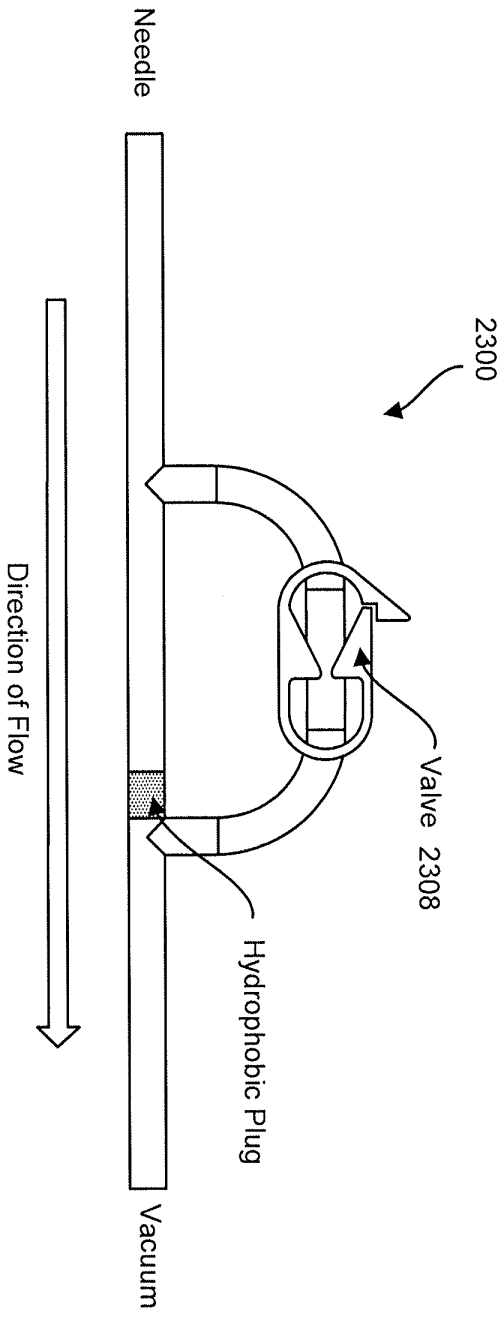

2300
Needle
Valve 2308
Hydrophobic Plug
Vacuum
Direction of Flow

FIG. 23B

PTO/AIA/01 (06-12)
Approved for use through 01/31/2014. OMB 0651-0032
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

DECLARATION (37 CFR 1.63) FOR UTILITY OR DESIGN APPLICATION USING AN APPLICATION DATA SHEET (37 CFR 1.76)

Title of Invention	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD

As the below named inventor, I hereby declare that:

This declaration is directed to:

☐ The attached application, or

☒ United States application or PCT international application number 15/140,448 filed on April 27, 2016.

The above-identified application was made or authorized to be made by me.

I believe that I am the original inventor or an original joint inventor of a claimed invention in the application.

I hereby acknowledge that any willful false statement made in this declaration is punishable under 18 U.S.C. 1001 by fine or imprisonment of not more than five (5) years, or both.

WARNING:

Petitioner/applicant is cautioned to avoid submitting personal information in documents filed in a patent application that may contribute to identity theft. Personal information such as social security numbers, bank account numbers, or credit card numbers (other than a check or credit card authorization form PTO-2038 submitted for payment purposes) is never required by the USPTO to support a petition or an application. If this type of personal information is included in documents submitted to the USPTO, petitioners/applicants should consider redacting such personal information from the documents before submitting them to the USPTO. Petitioner/applicant is advised that the record of a patent application is available to the public after publication of the application (unless a non-publication request in compliance with 37 CFR 1.213(a) is made in the application) or issuance of a patent. Furthermore, the record from an abandoned application may also be available to the public if the application is referenced in a published application or an issued patent (see 37 CFR 1.14). Checks and credit card authorization forms PTO-2038 submitted for payment purposes are not retained in the application file and therefore are not publicly available.

LEGAL NAME OF INVENTOR

Inventor: Bobby E. Rogers Date (Optional): _____

Signature: Bobby E. Rogers

Note: An application data sheet (PTO/SB/14 or equivalent), including naming the entire inventive entity, must accompany this form or must have been previously filed. Use an additional PTO/AIA/01 form for each additional inventor.

This collection of information is required by 35 U.S.C. 115 and 37 CFR 1.63. The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.11 and 1.14. This collection is estimated to take 1 minute to complete, including gathering, preparing, and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. **SEND TO: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.**

If you need assistance in completing the form, call 1-800-PTO-9199 and select option 2.

PTO/AIA/01 (06-12)
Approved for use through 01/31/2014. OMB 0651-0032
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

DECLARATION (37 CFR 1.63) FOR UTILITY OR DESIGN APPLICATION USING AN APPLICATION DATA SHEET (37 CFR 1.76)

Title of Invention	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD

As the below named inventor, I hereby declare that:

This declaration is directed to:

- ☐ The attached application, or
- ■ United States application or PCT international application number 15/140,448 filed on April 27, 2016.

The above-identified application was made or authorized to be made by me.

I believe that I am the original inventor or an original joint inventor of a claimed invention in the application.

I hereby acknowledge that any willful false statement made in this declaration is punishable under 18 U.S.C. 1001 by fine or imprisonment of not more than five (5) years, or both.

WARNING:

Petitioner/applicant is cautioned to avoid submitting personal information in documents filed in a patent application that may contribute to identity theft. Personal information such as social security numbers, bank account numbers, or credit card numbers (other than a check or credit card authorization form PTO-2038 submitted for payment purposes) is never required by the USPTO to support a petition or an application. If this type of personal information is included in documents submitted to the USPTO, petitioners/applicants should consider redacting such personal information from the documents before submitting them to the USPTO. Petitioner/applicant is advised that the record of a patent application is available to the public after publication of the application (unless a non-publication request in compliance with 37 CFR 1.213(a) is made in the application) or issuance of a patent. Furthermore, the record from an abandoned application may also be available to the public if the application is referenced in a published application or an issued patent (see 37 CFR 1.14). Checks and credit card authorization forms PTO-2038 submitted for payment purposes are not retained in the application file and therefore are not publicly available.

LEGAL NAME OF INVENTOR

Inventor: Gino Kang Date (Optional): 1/22/2018

Signature: _____

Note: An application data sheet (PTO/SB/14 or equivalent), including naming the entire inventive entity, must accompany this form or must have been previously filed. Use an additional PTO/AIA/01 form for each additional inventor.

This collection of information is required by 35 U.S.C. 115 and 37 CFR 1.63. The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.11 and 1.14. This collection is estimated to take 1 minute to complete, including gathering, preparing, and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. **SEND TO: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.**

If you need assistance in completing the form, call 1-800-PTO-9199 and select option 2.

PTO/AIA/01 (06-12)
Approved for use through 01/31/2014. OMB 0651-0032
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

DECLARATION (37 CFR 1.63) FOR UTILITY OR DESIGN APPLICATION USING AN APPLICATION DATA SHEET (37 CFR 1.76)

Title of Invention	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD

As the below named inventor, I hereby declare that:

This declaration is directed to:

☐ The attached application, or

■ United States application or PCT international application number 15/140,448 filed on April 27, 2016.

The above-identified application was made or authorized to be made by me.

I believe that I am the original inventor or an original joint inventor of a claimed invention in the application.

I hereby acknowledge that any willful false statement made in this declaration is punishable under 18 U.S.C. 1001 by fine or imprisonment of not more than five (5) years, or both.

WARNING:

Petitioner/applicant is cautioned to avoid submitting personal information in documents filed in a patent application that may contribute to identity theft. Personal information such as social security numbers, bank account numbers, or credit card numbers (other than a check or credit card authorization form PTO-2038 submitted for payment purposes) is never required by the USPTO to support a petition or an application. If this type of personal information is included in documents submitted to the USPTO, petitioners/applicants should consider redacting such personal information from the documents before submitting them to the USPTO. Petitioner/applicant is advised that the record of a patent application is available to the public after publication of the application (unless a non-publication request in compliance with 37 CFR 1.213(a) is made in the application) or issuance of a patent. Furthermore, the record from an abandoned application may also be available to the public if the application is referenced in a published application or an issued patent (see 37 CFR 1.14). Checks and credit card authorization forms PTO-2038 submitted for payment purposes are not retained in the application file and therefore are not publicly available.

LEGAL NAME OF INVENTOR

Inventor: John Detloff Date (Optional): 1-23-18

Signature: John E. Detloff

Note: An application data sheet (PTO/SB/14 or equivalent), including naming the entire inventive entity, must accompany this form or must have been previously filed. Use an additional PTO/AIA/01 form for each additional inventor.

This collection of information is required by 35 U.S.C. 115 and 37 CFR 1.63. The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.11 and 1.14. This collection is estimated to take 1 minute to complete, including gathering, preparing, and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. **SEND TO: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.**

If you need assistance in completing the form, call 1-800-PTO-9199 and select option 2.

PTO/AIA/14 (02-18)
Approved for use through 11/30/2020. OMB 0651-0032
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it contains a valid OMB control number.

Application Data Sheet 37 CFR 1.76	Attorney Docket Number	251102.000027.KURIN2CON2
	Application Number	
Title of Invention	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD	

The application data sheet is part of the provisional or nonprovisional application for which it is being submitted. The following form contains the bibliographic data arranged in a format specified by the United States Patent and Trademark Office as outlined in 37 CFR 1.76.
This document may be completed electronically and submitted to the Office in electronic format using the Electronic Filing System (EFS) or the document may be printed and included in a paper filed application.

Secrecy Order 37 CFR 5.2:

☐ Portions or all of the application associated with this Application Data Sheet may fall under a Secrecy Order pursuant to 37 CFR 5.2 (Paper filers only. Applications that fall under Secrecy Order may not be filed electronically.)

Inventor Information:

Inventor 1 Remove

Legal Name

Prefix	Given Name	Middle Name	Family Name	Suffix
	Bobby	E.	ROGERS	

Residence Information (Select One) ◉ US Residency ○ Non US Residency ○ Active US Military Service

City	San Diego	State/Province	CA	Country of Residence	US

Mailing Address of Inventor:

Address 1	14777 Whispering Ridge Road		
Address 2			
City	San Diego	State/Province	CA
Postal Code	92131	Country	US

Inventor 2 Remove

Legal Name

Prefix	Given Name	Middle Name	Family Name	Suffix
	Gino		KANG	

Residence Information (Select One) ◉ US Residency ○ Non US Residency ○ Active US Military Service

City	Irvine	State/Province	CA	Country of Residence	US

Mailing Address of Inventor:

Address 1	71 Shade Tree		
Address 2			
City	Irvine	State/Province	CA
Postal Code	92603	Country	US

Inventor 3 Remove

Legal Name

Prefix	Given Name	Middle Name	Family Name	Suffix
	John		DETLOFF	

Residence Information (Select One) ◉ US Residency ○ Non US Residency ○ Active US Military Service

PTO/AIA/14 (02-18)
Approved for use through 11/30/2020. OMB 0651-0032
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it contains a valid OMB control number.

Application Data Sheet 37 CFR 1.76	Attorney Docket Number	251102.000027.KURIN2CON2
	Application Number	
Title of Invention	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD	

City	San Diego	State/Province	CA	Country of Residence	US

Mailing Address of Inventor:

Address 1	4696 La Cuenta Dr.		
Address 2			
City	San Diego	**State/Province**	CA
Postal Code	92124	**Country**	US

All Inventors Must Be Listed - Additional Inventor Information blocks may be generated within this form by selecting the **Add** button. Add

Correspondence Information:

Enter either Customer Number or complete the Correspondence Information section below.
For further information see 37 CFR 1.33(a).

☐ **An Address is being provided for the correspondence Information of this application.**

Customer Number	153290		
Email Address	patents@troutman.com	Add Email	Remove Email

Application Information:

Title of the Invention	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD		
Attorney Docket Number	251102.000027.KURIN2CON2	**Small Entity Status Claimed**	☒
Application Type	Nonprovisional		
Subject Matter	Utility		
Total Number of Drawing Sheets (if any)	50	**Suggested Figure for Publication (if any)**	

Filing By Reference:

Only complete this section when filing an application by reference under 35 U.S.C. 111(c) and 37 CFR 1.57(a). Do not complete this section if application papers including a specification and any drawings are being filed. Any domestic benefit or foreign priority information must be provided in the appropriate section(s) below (i.e., "Domestic Benefit/National Stage Information" and "Foreign Priority Information").

For the purposes of a filing date under 37 CFR 1.53(b), the description and any drawings of the present application are replaced by this reference to the previously filed application, subject to conditions and requirements of 37 CFR 1.57(a).

Application number of the previously filed application	Filing date (YYYY-MM-DD)	Intellectual Property Authority or Country

Publication Information:

☐ Request Early Publication (Fee required at time of Request 37 CFR 1.219)

☐ **Request Not to Publish.** I hereby request that the attached application not be published under 35 U.S.C. 122(b) and certify that the invention disclosed in the attached application **has not and will not** be the subject of an application filed in another country, or under a multilateral international agreement, that requires publication at eighteen months after filing.

Application Data Sheet 37 CFR 1.76	Attorney Docket Number	251102.000027.KURIN2CON2
	Application Number	
Title of Invention	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD	

Representative Information:

Representative information should be provided for all practitioners having a power of attorney in the application. Providing this information in the Application Data Sheet does not constitute a power of attorney in the application (see 37 CFR 1.32). Either enter Customer Number or complete the Representative Name section below. If both sections are completed the customer Number will be used for the Representative Information during processing.

Please Select One:	◉ Customer Number	○ US Patent Practitioner	○ Limited Recognition (37 CFR 11.9)
Customer Number	153290		

Domestic Benefit/National Stage Information:

This section allows for the applicant to either claim benefit under 35 U.S.C. 119(e), 120, 121, 365(c), or 386(c) or indicate National Stage entry from a PCT application. Providing benefit claim information in the Application Data Sheet constitutes the specific reference required by 35 U.S.C. 119(e) or 120, and 37 CFR 1.78.
When referring to the current application, please leave the "Application Number" field blank.

Prior Application Status	Pending		Remove
Application Number	Continuity Type	Prior Application Number	Filing or 371(c) Date (YYYY-MM-DD)
	Continuation of	15/140448	2016-04-27
Prior Application Status	Expired		Remove
Application Number	Continuity Type	Prior Application Number	Filing or 371(c) Date (YYYY-MM-DD)
15/140448	Claims benefit of provisional	62/196797	2015-07-24
Prior Application Status	Expired		Remove
Application Number	Continuity Type	Prior Application Number	Filing or 371(c) Date (YYYY-MM-DD)
15/140448	Claims benefit of provisional	62/238636	2015-10-07
Prior Application Status	Expired		Remove
Application Number	Continuity Type	Prior Application Number	Filing or 371(c) Date (YYYY-MM-DD)
15/140448	Claims benefit of provisional	62/318194	2016-04-04

Additional Domestic Benefit/National Stage Data may be generated within this form by selecting the **Add** button.

Foreign Priority Information:

Application Data Sheet 37 CFR 1.76	Attorney Docket Number	251102.000027.KURIN2CON2
	Application Number	
Title of Invention	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD	

This section allows for the applicant to claim priority to a foreign application. Providing this information in the application data sheet constitutes the claim for priority as required by 35 U.S.C. 119(b) and 37 CFR 1.55. When priority is claimed to a foreign application that is eligible for retrieval under the priority document exchange program (PDX)[i] the information will be used by the Office to automatically attempt retrieval pursuant to 37 CFR 1.55(i)(1) and (2). Under the PDX program, applicant bears the ultimate responsibility for ensuring that a copy of the foreign application is received by the Office from the participating foreign intellectual property office, or a certified copy of the foreign priority application is filed, within the time period specified in 37 CFR 1.55(g)(1).

Remove

Application Number	Country[i]	Filing Date (YYYY-MM-DD)	Access Code[i] (if applicable)

Additional Foreign Priority Data may be generated within this form by selecting the **Add** button.

Statement under 37 CFR 1.55 or 1.78 for AIA (First Inventor to File) Transition Applications

☐ This application (1) claims priority to or the benefit of an application filed before March 16, 2013 and (2) also contains, or contained at any time, a claim to a claimed invention that has an effective filing date on or after March 16, 2013.
NOTE: By providing this statement under 37 CFR 1.55 or 1.78, this application, with a filing date on or after March 16, 2013, will be examined under the first inventor to file provisions of the AIA.

Application Data Sheet 37 CFR 1.76	Attorney Docket Number	251102.000027.KURIN2CON2
	Application Number	
Title of Invention	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD	

Authorization or Opt-Out of Authorization to Permit Access:

When this Application Data Sheet is properly signed and filed with the application, applicant has provided written authority to permit a participating foreign intellectual property (IP) office access to the instant application-as-filed (see paragraph A in subsection 1 below) and the European Patent Office (EPO) access to any search results from the instant application (see paragraph B in subsection 1 below).

Should applicant choose not to provide an authorization identified in subsection 1 below, applicant **must opt-out** of the authorization by checking the corresponding box A or B or both in subsection 2 below.

NOTE: This section of the Application Data Sheet is **ONLY** reviewed and processed with the **INITIAL** filing of an application. After the initial filing of an application, an Application Data Sheet cannot be used to provide or rescind authorization for access by a foreign IP office(s). Instead, Form PTO/SB/39 or PTO/SB/69 must be used as appropriate.

1. Authorization to Permit Access by a Foreign Intellectual Property Office(s)

A. Priority Document Exchange (PDX) - Unless box A in subsection 2 (opt-out of authorization) is checked, the undersigned hereby **grants the USPTO authority** to provide the European Patent Office (EPO), the Japan Patent Office (JPO), the Korean Intellectual Property Office (KIPO), the State Intellectual Property Office of the People's Republic of China (SIPO), the World Intellectual Property Organization (WIPO), and any other foreign intellectual property office participating with the USPTO in a bilateral or multilateral priority document exchange agreement in which a foreign application claiming priority to the instant patent application is filed, access to: (1) the instant patent application-as-filed and its related bibliographic data, (2) any foreign or domestic application to which priority or benefit is claimed by the instant application and its related bibliographic data, and (3) the date of filing of this Authorization. See 37 CFR 1.14(h)(1).

B. Search Results from U.S. Application to EPO - Unless box B in subsection 2 (opt-out of authorization) is checked, the undersigned hereby **grants the USPTO authority** to provide the EPO access to the bibliographic data and search results from the instant patent application when a European patent application claiming priority to the instant patent application is filed. See 37 CFR 1.14(h)(2).

The applicant is reminded that the EPO's Rule 141(1) EPC (European Patent Convention) requires applicants to submit a copy of search results from the instant application without delay in a European patent application that claims priority to the instant application.

2. Opt-Out of Authorizations to Permit Access by a Foreign Intellectual Property Office(s)

☐ A. Applicant **DOES NOT** authorize the USPTO to permit a participating foreign IP office access to the instant application-as-filed. If this box is checked, the USPTO will not be providing a participating foreign IP office with any documents and information identified in subsection 1A above.

☐ B. Applicant **DOES NOT** authorize the USPTO to transmit to the EPO any search results from the instant patent application. If this box is checked, the USPTO will not be providing the EPO with search results from the instant application.

NOTE: Once the application has published or is otherwise publicly available, the USPTO may provide access to the application in accordance with 37 CFR 1.14.

PTO/AIA/14 (02-18)
Approved for use through 11/30/2020. OMB 0651-0032
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it contains a valid OMB control number.

Application Data Sheet 37 CFR 1.76	Attorney Docket Number	251102.000027.KURIN2CON2
	Application Number	
Title of Invention	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD	

Applicant Information:

Providing assignment information in this section does not substitute for compliance with any requirement of part 3 of Title 37 of CFR to have an assignment recorded by the Office.

Applicant 1

If the applicant is the inventor (or the remaining joint inventor or inventors under 37 CFR 1.45), this section should not be completed. The information to be provided in this section is the name and address of the legal representative who is the applicant under 37 CFR 1.43; or the name and address of the assignee, person to whom the inventor is under an obligation to assign the invention, or person who otherwise shows sufficient proprietary interest in the matter who is the applicant under 37 CFR 1.46. If the applicant is an applicant under 37 CFR 1.46 (assignee, person to whom the inventor is obligated to assign, or person who otherwise shows sufficient proprietary interest) together with one or more joint inventors, then the joint inventor or inventors who are also the applicant should be identified in this section.

Clear

(•) Assignee	( ) Legal Representative under 35 U.S.C. 117	( ) Joint Inventor
( ) Person to whom the inventor is obligated to assign.	( ) Person who shows sufficient proprietary interest	

If applicant is the legal representative, indicate the authority to file the patent application, the inventor is:

Name of the Deceased or Legally Incapacitated Inventor:

If the Applicant is an Organization check here. [x]

Organization Name	KURIN, INC.

Mailing Address Information For Applicant:

Address 1	10755 Scripps Poway Parkway #257		
Address 2			
City	San Diego	**State/Province**	CA
Country	US	Postal Code	92131
Phone Number		Fax Number	
Email Address			

Additional Applicant Data may be generated within this form by selecting the Add button.

Assignee Information including Non-Applicant Assignee Information:

Providing assignment information in this section does not substitute for compliance with any requirement of part 3 of Title 37 of CFR to have an assignment recorded by the Office.

PTO/AIA/14 (02-18)
Approved for use through 11/30/2020. OMB 0651-0032
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it contains a valid OMB control number.

Application Data Sheet 37 CFR 1.76	Attorney Docket Number	251102.000027.KURIN2CON2
	Application Number	
Title of Invention	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD	

Assignee 1

Complete this section if assignee information, including non-applicant assignee information, is desired to be included on the patent application publication. An assignee-applicant identified in the "Applicant Information" section will appear on the patent application publication as an applicant. For an assignee-applicant, complete this section only if identification as an assignee is also desired on the patent application publication.

If the Assignee or Non-Applicant Assignee is an Organization check here. ☒

Organization Name	KURIN, INC.

Mailing Address Information For Assignee including Non-Applicant Assignee:

Address 1	10755 Scripps Poway Parkway #257		
Address 2			
City	San Diego	**State/Province**	CA
Country	US	Postal Code	92131
Phone Number		Fax Number	
Email Address			

Additional Assignee or Non-Applicant Assignee Data may be generated within this form by selecting the Add button.

Signature:

NOTE: This Application Data Sheet must be signed in accordance with 37 CFR 1.33(b). **However, if this Application Data Sheet is submitted with the INITIAL filing of the application and either box A or B is not checked in subsection 2 of the "Authorization or Opt-Out of Authorization to Permit Access" section, then this form must also be signed in accordance with 37 CFR 1.14(c).**

This Application Data Sheet **must** be signed by a patent practitioner if one or more of the applicants is a **juristic entity** (e.g., corporation or association). If the applicant is two or more joint inventors, this form must be signed by a patent practitioner, **all** joint inventors who are the applicant, or one or more joint inventor-applicants who have been given power of attorney (e.g., see USPTO Form PTO/AIA/81) on behalf of **all** joint inventor-applicants.

See 37 CFR 1.4(d) for the manner of making signatures and certifications.

Signature	/David Devernoe/			Date (YYYY-MM-DD)	2018-05-31
First Name	David	Last Name	Devernoe	Registration Number	50,128

Additional Signature may be generated within this form by selecting the Add button.

PTO/AIA/14 (02-18)
Approved for use through 11/30/2020. OMB 0651-0032
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it contains a valid OMB control number.

Application Data Sheet 37 CFR 1.76	Attorney Docket Number	251102.000027.KURIN2CON2
	Application Number	
Title of Invention	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD	

This collection of information is required by 37 CFR 1.76. The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.14. This collection is estimated to take 23 minutes to complete, including gathering, preparing, and submitting the completed application data sheet form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. **SEND TO: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.**

Doc Code: PA..
Document Description: Power of Attorney

PTO/AIA/82A (07-13)
Approved for use through 11/30/2014. OMB 0651-0051
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

TRANSMITTAL FOR POWER OF ATTORNEY TO ONE OR MORE REGISTERED PRACTITIONERS

NOTE: This form is to be submitted with the Power of Attorney by Applicant form (PTO/AIA/82B) to identify the application to which the Power of Attorney is directed, in accordance with 37 CFR 1.5, unless the application number and filing date are identified in the Power of Attorney by Applicant form. If neither form PTO/AIA/82A nor form PTO/AIA82B identifies the application to which the Power of Attorney is directed, the Power of Attorney will not be recognized in the application.

Application Number	Assigned Herewith
Filing Date	Assigned Herewith
First Named Inventor	Bobby E. ROGERS
Title	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD
Art Unit	TBD
Examiner Name	TBD
Attorney Docket Number	251102.000027.KURIN2CON2

SIGNATURE of Applicant or Patent Practitioner

Signature	/David Devernoe/	Date (Optional)	2018-05-31
Name	David Devernoe	Registration Number	50,128
Title (if Applicant is a juristic entity)			
Applicant Name (if Applicant is a juristic entity)			

NOTE: This form must be signed in accordance with 37 CFR 1.33. See 37 CFR 1.4(d) for signature requirements and certifications. If more than one applicant, use multiple forms.

☐ *Total of _____ forms are submitted.

This collection of information is required by 37 CFR 1.131, 1.32, and 1.33. The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.11 and 1.14. This collection is estimated to take 3 minutes to complete, including gathering, preparing, and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. **SEND TO: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.**

If you need assistance in completing the form, call 1-800-PTO-9199 and select option 2.

Doc Code: PA..
Document Description: Power of Attorney

PTO/AIA/82B (07-13)
Approved for use through 11/30/2014. OMB 0651-0031
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number

POWER OF ATTORNEY BY APPLICANT

I hereby revoke all previous powers of attorney given in the application identified in either the attached transmittal letter or the boxes below.

Application Number	Filing Date

(Note: The boxes above may be left blank if information is provided on form PTO/AIA/82A.)

☑ I hereby appoint the Patent Practitioner(s) associated with the following Customer Number as my/our attorney(s) or agent(s), and to transact all business in the United States Patent and Trademark Office connected therewith for the application referenced in the attached transmittal letter (form PTO/AIA/82A) or identified above: 153290

OR

☐ I hereby appoint Practitioner(s) named in the attached list (form PTO/AIA/82C) as my/our attorney(s) or agent(s), and to transact all business in the United States Patent and Trademark Office connected therewith for the patent application referenced in the attached transmittal letter (form PTO/AIA/82A) or identified above. (Note: Complete form PTO/AIA/82C.)

Please recognize or change the correspondence address for the application identified in the attached transmittal letter or the boxes above to:

☑ The address associated with the above-mentioned Customer Number

OR

☐ The address associated with Customer Number:

OR

Firm or Individual Name					
Address					
City		State		Zip	
Country					
Telephone		Email			

I am the Applicant (if the Applicant is a juristic entity, list the Applicant name in the box):

Kurin, Inc.

☐ Inventor or Joint Inventor (title not required below)

☐ Legal Representative of a Deceased or Legally Incapacitated Inventor (title not required below)

☑ Assignee or Person to Whom the Inventor is Under an Obligation to Assign (provide signer's title if applicant is a juristic entity)

☐ Person Who Otherwise Shows Sufficient Proprietary Interest (e.g., a petition under 37 CFR 1.46(b)(2) was granted in the application or is concurrently being filed with this document) (provide signer's title if applicant is a juristic entity)

SIGNATURE of Applicant for Patent

The undersigned (whose title is supplied below) is authorized to act on behalf of the applicant (e.g., where the applicant is a juristic entity).

Signature	Bobby Kapur	Date (Optional)	
Name	Bobby Kapur		
Title	CEO		

NOTE: Signature - This form must be signed by the applicant in accordance with 37 CFR 1.33. See 37 CFR 1.4 for signature requirements and certifications. If more than one applicant, use multiple forms.

☐ Total of forms are submitted.

This collection of information is required by 37 CFR 1.191, 1.32, and 1.33. The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.11 and 1.14. This collection is estimated to take 3 minutes to complete, including gathering, preparing, and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. **SEND TO: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.**

If you need assistance in completing the form, call 1-800-PTO-9199 and select option 2.

PTO/SB/08a (01-10)
Approved for use through 07/31/2012. OMB 0651-0031
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE

Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it contains a valid OMB control number.

INFORMATION DISCLOSURE STATEMENT BY APPLICANT (**Not for submission under 37 CFR 1.99)**		
	Application Number	
	Filing Date	2018-05-31
	First Named Inventor	Bobby E. Rogers et al.
	Art Unit	
	Examiner Name	
	Attorney Docket Number	251102.000027.KURIN2CON2

U.S.PATENTS						Remove
Examiner Initial*	Cite No	Patent Number	Kind Code[1]	Issue Date	Name of Patentee or Applicant of cited Document	Pages,Columns,Lines where Relevant Passages or Relevant Figures Appear
	1	3648684	A	1972-03-14	BARNWELL et al	
	2	3817240	A	1974-06-18	AYRES	
	3	3874367	A	1975-04-01	AYRES	
	4	3886930	A	1975-06-03	RYAN	
	5	4056101	A	1977-11-01	GEISSLER et al	
	6	4057050	A	1977-11-08	SARSTEDT	
	7	4106497	A	1978-08-15	PERCARPIO	
	8	4154229	A	1979-05-15	NUGENT	

INFORMATION DISCLOSURE STATEMENT BY APPLICANT (Not for submission under 37 CFR 1.99)		
	Application Number	
	Filing Date	2018-05-31
	First Named Inventor	Bobby E. Rogers et al.
	Art Unit	
	Examiner Name	
	Attorney Docket Number	251102.000027.KURIN2CON2

	9	4207870	A	1980-06-17	ELDRIDGE	
	10	4412548	A	1983-11-01	HOCH	
	11	4416290	A	1983-11-22	LUTKOWSKI	
	12	5222502	A	1993-06-29	KUROSE	
	13	5520193	A	1996-05-28	SUZUKI et al	
	14	5749857	A	1998-05-12	CUPPY	
	15	6569117	B1	2003-05-27	ZIV et al	
	16	8070725	B2	2011-12-06	CHRISTENSEN et al	
	17	8197420	B2	2012-06-12	PATTON et al	
	18	8523826	B2	2013-09-03	LAYTON JR et al	
	19	8535241	B2	2013-09-17	BULLINGTON et al	

INFORMATION DISCLOSURE STATEMENT BY APPLICANT (Not for submission under 37 CFR 1.99)		
	Application Number	
	Filing Date	2018-05-31
	First Named Inventor	Bobby E. Rogers et al.
	Art Unit	
	Examiner Name	
	Attorney Docket Number	251102.000027.KURIN2CON2

	20	8540663	B2	2013-09-24	DAVEY et al	
	21	8568371	B2	2013-10-29	SIOPES et al	
	22	8864684	B2	2014-10-21	BULLINGTON et al	
	23	9022951	B2	2015-05-05	BULLINGTON et al	
	24	9060724	B2	2015-06-23	BULLINGTON et al	
	25	9138572	B2	2015-09-22	ZEYTOONIAN et al	
	26	9204864	B2	2015-12-08	BULLINGTON et al	

If you wish to add additional U.S. Patent citation information please click the Add button. Add

U.S.PATENT APPLICATION PUBLICATIONS Remove

Examiner Initial*	Cite No	Publication Number	Kind Code[1]	Publication Date	Name of Patentee or Applicant of cited Document	Pages,Columns,Lines where Relevant Passages or Relevant Figures Appear
	1	20020004647	A1	2002-01-10	LEONG	
	2	20020004647	A1	2003-06-05	LEONG	

INFORMATION DISCLOSURE STATEMENT BY APPLICANT (Not for submission under 37 CFR 1.99)		
	Application Number	
	Filing Date	2018-05-31
	First Named Inventor	Bobby E. Rogers et al.
	Art Unit	
	Examiner Name	
	Attorney Docket Number	251102.000027.KURIN2CON2

	3	20003208151	A1	2003-11-06	KRAUS et al	
	4	20040054333	A1	2004-03-18	THEEUWES et al	
	5	20040073171	A1	2004-04-15	ROGERS et al	
	6	20040147855	A1	2004-07-29	MARSDEN	
	7	20050004524	A1	2005-01-06	NEWBY et al	
	8	20050240161	A1	2005-10-27	CRAWFORD	
	9	20070088279	A1	2007-04-19	SHUE et al	
	10	20080145933	A1	2008-06-19	PATTON et al	
	11	20090227953	A1	2009-09-10	TAN et al	
	12	20100057004	A1	2010-03-04	CHRISTENSEN et al	
	13	20130317391	A1	2013-11-28	BULLINGTON et al	

INFORMATION DISCLOSURE STATEMENT BY APPLICANT (**Not for submission under 37 CFR 1.99)**		
	Application Number	
	Filing Date	2018-05-31
	First Named Inventor	Bobby E. Rogers et al.
	Art Unit	
	Examiner Name	
	Attorney Docket Number	251102.000027.KURIN2CON2

	14	20160174888	A1	2016-06-23	BERTHIER et al	
	15	20170020427	A1	2017-01-26	ROGERS et al	
	16	20170020428	A1	2017-01-26	ROGERS et al	

If you wish to add additional U.S. Published Application citation information please click the Add button.

FOREIGN PATENT DOCUMENTS

Examiner Initial*	Cite No	Foreign Document Number[3]	Country Code[2] i	Kind Code[4]	Publication Date	Name of Patentee or Applicant of cited Document	Pages,Columns,Lines where Relevant Passages or Relevant Figures Appear	T[5]
	1	H08257018	JP	A	1996-10-08	NISSHO KK		☐
	2	1665986	EP	A1	2006-06-07	BECTON DICKINSON CO		☐
	3	2011162772	WO	A2	2011-12-29	CLEARVIEW PATIENT SAFETY TECHNOLOGIES LLC et al		☐

If you wish to add additional Foreign Patent Document citation information please click the Add button

NON-PATENT LITERATURE DOCUMENTS

Examiner Initials*	Cite No	Include name of the author (in CAPITAL LETTERS), title of the article (when appropriate), title of the item (book, magazine, journal, serial, symposium, catalog, etc), date, pages(s), volume-issue number(s), publisher, city and/or country where published.	T[5]
	1		☐

If you wish to add additional non-patent literature document citation information please click the Add button

INFORMATION DISCLOSURE STATEMENT BY APPLICANT (**Not for submission under 37 CFR 1.99)**		
	Application Number	
	Filing Date	2018-05-31
	First Named Inventor	Bobby E. Rogers et al.
	Art Unit	
	Examiner Name	
	Attorney Docket Number	251102.000027.KURIN2CON2

EXAMINER SIGNATURE			
Examiner Signature		Date Considered	

*EXAMINER: Initial if reference considered, whether or not citation is in conformance with MPEP 609. Draw line through a citation if not in conformance and not considered. Include copy of this form with next communication to applicant.

[1] See Kind Codes of USPTO Patent Documents at www.USPTO.GOV or MPEP 901.04. [2] Enter office that issued the document, by the two-letter code (WIPO Standard ST.3). [3] For Japanese patent documents, the indication of the year of the reign of the Emperor must precede the serial number of the patent document. [4] Kind of document by the appropriate symbols as indicated on the document under WIPO Standard ST.16 if possible. [5] Applicant is to place a check mark here if English language translation is attached.

INFORMATION DISCLOSURE STATEMENT BY APPLICANT (**Not for submission under 37 CFR 1.99)**		
	Application Number	
	Filing Date	2018-05-31
	First Named Inventor	Bobby E. Rogers et al.
	Art Unit	
	Examiner Name	
	Attorney Docket Number	251102.000027.KURIN2CON2

CERTIFICATION STATEMENT

Please see 37 CFR 1.97 and 1.98 to make the appropriate selection(s):

☐ That each item of information contained in the information disclosure statement was first cited in any communication from a foreign patent office in a counterpart foreign application not more than three months prior to the filing of the information disclosure statement. See 37 CFR 1.97(e)(1).

OR

☐ That no item of information contained in the information disclosure statement was cited in a communication from a foreign patent office in a counterpart foreign application, and, to the knowledge of the person signing the certification after making reasonable inquiry, no item of information contained in the information disclosure statement was known to any individual designated in 37 CFR 1.56(c) more than three months prior to the filing of the information disclosure statement. See 37 CFR 1.97(e)(2).

☐ See attached certification statement.

☐ The fee set forth in 37 CFR 1.17 (p) has been submitted herewith.

☒ A certification statement is not submitted herewith.

SIGNATURE

A signature of the applicant or representative is required in accordance with CFR 1.33, 10.18. Please see CFR 1.4(d) for the form of the signature.

Signature	/David Devernoe/	Date (YYYY-MM-DD)	2018-05-31
Name/Print	David Devernoe	Registration Number	50,128

This collection of information is required by 37 CFR 1.97 and 1.98. The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.14. This collection is estimated to take 1 hour to complete, including gathering, preparing and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. **SEND TO: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.**

Doc Code: TRACK1.REQ
Document Description: TrackOne Request

PTO/AIA/424 (04-14)

CERTIFICATION AND REQUEST FOR PRIORITIZED EXAMINATION UNDER 37 CFR 1.102(e) (Page 1 of 1)

First Named Inventor:	Bobby E. ROGERS	Nonprovisional Application Number (if known):	Not Yet Assigned
Title of Invention:	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAINMENT SEQUESTRATION DEVICE AND METHOD		

APPLICANT HEREBY CERTIFIES THE FOLLOWING AND REQUESTS PRIORITIZED EXAMINATION FOR THE ABOVE-IDENTIFIED APPLICATION.

1. The processing fee set forth in 37 CFR 1.17(i)(1) and the prioritized examination fee set forth in 37 CFR 1.17(c) have been filed with the request. The publication fee requirement is met because that fee, set forth in 37 CFR 1.18(d), is currently $0. The basic filing fee, search fee, and examination fee are filed with the request or have been already been paid. I understand that any required excess claims fees or application size fee must be paid for the application.

2. I understand that the application may not contain, or be amended to contain, more than four independent claims, more than thirty total claims, or any multiple dependent claims, and that any request for an extension of time will cause an outstanding Track I request to be dismissed.

3. The applicable box is checked below:

I. ☑ Original Application (Track One) - Prioritized Examination under § 1.102(e)(1)

i. (a) The application is an original nonprovisional utility application filed under 35 U.S.C. 111(a). This certification and request is being filed with the utility application via EFS-Web.

---OR---

(b) The application is an original nonprovisional plant application filed under 35 U.S.C. 111(a). This certification and request is being filed with the plant application in paper.

ii. An executed inventor's oath or declaration under 37 CFR 1.63 or 37 CFR 1.64 for each inventor, **or** the application data sheet meeting the conditions specified in 37 CFR 1.53(f)(3)(i) is filed with the application.

II. ☐ Request for Continued Examination - Prioritized Examination under § 1.102(e)(2)

i. A request for continued examination has been filed with, or prior to, this form.
ii. If the application is a utility application, this certification and request is being filed via EFS-Web.
iii. The application is an original nonprovisional utility application filed under 35 U.S.C. 111(a), or is a national stage entry under 35 U.S.C. 371.
iv. This certification and request is being filed prior to the mailing of a first Office action responsive to the request for continued examination.
v. No prior request for continued examination has been granted prioritized examination status under 37 CFR 1.102(e)(2).

Signature /David Devernoe/	Date May 31, 2018
Name (Print/Typed) David Devernoe	Practitioner Registration Number 50,128

Note: *This form must be signed in accordance with 37 CFR 1.33. See 37 CFR 1.4(d) for signature requirements and certifications. Submit multiple forms if more than one signature is required.**

☑ *Total of 1 forms are submitted.

Electronic Patent Application Fee Transmittal

Application Number:	
Filing Date:	
Title of Invention:	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD
First Named Inventor/Applicant Name:	Bobby E. ROGERS
Filer:	David Lynn Devernoe/Lisa Leao
Attorney Docket Number:	251102.000027.KURIN2CON2

Filed as Small Entity

Filing Fees for Track I Prioritized Examination - Nonprovisional Application under 35 USC 111(a)

Description	Fee Code	Quantity	Amount	Sub-Total in USD($)
Basic Filing:				
UTILITY FILING FEE (ELECTRONIC FILING)	4011	1	75	75
UTILITY SEARCH FEE	2111	1	330	330
UTILITY EXAMINATION FEE	2311	1	380	380
REQUEST FOR PRIORITIZED EXAMINATION	2817	1	2000	2000
Pages:				
Claims:				
CLAIMS IN EXCESS OF 20	2202	6	50	300
Miscellaneous-Filing:				

Description	Fee Code	Quantity	Amount	Sub-Total in USD($)
PROCESSING FEE, EXCEPT PROV. APPLS.	2830	1	70	70
Petition:				
Patent-Appeals-and-Interference:				
Post-Allowance-and-Post-Issuance:				
Extension-of-Time:				
Miscellaneous:				
		Total in USD ($)		**3155**

Electronic Acknowledgement Receipt	
EFS ID:	32773490
Application Number:	15994559
International Application Number:	
Confirmation Number:	4704
Title of Invention:	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD
First Named Inventor/Applicant Name:	Bobby E. ROGERS
Customer Number:	153290
Filer:	David Lynn Devernoe/Lisa Leao
Filer Authorized By:	David Lynn Devernoe
Attorney Docket Number:	251102.000027.KURIN2CON2
Receipt Date:	31-MAY-2018
Filing Date:	
Time Stamp:	16:50:54
Application Type:	Utility under 35 USC 111(a)

Payment information:

Submitted with Payment	yes
Payment Type	DA
Payment was successfully received in RAM	$3155
RAM confirmation Number	060118INTEFSW00003753201507
Deposit Account	
Authorized User	
The Director of the USPTO is hereby authorized to charge indicated fees and credit any overpayment as follows:	

File Listing:

Document Number	Document Description	File Name	File Size(Bytes)/ Message Digest	Multi Part /.zip	Pages (if appl.)
1	Transmittal of New Application	Transmittal_KURIN2CON2.pdf	116143 d08aac5f0f60c33834b30de848681c0a70ebd931	no	1
Warnings:					
Information:					
2		Specification_KURIN2CON2.pdf	257220 3b4fc199530104b89e7888aa3e1fed89b3bff3dd	yes	39

	Multipart Description/PDF files in .zip description		
	Document Description	**Start**	**End**
	Specification	1	32
	Claims	33	38
	Abstract	39	39

Warnings:					
Information:					
3	Drawings-only black and white line drawings	Drawings_KURIN2CON2.pdf	526629 29a13a440e81ade7ec7b5f32c8436b00dc27e9ca	no	50
Warnings:					
Information:					
4	Oath or Declaration filed	Declarations_KURIN2CON2.pdf	1037448 d722d45bfb26d38bc53cf5b4e4599451f971b65c	no	3
Warnings:					
Information:					
5	Application Data Sheet	ADS_KURIN2CON2.pdf	86321 56a19dbac28ea7aefb89d615cd3c302d91159d74	no	8

Warnings:					
Information:					
This is not an USPTO supplied ADS fillable form					
6	Power of Attorney	POA_KURIN2CON2.pdf	532300 b706bab3c5c2756e77581d71a60ecb73e767b5e2	no	2
Warnings:					
Information:					
7	Information Disclosure Statement (IDS) Form (SB08)	IDS_KURIN2CON2.pdf	79914 3f38275e7dbef08278d3cac07dd4d25e36fe81d4	no	7
Warnings:					
Information:					
This is not an USPTO supplied IDS fillable form					
8	TrackOne Request	Track1_Request_KURIN2CON2.pdf	72465 978756d5ad493810504bc1016c2a54bad31fea16	no	1
Warnings:					
Information:					
9	Fee Worksheet (SB06)	fee-info.pdf	39909 cfbacea4dc10a41383eb9305836526f30b21063c	no	2
Warnings:					
Information:					
		Total Files Size (in bytes):	2748349		

This Acknowledgement Receipt evidences receipt on the noted date by the USPTO of the indicated documents, characterized by the applicant, and including page counts, where applicable. It serves as evidence of receipt similar to a Post Card, as described in MPEP 503.

New Applications Under 35 U.S.C. 111

If a new application is being filed and the application includes the necessary components for a filing date (see 37 CFR 1.53(b)-(d) and MPEP 506), a Filing Receipt (37 CFR 1.54) will be issued in due course and the date shown on this Acknowledgement Receipt will establish the filing date of the application.

National Stage of an International Application under 35 U.S.C. 371

If a timely submission to enter the national stage of an international application is compliant with the conditions of 35 U.S.C. 371 and other applicable requirements a Form PCT/DO/EO/903 indicating acceptance of the application as a national stage submission under 35 U.S.C. 371 will be issued in addition to the Filing Receipt, in due course.

New International Application Filed with the USPTO as a Receiving Office

If a new international application is being filed and the international application includes the necessary components for an international filing date (see PCT Article 11 and MPEP 1810), a Notification of the International Application Number and of the International Filing Date (Form PCT/RO/105) will be issued in due course, subject to prescriptions concerning national security, and the date shown on this Acknowledgement Receipt will establish the international filing date of the application.

UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

APPLICATION NUMBER	FILING OR 371(C) DATE	FIRST NAMED APPLICANT	ATTY. DOCKET NO./TITLE
15/994,559	05/31/2018	Bobby E. Rogers	251102.000027.KURIN2CON2

CONFIRMATION NO. 4704

153290
TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 3000
Atlanta, GA 30308-2219

FORMALITIES LETTER

OC000000100465755

Date Mailed: 06/22/2018

NOTICE TO FILE CORRECTED APPLICATION PAPERS

Filing Date Granted

An application number and filing date have been accorded to this application. The application is informal since it does not comply with the regulations for the reason(s) indicated below. Applicant is given TWO MONTHS from the date of this Notice within which to correct the informalities indicated below. Extensions of time may be obtained by filing a petition accompanied by the extension fee under the provisions of 37 CFR 1.136(a).

The required item(s) identified below must be timely submitted to avoid abandonment:

- A substitute specification in compliance with 37 CFR 1.52, 1.121(b)(3), and 1.125, is required. The substitute specification must be submitted with markings and be accompanied by a clean version (without markings) as set forth in 37 CFR 1.125(c) and a statement that the substitute specification contains no new matter (see 37 CFR 1.125(b)). The specification, claims, and/or abstract page(s) submitted is not acceptable and cannot be scanned or properly stored because:
  - The application contains drawings, but the specification does not contain a brief description of the several views of the drawings as required by 37 CFR 1.74 and 37 CFR 1.77(b)(9).

Applicant is cautioned that correction of the above items may cause the specification and drawings page count to exceed 100 pages. If the specification and drawings exceed 100 pages, applicant will need to submit the required application size fee.

- Additional claim fees of $ **230** as a small entity, including any required multiple dependent claim fee, are required. Applicant must submit the additional claim fees or cancel the additional claims for which fees are due.

SUMMARY OF FEES DUE:

The fee(s) required within **TWO MONTHS** from the date of this Notice to avoid abandonment is/are itemized below. Small entity discount is in effect. If applicant is qualified for micro entity status, an acceptable Certification of Micro Entity Status must be submitted to establish micro entity status. (See 37 CFR 1.29 and forms PTO/SB/15A and 15B.)

- $ **230** for **1** independent claims over 3.
- $(**0**) previous unapplied payment amount.
- $ **230** TOTAL FEE BALANCE DUE.

Replies must be received in the USPTO within the set time period or must include a proper Certificate of Mailing or Transmission under 37 CFR 1.8 with a mailing or transmission date within the set time period. For more information and a suggested format, see Form PTO/SB/92 and MPEP 512.

Replies should be mailed to:

Mail Stop Missing Parts
Commissioner for Patents
P.O. Box 1450
Alexandria VA 22313-1450

Registered users of EFS-Web may alternatively submit their reply to this notice via EFS-Web, including a copy of this Notice and selecting the document description "Applicant response to Pre-Exam Formalities Notice". https://sportal.uspto.gov/authenticate/AuthenticateUserLocalEPF.html

For more information about EFS-Web please call the USPTO Electronic Business Center at 1-866-217-9197 or visit our website at http://www.uspto.gov/ebc.

If you are not using EFS-Web to submit your reply, you must include a copy of this notice.

Questions about the contents of this notice and the requirements it sets forth should be directed to the Office of Data Management, Application Assistance Unit, at **(571) 272-4000** or **(571) 272-4200** or **1-888-786-0101**.

/jmilani/

PATENT APPLICATION FEE DETERMINATION RECORD

Substitute for Form PTO-875

Application or Docket Number: 15/994,559

APPLICATION AS FILED - PART I

FOR	(Column 1) NUMBER FILED	(Column 2) NUMBER EXTRA	SMALL ENTITY RATE($)	SMALL ENTITY FEE($)	OR	OTHER THAN SMALL ENTITY RATE($)	OTHER THAN SMALL ENTITY FEE($)
BASIC FEE (37 CFR 1.16(a), (b), or (c))	N/A	N/A	N/A	75		N/A	
SEARCH FEE (37 CFR 1.16(k), (i), or (m))	N/A	N/A	N/A	330		N/A	
EXAMINATION FEE (37 CFR 1.16(o), (p), or (q))	N/A	N/A	N/A	380		N/A	
TOTAL CLAIMS (37 CFR 1.16(i))	26 minus 20 =	* 6	x 50 =	300	OR		
INDEPENDENT CLAIMS (37 CFR 1.16(h))	4 minus 3 =	* 1	x 230 =	230			
APPLICATION SIZE FEE (37 CFR 1.16(s))	If the specification and drawings exceed 100 sheets of paper, the application size fee due is $310 ($155 for small entity) for each additional 50 sheets or fraction thereof. See 35 U.S.C. 41(a)(1)(G) and 37 CFR 1.16(s).			0.00			
MULTIPLE DEPENDENT CLAIM PRESENT (37 CFR 1.16(j))				0.00			
* If the difference in column 1 is less than zero, enter "0" in column 2.			TOTAL	1315		TOTAL	

APPLICATION AS AMENDED - PART II

AMENDMENT A

	(Column 1) CLAIMS REMAINING AFTER AMENDMENT		(Column 2) HIGHEST NUMBER PREVIOUSLY PAID FOR	(Column 3) PRESENT EXTRA	SMALL ENTITY RATE($)	SMALL ENTITY ADDITIONAL FEE($)	OR	OTHER THAN SMALL ENTITY RATE($)	OTHER THAN SMALL ENTITY ADDITIONAL FEE($)
Total (37 CFR 1.16(i))	*	Minus	**	=	x =		OR	x =	
Independent (37 CFR 1.16(h))	*	Minus	***	=	x =		OR	x =	
Application Size Fee (37 CFR 1.16(s))									
FIRST PRESENTATION OF MULTIPLE DEPENDENT CLAIM (37 CFR 1.16(j))							OR		
					TOTAL ADD'L FEE		OR	TOTAL ADD'L FEE	

AMENDMENT B

	(Column 1) CLAIMS REMAINING AFTER AMENDMENT		(Column 2) HIGHEST NUMBER PREVIOUSLY PAID FOR	(Column 3) PRESENT EXTRA	RATE($)	ADDITIONAL FEE($)		RATE($)	ADDITIONAL FEE($)
Total (37 CFR 1.16(i))	*	Minus	**	=	x =		OR	x =	
Independent (37 CFR 1.16(h))	*	Minus	***	=	x =		OR	x =	
Application Size Fee (37 CFR 1.16(s))									
FIRST PRESENTATION OF MULTIPLE DEPENDENT CLAIM (37 CFR 1.16(j))							OR		
					TOTAL ADD'L FEE		OR	TOTAL ADD'L FEE	

* If the entry in column 1 is less than the entry in column 2, write "0" in column 3.
** If the "Highest Number Previously Paid For" IN THIS SPACE is less than 20, enter "20".
*** If the "Highest Number Previously Paid For" IN THIS SPACE is less than 3, enter "3".
The "Highest Number Previously Paid For" (Total or Independent) is the highest found in the appropriate box in column 1.

UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

APPLICATION NUMBER	FILING or 371(c) DATE	GRP ART UNIT	FIL FEE REC'D	ATTY.DOCKET.NO	TOT CLAIMS	IND CLAIMS
15/994,559	05/31/2018	1629	1085	251102.000027.KURIN2CON2	26	4

CONFIRMATION NO. 4704

153290
TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 3000
Atlanta, GA 30308-2219

FILING RECEIPT

OC000000100485734

Date Mailed: 06/22/2018

Receipt is acknowledged of this non-provisional patent application. The application will be taken up for examination in due course. Applicant will be notified as to the results of the examination. Any correspondence concerning the application must include the following identification information: the U.S. APPLICATION NUMBER, FILING DATE, NAME OF APPLICANT, and TITLE OF INVENTION. Fees transmitted by check or draft are subject to collection. Please verify the accuracy of the data presented on this receipt. **If an error is noted on this Filing Receipt, please submit a written request for a Filing Receipt Correction. Please provide a copy of this Filing Receipt with the changes noted thereon. If you received a "Notice to File Missing Parts" for this application, please submit any corrections to this Filing Receipt with your reply to the Notice. When the USPTO processes the reply to the Notice, the USPTO will generate another Filing Receipt incorporating the requested corrections**

Inventor(s)

Bobby E. Rogers, San Diego, CA;
Gino Kang, Irvine, CA;
John Detloff, San Diego, CA;

Applicant(s)

KURIN, INC., San Diego, CA;

Assignment For Published Patent Application

KURIN, INC., San Diego, CA

Power of Attorney: The patent practitioners associated with Customer Number 153290

Domestic Priority data as claimed by applicant

This application is a CON of 15/140,448 04/27/2016 PAT 10010282
which claims benefit of 62/196,797 07/24/2015
and claims benefit of 62/238,636 10/07/2015
and claims benefit of 62/318,194 04/04/2016

Foreign Applications for which priority is claimed (You may be eligible to benefit from the **Patent Prosecution Highway** program at the USPTO. Please see http://www.uspto.gov for more information.) - None.
Foreign application information must be provided in an Application Data Sheet in order to constitute a claim to foreign priority. See 37 CFR 1.55 and 1.76.

Permission to Access Application via Priority Document Exchange: Yes

Permission to Access Search Results: Yes

Applicant may provide or rescind an authorization for access using Form PTO/SB/39 or Form PTO/SB/69 as appropriate.

If Required, Foreign Filing License Granted: 06/21/2018
The country code and number of your priority application, to be used for filing abroad under the Paris Convention, is **US 15/994,559**
Projected Publication Date: To Be Determined - pending completion of Corrected Papers
Non-Publication Request: No
Early Publication Request: No
**** SMALL ENTITY ****
Title

BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD

Preliminary Class

514

Statement under 37 CFR 1.55 or 1.78 for AIA (First Inventor to File) Transition Applications: No

PROTECTING YOUR INVENTION OUTSIDE THE UNITED STATES

Since the rights granted by a U.S. patent extend only throughout the territory of the United States and have no effect in a foreign country, an inventor who wishes patent protection in another country must apply for a patent in a specific country or in regional patent offices. Applicants may wish to consider the filing of an international application under the Patent Cooperation Treaty (PCT). An international (PCT) application generally has the same effect as a regular national patent application in each PCT-member country. The PCT process **simplifies** the filing of patent applications on the same invention in member countries, but **does not result** in a grant of "an international patent" and does not eliminate the need of applicants to file additional documents and fees in countries where patent protection is desired.

Almost every country has its own patent law, and a person desiring a patent in a particular country must make an application for patent in that country in accordance with its particular laws. Since the laws of many countries differ in various respects from the patent law of the United States, applicants are advised to seek guidance from specific foreign countries to ensure that patent rights are not lost prematurely.

Applicants also are advised that in the case of inventions made in the United States, the Director of the USPTO must issue a license before applicants can apply for a patent in a foreign country. The filing of a U.S. patent application serves as a request for a foreign filing license. The application's filing receipt contains further information and guidance as to the status of applicant's license for foreign filing.

Applicants may wish to consult the USPTO booklet, "General Information Concerning Patents" (specifically, the section entitled "Treaties and Foreign Patents") for more information on timeframes and deadlines for filing foreign patent applications. The guide is available either by contacting the USPTO Contact Center at 800-786-9199, or it can be viewed on the USPTO website at http://www.uspto.gov/web/offices/pac/doc/general/index.html.

For information on preventing theft of your intellectual property (patents, trademarks and copyrights), you may wish to consult the U.S. Government website, http://www.stopfakes.gov. Part of a Department of Commerce initiative, this website includes self-help "toolkits" giving innovators guidance on how to protect intellectual property in specific

countries such as China, Korea and Mexico. For questions regarding patent enforcement issues, applicants may call the U.S. Government hotline at 1-866-999-HALT (1-866-999-4258).

LICENSE FOR FOREIGN FILING UNDER

Title 35, United States Code, Section 184

Title 37, Code of Federal Regulations, 5.11 & 5.15

GRANTED

The applicant has been granted a license under 35 U.S.C. 184, if the phrase "IF REQUIRED, FOREIGN FILING LICENSE GRANTED" followed by a date appears on this form. Such licenses are issued in all applications where the conditions for issuance of a license have been met, regardless of whether or not a license may be required as set forth in 37 CFR 5.15. The scope and limitations of this license are set forth in 37 CFR 5.15(a) unless an earlier license has been issued under 37 CFR 5.15(b). The license is subject to revocation upon written notification. The date indicated is the effective date of the license, unless an earlier license of similar scope has been granted under 37 CFR 5.13 or 5.14.

This license is to be retained by the licensee and may be used at any time on or after the effective date thereof unless it is revoked. This license is automatically transferred to any related applications(s) filed under 37 CFR 1.53(d). This license is not retroactive.

The grant of a license does not in any way lessen the responsibility of a licensee for the security of the subject matter as imposed by any Government contract or the provisions of existing laws relating to espionage and the national security or the export of technical data. Licensees should apprise themselves of current regulations especially with respect to certain countries, of other agencies, particularly the Office of Defense Trade Controls, Department of State (with respect to Arms, Munitions and Implements of War (22 CFR 121-128)); the Bureau of Industry and Security, Department of Commerce (15 CFR parts 730-774); the Office of Foreign AssetsControl, Department of Treasury (31 CFR Parts 500+) and the Department of Energy.

NOT GRANTED

No license under 35 U.S.C. 184 has been granted at this time, if the phrase "IF REQUIRED, FOREIGN FILING LICENSE GRANTED" DOES NOT appear on this form. Applicant may still petition for a license under 37 CFR 5.12, if a license is desired before the expiration of 6 months from the filing date of the application. If 6 months has lapsed from the filing date of this application and the licensee has not received any indication of a secrecy order under 35 U.S.C. 181, the licensee may foreign file the application pursuant to 37 CFR 5.15(b).

SelectUSA

The United States represents the largest, most dynamic marketplace in the world and is an unparalleled location for business investment, innovation, and commercialization of new technologies. The U.S. offers tremendous resources and advantages for those who invest and manufacture goods here. Through SelectUSA, our nation works to promote and facilitate business investment. SelectUSA provides information assistance to the international investor community; serves as an ombudsman for existing and potential investors; advocates on behalf of U.S. cities, states, and regions competing for global investment; and counsels U.S. economic development organizations on investment attraction best practices. To learn more about why the United States is the best country in the world to develop

technology, manufacture products, deliver services, and grow your business, visit http://www.SelectUSA.gov or call +1-202-482-6800.

To: ryan.schneider@troutman.com,patents@troutman.com,chris.franich@troutman.com
From: PAIR_eOfficeAction@uspto.gov
Cc: PAIR_eOfficeAction@uspto.gov
Subject: Private PAIR Correspondence Notification for Customer Number 153290

Jun 22, 2018 04:09:40 AM

Dear PAIR Customer:

TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 3000
Atlanta, GA 30308-2219
UNITED STATES

The following USPTO patent application(s) associated with your Customer Number, 153290 , have new outgoing correspondence. This correspondence is now available for viewing in Private PAIR.

The official date of notification of the outgoing correspondence will be indicated on the form PTOL-90 accompanying the correspondence.

Disclaimer:
The list of documents shown below is provided as a courtesy and is not part of the official file wrapper. The content of the images shown in PAIR is the official record.

Application	Document	Mailroom Date	Attorney Docket No.
15994559	NT.CR.APP.PA	06/22/2018	251102.000027.KURIN2CON2
	APP.FILE.REC	06/22/2018	251102.000027.KURIN2CON2

To view your correspondence online or update your email addresses, please visit us anytime at https://sportal.uspto.gov/secure/myportal/privatepair.

If you have any questions, please email the Electronic Business Center (EBC) at EBC@uspto.gov with 'e-Office Action' on the subject line or call 1-866-217-9197 during the following hours:

Monday - Friday 6:00 a.m. to 12:00 a.m.

Thank you for prompt attention to this notice,

UNITED STATES PATENT AND TRADEMARK OFFICE

PATENT APPLICATION INFORMATION RETRIEVAL SYSTEM

PATENT

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

In re Patent Application of:	Customer No.: 153290
ROGERS, Bobby E. *et al.*	Confirmation No.: 4704
Serial No.: 15/994,559	Group Art Unit: 1629
Filing Date: May 31, 2018	Examiner: TBD
For: Blood sample optimization system and blood contaminant sequestration device and method	Docket No.: 251102.000027.KURIN2CON2

RESPONSE TO NOTICE TO FILE CORRECTED APPLICATION PAPERS

Mail Stop: Missing Parts
Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

Dear Commissioner:

This paper is filed in response to the *Notice to File Corrected Application Papers* ("*Notice*") mailed on June 22, 2018 for which a response is due August 22, 2018. Applicant respectfully submits this response is considered to be timely filed.

Applicant submits the following documents as requested by the office:

- A marked-up copy of the Substitute Specification;
- A clean copy of the Substitute Specification; and
- Additional claim fees of $230.

The Notice indicates that Applicant must submit a substitute specification in compliance with 37 CFR §§ 1.52, 1.121(b)(3), and 1.125. In response, Applicant hereby submits a substitute specification with markings accompanied by a clean version of the specification (without markings), as set forth in 37 CFR § 1.125(c). The specification has been formatted to conform with U.S. practice. Applicant hereby states that the substitute specification contains no new matter.

The Notice also requires payment of $230 for additional claim sees. In response, Applicant submits the additional claim fees of $230 for one independent claim in excess of three.

Applicant believes that the present submission is fully responsive to the Notice, and the Substitute Specification encompasses all the desired changes.

This Response to Notice to File Corrected Application Papers is being filed within two months of the Notice. Therefore, no other fees are believed due. The Commissioner is nonetheless authorized to charge any deficiency in fees to PTO Deposit Account No. 20-1507 should any fees be due.

Should the Examiner have any questions or reservations regarding the present Response to Notice to File Corrected Application Papers, the Examiner is invited to telephone the undersigned attorney at (858) 509-6065, or at david.devernoe@troutman.com

Respectfully submitted,

TROUTMAN SANDERS LLP

Date: July 2, 2018

/David Devernoe/
David Devernoe
Registration No. 50,128

Troutman Sanders LLP
11682 El Camino Real
Suite 400
San Diego, CA 92130-2092

UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

APPLICATION NUMBER	FILING OR 371(C) DATE	FIRST NAMED APPLICANT	ATTY. DOCKET NO./TITLE
15/994,559	05/31/2018	Bobby E. Rogers	251102.000027.KURIN2CON2

CONFIRMATION NO. 4704

153290
TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 3000
Atlanta, GA 30308-2219

FORMALITIES LETTER

OC000000100465755

Date Mailed: 06/22/2018

NOTICE TO FILE CORRECTED APPLICATION PAPERS

Filing Date Granted

An application number and filing date have been accorded to this application. The application is informal since it does not comply with the regulations for the reason(s) indicated below. Applicant is given TWO MONTHS from the date of this Notice within which to correct the informalities indicated below. Extensions of time may be obtained by filing a petition accompanied by the extension fee under the provisions of 37 CFR 1.136(a).

The required item(s) identified below must be timely submitted to avoid abandonment:

- A substitute specification in compliance with 37 CFR 1.52, 1.121(b)(3), and 1.125, is required. The substitute specification must be submitted with markings and be accompanied by a clean version (without markings) as set forth in 37 CFR 1.125(c) and a statement that the substitute specification contains no new matter (see 37 CFR 1.125(b)). The specification, claims, and/or abstract page(s) submitted is not acceptable and cannot be scanned or properly stored because:
  - The application contains drawings, but the specification does not contain a brief description of the several views of the drawings as required by 37 CFR 1.74 and 37 CFR 1.77(b)(9).

Applicant is cautioned that correction of the above items may cause the specification and drawings page count to exceed 100 pages. If the specification and drawings exceed 100 pages, applicant will need to submit the required application size fee.

- Additional claim fees of $ **230** as a small entity, including any required multiple dependent claim fee, are required. Applicant must submit the additional claim fees or cancel the additional claims for which fees are due.

SUMMARY OF FEES DUE:

The fee(s) required within **TWO MONTHS** from the date of this Notice to avoid abandonment is/are itemized below. Small entity discount is in effect. If applicant is qualified for micro entity status, an acceptable Certification of Micro Entity Status must be submitted to establish micro entity status. (See 37 CFR 1.29 and forms PTO/SB/15A and 15B.)

- $ **230** for **1** independent claims over 3.
- $(**0**) previous unapplied payment amount.
- $ **230** TOTAL FEE BALANCE DUE.

Replies must be received in the USPTO within the set time period or must include a proper Certificate of Mailing or Transmission under 37 CFR 1.8 with a mailing or transmission date within the set time period. For more information and a suggested format, see Form PTO/SB/92 and MPEP 512.

Replies should be mailed to:

Mail Stop Missing Parts
Commissioner for Patents
P.O. Box 1450
Alexandria VA 22313-1450

Registered users of EFS-Web may alternatively submit their reply to this notice via EFS-Web, including a copy of this Notice and selecting the document description "Applicant response to Pre-Exam Formalities Notice". https://sportal.uspto.gov/authenticate/AuthenticateUserLocalEPF.html

For more information about EFS-Web please call the USPTO Electronic Business Center at 1-866-217-9197 or visit our website at http://www.uspto.gov/ebc.

If you are not using EFS-Web to submit your reply, you must include a copy of this notice.

Questions about the contents of this notice and the requirements it sets forth should be directed to the Office of Data Management, Application Assistance Unit, at **(571) 272-4000** or **(571) 272-4200** or **1-888-786-0101**.

/jmilani/

BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a Continuation of U.S. Application No. 15/140,448, filed on April 27, 2016, which claims the benefit of U.S. Provisional Application Serial No. 62/196,797, filed on July 24, 2015 and titled "BLOOD CULTURE IMPROVEMENT SYSTEM AND METHOD"; U.S. Provisional Application Serial No. 62/238,636, filed on October 7, 2015 and titled "BLOOD SEQUESTRATION SYSTEM FOR NON-CONTAMINATED BLOOD SAMPLING"; and U.S. Provisional Application Serial No. 62/318,194, filed on April 4, 2016 and titled "BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD," the disclosures of which are incorporated by reference in their entirety.

BACKGROUND

[0002] Bacteraemia is the presence of microorganisms in the blood. Sepsis, on the other hand, is bacteraemia in the presence of clinical symptoms and signs such as fever, tachycardia, tachypnea and hypotension. Bacteraemia and sepsis are associated with a high mortality and an increased incidence and duration of hospital stay and associated costs. Many bacteraemias, sepsis, fungaemias and other pathogens actually occur within a hospital or other healthcare settings with catheters and venipunctures being a source of contamination as potential carriers of these pathogens.

[0003] Blood cultures are the standard test used to detect microbial pathogens related to bacteraemia and sepsis in a patient's blood. The term blood culture refers to a single venipuncture, either from a peripheral site or central or arterial line, with the blood inoculated into one or more blood culture bottles or containers. One bottle is considered a blood culture where two or more are considered a set. Multiple sets may be obtained from multiple venipunctures and are associated with different sites on the patient.

[0004] These methods allow for microbial identification and susceptibility testing to be performed, which is a critical component to managing sepsis, however the lack of rapid results and decreased sensitivity for fastidious pathogens has led to the development of improved systems and adjunctive molecular or proteomic testing.

[0005] Collection of blood samples for conducting blood cultures is a critical component of modern patient care and can either positively affect the patient outcome by providing an accurate diagnosis, or can adversely affect the outcome by prolonging unnecessary antimicrobial therapy, the length of hospital stays, and increasing costs.

[0006] One outcome of collection of blood cultures is contamination. Blood culture contamination can lead to a false positive culture result and/or significant increase in healthcare related costs. Sources of blood culture contamination include improper skin antisepsis, improper collection tube disinfection, and contamination of the initial blood draw which may then skew results.

[0007] Blood culture collection kits generally consist of a "butterfly" set, infusion set, or other type of venipuncture device as offered by companies like BD, Smiths, B. Braun and others, and aerobic and anaerobic blood culture bottles. Various different bottles are also available depending on the test requirements. These bottles are specifically designed to optimize recovery of both aerobic and anaerobic organisms. In conventional kits, a bottle used is known generally as a "Vacutainer," which is a blood collection tube formed of a sterile glass or plastic tube with a closure that is evacuated to create a vacuum inside the tube to facilitate the draw of a predetermined volume of liquid such as blood.

[0008] False positive blood cultures are typically a result of poor sampling techniques. They cause the use of antibiotics when not needed, increasing hospital costs and patient anxiety. Blood cultures are drawn from a needlestick into the skin, and then a Vacutainer is attached to capture a sample of blood. Contamination may occur from improper or incomplete disinfection of the skin area in and around the puncture site. It may also occur from the coring of the skin by the needle during insertion, with the cored skin cells and any associated contamination being pulled into the sample.

[0009] Blood flow through a hypodermic needle is laminar, and as such, a velocity gradient can be developed over the flow tube as a pressure drop is applied to the hypodermic needle. Either forceful aspiration of blood, or using a very small hypodermic needle, can cause lysis and a release of potassium from the red blood cells, thereby rendering the blood samples abnormal.

[0010] In other instances, some patients have delicate veins that can collapse under a pressure drop or vacuum, particularly as applied by a syringe's plunger that is drawn too quickly for the patient's condition. Since such condition is impossible to know beforehand, such vein collapses are a risk and very difficult to control.

[0011] Various strategies have been implemented to decrease blood culture contamination rates, e.g. training staff with regard to aseptic collection technique, feedback with regard to contamination rates and implementation of blood culture collection kits. Although skin antisepsis can reduce the burden of contamination, 20% or more of skin organisms are located deep within the dermis and are unaffected by antisepsis. Changing needles before bottle inoculation is not advisable as it increases the risk to acquire needle stick injuries without decreasing contamination rates.

[0012] Some conventional systems and techniques for reducing blood culture contamination include discarding the initial aliquot of blood taken from central venous catheters, venipunctures, and other vascular access systems. However, these systems require the user to mechanically manipulate an intravascular device, or require a complex series of steps that are difficult to ensure being followed.

SUMMARY

[0013] This document presents systems and methods for reducing blood culture contamination, lysing of cells, and vein collapse. In some implementations, a system and method can eliminate user variability in disinfection, and also eliminate the risk of skin cells getting into the blood culture sample. The systems and methods disclosed herein do not require a change in existing clinical processes, other than to potentially indicate when a vacutainer or other blood collection device (i.e., syringe) should be attached for drawing contaminant-free blood samples.

[0014] In some implementations of the systems and methods disclosed herein the withdrawal of blood is accomplished passively by use of the patient's own blood pressure, thereby reducing the risk of vein collapse and eliminating any additional user steps over current practice. The systems and methods can be applied to accommodate short-path direct stick or butterfly venipuncture systems. They can also be used with samples drawn through a catheter.

[0015] In one aspect, a blood sequestration device is presented. The blood sequestration device includes an inlet port and an outlet port. The blood sequestration device further includes a sequestration chamber connected with the inlet port, the sequestration chamber having a vent comprising an air permeable blood barrier. The blood sequestration device further includes a sampling channel having a proximal end connected with the inlet port and a distal end connected with the outlet port.

[0016] In another aspect, a blood sequestration device connected with a blood sampling pathway is described. The blood sampling pathway has a patient needle and a sample collection device. The blood sequestration device includes an inlet port connected with the patient needle, and a sequestration chamber connected with the inlet port, the sequestration chamber having a vent comprising an air permeable blood barrier. The blood sequestration device further includes a sampling channel having a proximal end connected with the inlet port, and an outlet port connected with a distal end of the sampling channel and with the sample collection device.

[0017] In yet another aspect, a blood sequestration device connected with a blood sampling system is described. The blood sampling system includes a patient needle for accessing a blood sample from a patient, and a sample needle that is sealed and adapted for receiving an evacuated blood collection tube. The blood sequestration device includes an inlet port connected with the patient needle to receive the blood sample from the patient. The blood sequestration device further includes a sequestration chamber connected with the inlet port and having a vent comprising an air permeable blood barrier, the sequestration chamber for receiving and sequestering a first portion of the blood sample prior to the sample needle being unsealed by the evacuated blood collection tube. The blood sequestration device further includes a sampling channel having a proximal end connected with the inlet port, the

sampling channel for conveying a subsequent portion of the blood sample once the sample needle is unsealed by the evacuated blood collection tube. The blood sequestration device further includes an outlet port connected with a distal end of the sampling channel for conveying the subsequent portion of the blood sample to the sample needle.

[0018] In yet another aspect, a blood sample optimization system is disclosed and described. The blood sample optimization system includes a blood sampling system for accessing and acquiring one or more samples of a patient's blood, and a blood sequestration device for receiving and sequestering a first portion of the one or more samples of the patient's blood which might be contaminated by a venipuncture process and which could result in a false positive identification of a pathogen in the patient's blood.

[0019] The blood sampling system includes a patient needle configured for a venipuncture of a patient to access a sample of blood of a patient, a blood sampling pathway connected with the patient needle for conveying the sample of blood, and a sample needle configured for receiving an evacuated blood collection container to collect and contain a subsequent portion of the sample of blood.

[0020] In yet another aspect, a blood sequestration device is disclosed and described. In some implementations, the blood sequestration device can include an inlet port, an outlet port connected with the inlet port, and a sequestration chamber connected with the inlet port. The sequestration chamber can have a vent comprising an air permeable blood barrier.

[0021] The blood sequestration device is connected along the blood sampling pathway between the patient needle and the sample needle, and includes an inlet port for receiving the sample of blood. The blood sequestration device further includes a sequestration chamber connected with the inlet port for receiving a first amount of the sample of blood, the sequestration chamber having a vent comprising an air permeable blood barrier for sequestering at least a first portion of the first amount of the sample of blood. The blood sequestration device may further include a sampling channel having a proximal end connected with the inlet port, the sampling channel conveying a subsequent amount of the sample of blood to the evacuated blood collection container upon the sequestration chamber sequestering at least the first portion of the first amount of the sample of blood. The blood

sequestration device further includes an outlet port connected with a distal end of the sampling channel, the outlet port for outputting the subsequent amount of the sample of blood.

[0022] The details of one or more embodiments are set forth in the accompanying drawings and the description below. Other features and advantages will be apparent from the description and drawings, and from the claims.

BRIEF DESCRIPTION OF THE DRAWINGS

[0023] These and other aspects will now be described in detail with reference to the following drawings.

[0024] FIG. 1 illustrates a blood sample optimization system.

[0025] FIG. 2 illustrates a blood sample optimization system in accordance with an alternative implementation.

[0026] FIG. 3 illustrates a blood sample optimization system in accordance with another alternative implementation.

[0027] FIG. 4 illustrates a blood sample optimization system in accordance with another alternative implementation.

[0028] FIG. 5 illustrates a blood sample optimization system in accordance with another alternative implementation.

[0029] FIG. 6 illustrates a blood sample optimization system in accordance with an alternative implementation.

[0030] FIG. 7 is a flowchart of a method for optimizing a quality of a blood culture.

[0031] FIGS. 8A – 8E illustrate a blood sequestration system for non-contaminated blood sampling, in accordance with some implementations.

[0032] FIG. 9 illustrates a pathway splitter for use in a blood sequestrations system.

[0033] FIGS. 10A – 10D illustrate a blood sequestration system for non-contaminated blood sampling, in accordance with alternative implementations.

[0034] FIGS. 11A – 11E illustrate a blood sequestration system for non-contaminated blood sampling, in accordance with other alternative implementations.

[0035] FIGS. 12A-12D illustrate a blood sample optimization system including a blood sequestration device in accordance with yet other alternative implementations.

[0036] FIGS. 13A-13D illustrate a blood sample optimization system 1300 in accordance with yet another alternative implementations.

[0037] FIGS. 14A-14E illustrate yet another implementation of a blood sampling system to sequester contaminates of an initial aliquot or sample to reduce false positives in blood cultures or tests performed on a patient's blood sample.

[0038] FIGS. 15A-15G illustrate a blood sequestration device and method of using the same, in accordance with yet another implementation.

[0039] FIGS. 16A-16D illustrate a blood sequestration device in accordance with yet another implementation.

[0040] FIGS. 17A – 17**[[**D**]]**E illustrate a bottom member of a housing for a blood sequestration device.

[0041] FIGS. 18A – 18F illustrate a top member of a housing for a blood sequestration device.

[0042] FIGS. 19A and 19B illustrate a blood sequestration device having a top member mated with a bottom member.

[0043] FIG. 20 shows a blood sample optimization system including a blood sequestration device.

[0044] FIG. 21 illustrates a non-vented blood sequestration device using a wicking material chamber.

[0045] FIGS. 22A and 22B illustrate a material makeup of a filter for sequestering blood in a sequestration chamber of a blood sequestration device.

[0046] FIGS. 23A and 23B illustrate another implementation of a blood sequestration device that uses a vacuum force from a blood collection device.

[0047] Like reference symbols in the various drawings indicate like elements.

DETAILED DESCRIPTION

[0048] This document describes blood sample optimization systems and methods for reducing or eliminating contaminates in collected blood samples, which in turn reduces or eliminates false positive readings in blood cultures or other testing of collected blood samples. In some implementations, a blood sample optimization system includes a patient needle for vascular access to a patient's bloodstream, a sample needle for providing a blood sample to a blood collection container, such as an evacuated blood collection container or tube like a Vacutainer™ or the like, or other sampling device, and a blood sequestration device located between the patient needle and the sample needle. The blood sequestration device includes a sequestration chamber for sequestering an initial, potentially contaminated aliquot of blood, and may further include a sampling channel that bypasses the sequestration chamber to convey likely uncontaminated blood between the patient needle and the sample needle after the initial aliquot of blood is sequestered in the sequestration chamber.

[0049] FIG. 1 illustrates a blood sample optimization system in accordance with some implementations. The system includes a patient needle 1 to puncture the skin of a patient to access the patient's vein and blood therein. The system further includes a sample needle (i.e., a resealably closed needle for use with Vacutainers™ or the like) 5, which may be contained within and initially sealed by a resealable boot 10, a Luer activated valve, or another collection interface or device. The resealable boot 10 can be pushed aside or around the sample needle 5 by application of a Vacutainer™ bottle (not shown) for drawing the patient's blood. The system can further include a low volume chamber 30 that leads to the sample needle 5, but also includes an orifice or one or more channels 45 that lead to a sequestration chamber 55 formed by a housing 50.

[0050] The sequestration chamber 55 is a chamber, channel, pathway, lock, or other structure for receiving and holding a first aliquot of the patient's blood, which may be in a predetermined or measured amount, depending on a volume of the sequestration chamber 55. The first draw of blood typically contains or is more susceptible to containing organisms that cause bacteraemia and sepsis or other pathogens than subsequent blood draws. The sequestration chamber 55 can be a vessel encased in a solid housing, formed in or defined by the housing itself, or can be implemented as tubing or a lumen. The sequestration chamber 55, regardless how formed and implemented, may have a predetermined volume. In some implementations, the predetermined volume may be based on a volume of the patient needle, i.e. ranging from less than the volume of the patient needle to any volume up to or greater than 20 times or more of the volume of the patient needle. The predetermined volume of the sequestration chamber 55 may also be established to economize or minimize an amount of blood to be sequestered and disposed of.

[0051] The sequestration chamber 55 can be formed, contained or housed in a chamber housing 50, and can be made of plastic, rubber, steel, aluminum or other suitable material. For example, the sequestration chamber 55 could be formed of flexible tubing or other elastomeric materials. The sequestration chamber 55 further includes an air permeable blood barrier 20 that allows air to exit the sequestration chamber 55. As used herein the term "air permeable blood barrier" means an air permeable but substantially blood impermeable substance, material, or structure. Examples may include hydrophobic membranes and coatings, a hydrophilic membrane or coating combined with a hydrophobic membrane or coating, mesh, a filter, a mechanical valve, antimicrobial material, or any other means of allowing air to be displaced from the sequestration chamber 55 as it is filled with blood. In various exemplary embodiments, an air permeable blood barrier may be formed by one or more materials that allow air to pass through until contacted by a liquid, such material then becomes completely or partially sealed to prevent or inhibit the passage of air and/or liquid. In other words, prior to contact with liquid, the material forms a barrier that is air permeable. After contact with a liquid, the material substantially or completely prevents the further passage of air and/or liquid.

[0052] The orifice or channel 45 can be any desired length, cross-sectional shape or size, and/or can be formed to depart from the low volume chamber 30 at any desired angle or orientation. The orifice or channel 45 may also include a one-way flap or valve 60 that maintains an initial aliquot of blood sample within the sequestration chamber 55. In some specific implementations, the orifice or channel 45 can include a "duck bill" or flapper valve 60, or the like, for one-way flow of blood from low volume chamber 30 to the sequestration chamber 55. The air permeable blood barrier 20 can also be constructed of a material that allows air to exit but then seals upon contact with blood, thereby not allowing external air to enter sequestration chamber 55. This sealing would eliminate the need for a valve.

[0053] Valve 60 can be any type of valve or closing mechanism. Chamber 30 is designed to hold virtually no residual blood, and can be designed to be adapted to hold or allow pass-through of a particular volume or rate of blood into sequestration chamber 55. Likewise, sequestration chamber 55 may also include any type of coating, such as an anti-microbial coating, or a coating that aids identification and/or diagnosis of components of the first, sequestered blood draw.

[0054] Housing 50 and 40 can be formed of any suitable material, including plastic, such as acrylonitrile butadiene styrene (ABS) or other thermoplastic or polymeric material, rubber, steel, or aluminum. The air permeable blood barrier 20 can include a color-providing substance, or other signaling mechanism, that is activated upon contact with blood from the initial blood draw, or when air displacement is stopped, or any combination of events with blood in the sequestration chamber 55. The air permeable barrier may also include an outer layer such as a hydrophobic membrane or cover that inhibits or prevents the inadvertent or premature sealing of the filter by an external fluid source, splash etc. Sequestration chamber 55 can also be translucent or clear to enable a user to visually confirm the chamber is filled.

[0055] FIG. 2 illustrates a blood sample optimization system in accordance with some alternative implementations. In the implementation shown in FIG. 2, a sequestration chamber 55, or waste chamber, surrounds the patient needle 1, with an open-ended cuff or housing connected with the waste chamber and encircling the sample needle housing base and housing. The patient needle 1 and sample needle 5 are connected together by a boot 56, which forms a continuous blood draw channel therethrough. The boot 56 includes a single

orifice or channel leading from the blood draw channel into sequestration chamber 55. The device can include more than one single orifice or channel, in other implementations. Each orifice or channel can include a one-way valve, and can be sized and adapted for predetermined amount of blood flow.

[0056] The sequestration chamber 55 includes an air permeable blood barrier. The filter can further include a sensor or indicator to sense and/or indicate, respectively, when a predetermined volume of blood has been collected in the sequestration chamber 55. That indication will alert a user to attach an evacuated blood collection tube or bottle, such as a Vacutainer™ to the sample needle 5. The housing for the sequestration chamber 55 can be any size or shape, and can include any type of material to define an interior space or volume therein. The interior space is initially filled only with air, but can also be coated with an agent or substance, such as a decontaminate, solidifying agent, or the like. Once evacuated blood collection tube is attached to the sample needle 5, blood will flow automatically into the patient needle 1, through the blood draw channel and sample needle 5, and into the bottle. The sample needle 5 is covered by a resealable boot, coating or membrane that seals the sample needle when a blood collection bottle is not attached thereon or thereto.

[0057] FIG. 3 illustrates a blood sample optimization system in accordance with some alternative implementations. In the implementation shown, a sample needle 5 is surrounded by a resealable boot or membrane, and is further connected with a patient needle 1. A blood flow channel is formed through the sample needle and the patient needle. The connection between the sample needle and patient needle includes a "T" or "Y" connector 102, which includes a channel, port or aperture leading out from the main blood flow channel to a sequestration chamber 104.

[0058] The T or Y connector 102 may include a flap or one-way valve, and have an opening that is sized and adapted for a predetermined rate of flow of blood. The sequestration chamber 104 can be formed from tubing, or be formed by a solid housing, and is initially filled with air. The sequestration chamber 104 will receive blood that flows out of a patient automatically, i.e. under pressure from the patient's own blood pressure. The sequestration chamber 104 includes an air permeable blood barrier 106, preferably at the distal end of tubing that forms the sequestration chamber 104, and which is connected at the

proximal end to the T or Y connector 102. The T or Y connector 102 can branch off at any desired angle for most efficient blood flow, and can be formed so as to minimize an interface between the aperture and channel and the main blood flow channel, so as to minimize or eliminate mixing of the initial aliquot of blood with main blood draw samples.

[0059] In some alternative implementations, the sample needle may be affixed to a tubing of any length, as shown in FIG. 4, connecting at its opposite end to the T or Y connector 102. The sequestration chamber 104 can be any shape or volume so long as it will contain a predetermined amount of blood sample in the initial aliquot. The T or Y connector 102 may also include an opening or channel that is parallel to the main blood flow channel. The air permeable blood barrier may further include an indicator 107 or other mechanism to indicate when a predetermined amount of blood has been collected in the sequestration chamber, or when air being expelled reaches a certain threshold, i.e. to zero. The tubing can also include a clip 109 that can be used to pinch off and prevent fluid flow therethrough.

[0060] Once the air permeable blood barrier and primary chamber are sealed the initial aliquot of blood is trapped in the sequestration chamber 104, an evacuated blood collection tube, such as a Vacutainer™ bottle may be attached to the sample needle 5 to obtain the sample. The blood collection tube can be removed, and the sample needle 5 will be resealed. Any number of follow-on blood collection tubes can then be attached for further blood draws or samples. Upon completion of all blood draws, the system can be discarded, with the initial aliquot of blood remaining trapped in the sequestration chamber 104.

[0061] FIG. 5 illustrates a blood sample optimization system in accordance with some alternative implementations. In the implementation shown, a sample needle 5 is connected with a patient needle by tubing. A "T" or "Y" connector 120 is added along the tubing at any desired location, and includes an aperture, port or channel leading to a sequestration chamber 204, substantially as described above.

[0062] FIG. 6 illustrates a blood sample optimization system in accordance with some alternative implementations, in which a sequestration chamber 304, formed as a primary collection channel, receives an initial aliquot of blood, and is provided adjacent to the blood sampling channel. The sequestration chamber 304 can encircle the blood sampling

channel, the patient needle 1, and/or the sample needle 5. The primary collection channel can include a T or Y connector 120, or other type of aperture or channel. The sequestration chamber 304 includes an air permeable blood barrier, which can also include an indicator of being contacted by a fluid such as blood, as described above.

[0063] In some implementations, either the patient needle 1 or the sample needle 5, or both, can be replaced by a Luer lock male or female connector. However, in various implementations, the connector at a sample needle end of the blood sample optimization system is initially sealed to permit the diversion of the initial aliquot of blood to the sequestration chamber, which is pressured at ambient air pressure and includes the air outlet of the air permeable blood barrier. In this way, the system passively and automatically uses a patient's own blood pressure to overcome the ambient air pressure of the sequestration chamber to push out air through the air permeable blood barrier and displace air in the sequestration chamber with blood.

[0064] FIG. 7 is a flowchart of an exemplary method for optimizing the quality of a blood culture. At 702, a clinician places a needle into a patient's vein. At 704, blood then flows into a sequestration chamber, pushing the air in the sequestration chamber out of the sequestration chamber through an air permeable blood barrier. In some implementations, the volume of the sequestration chamber is less than 0.1 to more than 5 cubic centimeters (cc's), or more. The sequestration chamber is sized and adapted to collect a first portion of a blood sample, which is more prone to contamination than secondary and other subsequent portion of the blood sample or subsequent draws. Since the sequestration chamber has an air-permeable blood barrier through which air can be displaced by blood pushed from the patient's vein, such blood will naturally and automatically flow into the sequestration chamber before it is drawn into or otherwise enters into a Vacutainer or other bottle for receiving and storing a blood sample.

[0065] When the sequestration chamber fills, the blood will gather at or otherwise make contact with the air permeable blood barrier, which will inhibit or prevent blood from passing therethrough. At 706, when the blood comes into contact with the entire internal surface area of the air permeable blood barrier, the air permeable blood barrier is then closed and air no longer flows out or in. At 708, the clinician may be provided an indictor or can

see the full chamber, to indicate the evacuated blood collection tube, such as a Vacutainer™ can be attached. The indicator can include visibility into the primary chamber to see whether it is full, the blood barrier changing color, for example, or other indicator. The fill time of the sequestration chamber may be substantially instantaneous, so such indicator, if present, may be only that the sequestration chamber is filled.

[0066] Prior to an evacuated blood collection tube being attached, communication between the needle, sampling channel, and the sequestration chamber is restricted by the sealing of the sequestration chamber blood barrier thereby not permitting air to reenter the system through the sequestration. Sealing the communication path could also be accomplished with a mechanical twist or other movement, a small orifice or tortuous pathway, eliminating the need for a separate valve or mechanical movement or operation by the clinician. At 710, once the evacuated blood collection tube is removed, the self-sealing membrane closes the sample needle, and at 712, additional subsequent evacuated blood collection tubes may be attached. Once samples have been taken, at 714 the device is removed from the patient and discarded.

[0067] FIGS. 8A – 8E illustrate an exemplary blood sample optimization system 800 for non-contaminated blood sampling, in accordance with some implementations. The blood sample optimization system 800 includes an inlet port 802 that can be connected to tubing, a patient needle (or both), or other vascular or venous access device, and a pathway splitter 804 having a first outlet to a sequestration chamber tubing 806 and a second outlet to sample collection tubing 808. One or both of the sequestration chamber tubing 806 and the sample collection tubing 808 can be formed of tubing. In some implementations, the sequestration chamber tubing 806 is sized so as to contain a particular volume of initial blood sample. The sample collection tubing 808 will receive a blood sample once the sequestration chamber tubing 806 is filled. The sample collection tubing 808 can be connected to a Vacutainer™ base or housing 810, or other blood sample collection device.

[0068] The blood sequestration system 800 further includes a blood sequestration device 812 which, as shown in more detail in FIGS. 8B – 8D, includes a housing 818 that includes a sampling channel 820 defining a pathway for the non-contaminated sample collection tubing 808 or connected at either end to the non-contaminated sample collection

tubing 808. The sampling channel 820 can be curved through the housing 818 so as to better affix and stabilize the housing 818 at a location along the non-contaminated sample collection tubing 808.

[0069] The blood sequestration device 812 further includes a sequestration chamber 822 connected with the sequestration chamber tubing 806 or other chamber. The sequestration chamber 822 terminates at an air permeable blood barrier 824. The air permeable blood barrier 824 can also include a coloring agent that turns a different color upon full contact with blood, as an indicator that the regular collection of blood samples (i.e. the non-contaminated blood samples) can be initiated. Other indicators may be used, such as a small light, a sound generation mechanism, or the like. In some implementations, the air permeable blood barrier is positioned at a right angle from the direction of sequestration chamber 822, but can be positioned at any distance or orientation in order to conserve space and materials used for the housing 818. The housing 818 and its contents can be formed of any rigid or semi-rigid material or set of materials.

[0070] FIG. 9 illustrates a pathway splitter 900 for use in a blood sequestrations system, such as those shown in FIGS. 8A – 8E, for example. The pathway splitter 900 includes an inlet port 902, a main line outlet port 904, and a sequestration channel outlet port 906. The inlet port 902 can be connected to main tubing that is in turn connected to a patient needle system, or directly to a patient needle. The main line outlet port 904 can be connected to main line tubing to a blood sampling system, such as a vacutainer base or housing, or directly to such blood sampling system. The sequestration channel outlet port 906 can be connected to sequestration tubing for receiving and sequestering a first sample of blood, up to a measured amount or predetermined threshold. Alternatively, the sequestration channel outlet port 906 can be connected to a sequestration chamber. The sequestration channel outlet port 906 is preferably 20-70 degrees angled from the main line outlet port 904, which in turn is preferably in-line with the inlet port 902. Once the predetermined amount of initial blood sample is sequestered in the sequestration tubing or chamber, in accordance with mechanisms and techniques described herein, follow-on blood samples will flow into the inlet port 902 and directly out the main line outlet port 904, without impedance.

[0071] FIGS. 10A – 10D illustrate a blood sequestration device 1000 in accordance with alternative implementations. The blood sequestration device 1000 includes an inlet port 1002, a main outlet port 1004, and a sequestration channel port 1006. The inlet port 1002 can be connected to a patient needle or related tubing. The main outlet port 1004 can be connected to a blood sample collection device such as a Vacutainer, associated tubing, or a Luer activated valve, or the like. The sequestration channel port 1006 splits off from the main outlet port 1004 to a sequestration chamber 1008. In some implementations, the sequestration chamber 1008 is formed as a helical channel within a housing or other container 1001.

[0072] The sequestration chamber 1008 is connected at the distal end to an air permeable blood barrier 1010, substantially as described above. Air in the sequestration chamber 1008 is displaced through the air permeable blood barrier 1010 by an initial aliquot of blood that is guided into the sequestration channel port 1006. Once the sequestration chamber 1008 is filled, further blood draws through the main outlet port 1004 can be accomplished, where these samples will be non-contaminated.

[0073] FIGS. 11A – 11E illustrate a blood sequestration device 1100 in accordance with other alternative implementations. The blood sequestration device 1100 includes an inlet port 1102, similar to the inlet ports described above, a main outlet port 1104, and a sequestration channel port 1106 that splits off from the main outlet port 1104 and inlet port 1102. The sequestration channel port is connected to a sequestration chamber 1108. In the implementation shown in FIGS. 11A – 11E, the blood sequestration device includes a base member 1101 having a channel therein, which functions as the sequestration chamber 1108. The channel can be formed as a tortuous path through the base member 1101, which is in turn shaped and formed to rest on a limb of a patient.

[0074] A portion of the sequestration chamber 1108 can protrude from the base member or near a top surface of the base member, just before exiting to an air permeable blood barrier 1110, to serve as a blood sequestration indicator 1109. The indicator 1109 can be formed of a clear material, or a material that changes color when in contact with blood.

[0075] In some implementations, the blood sequestration device 1100 can include a blood sampling device 1120 such as a normally closed needle, Vacutainer™ shield or other collection device. The blood sampling device 1120 can be manufactured and sold with the blood sequestration device 1100 for efficiency and convenience, so that a first aliquot of blood that may be contaminated by a patient needle insertion process can be sequestered. Thereafter, the blood sampling device 1120 can draw non-contaminated blood samples to reduce the risk of false positive testing and ensure a non-contaminated sample.

[0076] FIGS. 12A-12D illustrate a blood sample optimization system 1200 in accordance with yet other alternative implementations. The system 1200 includes a blood sequestration device 1202 for attaching to a blood sampling device 1204, such as a Vacutainer™ or other collection and sampling device. The blood sequestration device 1202 is configured and arranged to receive, prior to a Vacutainer™ container or vial being attached to a collection needle of the blood sampling device 1204, a first aliquot or amount of blood, and sequester that first aliquot or amount in a sequestration channel of the blood sequestration device 1202.

[0077] In some implementations, the blood sequestration device 1202 can include an inlet port 1212, a main outlet port, and a sequestration channel port. The inlet port 1212 can be connected to a patient needle or related tubing. The main outlet port 1214 can be connected to a normally closed needle or device to enable connection with an evacuated blood collection container or other collection device such as a Vacutainer™, associated tubing, luer connectors, syringe, a Luer activated valve, or the like. The sequestration channel port splits off from the main outlet port to a sequestration chamber 1218.

[0078] In some implementations, the sequestration chamber 1218 is formed as a channel within the body of a sequestration device 1202. The sequestration chamber 1218 can be a winding channel, such as a U-shaped channel, an S-shaped channel, a helical channel, or any other winding channel. The sequestration device 1202 can include a housing or other containing body, and one or more channels formed therein. As shown in FIGS. 12A and 12B, the sequestration device 1202 includes a main body 1206 and a cap 1208. The main body 1206 is formed with one or more cavities or channels, which are further formed with

one or more arms 1210 that extend from the cap 1208, and which abut the cavities or channels in the main body 1206 to form the primary collection port and main outlet port.

[0079] FIGS. 13A-13D illustrate a blood sample optimization system 1300 in accordance with yet other alternative implementations. The system 1300 includes a blood sequestration device 1302 for attaching to a blood sampling device 1304, such as a Vacutainer or other bodily fluid collection and sampling device. The blood sequestration device 1302 is configured and arranged to receive, prior to a Vacutainer container or vial being attached to a collection needle of the blood sampling device 1304, a first aliquot or amount of blood, and to sequester that first aliquot or amount of blood or other bodily fluid in a sequestration channel of the blood sequestration device 1302.

[0080] The blood sequestration device 1302 includes a housing 1301 having an inlet port 1314, a main outlet port 1312, and a sequestration channel port 1316. The inlet port 1314 can be connected to a patient needle or associated tubing. The main outlet port 1312 can be connected to a normally closed needle or device to enable connection with an evacuated blood collection container or other collection device such as a Vacutainer™, associated tubing, luer connectors, syringe, a Luer activated valve, or the like. The sequestration channel port 1316 splits off from the main inlet port 1314 to a sequestration chamber 1318.

[0081] In the implementation shown in FIGS. 13A-D, the sequestration chamber 1318 is formed as a cavity or chamber within housing 1301 or formed by walls that define housing 1301. The sequestration chamber 1318 can be a winding channel, such as a U-shaped channel, an S-shaped channel, a helical channel, or any other winding channel, that is defined by the cooperation and connection of housing 1301 with cap 1307 which cap 1307 can include a protrusion 1305 that provides one or more walls or directors for the winding channel in the sequestration chamber 1318. The protrusion 1305 from the cap 1307 can be straight or curved, and may have various channels, apertures or grooves embedded therein, and can extend from the cap 1307 any angle or orientation. When the cap 1307 is connected with the housing 1301 to complete the formation of the sequestration chamber 1318, the protrusion 1305 forms at least part of the winding channel to sequester a first aliquot or

amount of blood or other bodily fluid in a sequestration channel formed in the sequestration chamber 1318 and by the winding channel.

[0082] The sequestration chamber 1318 includes an air permeable blood barrier 1310, substantially as described above. Air in the sequestration chamber 1318 is displaced through the air permeable blood barrier 1310 by an initial aliquot of blood that is provided into the sequestration chamber 1318 by the blood pressure of the patient. Once the sequestration chamber 1318 is filled and the air in the sequestration chamber 1318 displaced, the blood pressure of the patient will be insufficient to drive or provide further blood into the blood sequestration device 1302, and in particular the outlet port 1312, until a force such as a vacuum or other pressure, such as provided by the blood sample collection device like Vacutainer is provided to draw out a next aliquot or amount of blood or bodily fluid. Further blood draws through the main outlet port 1312 can be accomplished, where these samples will be non-contaminated since any contaminants would be sequestered in the sequestration chamber 1318 with the first aliquot of blood.

[0083] FIGS. 14A-14E illustrate yet another implementation of a blood sampling system 1400 to sequester contaminates of an initial aliquot or sample to reduce false positives in blood cultures or tests performed on a patient's blood sample. The blood sampling system 1400 includes a blood sequestration device 1401 that can be connected between a blood sample collection device 1403 and a patient needle (not shown). The blood sample collection device 1403 can be a Vacutainer or the like. The blood sequestration device 1401 includes an inlet port 1402 that can be connected with a patient needle that is inserted into a patient's vascular system for access to and withdrawing of a blood sample. The inlet port 1402 may also be connected with tubing or other conduit that is in turn connected with the patient needle.

[0084] The inlet port 1402 defines an opening into the blood sequestration device 1401, which opening can be the same cross sectional dimensions as tubing or other conduit connected with the patient needle or the patient needle itself. For instance, the opening can be circular with a diameter of approximately 0.045 inches, but can have a diameter of between 0.01 inches or less to 0.2 inches or more. The blood sequestration device 1401 further includes an outlet port 1404, which defines an opening out of the blood sequestration

device 1401 and to the blood sample collection device 1403. The outlet port 1404 may also be connected with tubing or other conduit that is in turn connected with the blood sequestration device 1403. The outlet port 1404 can further include a connector device such as a threaded cap, a Luer connector (male or female), a non threaded interference or glue joint fitting for attachment of various devices including but not limited to tubing, or the like.

[0085] The blood sequestration device 1401 further includes a sampling channel 1406 between the inlet port 1402 and the outlet port 1404, and which functions as a blood sample pathway once a first aliquot of blood has been sequestered. The sampling channel 1406 can be any sized, shaped or configured channel, or conduit. In some implementations, the sampling channel 1406 has a substantially similar cross sectional area as the opening of the inlet port 1402. In other implementations, the sampling channel 1406 can gradually widen from the inlet port 1402 to the outlet port 1404.

[0086] The blood sequestration device 1401 further includes a sequestration chamber 1408 that is connected to and split off or diverted from the sampling channel 1406 at any point between the inlet port 1402 and the outlet port 1404, but preferably from a proximal end of the sampling channel 1406 near the inlet port 1402. The sequestration chamber 1408 is at first maintained at atmospheric pressure, and includes an air outlet 1412 at or near a distal end of the sequestration chamber 1408 opposite the diversion point from the sampling channel 1406. The air outlet 1412 includes an air permeable blood barrier 1412. As shown in FIG. 14B, the air permeable blood barrier 1412 can be overlaid with a protective cover 1416. The protective cover 1416 can be sized and configured to inhibit a user from touching the air permeable blood barrier 1412 with their finger or other external implement, while still allowing air to exit the air permeable blood barrier 1412 as the air is displaced from the sequestration chamber 1408 by blood being forced into the sequestration chamber 1408 by a patient's own blood pressure. In addition the protective cover 1416 can be constructed to inhibit or prevent accidental exposure of the air permeable blood barrier to environmental fluids or splashes. This can be accomplished in a variety of mechanical ways including but not limited to the addition of a hydrophobic membrane to the protective cover.

[0087] As shown in FIGS. 14C and 14D, the sampling channel 1406 can be cylindrical or frusto-conical in shape, going from a smaller diameter to a larger diameter, to

minimize a potential to lyse red blood cells. Likewise, the sampling channel 1406 is formed with a minimal amount of or no sharp turns or edges, which can also lyse red blood cells. The sampling channel 1406 splits off to the sequestration chamber 1408 near the inlet port 1402 via a diversion pathway 1409. The diversion pathway 1409 can have any cross-sectional shape or size, but is preferably similar to the cross-sectional shape of at least part of the inlet port 1402.

[0088] In some implementations, the sampling channel 1406 and the sequestration chamber 1408 are formed by grooves, channels, locks or other pathways formed in housing 1414. The housing 1414 can be made of plastic, metal or other rigid or semi-rigid material. The housing 1414 can have a bottom member that sealably mates with a top member. One or both of the bottom member and the top member can include the sampling channel 1406 and the sequestration chamber 1408, as well as the diversion pathway 1409, the inlet port 1402, and the outlet port 1404. In some other implementations, one or more of the diversion pathway 1409, the inlet port 1402, and/or the outlet port 1404 can be at least partially formed by a cap member that is connected to either end of the housing 1414. In some implementations, the top member and the bottom member, as well as the cap member(s), can be coupled together by laser welding, heat sealing, gluing, snapping, screwing, bolting, or the like. In other implementations, some or all of the interior surface of the diversion pathway 1409 and/or sequestration chamber 1408 can be coated or loaded with an agent or substance, such as a decontaminate, solidifying agent, or the like. For instance, a solidifying agent can be provided at the diversion pathway 1409 such that when the sequestration chamber 1408 is filled and the initial aliquot of blood backs up to the diversion pathway 1409, that last amount of sequestered blood could solidify, creating a barrier between the sequestration chamber 1408 and the sampling channel 1406.

[0089] FIGS. 15A-15G illustrate a blood sequestration device 1500. The blood sequestration device 1500 can be connected to a normally closed needle or device to enable connection with an evacuated blood collection container or other collection device such as a Vacutainer™, associated tubing, luer connectors, syringe, a Luer activated valve, or the like.

[0090] The blood sequestration device 1500 includes an inlet port 1502 that can be connected with a patient needle that is inserted into a patient's vascular system for access to

and withdrawing of a blood sample. The inlet port 1502 may also be connected with tubing or other conduit that is in turn connected with the patient needle. The inlet port 1502 defines an opening into the blood sequestration device 1500, which opening may be the same cross sectional dimensions as tubing or other conduit connected with the patient needle or the patient needle itself. For instance, the opening can be circular with a diameter of approximately 0.045 inches, but can have a diameter of between 0.01 inches or less to 0.2 inches or more.

[0091] The inlet port 1502 can also include a sealing or fluid-tight connector or connection, such as threading or Luer fitting, or the like. In some implementations, tubing or other conduit associated with the patient needle can be integral with the inlet port 1502, such as by co-molding, gluing, laser weld, or thermally bonding the parts together. In this manner, the blood sequestration device 1500 can be fabricated and sold with the patient needle as a single unit, eliminating the need for connecting the patient needle to the blood sequestration device 1500 at the time of blood draw or sampling.

[0092] The blood sequestration device 1500 further includes an outlet port 1504, which defines an opening out of the blood sequestration device 1500 and to the blood sample collection device. The outlet port 1504 may also be connected with tubing or other conduit that is in turn connected with the blood sequestration device, and may also include a sealing or fluid-tight connector or connection, such as threading or Luer fitting, or the like. Accordingly, as discussed above, the blood sequestration device 1500 can be fabricated and sold with the patient needle and/or tubing and the blood sample collection device as a single unit, eliminating the need for connecting the patient needle and the blood sample collection device to the blood sequestration device 1500 at the time of blood draw or sampling.

[0093] The blood sequestration device 1500 further includes a sampling channel 1506 between the inlet port 1502 and the outlet port 1504, and which functions as a blood sample pathway once a first aliquot of blood has been sequestered. The sampling channel 1506 can be any sized, shaped or configured channel or conduit. In some implementations, the sampling channel 1506 has a substantially similar cross sectional area as the opening of the inlet port 1502. In other implementations, the sampling channel 1506 can gradually widen from the inlet port 1502 to the outlet port 1504.

[0094] The blood sequestration device 1500 further includes a sequestration chamber 1508 that is connected to and split off or diverted from the sampling channel 1506 at any point between the inlet port 1502 and the outlet port 1504, but preferably from a proximal end of the sampling channel 1506 near the inlet port 1502. In some implementations, the diversion includes a Y-shaped junction. The sequestration chamber 1508 is preferably maintained at atmospheric pressure, and includes a vent 1510 at or near a distal end of the sequestration chamber 1508. The vent 1510 includes an air permeable blood barrier 1512. FIG. 15C illustrates the blood sequestration device 1500 with the sequestration chamber 1508 filled with a first aliquot or sample of blood from the patient.

[0095] The air permeable blood barrier 1512 can be covered with a protective cover 1516. The protective cover 1516 can be sized and configured to inhibit a user from touching the air permeable blood barrier 1512 with their finger or other external implement, while still allowing air to exit the air permeable blood barrier 1512 as the air is displaced from the sequestration chamber 1508 by blood being forced into the sequestration chamber 1508 by a patient's own blood pressure. The protective cover 1516 can be constructed to inhibit or prevent accidental exposure of the filter to environmental fluids or splashes. This can be accomplished in a variety of mechanical ways including but not limited to the addition of a hydrophobic membrane to the protective cover.

[0096] FIG. 15B is a perspective view of the blood sequestration device 1500 from the outlet port 1504 and top side of a housing 1501 of the blood sequestration device 1500 that includes the vent 1510, and illustrating an initial aliquot of blood filling sequestration chamber 1508 while the sampling channel 1506 is empty, before a sample collection device is activated. FIG. 15G is a perspective view of the blood sequestration device 1500 from the outlet port 1504 and bottom side of the housing 1501 of the blood sequestration device 1500, and illustrating the initial aliquot of blood filling sequestration chamber 1508 while the sampling channel 1506 is empty, before the sample collection device is activated. FIG. 15C is another perspective view of the blood sequestration device 1500 from the inlet port 1502 and top side of a housing 1501 of the blood sequestration device 1500 that includes the vent 1510, and illustrating blood now being drawn through sampling channel 1506 while the sequestered blood remains substantially in the sequestration chamber 1508.

[0097] FIG. 15D is a cross section of the blood sequestration device 1500 in accordance with some implementations, showing the housing 1501 that defines the sampling channel 1506 and the sequestration chamber 1508. FIGS. 15E and 15F illustrate various form factors of a housing for a blood sequestration device, in accordance with one or more implementations described herein.

[0098] The sequestration chamber 1508 can have a larger cross-sectional area than the sampling channel 1506, and the cross-sectional area and length can be configured for a predetermined or specific volume of blood to be sequestered or locked. The sampling channel 1506 can be sized to be compatible with tubing for either or both of the patient needle tubing or the blood collection device tubing.

[0099] The housing 1501 can be formed of multiple parts or a single, unitary part. In some implementations, and as illustrated in FIG. 15D, the housing 1501 includes a top member 1520 and a bottom member 1522 that are mated together, one or both of which having grooves, channels, locks, conduits or other pathways pre-formed therein, such as by an injection molding process or by etching, cutting, drilling, etc. The top member 1520 can be connected with the bottom member 1522 by any mating or connection mechanism, such as by laser welding, thermal bonding, ultrasonic welding, gluing, using screws, rivets, bolts, or the like, or by other mating mechanisms such as latches, grooves, tongues, pins, flanges, or the like.

[00100] In some implementations, such as shown in FIG. 15D, the top member 1520 can include the grooves, channels, locks, conduits or other pathways, while the bottom member 1522 can include a protrusion 1524 that is sized and adapted to fit into at least one of the grooves, channels, locks or other pathways of the top member 1520. The protrusion 1524 can provide a surface feature, such as a partial groove or channel, for instance, to complete the formation of either the sampling channel 1506 and/or the sequestration chamber 1508. In some implementations, the protrusion 1524 can be formed with one or more angled sides or surfaces for a tighter fit within the corresponding groove, channel, lock or other pathway. In yet other implementations, both the top member 1520 and the bottom member can include grooves, channels, locks or other pathways, as well as one or more protrusions 1524.

[00101] In some implementations, the sampling channel 1506 and the sequestration chamber 1508 are formed by grooves, channels, locks or other pathways formed in housing 1501. The housing 1501 can be made of any suitable material, including rubber, plastic, metal or other material. The housing 1501 can be formed of a clear or translucent material, or of an opaque or non-translucent material. In other implementations, the housing 1501 can be mostly opaque or non-translucent, while the housing surface directly adjacent to the sampling channel 1506 and/or the sequestration chamber 1508 is clear or translucent, giving a practitioner a visual cue or sign that the sequestration chamber 1508 is first filled to the extent necessary or desired, and/or then a visual cue or sign that the sequestered blood remains sequestered while a clean sample of blood is drawn through the sampling channel 1506. Other visual cues or signs of the sequestration can include, without limitation: the air permeable blood barrier 1512 turning a different color upon contact, saturation, or partial saturation with blood; a color-coded tab or indicator at any point along or adjacent to the sequestration chamber; an audible signal; a vibratory signal; or other signal.

[00102] After a venipuncture by a patient needle of a patient (not shown), which could gather a number of pathogens from the patient's skin, a first amount of the patient's blood with those pathogens will make its way into the input port 1502 blood sequestration device 1500 and flow into the sequestration chamber 1508 by following the path of least resistance, as the patient's own blood pressure overcomes the atmospheric pressure in the sequestration chamber 1508 to displace air therein through the air permeable blood barrier 1512. The patient's blood pressure will not be sufficient to overcome the air pressure that builds up in the sealed sampling channel 1506. Eventually, the sequestration chamber 1508, which has a predetermined volume, is filled with blood that displaces air through the air permeable blood barrier 1512. Once the blood hits the air permeable blood barrier, the blood interacts with the air permeable blood barrier 1512 material to completely or partially seal the vent 1510. A signal or indication may be provided that the practitioner can now utilize the Vacutainer capsule or other blood sample collection device to acquire a next amount of the patient's blood for sampling. The blood in the sequestration chamber 1508 is now effectively sequestered in the sequestration chamber.

[00103] Upon filling the blood sequestration pathway 1508 but prior to use of the Vacutainer or other blood sample collection device, the patient's blood pressure may drive compression of the air in the sampling channel 1506, possibly resulting in a small amount of blood moving past the diversion point to the sequestration chamber 1508 and into the sampling channel 1506, queuing up the uncontaminated blood to be drawn through the sampling channel 1506.

[00104] FIGS. 16-19 illustrate yet another implementation of a blood sequestration device. FIGS. 16A-16D illustrate a blood sequestration device 1600 that can be connected between a blood sample collection device, such as an evacuated blood collection container like a Vacutainer™ (not shown), and a patient needle (not shown) and/or associated tubing. FIG. 17 illustrates a bottom member of the blood sequestration device, and FIG. 18 illustrates a top member of the blood sequestration device, which top member and bottom member can be mated together to form an input port, and output port, a sequestration chamber and a sampling channel, as explained more fully below. FIGS. 19A and B show the top member and bottom member mated together. It should be understood that FIGS. 16-19 illustrate one exemplary manner of constructing a blood sequestration device as described herein, and other forms of construction are possible.

[00105] Referring to FIGS. 16A – D, the blood sequestration device 1600 includes an inlet port 1602 that can be connected with a patient needle that is inserted into a patient's vascular system for access to and withdrawing of a blood sample. The inlet port 1602 may also be connected with tubing or other conduit that is in turn connected with the patient needle. The inlet port 1602 defines an opening into the blood sequestration device 1600, which opening can be the same cross sectional dimensions as tubing or other conduit connected with the patient needle or the patient needle itself. For instance, the opening can be circular with a diameter of approximately 0.045 inches, but can have a diameter of between 0.01 inches or less to 0.2 inches or more.

[00106] The inlet port 1602 can also include a sealing or fluid-tight connector or connection, such as threading or Luer fitting, or the like. In some implementations, tubing or other conduit associated with the patient needle can be integral with the inlet port 1602, such as by co-molding, gluing, laser weld, or thermally bonding the parts together. In this manner,

the blood sequestration device 1600 can be fabricated and sold with the patient needle and/or tubing as a single unit, eliminating the need for connecting the patient needle to the blood sequestration device 1600 at the time of blood draw or sampling.

[00107] The blood sequestration device 1600 further includes an outlet port 1604, which defines an opening out of the blood sequestration device 1600 and to the blood sample collection device. The outlet port 1604 may also be connected with tubing or other conduit that is in turn connected with the blood sequestration device, and may also include a sealing or fluid-tight connector or connection, such as threading or Luer fitting, or the like. Accordingly, as discussed above, the blood sequestration device 1600 can be fabricated and sold with the patient needle and/or tubing and the blood sample collection device as a single unit, eliminating the need for connecting the patient needle and the blood sample collection device to the blood sequestration device 1600 at the time of blood draw or sampling.

[00108] The blood sequestration device 1600 further includes a sampling channel 1606 between the inlet port 1602 and the outlet port 1604, and a sequestration chamber 1608 that is connected to and split off or diverted from the sampling channel 1606 at any point between the inlet port 1602 and the outlet port 1604. The sampling channel 1606 functions as a blood sampling pathway once a first aliquot of blood has been sequestered in the sequestration chamber 1608. The sampling channel 1606 can be any sized, shaped or configured channel, or conduit. In some implementations, the sampling channel 1606 has a substantially similar cross sectional area as the opening of the inlet port 1602. In other implementations, the sampling channel 1606 can gradually widen from the inlet port 1602 to the outlet port 1604. The sequestration chamber 1608 may have a larger cross section to form a big reservoir toward the sequestration channel path so that the blood will want to enter the reservoir first versus entering a smaller diameter on the sampling channel 1606, as is shown more fully in FIGS. 17 and 19.

[00109] In some exemplary implementations, the diversion between the sampling channel 1606 and the sequestration chamber 1608 is by diverter junction 1607. Diverter junction 1607 may be a substantially Y-shaped, T-shaped, or U-shaped. In some preferred exemplary implementations, and as shown in FIG. 17A – 17B, the diverter junction 1607 is configured such that the flow out of the inlet port 1602 is preferentially directed toward the

sequestration chamber 1608. The sequestration chamber 1608 may also include or form a curve or ramp to direct the initial blood flow toward and into the sequestration chamber 1608.

[00110] The sequestration chamber 1608 is preferably maintained at atmospheric pressure, and includes a vent 1610 at or near a distal end of the sequestration chamber 1608. The vent 1610 may include an air permeable blood barrier 1612 as described above.

[00111] The blood sequestration device 1600 can include a housing 1601 that can be formed of multiple parts or a single, unitary part. In some implementations, and as illustrated in FIGS. 17A – 17**[[**D**]]**E and FIGS. 18A – 18F, the housing 1601 includes a top member 1620 and a bottom member 1622 that are mated together. The blood sequestration device 1600 can also include a gasket or other sealing member (not shown) so that when the top member 1620 is mechanically attached with the bottom member 1622, the interface between the two is sealed by the gasket or sealing member. The FIGS. 17A – 17**[[**D**]]**E illustrate a bottom member 1622 of a housing for a blood sequestration device 1600. The bottom member 1622 can include grooves, channels, locks, conduits or other pathways pre-formed therein, such as by an injection molding process or by etching, cutting, drilling, etc., to form the sampling channel 1606, the sequestration chamber 1608, and diverter junction 1607.

[00112] The sequestration chamber 1608 may have a larger cross section than the sampling channel 1606 so that the blood will preferentially move into the sequestration chamber first versus entering a smaller diameter on the sampling channel 1606.

[00113] FIGS. 18A – 18F illustrate the top member 1620, which can be connected with the bottom member 1622 by any mating or connection mechanism, such as by laser welding, thermal bonding, gluing, using screws, rivets, bolts, or the like, or by other mating mechanisms such as latches, grooves, tongues, pins, flanges, or the like. The top member 1620 can include some or all of the grooves, channels, locks, conduits or other pathways to form the sampling channel 1606, the sequestration chamber 1608, and the diverter junction 1607. In yet other implementations, both the top member 1620 and the bottom member 1622 can include the grooves, channels, locks or other pathways.

[00114] In some implementations, the sampling channel 1606 and the sequestration chamber 1608 are formed by grooves, channels, locks or other pathways formed in housing 1601. The housing 1601 can be made of rubber, plastic, metal or any other suitable material. The housing 1601 can be formed of a clear or translucent material, or of an opaque or non-translucent material. In other implementations, the housing 1601 can be mostly opaque or non-translucent, while the housing surface directly adjacent to the sampling channel 1606 and/or the sequestration chamber 1608 may be clear or translucent, giving a practitioner a visual cue or sign that the sequestration chamber 1608 is first filled to the extent necessary or desired, and/or then a visual cue or sign that the sequestered blood remains sequestered while a clean sample of blood is drawn through the sampling channel 1606. Other visual cues or signs of the sequestration can include, without limitation: the air permeable blood barrier 1612 turning a different color upon contact, saturation, or partial saturation with blood; a color-coded tab or indicator at any point along or adjacent to the sequestration chamber; an audible signal; a vibratory signal; or other signal.

[00115] As shown in FIGS. 18A – 18F, the air permeable blood barrier 1612 can be covered with, or surrounded by, a protective member 1616. The protective member 1616 can be sized and configured to inhibit a user from touching the air permeable blood barrier 1612 with their finger or other external implement, while still allowing air to exit the air permeable blood barrier 1612 as the air is displaced from the sequestration chamber 1608. In some implementations, the protective member 1616 includes a protrusion that extends up from a top surface of the top member 1620 and around the air permeable blood barrier 1612. The protective cover 1616 can be constructed to inhibit or prevent accidental exposure of the filter to environmental fluids or splashes. This can be accomplished in a variety of mechanical ways including but not limited to the addition of a hydrophobic membrane to the protective cover.

[00116] In use, the blood sequestration device 1600 includes a sampling channel 1606 and a sequestration chamber 1608. Both pathways are initially air-filled at atmospheric pressure, but the sampling channel 1606 is directed to an output port 1604 that will be initially sealed by a Vacutainer or other such sealed blood sampling device, and the

sequestration chamber 1608 terminates at a vent 1610 to atmosphere that includes an air permeable blood barrier 1612.

[00117] After a venipuncture by a patient needle of a patient (not shown), which could gather a number of pathogens from the patient's skin, a first amount of the patient's blood with those pathogens will pass through input port 1602 of blood sequestration device 1600. This initial volume of potentially contaminated blood will preferentially flow into the sequestration chamber 1608 by finding the path of least resistance. The patient's own blood pressure overcomes the atmospheric pressure in the vented sequestration chamber 1608 to displace air therein through the air permeable blood barrier 1612, but is not sufficient to overcome the air pressure that builds up in the sealed sampling channel 1606. In various exemplary embodiments, the sequestration chamber 1608 and sampling channel 1606 can be configured such that the force generated by the patient's blood pressure is sufficient to overcome any effect of gravity, regardless of the blood sequestration device's orientation.

[00118] Eventually, the sequestration chamber 1608 fills with blood that displaces air through the air permeable blood barrier 1612. Once the blood contacts the air permeable blood barrier, the blood interacts with the air permeable blood barrier 1612 material to completely or partially seal the vent 1610. A signal or indication may be provided that the practitioner can now utilize the Vacutainer or other blood sampling device.

[00119] Upon filling the blood sequestration pathway 1608 but prior to use of the Vacutainer or other blood sample collection device, the patient's blood pressure may drive compression of the air in the sampling channel 1606, possibly resulting in a small amount of blood moving past the diversion point into the sampling channel 1606, queuing up the uncontaminated blood to be drawn through the sampling channel 1606.

[00120] FIG. 19A is a side view, and FIG. 19B is a cross-sectional view, of the blood sequestration device 1600, illustrating the top member 1620 mated with the bottom member 1622.

[00121] FIG. 20 shows a blood sample optimization system 2000 that includes a patient needle 2002 for vascular access to a patient's bloodstream, a blood sample collection device 2004 to facilitate the collecting of one or more blood samples, and a conduit 2006

providing a fluid connection between the patient needle 2002 and the blood sample collection device 2004. In some implementations, the blood sample collection device 2004 includes a protective shield that includes a sealed collection needle on which a sealed vacuum-loaded container is placed, which, once pierced by the collection needle, draws in a blood sample under vacuum pressure or force through the conduit 2006 from the patient needle 2002.

[00122] The blood sample optimization system 2000 further includes a blood sequestration device 2008, located at any point on the conduit 2006 between the patient needle 2002 and the blood sample collection device 2004 as described herein.

[00123] FIG. 21 illustrates a non-vented blood sequestration device 2100 using a wicking material chamber. The blood sequestration device 2100 includes a housing 2101 that has a sampling channel 2104 that is at least partially surrounded or abutted by a sequestration chamber 2102 that is filled with a wicking material. An initial aliquot of blood is drawn in from the patient needle into the sampling channel 2104 where it is immediately wicked into the wicking material of the sequestration chamber 2102. The wicking material and/or sequestration chamber 2102 is sized and adapted to receive and hold a predetermined amount of blood, such that follow-on or later blood draws pass by the wicking material and flow straight through the sampling channel 2104 to a sampling device such as a Vacutainer. The wicking material can include a substance such as a solidifier, a decontaminate, or other additive.

[00124] As described herein, an air permeable blood barrier may be created using a wide variety of different structures and materials. As shown in FIGS. 22A and B, an air permeable blood barrier 2202 of a blood sequestration device 2200 can include a polymer bead matrix 2204, in which at least some beads are treated to make them hydrophilic. The air permeable blood barrier 2202 further includes a self-sealing material 2206, such as carboxymethyl cellulose (CMC) or cellulose gum, or other sealing material. The air permeable blood barrier 2202 can further include voids 2208 that permit air flow before contact or during partial contact with a fluid such as blood. As shown in FIG. 22B, contact with a fluid causes the self-sealing material 2206 to swell and close off the voids 2208, occluding air flow through the voids 2208 and creating a complete or partial seal.

[00125] FIGS. 23A and B illustrate yet another implementation of a blood sequestration device 2300, having an inlet port 2302 to connect with a patient needle, an outlet port 2304 to connect with a blood sample collection device, a sequestration chamber 2306, and a sampling channel 2308 that bypasses the sequestration chamber 2306 once the sequestration chamber is filled to an initial aliquot of potentially contaminated blood to be sequestered. The sequestration chamber 2306 includes a hydrophobic plug 2312 at a distal end of the sequestration chamber 2306 that is farthest from the inlet port 2302. A vacuum or other drawing force applied from the outlet port 2304, such as from a Vacutainer or the like, draws in blood into the inlet port 2302 and directly into the sequestration chamber 2306, where the initial aliquot of blood will contact the hydrophobic plug 2312 and cause the initial aliquot of blood to back up into the sequestration chamber 2306 and be sequestered there. A small amount of blood may make its way into the sampling channel 2308, which is initially closed off by valve 2308. Upon release of the valve 2308, and under further force of the vacuum or other force, follow-on amounts of blood will flow into inlet port 2302, bypass the sequestration chamber 2306, and flow into and through sampling channel 2308 toward the outlet port 2304 and to the collection device.

[00126] The sampling channel 2308 can have any suitable geometry and can be formed of plastic tubing or any other suitable material. Valve 2308 can be a clip or other enclosing device to pinch, shunt, bend or otherwise close off the sampling channel before the initial aliquot of blood is sequestered in the sequestration chamber 2306.

[00127] Although a variety of embodiments have been described in detail above, other modifications are possible. Other embodiments may be within the scope of the following claims.

CLAIMS

1. A blood sequestration device comprising;

an inlet port;

an outlet port;

a sequestration chamber having a vent that includes an air permeable blood barrier; and

a sampling channel having a distal end connected with the outlet port;

each of the sequestration chamber and the sampling channel being connected with the inlet port via a junction that is sized and configured such that a first portion of blood flows into the sequestration chamber to displace air therein through the air permeable blood barrier and to be sequestered in the sequestration chamber, and a second portion of blood is allowed to bypass the sequestration chamber and the first portion of blood sequestered therein to be directed into the sampling channel toward the outlet port.

2. The blood sequestration device in accordance with claim 1, wherein the air permeable blood barrier includes an air permeable material that seals at least partially upon contact with blood.

3. The blood sequestration device in accordance with claim 1, further comprising a housing that defines a part of each of the inlet port, the outlet port, the sequestration chamber, and the sampling channel.

4. The blood sequestration device in accordance with claim 3, wherein the sequestration chamber includes a sequestration channel defined in the housing.

5. The blood sequestration device in accordance with claim 2, wherein the housing comprises a bottom member mated with a top member, each of the bottom

member and the top member defining a part of each of the inlet port, the outlet port, the sequestration chamber, and the sampling channel.

6. A blood sequestration device connected with a blood sampling pathway having a patient needle and a sample collection device, the blood sequestration device comprising:

an inlet port connected with the patient needle;

an outlet port connected with the sample collection device;

a sequestration chamber having a vent that includes an air permeable blood barrier; and

and a sampling channel having a distal end connected with the outlet port;

each of the sequestration chamber and the sampling channel being connected with the inlet port via a junction that is sized and configured such that a first portion of blood flows into the sequestration chamber to displace air therein through the air permeable blood barrier and to be sequestered in the sequestration chamber, and a second portion of blood is allowed to bypass the sequestration chamber and the first portion of blood sequestered therein to be directed into the sampling channel toward the outlet port and the sample collection device.

7. The blood sequestration device in accordance with claim 6, further comprising a housing that houses and defines the inlet port, the outlet port, the sequestration chamber, and the sampling channel.

8. The blood sequestration device in accordance with claim 6, wherein the inlet port is connected with the patient needle via a first portion of the blood sampling pathway.

9. The blood sequestration device in accordance with claim 6, wherein the outlet port is connected with the sample collection device via a second portion of the blood sampling pathway.

10. The blood sequestration device in accordance with claim 6, wherein the air permeable blood barrier includes an air permeable material that seals at least partially upon contact with blood.

11. The blood sequestration device in accordance with claim 7, wherein the sequestration chamber includes a sequestration channel defined in the housing.

12. The blood sequestration device in accordance with claim 11, wherein the sequestration channel has a proximal end connected with the inlet port, and a distal end having the vent comprising an air permeable blood barrier.

13. A bodily fluid sequestration device comprising;

an inlet port;

an outlet port connected with the inlet port;

a sequestration chamber connected with the inlet port via a junction, the sequestration chamber having a vent that includes an air permeable bodily fluid barrier; and

a housing that houses and defines the inlet port, the outlet port, and the sequestration chamber, the sequestration chamber and the junction configured to direct a first portion of bodily fluid from the inlet port into the sequestration chamber toward the air permeable bodily fluid barrier, the air permeable bodily fluid barrier including an air permeable material that forms a barrier to bodily fluids upon contact with the bodily fluids,

whereupon formation of the barrier enables sequestration of the first portion of bodily fluid in the sequestration chamber, and enables a second portion of bodily fluid from the inlet port to bypass the sequestration chamber via the junction and the first portion of bodily fluid, toward the outlet port.

14. The bodily fluid sequestration device in accordance with claim 13, wherein the air permeable bodily fluid barrier includes an air permeable material that seals upon contact with the bodily fluids.

15. The bodily fluid sequestration device in accordance with claim 13, wherein the sequestration chamber includes a sequestration channel defined in the housing.

16. The bodily fluid sequestration device in accordance with claim 13, further comprising a sampling pathway connected with the inlet port, wherein the sampling pathway conveys the second portion of bodily fluid from the inlet port to the outlet port via the junction.

17. The bodily fluid sequestration device in accordance with claim 13, wherein the housing comprises a bottom member mated with a top member, each of the bottom member and the top member defining a part of each of the inlet port, the outlet port, and the sequestration chamber.

18. The bodily fluid sequestration device in accordance with claim 13, further comprising a sampling channel having a proximal end connected with the inlet port via the junction.

19. The blood sequestration device in accordance with claim 18, wherein the housing comprises a bottom member mated with a top member, each of the bottom member and the top member defining a part of each of the inlet port, the outlet port, the sequestration chamber, and the sampling channel.

20. A blood sequestration system comprising:

a blood sampling pathway having a patient needle and a sample collection device; and

a blood sequestration device, the blood sequestration device comprising:

an inlet port connected with the patient needle;

an outlet port connected with the sample collection device;

a sequestration chamber having a vent that includes an air permeable blood barrier; and

and a sampling channel having a distal end connected with the outlet port;

each of the sequestration chamber and the sampling channel being connected with the inlet port via a junction that is sized and configured such that a first portion of blood flows into the sequestration chamber to displace air therein through the air permeable blood barrier and to be sequestered in the sequestration chamber, and a second portion of blood is allowed to bypass the sequestration chamber and the first portion of blood sequestered therein to be directed into the sampling channel toward the outlet port and the sample collection device.

21. The blood sequestration system in accordance with claim 20, further comprising a housing that houses and defines the inlet port, the outlet port, the sequestration chamber, and the sampling channel.

22. The blood sequestration system in accordance with claim 20, wherein the inlet port is connected with the patient needle via a first portion of the blood sampling pathway.

23. The blood sequestration system in accordance with claim 20, wherein the outlet port is connected with the sample collection device via a second portion of the blood sampling pathway.

24. The blood sequestration system in accordance with claim 20, wherein the air permeable blood barrier includes an air permeable material that seals at least partially upon contact with blood.

25. The blood sequestration system in accordance with claim 24, wherein the sequestration chamber includes a sequestration channel defined in the housing.

26. The blood sequestration device in accordance with claim 25, wherein the sequestration channel has a proximal end connected with the inlet port, and a distal end having the vent comprising an air permeable blood barrier.

ABSTRACT

Blood sample optimization systems and methods are described that reduce or eliminate contaminates in collected blood samples, which in turn reduces or eliminates false positive readings in blood cultures or other testing of collected blood samples. A blood sample optimization system can include a blood sequestration device located between a patient needle and a sample needle. The blood sequestration device can include a sequestration chamber for sequestering an initial, potentially contaminated aliquot of blood, and may further include a sampling channel that bypasses the sequestration chamber to convey likely uncontaminated blood between the patient needle and the sample needle after the initial aliquot of blood is sequestered in the sequestration chamber.

BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a Continuation of U.S. Application No. 15/140,448, filed on April 27, 2016, which claims the benefit of U.S. Provisional Application Serial No. 62/196,797, filed on July 24, 2015 and titled "BLOOD CULTURE IMPROVEMENT SYSTEM AND METHOD"; U.S. Provisional Application Serial No. 62/238,636, filed on October 7, 2015 and titled "BLOOD SEQUESTRATION SYSTEM FOR NON-CONTAMINATED BLOOD SAMPLING"; and U.S. Provisional Application Serial No. 62/318,194, filed on April 4, 2016 and titled "BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD," the disclosures of which are incorporated by reference in their entirety.

BACKGROUND

[0002] Bacteraemia is the presence of microorganisms in the blood. Sepsis, on the other hand, is bacteraemia in the presence of clinical symptoms and signs such as fever, tachycardia, tachypnea and hypotension. Bacteraemia and sepsis are associated with a high mortality and an increased incidence and duration of hospital stay and associated costs. Many bacteraemias, sepsis, fungaemias and other pathogens actually occur within a hospital or other healthcare settings with catheters and venipunctures being a source of contamination as potential carriers of these pathogens.

[0003] Blood cultures are the standard test used to detect microbial pathogens related to bacteraemia and sepsis in a patient's blood. The term blood culture refers to a single venipuncture, either from a peripheral site or central or arterial line, with the blood inoculated into one or more blood culture bottles or containers. One bottle is considered a blood culture where two or more are considered a set. Multiple sets may be obtained from multiple venipunctures and are associated with different sites on the patient.

[0004] These methods allow for microbial identification and susceptibility testing to be performed, which is a critical component to managing sepsis, however the lack of rapid results and decreased sensitivity for fastidious pathogens has led to the development of improved systems and adjunctive molecular or proteomic testing.

[0005] Collection of blood samples for conducting blood cultures is a critical component of modern patient care and can either positively affect the patient outcome by providing an accurate diagnosis, or can adversely affect the outcome by prolonging unnecessary antimicrobial therapy, the length of hospital stays, and increasing costs.

[0006] One outcome of collection of blood cultures is contamination. Blood culture contamination can lead to a false positive culture result and/or significant increase in healthcare related costs. Sources of blood culture contamination include improper skin antisepsis, improper collection tube disinfection, and contamination of the initial blood draw which may then skew results.

[0007] Blood culture collection kits generally consist of a "butterfly" set, infusion set, or other type of venipuncture device as offered by companies like BD, Smiths, B. Braun and others, and aerobic and anaerobic blood culture bottles. Various different bottles are also available depending on the test requirements. These bottles are specifically designed to optimize recovery of both aerobic and anaerobic organisms. In conventional kits, a bottle used is known generally as a "Vacutainer," which is a blood collection tube formed of a sterile glass or plastic tube with a closure that is evacuated to create a vacuum inside the tube to facilitate the draw of a predetermined volume of liquid such as blood.

[0008] False positive blood cultures are typically a result of poor sampling techniques. They cause the use of antibiotics when not needed, increasing hospital costs and patient anxiety. Blood cultures are drawn from a needlestick into the skin, and then a Vacutainer is attached to capture a sample of blood. Contamination may occur from improper or incomplete disinfection of the skin area in and around the puncture site. It may also occur from the coring of the skin by the needle during insertion, with the cored skin cells and any associated contamination being pulled into the sample.

[0009] Blood flow through a hypodermic needle is laminar, and as such, a velocity gradient can be developed over the flow tube as a pressure drop is applied to the hypodermic needle. Either forceful aspiration of blood, or using a very small hypodermic needle, can cause lysis and a release of potassium from the red blood cells, thereby rendering the blood samples abnormal.

[0010] In other instances, some patients have delicate veins that can collapse under a pressure drop or vacuum, particularly as applied by a syringe's plunger that is drawn too quickly for the patient's condition. Since such condition is impossible to know beforehand, such vein collapses are a risk and very difficult to control.

[0011] Various strategies have been implemented to decrease blood culture contamination rates, e.g. training staff with regard to aseptic collection technique, feedback with regard to contamination rates and implementation of blood culture collection kits. Although skin antisepsis can reduce the burden of contamination, 20% or more of skin organisms are located deep within the dermis and are unaffected by antisepsis. Changing needles before bottle inoculation is not advisable as it increases the risk to acquire needle stick injuries without decreasing contamination rates.

[0012] Some conventional systems and techniques for reducing blood culture contamination include discarding the initial aliquot of blood taken from central venous catheters, venipunctures, and other vascular access systems. However, these systems require the user to mechanically manipulate an intravascular device, or require a complex series of steps that are difficult to ensure being followed.

SUMMARY

[0013] This document presents systems and methods for reducing blood culture contamination, lysing of cells, and vein collapse. In some implementations, a system and method can eliminate user variability in disinfection, and also eliminate the risk of skin cells getting into the blood culture sample. The systems and methods disclosed herein do not require a change in existing clinical processes, other than to potentially indicate when a vacutainer or other blood collection device (i.e., syringe) should be attached for drawing contaminant-free blood samples.

[0014] In some implementations of the systems and methods disclosed herein the withdrawal of blood is accomplished passively by use of the patient's own blood pressure, thereby reducing the risk of vein collapse and eliminating any additional user steps over current practice. The systems and methods can be applied to accommodate short-path direct stick or butterfly venipuncture systems. They can also be used with samples drawn through a catheter.

[0015] In one aspect, a blood sequestration device is presented. The blood sequestration device includes an inlet port and an outlet port. The blood sequestration device further includes a sequestration chamber connected with the inlet port, the sequestration chamber having a vent comprising an air permeable blood barrier. The blood sequestration device further includes a sampling channel having a proximal end connected with the inlet port and a distal end connected with the outlet port.

[0016] In another aspect, a blood sequestration device connected with a blood sampling pathway is described. The blood sampling pathway has a patient needle and a sample collection device. The blood sequestration device includes an inlet port connected with the patient needle, and a sequestration chamber connected with the inlet port, the sequestration chamber having a vent comprising an air permeable blood barrier. The blood sequestration device further includes a sampling channel having a proximal end connected with the inlet port, and an outlet port connected with a distal end of the sampling channel and with the sample collection device.

[0017] In yet another aspect, a blood sequestration device connected with a blood sampling system is described. The blood sampling system includes a patient needle for accessing a blood sample from a patient, and a sample needle that is sealed and adapted for receiving an evacuated blood collection tube. The blood sequestration device includes an inlet port connected with the patient needle to receive the blood sample from the patient. The blood sequestration device further includes a sequestration chamber connected with the inlet port and having a vent comprising an air permeable blood barrier, the sequestration chamber for receiving and sequestering a first portion of the blood sample prior to the sample needle being unsealed by the evacuated blood collection tube. The blood sequestration device further includes a sampling channel having a proximal end connected with the inlet port, the

sampling channel for conveying a subsequent portion of the blood sample once the sample needle is unsealed by the evacuated blood collection tube. The blood sequestration device further includes an outlet port connected with a distal end of the sampling channel for conveying the subsequent portion of the blood sample to the sample needle.

[0018] In yet another aspect, a blood sample optimization system is disclosed and described. The blood sample optimization system includes a blood sampling system for accessing and acquiring one or more samples of a patient's blood, and a blood sequestration device for receiving and sequestering a first portion of the one or more samples of the patient's blood which might be contaminated by a venipuncture process and which could result in a false positive identification of a pathogen in the patient's blood.

[0019] The blood sampling system includes a patient needle configured for a venipuncture of a patient to access a sample of blood of a patient, a blood sampling pathway connected with the patient needle for conveying the sample of blood, and a sample needle configured for receiving an evacuated blood collection container to collect and contain a subsequent portion of the sample of blood.

[0020] In yet another aspect, a blood sequestration device is disclosed and described. In some implementations, the blood sequestration device can include an inlet port, an outlet port connected with the inlet port, and a sequestration chamber connected with the inlet port. The sequestration chamber can have a vent comprising an air permeable blood barrier.

[0021] The blood sequestration device is connected along the blood sampling pathway between the patient needle and the sample needle, and includes an inlet port for receiving the sample of blood. The blood sequestration device further includes a sequestration chamber connected with the inlet port for receiving a first amount of the sample of blood, the sequestration chamber having a vent comprising an air permeable blood barrier for sequestering at least a first portion of the first amount of the sample of blood. The blood sequestration device may further include a sampling channel having a proximal end connected with the inlet port, the sampling channel conveying a subsequent amount of the sample of blood to the evacuated blood collection container upon the sequestration chamber sequestering at least the first portion of the first amount of the sample of blood. The blood

sequestration device further includes an outlet port connected with a distal end of the sampling channel, the outlet port for outputting the subsequent amount of the sample of blood.

[0022] The details of one or more embodiments are set forth in the accompanying drawings and the description below. Other features and advantages will be apparent from the description and drawings, and from the claims.

BRIEF DESCRIPTION OF THE DRAWINGS

[0023] These and other aspects will now be described in detail with reference to the following drawings.

[0024] FIG. 1 illustrates a blood sample optimization system.

[0025] FIG. 2 illustrates a blood sample optimization system in accordance with an alternative implementation.

[0026] FIG. 3 illustrates a blood sample optimization system in accordance with another alternative implementation.

[0027] FIG. 4 illustrates a blood sample optimization system in accordance with another alternative implementation.

[0028] FIG. 5 illustrates a blood sample optimization system in accordance with another alternative implementation.

[0029] FIG. 6 illustrates a blood sample optimization system in accordance with an alternative implementation.

[0030] FIG. 7 is a flowchart of a method for optimizing a quality of a blood culture.

[0031] FIGS. 8A – 8E illustrate a blood sequestration system for non-contaminated blood sampling, in accordance with some implementations.

[0032] FIG. 9 illustrates a pathway splitter for use in a blood sequestrations system.

[0033] FIGS. 10A – 10D illustrate a blood sequestration system for non-contaminated blood sampling, in accordance with alternative implementations.

[0034] FIGS. 11A – 11E illustrate a blood sequestration system for non-contaminated blood sampling, in accordance with other alternative implementations.

[0035] FIGS. 12A-12D illustrate a blood sample optimization system including a blood sequestration device in accordance with yet other alternative implementations.

[0036] FIGS. 13A-13D illustrate a blood sample optimization system 1300 in accordance with yet another alternative implementations.

[0037] FIGS. 14A-14E illustrate yet another implementation of a blood sampling system to sequester contaminates of an initial aliquot or sample to reduce false positives in blood cultures or tests performed on a patient's blood sample.

[0038] FIGS. 15A-15G illustrate a blood sequestration device and method of using the same, in accordance with yet another implementation.

[0039] FIGS. 16A-16D illustrate a blood sequestration device in accordance with yet another implementation.

[0040] FIGS. 17A – 17E illustrate a bottom member of a housing for a blood sequestration device.

[0041] FIGS. 18A – 18F illustrate a top member of a housing for a blood sequestration device.

[0042] FIGS. 19A and 19B illustrate a blood sequestration device having a top member mated with a bottom member.

[0043] FIG. 20 shows a blood sample optimization system including a blood sequestration device.

[0044] FIG. 21 illustrates a non-vented blood sequestration device using a wicking material chamber.

[0045] FIGS. 22A and 22B illustrate a material makeup of a filter for sequestering blood in a sequestration chamber of a blood sequestration device.

[0046] FIGS. 23A and 23B illustrate another implementation of a blood sequestration device that uses a vacuum force from a blood collection device.

[0047] Like reference symbols in the various drawings indicate like elements.

DETAILED DESCRIPTION

[0048] This document describes blood sample optimization systems and methods for reducing or eliminating contaminates in collected blood samples, which in turn reduces or eliminates false positive readings in blood cultures or other testing of collected blood samples. In some implementations, a blood sample optimization system includes a patient needle for vascular access to a patient's bloodstream, a sample needle for providing a blood sample to a blood collection container, such as an evacuated blood collection container or tube like a Vacutainer™ or the like, or other sampling device, and a blood sequestration device located between the patient needle and the sample needle. The blood sequestration device includes a sequestration chamber for sequestering an initial, potentially contaminated aliquot of blood, and may further include a sampling channel that bypasses the sequestration chamber to convey likely uncontaminated blood between the patient needle and the sample needle after the initial aliquot of blood is sequestered in the sequestration chamber.

[0049] FIG. 1 illustrates a blood sample optimization system in accordance with some implementations. The system includes a patient needle 1 to puncture the skin of a patient to access the patient's vein and blood therein. The system further includes a sample needle (i.e., a resealably closed needle for use with Vacutainers™ or the like) 5, which may be contained within and initially sealed by a resealable boot 10, a Luer activated valve, or another collection interface or device. The resealable boot 10 can be pushed aside or around the sample needle 5 by application of a Vacutainer™ bottle (not shown) for drawing the patient's blood. The system can further include a low volume chamber 30 that leads to the sample needle 5, but also includes an orifice or one or more channels 45 that lead to a sequestration chamber 55 formed by a housing 50.

[0050] The sequestration chamber 55 is a chamber, channel, pathway, lock, or other structure for receiving and holding a first aliquot of the patient's blood, which may be in a predetermined or measured amount, depending on a volume of the sequestration chamber 55. The first draw of blood typically contains or is more susceptible to containing organisms that cause bacteraemia and sepsis or other pathogens than subsequent blood draws. The sequestration chamber 55 can be a vessel encased in a solid housing, formed in or defined by the housing itself, or can be implemented as tubing or a lumen. The sequestration chamber 55, regardless how formed and implemented, may have a predetermined volume. In some implementations, the predetermined volume may be based on a volume of the patient needle, i.e. ranging from less than the volume of the patient needle to any volume up to or greater than 20 times or more of the volume of the patient needle. The predetermined volume of the sequestration chamber 55 may also be established to economize or minimize an amount of blood to be sequestered and disposed of.

[0051] The sequestration chamber 55 can be formed, contained or housed in a chamber housing 50, and can be made of plastic, rubber, steel, aluminum or other suitable material. For example, the sequestration chamber 55 could be formed of flexible tubing or other elastomeric materials. The sequestration chamber 55 further includes an air permeable blood barrier 20 that allows air to exit the sequestration chamber 55. As used herein the term "air permeable blood barrier" means an air permeable but substantially blood impermeable substance, material, or structure. Examples may include hydrophobic membranes and coatings, a hydrophilic membrane or coating combined with a hydrophobic membrane or coating, mesh, a filter, a mechanical valve, antimicrobial material, or any other means of allowing air to be displaced from the sequestration chamber 55 as it is filled with blood. In various exemplary embodiments, an air permeable blood barrier may be formed by one or more materials that allow air to pass through until contacted by a liquid, such material then becomes completely or partially sealed to prevent or inhibit the passage of air and/or liquid. In other words, prior to contact with liquid, the material forms a barrier that is air permeable. After contact with a liquid, the material substantially or completely prevents the further passage of air and/or liquid.

[0052] The orifice or channel 45 can be any desired length, cross-sectional shape or size, and/or can be formed to depart from the low volume chamber 30 at any desired angle or orientation. The orifice or channel 45 may also include a one-way flap or valve 60 that maintains an initial aliquot of blood sample within the sequestration chamber 55. In some specific implementations, the orifice or channel 45 can include a "duck bill" or flapper valve 60, or the like, for one-way flow of blood from low volume chamber 30 to the sequestration chamber 55. The air permeable blood barrier 20 can also be constructed of a material that allows air to exit but then seals upon contact with blood, thereby not allowing external air to enter sequestration chamber 55. This sealing would eliminate the need for a valve.

[0053] Valve 60 can be any type of valve or closing mechanism. Chamber 30 is designed to hold virtually no residual blood, and can be designed to be adapted to hold or allow pass-through of a particular volume or rate of blood into sequestration chamber 55. Likewise, sequestration chamber 55 may also include any type of coating, such as an anti-microbial coating, or a coating that aids identification and/or diagnosis of components of the first, sequestered blood draw.

[0054] Housing 50 and 40 can be formed of any suitable material, including plastic, such as acrylonitrile butadiene styrene (ABS) or other thermoplastic or polymeric material, rubber, steel, or aluminum. The air permeable blood barrier 20 can include a color-providing substance, or other signaling mechanism, that is activated upon contact with blood from the initial blood draw, or when air displacement is stopped, or any combination of events with blood in the sequestration chamber 55. The air permeable barrier may also include an outer layer such as a hydrophobic membrane or cover that inhibits or prevents the inadvertent or premature sealing of the filter by an external fluid source, splash etc. Sequestration chamber 55 can also be translucent or clear to enable a user to visually confirm the chamber is filled.

[0055] FIG. 2 illustrates a blood sample optimization system in accordance with some alternative implementations. In the implementation shown in FIG. 2, a sequestration chamber 55, or waste chamber, surrounds the patient needle 1, with an open-ended cuff or housing connected with the waste chamber and encircling the sample needle housing base and housing. The patient needle 1 and sample needle 5 are connected together by a boot 56, which forms a continuous blood draw channel therethrough. The boot 56 includes a single

orifice or channel leading from the blood draw channel into sequestration chamber 55. The device can include more than one single orifice or channel, in other implementations. Each orifice or channel can include a one-way valve, and can be sized and adapted for predetermined amount of blood flow.

[0056] The sequestration chamber 55 includes an air permeable blood barrier. The filter can further include a sensor or indicator to sense and/or indicate, respectively, when a predetermined volume of blood has been collected in the sequestration chamber 55. That indication will alert a user to attach an evacuated blood collection tube or bottle, such as a Vacutainer™ to the sample needle 5. The housing for the sequestration chamber 55 can be any size or shape, and can include any type of material to define an interior space or volume therein. The interior space is initially filled only with air, but can also be coated with an agent or substance, such as a decontaminate, solidifying agent, or the like. Once evacuated blood collection tube is attached to the sample needle 5, blood will flow automatically into the patient needle 1, through the blood draw channel and sample needle 5, and into the bottle. The sample needle 5 is covered by a resealable boot, coating or membrane that seals the sample needle when a blood collection bottle is not attached thereon or thereto.

[0057] FIG. 3 illustrates a blood sample optimization system in accordance with some alternative implementations. In the implementation shown, a sample needle 5 is surrounded by a resealable boot or membrane, and is further connected with a patient needle 1. A blood flow channel is formed through the sample needle and the patient needle. The connection between the sample needle and patient needle includes a "T" or "Y" connector 102, which includes a channel, port or aperture leading out from the main blood flow channel to a sequestration chamber 104.

[0058] The T or Y connector 102 may include a flap or one-way valve, and have an opening that is sized and adapted for a predetermined rate of flow of blood. The sequestration chamber 104 can be formed from tubing, or be formed by a solid housing, and is initially filled with air. The sequestration chamber 104 will receive blood that flows out of a patient automatically, i.e. under pressure from the patient's own blood pressure. The sequestration chamber 104 includes an air permeable blood barrier 106, preferably at the distal end of tubing that forms the sequestration chamber 104, and which is connected at the

proximal end to the T or Y connector 102. The T or Y connector 102 can branch off at any desired angle for most efficient blood flow, and can be formed so as to minimize an interface between the aperture and channel and the main blood flow channel, so as to minimize or eliminate mixing of the initial aliquot of blood with main blood draw samples.

[0059] In some alternative implementations, the sample needle may be affixed to a tubing of any length, as shown in FIG. 4, connecting at its opposite end to the T or Y connector 102. The sequestration chamber 104 can be any shape or volume so long as it will contain a predetermined amount of blood sample in the initial aliquot. The T or Y connector 102 may also include an opening or channel that is parallel to the main blood flow channel. The air permeable blood barrier may further include an indicator 107 or other mechanism to indicate when a predetermined amount of blood has been collected in the sequestration chamber, or when air being expelled reaches a certain threshold, i.e. to zero. The tubing can also include a clip 109 that can be used to pinch off and prevent fluid flow therethrough.

[0060] Once the air permeable blood barrier and primary chamber are sealed the initial aliquot of blood is trapped in the sequestration chamber 104, an evacuated blood collection tube, such as a Vacutainer™ bottle may be attached to the sample needle 5 to obtain the sample. The blood collection tube can be removed, and the sample needle 5 will be resealed. Any number of follow-on blood collection tubes can then be attached for further blood draws or samples. Upon completion of all blood draws, the system can be discarded, with the initial aliquot of blood remaining trapped in the sequestration chamber 104.

[0061] FIG. 5 illustrates a blood sample optimization system in accordance with some alternative implementations. In the implementation shown, a sample needle 5 is connected with a patient needle by tubing. A "T" or "Y" connector 120 is added along the tubing at any desired location, and includes an aperture, port or channel leading to a sequestration chamber 204, substantially as described above.

[0062] FIG. 6 illustrates a blood sample optimization system in accordance with some alternative implementations, in which a sequestration chamber 304, formed as a primary collection channel, receives an initial aliquot of blood, and is provided adjacent to the blood sampling channel. The sequestration chamber 304 can encircle the blood sampling

channel, the patient needle 1, and/or the sample needle 5. The primary collection channel can include a T or Y connector 120, or other type of aperture or channel. The sequestration chamber 304 includes an air permeable blood barrier, which can also include an indicator of being contacted by a fluid such as blood, as described above.

[0063] In some implementations, either the patient needle 1 or the sample needle 5, or both, can be replaced by a Luer lock male or female connector. However, in various implementations, the connector at a sample needle end of the blood sample optimization system is initially sealed to permit the diversion of the initial aliquot of blood to the sequestration chamber, which is pressured at ambient air pressure and includes the air outlet of the air permeable blood barrier. In this way, the system passively and automatically uses a patient's own blood pressure to overcome the ambient air pressure of the sequestration chamber to push out air through the air permeable blood barrier and displace air in the sequestration chamber with blood.

[0064] FIG. 7 is a flowchart of an exemplary method for optimizing the quality of a blood culture. At 702, a clinician places a needle into a patient's vein. At 704, blood then flows into a sequestration chamber, pushing the air in the sequestration chamber out of the sequestration chamber through an air permeable blood barrier. In some implementations, the volume of the sequestration chamber is less than 0.1 to more than 5 cubic centimeters (cc's), or more. The sequestration chamber is sized and adapted to collect a first portion of a blood sample, which is more prone to contamination than secondary and other subsequent portion of the blood sample or subsequent draws. Since the sequestration chamber has an air-permeable blood barrier through which air can be displaced by blood pushed from the patient's vein, such blood will naturally and automatically flow into the sequestration chamber before it is drawn into or otherwise enters into a Vacutainer or other bottle for receiving and storing a blood sample.

[0065] When the sequestration chamber fills, the blood will gather at or otherwise make contact with the air permeable blood barrier, which will inhibit or prevent blood from passing therethrough. At 706, when the blood comes into contact with the entire internal surface area of the air permeable blood barrier, the air permeable blood barrier is then closed and air no longer flows out or in. At 708, the clinician may be provided an indictor or can

see the full chamber, to indicate the evacuated blood collection tube, such as a Vacutainer™ can be attached. The indicator can include visibility into the primary chamber to see whether it is full, the blood barrier changing color, for example, or other indicator. The fill time of the sequestration chamber may be substantially instantaneous, so such indicator, if present, may be only that the sequestration chamber is filled.

[0066] Prior to an evacuated blood collection tube being attached, communication between the needle, sampling channel, and the sequestration chamber is restricted by the sealing of the sequestration chamber blood barrier thereby not permitting air to reenter the system through the sequestration. Sealing the communication path could also be accomplished with a mechanical twist or other movement, a small orifice or tortuous pathway, eliminating the need for a separate valve or mechanical movement or operation by the clinician. At 710, once the evacuated blood collection tube is removed, the self-sealing membrane closes the sample needle, and at 712, additional subsequent evacuated blood collection tubes may be attached. Once samples have been taken, at 714 the device is removed from the patient and discarded.

[0067] FIGS. 8A – 8E illustrate an exemplary blood sample optimization system 800 for non-contaminated blood sampling, in accordance with some implementations. The blood sample optimization system 800 includes an inlet port 802 that can be connected to tubing, a patient needle (or both), or other vascular or venous access device, and a pathway splitter 804 having a first outlet to a sequestration chamber tubing 806 and a second outlet to sample collection tubing 808. One or both of the sequestration chamber tubing 806 and the sample collection tubing 808 can be formed of tubing. In some implementations, the sequestration chamber tubing 806 is sized so as to contain a particular volume of initial blood sample. The sample collection tubing 808 will receive a blood sample once the sequestration chamber tubing 806 is filled. The sample collection tubing 808 can be connected to a Vacutainer™ base or housing 810, or other blood sample collection device.

[0068] The blood sequestration system 800 further includes a blood sequestration device 812 which, as shown in more detail in FIGS. 8B – 8D, includes a housing 818 that includes a sampling channel 820 defining a pathway for the non-contaminated sample collection tubing 808 or connected at either end to the non-contaminated sample collection

tubing 808. The sampling channel 820 can be curved through the housing 818 so as to better affix and stabilize the housing 818 at a location along the non-contaminated sample collection tubing 808.

[0069] The blood sequestration device 812 further includes a sequestration chamber 822 connected with the sequestration chamber tubing 806 or other chamber. The sequestration chamber 822 terminates at an air permeable blood barrier 824. The air permeable blood barrier 824 can also include a coloring agent that turns a different color upon full contact with blood, as an indicator that the regular collection of blood samples (i.e. the non-contaminated blood samples) can be initiated. Other indicators may be used, such as a small light, a sound generation mechanism, or the like. In some implementations, the air permeable blood barrier is positioned at a right angle from the direction of sequestration chamber 822, but can be positioned at any distance or orientation in order to conserve space and materials used for the housing 818. The housing 818 and its contents can be formed of any rigid or semi-rigid material or set of materials.

[0070] FIG. 9 illustrates a pathway splitter 900 for use in a blood sequestrations system, such as those shown in FIGS. 8A – 8E, for example. The pathway splitter 900 includes an inlet port 902, a main line outlet port 904, and a sequestration channel outlet port 906. The inlet port 902 can be connected to main tubing that is in turn connected to a patient needle system, or directly to a patient needle. The main line outlet port 904 can be connected to main line tubing to a blood sampling system, such as a vacutainer base or housing, or directly to such blood sampling system. The sequestration channel outlet port 906 can be connected to sequestration tubing for receiving and sequestering a first sample of blood, up to a measured amount or predetermined threshold. Alternatively, the sequestration channel outlet port 906 can be connected to a sequestration chamber. The sequestration channel outlet port 906 is preferably 20-70 degrees angled from the main line outlet port 904, which in turn is preferably in-line with the inlet port 902. Once the predetermined amount of initial blood sample is sequestered in the sequestration tubing or chamber, in accordance with mechanisms and techniques described herein, follow-on blood samples will flow into the inlet port 902 and directly out the main line outlet port 904, without impedance.

[0071] FIGS. 10A – 10D illustrate a blood sequestration device 1000 in accordance with alternative implementations. The blood sequestration device 1000 includes an inlet port 1002, a main outlet port 1004, and a sequestration channel port 1006. The inlet port 1002 can be connected to a patient needle or related tubing. The main outlet port 1004 can be connected to a blood sample collection device such as a Vacutainer, associated tubing, or a Luer activated valve, or the like. The sequestration channel port 1006 splits off from the main outlet port 1004 to a sequestration chamber 1008. In some implementations, the sequestration chamber 1008 is formed as a helical channel within a housing or other container 1001.

[0072] The sequestration chamber 1008 is connected at the distal end to an air permeable blood barrier 1010, substantially as described above. Air in the sequestration chamber 1008 is displaced through the air permeable blood barrier 1010 by an initial aliquot of blood that is guided into the sequestration channel port 1006. Once the sequestration chamber 1008 is filled, further blood draws through the main outlet port 1004 can be accomplished, where these samples will be non-contaminated.

[0073] FIGS. 11A – 11E illustrate a blood sequestration device 1100 in accordance with other alternative implementations. The blood sequestration device 1100 includes an inlet port 1102, similar to the inlet ports described above, a main outlet port 1104, and a sequestration channel port 1106 that splits off from the main outlet port 1104 and inlet port 1102. The sequestration channel port is connected to a sequestration chamber 1108. In the implementation shown in FIGS. 11A – 11E, the blood sequestration device includes a base member 1101 having a channel therein, which functions as the sequestration chamber 1108. The channel can be formed as a tortuous path through the base member 1101, which is in turn shaped and formed to rest on a limb of a patient.

[0074] A portion of the sequestration chamber 1108 can protrude from the base member or near a top surface of the base member, just before exiting to an air permeable blood barrier 1110, to serve as a blood sequestration indicator 1109. The indicator 1109 can be formed of a clear material, or a material that changes color when in contact with blood.

[0075] In some implementations, the blood sequestration device 1100 can include a blood sampling device 1120 such as a normally closed needle, Vacutainer™ shield or other collection device. The blood sampling device 1120 can be manufactured and sold with the blood sequestration device 1100 for efficiency and convenience, so that a first aliquot of blood that may be contaminated by a patient needle insertion process can be sequestered. Thereafter, the blood sampling device 1120 can draw non-contaminated blood samples to reduce the risk of false positive testing and ensure a non-contaminated sample.

[0076] FIGS. 12A-12D illustrate a blood sample optimization system 1200 in accordance with yet other alternative implementations. The system 1200 includes a blood sequestration device 1202 for attaching to a blood sampling device 1204, such as a Vacutainer™ or other collection and sampling device. The blood sequestration device 1202 is configured and arranged to receive, prior to a Vacutainer™ container or vial being attached to a collection needle of the blood sampling device 1204, a first aliquot or amount of blood, and sequester that first aliquot or amount in a sequestration channel of the blood sequestration device 1202.

[0077] In some implementations, the blood sequestration device 1202 can include an inlet port 1212, a main outlet port, and a sequestration channel port. The inlet port 1212 can be connected to a patient needle or related tubing. The main outlet port 1214 can be connected to a normally closed needle or device to enable connection with an evacuated blood collection container or other collection device such as a Vacutainer™, associated tubing, luer connectors, syringe, a Luer activated valve, or the like. The sequestration channel port splits off from the main outlet port to a sequestration chamber 1218.

[0078] In some implementations, the sequestration chamber 1218 is formed as a channel within the body of a sequestration device 1202. The sequestration chamber 1218 can be a winding channel, such as a U-shaped channel, an S-shaped channel, a helical channel, or any other winding channel. The sequestration device 1202 can include a housing or other containing body, and one or more channels formed therein. As shown in FIGS. 12A and 12B, the sequestration device 1202 includes a main body 1206 and a cap 1208. The main body 1206 is formed with one or more cavities or channels, which are further formed with

one or more arms 1210 that extend from the cap 1208, and which abut the cavities or channels in the main body 1206 to form the primary collection port and main outlet port.

[0079] FIGS. 13A-13D illustrate a blood sample optimization system 1300 in accordance with yet other alternative implementations. The system 1300 includes a blood sequestration device 1302 for attaching to a blood sampling device 1304, such as a Vacutainer or other bodily fluid collection and sampling device. The blood sequestration device 1302 is configured and arranged to receive, prior to a Vacutainer container or vial being attached to a collection needle of the blood sampling device 1304, a first aliquot or amount of blood, and to sequester that first aliquot or amount of blood or other bodily fluid in a sequestration channel of the blood sequestration device 1302.

[0080] The blood sequestration device 1302 includes a housing 1301 having an inlet port 1314, a main outlet port 1312, and a sequestration channel port 1316. The inlet port 1314 can be connected to a patient needle or associated tubing. The main outlet port 1312 can be connected to a normally closed needle or device to enable connection with an evacuated blood collection container or other collection device such as a Vacutainer™, associated tubing, luer connectors, syringe, a Luer activated valve, or the like. The sequestration channel port 1316 splits off from the main inlet port 1314 to a sequestration chamber 1318.

[0081] In the implementation shown in FIGS. 13A-D, the sequestration chamber 1318 is formed as a cavity or chamber within housing 1301 or formed by walls that define housing 1301. The sequestration chamber 1318 can be a winding channel, such as a U-shaped channel, an S-shaped channel, a helical channel, or any other winding channel, that is defined by the cooperation and connection of housing 1301 with cap 1307 which cap 1307 can include a protrusion 1305 that provides one or more walls or directors for the winding channel in the sequestration chamber 1318. The protrusion 1305 from the cap 1307 can be straight or curved, and may have various channels, apertures or grooves embedded therein, and can extend from the cap 1307 any angle or orientation. When the cap 1307 is connected with the housing 1301 to complete the formation of the sequestration chamber 1318, the protrusion 1305 forms at least part of the winding channel to sequester a first aliquot or

amount of blood or other bodily fluid in a sequestration channel formed in the sequestration chamber 1318 and by the winding channel.

[0082] The sequestration chamber 1318 includes an air permeable blood barrier 1310, substantially as described above. Air in the sequestration chamber 1318 is displaced through the air permeable blood barrier 1310 by an initial aliquot of blood that is provided into the sequestration chamber 1318 by the blood pressure of the patient. Once the sequestration chamber 1318 is filled and the air in the sequestration chamber 1318 displaced, the blood pressure of the patient will be insufficient to drive or provide further blood into the blood sequestration device 1302, and in particular the outlet port 1312, until a force such as a vacuum or other pressure, such as provided by the blood sample collection device like Vacutainer is provided to draw out a next aliquot or amount of blood or bodily fluid. Further blood draws through the main outlet port 1312 can be accomplished, where these samples will be non-contaminated since any contaminants would be sequestered in the sequestration chamber 1318 with the first aliquot of blood.

[0083] FIGS. 14A-14E illustrate yet another implementation of a blood sampling system 1400 to sequester contaminates of an initial aliquot or sample to reduce false positives in blood cultures or tests performed on a patient's blood sample. The blood sampling system 1400 includes a blood sequestration device 1401 that can be connected between a blood sample collection device 1403 and a patient needle (not shown). The blood sample collection device 1403 can be a Vacutainer or the like. The blood sequestration device 1401 includes an inlet port 1402 that can be connected with a patient needle that is inserted into a patient's vascular system for access to and withdrawing of a blood sample. The inlet port 1402 may also be connected with tubing or other conduit that is in turn connected with the patient needle.

[0084] The inlet port 1402 defines an opening into the blood sequestration device 1401, which opening can be the same cross sectional dimensions as tubing or other conduit connected with the patient needle or the patient needle itself. For instance, the opening can be circular with a diameter of approximately 0.045 inches, but can have a diameter of between 0.01 inches or less to 0.2 inches or more. The blood sequestration device 1401 further includes an outlet port 1404, which defines an opening out of the blood sequestration

device 1401 and to the blood sample collection device 1403. The outlet port 1404 may also be connected with tubing or other conduit that is in turn connected with the blood sequestration device 1403. The outlet port 1404 can further include a connector device such as a threaded cap, a Luer connector (male or female), a non threaded interference or glue joint fitting for attachment of various devices including but not limited to tubing, or the like.

[0085] The blood sequestration device 1401 further includes a sampling channel 1406 between the inlet port 1402 and the outlet port 1404, and which functions as a blood sample pathway once a first aliquot of blood has been sequestered. The sampling channel 1406 can be any sized, shaped or configured channel, or conduit. In some implementations, the sampling channel 1406 has a substantially similar cross sectional area as the opening of the inlet port 1402. In other implementations, the sampling channel 1406 can gradually widen from the inlet port 1402 to the outlet port 1404.

[0086] The blood sequestration device 1401 further includes a sequestration chamber 1408 that is connected to and split off or diverted from the sampling channel 1406 at any point between the inlet port 1402 and the outlet port 1404, but preferably from a proximal end of the sampling channel 1406 near the inlet port 1402. The sequestration chamber 1408 is at first maintained at atmospheric pressure, and includes an air outlet 1412 at or near a distal end of the sequestration chamber 1408 opposite the diversion point from the sampling channel 1406. The air outlet 1412 includes an air permeable blood barrier 1412. As shown in FIG. 14B, the air permeable blood barrier 1412 can be overlaid with a protective cover 1416. The protective cover 1416 can be sized and configured to inhibit a user from touching the air permeable blood barrier 1412 with their finger or other external implement, while still allowing air to exit the air permeable blood barrier 1412 as the air is displaced from the sequestration chamber 1408 by blood being forced into the sequestration chamber 1408 by a patient's own blood pressure. In addition the protective cover 1416 can be constructed to inhibit or prevent accidental exposure of the air permeable blood barrier to environmental fluids or splashes. This can be accomplished in a variety of mechanical ways including but not limited to the addition of a hydrophobic membrane to the protective cover.

[0087] As shown in FIGS. 14C and 14D, the sampling channel 1406 can be cylindrical or frusto-conical in shape, going from a smaller diameter to a larger diameter, to

minimize a potential to lyse red blood cells. Likewise, the sampling channel 1406 is formed with a minimal amount of or no sharp turns or edges, which can also lyse red blood cells. The sampling channel 1406 splits off to the sequestration chamber 1408 near the inlet port 1402 via a diversion pathway 1409. The diversion pathway 1409 can have any cross-sectional shape or size, but is preferably similar to the cross-sectional shape of at least part of the inlet port 1402.

[0088] In some implementations, the sampling channel 1406 and the sequestration chamber 1408 are formed by grooves, channels, locks or other pathways formed in housing 1414. The housing 1414 can be made of plastic, metal or other rigid or semi-rigid material. The housing 1414 can have a bottom member that sealably mates with a top member. One or both of the bottom member and the top member can include the sampling channel 1406 and the sequestration chamber 1408, as well as the diversion pathway 1409, the inlet port 1402, and the outlet port 1404. In some other implementations, one or more of the diversion pathway 1409, the inlet port 1402, and/or the outlet port 1404 can be at least partially formed by a cap member that is connected to either end of the housing 1414. In some implementations, the top member and the bottom member, as well as the cap member(s), can be coupled together by laser welding, heat sealing, gluing, snapping, screwing, bolting, or the like. In other implementations, some or all of the interior surface of the diversion pathway 1409 and/or sequestration chamber 1408 can be coated or loaded with an agent or substance, such as a decontaminate, solidifying agent, or the like. For instance, a solidifying agent can be provided at the diversion pathway 1409 such that when the sequestration chamber 1408 is filled and the initial aliquot of blood backs up to the diversion pathway 1409, that last amount of sequestered blood could solidify, creating a barrier between the sequestration chamber 1408 and the sampling channel 1406.

[0089] FIGS. 15A-15G illustrate a blood sequestration device 1500. The blood sequestration device 1500 can be connected to a normally closed needle or device to enable connection with an evacuated blood collection container or other collection device such as a Vacutainer™, associated tubing, luer connectors, syringe, a Luer activated valve, or the like.

[0090] The blood sequestration device 1500 includes an inlet port 1502 that can be connected with a patient needle that is inserted into a patient's vascular system for access to

and withdrawing of a blood sample. The inlet port 1502 may also be connected with tubing or other conduit that is in turn connected with the patient needle. The inlet port 1502 defines an opening into the blood sequestration device 1500, which opening may be the same cross sectional dimensions as tubing or other conduit connected with the patient needle or the patient needle itself. For instance, the opening can be circular with a diameter of approximately 0.045 inches, but can have a diameter of between 0.01 inches or less to 0.2 inches or more.

[0091] The inlet port 1502 can also include a sealing or fluid-tight connector or connection, such as threading or Luer fitting, or the like. In some implementations, tubing or other conduit associated with the patient needle can be integral with the inlet port 1502, such as by co-molding, gluing, laser weld, or thermally bonding the parts together. In this manner, the blood sequestration device 1500 can be fabricated and sold with the patient needle as a single unit, eliminating the need for connecting the patient needle to the blood sequestration device 1500 at the time of blood draw or sampling.

[0092] The blood sequestration device 1500 further includes an outlet port 1504, which defines an opening out of the blood sequestration device 1500 and to the blood sample collection device. The outlet port 1504 may also be connected with tubing or other conduit that is in turn connected with the blood sequestration device, and may also include a sealing or fluid-tight connector or connection, such as threading or Luer fitting, or the like. Accordingly, as discussed above, the blood sequestration device 1500 can be fabricated and sold with the patient needle and/or tubing and the blood sample collection device as a single unit, eliminating the need for connecting the patient needle and the blood sample collection device to the blood sequestration device 1500 at the time of blood draw or sampling.

[0093] The blood sequestration device 1500 further includes a sampling channel 1506 between the inlet port 1502 and the outlet port 1504, and which functions as a blood sample pathway once a first aliquot of blood has been sequestered. The sampling channel 1506 can be any sized, shaped or configured channel or conduit. In some implementations, the sampling channel 1506 has a substantially similar cross sectional area as the opening of the inlet port 1502. In other implementations, the sampling channel 1506 can gradually widen from the inlet port 1502 to the outlet port 1504.

[0094] The blood sequestration device 1500 further includes a sequestration chamber 1508 that is connected to and split off or diverted from the sampling channel 1506 at any point between the inlet port 1502 and the outlet port 1504, but preferably from a proximal end of the sampling channel 1506 near the inlet port 1502. In some implementations, the diversion includes a Y-shaped junction. The sequestration chamber 1508 is preferably maintained at atmospheric pressure, and includes a vent 1510 at or near a distal end of the sequestration chamber 1508. The vent 1510 includes an air permeable blood barrier 1512. FIG. 15C illustrates the blood sequestration device 1500 with the sequestration chamber 1508 filled with a first aliquot or sample of blood from the patient.

[0095] The air permeable blood barrier 1512 can be covered with a protective cover 1516. The protective cover 1516 can be sized and configured to inhibit a user from touching the air permeable blood barrier 1512 with their finger or other external implement, while still allowing air to exit the air permeable blood barrier 1512 as the air is displaced from the sequestration chamber 1508 by blood being forced into the sequestration chamber 1508 by a patient's own blood pressure. The protective cover 1516 can be constructed to inhibit or prevent accidental exposure of the filter to environmental fluids or splashes. This can be accomplished in a variety of mechanical ways including but not limited to the addition of a hydrophobic membrane to the protective cover.

[0096] FIG. 15B is a perspective view of the blood sequestration device 1500 from the outlet port 1504 and top side of a housing 1501 of the blood sequestration device 1500 that includes the vent 1510, and illustrating an initial aliquot of blood filling sequestration chamber 1508 while the sampling channel 1506 is empty, before a sample collection device is activated. FIG. 15G is a perspective view of the blood sequestration device 1500 from the outlet port 1504 and bottom side of the housing 1501 of the blood sequestration device 1500, and illustrating the initial aliquot of blood filling sequestration chamber 1508 while the sampling channel 1506 is empty, before the sample collection device is activated. FIG. 15C is another perspective view of the blood sequestration device 1500 from the inlet port 1502 and top side of a housing 1501 of the blood sequestration device 1500 that includes the vent 1510, and illustrating blood now being drawn through sampling channel 1506 while the sequestered blood remains substantially in the sequestration chamber 1508.

[0097] FIG. 15D is a cross section of the blood sequestration device 1500 in accordance with some implementations, showing the housing 1501 that defines the sampling channel 1506 and the sequestration chamber 1508. FIGS. 15E and 15F illustrate various form factors of a housing for a blood sequestration device, in accordance with one or more implementations described herein.

[0098] The sequestration chamber 1508 can have a larger cross-sectional area than the sampling channel 1506, and the cross-sectional area and length can be configured for a predetermined or specific volume of blood to be sequestered or locked. The sampling channel 1506 can be sized to be compatible with tubing for either or both of the patient needle tubing or the blood collection device tubing.

[0099] The housing 1501 can be formed of multiple parts or a single, unitary part. In some implementations, and as illustrated in FIG. 15D, the housing 1501 includes a top member 1520 and a bottom member 1522 that are mated together, one or both of which having grooves, channels, locks, conduits or other pathways pre-formed therein, such as by an injection molding process or by etching, cutting, drilling, etc. The top member 1520 can be connected with the bottom member 1522 by any mating or connection mechanism, such as by laser welding, thermal bonding, ultrasonic welding, gluing, using screws, rivets, bolts, or the like, or by other mating mechanisms such as latches, grooves, tongues, pins, flanges, or the like.

[00100] In some implementations, such as shown in FIG. 15D, the top member 1520 can include the grooves, channels, locks, conduits or other pathways, while the bottom member 1522 can include a protrusion 1524 that is sized and adapted to fit into at least one of the grooves, channels, locks or other pathways of the top member 1520. The protrusion 1524 can provide a surface feature, such as a partial groove or channel, for instance, to complete the formation of either the sampling channel 1506 and/or the sequestration chamber 1508. In some implementations, the protrusion 1524 can be formed with one or more angled sides or surfaces for a tighter fit within the corresponding groove, channel, lock or other pathway. In yet other implementations, both the top member 1520 and the bottom member can include grooves, channels, locks or other pathways, as well as one or more protrusions 1524.

[00101] In some implementations, the sampling channel 1506 and the sequestration chamber 1508 are formed by grooves, channels, locks or other pathways formed in housing 1501. The housing 1501 can be made of any suitable material, including rubber, plastic, metal or other material. The housing 1501 can be formed of a clear or translucent material, or of an opaque or non-translucent material. In other implementations, the housing 1501 can be mostly opaque or non-translucent, while the housing surface directly adjacent to the sampling channel 1506 and/or the sequestration chamber 1508 is clear or translucent, giving a practitioner a visual cue or sign that the sequestration chamber 1508 is first filled to the extent necessary or desired, and/or then a visual cue or sign that the sequestered blood remains sequestered while a clean sample of blood is drawn through the sampling channel 1506. Other visual cues or signs of the sequestration can include, without limitation: the air permeable blood barrier 1512 turning a different color upon contact, saturation, or partial saturation with blood; a color-coded tab or indicator at any point along or adjacent to the sequestration chamber; an audible signal; a vibratory signal; or other signal.

[00102] After a venipuncture by a patient needle of a patient (not shown), which could gather a number of pathogens from the patient's skin, a first amount of the patient's blood with those pathogens will make its way into the input port 1502 blood sequestration device 1500 and flow into the sequestration chamber 1508 by following the path of least resistance, as the patient's own blood pressure overcomes the atmospheric pressure in the sequestration chamber 1508 to displace air therein through the air permeable blood barrier 1512. The patient's blood pressure will not be sufficient to overcome the air pressure that builds up in the sealed sampling channel 1506. Eventually, the sequestration chamber 1508, which has a predetermined volume, is filled with blood that displaces air through the air permeable blood barrier 1512. Once the blood hits the air permeable blood barrier, the blood interacts with the air permeable blood barrier 1512 material to completely or partially seal the vent 1510. A signal or indication may be provided that the practitioner can now utilize the Vacutainer capsule or other blood sample collection device to acquire a next amount of the patient's blood for sampling. The blood in the sequestration chamber 1508 is now effectively sequestered in the sequestration chamber.

[00103] Upon filling the blood sequestration pathway 1508 but prior to use of the Vacutainer or other blood sample collection device, the patient's blood pressure may drive compression of the air in the sampling channel 1506, possibly resulting in a small amount of blood moving past the diversion point to the sequestration chamber 1508 and into the sampling channel 1506, queuing up the uncontaminated blood to be drawn through the sampling channel 1506.

[00104] FIGS. 16-19 illustrate yet another implementation of a blood sequestration device. FIGS. 16A-16D illustrate a blood sequestration device 1600 that can be connected between a blood sample collection device, such as an evacuated blood collection container like a Vacutainer™ (not shown), and a patient needle (not shown) and/or associated tubing. FIG. 17 illustrates a bottom member of the blood sequestration device, and FIG. 18 illustrates a top member of the blood sequestration device, which top member and bottom member can be mated together to form an input port, and output port, a sequestration chamber and a sampling channel, as explained more fully below. FIGS. 19A and B show the top member and bottom member mated together. It should be understood that FIGS. 16-19 illustrate one exemplary manner of constructing a blood sequestration device as described herein, and other forms of construction are possible.

[00105] Referring to FIGS. 16A – D, the blood sequestration device 1600 includes an inlet port 1602 that can be connected with a patient needle that is inserted into a patient's vascular system for access to and withdrawing of a blood sample. The inlet port 1602 may also be connected with tubing or other conduit that is in turn connected with the patient needle. The inlet port 1602 defines an opening into the blood sequestration device 1600, which opening can be the same cross sectional dimensions as tubing or other conduit connected with the patient needle or the patient needle itself. For instance, the opening can be circular with a diameter of approximately 0.045 inches, but can have a diameter of between 0.01 inches or less to 0.2 inches or more.

[00106] The inlet port 1602 can also include a sealing or fluid-tight connector or connection, such as threading or Luer fitting, or the like. In some implementations, tubing or other conduit associated with the patient needle can be integral with the inlet port 1602, such as by co-molding, gluing, laser weld, or thermally bonding the parts together. In this manner,

the blood sequestration device 1600 can be fabricated and sold with the patient needle and/or tubing as a single unit, eliminating the need for connecting the patient needle to the blood sequestration device 1600 at the time of blood draw or sampling.

[00107] The blood sequestration device 1600 further includes an outlet port 1604, which defines an opening out of the blood sequestration device 1600 and to the blood sample collection device. The outlet port 1604 may also be connected with tubing or other conduit that is in turn connected with the blood sequestration device, and may also include a sealing or fluid-tight connector or connection, such as threading or Luer fitting, or the like. Accordingly, as discussed above, the blood sequestration device 1600 can be fabricated and sold with the patient needle and/or tubing and the blood sample collection device as a single unit, eliminating the need for connecting the patient needle and the blood sample collection device to the blood sequestration device 1600 at the time of blood draw or sampling.

[00108] The blood sequestration device 1600 further includes a sampling channel 1606 between the inlet port 1602 and the outlet port 1604, and a sequestration chamber 1608 that is connected to and split off or diverted from the sampling channel 1606 at any point between the inlet port 1602 and the outlet port 1604. The sampling channel 1606 functions as a blood sampling pathway once a first aliquot of blood has been sequestered in the sequestration chamber 1608. The sampling channel 1606 can be any sized, shaped or configured channel, or conduit. In some implementations, the sampling channel 1606 has a substantially similar cross sectional area as the opening of the inlet port 1602. In other implementations, the sampling channel 1606 can gradually widen from the inlet port 1602 to the outlet port 1604. The sequestration chamber 1608 may have a larger cross section to form a big reservoir toward the sequestration channel path so that the blood will want to enter the reservoir first versus entering a smaller diameter on the sampling channel 1606, as is shown more fully in FIGS. 17 and 19.

[00109] In some exemplary implementations, the diversion between the sampling channel 1606 and the sequestration chamber 1608 is by diverter junction 1607. Diverter junction 1607 may be a substantially Y-shaped, T-shaped, or U-shaped. In some preferred exemplary implementations, and as shown in FIG. 17A – 17B, the diverter junction 1607 is configured such that the flow out of the inlet port 1602 is preferentially directed toward the

sequestration chamber 1608. The sequestration chamber 1608 may also include or form a curve or ramp to direct the initial blood flow toward and into the sequestration chamber 1608.

[00110] The sequestration chamber 1608 is preferably maintained at atmospheric pressure, and includes a vent 1610 at or near a distal end of the sequestration chamber 1608. The vent 1610 may include an air permeable blood barrier 1612 as described above.

[00111] The blood sequestration device 1600 can include a housing 1601 that can be formed of multiple parts or a single, unitary part. In some implementations, and as illustrated in FIGS. 17A – 17E and FIGS. 18A – 18F, the housing 1601 includes a top member 1620 and a bottom member 1622 that are mated together. The blood sequestration device 1600 can also include a gasket or other sealing member (not shown) so that when the top member 1620 is mechanically attached with the bottom member 1622, the interface between the two is sealed by the gasket or sealing member. The FIGS. 17A – 17E illustrate a bottom member 1622 of a housing for a blood sequestration device 1600. The bottom member 1622 can include grooves, channels, locks, conduits or other pathways pre-formed therein, such as by an injection molding process or by etching, cutting, drilling, etc., to form the sampling channel 1606, the sequestration chamber 1608, and diverter junction 1607.

[00112] The sequestration chamber 1608 may have a larger cross section than the sampling channel 1606 so that the blood will preferentially move into the sequestration chamber first versus entering a smaller diameter on the sampling channel 1606.

[00113] FIGS. 18A – 18F illustrate the top member 1620, which can be connected with the bottom member 1622 by any mating or connection mechanism, such as by laser welding, thermal bonding, gluing, using screws, rivets, bolts, or the like, or by other mating mechanisms such as latches, grooves, tongues, pins, flanges, or the like. The top member 1620 can include some or all of the grooves, channels, locks, conduits or other pathways to form the sampling channel 1606, the sequestration chamber 1608, and the diverter junction 1607. In yet other implementations, both the top member 1620 and the bottom member 1622 can include the grooves, channels, locks or other pathways.

[00114] In some implementations, the sampling channel 1606 and the sequestration chamber 1608 are formed by grooves, channels, locks or other pathways formed in housing 1601. The housing 1601 can be made of rubber, plastic, metal or any other suitable material. The housing 1601 can be formed of a clear or translucent material, or of an opaque or non-translucent material. In other implementations, the housing 1601 can be mostly opaque or non-translucent, while the housing surface directly adjacent to the sampling channel 1606 and/or the sequestration chamber 1608 may be clear or translucent, giving a practitioner a visual cue or sign that the sequestration chamber 1608 is first filled to the extent necessary or desired, and/or then a visual cue or sign that the sequestered blood remains sequestered while a clean sample of blood is drawn through the sampling channel 1606. Other visual cues or signs of the sequestration can include, without limitation: the air permeable blood barrier 1612 turning a different color upon contact, saturation, or partial saturation with blood; a color-coded tab or indicator at any point along or adjacent to the sequestration chamber; an audible signal; a vibratory signal; or other signal.

[00115] As shown in FIGS. 18A – 18F, the air permeable blood barrier 1612 can be covered with, or surrounded by, a protective member 1616. The protective member 1616 can be sized and configured to inhibit a user from touching the air permeable blood barrier 1612 with their finger or other external implement, while still allowing air to exit the air permeable blood barrier 1612 as the air is displaced from the sequestration chamber 1608. In some implementations, the protective member 1616 includes a protrusion that extends up from a top surface of the top member 1620 and around the air permeable blood barrier 1612. The protective cover 1616 can be constructed to inhibit or prevent accidental exposure of the filter to environmental fluids or splashes. This can be accomplished in a variety of mechanical ways including but not limited to the addition of a hydrophobic membrane to the protective cover.

[00116] In use, the blood sequestration device 1600 includes a sampling channel 1606 and a sequestration chamber 1608. Both pathways are initially air-filled at atmospheric pressure, but the sampling channel 1606 is directed to an output port 1604 that will be initially sealed by a Vacutainer or other such sealed blood sampling device, and the

sequestration chamber 1608 terminates at a vent 1610 to atmosphere that includes an air permeable blood barrier 1612.

[00117] After a venipuncture by a patient needle of a patient (not shown), which could gather a number of pathogens from the patient's skin, a first amount of the patient's blood with those pathogens will pass through input port 1602 of blood sequestration device 1600. This initial volume of potentially contaminated blood will preferentially flow into the sequestration chamber 1608 by finding the path of least resistance. The patient's own blood pressure overcomes the atmospheric pressure in the vented sequestration chamber 1608 to displace air therein through the air permeable blood barrier 1612, but is not sufficient to overcome the air pressure that builds up in the sealed sampling channel 1606. In various exemplary embodiments, the sequestration chamber 1608 and sampling channel 1606 can be configured such that the force generated by the patient's blood pressure is sufficient to overcome any effect of gravity, regardless of the blood sequestration device's orientation.

[00118] Eventually, the sequestration chamber 1608 fills with blood that displaces air through the air permeable blood barrier 1612. Once the blood contacts the air permeable blood barrier, the blood interacts with the air permeable blood barrier 1612 material to completely or partially seal the vent 1610. A signal or indication may be provided that the practitioner can now utilize the Vacutainer or other blood sampling device.

[00119] Upon filling the blood sequestration pathway 1608 but prior to use of the Vacutainer or other blood sample collection device, the patient's blood pressure may drive compression of the air in the sampling channel 1606, possibly resulting in a small amount of blood moving past the diversion point into the sampling channel 1606, queuing up the uncontaminated blood to be drawn through the sampling channel 1606.

[00120] FIG. 19A is a side view, and FIG. 19B is a cross-sectional view, of the blood sequestration device 1600, illustrating the top member 1620 mated with the bottom member 1622.

[00121] FIG. 20 shows a blood sample optimization system 2000 that includes a patient needle 2002 for vascular access to a patient's bloodstream, a blood sample collection device 2004 to facilitate the collecting of one or more blood samples, and a conduit 2006

providing a fluid connection between the patient needle 2002 and the blood sample collection device 2004. In some implementations, the blood sample collection device 2004 includes a protective shield that includes a sealed collection needle on which a sealed vacuum-loaded container is placed, which, once pierced by the collection needle, draws in a blood sample under vacuum pressure or force through the conduit 2006 from the patient needle 2002.

[00122] The blood sample optimization system 2000 further includes a blood sequestration device 2008, located at any point on the conduit 2006 between the patient needle 2002 and the blood sample collection device 2004 as described herein.

[00123] FIG. 21 illustrates a non-vented blood sequestration device 2100 using a wicking material chamber. The blood sequestration device 2100 includes a housing 2101 that has a sampling channel 2104 that is at least partially surrounded or abutted by a sequestration chamber 2102 that is filled with a wicking material. An initial aliquot of blood is drawn in from the patient needle into the sampling channel 2104 where it is immediately wicked into the wicking material of the sequestration chamber 2102. The wicking material and/or sequestration chamber 2102 is sized and adapted to receive and hold a predetermined amount of blood, such that follow-on or later blood draws pass by the wicking material and flow straight through the sampling channel 2104 to a sampling device such as a Vacutainer. The wicking material can include a substance such as a solidifier, a decontaminate, or other additive.

[00124] As described herein, an air permeable blood barrier may be created using a wide variety of different structures and materials. As shown in FIGS. 22A and B, an air permeable blood barrier 2202 of a blood sequestration device 2200 can include a polymer bead matrix 2204, in which at least some beads are treated to make them hydrophilic. The air permeable blood barrier 2202 further includes a self-sealing material 2206, such as carboxymethyl cellulose (CMC) or cellulose gum, or other sealing material. The air permeable blood barrier 2202 can further include voids 2208 that permit air flow before contact or during partial contact with a fluid such as blood. As shown in FIG. 22B, contact with a fluid causes the self-sealing material 2206 to swell and close off the voids 2208, occluding air flow through the voids 2208 and creating a complete or partial seal.

[00125] FIGS. 23A and B illustrate yet another implementation of a blood sequestration device 2300, having an inlet port 2302 to connect with a patient needle, an outlet port 2304 to connect with a blood sample collection device, a sequestration chamber 2306, and a sampling channel 2308 that bypasses the sequestration chamber 2306 once the sequestration chamber is filled to an initial aliquot of potentially contaminated blood to be sequestered. The sequestration chamber 2306 includes a hydrophobic plug 2312 at a distal end of the sequestration chamber 2306 that is farthest from the inlet port 2302. A vacuum or other drawing force applied from the outlet port 2304, such as from a Vacutainer or the like, draws in blood into the inlet port 2302 and directly into the sequestration chamber 2306, where the initial aliquot of blood will contact the hydrophobic plug 2312 and cause the initial aliquot of blood to back up into the sequestration chamber 2306 and be sequestered there. A small amount of blood may make its way into the sampling channel 2308, which is initially closed off by valve 2308. Upon release of the valve 2308, and under further force of the vacuum or other force, follow-on amounts of blood will flow into inlet port 2302, bypass the sequestration chamber 2306, and flow into and through sampling channel 2308 toward the outlet port 2304 and to the collection device.

[00126] The sampling channel 2308 can have any suitable geometry and can be formed of plastic tubing or any other suitable material. Valve 2308 can be a clip or other enclosing device to pinch, shunt, bend or otherwise close off the sampling channel before the initial aliquot of blood is sequestered in the sequestration chamber 2306.

[00127] Although a variety of embodiments have been described in detail above, other modifications are possible. Other embodiments may be within the scope of the following claims.

CLAIMS

1. A blood sequestration device comprising;

an inlet port;

an outlet port;

a sequestration chamber having a vent that includes an air permeable blood barrier; and

a sampling channel having a distal end connected with the outlet port;

each of the sequestration chamber and the sampling channel being connected with the inlet port via a junction that is sized and configured such that a first portion of blood flows into the sequestration chamber to displace air therein through the air permeable blood barrier and to be sequestered in the sequestration chamber, and a second portion of blood is allowed to bypass the sequestration chamber and the first portion of blood sequestered therein to be directed into the sampling channel toward the outlet port.

2. The blood sequestration device in accordance with claim 1, wherein the air permeable blood barrier includes an air permeable material that seals at least partially upon contact with blood.

3. The blood sequestration device in accordance with claim 1, further comprising a housing that defines a part of each of the inlet port, the outlet port, the sequestration chamber, and the sampling channel.

4. The blood sequestration device in accordance with claim 3, wherein the sequestration chamber includes a sequestration channel defined in the housing.

5. The blood sequestration device in accordance with claim 2, wherein the housing comprises a bottom member mated with a top member, each of the bottom

member and the top member defining a part of each of the inlet port, the outlet port, the sequestration chamber, and the sampling channel.

6. A blood sequestration device connected with a blood sampling pathway having a patient needle and a sample collection device, the blood sequestration device comprising:

an inlet port connected with the patient needle;

an outlet port connected with the sample collection device;

a sequestration chamber having a vent that includes an air permeable blood barrier; and

and a sampling channel having a distal end connected with the outlet port;

each of the sequestration chamber and the sampling channel being connected with the inlet port via a junction that is sized and configured such that a first portion of blood flows into the sequestration chamber to displace air therein through the air permeable blood barrier and to be sequestered in the sequestration chamber, and a second portion of blood is allowed to bypass the sequestration chamber and the first portion of blood sequestered therein to be directed into the sampling channel toward the outlet port and the sample collection device.

7. The blood sequestration device in accordance with claim 6, further comprising a housing that houses and defines the inlet port, the outlet port, the sequestration chamber, and the sampling channel.

8. The blood sequestration device in accordance with claim 6, wherein the inlet port is connected with the patient needle via a first portion of the blood sampling pathway.

9. The blood sequestration device in accordance with claim 6, wherein the outlet port is connected with the sample collection device via a second portion of the blood sampling pathway.

10. The blood sequestration device in accordance with claim 6, wherein the air permeable blood barrier includes an air permeable material that seals at least partially upon contact with blood.

11. The blood sequestration device in accordance with claim 7, wherein the sequestration chamber includes a sequestration channel defined in the housing.

12. The blood sequestration device in accordance with claim 11, wherein the sequestration channel has a proximal end connected with the inlet port, and a distal end having the vent comprising an air permeable blood barrier.

13. A bodily fluid sequestration device comprising;

an inlet port;

an outlet port connected with the inlet port;

a sequestration chamber connected with the inlet port via a junction, the sequestration chamber having a vent that includes an air permeable bodily fluid barrier; and

a housing that houses and defines the inlet port, the outlet port, and the sequestration chamber, the sequestration chamber and the junction configured to direct a first portion of bodily fluid from the inlet port into the sequestration chamber toward the air permeable bodily fluid barrier, the air permeable bodily fluid barrier including an air permeable material that forms a barrier to bodily fluids upon contact with the bodily fluids,

whereupon formation of the barrier enables sequestration of the first portion of bodily fluid in the sequestration chamber, and enables a second portion of bodily fluid from the inlet port to bypass the sequestration chamber via the junction and the first portion of bodily fluid, toward the outlet port.

14. The bodily fluid sequestration device in accordance with claim 13, wherein the air permeable bodily fluid barrier includes an air permeable material that seals upon contact with the bodily fluids.

15. The bodily fluid sequestration device in accordance with claim 13, wherein the sequestration chamber includes a sequestration channel defined in the housing.

16. The bodily fluid sequestration device in accordance with claim 13, further comprising a sampling pathway connected with the inlet port, wherein the sampling pathway conveys the second portion of bodily fluid from the inlet port to the outlet port via the junction.

17. The bodily fluid sequestration device in accordance with claim 13, wherein the housing comprises a bottom member mated with a top member, each of the bottom member and the top member defining a part of each of the inlet port, the outlet port, and the sequestration chamber.

18. The bodily fluid sequestration device in accordance with claim 13, further comprising a sampling channel having a proximal end connected with the inlet port via the junction.

19. The blood sequestration device in accordance with claim 18, wherein the housing comprises a bottom member mated with a top member, each of the bottom member and the top member defining a part of each of the inlet port, the outlet port, the sequestration chamber, and the sampling channel.

20. A blood sequestration system comprising:

a blood sampling pathway having a patient needle and a sample collection device; and

a blood sequestration device, the blood sequestration device comprising:

an inlet port connected with the patient needle;

an outlet port connected with the sample collection device;

a sequestration chamber having a vent that includes an air permeable blood barrier; and

and a sampling channel having a distal end connected with the outlet port;

each of the sequestration chamber and the sampling channel being connected with the inlet port via a junction that is sized and configured such that a first portion of blood flows into the sequestration chamber to displace air therein through the air permeable blood barrier and to be sequestered in the sequestration chamber, and a second portion of blood is allowed to bypass the sequestration chamber and the first portion of blood sequestered therein to be directed into the sampling channel toward the outlet port and the sample collection device.

21. The blood sequestration system in accordance with claim 20, further comprising a housing that houses and defines the inlet port, the outlet port, the sequestration chamber, and the sampling channel.

22. The blood sequestration system in accordance with claim 20, wherein the inlet port is connected with the patient needle via a first portion of the blood sampling pathway.

23. The blood sequestration system in accordance with claim 20, wherein the outlet port is connected with the sample collection device via a second portion of the blood sampling pathway.

24. The blood sequestration system in accordance with claim 20, wherein the air permeable blood barrier includes an air permeable material that seals at least partially upon contact with blood.

25. The blood sequestration system in accordance with claim 24, wherein the sequestration chamber includes a sequestration channel defined in the housing.

26. The blood sequestration device in accordance with claim 25, wherein the sequestration channel has a proximal end connected with the inlet port, and a distal end having the vent comprising an air permeable blood barrier.

ABSTRACT

Blood sample optimization systems and methods are described that reduce or eliminate contaminates in collected blood samples, which in turn reduces or eliminates false positive readings in blood cultures or other testing of collected blood samples. A blood sample optimization system can include a blood sequestration device located between a patient needle and a sample needle. The blood sequestration device can include a sequestration chamber for sequestering an initial, potentially contaminated aliquot of blood, and may further include a sampling channel that bypasses the sequestration chamber to convey likely uncontaminated blood between the patient needle and the sample needle after the initial aliquot of blood is sequestered in the sequestration chamber.

Electronic Patent Application Fee Transmittal

Application Number:	15994559
Filing Date:	31-May-2018
Title of Invention:	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD
First Named Inventor/Applicant Name:	Bobby E. Rogers
Filer:	David Lynn Devernoe/Lisa Leao
Attorney Docket Number:	251102.000027.KURIN2CON2

Filed as Small Entity

Filing Fees for Utility under 35 USC 111(a)

Description	Fee Code	Quantity	Amount	Sub-Total in USD($)
Basic Filing:				
Pages:				
Claims:				
INDEPENDENT CLAIMS IN EXCESS OF 3	2201	1	230	230
Miscellaneous-Filing:				
Petition:				
Patent-Appeals-and-Interference:				
Post-Allowance-and-Post-Issuance:				

Description	Fee Code	Quantity	Amount	Sub-Total in USD($)
Extension-of-Time:				
Miscellaneous:				
			Total in USD ($)	**230**

Electronic Acknowledgement Receipt	
EFS ID:	33072942
Application Number:	15994559
International Application Number:	
Confirmation Number:	4704
Title of Invention:	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD
First Named Inventor/Applicant Name:	Bobby E. Rogers
Customer Number:	153290
Filer:	David Lynn Devernoe/Lisa Leao
Filer Authorized By:	David Lynn Devernoe
Attorney Docket Number:	251102.000027.KURIN2CON2
Receipt Date:	02-JUL-2018
Filing Date:	31-MAY-2018
Time Stamp:	19:16:17
Application Type:	Utility under 35 USC 111(a)

Payment information:

Submitted with Payment	yes
Payment Type	DA
Payment was successfully received in RAM	$230
RAM confirmation Number	070318INTEFSW00006270201507
Deposit Account	
Authorized User	
The Director of the USPTO is hereby authorized to charge indicated fees and credit any overpayment as follows:	

File Listing:

Document Number	Document Description	File Name	File Size(Bytes)/ Message Digest	Multi Part /.zip	Pages (if appl.)
1	Applicant Response to Pre-Exam Formalities Notice	Response_NTFCAP_KURIN2CON2.pdf	226378 f824707a8fb77f26838d303ac1ac86099452f9a0	no	4
Warnings:					
Information:					
2	Specification	Substitute_Specification_MU_KURIN2CON2.pdf	295474 dccd188ea46bbf47afcfc71beb564d395c5093dd	no	39
Warnings:					
Information:					
3	Specification	Substitute_Specification_CLEAN_KURIN2CON2.pdf	292518 0665aa75275653474a79bfc3592a7be230000474	no	39
Warnings:					
Information:					
4	Fee Worksheet (SB06)	fee-info.pdf	30595 2fb7bde1725ee2e9194017f1534f01dfed9ce0ef	no	2
Warnings:					
Information:					
		Total Files Size (in bytes):	844965		

This Acknowledgement Receipt evidences receipt on the noted date by the USPTO of the indicated documents, characterized by the applicant, and including page counts, where applicable. It serves as evidence of receipt similar to a Post Card, as described in MPEP 503.

New Applications Under 35 U.S.C. 111

If a new application is being filed and the application includes the necessary components for a filing date (see 37 CFR 1.53(b)-(d) and MPEP 506), a Filing Receipt (37 CFR 1.54) will be issued in due course and the date shown on this Acknowledgement Receipt will establish the filing date of the application.

National Stage of an International Application under 35 U.S.C. 371

If a timely submission to enter the national stage of an international application is compliant with the conditions of 35 U.S.C. 371 and other applicable requirements a Form PCT/DO/EO/903 indicating acceptance of the application as a national stage submission under 35 U.S.C. 371 will be issued in addition to the Filing Receipt, in due course.

New International Application Filed with the USPTO as a Receiving Office

If a new international application is being filed and the international application includes the necessary components for an international filing date (see PCT Article 11 and MPEP 1810), a Notification of the International Application Number and of the International Filing Date (Form PCT/RO/105) will be issued in due course, subject to prescriptions concerning national security, and the date shown on this Acknowledgement Receipt will establish the international filing date of the application.

UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

APPLICATION NUMBER	FILING or 371(c) DATE	GRP ART UNIT	FIL FEE REC'D	ATTY.DOCKET.NO	TOT CLAIMS	IND CLAIMS
15/994,559	05/31/2018	1629	1315	251102.000027.KURIN2CON2	26	4

CONFIRMATION NO. 4704

UPDATED FILING RECEIPT

153290
TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 3000
Atlanta, GA 30308-2219

OC000000100747956

Date Mailed: 07/06/2018

Receipt is acknowledged of this non-provisional patent application. The application will be taken up for examination in due course. Applicant will be notified as to the results of the examination. Any correspondence concerning the application must include the following identification information: the U.S. APPLICATION NUMBER, FILING DATE, NAME OF APPLICANT, and TITLE OF INVENTION. Fees transmitted by check or draft are subject to collection. Please verify the accuracy of the data presented on this receipt. **If an error is noted on this Filing Receipt, please submit a written request for a Filing Receipt Correction. Please provide a copy of this Filing Receipt with the changes noted thereon. If you received a "Notice to File Missing Parts" for this application, please submit any corrections to this Filing Receipt with your reply to the Notice. When the USPTO processes the reply to the Notice, the USPTO will generate another Filing Receipt incorporating the requested corrections**

Inventor(s)

Bobby E. Rogers, San Diego, CA;
Gino Kang, Irvine, CA;
John Detloff, San Diego, CA;

Applicant(s)

KURIN, INC., San Diego, CA;

Assignment For Published Patent Application

KURIN, INC., San Diego, CA

Power of Attorney: The patent practitioners associated with Customer Number 153290

Domestic Priority data as claimed by applicant

This application is a CON of 15/140,448 04/27/2016 PAT 10010282
which claims benefit of 62/196,797 07/24/2015
and claims benefit of 62/238,636 10/07/2015
and claims benefit of 62/318,194 04/04/2016

Foreign Applications for which priority is claimed (You may be eligible to benefit from the **Patent Prosecution Highway** program at the USPTO. Please see http://www.uspto.gov for more information.) - None.
Foreign application information must be provided in an Application Data Sheet in order to constitute a claim to foreign priority. See 37 CFR 1.55 and 1.76.

Permission to Access Application via Priority Document Exchange: Yes

Permission to Access Search Results: Yes

Applicant may provide or rescind an authorization for access using Form PTO/SB/39 or Form PTO/SB/69 as appropriate.

If Required, Foreign Filing License Granted: 06/21/2018
The country code and number of your priority application, to be used for filing abroad under the Paris Convention, is **US 15/994,559**
Projected Publication Date: 10/11/2018
Non-Publication Request: No
Early Publication Request: No
**** SMALL ENTITY ****
Title

BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD

Preliminary Class

514

Statement under 37 CFR 1.55 or 1.78 for AIA (First Inventor to File) Transition Applications: No

PROTECTING YOUR INVENTION OUTSIDE THE UNITED STATES

Since the rights granted by a U.S. patent extend only throughout the territory of the United States and have no effect in a foreign country, an inventor who wishes patent protection in another country must apply for a patent in a specific country or in regional patent offices. Applicants may wish to consider the filing of an international application under the Patent Cooperation Treaty (PCT). An international (PCT) application generally has the same effect as a regular national patent application in each PCT-member country. The PCT process **simplifies** the filing of patent applications on the same invention in member countries, but **does not result** in a grant of "an international patent" and does not eliminate the need of applicants to file additional documents and fees in countries where patent protection is desired.

Almost every country has its own patent law, and a person desiring a patent in a particular country must make an application for patent in that country in accordance with its particular laws. Since the laws of many countries differ in various respects from the patent law of the United States, applicants are advised to seek guidance from specific foreign countries to ensure that patent rights are not lost prematurely.

Applicants also are advised that in the case of inventions made in the United States, the Director of the USPTO must issue a license before applicants can apply for a patent in a foreign country. The filing of a U.S. patent application serves as a request for a foreign filing license. The application's filing receipt contains further information and guidance as to the status of applicant's license for foreign filing.

Applicants may wish to consult the USPTO booklet, "General Information Concerning Patents" (specifically, the section entitled "Treaties and Foreign Patents") for more information on timeframes and deadlines for filing foreign patent applications. The guide is available either by contacting the USPTO Contact Center at 800-786-9199, or it can be viewed on the USPTO website at http://www.uspto.gov/web/offices/pac/doc/general/index.html.

For information on preventing theft of your intellectual property (patents, trademarks and copyrights), you may wish to consult the U.S. Government website, http://www.stopfakes.gov. Part of a Department of Commerce initiative, this website includes self-help "toolkits" giving innovators guidance on how to protect intellectual property in specific

countries such as China, Korea and Mexico. For questions regarding patent enforcement issues, applicants may call the U.S. Government hotline at 1-866-999-HALT (1-866-999-4258).

LICENSE FOR FOREIGN FILING UNDER

Title 35, United States Code, Section 184

Title 37, Code of Federal Regulations, 5.11 & 5.15

GRANTED

The applicant has been granted a license under 35 U.S.C. 184, if the phrase "IF REQUIRED, FOREIGN FILING LICENSE GRANTED" followed by a date appears on this form. Such licenses are issued in all applications where the conditions for issuance of a license have been met, regardless of whether or not a license may be required as set forth in 37 CFR 5.15. The scope and limitations of this license are set forth in 37 CFR 5.15(a) unless an earlier license has been issued under 37 CFR 5.15(b). The license is subject to revocation upon written notification. The date indicated is the effective date of the license, unless an earlier license of similar scope has been granted under 37 CFR 5.13 or 5.14.

This license is to be retained by the licensee and may be used at any time on or after the effective date thereof unless it is revoked. This license is automatically transferred to any related applications(s) filed under 37 CFR 1.53(d). This license is not retroactive.

The grant of a license does not in any way lessen the responsibility of a licensee for the security of the subject matter as imposed by any Government contract or the provisions of existing laws relating to espionage and the national security or the export of technical data. Licensees should apprise themselves of current regulations especially with respect to certain countries, of other agencies, particularly the Office of Defense Trade Controls, Department of State (with respect to Arms, Munitions and Implements of War (22 CFR 121-128)); the Bureau of Industry and Security, Department of Commerce (15 CFR parts 730-774); the Office of Foreign AssetsControl, Department of Treasury (31 CFR Parts 500+) and the Department of Energy.

NOT GRANTED

No license under 35 U.S.C. 184 has been granted at this time, if the phrase "IF REQUIRED, FOREIGN FILING LICENSE GRANTED" DOES NOT appear on this form. Applicant may still petition for a license under 37 CFR 5.12, if a license is desired before the expiration of 6 months from the filing date of the application. If 6 months has lapsed from the filing date of this application and the licensee has not received any indication of a secrecy order under 35 U.S.C. 181, the licensee may foreign file the application pursuant to 37 CFR 5.15(b).

SelectUSA

The United States represents the largest, most dynamic marketplace in the world and is an unparalleled location for business investment, innovation, and commercialization of new technologies. The U.S. offers tremendous resources and advantages for those who invest and manufacture goods here. Through SelectUSA, our nation works to promote and facilitate business investment. SelectUSA provides information assistance to the international investor community; serves as an ombudsman for existing and potential investors; advocates on behalf of U.S. cities, states, and regions competing for global investment; and counsels U.S. economic development organizations on investment attraction best practices. To learn more about why the United States is the best country in the world to develop

technology, manufacture products, deliver services, and grow your business, visit http://www.SelectUSA.gov or call +1-202-482-6800.

PATENT APPLICATION FEE DETERMINATION RECORD

Substitute for Form PTO-875

Application or Docket Number: 15/994,559

APPLICATION AS FILED - PART I

FOR	(Column 1) NUMBER FILED	(Column 2) NUMBER EXTRA	SMALL ENTITY RATE($)	SMALL ENTITY FEE($)	OR	OTHER THAN SMALL ENTITY RATE($)	OTHER THAN SMALL ENTITY FEE($)
BASIC FEE (37 CFR 1.16(a), (b), or (c))	N/A	N/A	N/A	75		N/A	
SEARCH FEE (37 CFR 1.16(k), (i), or (m))	N/A	N/A	N/A	330		N/A	
EXAMINATION FEE (37 CFR 1.16(o), (p), or (q))	N/A	N/A	N/A	380		N/A	
TOTAL CLAIMS (37 CFR 1.16(i))	26 minus 20 =	* 6	x 50 =	300	OR		
INDEPENDENT CLAIMS (37 CFR 1.16(h))	4 minus 3 =	* 1	x 230 =	230			
APPLICATION SIZE FEE (37 CFR 1.16(s))	If the specification and drawings exceed 100 sheets of paper, the application size fee due is $310 ($155 for small entity) for each additional 50 sheets or fraction thereof. See 35 U.S.C. 41(a)(1)(G) and 37 CFR 1.16(s).			0.00			
MULTIPLE DEPENDENT CLAIM PRESENT (37 CFR 1.16(j))				0.00			
* If the difference in column 1 is less than zero, enter "0" in column 2.			TOTAL	1315		TOTAL	

APPLICATION AS AMENDED - PART II

AMENDMENT A

	(Column 1) CLAIMS REMAINING AFTER AMENDMENT		(Column 2) HIGHEST NUMBER PREVIOUSLY PAID FOR	(Column 3) PRESENT EXTRA	SMALL ENTITY RATE($)	SMALL ENTITY ADDITIONAL FEE($)	OR	OTHER THAN SMALL ENTITY RATE($)	OTHER THAN SMALL ENTITY ADDITIONAL FEE($)
Total (37 CFR 1.16(i))	*	Minus	**	=	x =		OR	x =	
Independent (37 CFR 1.16(h))	*	Minus	***	=	x =		OR	x =	
Application Size Fee (37 CFR 1.16(s))									
FIRST PRESENTATION OF MULTIPLE DEPENDENT CLAIM (37 CFR 1.16(j))							OR		
					TOTAL ADD'L FEE		OR	TOTAL ADD'L FEE	

AMENDMENT B

	(Column 1) CLAIMS REMAINING AFTER AMENDMENT		(Column 2) HIGHEST NUMBER PREVIOUSLY PAID FOR	(Column 3) PRESENT EXTRA	RATE($)	ADDITIONAL FEE($)		RATE($)	ADDITIONAL FEE($)
Total (37 CFR 1.16(i))	*	Minus	**	=	x =		OR	x =	
Independent (37 CFR 1.16(h))	*	Minus	***	=	x =		OR	x =	
Application Size Fee (37 CFR 1.16(s))									
FIRST PRESENTATION OF MULTIPLE DEPENDENT CLAIM (37 CFR 1.16(j))							OR		
					TOTAL ADD'L FEE		OR	TOTAL ADD'L FEE	

* If the entry in column 1 is less than the entry in column 2, write "0" in column 3.
** If the "Highest Number Previously Paid For" IN THIS SPACE is less than 20, enter "20".
*** If the "Highest Number Previously Paid For" IN THIS SPACE is less than 3, enter "3".
The "Highest Number Previously Paid For" (Total or Independent) is the highest found in the appropriate box in column 1.

To: ryan.schneider@troutman.com,patents@troutman.com,chris.franich@troutman.com
From: PAIR_eOfficeAction@uspto.gov
Cc: PAIR_eOfficeAction@uspto.gov
Subject: Private PAIR Correspondence Notification for Customer Number 153290

Jul 06, 2018 04:24:47 AM

Dear PAIR Customer:

TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 3000
Atlanta, GA 30308-2219
UNITED STATES

The following USPTO patent application(s) associated with your Customer Number, 153290 , have new outgoing correspondence. This correspondence is now available for viewing in Private PAIR.

The official date of notification of the outgoing correspondence will be indicated on the form PTOL-90 accompanying the correspondence.

Disclaimer:
The list of documents shown below is provided as a courtesy and is not part of the official file wrapper. The content of the images shown in PAIR is the official record.

Application	Document	Mailroom Date	Attorney Docket No.
15994559	APP.FILE.REC	07/06/2018	251102.000027.KURIN2CON2

To view your correspondence online or update your email addresses, please visit us anytime at https://sportal.uspto.gov/secure/myportal/privatepair.

If you have any questions, please email the Electronic Business Center (EBC) at EBC@uspto.gov with 'e-Office Action' on the subject line or call 1-866-217-9197 during the following hours:

Monday - Friday 6:00 a.m. to 12:00 a.m.

Thank you for prompt attention to this notice,

UNITED STATES PATENT AND TRADEMARK OFFICE

PATENT APPLICATION INFORMATION RETRIEVAL SYSTEM

UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

APPLICATION NO.	FILING DATE	FIRST NAMED INVENTOR	ATTORNEY DOCKET NO.	CONFIRMATION NO.
15/994,559	05/31/2018	Bobby E. Rogers	251102.000027.KURIN2CON2	4704

153290 7590 07/10/2018

TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 3000
Atlanta, GEORGIA 30308-2219
UNITED STATES OF AMERICA

EXAMINER	
HOEKSTRA, JEFFREY GERBEN	
ART UNIT	**PAPER NUMBER**
3736	
NOTIFICATION DATE	**DELIVERY MODE**
07/10/2018	ELECTRONIC

Please find below and/or attached an Office communication concerning this application or proceeding.

The time period for reply, if any, is set in the attached communication.

Notice of the Office communication was sent electronically on above-indicated "Notification Date" to the following e-mail address(es):

chris.franich@troutman.com
patents@troutman.com
ryan.schneider@troutman.com

PTOL-90A (Rev. 04/07)

Decision Granting Request for Prioritized Examination (Track I)	**Application No.** 15/994,559	**Applicant(s)** Rogers et al.	
	Examiner JoAnne Burke	**Art Unit** OPET	**AIA (First Inventor to File) Status** Yes

1. THE REQUEST FILED 31 May 2018 IS **GRANTED** .

The above-identified application has met the requirements for prioritized examination
- A. ☑ for an original nonprovisional application (Track I).
- B. ☐ for an application undergoing continued examination (RCE).

2. **The above-identified application will undergo prioritized examination**. The application will be accorded special status throughout its entire course of prosecution until one of the following occurs:
   - A. filing a **petition for extension of time** to extend the time period for filing a reply;
   - B. filing an **amendment to amend the application to contain more than four independent claims, more than thirty total claims** , or a multiple dependent claim;
   - C. filing a **request for continued examination** ;
   - D. filing a notice of appeal;
   - E. filing a request for suspension of action;
   - F. mailing of a notice of allowance;
   - G. mailing of a final Office action;
   - H. completion of examination as defined in 37 CFR 41.102; or
   - I. abandonment of the application.

Telephone inquiries with regard to this decision should be directed to JoAnne Burke at (571)272-4584. In his/her absence, calls may be directed to Petition Help Desk at (571) 272-3282.

/JOANNE L BURKE/ Paralegal Specialist, OPET	

U.S. Patent and Trademark Office
PTO-2298 (Rev. 02-2012)

To: ryan.schneider@troutman.com,patents@troutman.com,chris.franich@troutman.com
From: PAIR_eOfficeAction@uspto.gov
Cc: PAIR_eOfficeAction@uspto.gov
Subject: Private PAIR Correspondence Notification for Customer Number 153290

Jul 11, 2018 04:11:37 AM

Dear PAIR Customer:

TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 3000
Atlanta, GA 30308-2219
UNITED STATES

The following USPTO patent application(s) associated with your Customer Number, 153290 , have new outgoing correspondence. This correspondence is now available for viewing in Private PAIR.

The official date of notification of the outgoing correspondence will be indicated on the form PTOL-90 accompanying the correspondence.

Disclaimer:
The list of documents shown below is provided as a courtesy and is not part of the official file wrapper. The content of the images shown in PAIR is the official record.

Application	Document	Mailroom Date	Attorney Docket No.
15994559	TRACK1.GRANT	07/10/2018	251102.000027.KURIN2CON2

To view your correspondence online or update your email addresses, please visit us anytime at https://sportal.uspto.gov/secure/myportal/privatepair.

If you have any questions, please email the Electronic Business Center (EBC) at EBC@uspto.gov with 'e-Office Action' on the subject line or call 1-866-217-9197 during the following hours:

Monday - Friday 6:00 a.m. to 12:00 a.m.

Thank you for prompt attention to this notice,

UNITED STATES PATENT AND TRADEMARK OFFICE

PATENT APPLICATION INFORMATION RETRIEVAL SYSTEM

Doc Code: DIST.E.FILE **Document Description: Electronic Terminal Disclaimer - Filed**	PTO/SB/26 U.S. Patent and Trademark Office Department of Commerce

Electronic Petition Request	**TERMINAL DISCLAIMER TO OBVIATE A DOUBLE PATENTING REJECTION OVER A "PRIOR" PATENT**
Application Number	15994559
Filing Date	31-May-2018
First Named Inventor	Bobby Rogers
Attorney Docket Number	251102.000027.KURIN2CON2
Title of Invention	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD

☒ Filing of terminal disclaimer does not obviate requirement for response under 37 CFR 1.111 to outstanding Office Action

☒ This electronic Terminal Disclaimer is not being used for a Joint Research Agreement.

Owner	Percent Interest
Kurin, Inc.	100%

The owner(s) with percent interest listed above in the instant application hereby disclaims, except as provided below, the terminal part of the statutory term of any patent granted on the instant application which would extend beyond the expiration date of the full statutory term of prior patent number(s)

10010282

9820682

as the term of said prior patent is presently shortened by any terminal disclaimer. The owner hereby agrees that any patent so granted on the instant application shall be enforceable only for and during such period that it and the prior patent are commonly owned. This agreement runs with any patent granted on the instant application and is binding upon the grantee, its successors or assigns.

In making the above disclaimer, the owner does not disclaim the terminal part of the term of any patent granted on the instant application that would extend to the expiration date of the full statutory term of the prior patent, "as the term of said prior patent is presently shortened by any terminal disclaimer," in the event that said prior patent later:
- expires for failure to pay a maintenance fee;
- is held unenforceable;
- is found invalid by a court of competent jurisdiction;
- is statutorily disclaimed in whole or terminally disclaimed under 37 CFR 1.321;
- has all claims canceled by a reexamination certificate;
- is reissued; or
- is in any manner terminated prior to the expiration of its full statutory term as presently shortened by any terminal disclaimer.

◉ Terminal disclaimer fee under 37 CFR 1.20(d) is included with Electronic Terminal Disclaimer request. ○ I certify, in accordance with 37 CFR 1.4(d)(4), that the terminal disclaimer fee under 37 CFR 1.20(d) required for this terminal disclaimer has already been paid in the above-identified application.	
Applicant claims the following fee status: ◉ Small Entity ○ Micro Entity ○ Regular Undiscounted I hereby declare that all statements made herein of my own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under Section 1001 of Title 18 of the United States Code and that such willful false statements may jeopardize the validity of the application or any patent issued thereon.	
THIS PORTION MUST BE COMPLETED BY THE SIGNATORY OR SIGNATORIES I certify, in accordance with 37 CFR 1.4(d)(4) that I am: ◉ An attorney or agent registered to practice before the Patent and Trademark Office who is of record in this application Registration Number 50128 ○ A sole inventor ○ A joint inventor; I certify that I am authorized to sign this submission on behalf of all of the inventors as evidenced by the power of attorney in the application ○ A joint inventor; all of whom are signing this request	
Signature	/David Devernoe/
Name	David Devernoe

*Statement under 37 CFR 3.73(b) is required if terminal disclaimer is signed by the assignee (owner).
Form PTO/SB/96 may be used for making this certification. See MPEP § 324.

Electronic Patent Application Fee Transmittal

Application Number:	15994559
Filing Date:	31-May-2018
Title of Invention:	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD
First Named Inventor/Applicant Name:	Bobby E. Rogers
Filer:	David Lynn Devernoe
Attorney Docket Number:	251102.000027.KURIN2CON2

Filed as Small Entity

Filing Fees for Utility under 35 USC 111(a)

Description	Fee Code	Quantity	Amount	Sub-Total in USD($)
Basic Filing:				
STATUTORY OR TERMINAL DISCLAIMER	2814	1	160	160
Pages:				
Claims:				
Miscellaneous-Filing:				
Petition:				
Patent-Appeals-and-Interference:				
Post-Allowance-and-Post-Issuance:				

Description	Fee Code	Quantity	Amount	Sub-Total in USD($)
Extension-of-Time:				
Miscellaneous:				
			Total in USD ($)	**160**

Doc Code: DISQ.E.FILE
Document Description: Electronic Terminal Disclaimer – Approved

Application No.: 15994559

Filing Date: 31-May-2018

Applicant/Patent under Reexamination: Rogers

Electronic Terminal Disclaimer filed on July 25, 2018

☒ APPROVED

This patent is subject to a terminal disclaimer

☐ DISAPPROVED

Approved/Disapproved by: Electronic Terminal Disclaimer automatically approved by EFS-Web

U.S. Patent and Trademark Office

Electronic Acknowledgement Receipt	
EFS ID:	33279751
Application Number:	15994559
International Application Number:	
Confirmation Number:	4704
Title of Invention:	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD
First Named Inventor/Applicant Name:	Bobby E. Rogers
Customer Number:	153290
Filer:	David Lynn Devernoe
Filer Authorized By:	
Attorney Docket Number:	251102.000027.KURIN2CON2
Receipt Date:	25-JUL-2018
Filing Date:	31-MAY-2018
Time Stamp:	14:38:12
Application Type:	Utility under 35 USC 111(a)

Payment information:

Submitted with Payment	yes
Payment Type	DA
Payment was successfully received in RAM	$160
RAM confirmation Number	072618INTEFSW00000802201507
Deposit Account	
Authorized User	
The Director of the USPTO is hereby authorized to charge indicated fees and credit any overpayment as follows:	

File Listing:

Document Number	Document Description	File Name	File Size(Bytes)/ Message Digest	Multi Part /.zip	Pages (if appl.)
1	Terminal Disclaimer-Filed (Electronic)	eTerminal-Disclaimer.pdf	33679 2490bbacc43f1f12d45911adfb8b4fdaacd73157	no	2
Warnings:					
Information:					
2	Fee Worksheet (SB06)	fee-info.pdf	30637 0826aaf87e74a45f22035c56bff3c35c969afadf	no	2
Warnings:					
Information:					
		Total Files Size (in bytes):	64316		

This Acknowledgement Receipt evidences receipt on the noted date by the USPTO of the indicated documents, characterized by the applicant, and including page counts, where applicable. It serves as evidence of receipt similar to a Post Card, as described in MPEP 503.

New Applications Under 35 U.S.C. 111
If a new application is being filed and the application includes the necessary components for a filing date (see 37 CFR 1.53(b)-(d) and MPEP 506), a Filing Receipt (37 CFR 1.54) will be issued in due course and the date shown on this Acknowledgement Receipt will establish the filing date of the application.
National Stage of an International Application under 35 U.S.C. 371
If a timely submission to enter the national stage of an international application is compliant with the conditions of 35 U.S.C. 371 and other applicable requirements a Form PCT/DO/EO/903 indicating acceptance of the application as a national stage submission under 35 U.S.C. 371 will be issued in addition to the Filing Receipt, in due course.
New International Application Filed with the USPTO as a Receiving Office
If a new international application is being filed and the international application includes the necessary components for an international filing date (see PCT Article 11 and MPEP 1810), a Notification of the International Application Number and of the International Filing Date (Form PCT/RO/105) will be issued in due course, subject to prescriptions concerning national security, and the date shown on this Acknowledgement Receipt will establish the international filing date of the application.

UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

NOTICE OF ALLOWANCE AND FEE(S) DUE

153290 7590 08/08/2018

TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 5200
Atlanta, GA 30308

EXAMINER
ABOUELELA, MAY A

ART UNIT	PAPER NUMBER
3736	

DATE MAILED: 08/08/2018

APPLICATION NO.	FILING DATE	FIRST NAMED INVENTOR	ATTORNEY DOCKET NO.	CONFIRMATION NO.
15/994,559	05/31/2018	Bobby E. Rogers	251102.000027.KURIN2CON2	4704

TITLE OF INVENTION: BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD

APPLN. TYPE	ENTITY STATUS	ISSUE FEE DUE	PUBLICATION FEE DUE	PREV. PAID ISSUE FEE	TOTAL FEE(S) DUE	DATE DUE
nonprovisional	SMALL	$500	$0	$0	$500	11/08/2018

THE APPLICATION IDENTIFIED ABOVE HAS BEEN EXAMINED AND IS ALLOWED FOR ISSUANCE AS A PATENT. PROSECUTION ON THE MERITS IS CLOSED. THIS NOTICE OF ALLOWANCE IS NOT A GRANT OF PATENT RIGHTS. THIS APPLICATION IS SUBJECT TO WITHDRAWAL FROM ISSUE AT THE INITIATIVE OF THE OFFICE OR UPON PETITION BY THE APPLICANT. SEE 37 CFR 1.313 AND MPEP 1308.

THE ISSUE FEE AND PUBLICATION FEE (IF REQUIRED) MUST BE PAID WITHIN THREE MONTHS FROM THE MAILING DATE OF THIS NOTICE OR THIS APPLICATION SHALL BE REGARDED AS ABANDONED. THIS STATUTORY PERIOD CANNOT BE EXTENDED. SEE 35 U.S.C. 151. THE ISSUE FEE DUE INDICATED ABOVE DOES NOT REFLECT A CREDIT FOR ANY PREVIOUSLY PAID ISSUE FEE IN THIS APPLICATION. IF AN ISSUE FEE HAS PREVIOUSLY BEEN PAID IN THIS APPLICATION (AS SHOWN ABOVE), THE RETURN OF PART B OF THIS FORM WILL BE CONSIDERED A REQUEST TO REAPPLY THE PREVIOUSLY PAID ISSUE FEE TOWARD THE ISSUE FEE NOW DUE.

HOW TO REPLY TO THIS NOTICE:

I. Review the ENTITY STATUS shown above. If the ENTITY STATUS is shown as SMALL or MICRO, verify whether entitlement to that entity status still applies.

If the ENTITY STATUS is the same as shown above, pay the TOTAL FEE(S) DUE shown above.

If the ENTITY STATUS is changed from that shown above, on PART B - FEE(S) TRANSMITTAL, complete section number 5 titled "Change in Entity Status (from status indicated above)".

For purposes of this notice, small entity fees are 1/2 the amount of undiscounted fees, and micro entity fees are 1/2 the amount of small entity fees.

II. PART B - FEE(S) TRANSMITTAL, or its equivalent, must be completed and returned to the United States Patent and Trademark Office (USPTO) with your ISSUE FEE and PUBLICATION FEE (if required). If you are charging the fee(s) to your deposit account, section "4b" of Part B - Fee(s) Transmittal should be completed and an extra copy of the form should be submitted. If an equivalent of Part B is filed, a request to reapply a previously paid issue fee must be clearly made, and delays in processing may occur due to the difficulty in recognizing the paper as an equivalent of Part B.

III. All communications regarding this application must give the application number. Please direct all communications prior to issuance to Mail Stop ISSUE FEE unless advised to the contrary.

IMPORTANT REMINDER: Maintenance fees are due in utility patents issuing on applications filed on or after Dec. 12, 1980. It is patentee's responsibility to ensure timely payment of maintenance fees when due. More information is available at www.uspto.gov/PatentMaintenanceFees.

PART B - FEE(S) TRANSMITTAL

Complete and send this form, together with applicable fee(s), to: Mail **Mail Stop ISSUE FEE**
Commissioner for Patents
P.O. Box 1450
Alexandria, Virginia 22313-1450
or Fax (571)-273-2885

INSTRUCTIONS: This form should be used for transmitting the ISSUE FEE and PUBLICATION FEE (if required). Blocks 1 through 5 should be completed where appropriate. All further correspondence including the Patent, advance orders and notification of maintenance fees will be mailed to the current correspondence address as indicated unless corrected below or directed otherwise in Block 1, by (a) specifying a new correspondence address; and/or (b) indicating a separate "FEE ADDRESS" for maintenance fee notifications.

CURRENT CORRESPONDENCE ADDRESS (Note: Use Block 1 for any change of address)

153290 7590 08/08/2018
TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 5200
Atlanta, GA 30308

Note: A certificate of mailing can only be used for domestic mailings of the Fee(s) Transmittal. This certificate cannot be used for any other accompanying papers. Each additional paper, such as an assignment or formal drawing, must have its own certificate of mailing or transmission.

Certificate of Mailing or Transmission
I hereby certify that this Fee(s) Transmittal is being deposited with the United States Postal Service with sufficient postage for first class mail in an envelope addressed to the Mail Stop ISSUE FEE address above, or being facsimile transmitted to the USPTO (571) 273-2885, on the date indicated below.

(Depositor's name)
(Signature)
(Date)

APPLICATION NO.	FILING DATE	FIRST NAMED INVENTOR	ATTORNEY DOCKET NO.	CONFIRMATION NO.
15/994,559	05/31/2018	Bobby E. Rogers	251102.000027.KURIN2CON2	4704

TITLE OF INVENTION: BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD

APPLN. TYPE	ENTITY STATUS	ISSUE FEE DUE	PUBLICATION FEE DUE	PREV. PAID ISSUE FEE	TOTAL FEE(S) DUE	DATE DUE
nonprovisional	SMALL	$500	$0	$0	$500	11/08/2018

EXAMINER	ART UNIT	CLASS-SUBCLASS
ABOUELELA, MAY A	3736	600-573000

1. Change of correspondence address or indication of "Fee Address" (37 CFR 1.363).
- ❑ Change of correspondence address (or Change of Correspondence Address form PTO/SB/122) attached.
- ❑ "Fee Address" indication (or "Fee Address" Indication form PTO/SB/47; Rev 03-02 or more recent) attached. **Use of a Customer Number is required.**

2. For printing on the patent front page, list
(1) The names of up to 3 registered patent attorneys or agents OR, alternatively,
(2) The name of a single firm (having as a member a registered attorney or agent) and the names of up to 2 registered patent attorneys or agents. If no name is listed, no name will be printed.
1 _____
2 _____
3 _____

3. ASSIGNEE NAME AND RESIDENCE DATA TO BE PRINTED ON THE PATENT (print or type)

PLEASE NOTE: Unless an assignee is identified below, no assignee data will appear on the patent. If an assignee is identified below, the document has been filed for recordation as set forth in 37 CFR 3.11. Completion of this form is NOT a substitute for filing an assignment.

(A) NAME OF ASSIGNEE (B) RESIDENCE: (CITY and STATE OR COUNTRY)

Please check the appropriate assignee category or categories (will not be printed on the patent) : ❑ Individual ❑ Corporation or other private group entity ❑ Government

4a. The following fee(s) are submitted:
- ❑ Issue Fee
- ❑ Publication Fee (No small entity discount permitted)
- ❑ Advance Order - # of Copies _____

4b. Payment of Fee(s): **(Please first reapply any previously paid issue fee shown above)**
- ❑ A check is enclosed.
- ❑ Payment by credit card. Form PTO-2038 is attached.
- ❑ The director is hereby authorized to charge the required fee(s), any deficiency, or credits any overpayment, to Deposit Account Number _____ (enclose an extra copy of this form).

5. **Change in Entity Status** (from status indicated above)
- ❑ Applicant certifying micro entity status. See 37 CFR 1.29 — NOTE: Absent a valid certification of Micro Entity Status (see forms PTO/SB/15A and 15B), issue fee payment in the micro entity amount will not be accepted at the risk of application abandonment.
- ❑ Applicant asserting small entity status. See 37 CFR 1.27 — NOTE: If the application was previously under micro entity status, checking this box will be taken to be a notification of loss of entitlement to micro entity status.
- ❑ Applicant changing to regular undiscounted fee status. — NOTE: Checking this box will be taken to be a notification of loss of entitlement to small or micro entity status, as applicable.

NOTE: This form must be signed in accordance with 37 CFR 1.31 and 1.33. See 37 CFR 1.4 for signature requirements and certifications.

Authorized Signature _____ Date _____

Typed or printed name _____ Registration No. _____

PTOL-85 Part B (10-13) Approved for use through 10/31/2013. OMB 0651-0033 U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE

UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

APPLICATION NO.	FILING DATE	FIRST NAMED INVENTOR	ATTORNEY DOCKET NO.	CONFIRMATION NO.
15/994,559	05/31/2018	Bobby E. Rogers	251102.000027.KURIN2CON2	4704

153290 7590 08/08/2018

TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 5200
Atlanta, GA 30308

EXAMINER	
ABOUELELA, MAY A	
ART UNIT	PAPER NUMBER
3736	

DATE MAILED: 08/08/2018

Determination of Patent Term Adjustment under 35 U.S.C. 154 (b)
(Applications filed on or after May 29, 2000)

The Office has discontinued providing a Patent Term Adjustment (PTA) calculation with the Notice of Allowance.

Section 1(h)(2) of the AIA Technical Corrections Act amended 35 U.S.C. 154(b)(3)(B)(i) to eliminate the requirement that the Office provide a patent term adjustment determination with the notice of allowance. See Revisions to Patent Term Adjustment, 78 Fed. Reg. 19416, 19417 (Apr. 1, 2013). Therefore, the Office is no longer providing an initial patent term adjustment determination with the notice of allowance. The Office will continue to provide a patent term adjustment determination with the Issue Notification Letter that is mailed to applicant approximately three weeks prior to the issue date of the patent, and will include the patent term adjustment on the patent. Any request for reconsideration of the patent term adjustment determination (or reinstatement of patent term adjustment) should follow the process outlined in 37 CFR 1.705.

Any questions regarding the Patent Term Extension or Adjustment determination should be directed to the Office of Patent Legal Administration at (571)-272-7702. Questions relating to issue and publication fee payments should be directed to the Customer Service Center of the Office of Patent Publication at 1-(888)-786-0101 or (571)-272-4200.

OMB Clearance and PRA Burden Statement for PTOL-85 Part B

The Paperwork Reduction Act (PRA) of 1995 requires Federal agencies to obtain Office of Management and Budget approval before requesting most types of information from the public. When OMB approves an agency request to collect information from the public, OMB (i) provides a valid OMB Control Number and expiration date for the agency to display on the instrument that will be used to collect the information and (ii) requires the agency to inform the public about the OMB Control Number's legal significance in accordance with 5 CFR 1320.5(b).

The information collected by PTOL-85 Part B is required by 37 CFR 1.311. The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.14. This collection is estimated to take 12 minutes to complete, including gathering, preparing, and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, Virginia 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. SEND TO: Commissioner for Patents, P.O. Box 1450, Alexandria, Virginia 22313-1450. Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

Privacy Act Statement

The Privacy Act of 1974 (P.L. 93-579) requires that you be given certain information in connection with your submission of the attached form related to a patent application or patent. Accordingly, pursuant to the requirements of the Act, please be advised that: (1) the general authority for the collection of this information is 35 U.S.C. 2(b)(2); (2) furnishing of the information solicited is voluntary; and (3) the principal purpose for which the information is used by the U.S. Patent and Trademark Office is to process and/or examine your submission related to a patent application or patent. If you do not furnish the requested information, the U.S. Patent and Trademark Office may not be able to process and/or examine your submission, which may result in termination of proceedings or abandonment of the application or expiration of the patent.

The information provided by you in this form will be subject to the following routine uses:

1. The information on this form will be treated confidentially to the extent allowed under the Freedom of Information Act (5 U.S.C. 552) and the Privacy Act (5 U.S.C 552a). Records from this system of records may be disclosed to the Department of Justice to determine whether disclosure of these records is required by the Freedom of Information Act.
2. A record from this system of records may be disclosed, as a routine use, in the course of presenting evidence to a court, magistrate, or administrative tribunal, including disclosures to opposing counsel in the course of settlement negotiations.
3. A record in this system of records may be disclosed, as a routine use, to a Member of Congress submitting a request involving an individual, to whom the record pertains, when the individual has requested assistance from the Member with respect to the subject matter of the record.
4. A record in this system of records may be disclosed, as a routine use, to a contractor of the Agency having need for the information in order to perform a contract. Recipients of information shall be required to comply with the requirements of the Privacy Act of 1974, as amended, pursuant to 5 U.S.C. 552a(m).
5. A record related to an International Application filed under the Patent Cooperation Treaty in this system of records may be disclosed, as a routine use, to the International Bureau of the World Intellectual Property Organization, pursuant to the Patent Cooperation Treaty.
6. A record in this system of records may be disclosed, as a routine use, to another federal agency for purposes of National Security review (35 U.S.C. 181) and for review pursuant to the Atomic Energy Act (42 U.S.C. 218(c)).
7. A record from this system of records may be disclosed, as a routine use, to the Administrator, General Services, or his/her designee, during an inspection of records conducted by GSA as part of that agency's responsibility to recommend improvements in records management practices and programs, under authority of 44 U.S.C. 2904 and 2906. Such disclosure shall be made in accordance with the GSA regulations governing inspection of records for this purpose, and any other relevant (i.e., GSA or Commerce) directive. Such disclosure shall not be used to make determinations about individuals.
8. A record from this system of records may be disclosed, as a routine use, to the public after either publication of the application pursuant to 35 U.S.C. 122(b) or issuance of a patent pursuant to 35 U.S.C. 151. Further, a record may be disclosed, subject to the limitations of 37 CFR 1.14, as a routine use, to the public if the record was filed in an application which became abandoned or in which the proceedings were terminated and which application is referenced by either a published application, an application open to public inspection or an issued patent.
9. A record from this system of records may be disclosed, as a routine use, to a Federal, State, or local law enforcement agency, if the USPTO becomes aware of a violation or potential violation of law or regulation.

Notice of Allowability	Application No. 15/994,559	Applicant(s) ROGERS ET AL.	
	Examiner MAY ABOUELELA	Art Unit 3736	AIA (First Inventor to File) Status Yes

-- The MAILING DATE of this communication appears on the cover sheet with the correspondence address--

All claims being allowable, PROSECUTION ON THE MERITS IS (OR REMAINS) CLOSED in this application. If not included herewith (or previously mailed), a Notice of Allowance (PTOL-85) or other appropriate communication will be mailed in due course. **THIS NOTICE OF ALLOWABILITY IS NOT A GRANT OF PATENT RIGHTS.** This application is subject to withdrawal from issue at the initiative of the Office or upon petition by the applicant. See 37 CFR 1.313 and MPEP 1308.

1. ☒ This communication is responsive to *07/02/2018*.
   ☐ A declaration(s)/affidavit(s) under **37 CFR 1.130(b)** was/were filed on_____.
2. ☐ An election was made by the applicant in response to a restriction requirement set forth during the interview on _____; the restriction requirement and election have been incorporated into this action.
3. ☒ The allowed claim(s) is/are *1,2,4-6,8-20 and 22-26*. As a result of the allowed claim(s), you may be eligible to benefit from the **Patent Prosecution Highway** program at a participating intellectual property office for the corresponding application. For more information, please see http://www.uspto.gov/patents/init_events/pph/index.jsp or send an inquiry to PPHfeedback@uspto.gov.
4. ☐ Acknowledgment is made of a claim for foreign priority under 35 U.S.C. § 119(a)-(d) or (f).
   Certified copies:
   a) ☐ All b) ☐ Some *c) ☐ None of the:
      1. ☐ Certified copies of the priority documents have been received.
      2. ☐ Certified copies of the priority documents have been received in Application No. _____ .
      3. ☐ Copies of the certified copies of the priority documents have been received in this national stage application from the International Bureau (PCT Rule 17.2(a)).

   * Certified copies not received: _____.

Applicant has THREE MONTHS FROM THE "MAILING DATE" of this communication to file a reply complying with the requirements noted below. Failure to timely comply will result in ABANDONMENT of this application.
THIS THREE-MONTH PERIOD IS NOT EXTENDABLE.

5. ☐ CORRECTED DRAWINGS (as "replacement sheets") must be submitted.
   ☐ including changes required by the attached Examiner's Amendment / Comment or in the Office action of Paper No./Mail Date _____.

   Identifying indicia such as the application number (see 37 CFR 1.84(c)) should be written on the drawings in the front (not the back) of each sheet. Replacement sheet(s) should be labeled as such in the header according to 37 CFR 1.121(d).
6. ☐ DEPOSIT OF and/or INFORMATION about the deposit of BIOLOGICAL MATERIAL must be submitted. Note the attached Examiner's comment regarding REQUIREMENT FOR THE DEPOSIT OF BIOLOGICAL MATERIAL.

Attachment(s)

1. ☐ Notice of References Cited (PTO-892)
2. ☒ Information Disclosure Statements (PTO/SB/08), Paper No./Mail Date _____
3. ☐ Examiner's Comment Regarding Requirement for Deposit of Biological Material
4. ☒ Interview Summary (PTO-413), Paper No./Mail Date *07/25/2018* .
5. ☒ Examiner's Amendment/Comment
6. ☒ Examiner's Statement of Reasons for Allowance
7. ☐ Other _____.

/MAY ABOUELELA/
Primary Examiner, Art Unit 3736

DETAILED ACTION

1. The present application, filed on or after March 16, 2013, is being examined under the first inventor to file provisions of the AIA.

Information Disclosure Statement

2. The information disclosure statement (IDS) submitted on 05/31/2018. The submission is in compliance with the provisions of 37 CFR 1.97. Accordingly, the information disclosure statement is being considered by the examiner.

Terminal Disclaimer

3. The terminal disclaimer filed on 07/25/2018 disclaiming the terminal portion of any patent granted on this application which would extend beyond the expiration date of U.S Patent Applications No. 10,010,282 and 9,820,682 has been reviewed and is accepted. The terminal disclaimer has been recorded.

EXAMINER'S AMENDMENT

4. An examiner's amendment to the record appears below. Should the changes and/or additions be unacceptable to applicant, an amendment may be filed as provided by 37 CFR 1.312. To ensure consideration of such an amendment, it MUST be submitted no later than the payment of the issue fee.

Authorization for this examiner's amendment was given in an interview with JAMES P. CLEARY on 07/25/2018.

The claims should be amended as follows:

Claim 1 should be amended as follow:

1. A blood sequestration device comprising;

an inlet port;

an outlet port;

a sequestration chamber having a vent that includes an air permeable blood barrier; ~~and~~

a sampling channel having a distal end connected with the outlet port; **and**

a housing that houses and defines the inlet port, the outlet port, the sequestration chamber, and the sampling channel;

each of the sequestration chamber and the sampling channel being connected with the inlet port via a junction that is sized and configured **to allow** ~~such that~~ a first portion of blood flows into the sequestration chamber to displace air therein through the air permeable blood barrier and to be sequestered in the sequestration chamber, and **to allow** a second portion of blood ~~is allowed~~ to bypass the sequestration chamber and the first portion of blood sequestered therein to be directed into the sampling channel toward the outlet port.

Claim 3 should be amended as follow:

3. (Cancelled)

Claim 4 should be amended as follow:

4. The blood sequestration device in accordance with claim **1** ~~3~~, wherein the sequestration chamber includes a sequestration channel defined in the housing.

Claim 6 should be amended as follow:

6. A blood sequestration device connected with a blood sampling pathway having a patient needle and a sample collection device, the blood sequestration device comprising:

an inlet port connected with the patient needle;

an outlet port connected with the sample collection device;

a sequestration chamber having a vent that includes an air permeable blood barrier; ~~and~~

~~and~~ a sampling channel having a distal end connected with the outlet port; **and**

a housing that houses and defines the inlet port, the outlet port, the sequestration chamber, and the sampling channel;

each of the sequestration chamber and the sampling channel being connected with the inlet port via a junction that is sized and configured **to allow** ~~such that~~ a first portion of blood flows into the sequestration chamber to displace air therein through the air permeable blood barrier and to be sequestered in the sequestration chamber, and **to allow** a second portion of blood ~~is allowed~~ to bypass the sequestration chamber and the first portion of blood sequestered therein to be directed into the sampling channel toward the outlet port and the sample collection device.

Claim 7 should be amended as follow:

7. (Cancelled)

Claim 11 should be amended as follow:

11. The blood sequestration device in accordance with claim **6** ~~7~~, wherein the sequestration chamber includes a sequestration channel defined in the housing.

Claim 13 should be amended as follow:

13. A bodily fluid sequestration device comprising;

an inlet port;

an outlet port connected with the inlet port;

a sequestration chamber connected with the inlet port via a junction, the sequestration chamber having a vent that includes an air permeable bodily fluid barrier; and

a housing that houses and defines the inlet port, the outlet port, and the sequestration chamber, the sequestration chamber and the junction configured to direct a first portion of bodily fluid from the inlet port into the sequestration chamber toward the air permeable bodily fluid barrier, the air permeable bodily fluid barrier including an air permeable material that forms a barrier to bodily fluids upon contact with the bodily fluids, whereupon formation of the barrier ~~enables~~ **configured to allow** sequestration of the first portion of bodily fluid in the sequestration chamber, and **to allow** ~~enables~~ a second portion of bodily fluid from the inlet port to bypass the sequestration chamber via the junction and the first portion of bodily fluid, toward the outlet port.

Claim 20 should be amended as follow:

20. A blood sequestration system comprising:

a blood sampling pathway having a patient needle and a sample collection device; and

a blood sequestration device, the blood sequestration device comprising:

an inlet port connected with the patient needle;

an outlet port connected with the sample collection device;

a sequestration chamber having a vent that includes an air permeable blood barrier; ~~and~~

~~and~~ a sampling channel having a distal end connected with the outlet port; **and**

a housing that houses and defines the inlet port, the outlet port, the sequestration chamber, and the sampling channel;

each of the sequestration chamber and the sampling channel being connected with the inlet port via a junction that is sized and configured ~~such that~~ **to allow** a first portion of blood flows into the sequestration chamber to displace air therein through the air permeable blood barrier and to be sequestered in the sequestration chamber, and **to allow** a second portion of blood ~~is allowed~~ to bypass the sequestration chamber and the first portion of blood sequestered therein to be directed into the sampling channel toward the outlet port and the sample collection device.

Claim 21 should be amended as follow:

21. (Cancelled)

Allowable Subject Matter

5. Claims 1, 2, 3-6, 8-20 and 22-26 are allowed.

6. The following is an examiner's statement of reasons for allowance: the prior art fairly suggest a blood/fluid sampling devices with vacuum chamber that collects/withdraws first portion of blood/fluid sample therein, where the vacuum chamber includes an outlet port that directs a second portion of blood/fluid to a sampling chamber.

However the prior art does not disclose, teach, and/or fairly suggest a blood sequestration/sampling device comprising; a sequestration chamber and a sampling channel defined in a housing, each of the sequestration chamber and the sampling channel being connected with an inlet port via a junction, where the junction is configured to allow a first

portion of blood flows into the sequestration chamber, and to allow a second portion of blood to bypass the sequestration chamber and the first portion of blood sequestered therein and is directed into the sampling channel toward an outlet port.

Any comments considered necessary by applicant must be submitted no later than the payment of the issue fee and, to avoid processing delays, should preferably accompany the issue fee. Such submissions should be clearly labeled "Comments on Statement of Reasons for Allowance."

Conclusion

Any inquiry concerning this communication or earlier communications from the examiner should be directed to MAY ABOUELELA whose telephone number is (571)270-7917. The examiner can normally be reached on Monday through Friday 8:30 to 5:00.

Examiner interviews are available via telephone, in-person, and video conferencing using a USPTO supplied web-based collaboration tool. To schedule an interview, applicant is encouraged to use the USPTO Automated Interview Request (AIR) at http://www.uspto.gov/interviewpractice.

If attempts to reach the examiner by telephone are unsuccessful, the examiner's supervisor, JEFFREY G. HOEKSTRA can be reached on (571)272-7232. The fax phone number for the organization where this application or proceeding is assigned is 571-273-8300.

Information regarding the status of an application may be obtained from the Patent Application Information Retrieval (PAIR) system. Status information for published applications may be obtained from either Private PAIR or Public PAIR. Status information for unpublished applications is available through Private PAIR only. For more information about the PAIR system, see http://pair-direct.uspto.gov. Should you have questions on access to the Private PAIR system, contact the Electronic Business Center (EBC) at 866-217-9197 (toll-free). If you would like assistance from a USPTO Customer Service Representative or access to the automated information system, call 800-786-9199 (IN USA OR CANADA) or 571-272-1000.

/MAY ABOUELELA/
Primary Examiner, Art Unit 3736

Examiner-Initiated Interview Summary	Application No.	Applicant(s)	
	15/994,559	ROGERS ET AL.	
	Examiner	Art Unit	
	MAY ABOUELELA	3736	

All participants (applicant, applicant's representative, PTO personnel):

(1) *MAY ABOUELELA*. (3)_____.

(2) *JAMES P. CLEARY* . (4)_____.

Date of Interview: *25 July 2018*.

Type: ☒ Telephonic ☐ Video Conference
☐ Personal [copy given to: ☐ applicant ☐ applicant's representative]

Exhibit shown or demonstration conducted: ☐ Yes ☒ No.
If Yes, brief description: _____.

Issues Discussed ☐101 ☒112 ☐102 ☐103 ☐Others
(For each of the checked box(es) above, please describe below the issue and detailed description of the discussion)

Claim(s) discussed: *1,3,6,7,13,20 and 21*.

Identification of prior art discussed: *N/A*.

Substance of Interview
(For each issue discussed, provide a detailed description and indicate if agreement was reached. Some topics may include: identification or clarification of a reference or a portion thereof, claim interpretation, proposed amendments, arguments of any applied references etc...)

Applicant and Examiner discussed the claims set mailed on 07/02/2018. Applicant and Examiner discussed the claim language with respect to the applied prior art and the disclosure. Applicant and Examiner discussed proposed claim amendments represented by the Examiner to overcome 112(b) rejections. The Applicant has authorized the Examiner to amend the claims.

Applicant recordation instructions: It is not necessary for applicant to provide a separate record of the substance of interview.

Examiner recordation instructions: Examiners must summarize the substance of any interview of record. A complete and proper recordation of the substance of an interview should include the items listed in MPEP 713.04 for complete and proper recordation including the identification of the general thrust of each argument or issue discussed, a general indication of any other pertinent matters discussed regarding patentability and the general results or outcome of the interview, to include an indication as to whether or not agreement was reached on the issues raised.

☐ Attachment

/MAY ABOUELELA/ Primary Examiner, Art Unit 3736	

Index of Claims	Application/Control No.	Applicant(s)/Patent Under Reexamination
	15994559	ROGERS ET AL.
	Examiner	**Art Unit**
	MAY ABOUELELA	3736

✓	Rejected	-	Cancelled	N	Non-Elected	A	Appeal
=	Allowed	÷	Restricted	I	Interference	O	Objected

☐ Claims renumbered in the same order as presented by applicant ☐ CPA ☒ T.D. ☐ R.1.47

CLAIM		DATE								
Final	Original	07/25/2018								
1	1	=								
2	2	=								
	3	-								
3	4	=								
4	5	=								
5	6	=								
	7	-								
6	8	=								
7	9	=								
8	10	=								
9	11	=								
10	12	=								
11	13	=								
12	14	=								
13	15	=								
14	16	=								
15	17	=								
16	18	=								
17	19	=								
18	20	=								
	21	-								
19	22	=								
20	23	=								
21	24	=								
22	25	=								
23	26	=								

Bibliographic Data

Application No: 15/994,559

Foreign Priority claimed: ○ Yes ◉ No

35 USC 119 (a-d) conditions met: ☐ Yes ☑ No ☐ Met After Allowance

Verified and Acknowledged: /MAY A ABOUELELA/ (Examiner's Signature) | M.A.A (Initials)

Title: BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD

FILING or 371(c) DATE	CLASS	GROUP ART UNIT	ATTORNEY DOCKET NO.
05/31/2018	600	3736	251102.000027.KURIN2CON2
RULE			

APPLICANTS

KURIN, INC., San Diego, CA, UNITED STATES

INVENTORS

Bobby E. Rogers San Diego, CA, UNITED STATES

Gino Kang Irvine, CA, UNITED STATES

John Detloff San Diego, CA, UNITED STATES

CONTINUING DATA

This application is a CON of 15140448 04/27/2016 PAT 10010282

15140448 has PRO of 62318194 04/04/2016

15140448 has PRO of 62238636 10/07/2015

15140448 has PRO of 62196797 07/24/2015

FOREIGN APPLICATIONS

IF REQUIRED, FOREIGN LICENSE GRANTED**

06/21/2018

**** SMALL ENTITY ****

STATE OR COUNTRY

UNITED STATES

ADDRESS

TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 5200
Atlanta, GA 30308
UNITED STATES

FILING FEE RECEIVED

$3,155

EAST Search History

EAST Search History (Prior Art)

Ref #	Hits	Search Query	DBs	Default Operator	Plurals	Time Stamp
S1	0	("15140443").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2016/12/20 23:05
S2	1	("20020099309").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2016/12/21 11:38
S3	1	("14055232").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2016/12/21 11:39
S4	1763	(600/573).CCLS.	US-PGPUB; USPAT; USOCR	OR	OFF	2016/12/21 17:18
S5	63	(("ROGERS") near3 ("Bobby")).INV.	US-PGPUB; USPAT; USOCR	OR	OFF	2016/12/21 17:19
S6	28	("2004/0073171").URPN.	USPAT	OR	OFF	2016/12/21 17:36
S7	0	("1and(bloodnear4sequest$5)").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2016/12/21 17:41
S8	5225	1and (blood near4 sequest$5)	US-PGPUB; USPAT	OR	OFF	2016/12/21 17:42
S9	7	S4 and (blood near4 sequest$5)	US-PGPUB; USPAT	OR	OFF	2016/12/21 17:42
S10	73	("20020002349" | "20020183651" | "20030055381" | "20040010228" | "20040054333" | "20040147855" | "20050004524" | "20050240161" | "20050245885" | "20050281713" | "20060287639" | "2707953" | "3013557" | "3098016" | "3382865" | "3405706" | "3494351" | "3577980" | "3648684" | "3848579" | "3937211" | "4057050" | "4133863" | "4166450" | "4340067" | "4370987" | "4444203" | "4459997" | "4509534" | "4676256" | "4865583" | "4890627" | "4988339" | "5009847" | "5097842" | "5108927" | "5122129" | "5269317" | "5360011" | "5429610" | "5450856" | "5507299" | "5577513" | "5762633" | "5882318" | "5922551" | "6016712" | "6057105" | "6159164" | "6210909" | "6364890" | "6387086" | "6403381" | "6692479" | "6746420" | "6913580" | "7044941" | "7087047").PN. OR ("8197420").URPN.	US-PGPUB; USPAT; USOCR	OR	OFF	2016/12/21 17:43
S11	2	S10 and (blood near4 sequest$5)	US-PGPUB; USPAT	OR	OFF	2016/12/21 17:44
S12	77	("0453322" | "0577682" | "0729011" |	US-PGPUB;	OR	OFF	2016/12/21

		"1074965" | "1110189" | "1450016" | "1521890" | "2218899" | "2688325" | "2895773" | "3176595" | "3214069" | "3236268" | "3263874" | "3486503" | "3577980" | "3754644" | "3794221" | "3834387" | "3855997" | "3937211" | "3958570").PN. OR ("4057050").URPN.	USPAT; USOCR			17:47
S13	852	S4 and (blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT	OR	OFF	2016/12/21 17:47
S14	46	S10 and (blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT	OR	OFF	2016/12/21 17:47
S15	1	("8197420").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2016/12/21 18:29
S16	1	("20130317391").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2016/12/21 18:42
S17	1254	(600/583).CCLS.	US-PGPUB; USPAT; USOCR	OR	OFF	2016/12/21 18:43
S18	1070	S17 and (blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT	OR	OFF	2016/12/21 18:43
S19	265030	(blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT; USOCR; FPRS; EPO; JPO; DERWENT; IBM_TDB	OR	OFF	2016/12/21 19:09
S20	5653	S19 AND ((A61B10/0096 OR A61B5/150022).CPC.)	US-PGPUB; USPAT; USOCR; FPRS; EPO; JPO; DERWENT; IBM_TDB	OR	OFF	2016/12/21 19:10
S21	207	S20 and (seal near4 air)	US-PGPUB; USPAT; USOCR; FPRS; EPO; JPO; DERWENT; IBM_TDB	OR	OFF	2016/12/21 19:10
S22	23	"2004087258"	US-PGPUB; USPAT; USOCR; FPRS; EPO; JPO; DERWENT; IBM_TDB	OR	OFF	2016/12/21 20:59
S23	1	("20050004524").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/11 20:23
S24	1	("20030105414").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/11 20:24
S25	1	("5749857").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/11 20:26

S26	13	("20040073171" | "20040147855" | "20050240161" | "20130317391" | "20160174888" | "4057050" | "8197420" | "8523826" | "8535241" | "8540663" | "8568371" | "8864684" | "9138572").PN.	US-PGPUB; USPAT	OR	OFF	2017/04/11 20:39
S27	1	("15140443").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/11 21:43
S28	0	("4and(bloodnear4air)").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/11 22:01
S29	3	S26 and (blood near4 air)	US-PGPUB; USPAT	OR	OFF	2017/04/11 22:01
S30	6	S26 and vent$4	US-PGPUB; USPAT	OR	OFF	2017/04/11 22:02
S31	5	("2013/0317391").URPN.	USPAT	OR	OFF	2017/04/11 22:06
S32	48	("2005/0004524").URPN.	USPAT	OR	OFF	2017/04/11 22:17
S33	1	("20120170037").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/12 16:11
S34	1	("6139540").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 12:52
S35	1	("20040116878").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 12:54
S36	1	("20100152752").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 13:16
S37	1	("6395003").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 13:20
S38	5	("2013/0317391").URPN.	USPAT	OR	OFF	2017/04/13 13:43
S39	1	("4444203").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 13:44
S40	1	("20020004647").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 13:48
S41	1	("3817240").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 13:57
S42	1	("3874367").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 13:57
S43	1	("3886930").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 13:58
S44	1	("4106497").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 13:59
S45	1	("4154229").PN.	US-PGPUB; USPAT;	OR	OFF	2017/04/13 13:59

			USOCR			
S46	1	("4207870").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 14:00
S47	292	("2913000" | "3817240" | "3859998" | "3864979" | "4016879" | "4046144").PN. OR ("4207870").URPN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 14:01
S48	1	("4412548").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 14:04
S49	1	("5222502").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 14:11
S50	1	("5520193").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 14:15
S51	1	("20100057004").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 14:16
S52	1	("20070088279").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 14:29
S53	1733	(600/573).CCLS.	US-PGPUB; USPAT	OR	OFF	2017/04/13 15:29
S54	13	S53 and ((vent$4 near4 air) and flash$6)	US-PGPUB; USPAT	OR	OFF	2017/04/13 15:52
S55	1255	(600/583).CCLS.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/13 16:23
S56	4	S55 and ((vent$4 near4 air) and flash$6)	US-PGPUB; USPAT	OR	OFF	2017/04/13 16:23
S57	272301	(blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT; USOCR; FPRS; EPO; JPO; DERWENT; IBM_TDB	OR	OFF	2017/04/13 16:29
S58	5898	S57 AND ((A61B10/0096 OR A61B5/150022).CPC.)	US-PGPUB; USPAT; USOCR; FPRS; EPO; JPO; DERWENT; IBM_TDB	OR	OFF	2017/04/13 16:29
S59	114	S58 and ((vent$4 near4 air) and flash$6)	US-PGPUB; USPAT	OR	OFF	2017/04/13 16:29
S60	2	("2007/0088279").URPN.	USPAT	OR	OFF	2017/04/13 17:58
S61	1	("6358217").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/04/21 14:02
S62	6	("2002/0004647").URPN.	USPAT	OR	OFF	2017/09/27 12:48
S63	2	("14493796").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/09/27 13:21

S64	2	("14494208").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/09/27 13:23
S65	1	("15140443").PN.	US-PGPUB; USPAT	OR	OFF	2017/09/27 13:28
S66	1	("20080145933").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/09/27 13:51
S67	9	("2008/0145933").URPN.	USPAT	OR	OFF	2017/09/27 13:55
S68	1	("20040054333").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/09/27 13:59
S69	1	("20120109034").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/09/27 14:37
S70	1	("20100228206").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/09/27 14:39
S71	3	("2010/0228206").URPN.	USPAT	OR	OFF	2017/09/27 14:47
S72	66	(("ROGERS") near3 ("Bobby")).INV.	US-PGPUB; USPAT	OR	OFF	2017/09/28 13:41
S73	4	S72 and (blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT	OR	OFF	2017/09/28 13:42
S74	1733	(600/573).CCLS.	US-PGPUB; USPAT	OR	OFF	2017/09/28 13:58
S75	845	S74 and (blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT	OR	OFF	2017/09/28 13:58
S76	9	S75 and ((vent$4 near4 air) and flash$6)	US-PGPUB; USPAT	OR	OFF	2017/09/28 13:59
S77	86	("2007/0083162").URPN.	USPAT	OR	OFF	2017/09/28 13:59
S78	1	("15140443").PN.	US-PGPUB; USPAT	OR	OFF	2017/09/28 13:59
S79	9	("2008/0145933").URPN.	USPAT	OR	OFF	2017/09/28 14:04
S80	1258	(600/583).CCLS.	US-PGPUB; USPAT	OR	OFF	2017/09/28 14:20
S81	1071	S80 and (blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT	OR	OFF	2017/09/28 14:20
S82	78	S81 and (vent$4 near4 air)	US-PGPUB; USPAT	OR	OFF	2017/09/28 14:21
S83	282596	(blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT; USOCR; FPRS; EPO; JPO; DERWENT; IBM_TDB	OR	OFF	2017/09/28 16:01
S84	6183	S83 AND ((A61B10/0096 OR A61B5/150022).CPC.)	US-PGPUB; USPAT; USOCR; FPRS; EPO; JPO; DERWENT;	OR	OFF	2017/09/28 16:01

			IBM_TDB			
S85	387	S84 and (vent$4 near4 air)	US-PGPUB; USPAT	OR	OFF	2017/09/28 16:01
S86	362	S85 and @ad<"20150724"	US-PGPUB; USPAT	OR	OFF	2017/09/28 16:02
S87	12	("2005/0010189").URPN.	USPAT	OR	OFF	2017/09/28 16:03
S88	1363	(604/164.01).CCLS.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/09/28 16:04
S89	74	S88 and (blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT	OR	OFF	2017/09/28 16:05
S90	21	("3965910" | "3996923" | "4131127" | "4301811" | "4450854" | "4506691" | "4819684" | "5147333" | "5393035" | "5636975").PN. OR ("6569117").URPN.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/09/28 16:09
S91	499	(435/294.1).CCLS.	US-PGPUB; USPAT; USOCR	OR	OFF	2017/09/28 16:12
S92	18	S91 and (blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT	OR	OFF	2017/09/28 16:12
S93	9	("2008/0145933").URPN.	USPAT	OR	OFF	2017/09/28 16:13
S95	67	(("ROGERS") near3 ("Bobby")).INV.	US-PGPUB; USPAT	OR	OFF	2018/01/09 16:23
S96	1258	(600/583).CCLS.	US-PGPUB; USPAT	OR	OFF	2018/01/09 16:25
S97	4	S96 and ((vent$4 near4 air) and flash$6)	US-PGPUB; USPAT	OR	OFF	2018/01/09 16:25
S98	3	S97 and (blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT	OR	OFF	2018/01/09 16:26
S99	1733	(600/573).CCLS.	US-PGPUB; USPAT	OR	OFF	2018/01/09 16:50
S100	13	S99 and ((vent$4 near4 air) and flash$6)	US-PGPUB; USPAT	OR	OFF	2018/01/09 16:50
S101	255	("1779451" | "2004050" | "2700385" | "2836942" | "2854976" | "2953243" | "3021942" | "3073307" | "3074542" | "3255873" | "3294231" | "3323523" | "3329146" | "3333682" | "3367488" | "3382865" | "3485239" | "3537452" | "3585984" | "3610240" | "3658061" | "3664879" | "3817240" | "3828775" | "3859998" | "3874367" | "3886930" | "3890971" | "3904033" | "3934722" | "3968876" | "4106497" | "4108175" | "4113090" | "4139009" | "4154229" | "4166450" | "4175008" | "4193400" | "4207870" | "4269186" | "4300678" | "4312362" | "4317445" | "4340068" | "4375849" | "4398544" | "4409990" | "4412548" | "4416290" | "4416291" | "4418703" | "4430082" | "4436098" | "4444203" | "4592744" | "4634428" | "4643722" | "4659330" | "4664249" | "4664654" | "4671408" | "4679571" | "4681567" | "4695274" | "4702738" | "4723943" | "4728320" | "4728321" |	US-PGPUB; USPAT; USOCR	OR	OFF	2018/01/09 16:51

		"4731059" | "4735311" | "4735618" | "4737144" | "4738663" | "4743233" | "4746008" | "4747836" | "4747837" | "4772272" | "4778453" | "4781697" | "4782841" | "4788986" | "4790828" | "4793484" | "4795432" | "4795443" | "4801295" | "4804372" | "4813426" | "4816022" | "4816024" | "4819659" | "4820277" | "4826490" | "4826491" | "4838871" | "4842587" | "4844089" | "4846796" | "4850968" | "4850976" | "4850977" | "4850978" | "4850994" | "4850996" | "4858607" | "4863434" | "4863435" | "4863436" | "4865592" | "4867746" | "4872552" | "4874383" | "4874384" | "4883469" | "4886072" | "4886503" | "4888001" | "4892107" | "4892521" | "4894052" | "4900309" | "4909791" | "4909792").PN. OR ("4921096" | "4927018" | "4944397" | "4966591" | "4971068" | "4976699" | "4982842" | "5011475" | "5011479" | "5030207" | "5032116" | "5033476" | "5055102" | "5069225" | "5078693" | "5078698" | "5092845" | "5112327" | "5116325" | "5120319" | "5122121" | "5135509" | "5137518" | "5139489" | "5151089" | "5154285" | "5181523" | "5188611" | "5197954" | "5201794" | "5207653" | "5217025" | "5222502" | "5232454" | "5232455" | "5242411" | "5242417" | "5277311" | "5290246" | "5295969" | "5303713" | "5306259" | "5312369" | "5401251" | "5405332" | "5423765" | "5450856" | "5462534" | "5485854" | "5486163" | "5490841" | "5496281" | "5509907" | "5520193" | "5533984" | "5542932" | "5584816" | "5599313" | "5599318" | "5603699" | "5632732" | "5643219" | "5662617" | "5665075" | "5669889" | "5693022" | "5697914" | "5702369" | "5733265" | "5755701" | "5807351" | "5830190" | "5836920" | "5885249" | "5893844" | "5913846" | "5984895" | "5993426" | "6059737" | "6077244" | "6077253" | "6080137" | "6096006" | "6110160" | "6120482" | "6156010" | "6190370" | "6261263" | "6511439" | "6533760" | "6964658" | "7160267" | "RE31086").PN. OR ("7615033").URPN.				
S102	215	S101 and @ad<"20150724"	US-PGPUB; USPAT	OR	OFF	2018/01/09 16:51
S103	1347	(604/164.01).CCLS.	US-PGPUB; USPAT	OR	OFF	2018/01/09 17:11
S104	17	S103 and ((vent$4 near4 air) and flash$6)	US-PGPUB; USPAT	OR	OFF	2018/01/09 17:11
S105	19	("2009/0312711").URPN.	USPAT	OR	OFF	2018/01/09 17:11
S106	11	("2007/0106220").URPN.	USPAT	OR	OFF	2018/01/09 17:11
S107	288967	(blood near4 (sequest$5 or sampl$4))	US-PGPUB;	OR	OFF	2018/01/09

			USPAT; USOCR; FPRS; EPO; JPO; DERWENT; IBM_TDB			17:16
S108	6321	S107 AND ((A61B10/0096 OR A61B5/150022).CPC.)	US-PGPUB; USPAT; USOCR; FPRS; EPO; JPO; DERWENT; IBM_TDB	OR	OFF	2018/01/09 17:16
S109	121	S108 and ((vent$4 near4 air) and flash$6)	US-PGPUB; USPAT	OR	OFF	2018/01/09 17:17
S110	448	(435/294.1).CCLS.	US-PGPUB; USPAT	OR	OFF	2018/01/09 17:31
S111	6	S110 and ((vent$4 near4 air) and flash$6)	US-PGPUB; USPAT	OR	OFF	2018/01/09 17:31
S113	71	(("ROGERS") near3 ("Bobby")).INV.	US-PGPUB; USPAT	OR	OFF	2018/07/24 13:31
S114	0	("15140443").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2018/07/24 13:38
S115	2	(15/140443).APP.	US-PGPUB; USPAT; USOCR	OR	OFF	2018/07/24 13:38
S116	2	(15/140448).APP.	US-PGPUB; USPAT; USOCR	OR	OFF	2018/07/24 13:40
S117	1735	(600/573).CCLS.	US-PGPUB; USPAT	OR	OFF	2018/07/24 13:56
S118	854	S117 and (blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT	OR	OFF	2018/07/24 13:56
S119	91	S118 and (vent$4 near4 air)	US-PGPUB; USPAT	OR	OFF	2018/07/24 13:57
S120	1258	(600/583).CCLS.	US-PGPUB; USPAT	OR	OFF	2018/07/24 14:06
S121	1074	S120 and (blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT	OR	OFF	2018/07/24 14:06
S122	80	S121 and (vent$4 near4 air)	US-PGPUB; USPAT	OR	OFF	2018/07/24 14:06
S123	301210	(blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT; USOCR; FPRS; EPO; JPO; DERWENT; IBM_TDB	OR	OFF	2018/07/24 14:11
S124	6556	S123 AND ((A61B10/0096 OR A61B5/150022).CPC.)	US-PGPUB; USPAT; USOCR; FPRS; EPO; JPO; DERWENT; IBM_TDB	OR	OFF	2018/07/24 14:11
S125	3664	S124 and @ad<"20150724"	US-PGPUB; USPAT	OR	OFF	2018/07/24 14:12

S126	12749	"19" and ((vent$4 near4 air) and flash$6)	US-PGPUB; USPAT	OR	OFF	2018/07/24 14:12
S127	117	S125 and ((vent$4 near4 air) and flash$6)	US-PGPUB; USPAT	OR	OFF	2018/07/24 14:12
S128	1348	(604/164.01).CCLS.	US-PGPUB; USPAT	OR	OFF	2018/07/24 14:16
S129	75	S128 and (blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT	OR	OFF	2018/07/24 14:17
S130	1	("20120291564").PN.	US-PGPUB; USPAT; USOCR	OR	OFF	2018/07/24 14:21
S131	448	(435/294.1).CCLS.	US-PGPUB; USPAT	OR	OFF	2018/07/24 14:25
S132	18	S131 and (blood near4 (sequest$5 or sampl$4))	US-PGPUB; USPAT	OR	OFF	2018/07/24 14:25
S133	98	("20020002349" | "20020183651" | "20030055381" | "20030208151" | "20040010228" | "20040054333" | "20040147855" | "20050004524" | "20050240161" | "20050245885" | "20050281713" | "20060287639" | "20080108954" | "20080145933" | "2707953" | "3013557" | "3098016" | "3382865" | "3405706" | "3494351" | "3577980" | "3648684" | "3848579" | "3937211" | "4057050" | "4133863" | "4166450" | "4340067" | "4370987" | "4444203" | "4459997" | "4509534" | "4657160" | "4676256" | "4865583" | "4890627" | "4988339" | "5009847" | "5097842" | "5108927" | "5122129" | "5269317" | "5330464" | "5360011" | "5429610" | "5450856" | "5507299" | "5577513" | "5762633" | "5865812" | "5882318" | "5922551" | "6016712" | "6057105" | "6159164" | "6210909" | "6364890" | "6387086" | "6403381" | "6626884" | "6692479" | "6746420" | "6913580" | "7044941" | "7087047" | "7335188" | "7744573" | "8197420" | "8231546" | "8337418").PN. OR ("8535241").URPN.	US-PGPUB; USPAT; USOCR	OR	ON	2018/07/24 14:44
S135	23	("4166450").PN. OR ("4412548").URPN.	US-PGPUB; USPAT; USOCR	OR	ON	2018/07/24 14:48
S136	307	("2913000" | "3817240" | "3859998" | "3864979" | "4016879" | "4046144").PN. OR ("4207870").URPN.	US-PGPUB; USPAT; USOCR	OR	ON	2018/07/24 14:48
S137	4	("2007/0088279").URPN.	USPAT	OR	ON	2018/07/24 14:48
S138	1	(14/990763).APP.	US-PGPUB; USPAT; USOCR	OR	OFF	2018/07/24 14:58
S139	9	(blood and sequest$5 and junction and first and portion and sampl$4).clm.	US-PGPUB; USPAT	OR	ON	2018/07/24 15:07

EAST Search History (Interference)

Ref	Hits	Search Query	DBs	Default	Plurals	Time

#				Operator		Stamp
S94	1	(port and sequest$5 and junction and chamber and sampl$4 and vent and barrier).clm.	US-PGPUB; USPAT	OR	OFF	2017/09/28 16:15
S112	3	(port and sequest$5 and chamber and sampl$4 and vent and barrier).clm.	US-PGPUB; USPAT	OR	OFF	2018/01/09 17:39

7/25/2018 7:49:09 PM
C:\Users\mabouelela\Documents\EAST\Workspaces\15140443 BLOOD OPTIMIZATION AND SEQUESTRATION.wsp

Search Notes	Application/Control No.	Applicant(s)/Patent Under Reexamination
	15994559	ROGERS ET AL.
	Examiner	Art Unit
	MAY ABOUELELA	3736

CPC- SEARCHED		
Symbol	Date	Examiner
A61B10/0096 OR A61B5/150022	7/24/2018	MA

CPC COMBINATION SETS - SEARCHED		
Symbol	Date	Examiner

US CLASSIFICATION SEARCHED			
Class	Subclass	Date	Examiner
600	573, 583	7/24/2018	MA
604	164.01	7/24/2018	MA
435	294.1	7/24/2018	MA

* See search history printout included with this form or the SEARCH NOTES box below to determine the scope of the search.

SEARCH NOTES		
Search Notes	Date	Examiner
class/subclass search	7/24/2018	MA
inventor name search	7/24/2018	MA
east text search	7/24/2018	MA
forward and backward search	7/24/2018	MA

INTERFERENCE SEARCH			
US Class/ CPC Symbol	US Subclass / CPC Group	Date	Examiner
as above		7/24/2018	MA

Issue Classification	Application/Control No.	Applicant(s)/Patent Under Reexamination
	15994559	ROGERS ET AL.
	Examiner	**Art Unit**
	MAY ABOUELELA	3736

CPC						
Symbol					**Type**	**Version**
A61B		5	/	150992	F	2013-01-01
A61M		2039	/	068	A	2013-01-01
A61M		2039	/	0202	A	2013-01-01
A61B		5	/	150221	I	2013-01-01
A61M		39	/	04	I	2013-01-01
A61B		5	/	154	I	2013-01-01
A61B		5	/	150572	I	2013-01-01
A61B		5	/	150473	I	2013-01-01
A61B		5	/	150389	I	2013-01-01
A61B		5	/	150213	I	2013-01-01
A61B		5	/	15003	I	2013-01-01
A61M		2039	/	0633	A	2013-01-01
A61B		5	/	153	I	2013-01-01
A61M		39	/	0693	I	2013-01-01
			/			

CPC Combination Sets							
Symbol					**Type**	**Set**	**Ranking**	**Version**
			/					
			/					

NONE		**Total Claims Allowed:**	
(Assistant Examiner)	(Date)	23	
/MAY ABOUELELA/ Primary Examiner.Art Unit 3736	07/25/2018	O.G. Print Claim(s)	O.G. Print Figure
(Primary Examiner)	(Date)	1	15B

U.S. Patent and Trademark Office — Part of Paper No. 20180725

Issue Classification	Application/Control No.	Applicant(s)/Patent Under Reexamination
	15994559	ROGERS ET AL.
	Examiner	**Art Unit**
	MAY ABOUELELA	3736

US ORIGINAL CLASSIFICATION	
CLASS	**SUBCLASS**
600	573

CROSS REFERENCE(S)

CLASS	SUBCLASS (ONE SUBCLASS PER BLOCK)				
600	583				
604	164.01				
435	294.1				

INTERNATIONAL CLASSIFICATION					
CLAIMED					**NON-CLAIMED**
A	6	1	B	5 / 00 (2006.01.01)	
B	6	5	D	81 / 00 (2006.01.01)	

NONE	Total Claims Allowed:	
(Assistant Examiner) (Date)	23	
/MAY ABOUELELA/ Primary Examiner.Art Unit 3736 07/25/2018	O.G. Print Claim(s)	O.G. Print Figure
(Primary Examiner) (Date)	1	15B

U.S. Patent and Trademark Office — Part of Paper No. 20180725

Issue Classification	Application/Control No.	Applicant(s)/Patent Under Reexamination
	15994559	ROGERS ET AL.
	Examiner	**Art Unit**
	MAY ABOUELELA	3736

☐ Claims renumbered in the same order as presented by applicant ☐ CPA ☒ T.D. ☐ R.1.47

Final	Original	Final	Original	Final	Original	Final	Original	Final	Original	Final	Original	Final	Original	Final	Original
1	1	15	17												
2	2	16	18												
	3	17	19												
3	4	18	20												
4	5		21												
5	6	19	22												
	7	20	23												
6	8	21	24												
7	9	22	25												
8	10	23	26												
9	11														
10	12														
11	13														
12	14														
13	15														
14	16														

NONE		**Total Claims Allowed:**	
(Assistant Examiner)	(Date)	23	
/MAY ABOUELELA/ Primary Examiner.Art Unit 3736	07/25/2018	O.G. Print Claim(s)	O.G. Print Figure
(Primary Examiner)	(Date)	1	15B

U.S. Patent and Trademark Office Part of Paper No. 20180725

Doc code: IDS
Doc description: Information Disclosure Statement (IDS) Filed

PTO/SB/08a (01-10)
Approved for use through 07/31/2012. OMB 0651-0031
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE

Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it contains a valid OMB control number.

INFORMATION DISCLOSURE STATEMENT BY APPLICANT (**Not for submission under 37 CFR 1.99)**		
	Application Number	
	Filing Date	2018-05-31
	First Named Inventor	Bobby E. Rogers et al.
	Art Unit	
	Examiner Name	
	Attorney Docket Number	251102.000027.KURIN2CON2

U.S.PATENTS						Remove
Examiner Initial*	Cite No	Patent Number	Kind Code[1]	Issue Date	Name of Patentee or Applicant of cited Document	Pages,Columns,Lines where Relevant Passages or Relevant Figures Appear
	1	3648684	A	1972-03-14	BARNWELL et al	
	2	3817240	A	1974-06-18	AYRES	
	3	3874367	A	1975-04-01	AYRES	
	4	3886930	A	1975-06-03	RYAN	
	5	4056101	A	1977-11-01	GEISSLER et al	
	6	4057050	A	1977-11-08	SARSTEDT	
	7	4106497	A	1978-08-15	PERCARPIO	
	8	4154229	A	1979-05-15	NUGENT	

ALL REFERENCES CONSIDERED EXCEPT WHERE LINED THROUGH. /M.A.A/

INFORMATION DISCLOSURE STATEMENT BY APPLICANT (Not for submission under 37 CFR 1.99)		
	Application Number	
	Filing Date	2018-05-31
	First Named Inventor	Bobby E. Rogers et al.
	Art Unit	
	Examiner Name	
	Attorney Docket Number	251102.000027.KURIN2CON2

	9	4207870	A	1980-06-17	ELDRIDGE	
	10	4412548	A	1983-11-01	HOCH	
	11	4416290	A	1983-11-22	LUTKOWSKI	
	12	5222502	A	1993-06-29	KUROSE	
	13	5520193	A	1996-05-28	SUZUKI et al	
	14	5749857	A	1998-05-12	CUPPY	
	15	6569117	B1	2003-05-27	ZIV et al	
	16	8070725	B2	2011-12-06	CHRISTENSEN et al	
	17	8197420	B2	2012-06-12	PATTON et al	
	18	8523826	B2	2013-09-03	LAYTON JR et al	
	19	8535241	B2	2013-09-17	BULLINGTON et al	

ALL REFERENCES CONSIDERED EXCEPT WHERE LINED THROUGH. /M.A.A/

INFORMATION DISCLOSURE STATEMENT BY APPLICANT (Not for submission under 37 CFR 1.99)		
	Application Number	
	Filing Date	2018-05-31
	First Named Inventor	Bobby E. Rogers et al.
	Art Unit	
	Examiner Name	
	Attorney Docket Number	251102.000027.KURIN2CON2

	20	8540663	B2	2013-09-24	DAVEY et al	
	21	8568371	B2	2013-10-29	SIOPES et al	
	22	8864684	B2	2014-10-21	BULLINGTON et al	
	23	9022951	B2	2015-05-05	BULLINGTON et al	
	24	9060724	B2	2015-06-23	BULLINGTON et al	
	25	9138572	B2	2015-09-22	ZEYTOONIAN et al	
	26	9204864	B2	2015-12-08	BULLINGTON et al	

If you wish to add additional U.S. Patent citation information please click the Add button. Add

U.S.PATENT APPLICATION PUBLICATIONS Remove

Examiner Initial*	Cite No	Publication Number	Kind Code[1]	Publication Date	Name of Patentee or Applicant of cited Document	Pages,Columns,Lines where Relevant Passages or Relevant Figures Appear
	1	20020004647	A1	2002-01-10	LEONG	
	2	20020004647	A1	2003-06-05	LEONG	

ALL REFERENCES CONSIDERED EXCEPT WHERE LINED THROUGH. /M.A.A/

INFORMATION DISCLOSURE STATEMENT BY APPLICANT (Not for submission under 37 CFR 1.99)		
	Application Number	
	Filing Date	2018-05-31
	First Named Inventor	Bobby E. Rogers et al.
	Art Unit	
	Examiner Name	
	Attorney Docket Number	251102.000027.KURIN2CON2

	3	20003208151	A1	2003-11-06	KRAUS et al	
	4	20040054333	A1	2004-03-18	THEEUWES et al	
	5	20040073171	A1	2004-04-15	ROGERS et al	
	6	20040147855	A1	2004-07-29	MARSDEN	
	7	20050004524	A1	2005-01-06	NEWBY et al	
	8	20050240161	A1	2005-10-27	CRAWFORD	
	9	20070088279	A1	2007-04-19	SHUE et al	
	10	20080145933	A1	2008-06-19	PATTON et al	
	11	20090227953	A1	2009-09-10	TAN et al	
	12	20100057004	A1	2010-03-04	CHRISTENSEN et al	
	13	20130317391	A1	2013-11-28	BULLINGTON et al	

ALL REFERENCES CONSIDERED EXCEPT WHERE LINED THROUGH. /M.A.A/

INFORMATION DISCLOSURE STATEMENT BY APPLICANT (Not for submission under 37 CFR 1.99)		
	Application Number	
	Filing Date	2018-05-31
	First Named Inventor	Bobby E. Rogers et al.
	Art Unit	
	Examiner Name	
	Attorney Docket Number	251102.000027.KURIN2CON2

	14	20160174888	A1	2016-06-23	BERTHIER et al	
	15	20170020427	A1	2017-01-26	ROGERS et al	
	16	20170020428	A1	2017-01-26	ROGERS et al	

If you wish to add additional U.S. Published Application citation information please click the Add button.

FOREIGN PATENT DOCUMENTS

Examiner Initial*	Cite No	Foreign Document Number[3]	Country Code[2]	Kind Code[4]	Publication Date	Name of Patentee or Applicant of cited Document	Pages,Columns,Lines where Relevant Passages or Relevant Figures Appear	T[5]
	1	H08257018	JP	A	1996-10-08	NISSHO KK		☐
	2	1665986	EP	A1	2006-06-07	BECTON DICKINSON CO		☐
	3	2011162772	WO	A2	2011-12-29	CLEARVIEW PATIENT SAFETY TECHNOLOGIES LLC et al		☐

If you wish to add additional Foreign Patent Document citation information please click the Add button

NON-PATENT LITERATURE DOCUMENTS

Examiner Initials*	Cite No	Include name of the author (in CAPITAL LETTERS), title of the article (when appropriate), title of the item (book, magazine, journal, serial, symposium, catalog, etc), date, pages(s), volume-issue number(s), publisher, city and/or country where published.	T[5]
	1		☐

If you wish to add additional non-patent literature document citation information please click the Add button

ALL REFERENCES CONSIDERED EXCEPT WHERE LINED THROUGH. /M.A.A/

INFORMATION DISCLOSURE STATEMENT BY APPLICANT (**Not for submission under 37 CFR 1.99)**		
	Application Number	
	Filing Date	2018-05-31
	First Named Inventor	Bobby E. Rogers et al.
	Art Unit	
	Examiner Name	
	Attorney Docket Number	251102.000027.KURIN2CON2

EXAMINER SIGNATURE			
Examiner Signature	/MAY A ABOUELELA/	Date Considered	07/25/2018

*EXAMINER: Initial if reference considered, whether or not citation is in conformance with MPEP 609. Draw line through a citation if not in conformance and not considered. Include copy of this form with next communication to applicant.

[1] See Kind Codes of USPTO Patent Documents at www.USPTO.GOV or MPEP 901.04. [2] Enter office that issued the document, by the two-letter code (WIPO Standard ST.3). [3] For Japanese patent documents, the indication of the year of the reign of the Emperor must precede the serial number of the patent document. [4] Kind of document by the appropriate symbols as indicated on the document under WIPO Standard ST.16 if possible. [5] Applicant is to place a check mark here if English language translation is attached.

ALL REFERENCES CONSIDERED EXCEPT WHERE LINED THROUGH. /M.A.A/

INFORMATION DISCLOSURE STATEMENT BY APPLICANT (**Not for submission under 37 CFR 1.99)**	Application Number	
	Filing Date	2018-05-31
	First Named Inventor	Bobby E. Rogers et al.
	Art Unit	
	Examiner Name	
	Attorney Docket Number	251102.000027.KURIN2CON2

CERTIFICATION STATEMENT

Please see 37 CFR 1.97 and 1.98 to make the appropriate selection(s):

☐ That each item of information contained in the information disclosure statement was first cited in any communication from a foreign patent office in a counterpart foreign application not more than three months prior to the filing of the information disclosure statement. See 37 CFR 1.97(e)(1).

OR

☐ That no item of information contained in the information disclosure statement was cited in a communication from a foreign patent office in a counterpart foreign application, and, to the knowledge of the person signing the certification after making reasonable inquiry, no item of information contained in the information disclosure statement was known to any individual designated in 37 CFR 1.56(c) more than three months prior to the filing of the information disclosure statement. See 37 CFR 1.97(e)(2).

☐ See attached certification statement.

☐ The fee set forth in 37 CFR 1.17 (p) has been submitted herewith.

☒ A certification statement is not submitted herewith.

SIGNATURE

A signature of the applicant or representative is required in accordance with CFR 1.33, 10.18. Please see CFR 1.4(d) for the form of the signature.

Signature	/David Devernoe/	Date (YYYY-MM-DD)	2018-05-31
Name/Print	David Devernoe	Registration Number	50,128

This collection of information is required by 37 CFR 1.97 and 1.98. The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.14. This collection is estimated to take 1 hour to complete, including gathering, preparing and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. **SEND TO: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.**

ALL REFERENCES CONSIDERED EXCEPT WHERE LINED THROUGH. /M.A.A/

To: ryan.schneider@troutman.com,patents@troutman.com,chris.franich@troutman.com
From: PAIR_eOfficeAction@uspto.gov
Cc: PAIR_eOfficeAction@uspto.gov
Subject: Private PAIR Correspondence Notification for Customer Number 153290

Aug 08, 2018 04:13:40 AM

Dear PAIR Customer:

TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 5200
Atlanta, GA 30308
UNITED STATES

The following USPTO patent application(s) associated with your Customer Number, 153290 , have new outgoing correspondence. This correspondence is now available for viewing in Private PAIR.

The official date of notification of the outgoing correspondence will be indicated on the form PTOL-90 accompanying the correspondence.

Disclaimer:
The list of documents shown below is provided as a courtesy and is not part of the official file wrapper. The content of the images shown in PAIR is the official record.

Application	Document	Mailroom Date	Attorney Docket No.
15994559	NOA	08/08/2018	251102.000027.KURIN2CON2
	INTV.SUM.EX	08/08/2018	251102.000027.KURIN2CON2
	1449	08/08/2018	251102.000027.KURIN2CON2

To view your correspondence online or update your email addresses, please visit us anytime at https://sportal.uspto.gov/secure/myportal/privatepair.

If you have any questions, please email the Electronic Business Center (EBC) at EBC@uspto.gov with 'e-Office Action' on the subject line or call 1-866-217-9197 during the following hours:

Monday - Friday 6:00 a.m. to 12:00 a.m.

Thank you for prompt attention to this notice,

UNITED STATES PATENT AND TRADEMARK OFFICE

PATENT APPLICATION INFORMATION RETRIEVAL SYSTEM

UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

APPLICATION NUMBER	FILING OR 371(C) DATE	FIRST NAMED APPLICANT	ATTY. DOCKET NO./TITLE
15/994,559	05/31/2018	Bobby E. Rogers	251102.000027.KURIN2CON2

CONFIRMATION NO. 4704

153290
TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 5200
Atlanta, GA 30308

PUBLICATION NOTICE

OC000000102968381

Title:BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD

Publication No.US-2018-0289304-A1
Publication Date:10/11/2018

NOTICE OF PUBLICATION OF APPLICATION

The above-identified application will be electronically published as a patent application publication pursuant to 37 CFR 1.211, et seq. The patent application publication number and publication date are set forth above.

The publication may be accessed through the USPTO's publically available Searchable Databases via the Internet at www.uspto.gov. The direct link to access the publication is currently http://www.uspto.gov/patft/.

The publication process established by the Office does not provide for mailing a copy of the publication to applicant. A copy of the publication may be obtained from the Office upon payment of the appropriate fee set forth in 37 CFR 1.19(a)(1). Orders for copies of patent application publications are handled by the USPTO's Public Records Division. The Public Records Division can be reached by telephone at (571) 272-3150 or (800) 972-6382, by facsimile at (571) 273-3250, by mail addressed to the United States Patent and Trademark Office, Public Records Division, Alexandria, VA 22313-1450 or via the Internet.

In addition, information on the status of the application, including the mailing date of Office actions and the dates of receipt of correspondence filed in the Office, may also be accessed via the Internet through the Patent Electronic Business Center at www.uspto.gov using the public side of the Patent Application Information and Retrieval (PAIR) system. The direct link to access this status information is currently https://portal.uspto.gov/pair/PublicPair. Prior to publication, such status information is confidential and may only be obtained by applicant using the private side of PAIR.

Further assistance in electronically accessing the publication, or about PAIR, is available by calling the Patent Electronic Business Center at 1-866-217-9197.

Office of Data Managment, Application Assistance Unit (571) 272-4000, or (571) 272-4200, or 1-888-786-0101

To: patents@troutman.com,ryan.schneider@troutman.com,chris.franich@troutman.com
From: PAIR_eOfficeAction@uspto.gov
Cc: PAIR_eOfficeAction@uspto.gov
Subject: Private PAIR Correspondence Notification for Customer Number 153290

Oct 12, 2018 03:29:50 AM

Dear PAIR Customer:

TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 5200
Atlanta, GA 30308
UNITED STATES

The following USPTO patent application(s) associated with your Customer Number, 153290 , have new outgoing correspondence. This correspondence is now available for viewing in Private PAIR.

The official date of notification of the outgoing correspondence will be indicated on the form PTOL-90 accompanying the correspondence.

Disclaimer:
The list of documents shown below is provided as a courtesy and is not part of the official file wrapper. The content of the images shown in PAIR is the official record.

Application	Document	Mailroom Date	Attorney Docket No.
15994559	NTC.PUB	10/11/2018	251102.000027.KURIN2CON2

To view your correspondence online or update your email addresses, please visit us anytime at https://sportal.uspto.gov/secure/myportal/privatepair.

If you have any questions, please email the Electronic Business Center (EBC) at EBC@uspto.gov with 'e-Office Action' on the subject line or call 1-866-217-9197 during the following hours:

Monday - Friday 6:00 a.m. to 12:00 a.m.

Thank you for prompt attention to this notice,

UNITED STATES PATENT AND TRADEMARK OFFICE

PATENT APPLICATION INFORMATION RETRIEVAL SYSTEM

PTO/AIA/80 (07-17)
Approved for use through 01/31/2018. OMB 0651-0035
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995, no person is required to respond to a collection of information unless it displays a valid OMB control number

POWER OF ATTORNEY TO PROSECUTE APPLICATIONS BEFORE THE USPTO

I hereby revoke all previous powers of attorney given in the application identified in the attached statement under 37 CFR 3.73(c).

I hereby appoint:

[X] Practitioners associated with Customer Number: 158174

OR

[ ] Practitioner(s) named below (if more than ten patent practitioners are to be named, then a customer number must be used):

Name	Registration Number	Name	Registration Number

As attorney(s) or agent(s) to represent the undersigned before the United States Patent and Trademark Office (USPTO) in connection with any and all patent applications assigned only to the undersigned according to the USPTO assignment records or assignment documents attached to this form in accordance with 37 CFR 3.73(c).

Please change the correspondence address for the application identified in the attached statement under 37 CFR 3.73(c) to:

[X] The address associated with Customer Number: 158174

OR

[ ]

Firm or individual name		
Address		
City	State	Zip
Country		
Telephone	Email	

Assignee name and address: KURIN, INC.
10755 SCRIPPS POWAY PARKWAY NO. 257
SAN DIEGO, CALIFORNIA 92131

A copy of this form, together with a statement under 37 CFR 3.73(c) (Form PTO/AIA/96 or equivalent) is required to be filed in each application in which this form is used. The statement under 37 CFR 3.73(c) may be completed by one of the practitioners appointed in this form, and must identify the application in which this Power of Attorney is to be filed.

SIGNATURE of Assignee of Record

The individual whose signature and title is supplied below is authorized to act on behalf of the assignee.

Signature Bob Rogers	Date 10/15/2018
Name Bob Rogers	Telephone
Title Founder, CEO	

This collection of information is required by 37 CFR 1.31, 1.32, and 1.33. The information is required to obtain or retain a benefit by the public, which is to update (and by the USPTO to process) the file of a patent or reexamination proceeding. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.11 and 1.14. This collection is estimated to take 18 minutes to complete, including gathering, preparing, and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. **SEND TO: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.**

If you need assistance in completing the form, call 1-800-PTO-9199 and select option 2.

Privacy Act Statement

The **Privacy Act of 1974 (P.L. 93-579)** requires that you be given certain information in connection with your submission of the attached form related to a patent application or patent. Accordingly, pursuant to the requirements of the Act, please be advised that: (1) the general authority for the collection of this information is 35 U.S.C. 2(b)(2); (2) furnishing of the information solicited is voluntary; and (3) the principal purpose for which the information is used by the U.S. Patent and Trademark Office is to process and/or examine your submission related to a patent application or patent. If you do not furnish the requested information, the U.S. Patent and Trademark Office may not be able to process and/or examine your submission, which may result in termination of proceedings or abandonment of the application or expiration of the patent.

The information provided by you in this form will be subject to the following routine uses:

1. The information on this form will be treated confidentially to the extent allowed under the Freedom of Information Act (5 U.S.C. 552) and the Privacy Act (5 U.S.C 552a). Records from this system of records may be disclosed to the Department of Justice to determine whether disclosure of these records is required by the Freedom of Information Act.
2. A record from this system of records may be disclosed, as a routine use, in the course of presenting evidence to a court, magistrate, or administrative tribunal, including disclosures to opposing counsel in the course of settlement negotiations.
3. A record in this system of records may be disclosed, as a routine use, to a Member of Congress submitting a request involving an individual, to whom the record pertains, when the individual has requested assistance from the Member with respect to the subject matter of the record.
4. A record in this system of records may be disclosed, as a routine use, to a contractor of the Agency having need for the information in order to perform a contract. Recipients of information shall be required to comply with the requirements of the Privacy Act of 1974, as amended, pursuant to 5 U.S.C. 552a(m).
5. A record related to an International Application filed under the Patent Cooperation Treaty in this system of records may be disclosed, as a routine use, to the International Bureau of the World Intellectual Property Organization, pursuant to the Patent Cooperation Treaty.
6. A record in this system of records may be disclosed, as a routine use, to another federal agency for purposes of National Security review (35 U.S.C. 181) and for review pursuant to the Atomic Energy Act (42 U.S.C. 218(c)).
7. A record from this system of records may be disclosed, as a routine use, to the Administrator, General Services, or his/her designee, during an inspection of records conducted by GSA as part of that agency's responsibility to recommend improvements in records management practices and programs, under authority of 44 U.S.C. 2904 and 2906. Such disclosure shall be made in accordance with the GSA regulations governing inspection of records for this purpose, and any other relevant (*i.e.*, GSA or Commerce) directive. Such disclosure shall not be used to make determinations about individuals.
8. A record from this system of records may be disclosed, as a routine use, to the public after either publication of the application pursuant to 35 U.S.C. 122(b) or issuance of a patent pursuant to 35 U.S.C. 151. Further, a record may be disclosed, subject to the limitations of 37 CFR 1.14, as a routine use, to the public if the record was filed in an application which became abandoned or in which the proceedings were terminated and which application is referenced by either a published application, an application open to public inspection or an issued patent.
9. A record from this system of records may be disclosed, as a routine use, to a Federal, State, or local law enforcement agency, if the USPTO becomes aware of a violation or potential violation of law or regulation.

PTO/AIA/96 (08-12)
Approved for use through 01/31/2013. OMB 0651-0031
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

STATEMENT UNDER 37 CFR 3.73(c)

Applicant/Patent Owner: KURIN, INC.

Application No./Patent No.: 15/994,559 Filed/Issue Date: 2018-05-31

Titled: BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD

KURIN, INC., a corporation

(Name of Assignee) (Type of Assignee, e.g., corporation, partnership, university, government agency, etc.)

states that, for the patent application/patent identified above, it is (choose **one** of options 1, 2, 3 or 4 below):

1. ☑ The assignee of the entire right, title, and interest.

2. ☐ An assignee of less than the entire right, title, and interest (check applicable box):

   ☐ The extent (by percentage) of its ownership interest is _____%. Additional Statement(s) by the owners holding the balance of the interest must be submitted to account for 100% of the ownership interest.

   ☐ There are unspecified percentages of ownership. The other parties, including inventors, who together own the entire right, title and interest are:

   Additional Statement(s) by the owner(s) holding the balance of the interest must be submitted to account for the entire right, title, and interest.

3. ☐ The assignee of an undivided interest in the entirety (a complete assignment from one of the joint inventors was made). The other parties, including inventors, who together own the entire right, title, and interest are:

   Additional Statement(s) by the owner(s) holding the balance of the interest must be submitted to account for the entire right, title, and interest.

4. ☐ The recipient, via a court proceeding or the like (*e.g.*, bankruptcy, probate), of an undivided interest in the entirety (a complete transfer of ownership interest was made). The certified document(s) showing the transfer is attached.

The interest identified in option 1, 2 or 3 above (not option 4) is evidenced by either (choose **one** of options A or B below):

A. ☑ An assignment from the inventor(s) of the patent application/patent identified above. The assignment was recorded in the United States Patent and Trademark Office at Reel 045957, Frame 0595, or for which a copy thereof is attached.

B. ☐ A chain of title from the inventor(s), of the patent application/patent identified above, to the current assignee as follows:

   1. From: _____ To: _____

      The document was recorded in the United States Patent and Trademark Office at

      Reel _____, Frame _____, or for which a copy thereof is attached.

   2. From: _____ To: _____

      The document was recorded in the United States Patent and Trademark Office at

      Reel _____, Frame _____, or for which a copy thereof is attached.

This collection of information is required by 37 CFR 3.73(b). The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.11 and 1.14. This collection is estimated to take 12 minutes to complete, including gathering, preparing, and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. **SEND TO: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450**.

If you need assistance in completing the form, call 1-800-PTO-9199 and select option 2.

PTO/AIA/96 (08-12)
Approved for use through 01/31/2013. OMB 0651-0031
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

STATEMENT UNDER 37 CFR 3.73(c)

3. From: _____ To: _____

The document was recorded in the United States Patent and Trademark Office at

Reel _____, Frame _____, or for which a copy thereof is attached.

4. From: _____ To: _____

The document was recorded in the United States Patent and Trademark Office at

Reel _____, Frame _____, or for which a copy thereof is attached.

5. From: _____ To: _____

The document was recorded in the United States Patent and Trademark Office at

Reel _____, Frame _____, or for which a copy thereof is attached.

6. From: _____ To: _____

The document was recorded in the United States Patent and Trademark Office at

Reel _____, Frame _____, or for which a copy thereof is attached.

☐ Additional documents in the chain of title are listed on a supplemental sheet(s).

☐ As required by 37 CFR 3.73(c)(1)(i), the documentary evidence of the chain of title from the original owner to the assignee was, or concurrently is being, submitted for recordation pursuant to 37 CFR 3.11.

[NOTE: A separate copy (i.e., a true copy of the original assignment document(s)) must be submitted to Assignment Division in accordance with 37 CFR Part 3, to record the assignment in the records of the USPTO. See MPEP 302.08]

The undersigned (whose title is supplied below) is authorized to act on behalf of the assignee.

Signature	Date
James Scott Nolan	53393
Printed or Typed Name	Title or Registration Number

10/17/2018

Privacy Act Statement

The **Privacy Act of 1974 (P.L. 93-579)** requires that you be given certain information in connection with your submission of the attached form related to a patent application or patent. Accordingly, pursuant to the requirements of the Act, please be advised that: (1) the general authority for the collection of this information is 35 U.S.C. 2(b)(2); (2) furnishing of the information solicited is voluntary; and (3) the principal purpose for which the information is used by the U.S. Patent and Trademark Office is to process and/or examine your submission related to a patent application or patent. If you do not furnish the requested information, the U.S. Patent and Trademark Office may not be able to process and/or examine your submission, which may result in termination of proceedings or abandonment of the application or expiration of the patent.

The information provided by you in this form will be subject to the following routine uses:

1. The information on this form will be treated confidentially to the extent allowed under the Freedom of Information Act (5 U.S.C. 552) and the Privacy Act (5 U.S.C 552a). Records from this system of records may be disclosed to the Department of Justice to determine whether disclosure of these records is required by the Freedom of Information Act.
2. A record from this system of records may be disclosed, as a routine use, in the course of presenting evidence to a court, magistrate, or administrative tribunal, including disclosures to opposing counsel in the course of settlement negotiations.
3. A record in this system of records may be disclosed, as a routine use, to a Member of Congress submitting a request involving an individual, to whom the record pertains, when the individual has requested assistance from the Member with respect to the subject matter of the record.
4. A record in this system of records may be disclosed, as a routine use, to a contractor of the Agency having need for the information in order to perform a contract. Recipients of information shall be required to comply with the requirements of the Privacy Act of 1974, as amended, pursuant to 5 U.S.C. 552a(m).
5. A record related to an International Application filed under the Patent Cooperation Treaty in this system of records may be disclosed, as a routine use, to the International Bureau of the World Intellectual Property Organization, pursuant to the Patent Cooperation Treaty.
6. A record in this system of records may be disclosed, as a routine use, to another federal agency for purposes of National Security review (35 U.S.C. 181) and for review pursuant to the Atomic Energy Act (42 U.S.C. 218(c)).
7. A record from this system of records may be disclosed, as a routine use, to the Administrator, General Services, or his/her designee, during an inspection of records conducted by GSA as part of that agency's responsibility to recommend improvements in records management practices and programs, under authority of 44 U.S.C. 2904 and 2906. Such disclosure shall be made in accordance with the GSA regulations governing inspection of records for this purpose, and any other relevant (*i.e.*, GSA or Commerce) directive. Such disclosure shall not be used to make determinations about individuals.
8. A record from this system of records may be disclosed, as a routine use, to the public after either publication of the application pursuant to 35 U.S.C. 122(b) or issuance of a patent pursuant to 35 U.S.C. 151. Further, a record may be disclosed, subject to the limitations of 37 CFR 1.14, as a routine use, to the public if the record was filed in an application which became abandoned or in which the proceedings were terminated and which application is referenced by either a published application, an application open to public inspection or an issued patent.
9. A record from this system of records may be disclosed, as a routine use, to a Federal, State, or local law enforcement agency, if the USPTO becomes aware of a violation or potential violation of law or regulation.

Electronic Acknowledgement Receipt

EFS ID:	34057934
Application Number:	15994559
International Application Number:	
Confirmation Number:	4704
Title of Invention:	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD
First Named Inventor/Applicant Name:	Bobby E. Rogers
Customer Number:	153290
Filer:	James Scott Nolan
Filer Authorized By:	
Attorney Docket Number:	251102.000027.KURIN2CON2
Receipt Date:	19-OCT-2018
Filing Date:	31-MAY-2018
Time Stamp:	11:11:33
Application Type:	Utility under 35 USC 111(a)

Payment information:

Submitted with Payment	no

File Listing:

Document Number	Document Description	File Name	File Size(Bytes)/ Message Digest	Multi Part /.zip	Pages (if appl.)
1	Power of Attorney	KurinUSPOA_Executed.pdf	174911 c055558c97891b8d6fbff0f3e3e3e6777a9c7389	no	2
Warnings:					

Information:					
2	Power of Attorney	KURIN2CON2_15994559_Executed373_4704.pdf	151724 b4ad85a09ce7610a041806ca991dd919d28c2d3c	no	3
Warnings:					
Information:					
			Total Files Size (in bytes):	326635	

This Acknowledgement Receipt evidences receipt on the noted date by the USPTO of the indicated documents, characterized by the applicant, and including page counts, where applicable. It serves as evidence of receipt similar to a Post Card, as described in MPEP 503.

New Applications Under 35 U.S.C. 111

If a new application is being filed and the application includes the necessary components for a filing date (see 37 CFR 1.53(b)-(d) and MPEP 506), a Filing Receipt (37 CFR 1.54) will be issued in due course and the date shown on this Acknowledgement Receipt will establish the filing date of the application.

National Stage of an International Application under 35 U.S.C. 371

If a timely submission to enter the national stage of an international application is compliant with the conditions of 35 U.S.C. 371 and other applicable requirements a Form PCT/DO/EO/903 indicating acceptance of the application as a national stage submission under 35 U.S.C. 371 will be issued in addition to the Filing Receipt, in due course.

New International Application Filed with the USPTO as a Receiving Office

If a new international application is being filed and the international application includes the necessary components for an international filing date (see PCT Article 11 and MPEP 1810), a Notification of the International Application Number and of the International Filing Date (Form PCT/RO/105) will be issued in due course, subject to prescriptions concerning national security, and the date shown on this Acknowledgement Receipt will establish the international filing date of the application.

UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

APPLICATION NUMBER	FILING OR 371(C) DATE	FIRST NAMED APPLICANT	ATTY. DOCKET NO./TITLE
15/994,559	05/31/2018	Bobby E. Rogers	251102.000027.KURIN2CON2

CONFIRMATION NO. 4704

153290
TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 5200
Atlanta, GA 30308

POWER OF ATTORNEY NOTICE

OC000000103272121

Date Mailed: 10/23/2018

NOTICE REGARDING CHANGE OF POWER OF ATTORNEY

This is in response to the Power of Attorney filed 10/19/2018.

- The Power of Attorney to you in this application has been revoked by the applicant. Future correspondence will be mailed to the new address of record(37 CFR 1.33).

Questions about the contents of this notice and the requirements it sets forth should be directed to the Office of Data Management, Application Assistance Unit, at **(571) 272-4000** or **(571) 272-4200** or **1-888-786-0101**.

/mteklemichael/

UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

APPLICATION NUMBER	FILING OR 371(C) DATE	FIRST NAMED APPLICANT	ATTY. DOCKET NO./TITLE
15/994,559	05/31/2018	Bobby E. Rogers	251102.000027.KURIN2CON2

CONFIRMATION NO. 4704

158174
Kurin, Inc.
P.O. Box 371710
San Diego, CA 92137

POA ACCEPTANCE LETTER

OC000000103272161

Date Mailed: 10/23/2018

NOTICE OF ACCEPTANCE OF POWER OF ATTORNEY

This is in response to the Power of Attorney filed 10/19/2018.

The Power of Attorney in this application is accepted. Correspondence in this application will be mailed to the above address as provided by 37 CFR 1.33.

Questions about the contents of this notice and the requirements it sets forth should be directed to the Office of Data Management, Application Assistance Unit, at **(571) 272-4000** or **(571) 272-4200** or **1-888-786-0101**.

/mteklemichael/

To: docketing@intelligentclicks.net,jsnolan1@hotmail.com,eofficeaction@appcoll.com
From: PAIR_eOfficeAction@uspto.gov
Cc: PAIR_eOfficeAction@uspto.gov
Subject: Private PAIR Correspondence Notification for Customer Number 158174

Oct 23, 2018 03:25:36 AM

Dear PAIR Customer:

Kurin, Inc.
P.O. Box 371710
San Diego, CA 92137
UNITED STATES

The following USPTO patent application(s) associated with your Customer Number, 158174 , have new outgoing correspondence. This correspondence is now available for viewing in Private PAIR.

The official date of notification of the outgoing correspondence will be indicated on the form PTOL-90 accompanying the correspondence.

Disclaimer:
The list of documents shown below is provided as a courtesy and is not part of the official file wrapper. The content of the images shown in PAIR is the official record.

Application	Document	Mailroom Date	Attorney Docket No.
15994559	N570	10/23/2018	251102.000027.KURIN2CON2
	N570	10/23/2018	251102.000027.KURIN2CON2

To view your correspondence online or update your email addresses, please visit us anytime at https://sportal.uspto.gov/secure/myportal/privatepair.

If you have any questions, please email the Electronic Business Center (EBC) at EBC@uspto.gov with 'e-Office Action' on the subject line or call 1-866-217-9197 during the following hours:

Monday - Friday 6:00 a.m. to 12:00 a.m.

Thank you for prompt attention to this notice,

UNITED STATES PATENT AND TRADEMARK OFFICE

PATENT APPLICATION INFORMATION RETRIEVAL SYSTEM

PART B - FEE(S) TRANSMITTAL

Complete and send this form, together with applicable fee(s), to: Mail **Mail Stop ISSUE FEE**
Commissioner for Patents
P.O. Box 1450
Alexandria, Virginia 22313-1450
or Fax (571)-273-2885

INSTRUCTIONS: This form should be used for transmitting the ISSUE FEE and PUBLICATION FEE (if required). Blocks 1 through 5 should be completed where appropriate. All further correspondence including the Patent, advance orders and notification of maintenance fees will be mailed to the current correspondence address as indicated unless corrected below or directed otherwise in Block 1, by (a) specifying a new correspondence address; and/or (b) indicating a separate "FEE ADDRESS" for maintenance fee notifications.

CURRENT CORRESPONDENCE ADDRESS (Note: Use Block 1 for any change of address)

153290 7590 08/08/2018
TROUTMAN SANDERS LLP/Kurin, Inc.
600 Peachtree St., NE, Suite 5200
Atlanta, GA 30308

Note: A certificate of mailing can only be used for domestic mailings of the Fee(s) Transmittal. This certificate cannot be used for any other accompanying papers. Each additional paper, such as an assignment or formal drawing, must have its own certificate of mailing or transmission.

Certificate of Mailing or Transmission
I hereby certify that this Fee(s) Transmittal is being deposited with the United States Postal Service with sufficient postage for first class mail in an envelope addressed to the Mail Stop ISSUE FEE address above, or being facsimile transmitted to the USPTO (571) 273-2885, on the date indicated below.

(Depositor's name)
(Signature)
(Date)

APPLICATION NO.	FILING DATE	FIRST NAMED INVENTOR	ATTORNEY DOCKET NO.	CONFIRMATION NO.
15/994,559	05/31/2018	Bobby E. Rogers	251102.000027.KURIN2CON2	4704

TITLE OF INVENTION: BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD

APPLN. TYPE	ENTITY STATUS	ISSUE FEE DUE	PUBLICATION FEE DUE	PREV. PAID ISSUE FEE	TOTAL FEE(S) DUE	DATE DUE
nonprovisional	SMALL	$500	$0	$0	$500	11/08/2018

EXAMINER	ART UNIT	CLASS-SUBCLASS
ABOUELELA, MAY A	3736	600-573000

1. Change of correspondence address or indication of "Fee Address" (37 CFR 1.363).
☐ Change of correspondence address (or Change of Correspondence Address form PTO/SB/122) attached.
☐ "Fee Address" indication (or "Fee Address" Indication form PTO/SB/47; Rev 03-02 or more recent) attached. **Use of a Customer Number is required.**

2. For printing on the patent front page, list
(1) The names of up to 3 registered patent attorneys or agents OR, alternatively,
(2) The name of a single firm (having as a member a registered attorney or agent) and the names of up to 2 registered patent attorneys or agents. If no name is listed, no name will be printed.
1 _____
2 _____
3 _____

3. ASSIGNEE NAME AND RESIDENCE DATA TO BE PRINTED ON THE PATENT (print or type)

PLEASE NOTE: Unless an assignee is identified below, no assignee data will appear on the patent. If an assignee is identified below, the document has been filed for recordation as set forth in 37 CFR 3.11. Completion of this form is NOT a substitute for filing an assignment.

(A) NAME OF ASSIGNEE: KURIN, INC.

(B) RESIDENCE: (CITY and STATE OR COUNTRY): SAN DIEGO, CALIFORNIA

Please check the appropriate assignee category or categories (will not be printed on the patent) : ☐ Individual ☒ Corporation or other private group entity ☐ Government

4a. The following fee(s) are submitted:
☒ Issue Fee
☐ Publication Fee (No small entity discount permitted)
☐ Advance Order - # of Copies _____

4b. Payment of Fee(s): **(Please first reapply any previously paid issue fee shown above)**
☐ A check is enclosed.
☐ Payment by credit card. Form PTO-2038 is attached.
☐ The director is hereby authorized to charge the required fee(s), any deficiency, or credits any overpayment, to Deposit Account Number _____ (enclose an extra copy of this form).

5. **Change in Entity Status** (from status indicated above)
☐ Applicant certifying micro entity status. See 37 CFR 1.29
NOTE: Absent a valid certification of Micro Entity Status (see forms PTO/SB/15A and 15B), issue fee payment in the micro entity amount will not be accepted at the risk of application abandonment.
☐ Applicant asserting small entity status. See 37 CFR 1.27
NOTE: If the application was previously under micro entity status, checking this box will be taken to be a notification of loss of entitlement to micro entity status.
☐ Applicant changing to regular undiscounted fee status.
NOTE: Checking this box will be taken to be a notification of loss of entitlement to small or micro entity status, as applicable.

NOTE: This form must be signed in accordance with 37 CFR 1.31 and 1.33. See 37 CFR 1.4 for signature requirements and certifications.

Authorized Signature _____ Date 10/29/2018

Typed or printed name James Scott Nolan Registration No. 53393

Electronic Patent Application Fee Transmittal

Application Number:	15994559
Filing Date:	31-May-2018
Title of Invention:	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD
First Named Inventor/Applicant Name:	Bobby E. Rogers
Filer:	James Scott Nolan
Attorney Docket Number:	KURIN2CON2

Filed as Small Entity

Filing Fees for Utility under 35 USC 111(a)

Description	Fee Code	Quantity	Amount	Sub-Total in USD($)
Basic Filing:				
Pages:				
Claims:				
Miscellaneous-Filing:				
Petition:				
Patent-Appeals-and-Interference:				
Post-Allowance-and-Post-Issuance:				
UTILITY APPL ISSUE FEE	2501	1	500	500

Description	Fee Code	Quantity	Amount	Sub-Total in USD($)
Extension-of-Time:				
Miscellaneous:				
			Total in USD ($)	**500**

Electronic Acknowledgement Receipt	
EFS ID:	34166911
Application Number:	15994559
International Application Number:	
Confirmation Number:	4704
Title of Invention:	BLOOD SAMPLE OPTIMIZATION SYSTEM AND BLOOD CONTAMINANT SEQUESTRATION DEVICE AND METHOD
First Named Inventor/Applicant Name:	Bobby E. Rogers
Customer Number:	158174
Filer:	James Scott Nolan
Filer Authorized By:	
Attorney Docket Number:	KURIN2CON2
Receipt Date:	30-OCT-2018
Filing Date:	31-MAY-2018
Time Stamp:	23:28:32
Application Type:	Utility under 35 USC 111(a)

Payment information:

Submitted with Payment	yes
Payment Type	CARD
Payment was successfully received in RAM	$500
RAM confirmation Number	103118INTEFSW23292100
Deposit Account	
Authorized User	
The Director of the USPTO is hereby authorized to charge indicated fees and credit any overpayment as follows:	

File Listing:

Document Number	Document Description	File Name	File Size(Bytes)/ Message Digest	Multi Part /.zip	Pages (if appl.)
1	Issue Fee Payment (PTO-85B)	Kurin2CON2_ISSUE_FEE.pdf	178123 085118d576ab2a610cc78ac684177aa671e8b4e0	no	1
Warnings:					
Information:					
2	Fee Worksheet (SB06)	fee-info.pdf	30412 36dcf4b8624984728918417311639 2d7404b2bf6	no	2
Warnings:					
Information:					
		Total Files Size (in bytes):	208535		

This Acknowledgement Receipt evidences receipt on the noted date by the USPTO of the indicated documents, characterized by the applicant, and including page counts, where applicable. It serves as evidence of receipt similar to a Post Card, as described in MPEP 503.

New Applications Under 35 U.S.C. 111
If a new application is being filed and the application includes the necessary components for a filing date (see 37 CFR 1.53(b)-(d) and MPEP 506), a Filing Receipt (37 CFR 1.54) will be issued in due course and the date shown on this Acknowledgement Receipt will establish the filing date of the application.
National Stage of an International Application under 35 U.S.C. 371
If a timely submission to enter the national stage of an international application is compliant with the conditions of 35 U.S.C. 371 and other applicable requirements a Form PCT/DO/EO/903 indicating acceptance of the application as a national stage submission under 35 U.S.C. 371 will be issued in addition to the Filing Receipt, in due course.
New International Application Filed with the USPTO as a Receiving Office
If a new international application is being filed and the international application includes the necessary components for an international filing date (see PCT Article 11 and MPEP 1810), a Notification of the International Application Number and of the International Filing Date (Form PCT/RO/105) will be issued in due course, subject to prescriptions concerning national security, and the date shown on this Acknowledgement Receipt will establish the international filing date of the application.

INFORMATION DISCLOSURE STATEMENT BY APPLICANT (Not for submission under 37 CFR 1.99)		
	Application Number	
	Filing Date	2018-05-31
	First Named Inventor	Bobby E. Rogers et al.
	Art Unit	
	Examiner Name	
	Attorney Docket Number	251102.000027.KURIN2CON2

	20	8540663	B2	2013-09-24	DAVEY et al	
	21	8568371	B2	2013-10-29	SIOPES et al	
	22	8864684	B2	2014-10-21	BULLINGTON et al	
	23	9022951	B2	2015-05-05	BULLINGTON et al	
	24	9060724	B2	2015-06-23	BULLINGTON et al	
	25	9138572	B2	2015-09-22	ZEYTOONIAN et al	
	26	9204864	B2	2015-12-08	BULLINGTON et al	

If you wish to add additional U.S. Patent citation information please click the Add button. Add

U.S.PATENT APPLICATION PUBLICATIONS Remove

Examiner Initial*	Cite No	Publication Number	Kind Code[1]	Publication Date	Name of Patentee or Applicant of cited Document	Pages,Columns,Lines where Relevant Passages or Relevant Figures Appear
	1	20020004647	A1	2002-01-10	LEONG	
	2	20020004647	A1	01-2002 ~~2003-06-05~~	LEONG	

Change(s) applied to document.

/D.D./

8/10/2018

ALL REFERENCES CONSIDERED EXCEPT WHERE LINED THROUGH. /M.A.A/

UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

APPLICATION NO.	ISSUE DATE	PATENT NO.	ATTORNEY DOCKET NO.	CONFIRMATION NO.
15/994,559	12/04/2018	10143412	KURIN2CON2	4704

158174 7590 11/14/2018

Kurin, Inc.
P.O. Box 371710
San Diego, CA 92137

ISSUE NOTIFICATION

The projected patent number and issue date are specified above.

Determination of Patent Term Adjustment under 35 U.S.C. 154 (b)
(application filed on or after May 29, 2000)

The Patent Term Adjustment is 0 day(s). Any patent to issue from the above-identified application will include an indication of the adjustment on the front page.

If a Continued Prosecution Application (CPA) was filed in the above-identified application, the filing date that determines Patent Term Adjustment is the filing date of the most recent CPA.

Applicant will be able to obtain more detailed information by accessing the Patent Application Information Retrieval (PAIR) WEB site (http://pair.uspto.gov).

Any questions regarding the Patent Term Extension or Adjustment determination should be directed to the Office of Patent Legal Administration at (571)-272-7702. Questions relating to issue and publication fee payments should be directed to the Application Assistance Unit (AAU) of the Office of Data Management (ODM) at (571)-272-4200.

APPLICANT(s) (Please see PAIR WEB site http://pair.uspto.gov for additional applicants):

Bobby E. Rogers, San Diego, CA;
KURIN, INC., San Diego, CA;
Gino Kang, Irvine, CA;
John Detloff, San Diego, CA;

The United States represents the largest, most dynamic marketplace in the world and is an unparalleled location for business investment, innovation, and commercialization of new technologies. The USA offers tremendous resources and advantages for those who invest and manufacture goods here. Through SelectUSA, our nation works to encourage and facilitate business investment. To learn more about why the USA is the best country in the world to develop technology, manufacture products, and grow your business, visit SelectUSA.gov.

IR103 (Rev. 10/09)

To: docketing@intelligentclicks.net,jsnolan1@hotmail.com,eofficeaction@appcoll.com
From: PAIR_eOfficeAction@uspto.gov
Cc: PAIR_eOfficeAction@uspto.gov
Subject: Private PAIR Correspondence Notification for Customer Number 158174

Nov 15, 2018 04:49:48 AM

Dear PAIR Customer:

Kurin, Inc.
P.O. Box 371710
San Diego, CA 92137
UNITED STATES

The following USPTO patent application(s) associated with your Customer Number, 158174 , have new outgoing correspondence. This correspondence is now available for viewing in Private PAIR.

The official date of notification of the outgoing correspondence will be indicated on the form PTOL-90 accompanying the correspondence.

Disclaimer:
The list of documents shown below is provided as a courtesy and is not part of the official file wrapper. The content of the images shown in PAIR is the official record.

Application	Document	Mailroom Date	Attorney Docket No.
15994559	ISSUE.NTF	11/14/2018	KURIN2CON2

To view your correspondence online or update your email addresses, please visit us anytime at https://sportal.uspto.gov/secure/myportal/privatepair.

If you have any questions, please email the Electronic Business Center (EBC) at EBC@uspto.gov with 'e-Office Action' on the subject line or call 1-866-217-9197 during the following hours:

Monday - Friday 6:00 a.m. to 12:00 a.m.

Thank you for prompt attention to this notice,

UNITED STATES PATENT AND TRADEMARK OFFICE

PATENT APPLICATION INFORMATION RETRIEVAL SYSTEM